

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
 Data File : PS005033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 08:11
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 11:34:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	4.954	0.000	1009.1E6	0	535.394	N.D.	#
5) T	DICAMBA	0.000	5.454	0	759.0E6	N.D.	197.642	
6) T	MCP	0.000	5.454	0	759.0E6	N.D.	262.694	
9) T	2,4-D	6.629	0.000	637.8E6	0	472.669	N.D.	#
15) T	Picloram	9.128	9.118	358.1E6	21495190	36.065	3.151	#
16) T	DCPA	0.000	9.118	0	21495190	N.D.	3.260	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
Data File : PS005033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 08:11
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 11:34:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

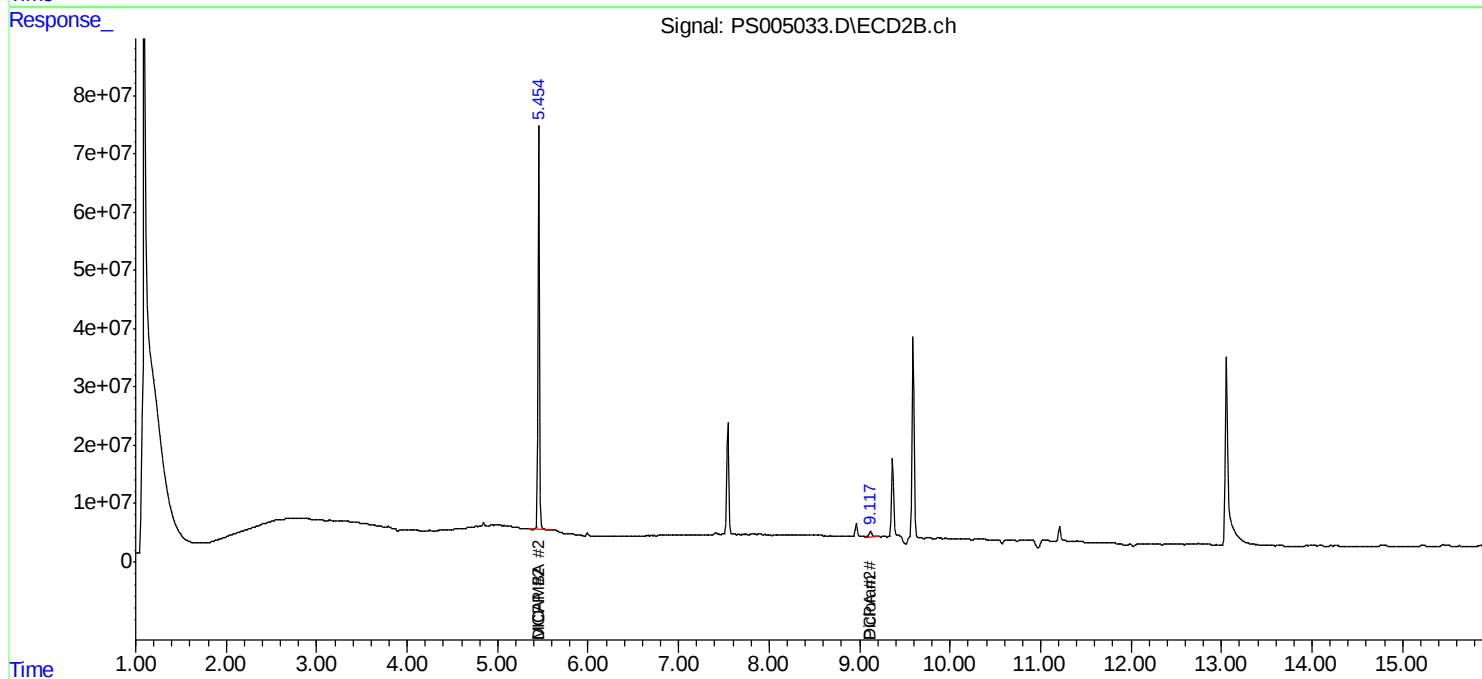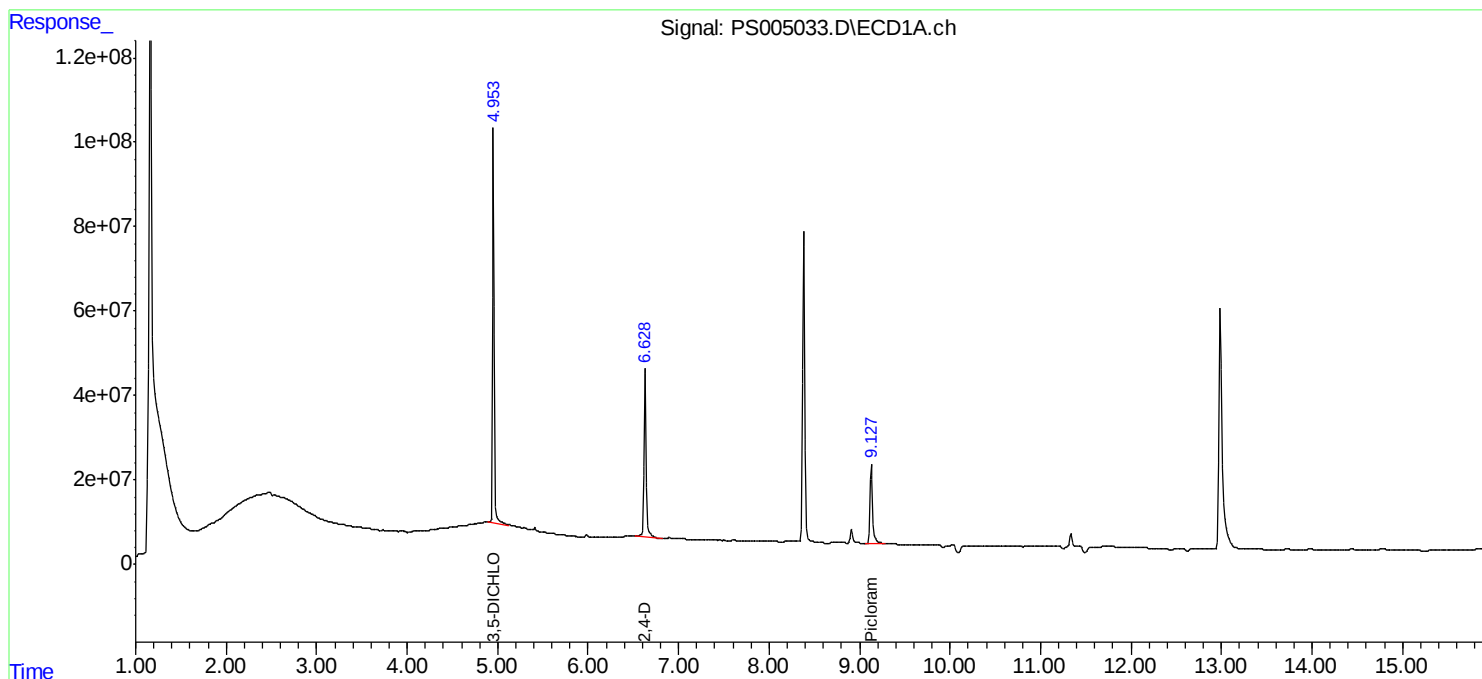


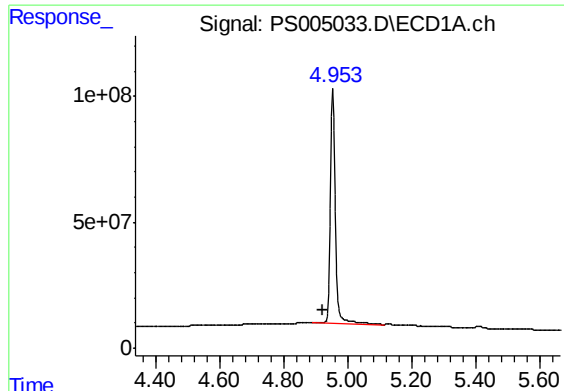

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.954 min
Delta R.T.: 0.032 min
Response: 1009131528
Conc: 535.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

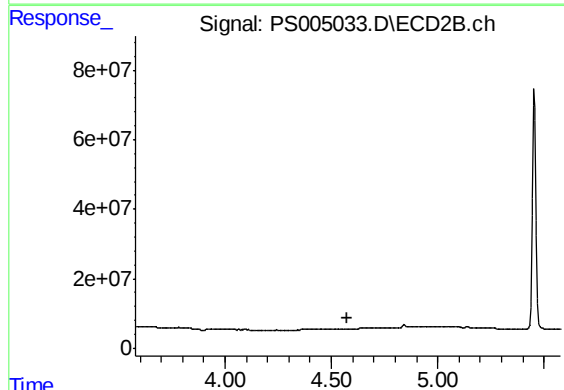


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.578 min
Response: 0
Conc: N.D.

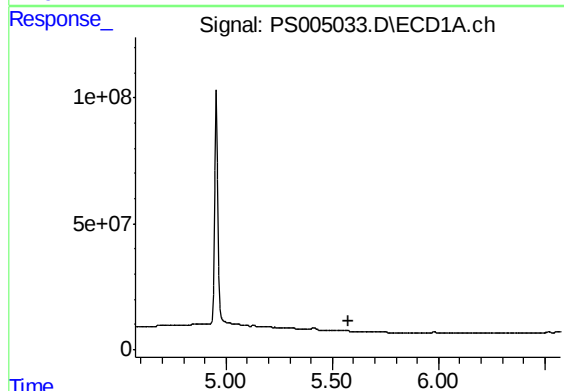


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.574 min
Response: 0
Conc: N.D.

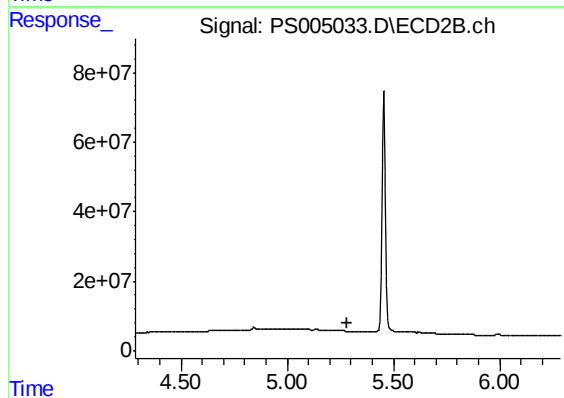

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.285 min
Response: 0
Conc: N.D.

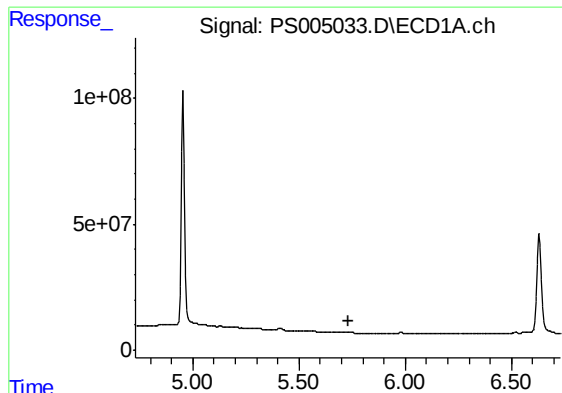

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

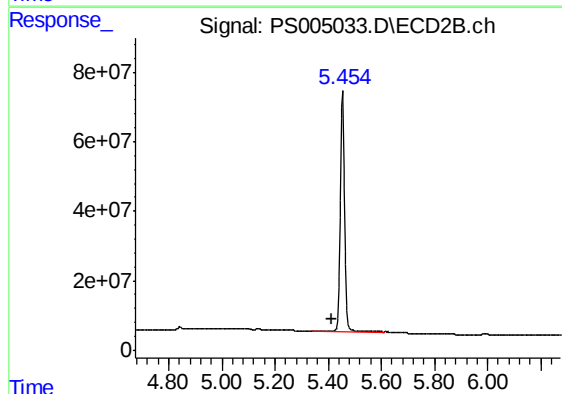


#5 DICAMBA

R.T.: 5.454 min
Delta R.T.: 0.037 min
Response: 759042287
Conc: 197.64 ng/ml

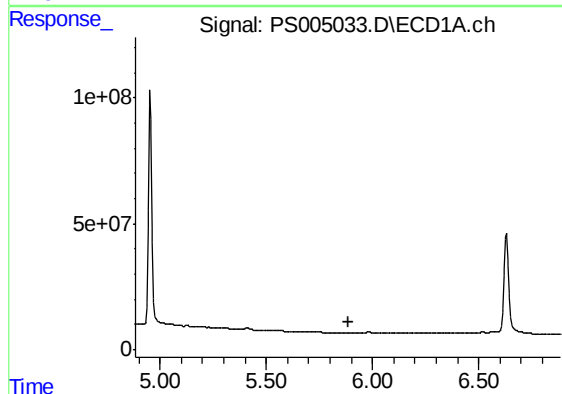


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.885 min
Response: 0
Conc: N.D.

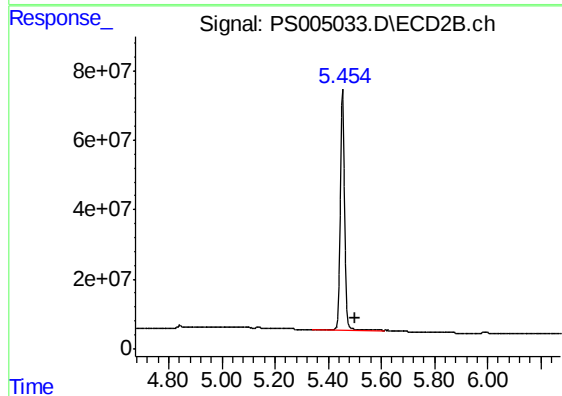

#6 MCPP


R.T.: 5.454 min
Delta R.T.: -0.046 min
Response: 759042287
Conc: 262.69 ug/ml

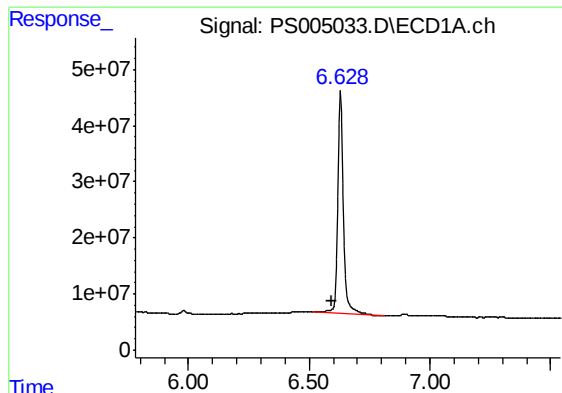

#9 2,4-D


R.T.: 6.629 min
Delta R.T.: 0.033 min
Response: 637794392
Conc: 472.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

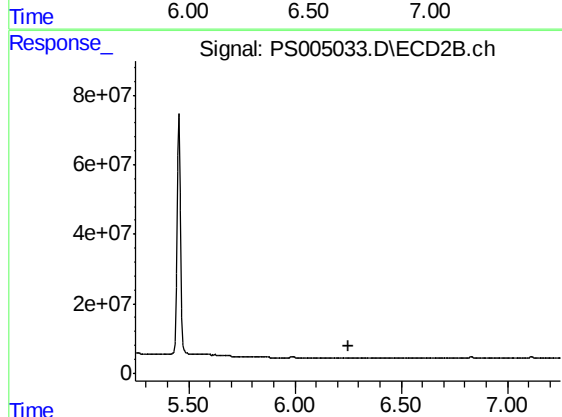


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

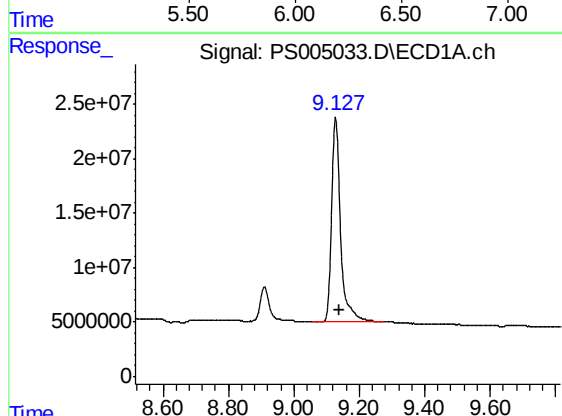


#15 Picloram

R.T.: 9.128 min
Delta R.T.: -0.012 min
Response: 358059369
Conc: 36.07 ng/ml

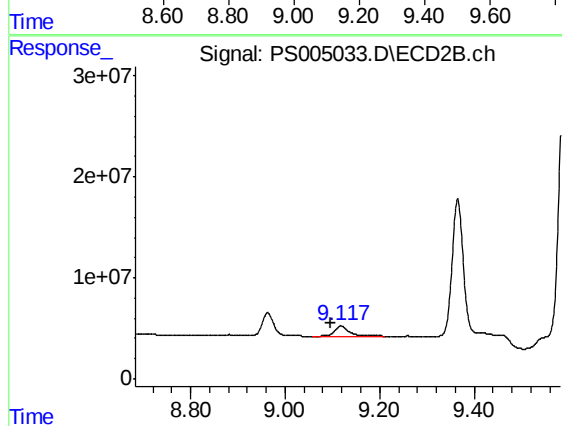

#15 Picloram


R.T.: 9.118 min
Delta R.T.: 0.023 min
Response: 21495190
Conc: 3.15 ng/ml

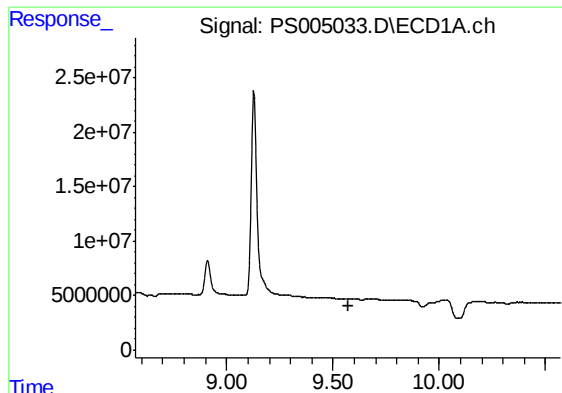

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

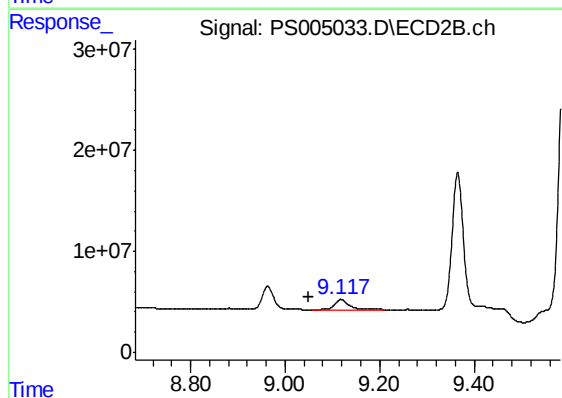

#16 DCPA

R.T.: 9.118 min
Delta R.T.: 0.068 min
Response: 21495190
Conc: 3.26 ng/ml