

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
 Data File : PS005039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 10:34
 Operator : SM\AJ
 Sample : PB120604BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB120604BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 11:35:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.573	5.284	613.8E6	442.7E6	465.788	443.837
Target Compounds							
2) T	3,5-DICHL...	0.000	4.602	0	57852509	N.D.	45.205
3) T	4-Nitroph...	5.377	0.000	11970692	0	26.282	N.D. #
5) T	DICAMBA	5.672	0.000	6720914	0	1.187	N.D. #
7) T	MCPA	5.978	5.676	39742046	20369721	6.342	4.832
8) T	DICHLORPROP	0.000	5.979	0	41151299	N.D.	42.371
9) T	2,4-D	6.657	0.000	60358852	0	44.732	N.D. #
15) T	Picloram	0.000	9.114	0	26734183	N.D.	3.919
16) T	DCPA	0.000	9.114	0	26734183	N.D.	4.054



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
Data File : PS005039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 10:34
Operator : SM\AJ
Sample : PB120604BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB120604BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 11:35:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

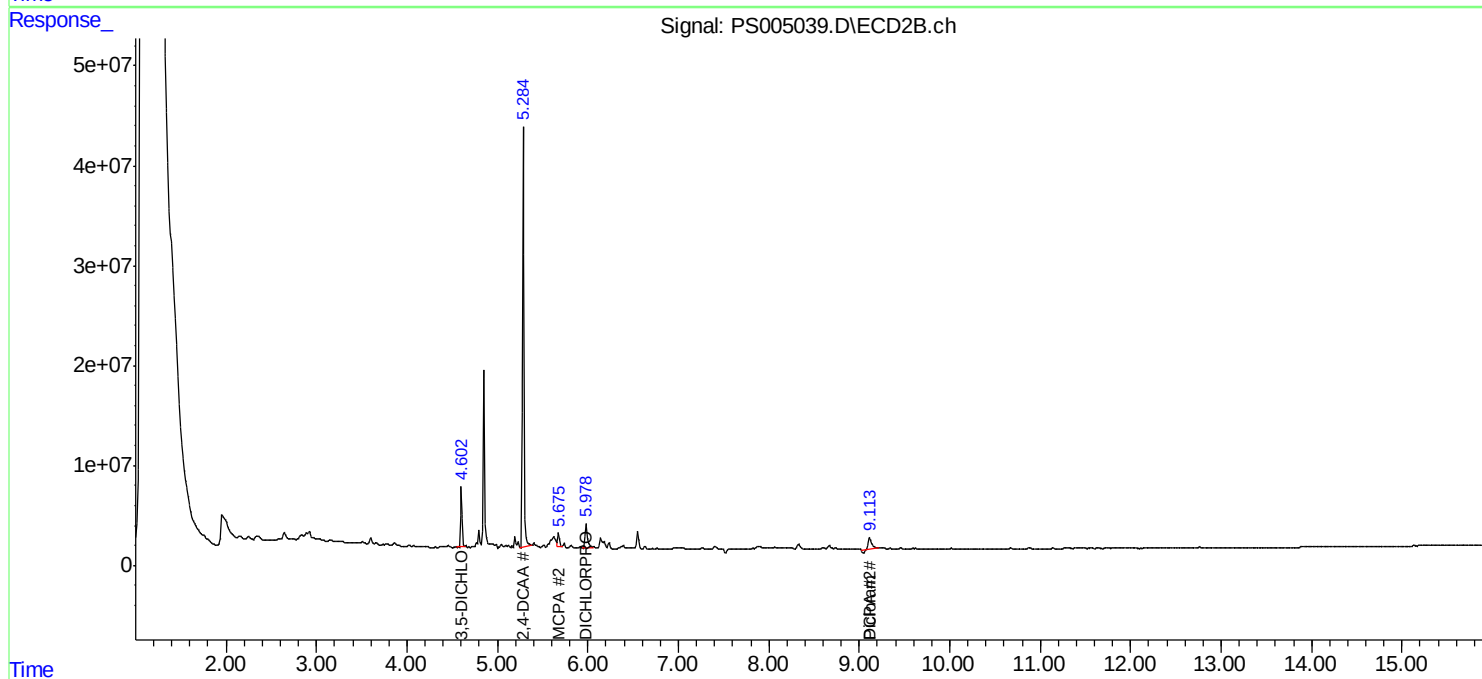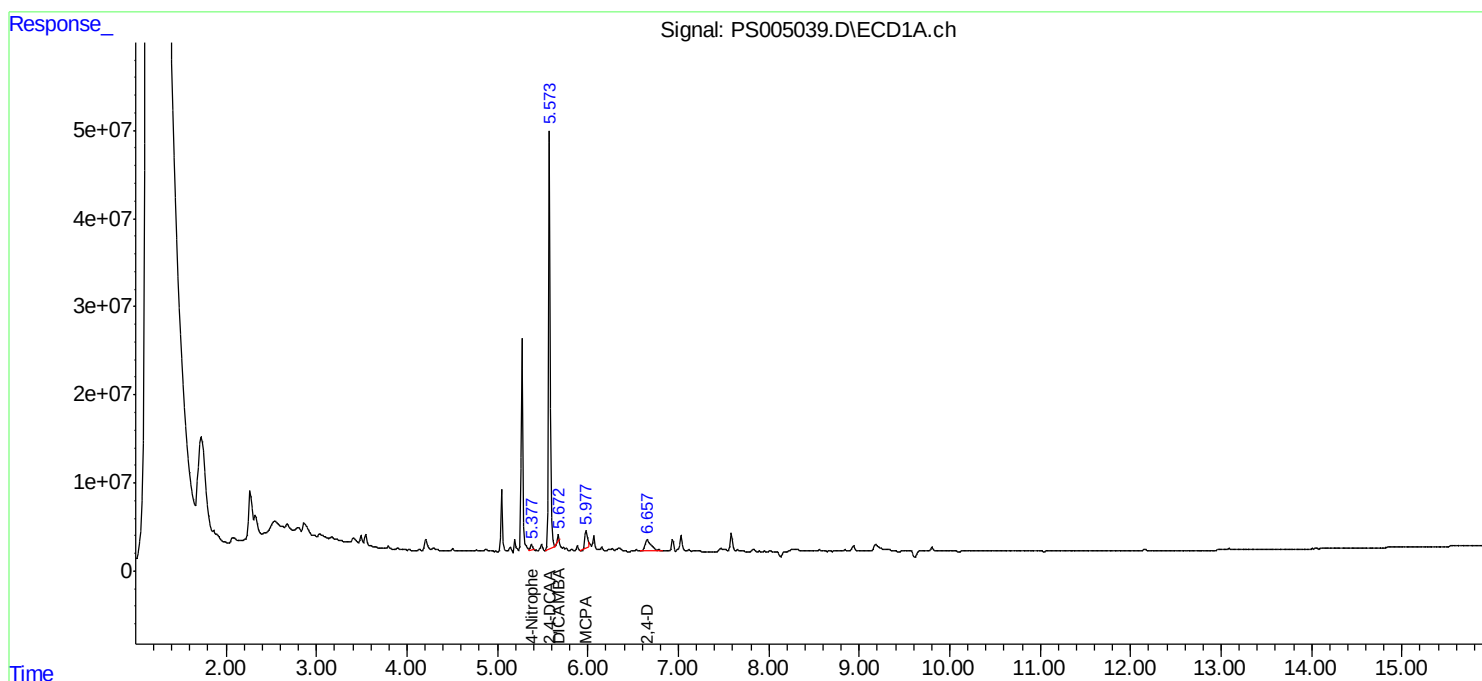


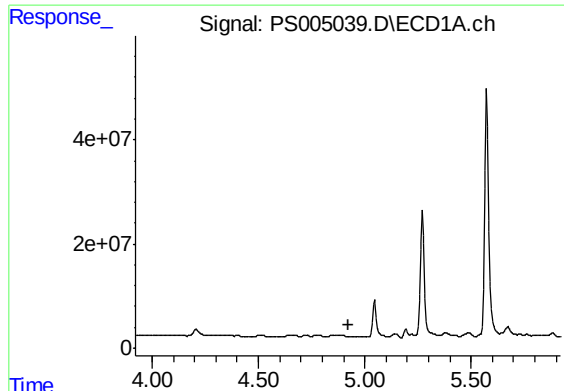

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.922 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB120604BL

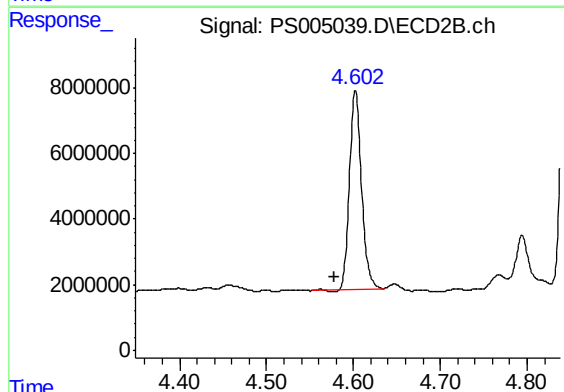


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.602 min
Delta R.T.: 0.025 min
Response: 57852509
Conc: 45.20 ng/ml

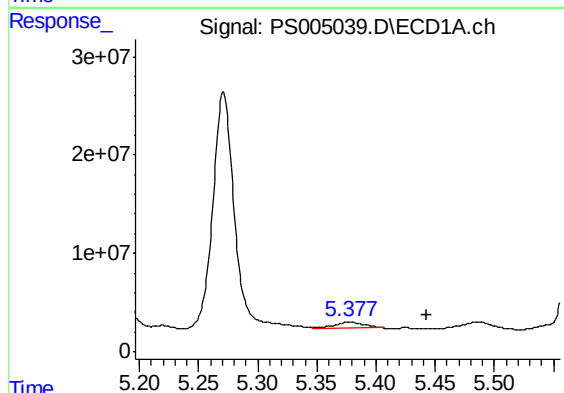


#3 4-Nitrophenol

R.T.: 5.377 min
Delta R.T.: -0.065 min
Response: 11970692
Conc: 26.28 ng/ml

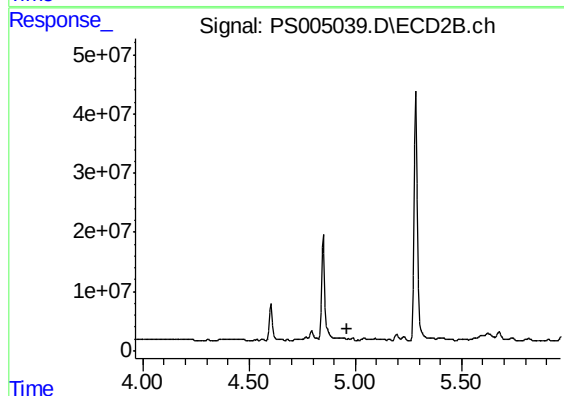

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.965 min
Response: 0
Conc: N.D.

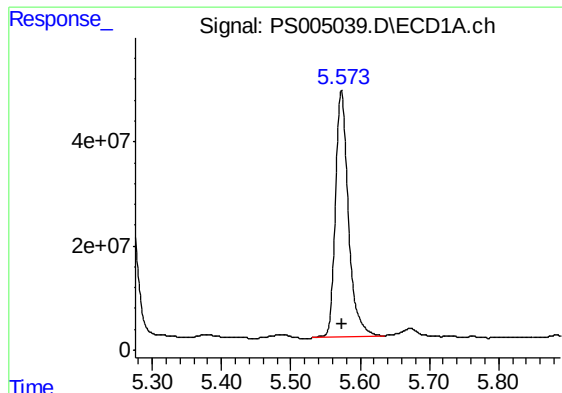

#4 2,4-DCAA


R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 613813561
Conc: 465.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB120604BL

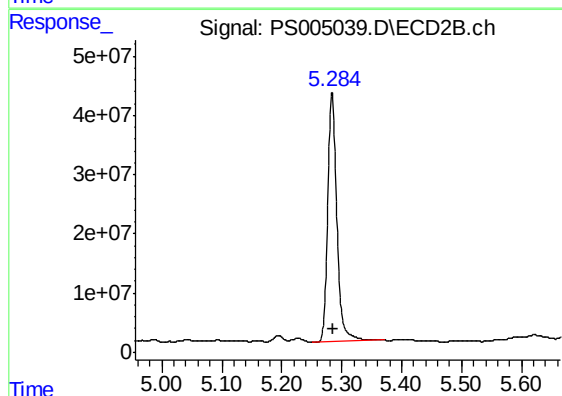


#4 2,4-DCAA

R.T.: 5.284 min
Delta R.T.: -0.001 min
Response: 442743301
Conc: 443.84 ng/ml

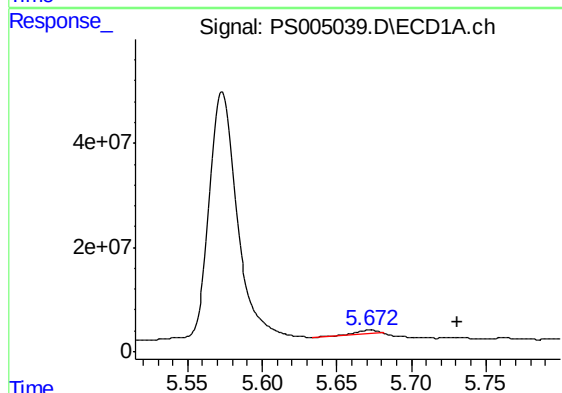


#5 DICAMBA

R.T.: 5.672 min
Delta R.T.: -0.059 min
Response: 6720914
Conc: 1.19 ng/ml

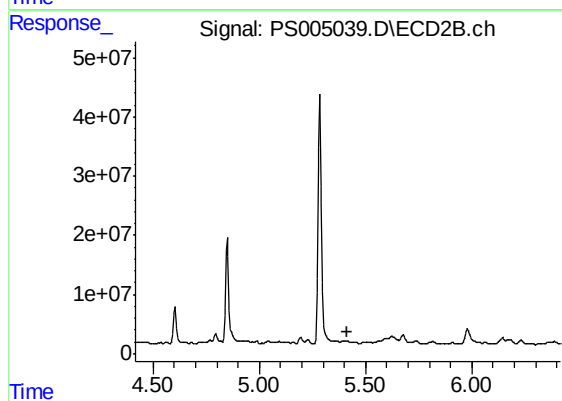

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.417 min
Response: 0
Conc: N.D.

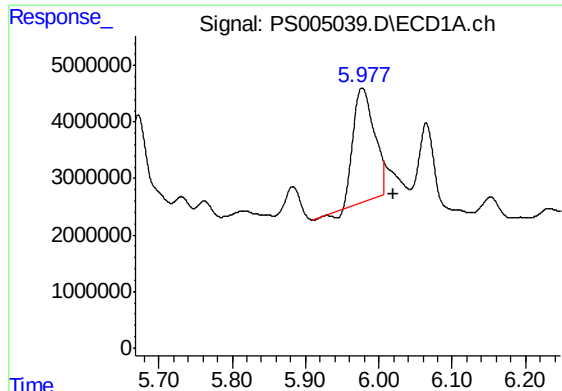

#7 MCPA


R.T.: 5.978 min
Delta R.T.: -0.042 min
Response: 39742046
Conc: 6.34 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB120604BL

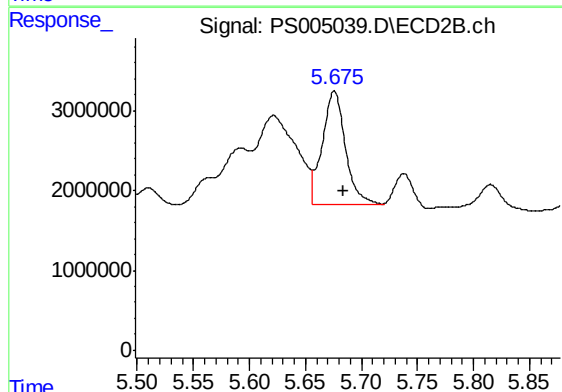


#7 MCPA

R.T.: 5.676 min
Delta R.T.: -0.008 min
Response: 20369721
Conc: 4.83 ug/ml

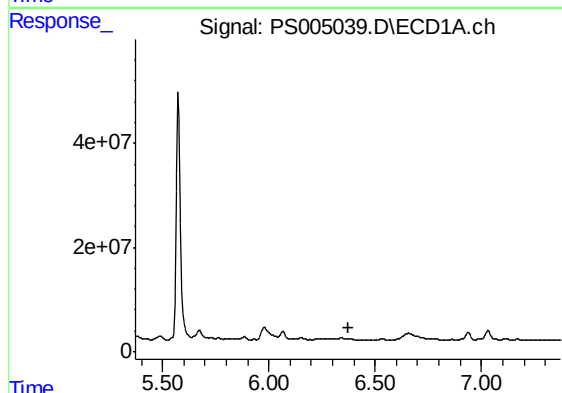


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.372 min
Response: 0
Conc: N.D.

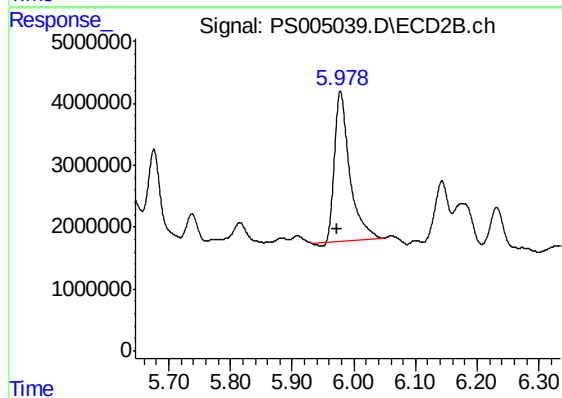

#8 DICHLORPROP


R.T.: 5.979 min
Delta R.T.: 0.005 min
Response: 41151299
Conc: 42.37 ng/ml

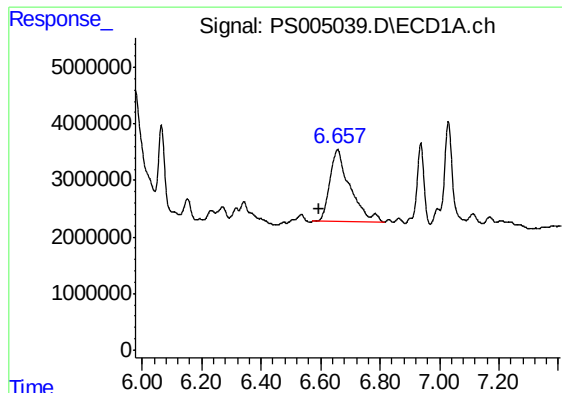

#9 2,4-D


R.T.: 6.657 min
Delta R.T.: 0.061 min
Response: 60358852
Conc: 44.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB120604BL

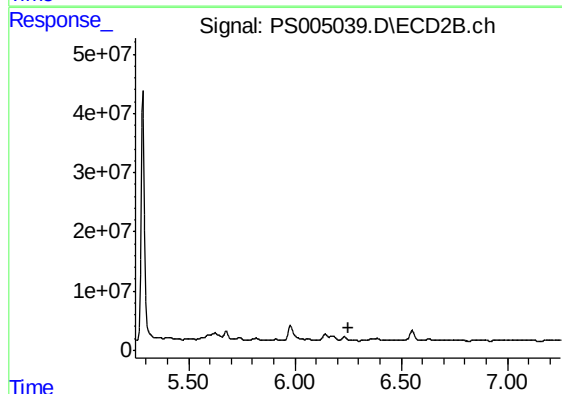


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

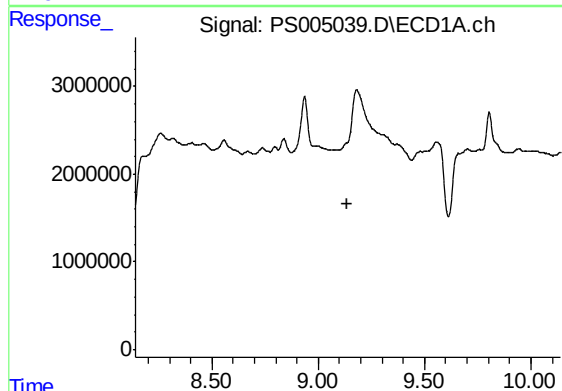


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.139 min
Response: 0
Conc: N.D.

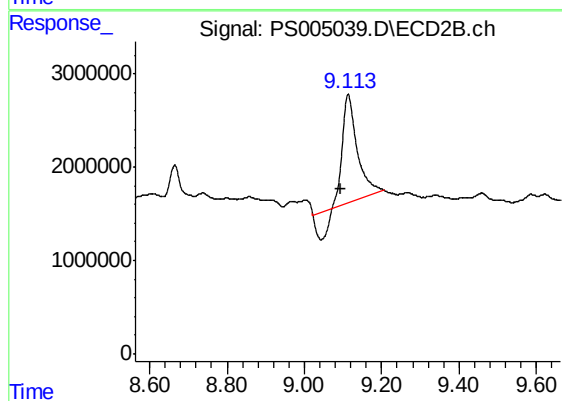

#15 Picloram


R.T.: 9.114 min
Delta R.T.: 0.018 min
Response: 26734183
Conc: 3.92 ng/ml

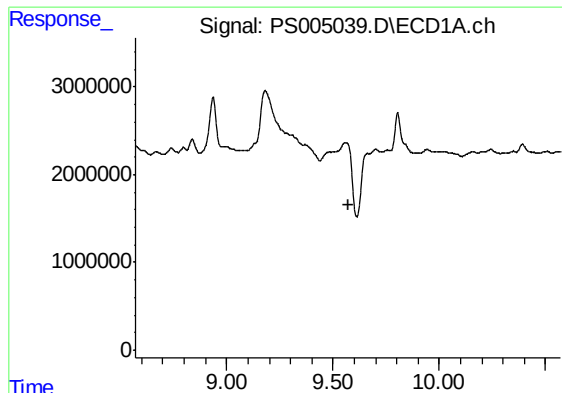

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB120604BL

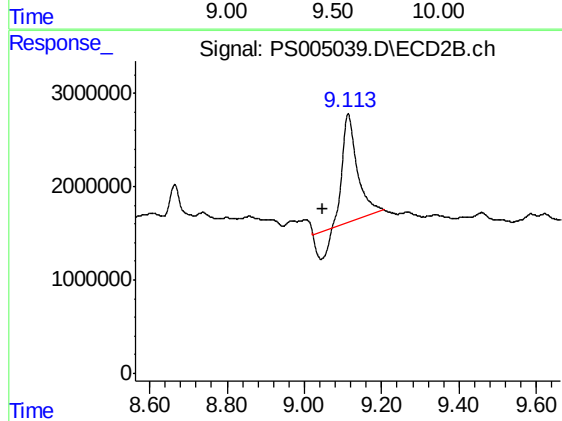

#16 DCPA

R.T.: 9.114 min
Delta R.T.: 0.064 min
Response: 26734183
Conc: 4.05 ng/ml