

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
 Data File : PS005041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 11:18
 Operator : SM\AJ
 Sample : K3303-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BAT-B13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 14:29:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.589	5.302	404.0E6	283.0E6	306.542	283.732
Target Compounds							
2) T	3,5-DICHL...	0.000	4.621	0	64634957	N.D.	50.504
3) T	4-Nitroph...	5.478	4.982	17986514	17138869	39.489	37.795
5) T	DICAMBA	0.000	5.430	0	28368111	N.D.	7.387
6) T	MCP	5.818	0.000	41272019	0	9.253	N.D. #
7) T	MCPA	6.046	5.694	17123474	18797976	2.732	4.459 #
8) T	DICHLORPROP	0.000	6.006	0	100.3E6	N.D.	103.260
9) T	2,4-D	6.603	0.000	16260402	0	12.051	N.D. #
10) T	Pentachlo...	0.000	6.569	0	24862509	N.D.	1.930
11) T	2,4,5-TP ...	0.000	7.047	0	19926364	N.D.	3.723
14) T	DINOSEB	9.322	0.000	51609280	0	7.870	N.D. #
15) T	Picloram	9.118	0.000	22440938	0	2.260	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
Data File : PS005041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 11:18
Operator : SM\AJ
Sample : K3303-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
BAT-B13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 14:29:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

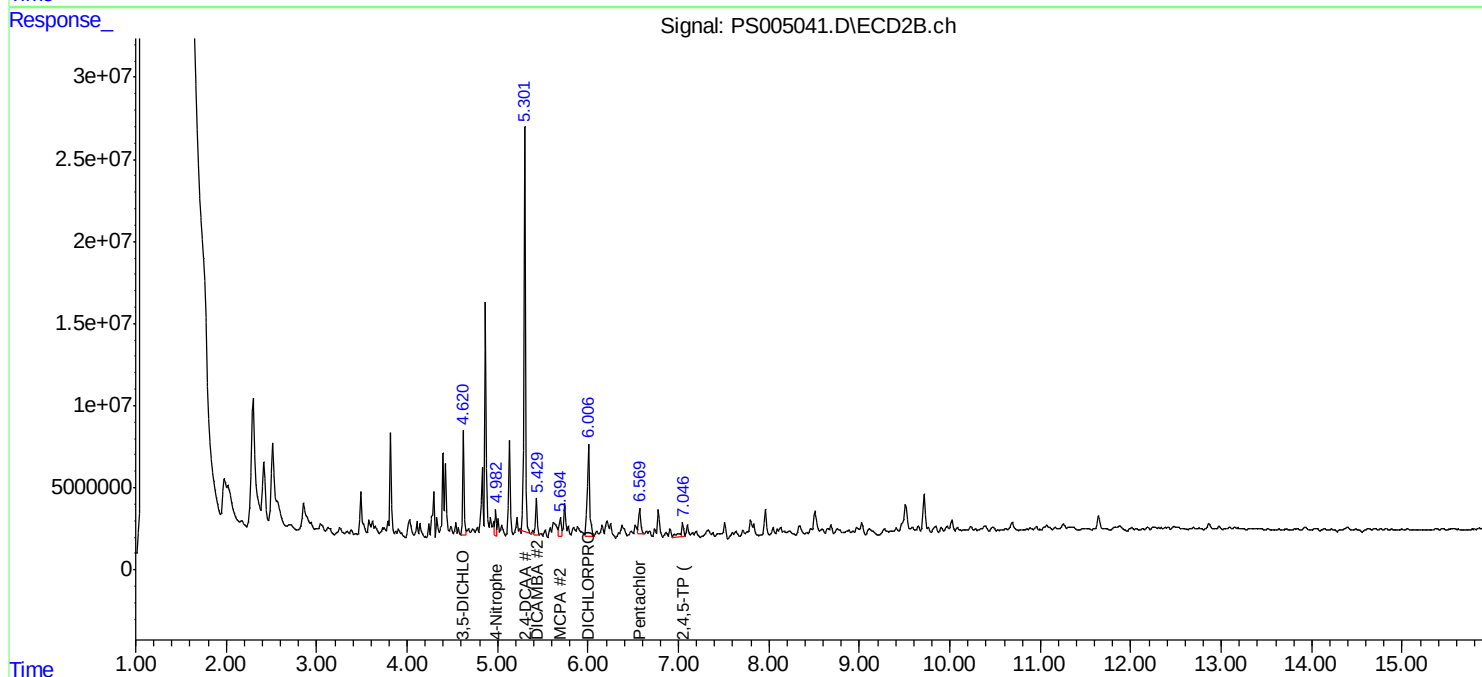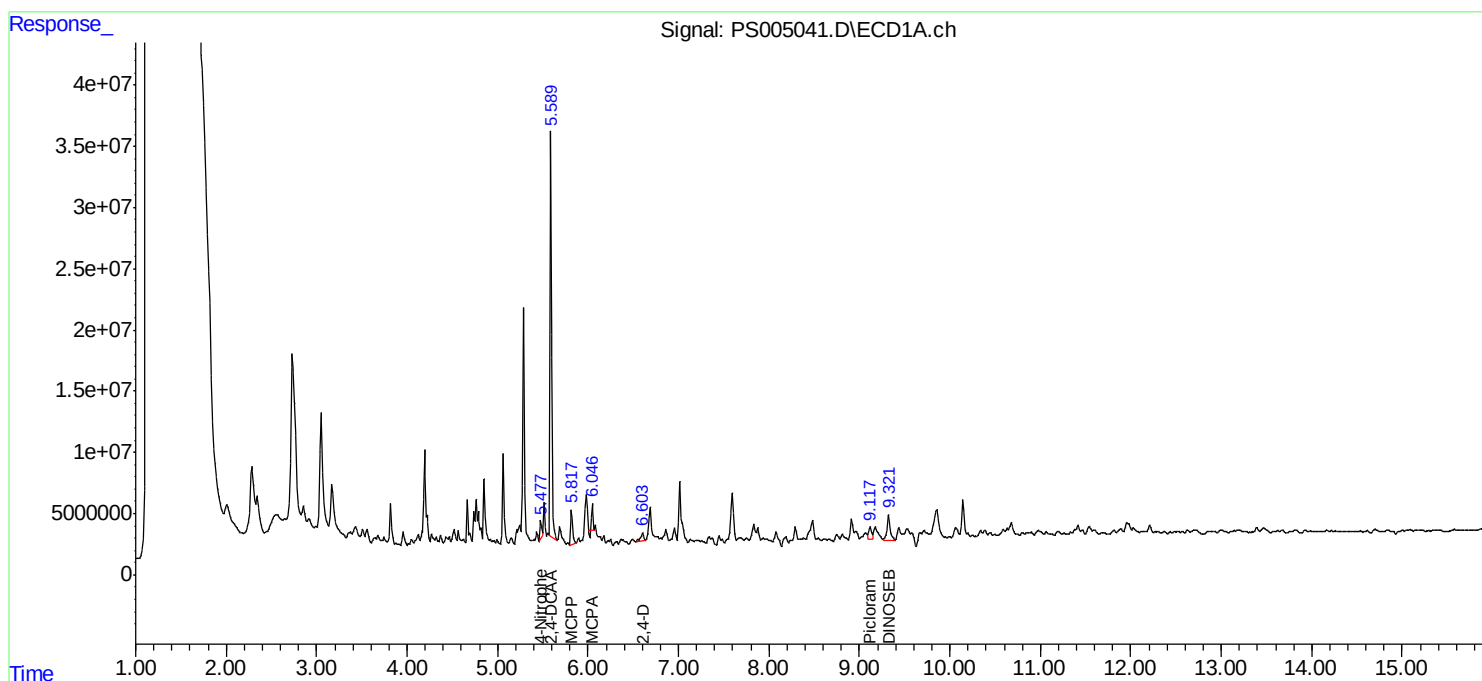


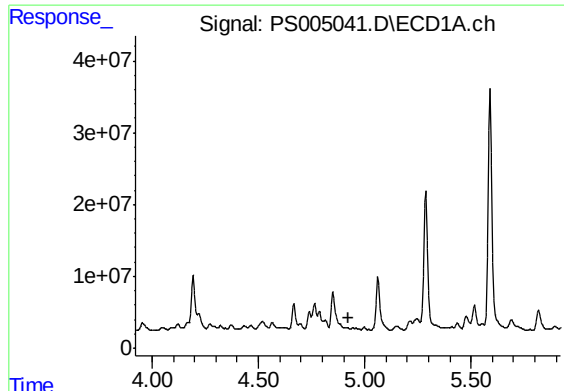

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.922 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B13

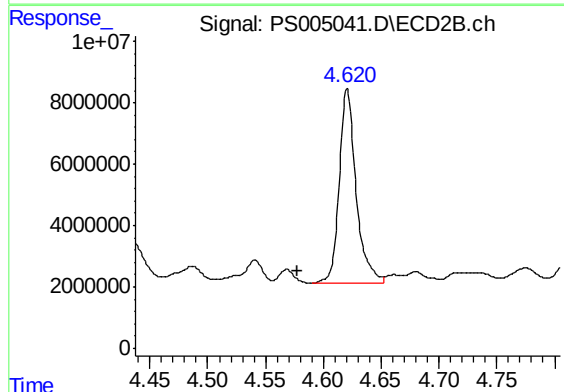


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.621 min
Delta R.T.: 0.043 min
Response: 64634957
Conc: 50.50 ng/ml

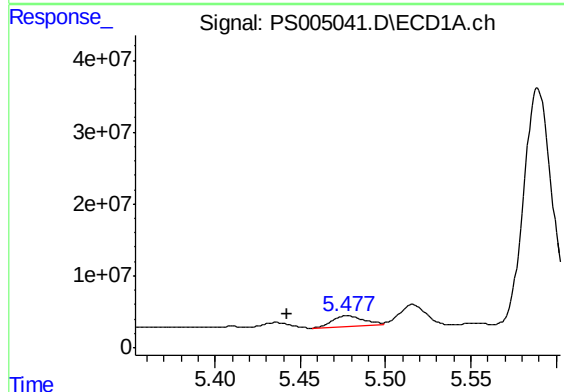


#3 4-Nitrophenol

R.T.: 5.478 min
Delta R.T.: 0.035 min
Response: 17986514
Conc: 39.49 ng/ml

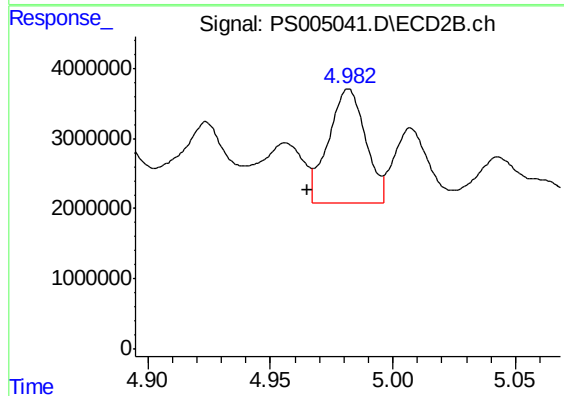

#3 4-Nitrophenol


R.T.: 4.982 min
Delta R.T.: 0.017 min
Response: 17138869
Conc: 37.80 ng/ml

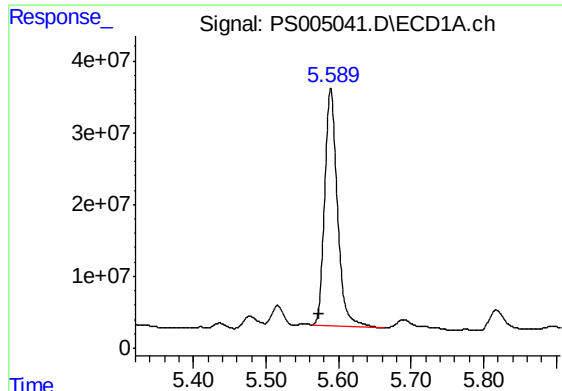

#4 2,4-DCAA


R.T.: 5.589 min
Delta R.T.: 0.016 min
Response: 403959540
Conc: 306.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B13

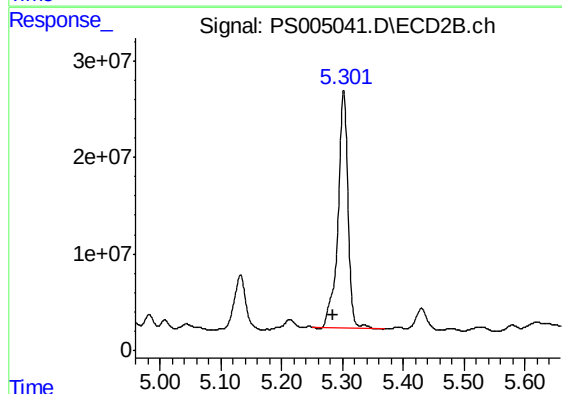


#4 2,4-DCAA

R.T.: 5.302 min
Delta R.T.: 0.017 min
Response: 283032761
Conc: 283.73 ng/ml

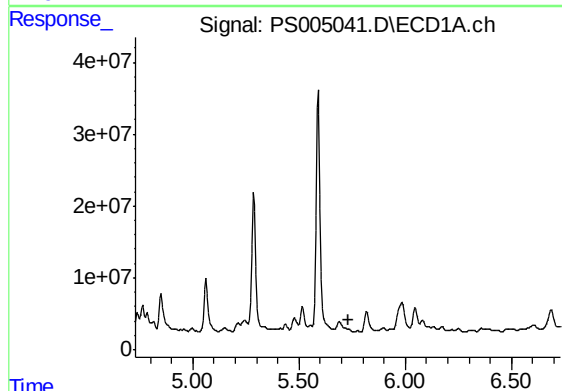


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.731 min
Response: 0
Conc: N.D.

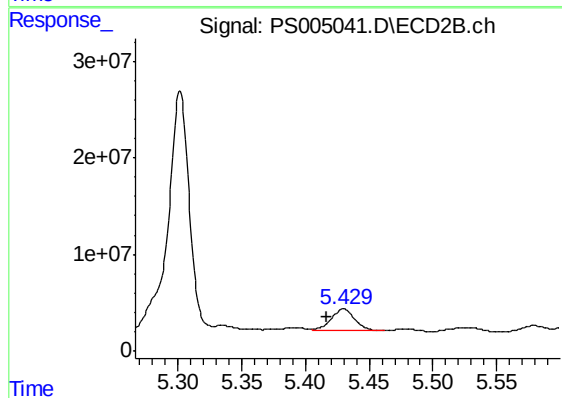

#5 DICAMBA


R.T.: 5.430 min
Delta R.T.: 0.013 min
Response: 28368111
Conc: 7.39 ng/ml

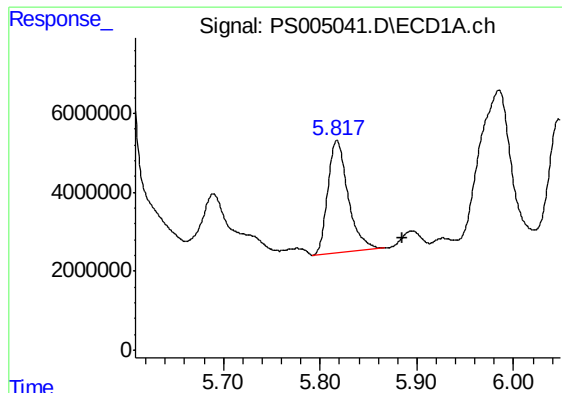

#6 MCPP


R.T.: 5.818 min
Delta R.T.: -0.067 min
Response: 41272019
Conc: 9.25 ug/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B13

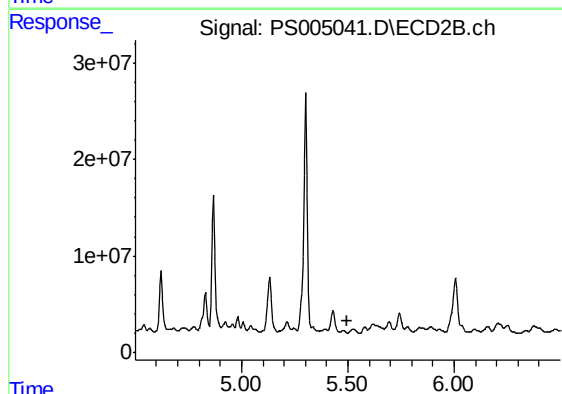


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.500 min
Response: 0
Conc: N.D.

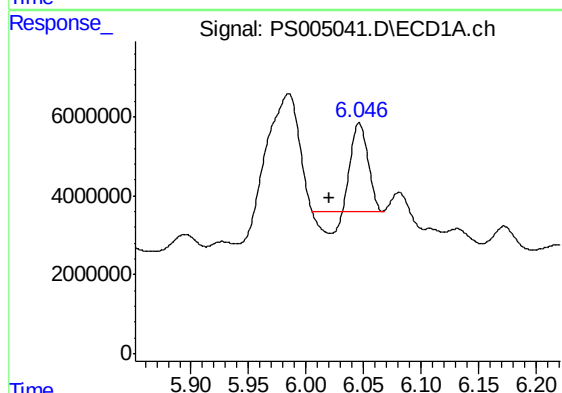


#7 MCPA

R.T.: 6.046 min
Delta R.T.: 0.026 min
Response: 17123474
Conc: 2.73 ug/ml

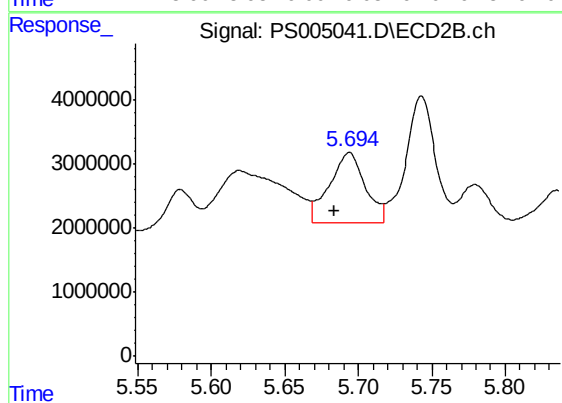

#7 MCPA


R.T.: 5.694 min
Delta R.T.: 0.010 min
Response: 18797976
Conc: 4.46 ug/ml

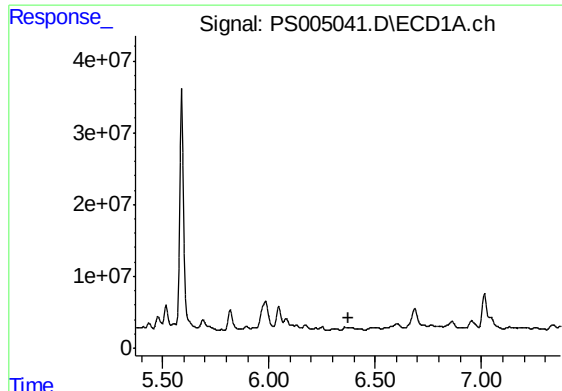

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B13

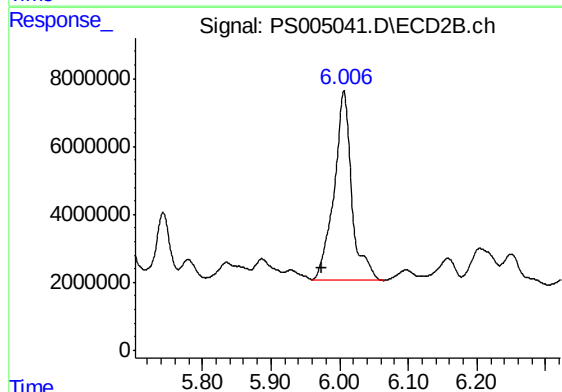


#8 DICHLORPROP

R.T.: 6.006 min
Delta R.T.: 0.033 min
Response: 100287991
Conc: 103.26 ng/ml

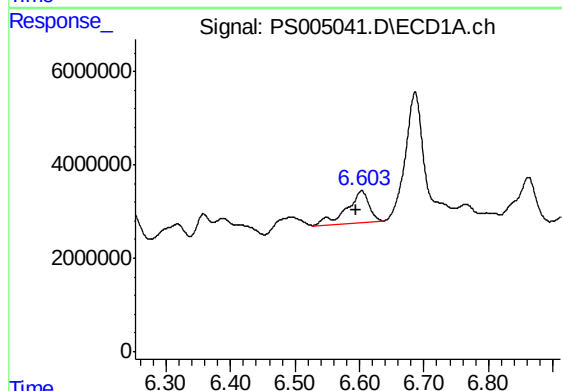


#9 2,4-D

R.T.: 6.603 min
Delta R.T.: 0.007 min
Response: 16260402
Conc: 12.05 ng/ml

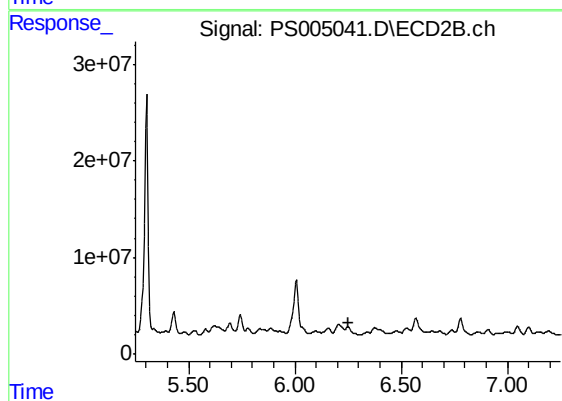

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

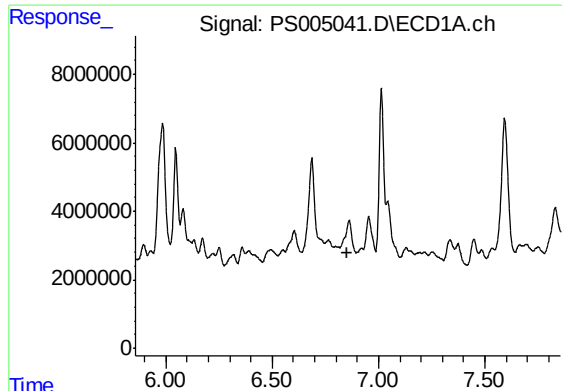

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.856 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B13

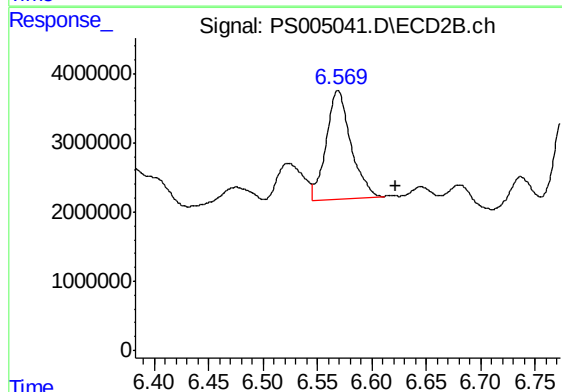


#10 Pentachlorophenol

R.T.: 6.569 min
Delta R.T.: -0.053 min
Response: 24862509
Conc: 1.93 ng/ml

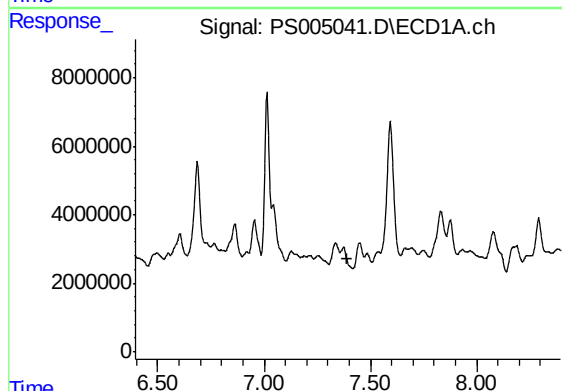


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.395 min
Response: 0
Conc: N.D.

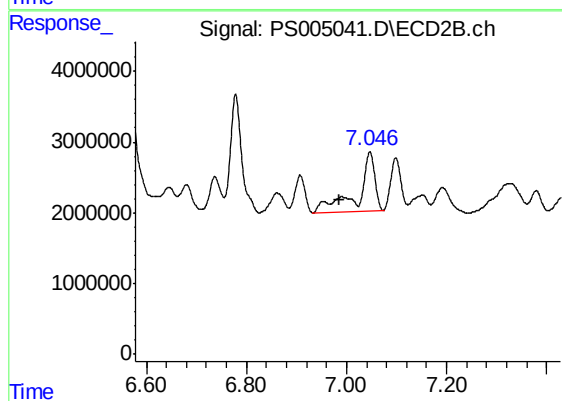

#11 2,4,5-TP (SILVEX)


R.T.: 7.047 min
Delta R.T.: 0.061 min
Response: 19926364
Conc: 3.72 ng/ml

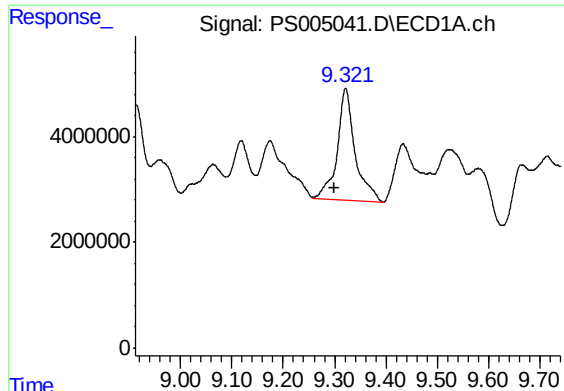

#14 DINOSEB


R.T.: 9.322 min
Delta R.T.: 0.022 min
Response: 51609280
Conc: 7.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B13

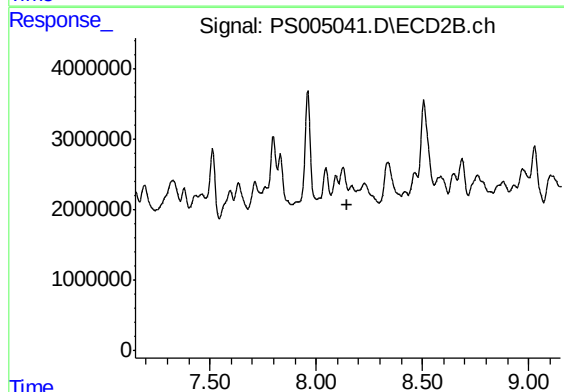


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.150 min
Response: 0
Conc: N.D.

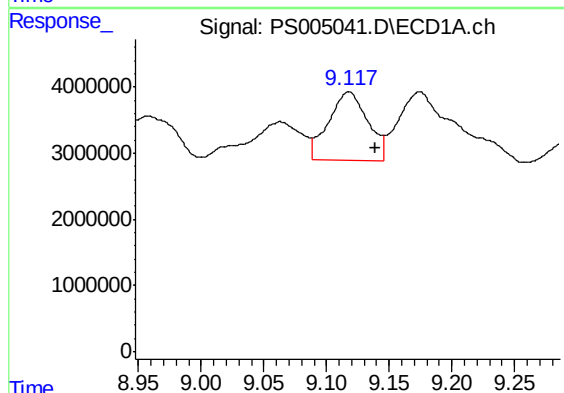

#15 Picloram

R.T.: 9.118 min
Delta R.T.: -0.022 min
Response: 22440938
Conc: 2.26 ng/ml

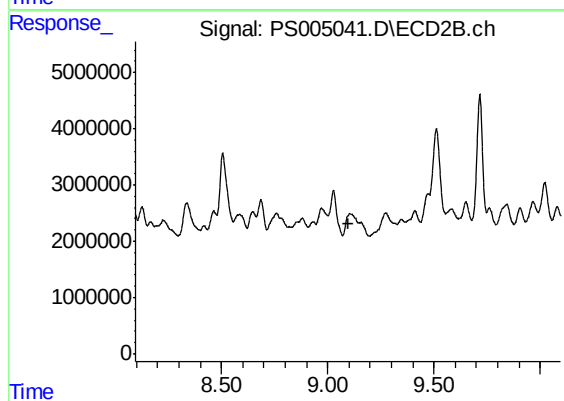

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.