

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
 Data File : PS005045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 12:46
 Operator : SM\AJ
 Sample : K3303-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BAT-B02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 14:30:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.570	5.262	27837204	16144154	21.124	16.184
Target Compounds							
2) T	3,5-DICHL...	0.000	4.639	0	62146979	N.D.	48.560
3) T	4-Nitroph...	5.452	4.975	53336797	41808356	117.101	92.198
5) T	DICAMBA	5.708	0.000	27066346	0	4.782	N.D. #
6) T	MCP	5.944	0.000	22096702	0	4.954	N.D. #
7) T	MCPA	0.000	5.712	0	24407101	N.D.	5.790
8) T	DICHLORPROP	0.000	6.013	0	14892073	N.D.	15.333
9) T	2,4-D	6.606	6.239	38484093	71657584	28.521	66.959 #
10) T	Pentachlo...	6.880	6.618	70422457	60670164	3.661	4.709 #
11) T	2,4,5-TP ...	0.000	7.032	0	23654362	N.D.	4.419
12) T	2,4,5-T	7.622	0.000	68903063	0	8.623	N.D. #
13) T	2,4-DB	8.207	0.000	13482820	0	14.687	N.D. #
14) T	DINOSEB	0.000	8.139	0	9977493	N.D.	2.568
15) T	Picloram	9.190	0.000	26640133	0	2.683	N.D. #
16) T	DCPA	9.559	0.000	99431694	0	10.241	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
Data File : PS005045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 12:46
Operator : SM\AJ
Sample : K3303-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BAT-B02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 14:30:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

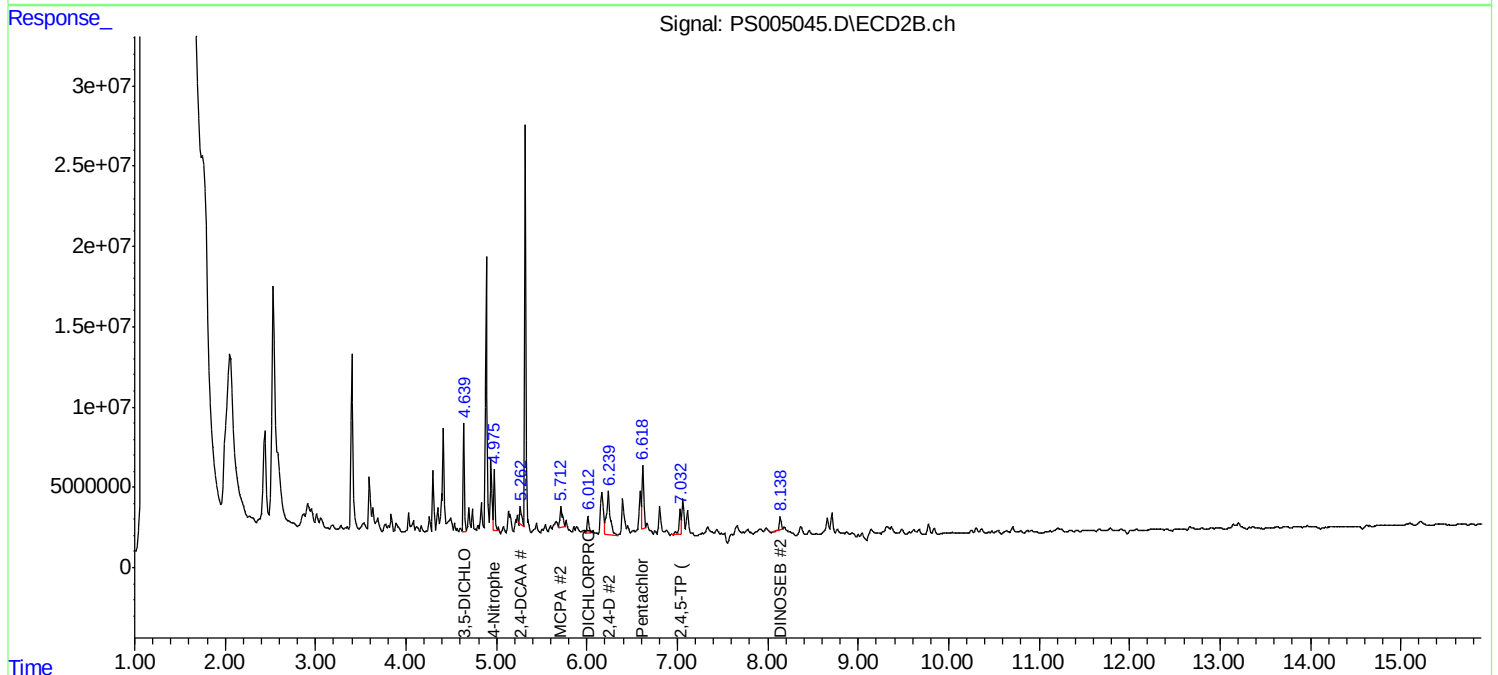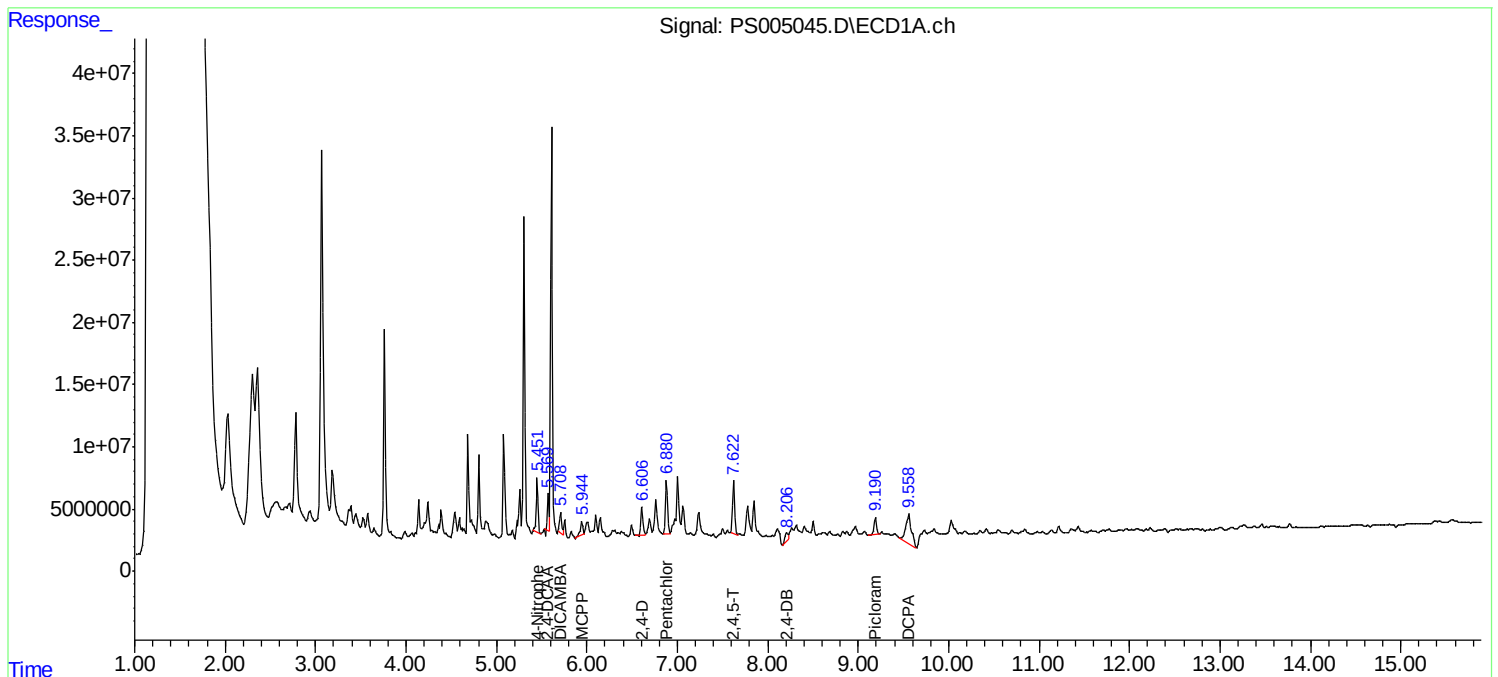


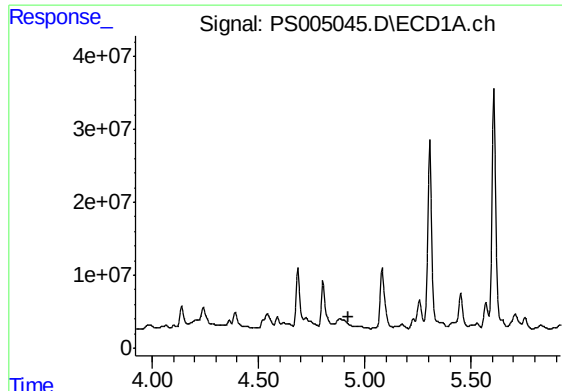

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.922 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B02

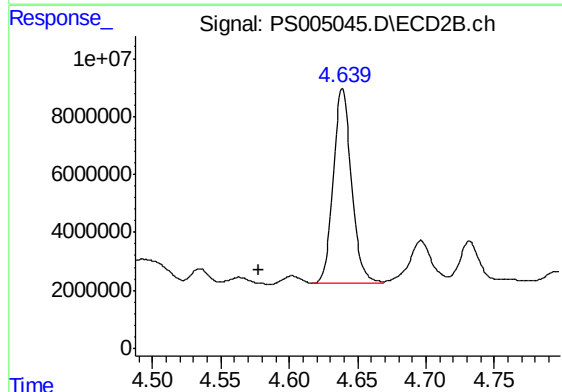


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.639 min
Delta R.T.: 0.061 min
Response: 62146979
Conc: 48.56 ng/ml

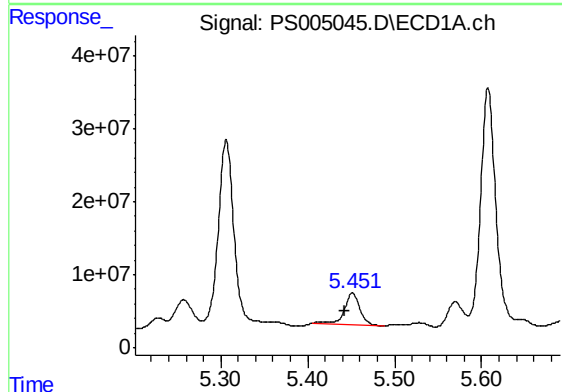


#3 4-Nitrophenol

R.T.: 5.452 min
Delta R.T.: 0.009 min
Response: 53336797
Conc: 117.10 ng/ml

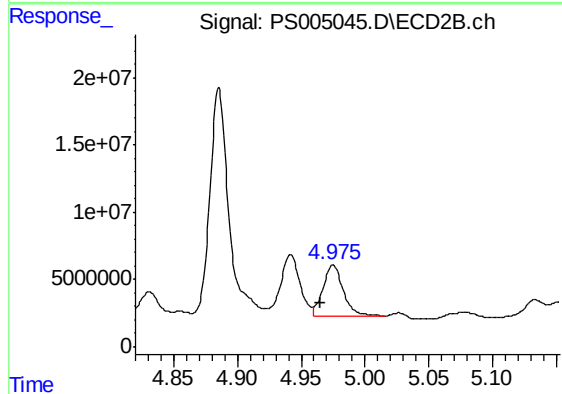

#3 4-Nitrophenol


R.T.: 4.975 min
Delta R.T.: 0.010 min
Response: 41808356
Conc: 92.20 ng/ml

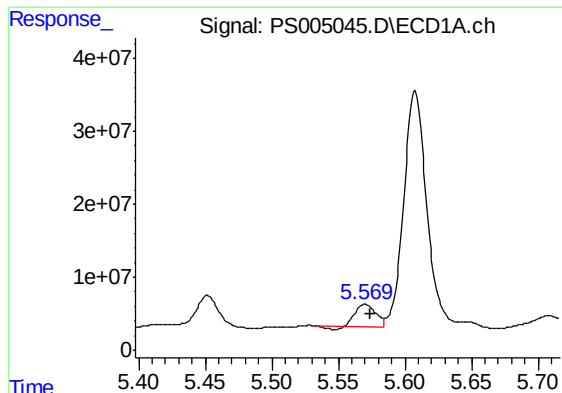

#4 2,4-DCAA


R.T.: 5.570 min
Delta R.T.: -0.004 min
Response: 27837204
Conc: 21.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B02

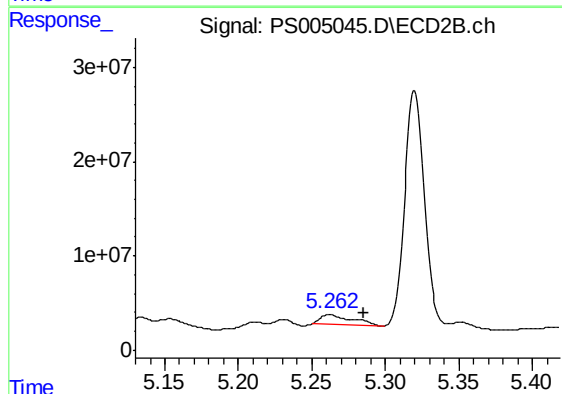


#4 2,4-DCAA

R.T.: 5.262 min
Delta R.T.: -0.023 min
Response: 16144154
Conc: 16.18 ng/ml

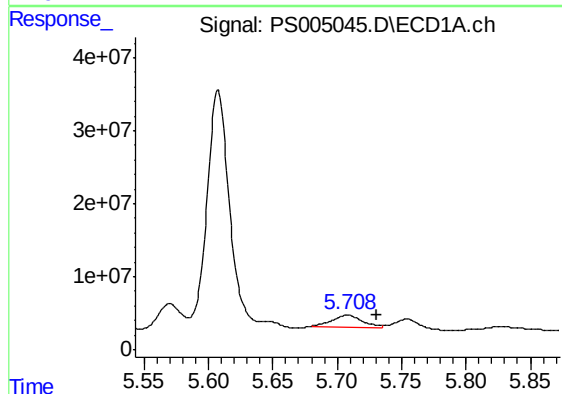


#5 DICAMBA

R.T.: 5.708 min
Delta R.T.: -0.023 min
Response: 27066346
Conc: 4.78 ng/ml

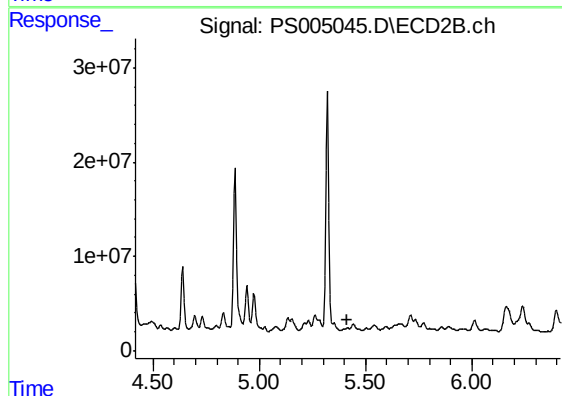

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.417 min
Response: 0
Conc: N.D.

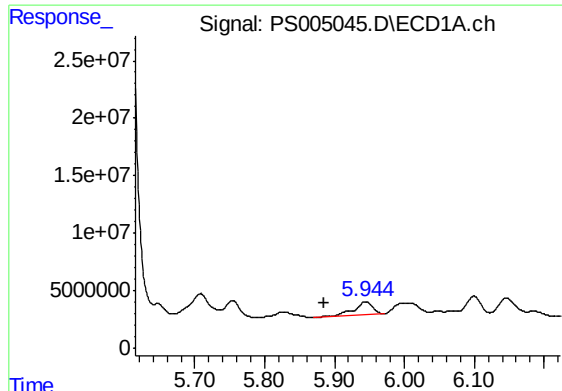

#6 MCPP


R.T.: 5.944 min
Delta R.T.: 0.059 min
Response: 22096702
Conc: 4.95 ug/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B02

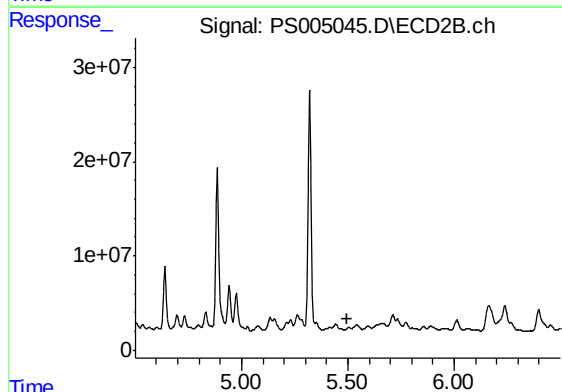


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.500 min
Response: 0
Conc: N.D.

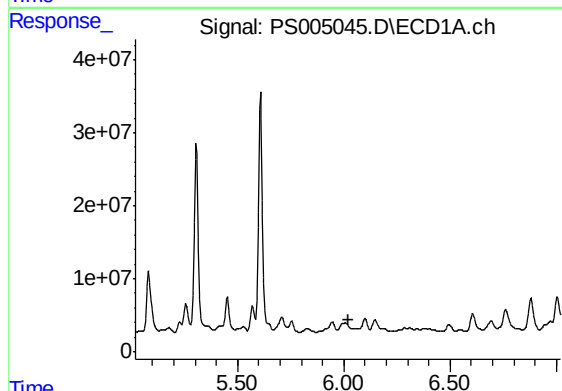


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.020 min
Response: 0
Conc: N.D.

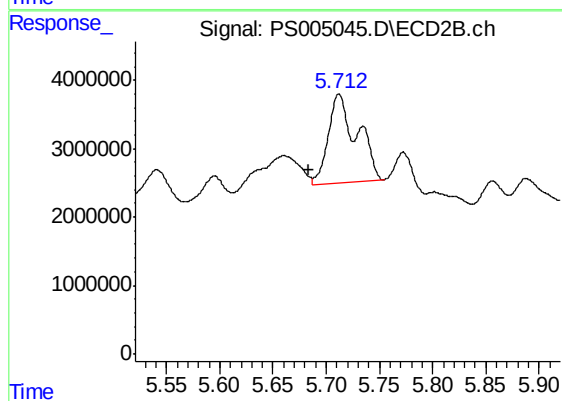

#7 MCPA


R.T.: 5.712 min
Delta R.T.: 0.028 min
Response: 24407101
Conc: 5.79 ug/ml

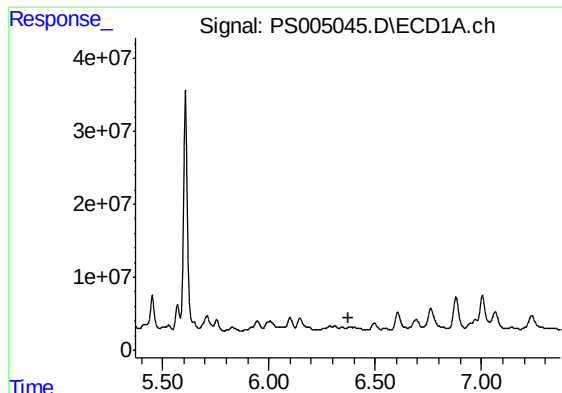

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B02

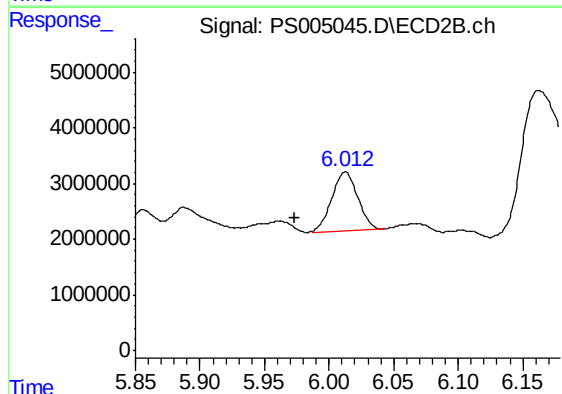


#8 DICHLORPROP

R.T.: 6.013 min
Delta R.T.: 0.039 min
Response: 14892073
Conc: 15.33 ng/ml

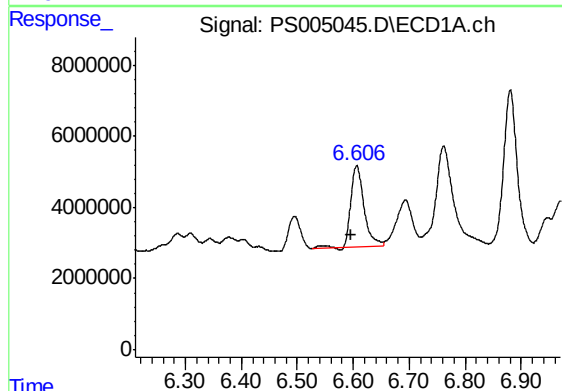


#9 2,4-D

R.T.: 6.606 min
Delta R.T.: 0.010 min
Response: 38484093
Conc: 28.52 ng/ml

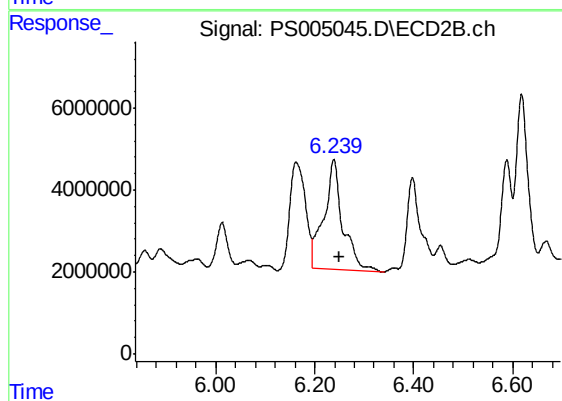

#9 2,4-D


R.T.: 6.239 min
Delta R.T.: -0.011 min
Response: 71657584
Conc: 66.96 ng/ml

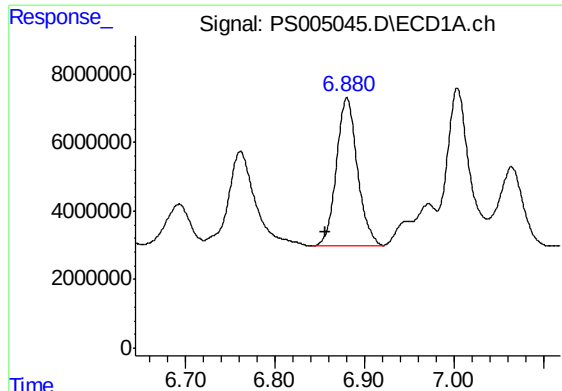

#10 Pentachlorophenol


R.T.: 6.880 min
Delta R.T.: 0.025 min
Response: 70422457
Conc: 3.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B02

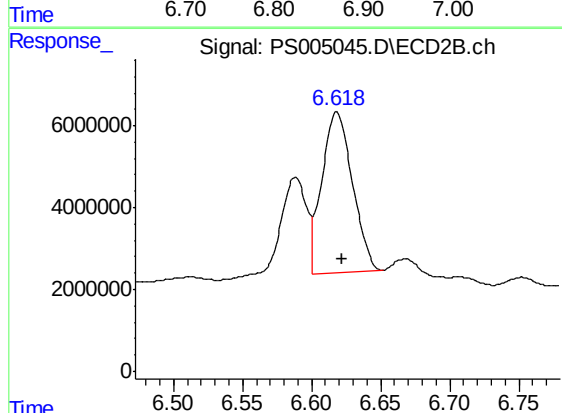


#10 Pentachlorophenol

R.T.: 6.618 min
Delta R.T.: -0.003 min
Response: 60670164
Conc: 4.71 ng/ml

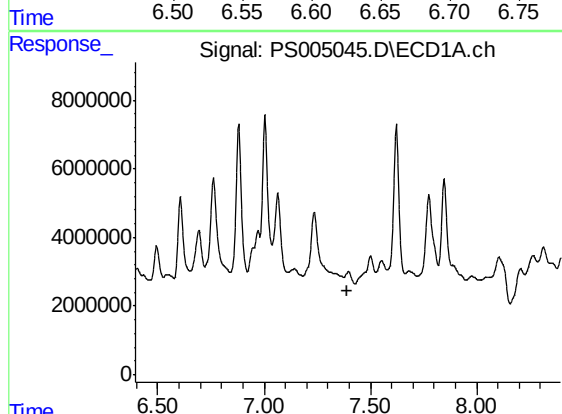


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.395 min
Response: 0
Conc: N.D.

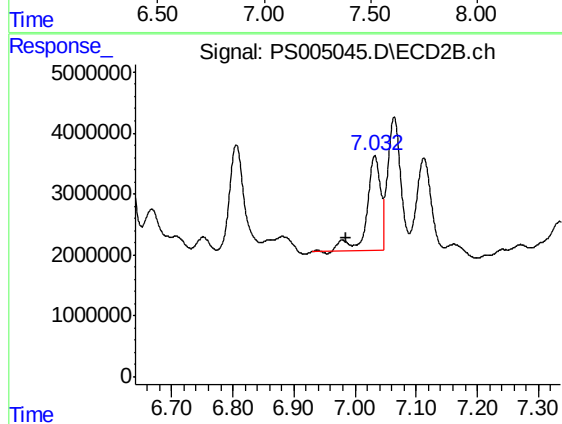

#11 2,4,5-TP (SILVEX)


R.T.: 7.032 min
Delta R.T.: 0.047 min
Response: 23654362
Conc: 4.42 ng/ml

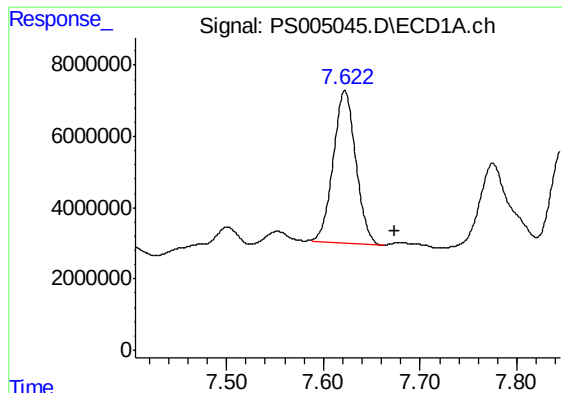

#12 2,4,5-T


R.T.: 7.622 min
Delta R.T.: -0.052 min
Response: 68903063
Conc: 8.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B02

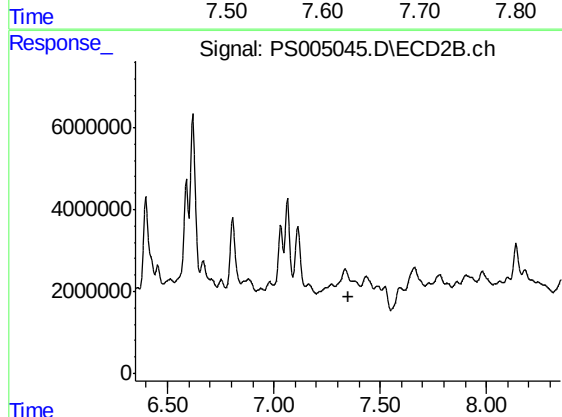


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.349 min
Response: 0
Conc: N.D.

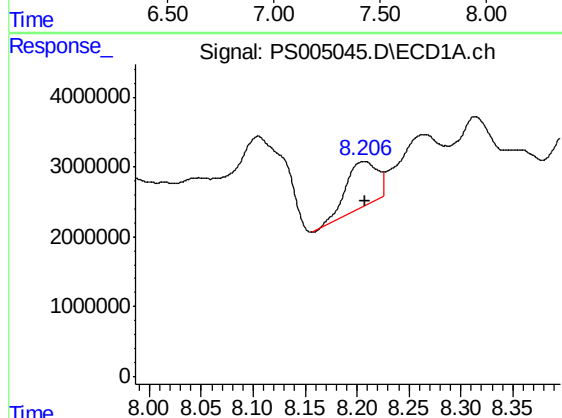


#13 2,4-DB

R.T.: 8.207 min
Delta R.T.: -0.002 min
Response: 13482820
Conc: 14.69 ng/ml

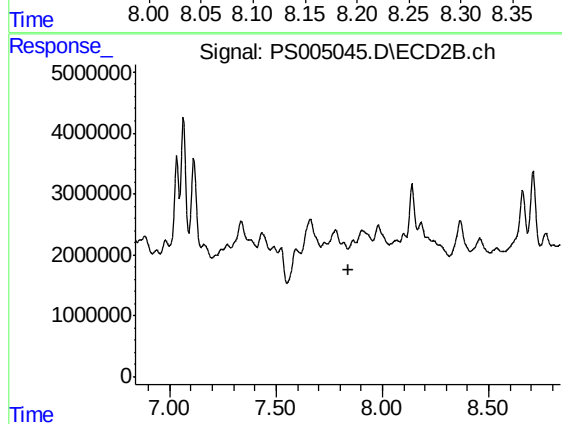

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

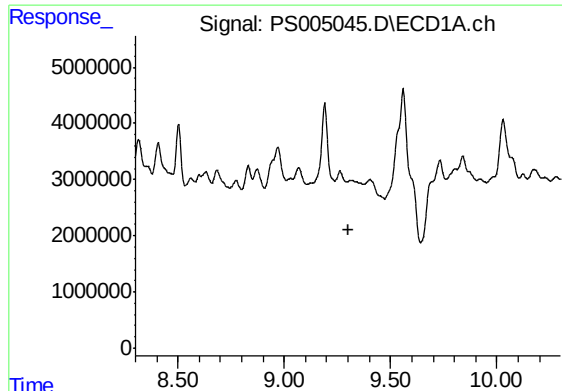

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.300 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B02

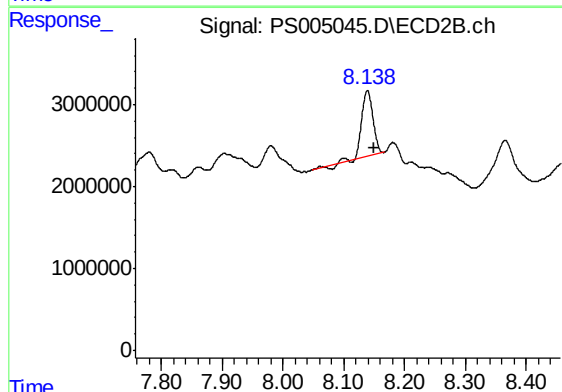


#14 DINOSEB

R.T.: 8.139 min
Delta R.T.: -0.011 min
Response: 9977493
Conc: 2.57 ng/ml

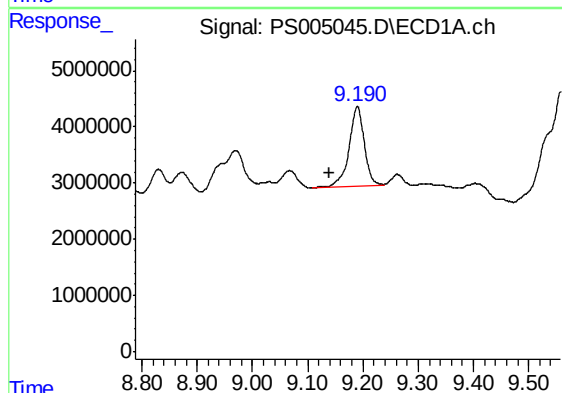


#15 Picloram

R.T.: 9.190 min
Delta R.T.: 0.051 min
Response: 26640133
Conc: 2.68 ng/ml

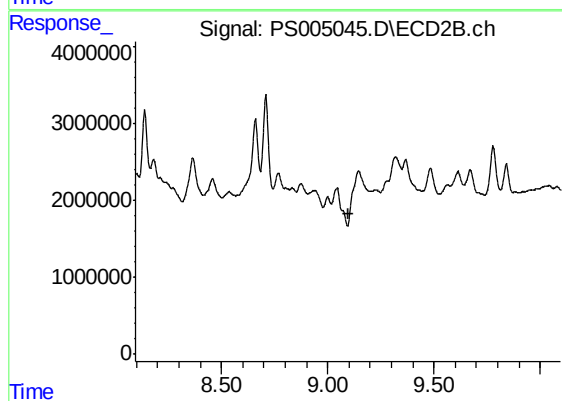

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 9.096 min
Response: 0
Conc: N.D.

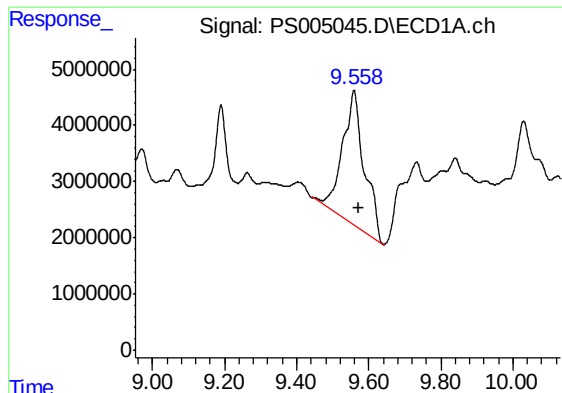

#16 DCPA

R.T.: 9.559 min
Delta R.T.: -0.012 min
Response: 99431694
Conc: 10.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B02

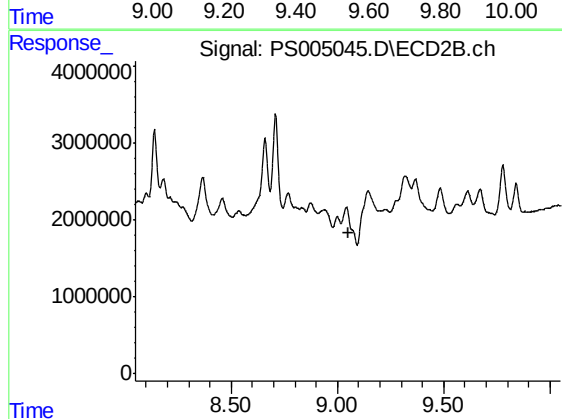

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.050 min
Response: 0
Conc: N.D.