

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
 Data File : PS005047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 13:30
 Operator : SM\AJ
 Sample : K3344-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-0D015-03-007

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 14:31:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.552	5.265	105.8E6	62951790	80.262	63.107
Target Compounds							
2) T	3,5-DICHL...	0.000	4.582	0	140.1E6	N.D.	109.452
6) T	MCP	5.941	0.000	32495987	0	7.285	N.D. #
7) T	MCPA	6.043	5.655	18921377	23251818	3.019	5.516 #
8) T	DICHLORPROP	0.000	5.956	0	16663519	N.D.	17.157
9) T	2,4-D	6.636	0.000	20810304	0	15.423	N.D. #
10) T	Pentachlo...	6.838	6.603	28904226	22424846	1.502	1.741
13) T	2,4-DB	8.210	7.837	85094945	45415431	92.697	71.561
14) T	DINOSEB	0.000	8.156	0	28606698	N.D.	7.364



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
Data File : PS005047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 13:30
Operator : SM\AJ
Sample : K3344-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 14:31:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

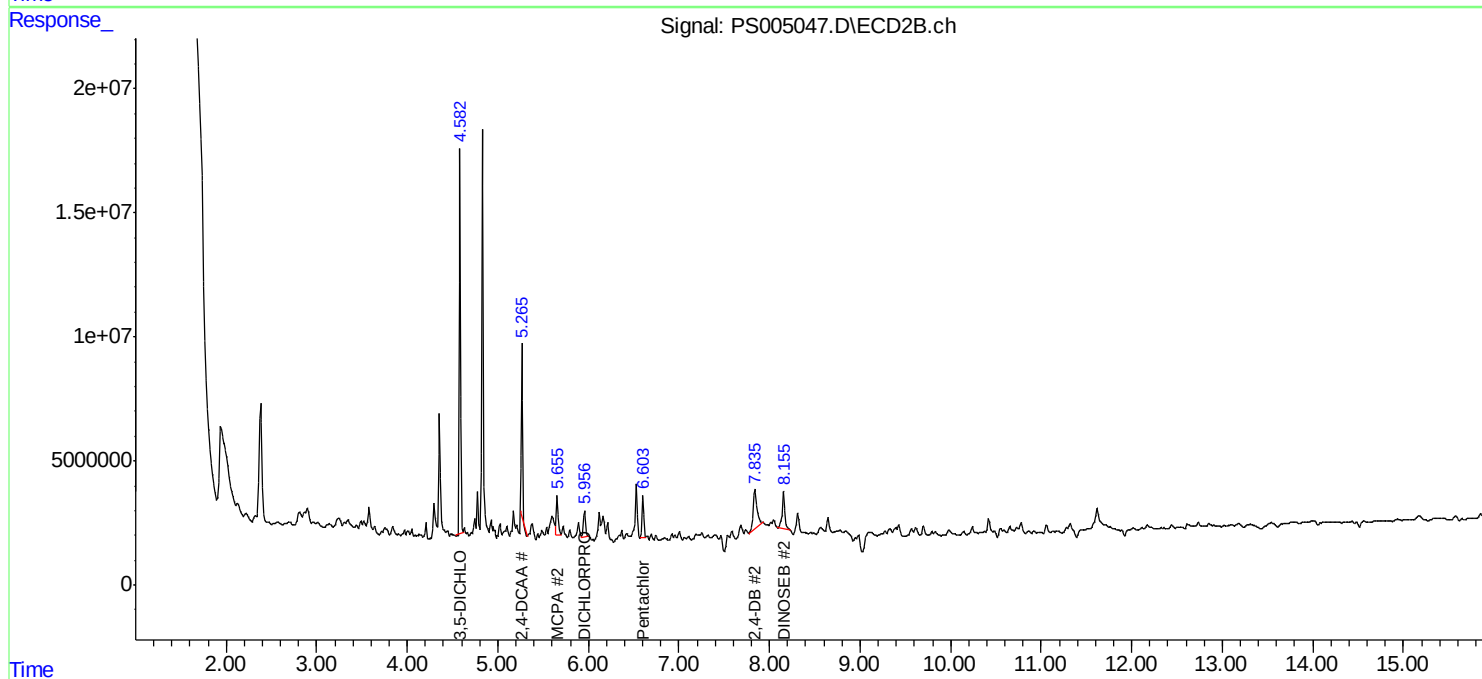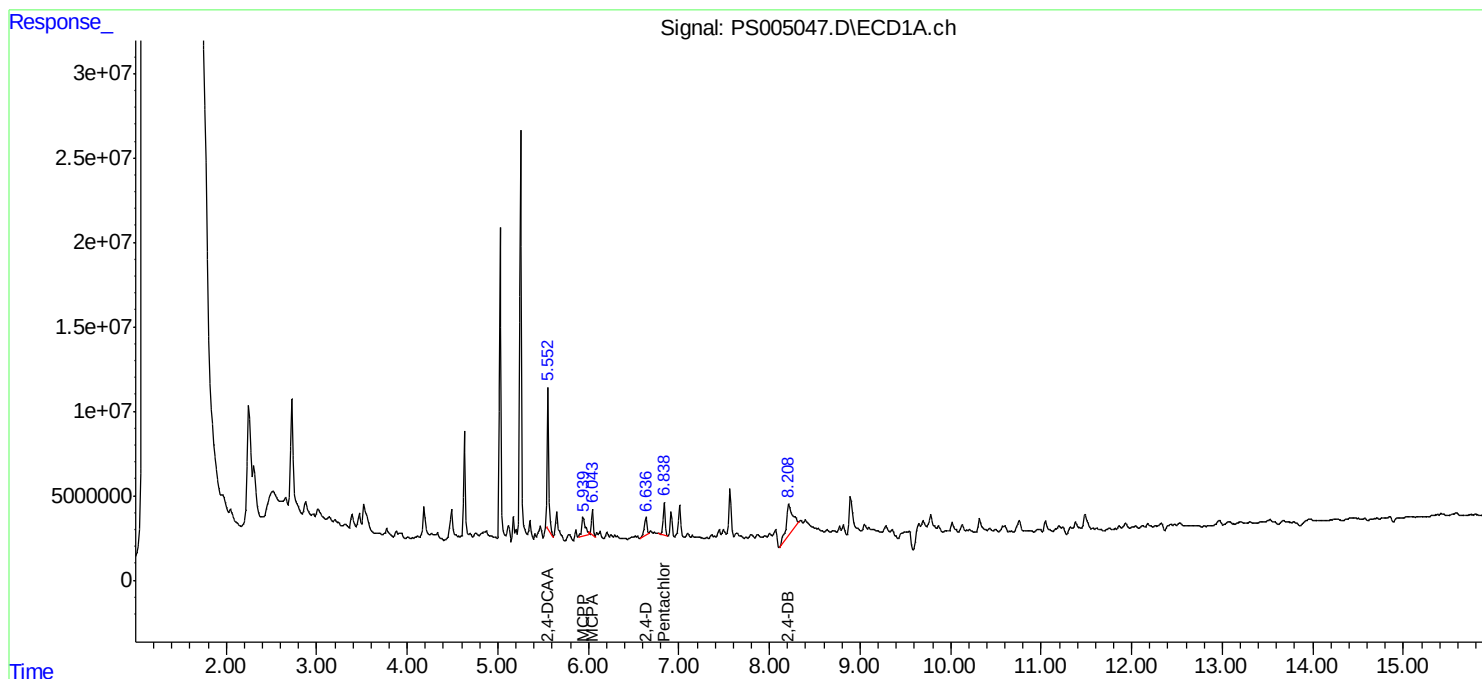


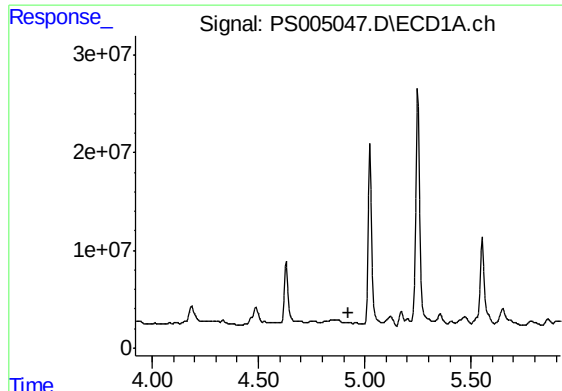

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.922 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-007

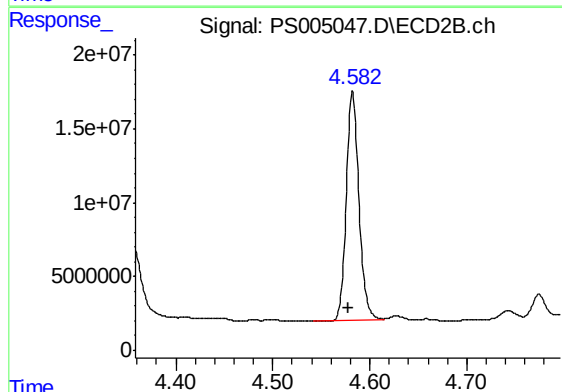


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.582 min
Delta R.T.: 0.005 min
Response: 140076000
Conc: 109.45 ng/ml

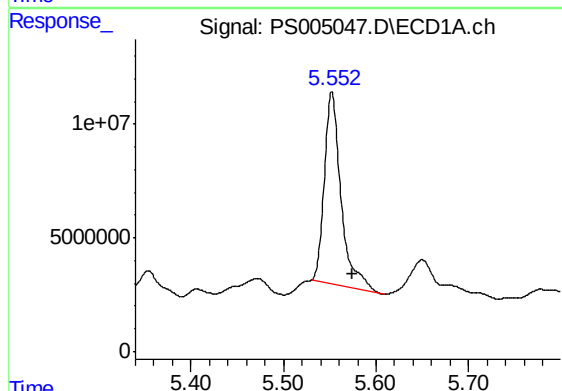


#4 2,4-DCAA

R.T.: 5.552 min
Delta R.T.: -0.021 min
Response: 105769255
Conc: 80.26 ng/ml

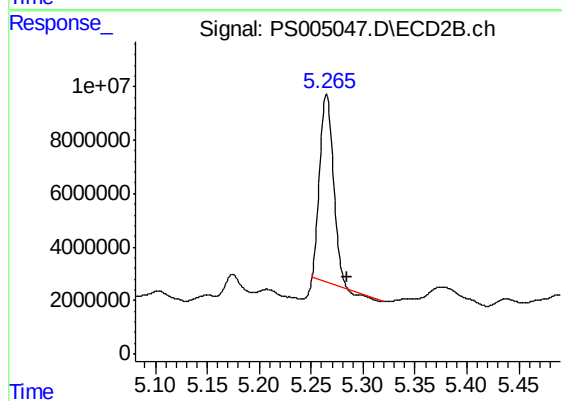

#4 2,4-DCAA


R.T.: 5.265 min
Delta R.T.: -0.020 min
Response: 62951790
Conc: 63.11 ng/ml

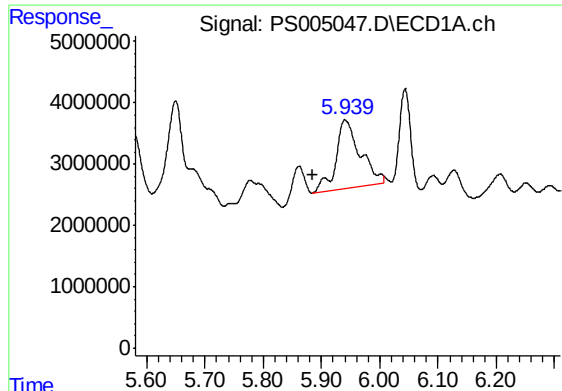

#6 MCPP


R.T.: 5.941 min
Delta R.T.: 0.056 min
Response: 32495987
Conc: 7.29 ug/ml

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-007

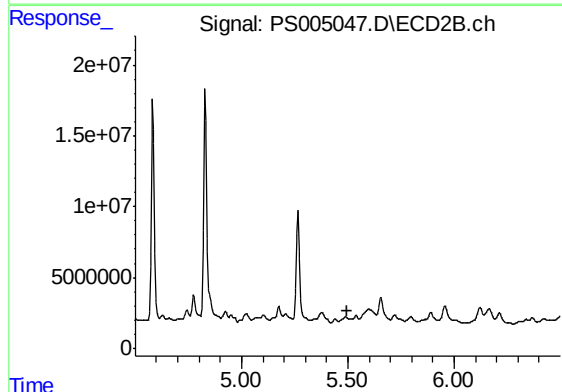


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.500 min
Response: 0
Conc: N.D.

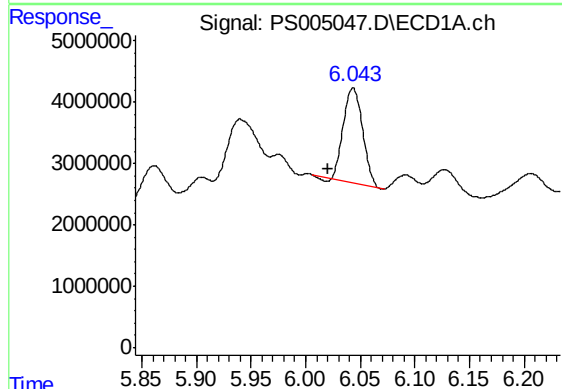


#7 MCPA

R.T.: 6.043 min
Delta R.T.: 0.023 min
Response: 18921377
Conc: 3.02 ug/ml

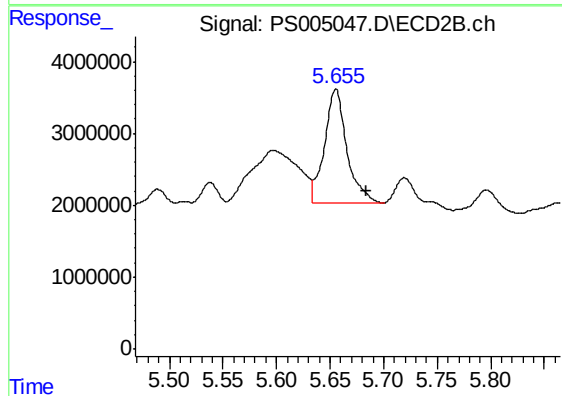

#7 MCPA


R.T.: 5.655 min
Delta R.T.: -0.028 min
Response: 23251818
Conc: 5.52 ug/ml

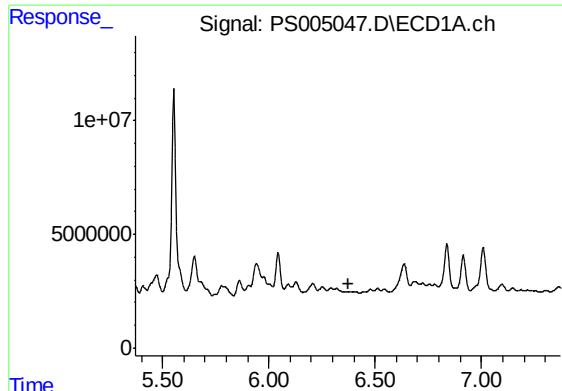

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-007

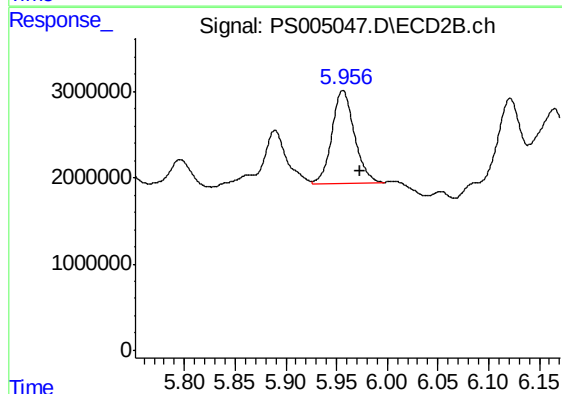


#8 DICHLORPROP

R.T.: 5.956 min
Delta R.T.: -0.017 min
Response: 16663519
Conc: 17.16 ng/ml

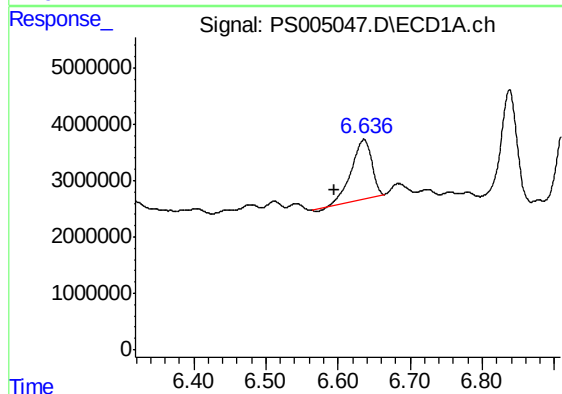


#9 2,4-D

R.T.: 6.636 min
Delta R.T.: 0.040 min
Response: 20810304
Conc: 15.42 ng/ml

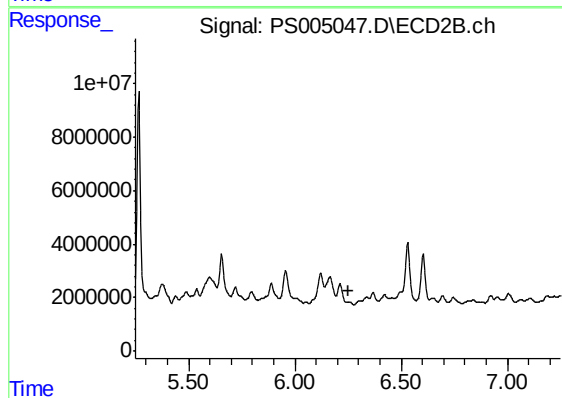

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.250 min
Response: 0
Conc: N.D.

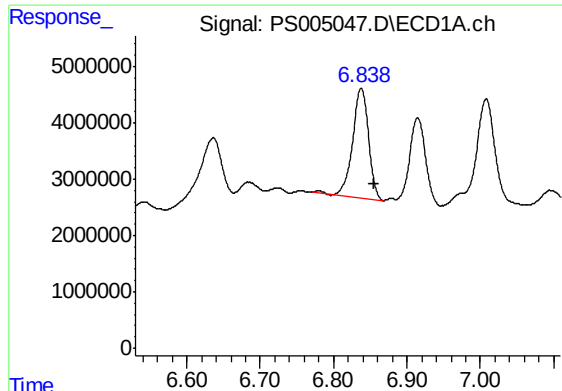

#10 Pentachlorophenol


R.T.: 6.838 min
Delta R.T.: -0.018 min
Response: 28904226
Conc: 1.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-007

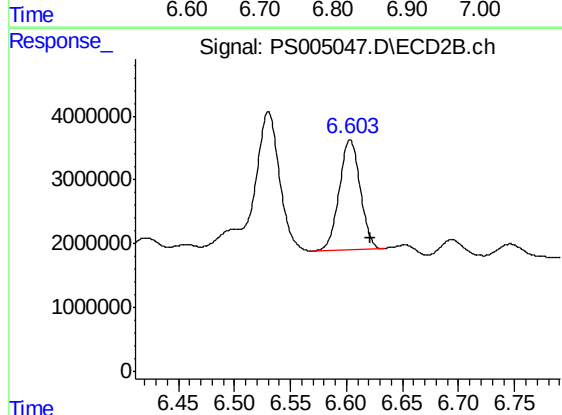


#10 Pentachlorophenol

R.T.: 6.603 min
Delta R.T.: -0.019 min
Response: 22424846
Conc: 1.74 ng/ml

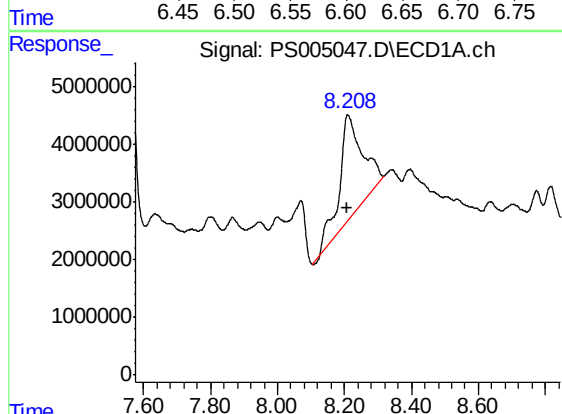


#13 2,4-DB

R.T.: 8.210 min
Delta R.T.: 0.002 min
Response: 85094945
Conc: 92.70 ng/ml

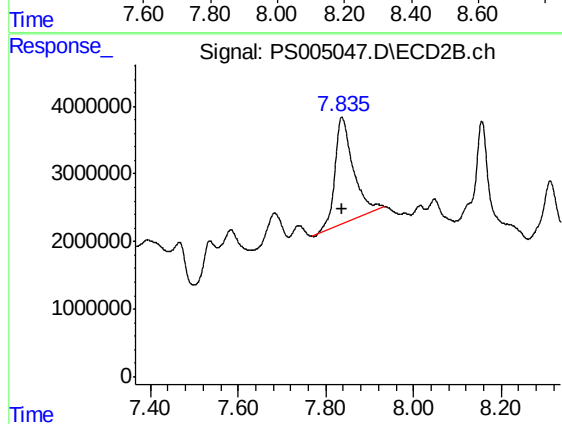

#13 2,4-DB


R.T.: 7.837 min
Delta R.T.: -0.002 min
Response: 45415431
Conc: 71.56 ng/ml

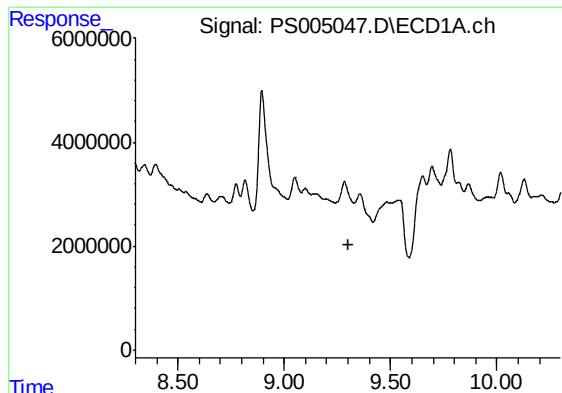

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.300 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-007

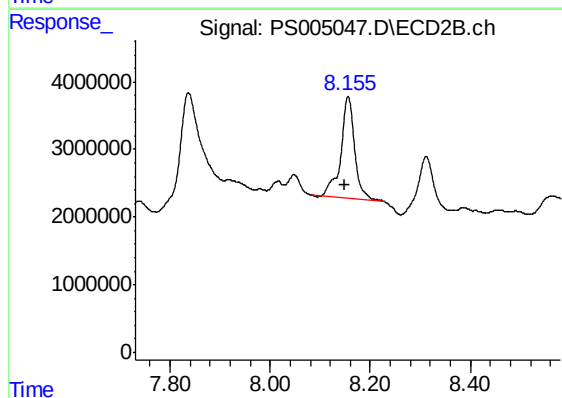

#14 DINOSEB

R.T.: 8.156 min
Delta R.T.: 0.006 min
Response: 28606698
Conc: 7.36 ng/ml