

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
 Data File : PS005050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 14:36
 Operator : SM\AJ
 Sample : K3343-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-0D015-03-008

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 16:08:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.289	181.6E6	118.9E6	137.781	119.243
Target Compounds							
2) T	3,5-DICHL...	0.000	4.607	0	167.7E6	N.D.	131.034
3) T	4-Nitroph...	5.495	0.000	17908114	0	39.317	N.D. #
5) T	DICAMBA	5.673	0.000	4321257	0	<MDL	N.D. #
7) T	MCPA	6.000	5.680	2087517	22361757	<MDL	5.305 #
8) T	DICHLORPROP	0.000	5.981	0	14389307	N.D.	14.816
9) T	2,4-D	6.659	0.000	21124987	0	15.656	N.D. #
10) T	Pentachlo...	6.861	6.628	25049837	19668123	1.302	1.527
13) T	2,4-DB	8.230	7.858	169.8E6	62261232	184.984	98.105 #
14) T	DINOSEB	0.000	8.180	0	41743597	N.D.	10.746



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
Data File : PS005050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 14:36
Operator : SM\AJ
Sample : K3343-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-008

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 16:08:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

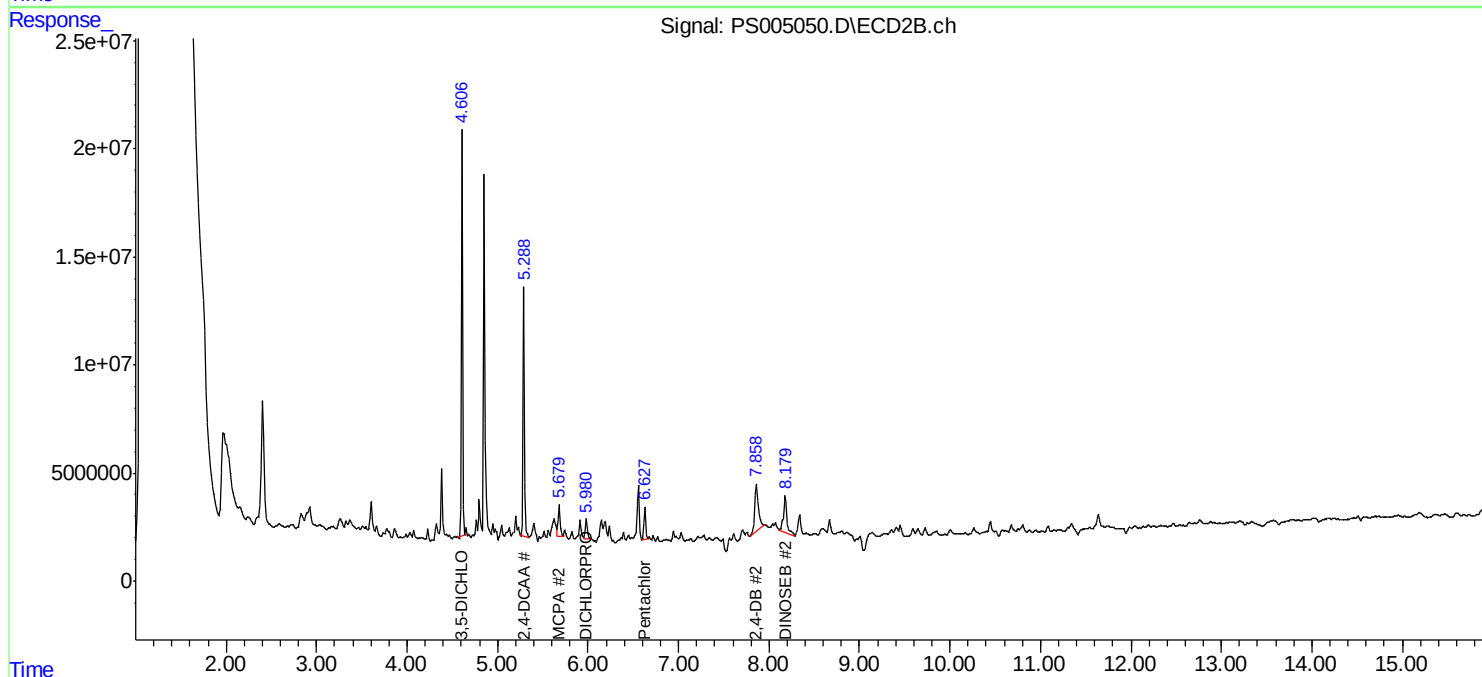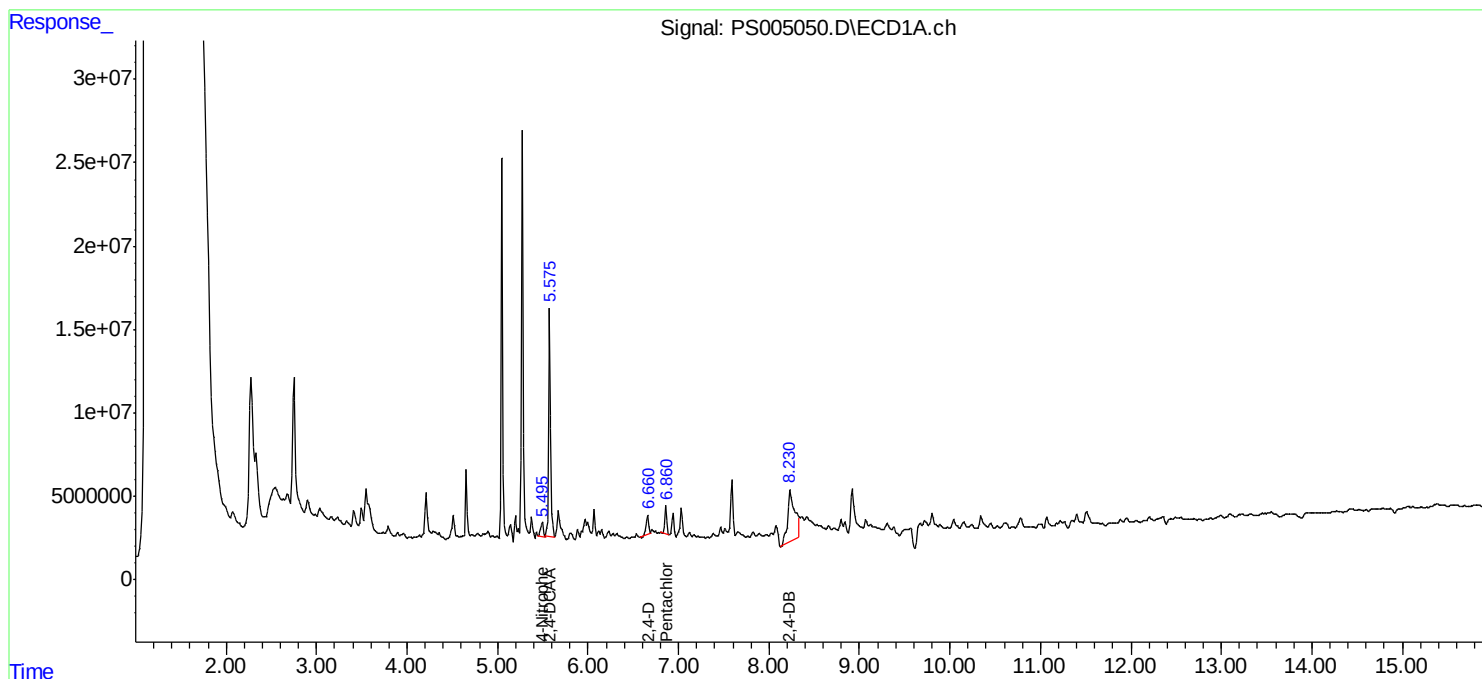


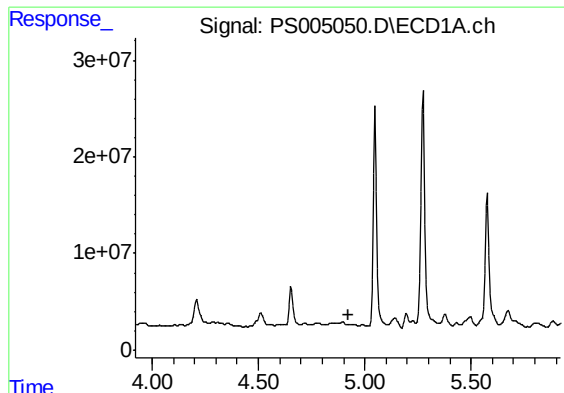

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.922 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-008

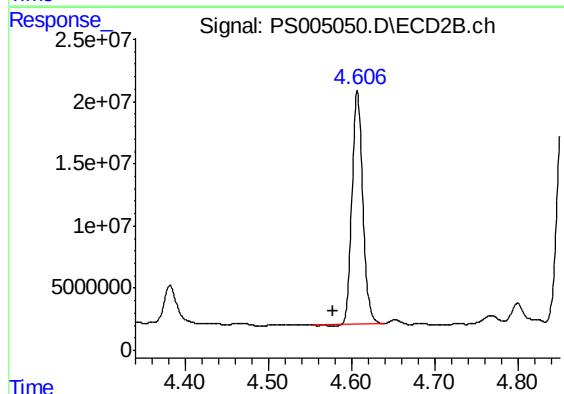


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.607 min
Delta R.T.: 0.029 min
Response: 167695651
Conc: 131.03 ng/ml

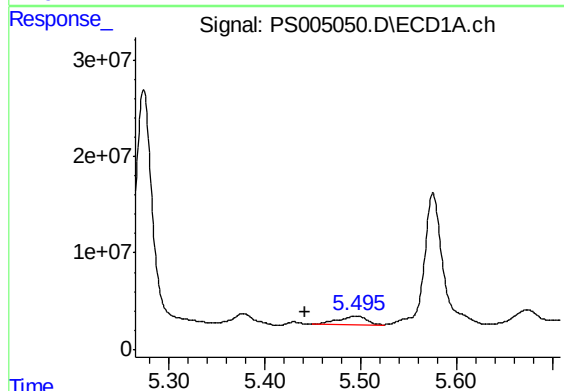


#3 4-Nitrophenol

R.T.: 5.495 min
Delta R.T.: 0.053 min
Response: 17908114
Conc: 39.32 ng/ml

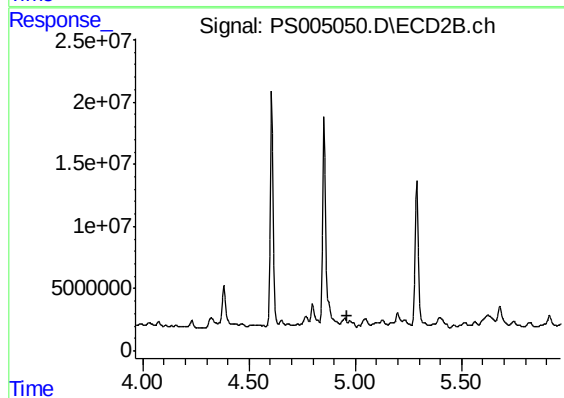

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.965 min
Response: 0
Conc: N.D.

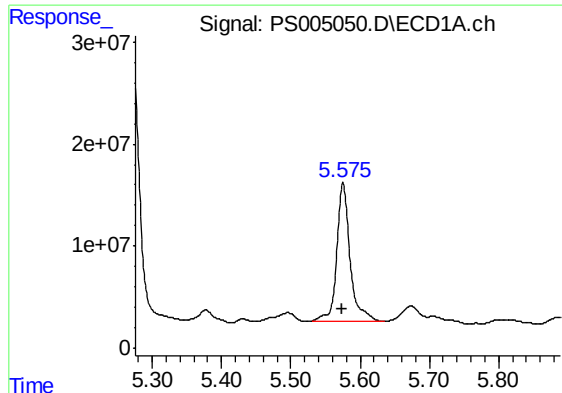

#4 2,4-DCAA


R.T.: 5.576 min
Delta R.T.: 0.002 min
Response: 181566854
Conc: 137.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-008

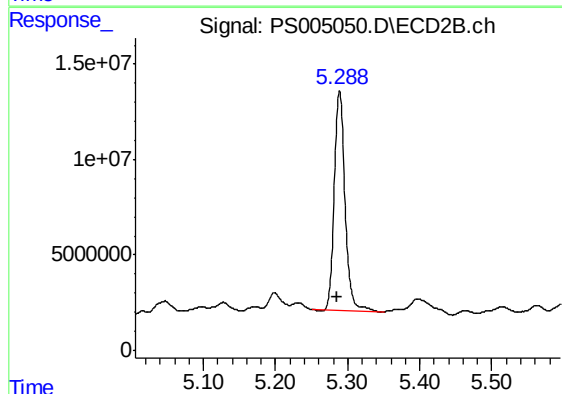


#4 2,4-DCAA

R.T.: 5.289 min
Delta R.T.: 0.004 min
Response: 118949126
Conc: 119.24 ng/ml

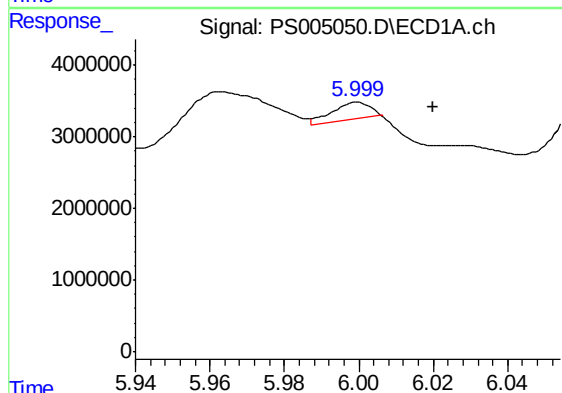


#7 MCPA

R.T.: 6.000 min
Delta R.T.: -0.020 min
Response: 2087517
Conc: N.D.

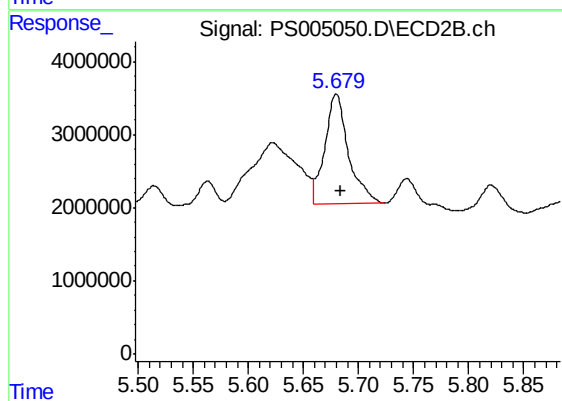

#7 MCPA


R.T.: 5.680 min
Delta R.T.: -0.004 min
Response: 22361757
Conc: 5.30 ug/ml

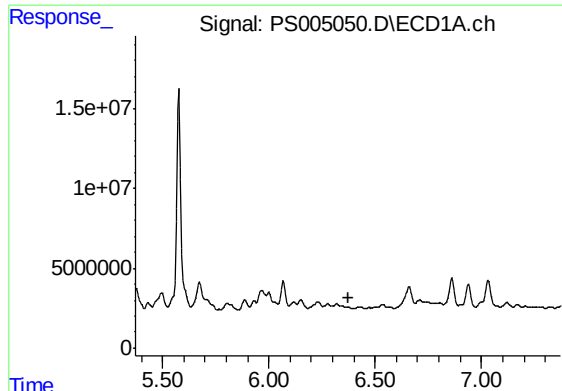

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-008

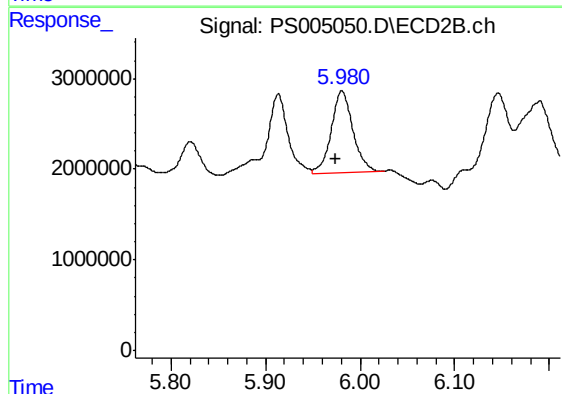


#8 DICHLORPROP

R.T.: 5.981 min
Delta R.T.: 0.007 min
Response: 14389307
Conc: 14.82 ng/ml

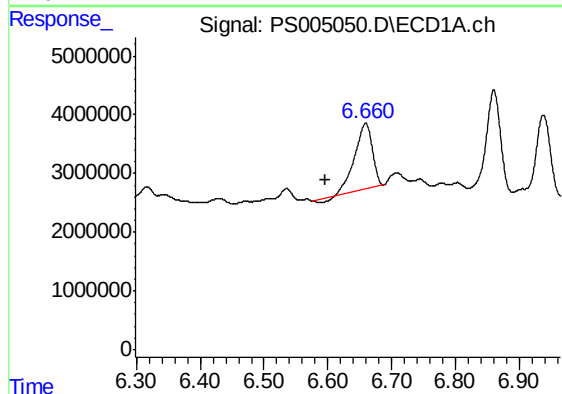


#9 2,4-D

R.T.: 6.659 min
Delta R.T.: 0.064 min
Response: 21124987
Conc: 15.66 ng/ml

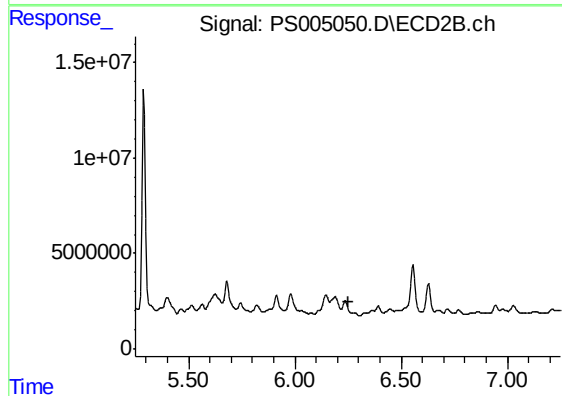

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.250 min
Response: 0
Conc: N.D.

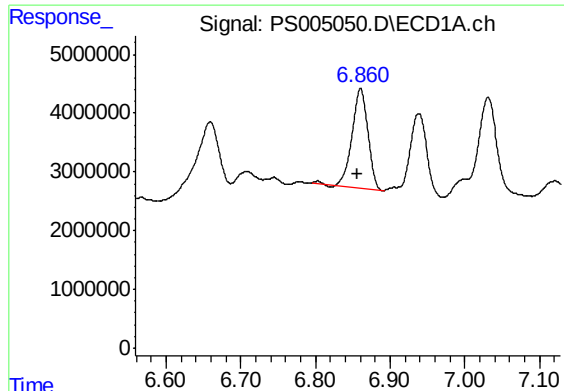

#10 Pentachlorophenol


R.T.: 6.861 min
Delta R.T.: 0.005 min
Response: 25049837
Conc: 1.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-008

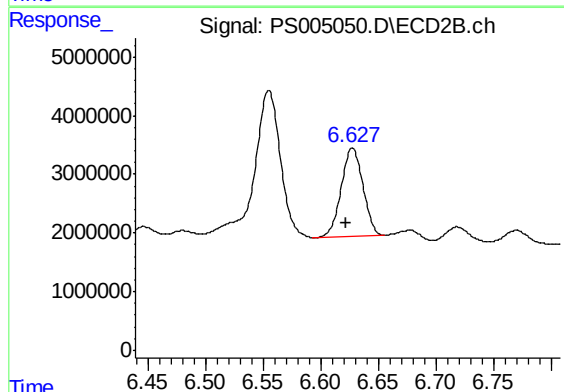


#10 Pentachlorophenol

R.T.: 6.628 min
Delta R.T.: 0.006 min
Response: 19668123
Conc: 1.53 ng/ml

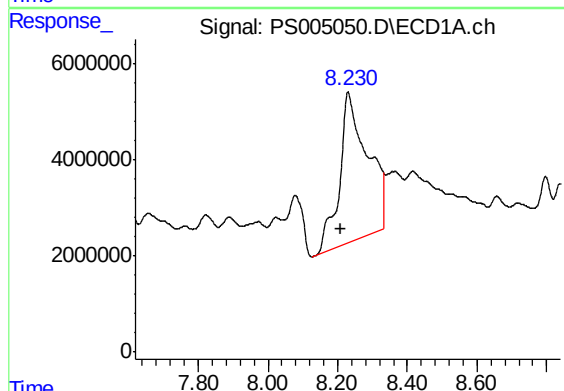


#13 2,4-DB

R.T.: 8.230 min
Delta R.T.: 0.022 min
Response: 169812458
Conc: 184.98 ng/ml

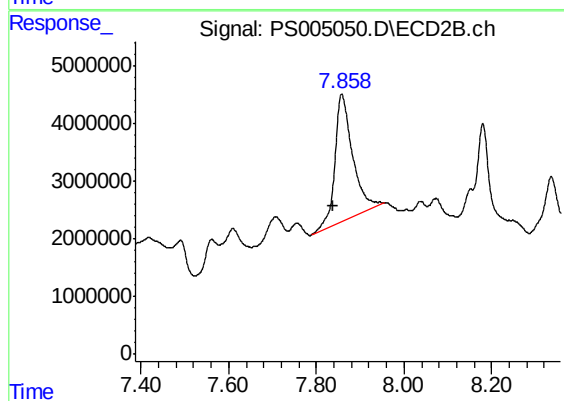

#13 2,4-DB


R.T.: 7.858 min
Delta R.T.: 0.020 min
Response: 62261232
Conc: 98.10 ng/ml

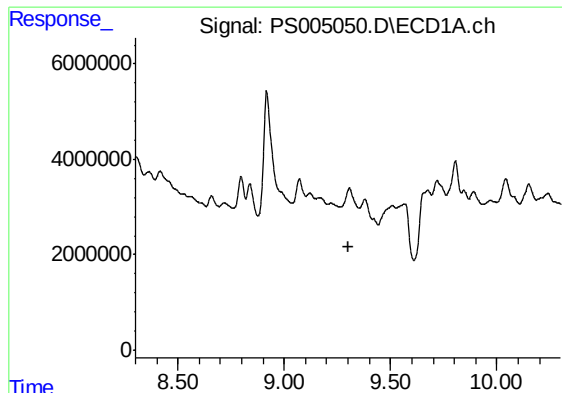

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.300 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-0D015-03-008

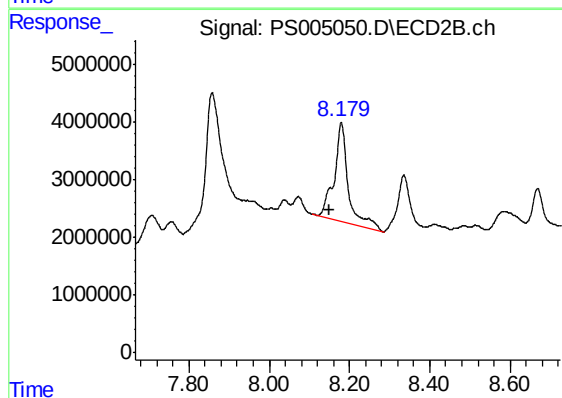

#14 DINOSEB

R.T.: 8.180 min
Delta R.T.: 0.030 min
Response: 41743597
Conc: 10.75 ng/ml