

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
 Data File : PS005052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 15:20
 Operator : SM\AJ
 Sample : K3361-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BAT-B10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 16:08:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.567	5.318	31664692	173.4E6	24.029	173.791 #
Target Compounds							
2) T	3,5-DICHL...	0.000	4.637	0	103.7E6	N.D.	81.007
3) T	4-Nitroph...	5.449	4.973	21972453	57792970	48.240	127.448 #
5) T	DICAMBA	5.704	0.000	15575268	0	2.752	N.D. #
6) T	MCPD	5.941	0.000	27297980	0	6.120	N.D. #
7) T	MCPA	0.000	5.709	0	19471026	N.D.	4.619
8) T	DICHLORPROP	0.000	6.010	0	13458780	N.D.	13.858
9) T	2,4-D	6.603	6.237	35155955	79889313	26.054	74.651 #
10) T	Pentachlo...	6.878	6.626	136.5E6	89324334	7.093	6.933
11) T	2,4,5-TP ...	0.000	7.030	0	22385829	N.D.	4.182
12) T	2,4,5-T	7.619	0.000	72290667	0	9.047	N.D. #
13) T	2,4-DB	8.199	0.000	26170099	0	28.508	N.D. #
15) T	Picloram	9.185	0.000	25950150	0	2.614	N.D. #
16) T	DCPA	9.555	0.000	103.0E6	0	10.604	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
Data File : PS005052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 15:20
Operator : SM\AJ
Sample : K3361-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
BAT-B10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 16:08:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

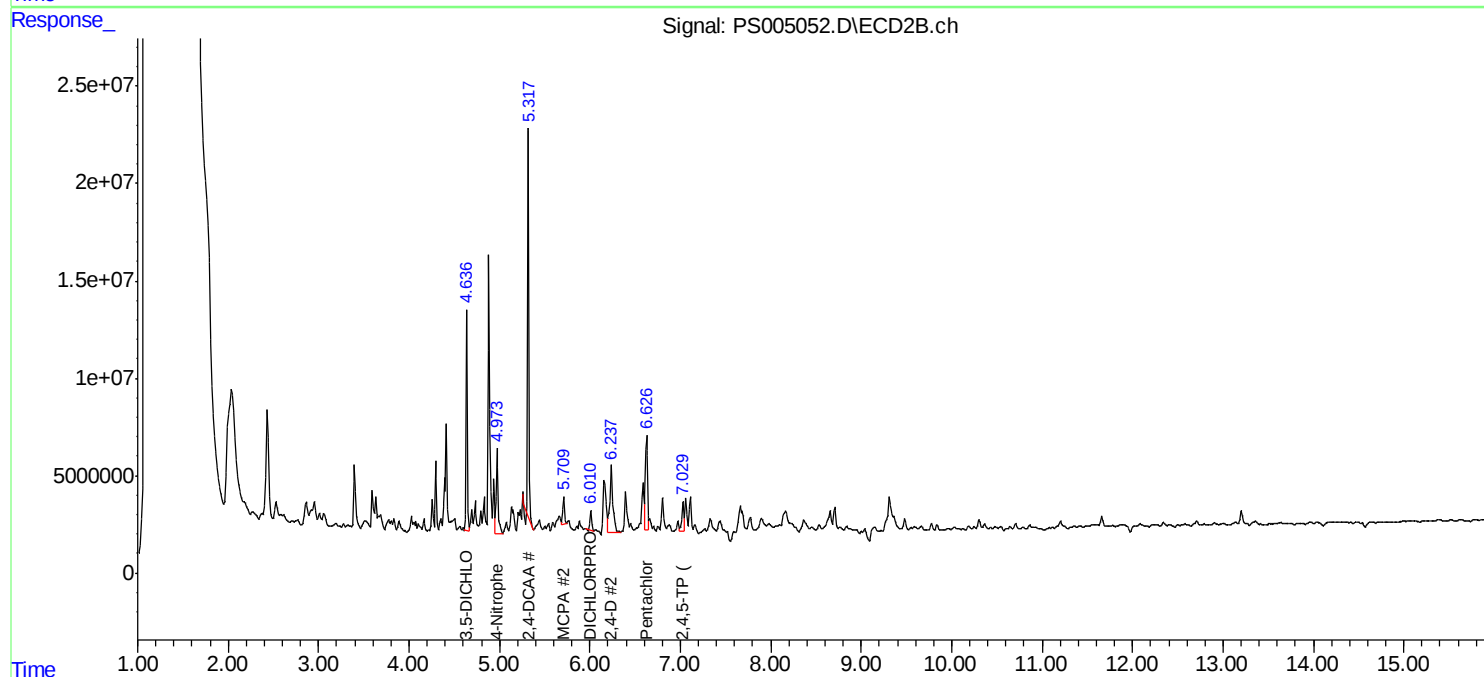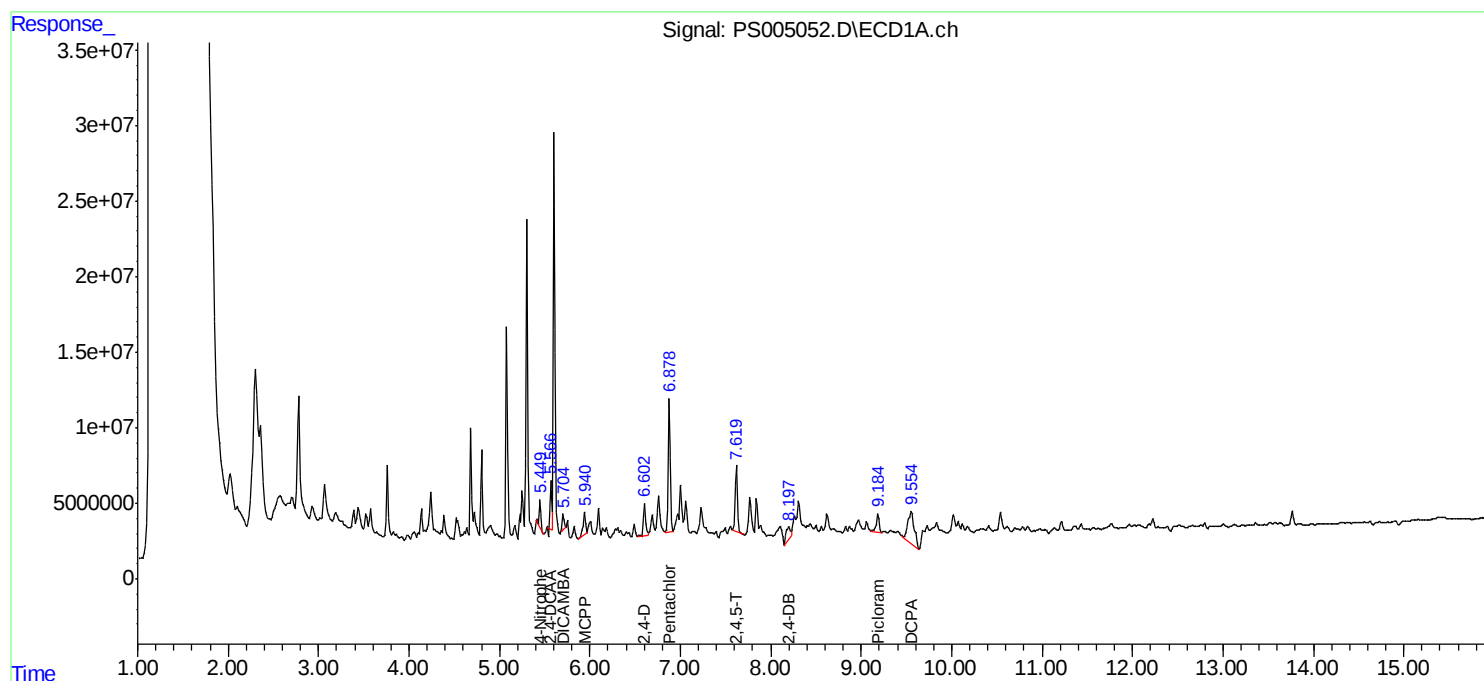


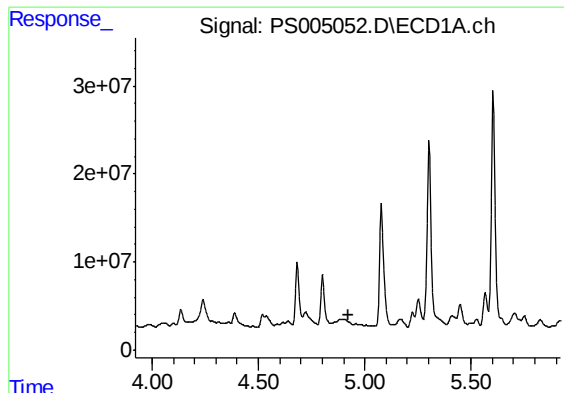

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.922 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B10

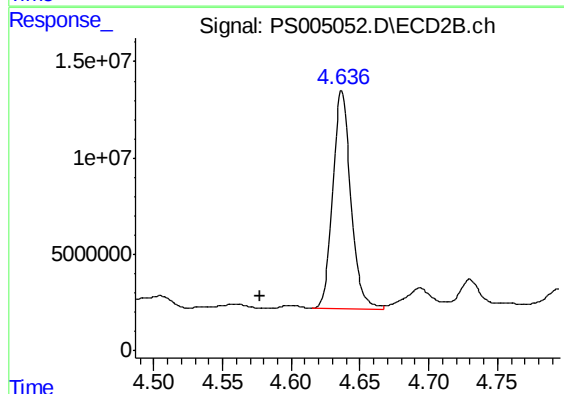


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.637 min
Delta R.T.: 0.059 min
Response: 103672522
Conc: 81.01 ng/ml

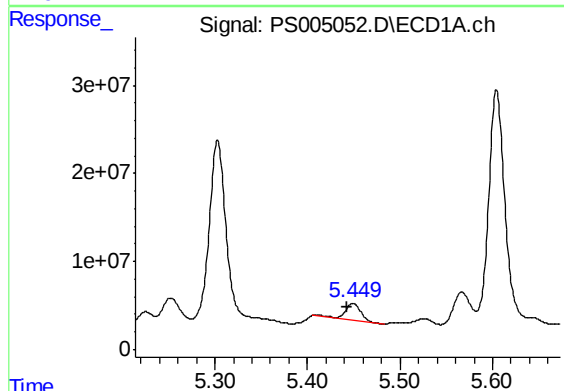


#3 4-Nitrophenol

R.T.: 5.449 min
Delta R.T.: 0.007 min
Response: 21972453
Conc: 48.24 ng/ml

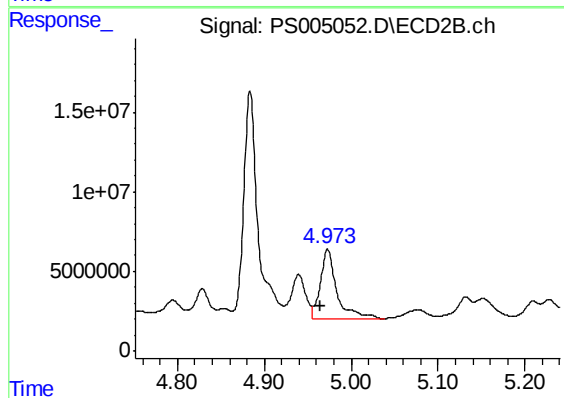

#3 4-Nitrophenol


R.T.: 4.973 min
Delta R.T.: 0.008 min
Response: 57792970
Conc: 127.45 ng/ml

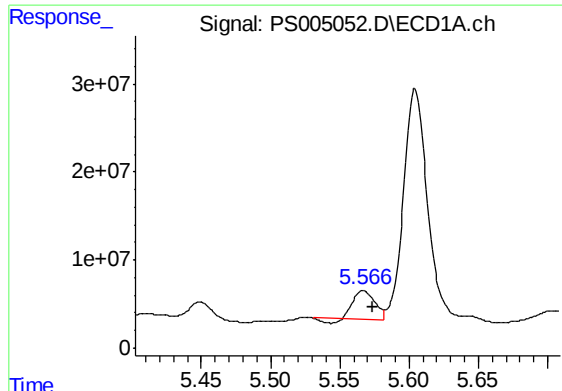

#4 2,4-DCAA


R.T.: 5.567 min
Delta R.T.: -0.007 min
Response: 31664692
Conc: 24.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B10

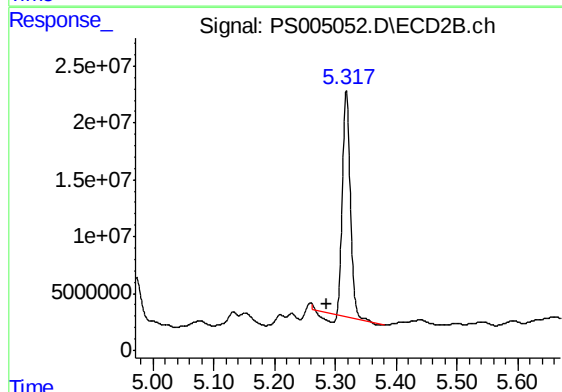


#4 2,4-DCAA

R.T.: 5.318 min
Delta R.T.: 0.033 min
Response: 173362474
Conc: 173.79 ng/ml

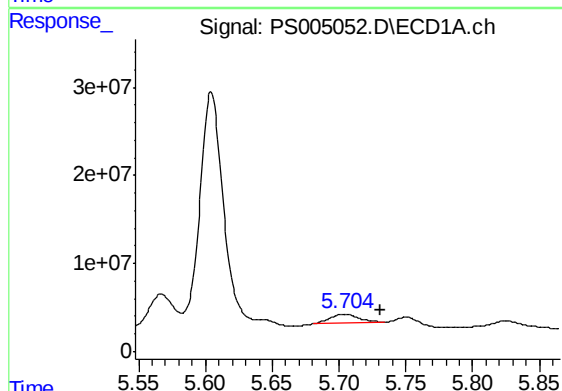


#5 DICAMBA

R.T.: 5.704 min
Delta R.T.: -0.027 min
Response: 15575268
Conc: 2.75 ng/ml

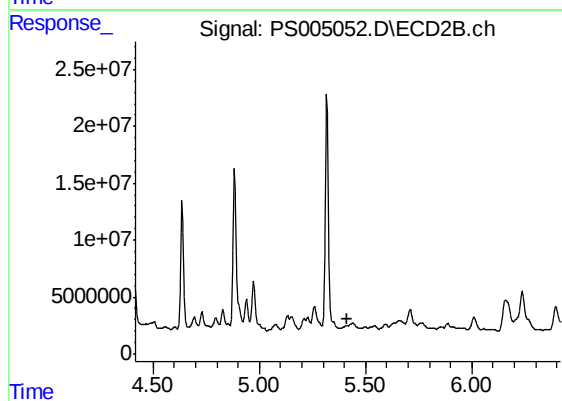

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.417 min
Response: 0
Conc: N.D.

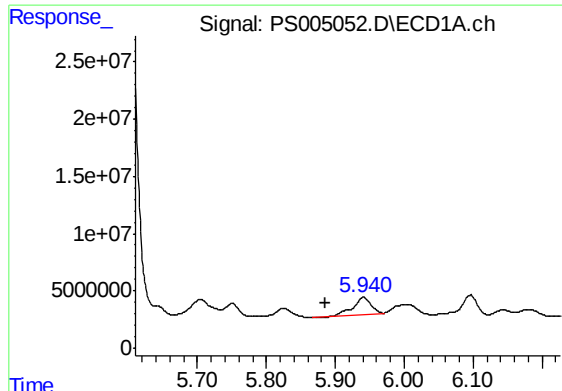

#6 MCPP


R.T.: 5.941 min
Delta R.T.: 0.056 min
Response: 27297980
Conc: 6.12 ug/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B10

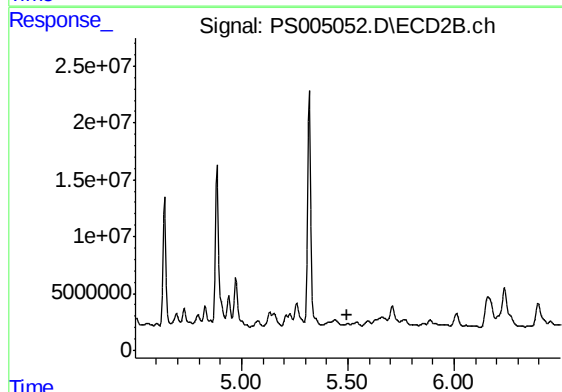


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.500 min
Response: 0
Conc: N.D.

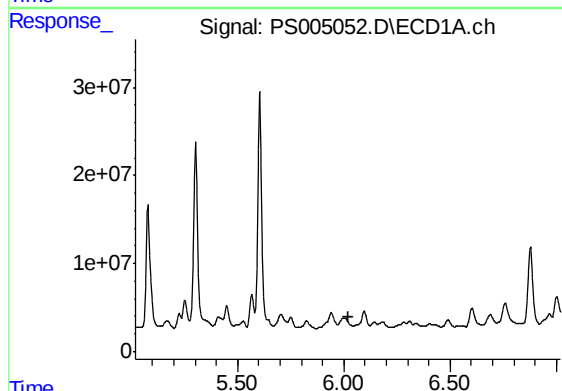


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.020 min
Response: 0
Conc: N.D.

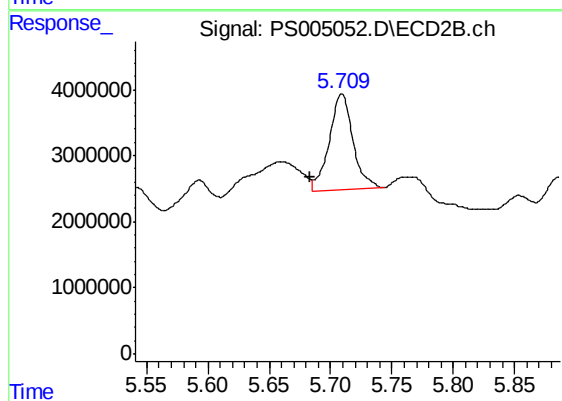

#7 MCPA


R.T.: 5.709 min
Delta R.T.: 0.026 min
Response: 19471026
Conc: 4.62 ug/ml

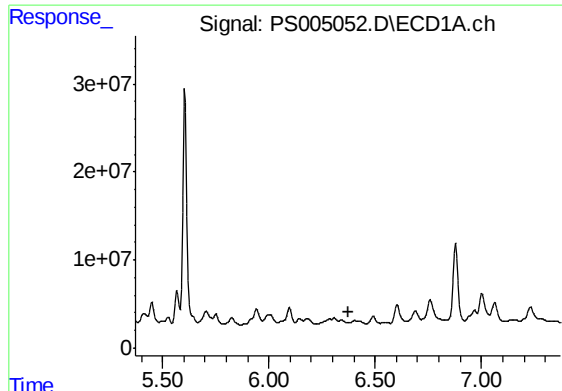

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BAT-B10

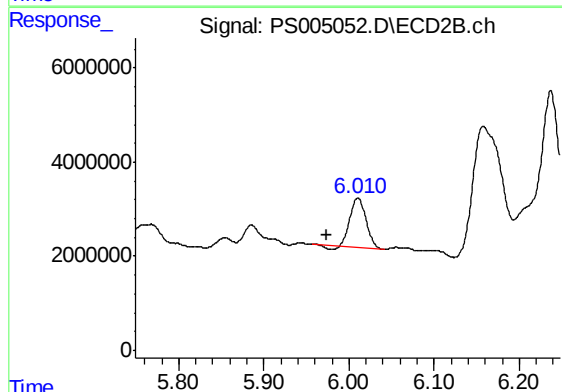


#8 DICHLORPROP

R.T.: 6.010 min
Delta R.T.: 0.037 min
Response: 13458780
Conc: 13.86 ng/ml

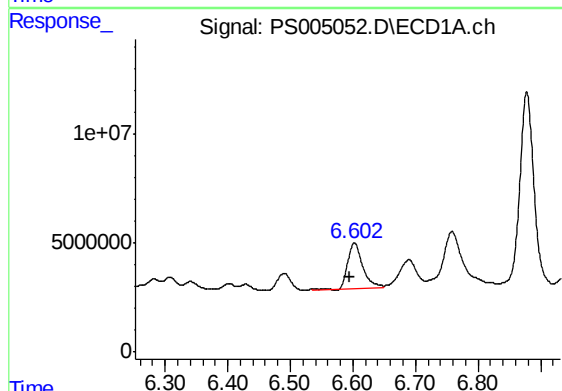


#9 2,4-D

R.T.: 6.603 min
Delta R.T.: 0.007 min
Response: 35155955
Conc: 26.05 ng/ml

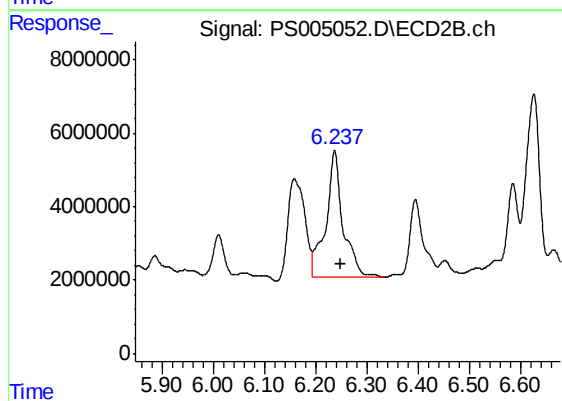

#9 2,4-D


R.T.: 6.237 min
Delta R.T.: -0.013 min
Response: 79889313
Conc: 74.65 ng/ml

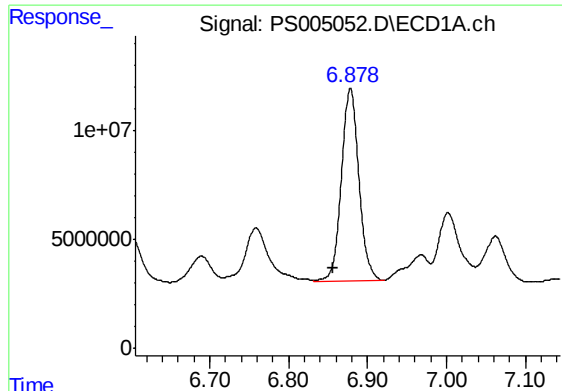

#10 Pentachlorophenol


R.T.: 6.878 min
Delta R.T.: 0.022 min
Response: 136454415
Conc: 7.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B10

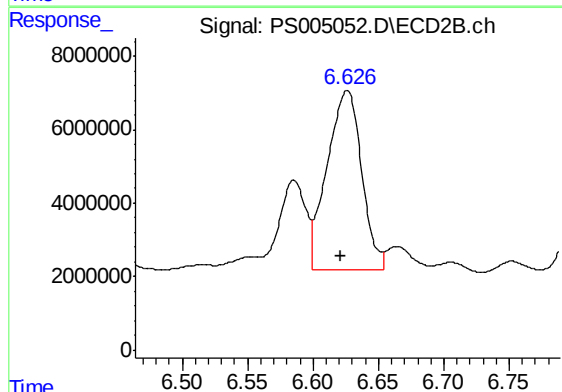


#10 Pentachlorophenol

R.T.: 6.626 min
Delta R.T.: 0.004 min
Response: 89324334
Conc: 6.93 ng/ml

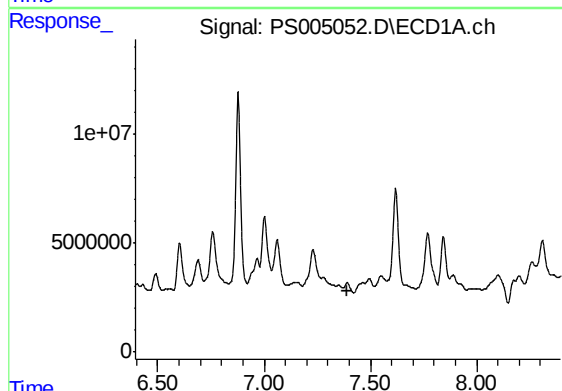


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.395 min
Response: 0
Conc: N.D.

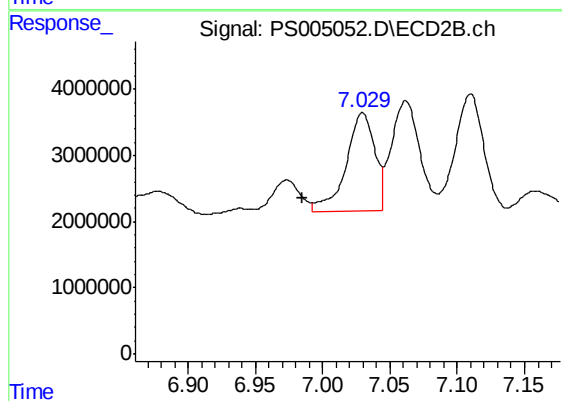

#11 2,4,5-TP (SILVEX)


R.T.: 7.030 min
Delta R.T.: 0.044 min
Response: 22385829
Conc: 4.18 ng/ml

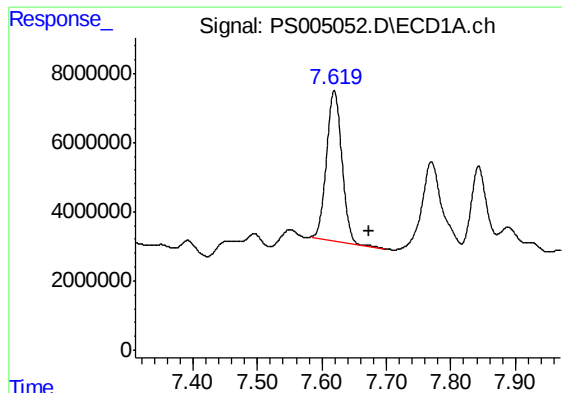

#12 2,4,5-T


R.T.: 7.619 min
Delta R.T.: -0.054 min
Response: 72290667
Conc: 9.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B10

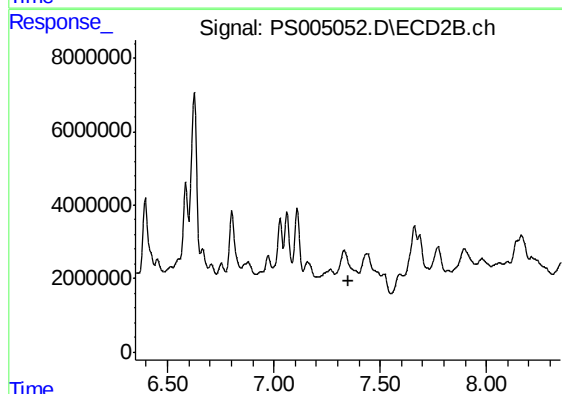


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.349 min
Response: 0
Conc: N.D.

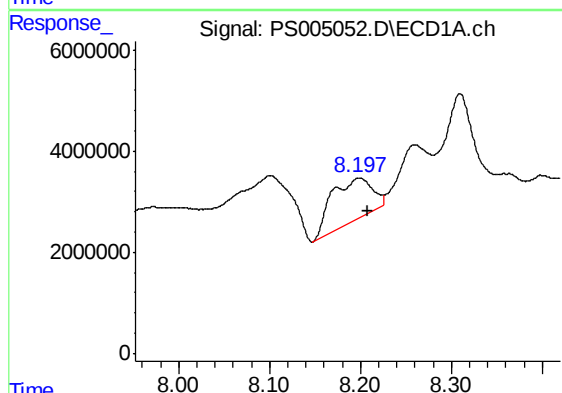


#13 2,4-DB

R.T.: 8.199 min
Delta R.T.: -0.010 min
Response: 26170099
Conc: 28.51 ng/ml

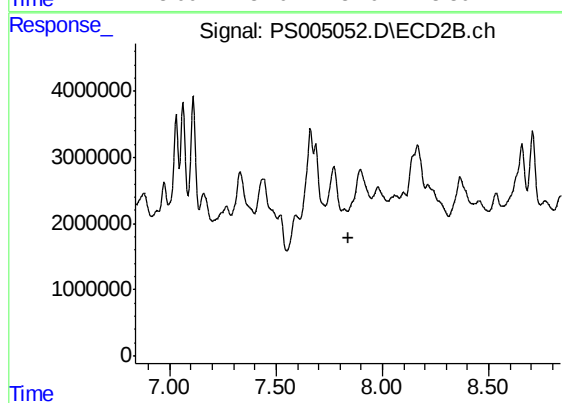

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

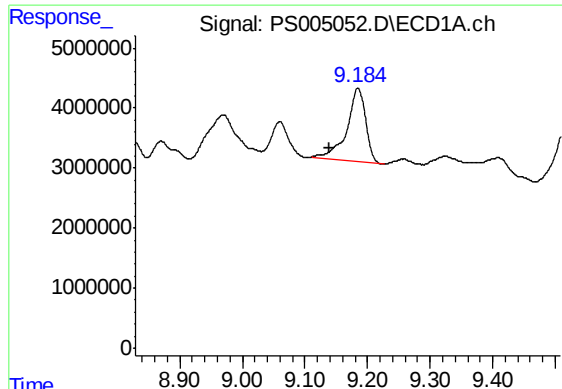

#15 Picloram


R.T.: 9.185 min
Delta R.T.: 0.046 min
Response: 25950150
Conc: 2.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
BAT-B10

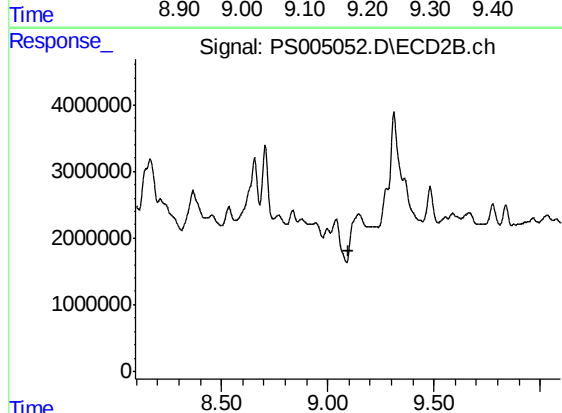


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

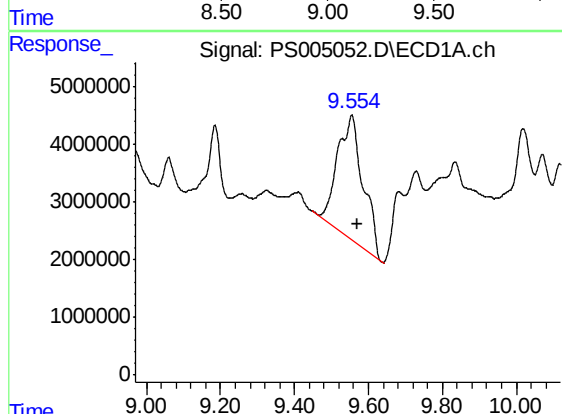

#16 DCPA

R.T.: 9.555 min
Delta R.T.: -0.015 min
Response: 102963275
Conc: 10.60 ng/ml

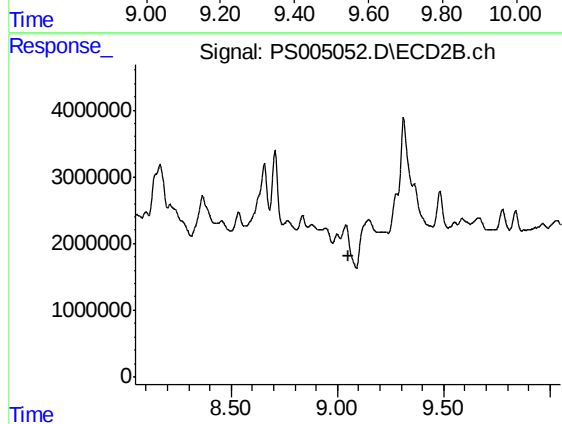

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.050 min
Response: 0
Conc: N.D.