

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
 Data File : PS005061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 18:38
 Operator : SM\AJ
 Sample : PB120672BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:04:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.609	5.322	678.7E6	502.5E6	515.021	503.704
Target Compounds							
1) T	Dalapon	2.107	0.000	27108586	0	15.563	N.D. #
2) T	3,5-DICHL...	0.000	4.641	0	203.7E6	N.D.	159.204
5) T	DICAMBA	5.707	0.000	20858581	0	3.685	N.D. #
7) T	MCPA	0.000	5.660	0	30141087	N.D.	7.150
8) T	DICHLORPROP	0.000	6.017	0	21611282	N.D.	22.252
9) T	2,4-D	6.570	6.181	12572212	-2285238	9.317	N.D. #
10) T	Pentachlo...	0.000	6.589	0	41207631	N.D.	3.198
12) T	2,4,5-T	7.624	0.000	76543686	0	9.579	N.D. #
15) T	Picloram	9.203	9.147	42865939	44527815	4.318	6.528 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
Data File : PS005061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 18:38
Operator : SM\AJ
Sample : PB120672BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:04:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

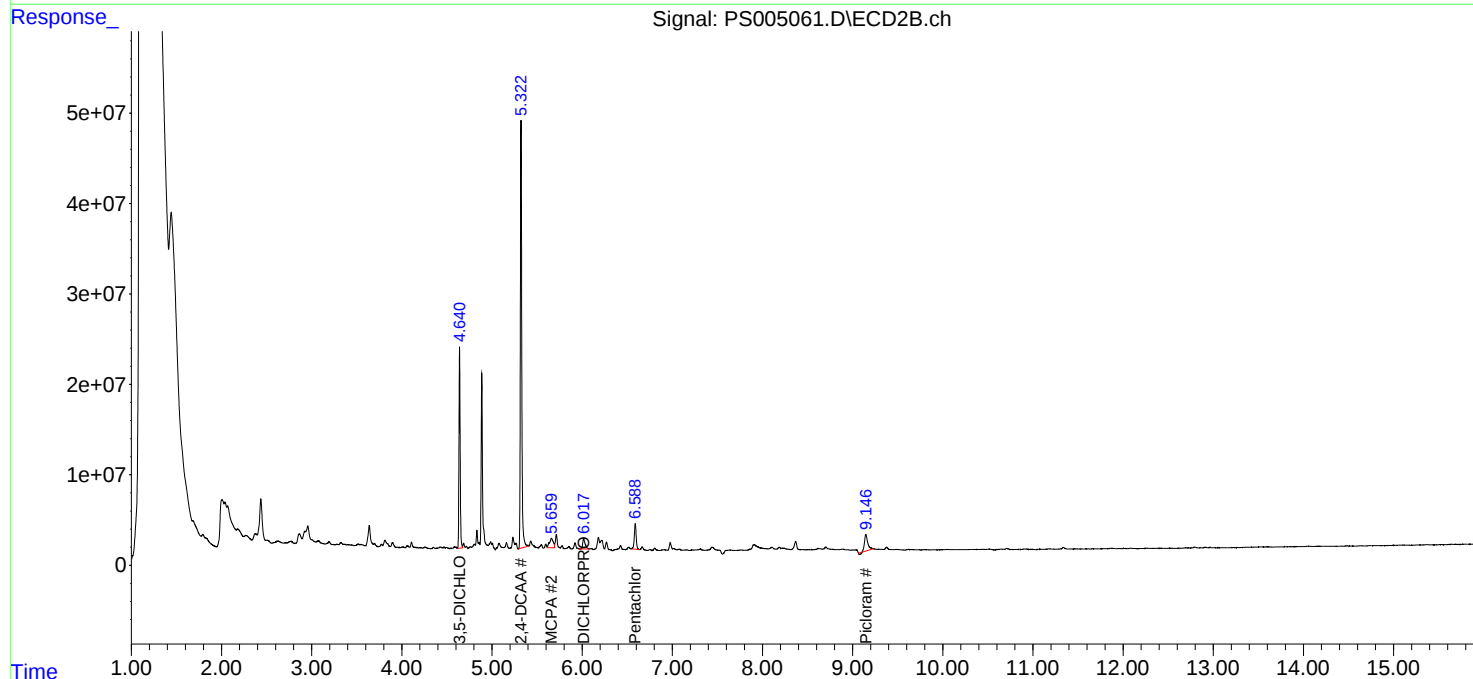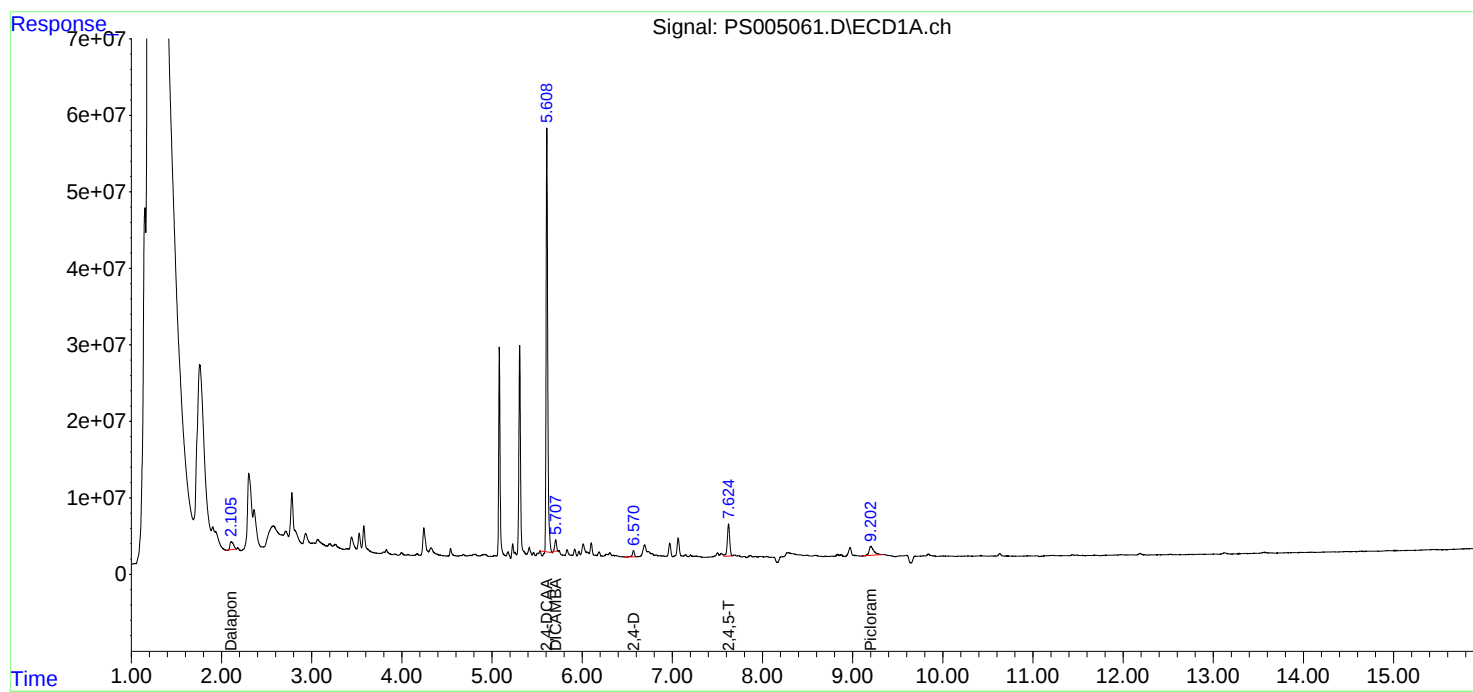


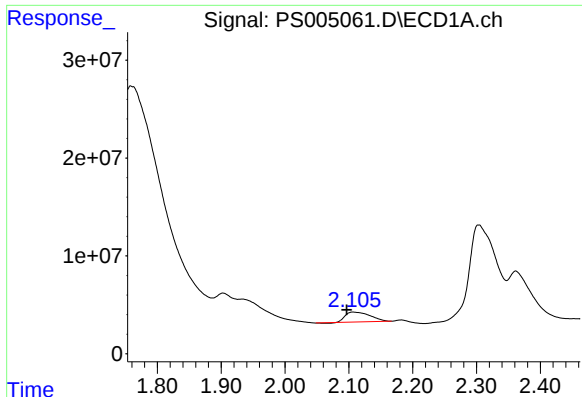

#1 Dalapon


R.T.: 2.107 min
Delta R.T.: 0.010 min
Response: 27108586
Conc: 15.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

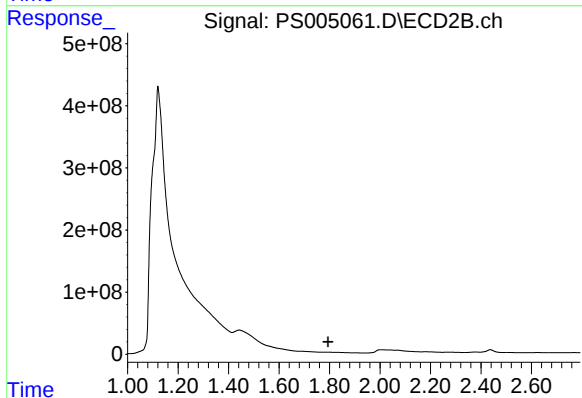


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.794 min
Response: 0
Conc: N.D.

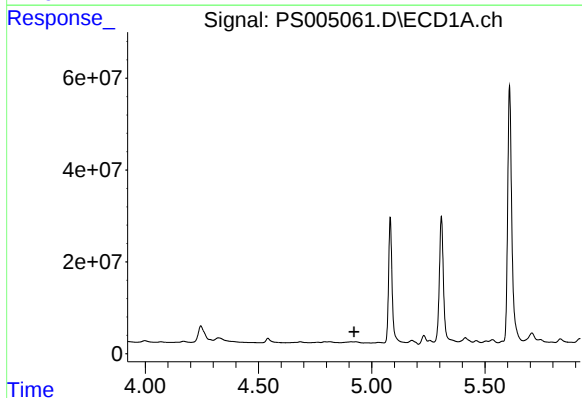


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

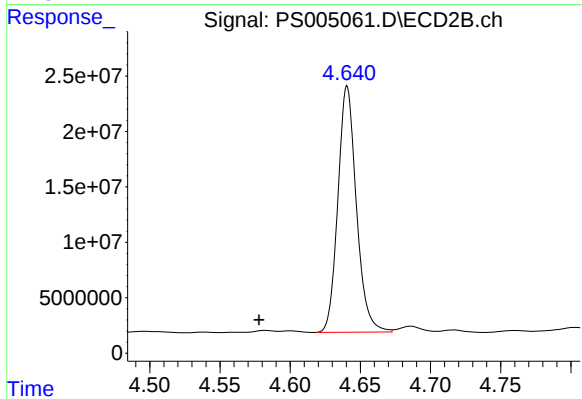

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.641 min
Delta R.T.: 0.063 min
Response: 203747415
Conc: 159.20 ng/ml

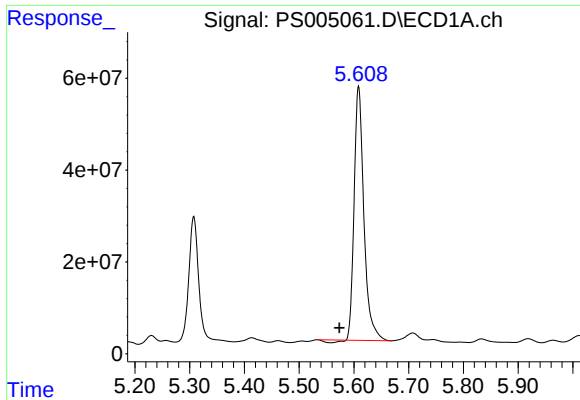

#4 2,4-DCAA


R.T.: 5.609 min
Delta R.T.: 0.035 min
Response: 678692209
Conc: 515.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

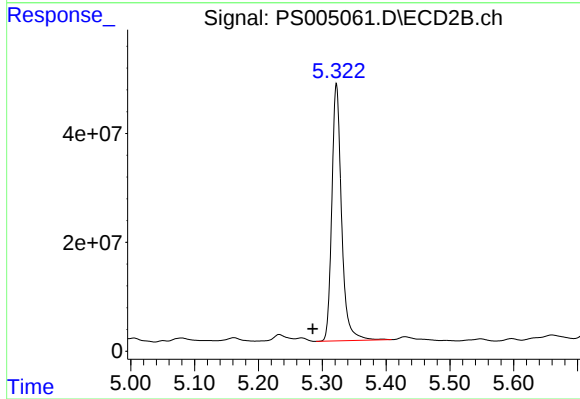


#4 2,4-DCAA

R.T.: 5.322 min
Delta R.T.: 0.037 min
Response: 502462715
Conc: 503.70 ng/ml

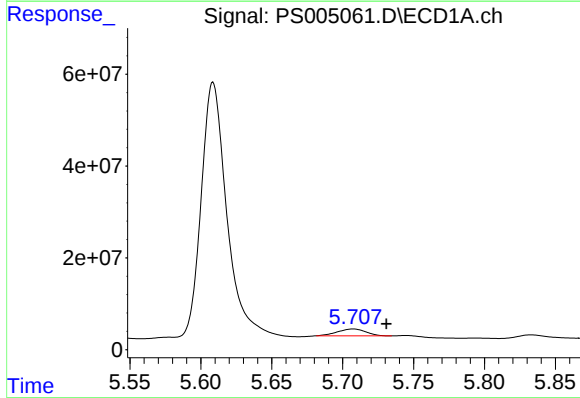


#5 DICAMBA

R.T.: 5.707 min
Delta R.T.: -0.024 min
Response: 20858581
Conc: 3.69 ng/ml

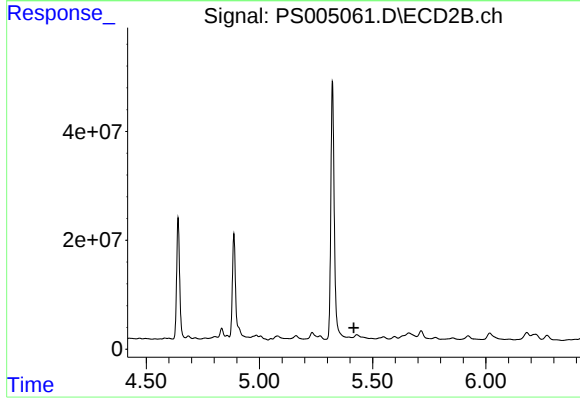

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.417 min
Response: 0
Conc: N.D.

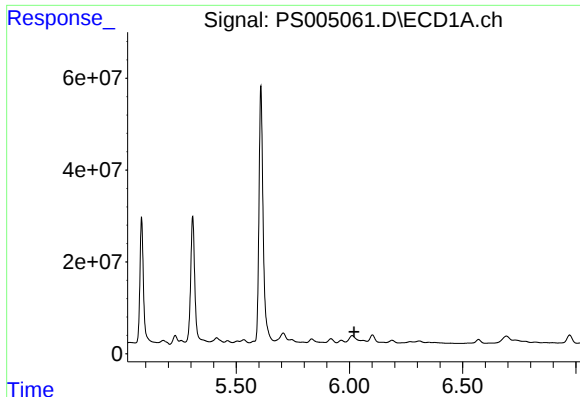

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

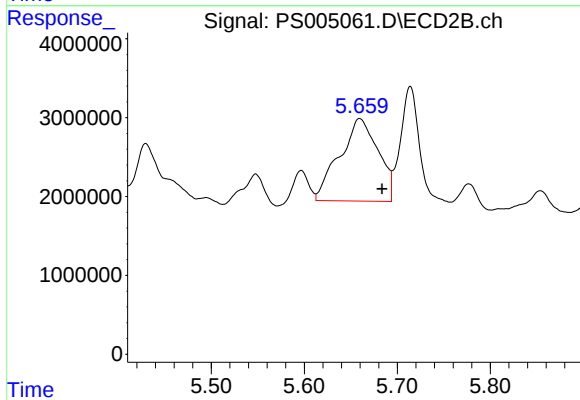


#7 MCPA

R.T.: 5.660 min
Delta R.T.: -0.024 min
Response: 30141087
Conc: 7.15 ug/ml

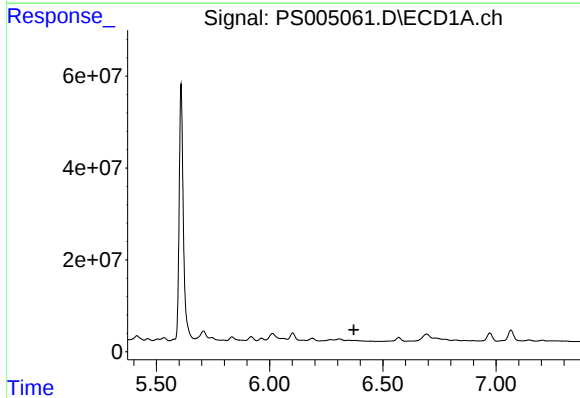


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

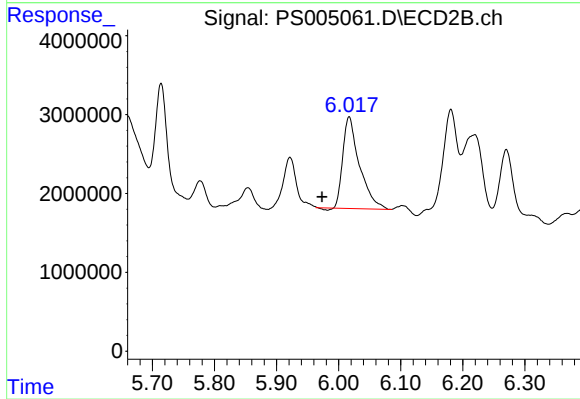

#8 DICHLORPROP


R.T.: 6.017 min
Delta R.T.: 0.043 min
Response: 21611282
Conc: 22.25 ng/ml

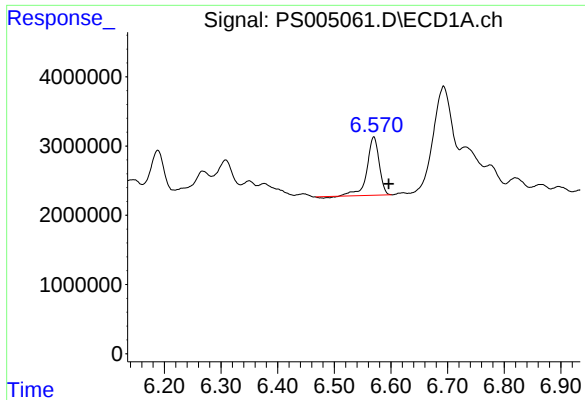

#9 2,4-D


R.T.: 6.570 min
Delta R.T.: -0.026 min
Response: 12572212
Conc: 9.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

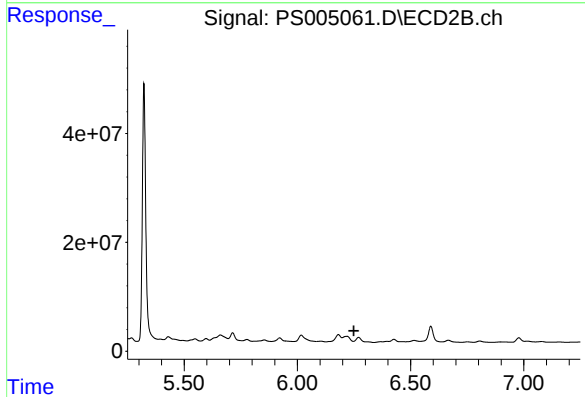


#9 2,4-D

R.T.: 6.181 min
Delta R.T.: -0.069 min
Response: -2285238
Conc: N.D.

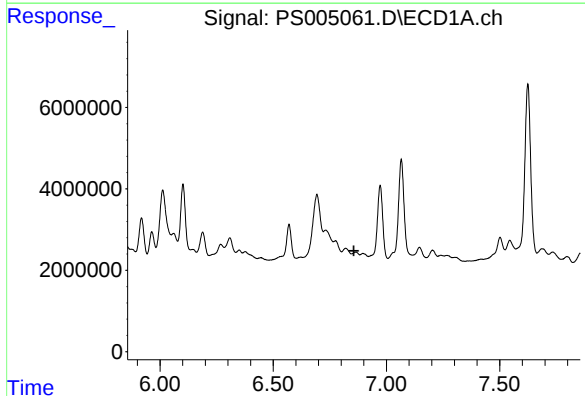


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.856 min
Response: 0
Conc: N.D.

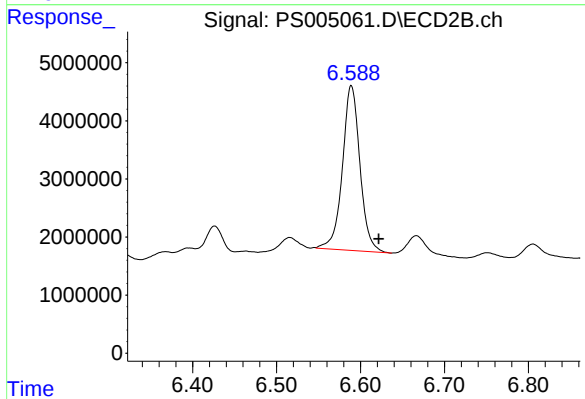

#10 Pentachlorophenol


R.T.: 6.589 min
Delta R.T.: -0.033 min
Response: 41207631
Conc: 3.20 ng/ml

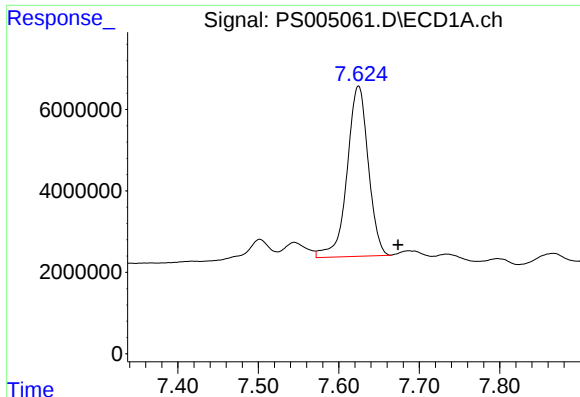

#12 2,4,5-T


R.T.: 7.624 min
Delta R.T.: -0.049 min
Response: 76543686
Conc: 9.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

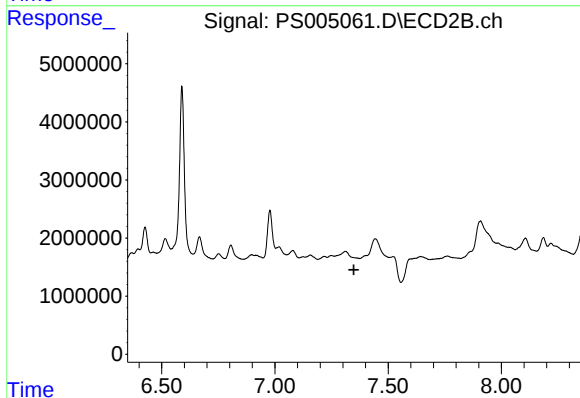


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.349 min
Response: 0
Conc: N.D.

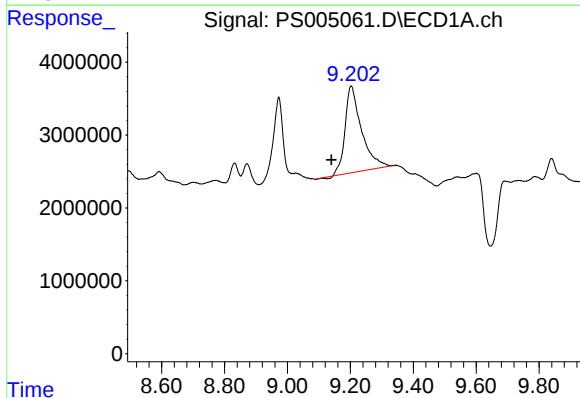

#15 Picloram

R.T.: 9.203 min
Delta R.T.: 0.063 min
Response: 42865939
Conc: 4.32 ng/ml

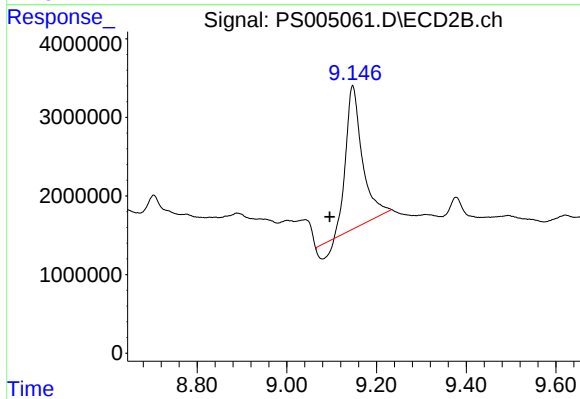

#15 Picloram

R.T.: 9.147 min
Delta R.T.: 0.051 min
Response: 44527815
Conc: 6.53 ng/ml