

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
 Data File : PS005051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2019 14:58
 Operator : SM\AJ
 Sample : K3369-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 Z-3-SOIL-4

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 16:08:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.571	5.284	340.1E6	209.0E6	258.065m	209.539m

Ankita

Target Compounds

6/18/2019 10:01:19 AM

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061719\
Data File : PS005051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2019 14:58
Operator : SM\AJ
Sample : K3369-16
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_S
ClientSampleId :
Z-3-SOIL-4

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 16:08:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

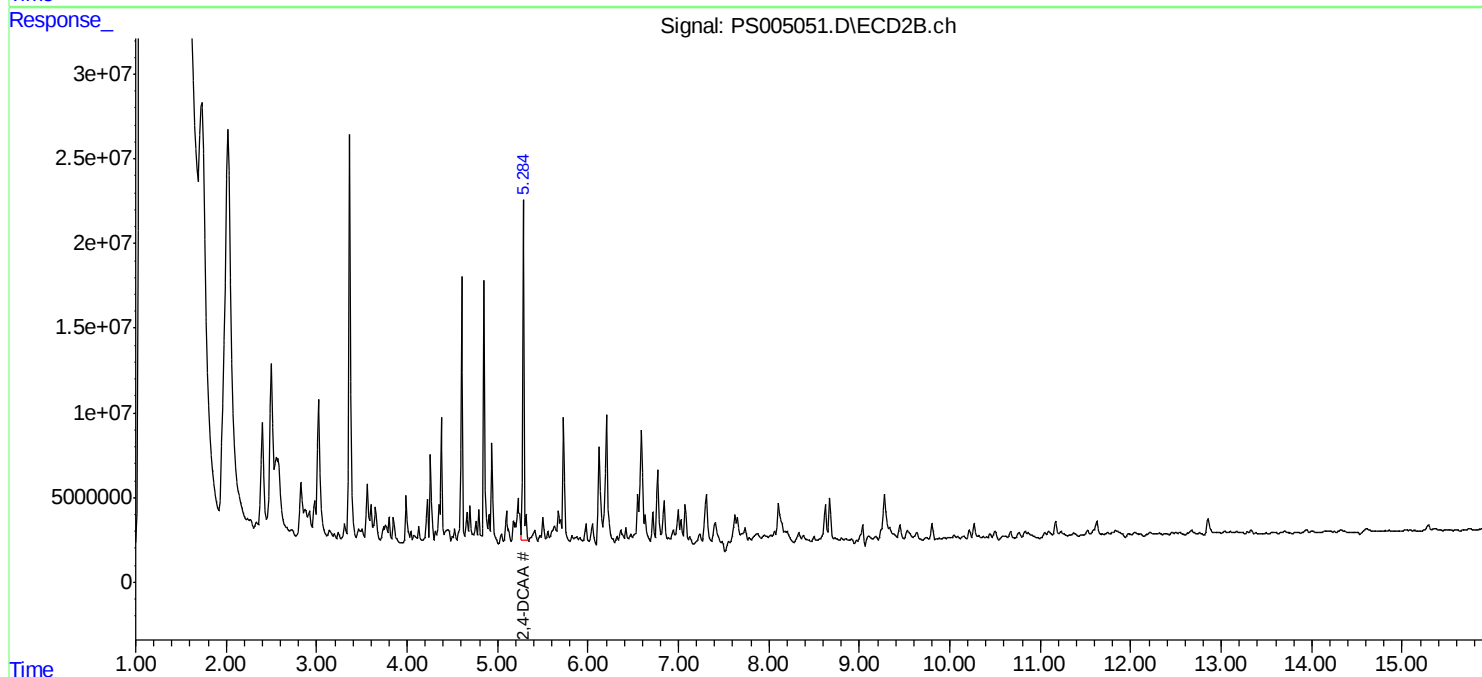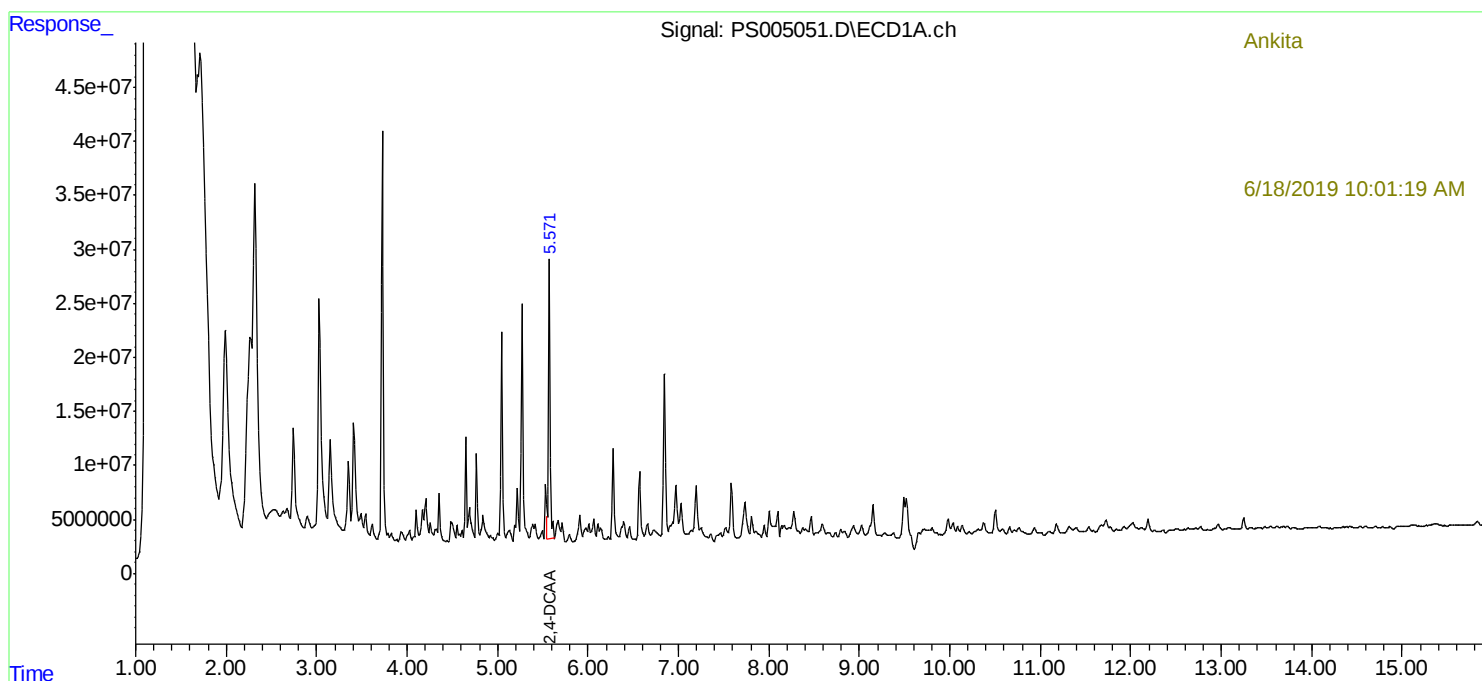

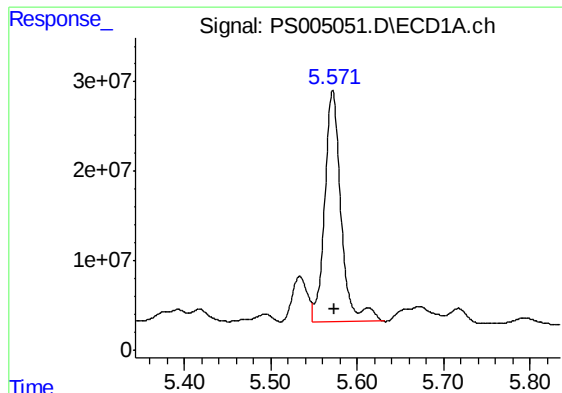


#4 2,4-DCAA

R.T.: 5.571 min
Delta R.T.: -0.003 min
Response: 340077053
Conc: 258.07 ng/ml m

Instrument :
ECD_S
ClientSampleId :
Z-3-SOIL-4

Manual Integrations
APPROVED

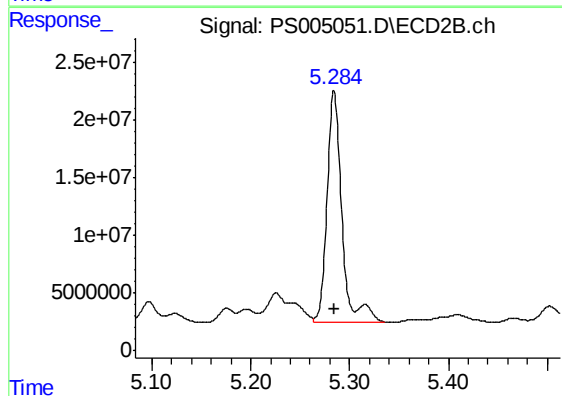

#4 2,4-DCAA

R.T.: 5.284 min
Delta R.T.: -0.001 min
Response: 209022829
Conc: 209.54 ng/ml m

Ankita

6/18/2019 10:01:19 AM