

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061721\
 Data File : PS015717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2021 17:01
 Operator : DD\AJ
 Sample : M2672-29
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:10:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.190	6.769	992.8E6	279.2E6	597.560	554.063
Target Compounds							
1) T	Dalapon	2.976f	2.484	33313347	46490081	16.505	71.580 #
2) T	3,5-DICHL...	0.000	5.984	0	86457289	N.D.	114.640
5) T	DICAMBA	7.369	0.000	13637197	0	2.121	N.D. #
6) T	MCP	7.548	0.000	5428130	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.571	0	10041821	N.D.	19.395
9) T	2,4-D	8.375f	0.000	38395344	0	21.908	N.D. #
10) T	Pentachlo...	8.679f	8.334f	13742202	6317456	<MDL	<MDL #
12) T	2,4,5-T	9.399f	9.082f	47133460	10977828	5.339	3.892 #
13) T	2,4-DB	9.969	0.000	52248664	0	25.543	N.D. #
14) T	DINOSEB	11.123	9.885	63541330	179.9E6	9.811	89.326 #
15) T	Picloram	10.953	0.000	179.1E6	0	13.103	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061721\
Data File : PS015717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2021 17:01
Operator : DD\AJ
Sample : M2672-29
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:10:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

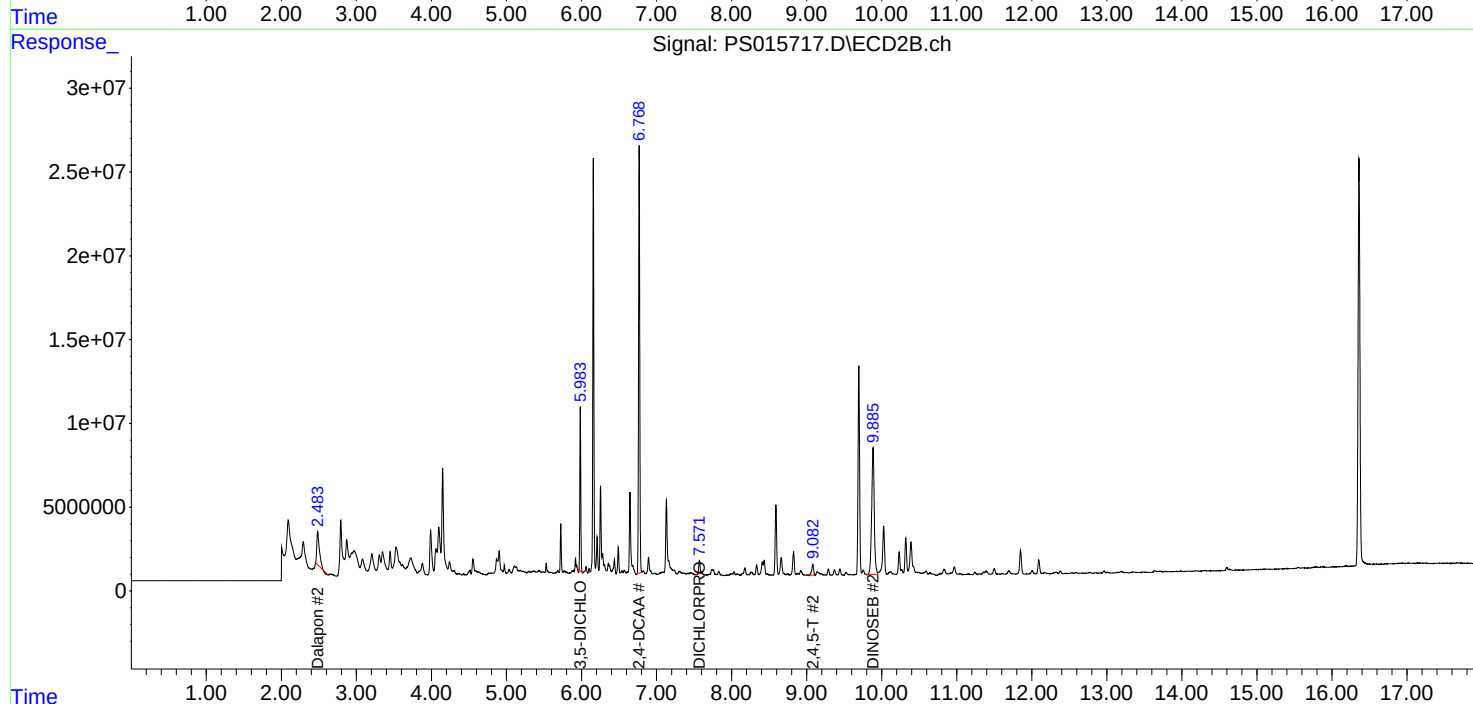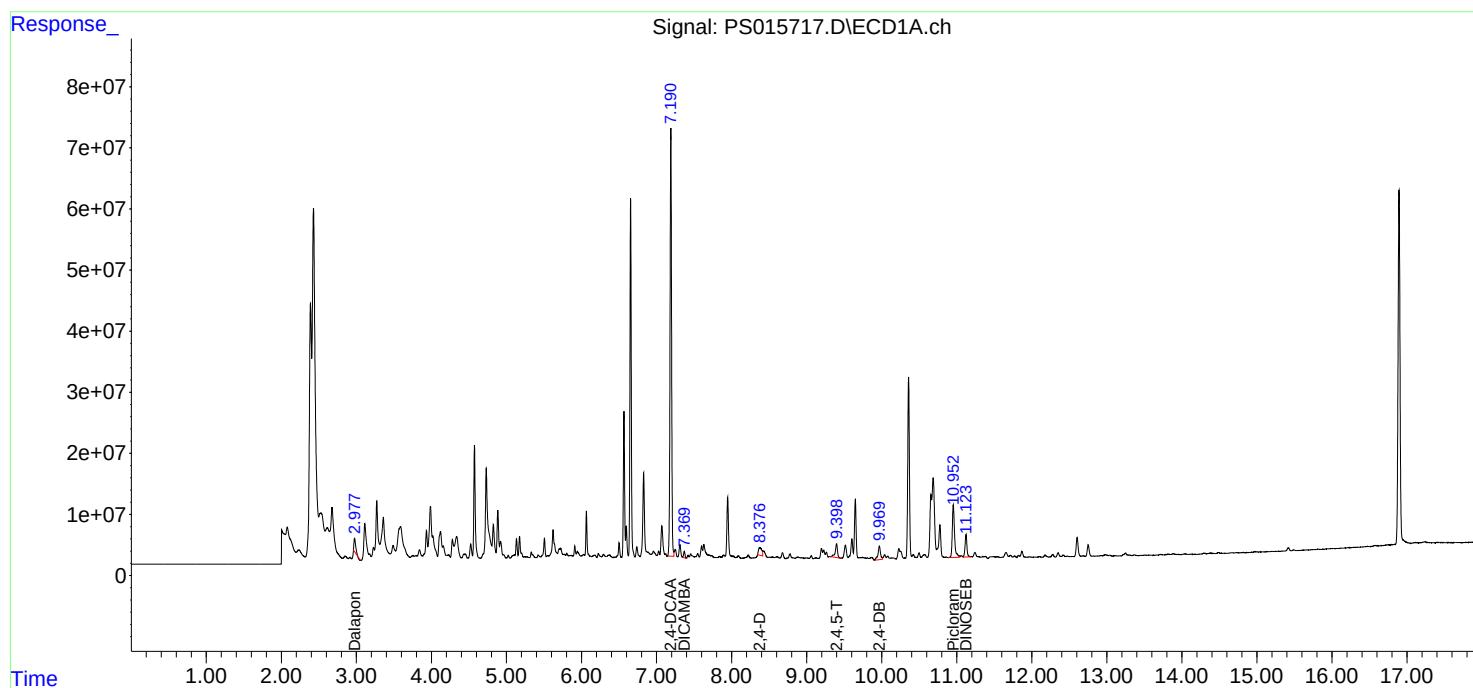


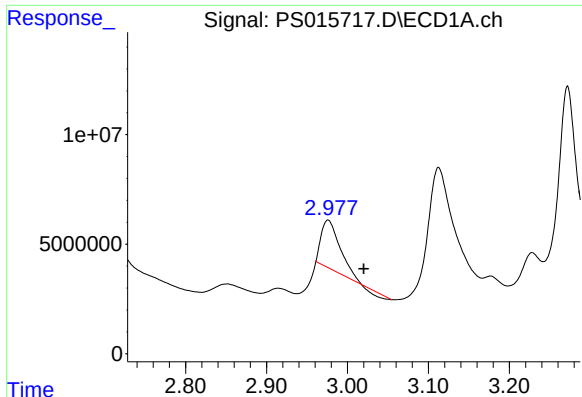

#1 Dalapon


R.T.: 2.976 min
Delta R.T.: -0.044 min
Response: 33313347
Conc: 16.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

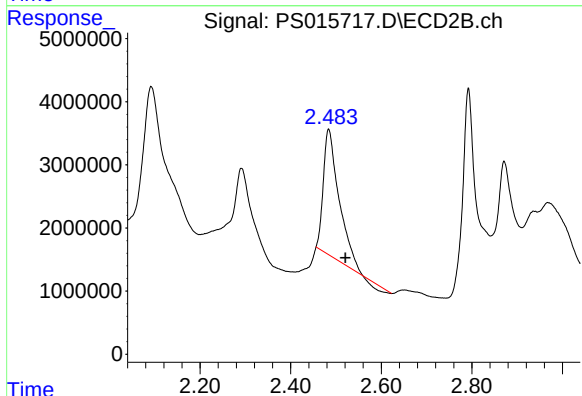


#1 Dalapon

R.T.: 2.484 min
Delta R.T.: -0.037 min
Response: 46490081
Conc: 71.58 ng/ml

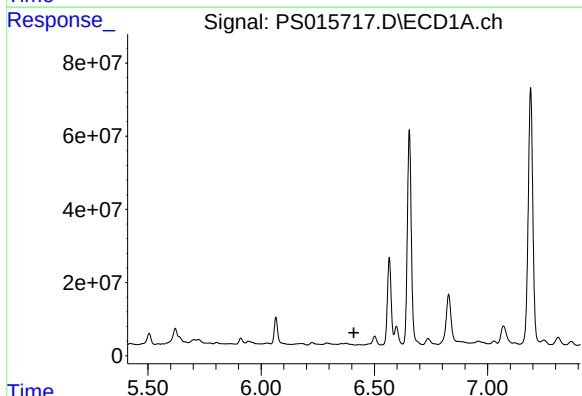


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

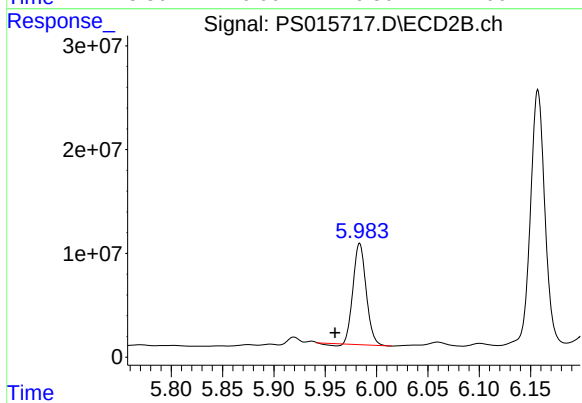

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.984 min
Delta R.T.: 0.024 min
Response: 86457289
Conc: 114.64 ng/ml

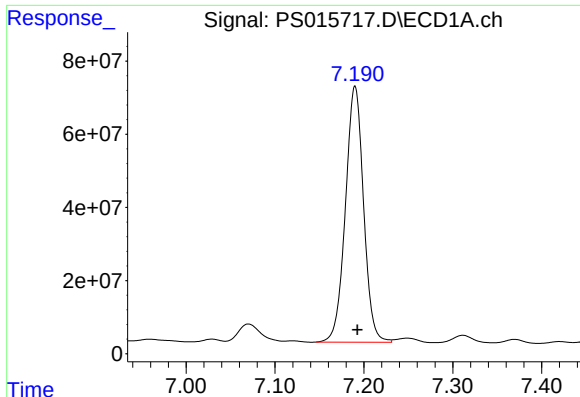

#4 2,4-DCAA


R.T.: 7.190 min
Delta R.T.: -0.003 min
Response: 992813429
Conc: 597.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

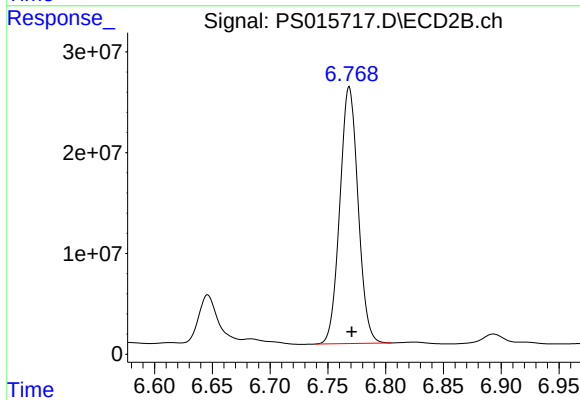


#4 2,4-DCAA

R.T.: 6.769 min
Delta R.T.: -0.002 min
Response: 279165665
Conc: 554.06 ng/ml

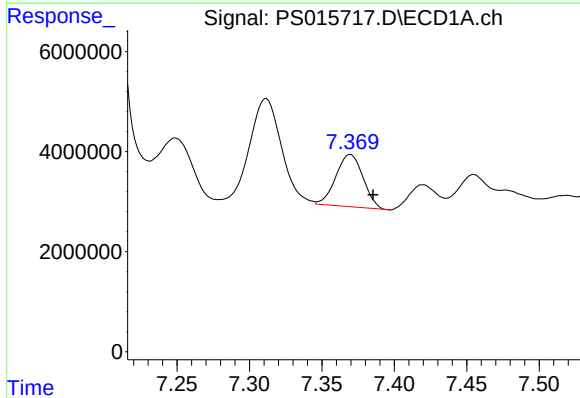


#5 DICAMBA

R.T.: 7.369 min
Delta R.T.: -0.016 min
Response: 13637197
Conc: 2.12 ng/ml

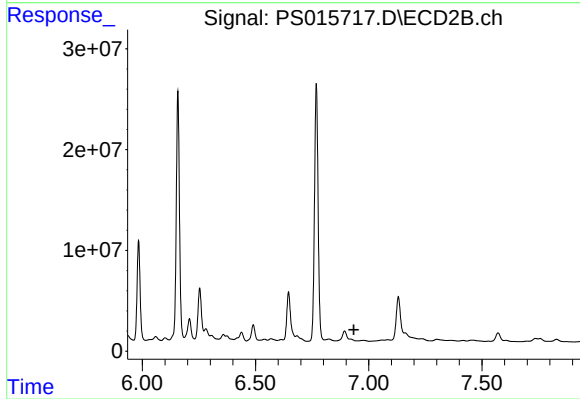

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

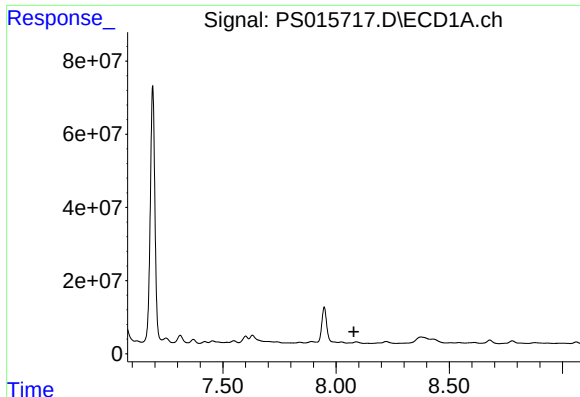

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

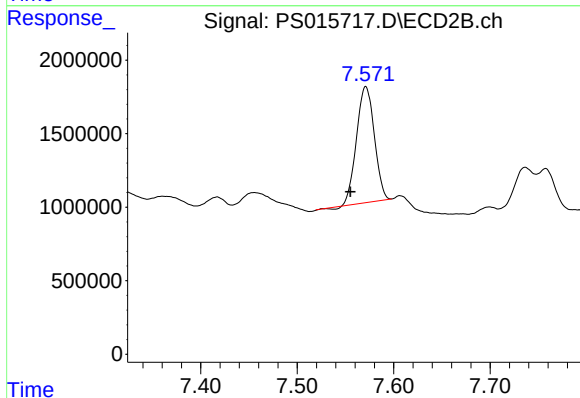


#8 DICHLORPROP

R.T.: 7.571 min
Delta R.T.: 0.016 min
Response: 10041821
Conc: 19.40 ng/ml

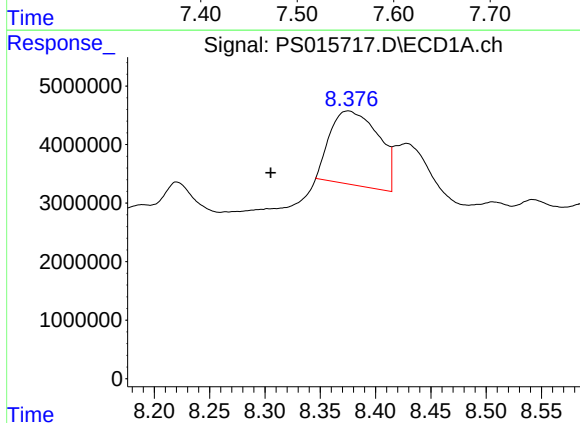


#9 2,4-D

R.T.: 8.375 min
Delta R.T.: 0.070 min
Response: 38395344
Conc: 21.91 ng/ml

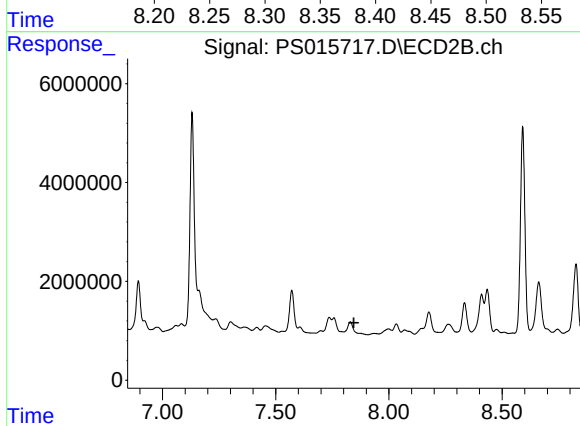

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

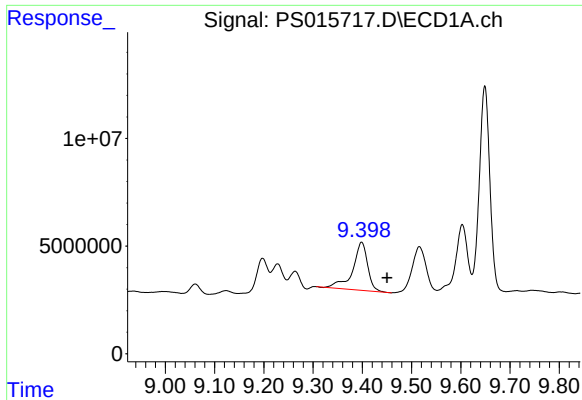

#12 2,4,5-T


R.T.: 9.399 min
Delta R.T.: -0.052 min
Response: 47133460
Conc: 5.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

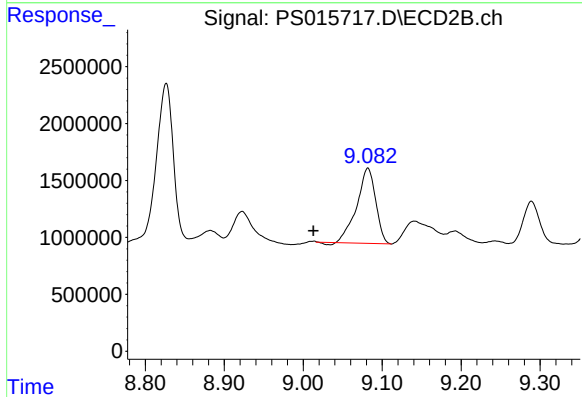


#12 2,4,5-T

R.T.: 9.082 min
Delta R.T.: 0.069 min
Response: 10977828
Conc: 3.89 ng/ml

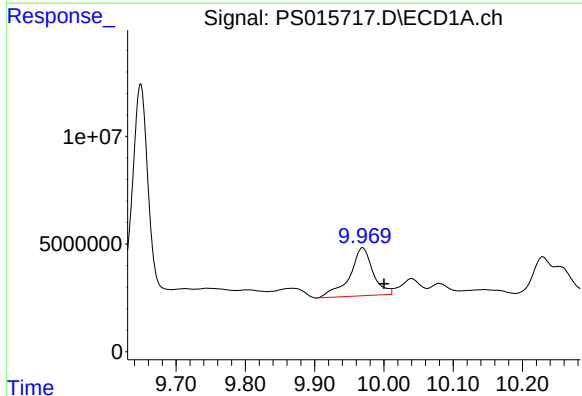


#13 2,4-DB

R.T.: 9.969 min
Delta R.T.: -0.031 min
Response: 52248664
Conc: 25.54 ng/ml

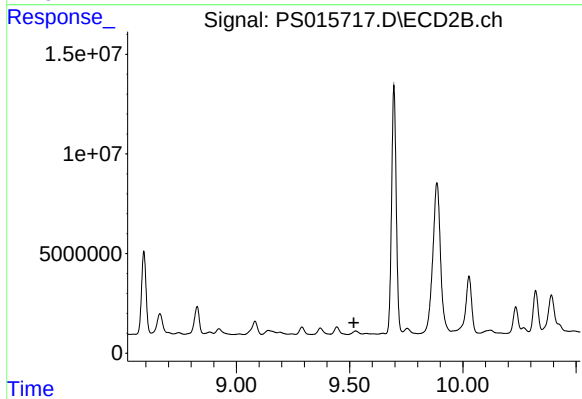

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.519 min
Response: 0
Conc: N.D.

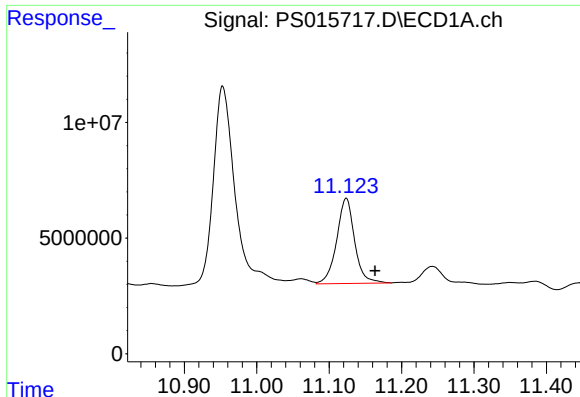

#14 DINOSEB


R.T.: 11.123 min
Delta R.T.: -0.040 min
Response: 63541330
Conc: 9.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

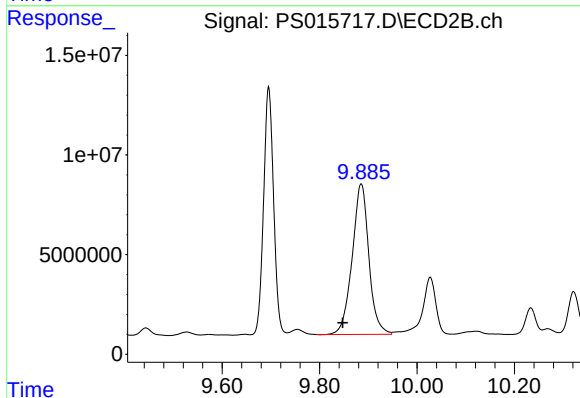


#14 DINOSEB

R.T.: 9.885 min
Delta R.T.: 0.038 min
Response: 179913294
Conc: 89.33 ng/ml

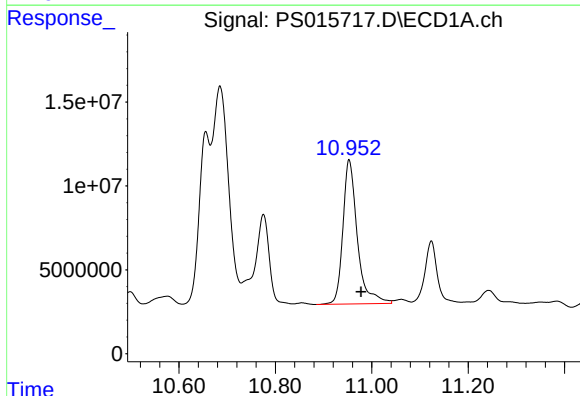

#15 Picloram

R.T.: 10.953 min
Delta R.T.: -0.025 min
Response: 179128281
Conc: 13.10 ng/ml

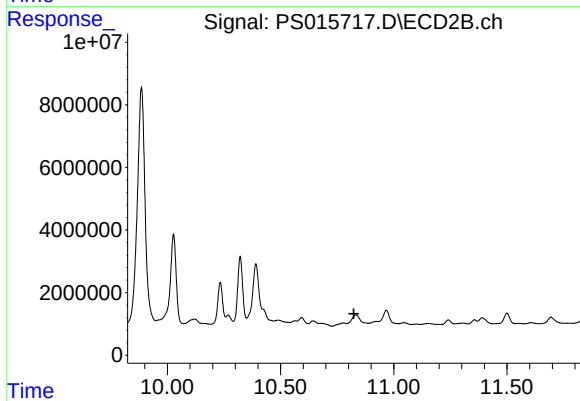

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.824 min
Response: 0
Conc: N.D.