

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061721\
 Data File : PS015730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2021 22:15
 Operator : DD\AJ
 Sample : M2672-40
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 01:12:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.190	6.769	1037.3E6	286.2E6	624.339	568.066
Target Compounds							
1) T	Dalapon	2.977f	2.484	34689232	53571866	17.187	82.484 #
2) T	3,5-DICHL...	0.000	5.984	0	87077865	N.D.	115.463
3) T	4-Nitroph...	7.028	0.000	3444994	0	3.789	N.D. #
5) T	DICAMBA	7.369	0.000	14577651	0	2.267	N.D. #
6) T	MCP	7.548	0.000	5427869	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.571	0	10420650	N.D.	20.127
10) T	Pentachlo...	8.678f	8.334f	12153230	4782362	<MDL	<MDL #
12) T	2,4,5-T	9.398f	9.081f	44869313	11194442	5.082	3.969
13) T	2,4-DB	9.968	0.000	57933988	0	28.322	N.D. #
14) T	DINOSEB	11.123f	9.885	71107640	129.5E6	10.979	64.271 #
15) T	Picloram	10.952	0.000	196.2E6	0	14.352	N.D. #
16) T	DCPA	11.494f	0.000	11388254	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061721\
Data File : PS015730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2021 22:15
Operator : DD\AJ
Sample : M2672-40
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 01:12:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

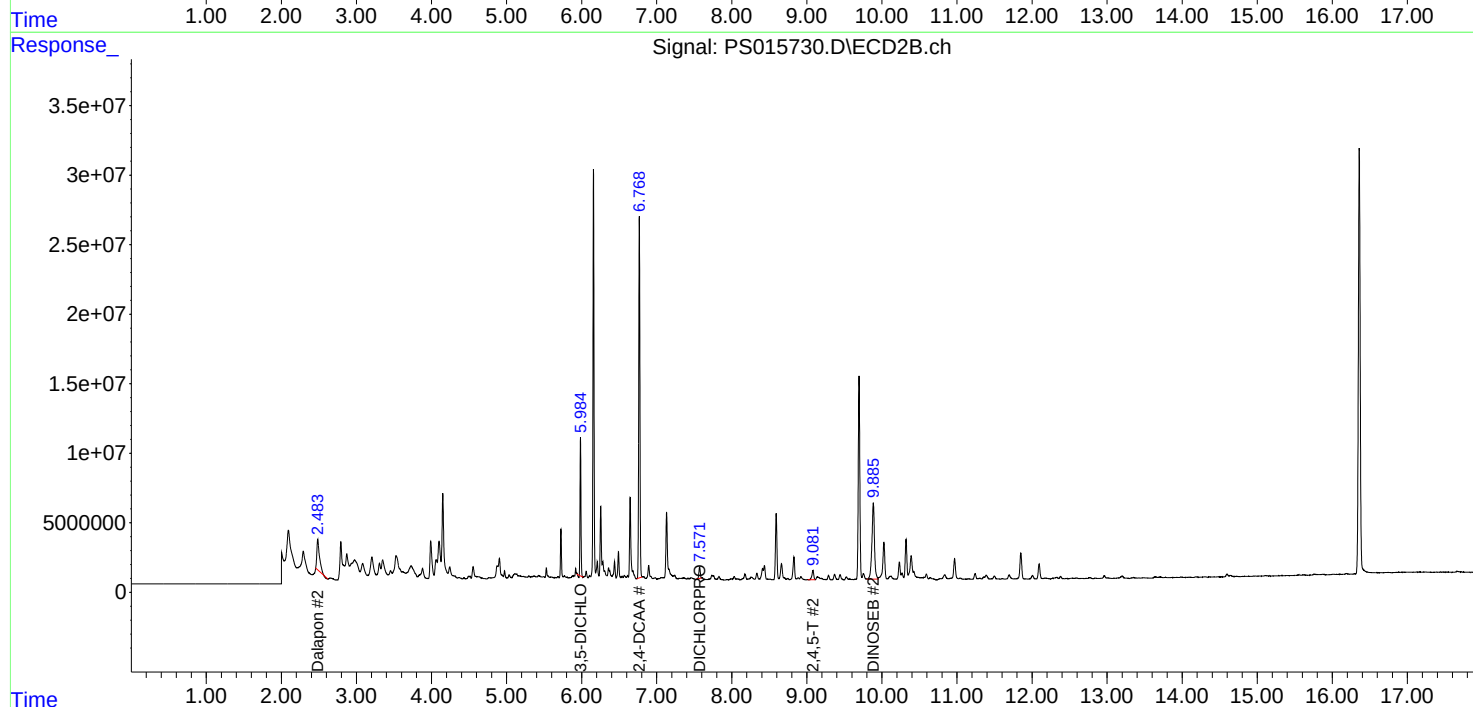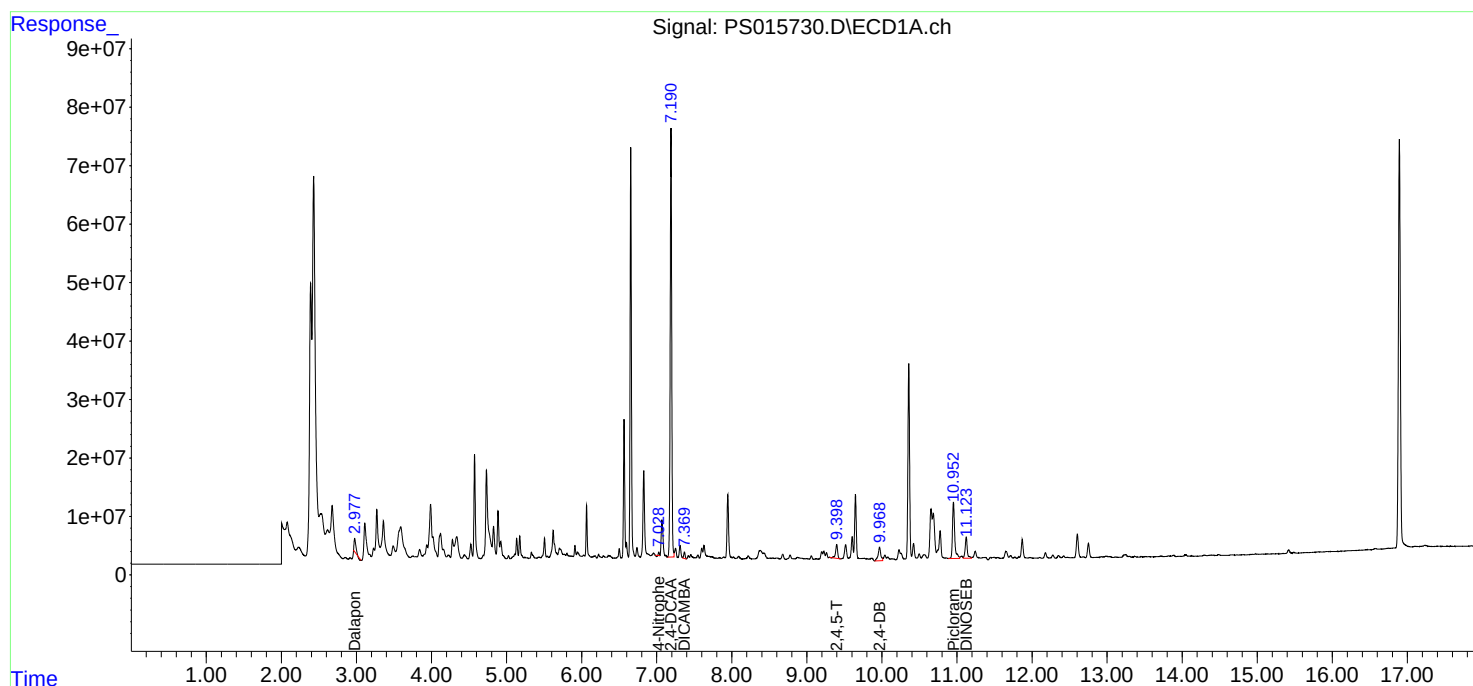


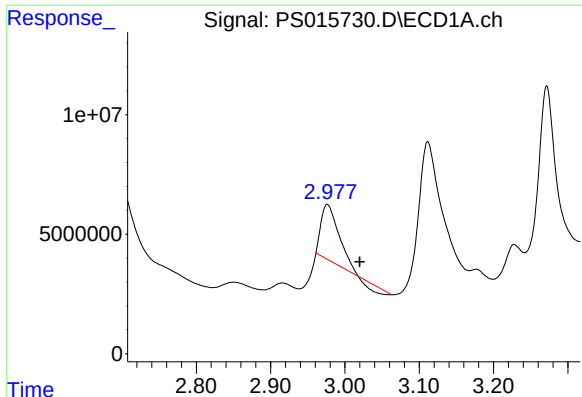

#1 Dalapon


R.T.: 2.977 min
Delta R.T.: -0.043 min
Response: 34689232
Conc: 17.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

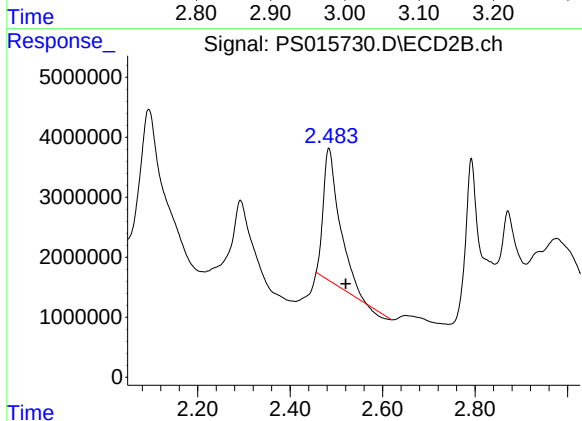


#1 Dalapon

R.T.: 2.484 min
Delta R.T.: -0.037 min
Response: 53571866
Conc: 82.48 ng/ml

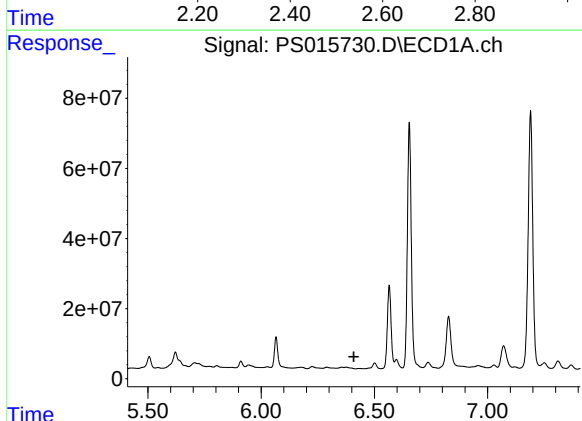


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

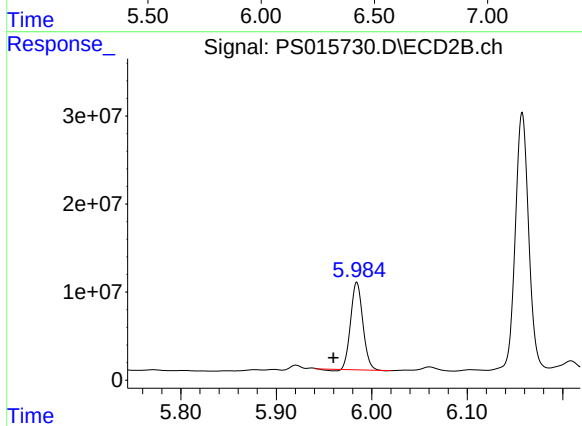

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.984 min
Delta R.T.: 0.025 min
Response: 87077865
Conc: 115.46 ng/ml

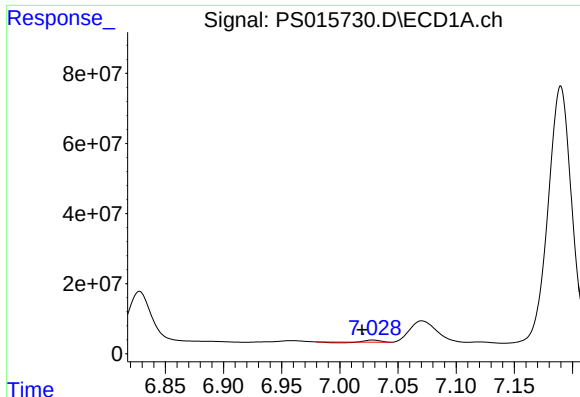

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: 0.009 min
Response: 3444994
Conc: 3.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

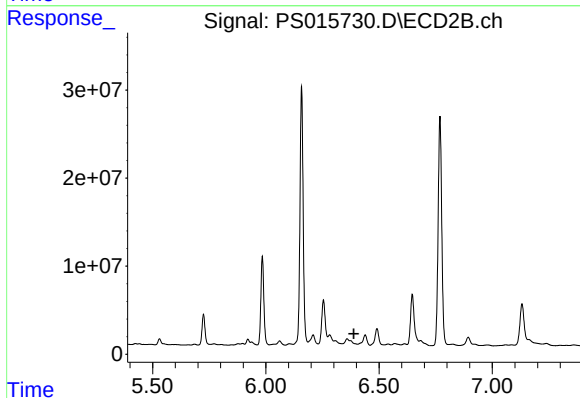


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

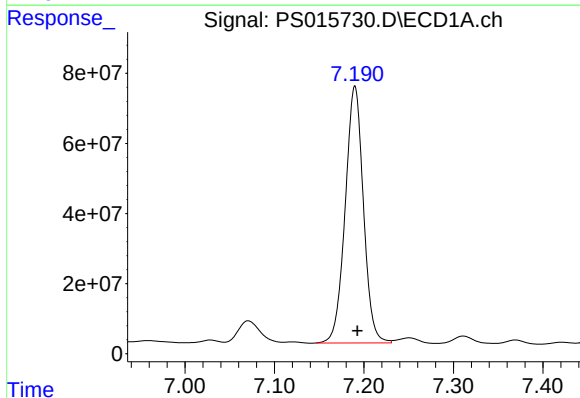


#4 2,4-DCAA

R.T.: 7.190 min
Delta R.T.: -0.003 min
Response: 1037306082
Conc: 624.34 ng/ml

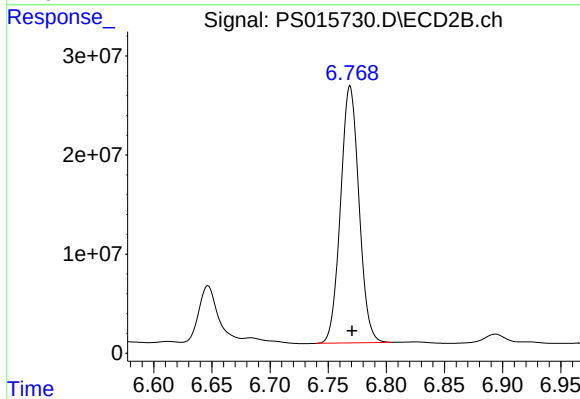

#4 2,4-DCAA


R.T.: 6.769 min
Delta R.T.: -0.002 min
Response: 286221168
Conc: 568.07 ng/ml

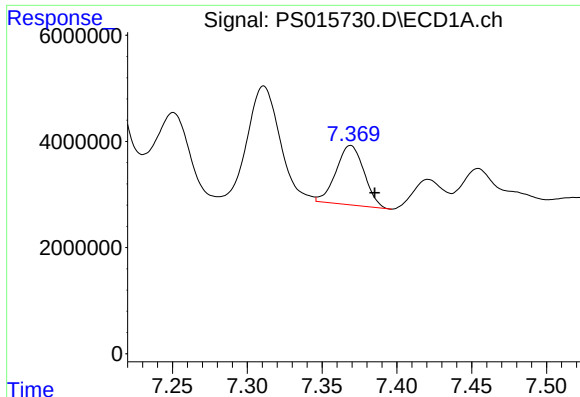

#5 DICAMBA


R.T.: 7.369 min
Delta R.T.: -0.016 min
Response: 14577651
Conc: 2.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

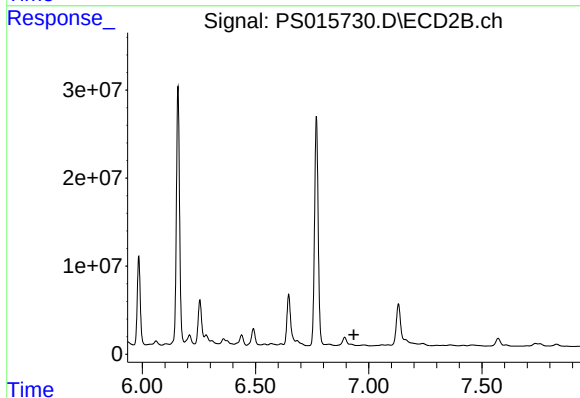


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

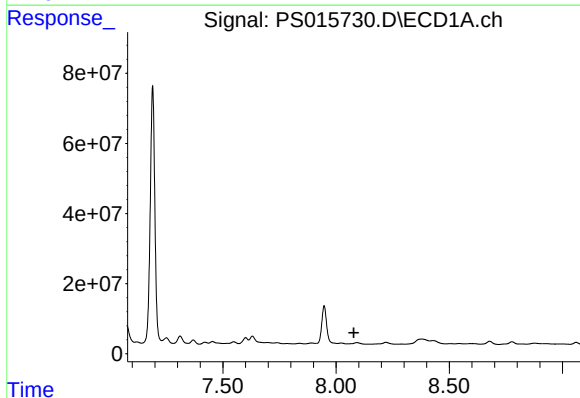


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.079 min
Response: 0
Conc: N.D.

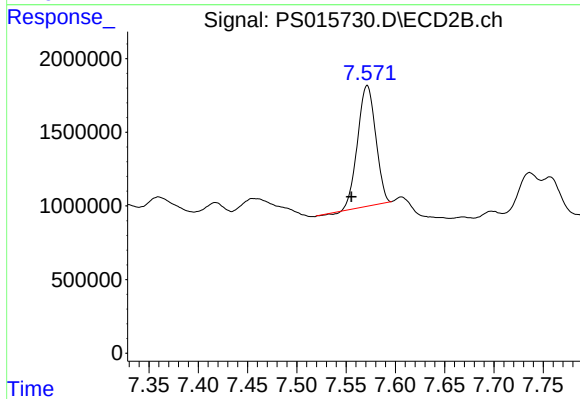

#8 DICHLORPROP


R.T.: 7.571 min
Delta R.T.: 0.016 min
Response: 10420650
Conc: 20.13 ng/ml

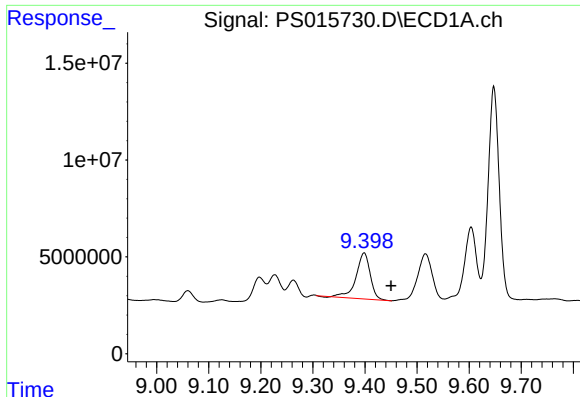

#12 2,4,5-T


R.T.: 9.398 min
Delta R.T.: -0.052 min
Response: 44869313
Conc: 5.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

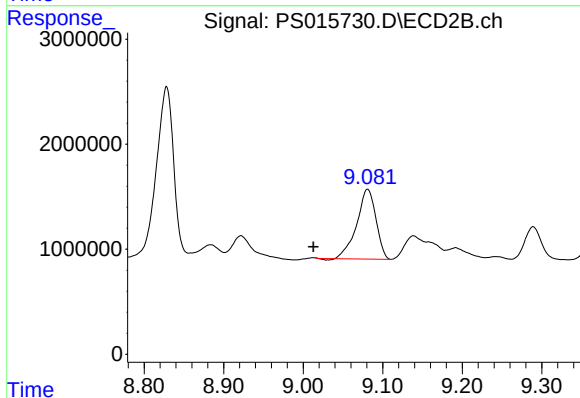


#12 2,4,5-T

R.T.: 9.081 min
Delta R.T.: 0.068 min
Response: 11194442
Conc: 3.97 ng/ml

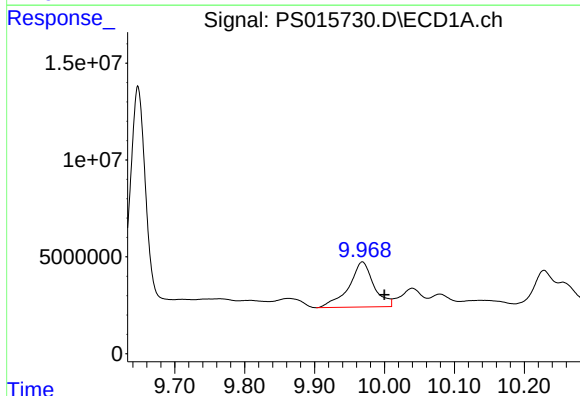


#13 2,4-DB

R.T.: 9.968 min
Delta R.T.: -0.032 min
Response: 57933988
Conc: 28.32 ng/ml

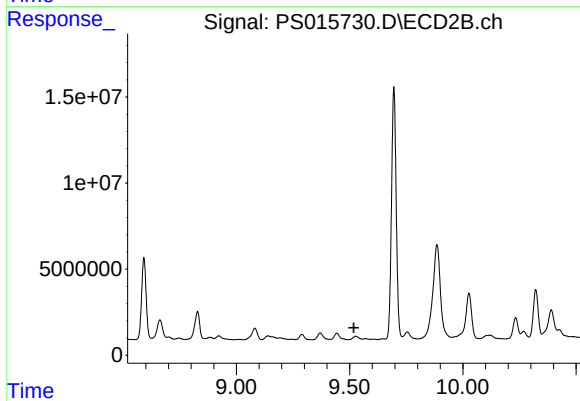

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.519 min
Response: 0
Conc: N.D.

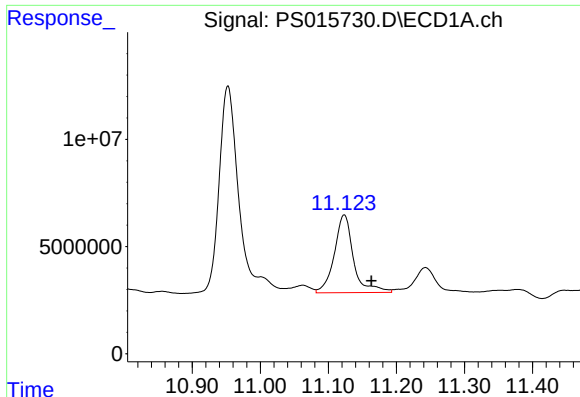

#14 DINOSEB


R.T.: 11.123 min
Delta R.T.: -0.040 min
Response: 71107640
Conc: 10.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

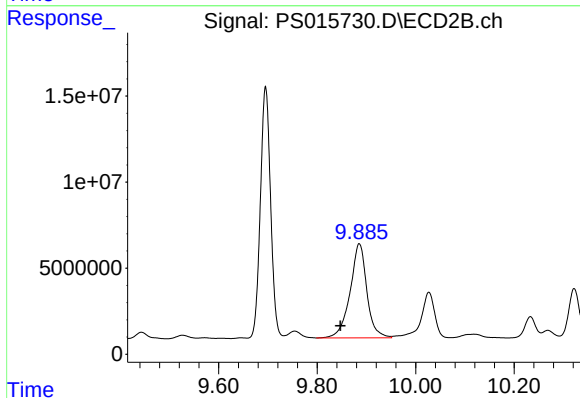


#14 DINOSEB

R.T.: 9.885 min
Delta R.T.: 0.038 min
Response: 129450085
Conc: 64.27 ng/ml

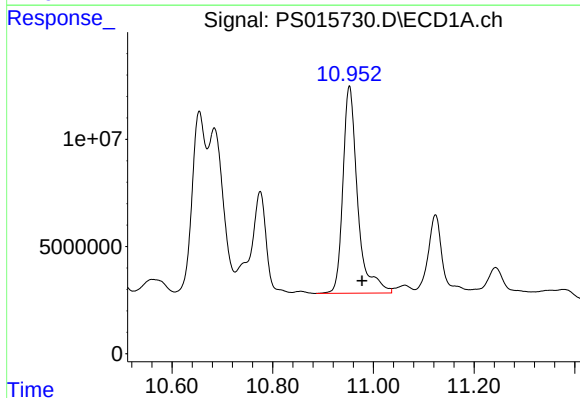

#15 Picloram

R.T.: 10.952 min
Delta R.T.: -0.025 min
Response: 196198260
Conc: 14.35 ng/ml

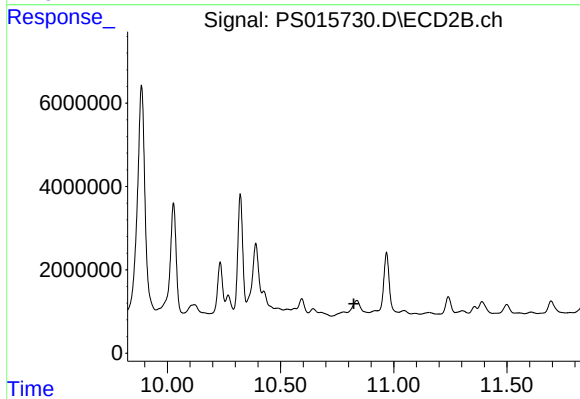

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.824 min
Response: 0
Conc: N.D.