

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061722\
 Data File : PS019738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2022 09:07
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 12:30:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.781	1072.3E6	436.3E6	446.938	563.056 #
Target Compounds							
1) T	Dalapon	3.004	0.000	1070087	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.367f	0.000	244133	0	<MDL	N.D. #
3) T	4-Nitroph...	0.000	6.392	0	459443	N.D.	1.073
7) T	MCPA	7.667	0.000	1012193	0	<MDL	N.D. #
10) T	Pentachlo...	8.622	8.285	638753	788797	<MDL	<MDL #
11) T	2,4,5-TP ...	9.198	8.629	1356509	583536	<MDL	<MDL #
12) T	2,4,5-T	9.461	9.063	7877476	229791	<MDL	<MDL #
13) T	2,4-DB	10.033	9.474f	5514129	988949	1.363	1.600
14) T	DINOSEB	0.000	9.853	0	335337	N.D.	<MDL
15) T	Picloram	10.991	10.894f	3147305	10878389	<MDL	1.691 #
16) T	DCPA	11.426	10.778	2772737	3003236	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061722\
Data File : PS019738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2022 09:07
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 12:30:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

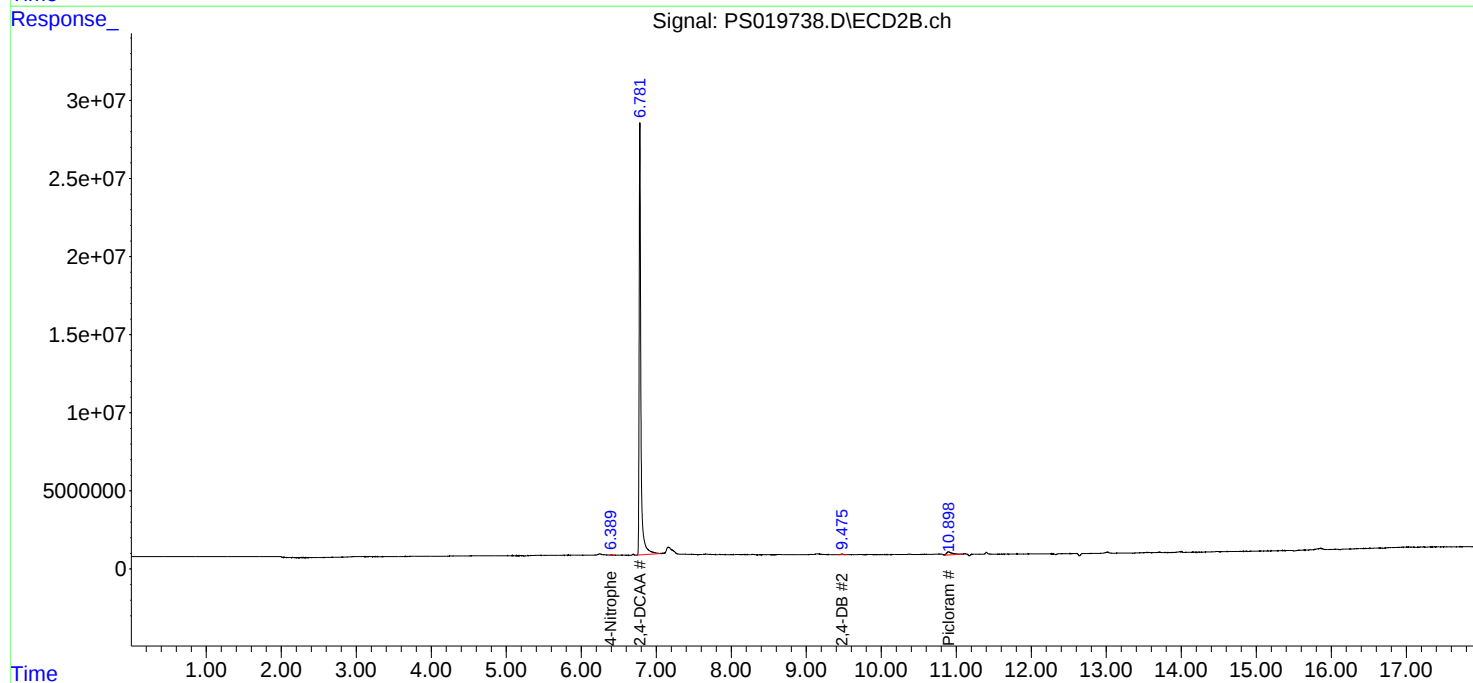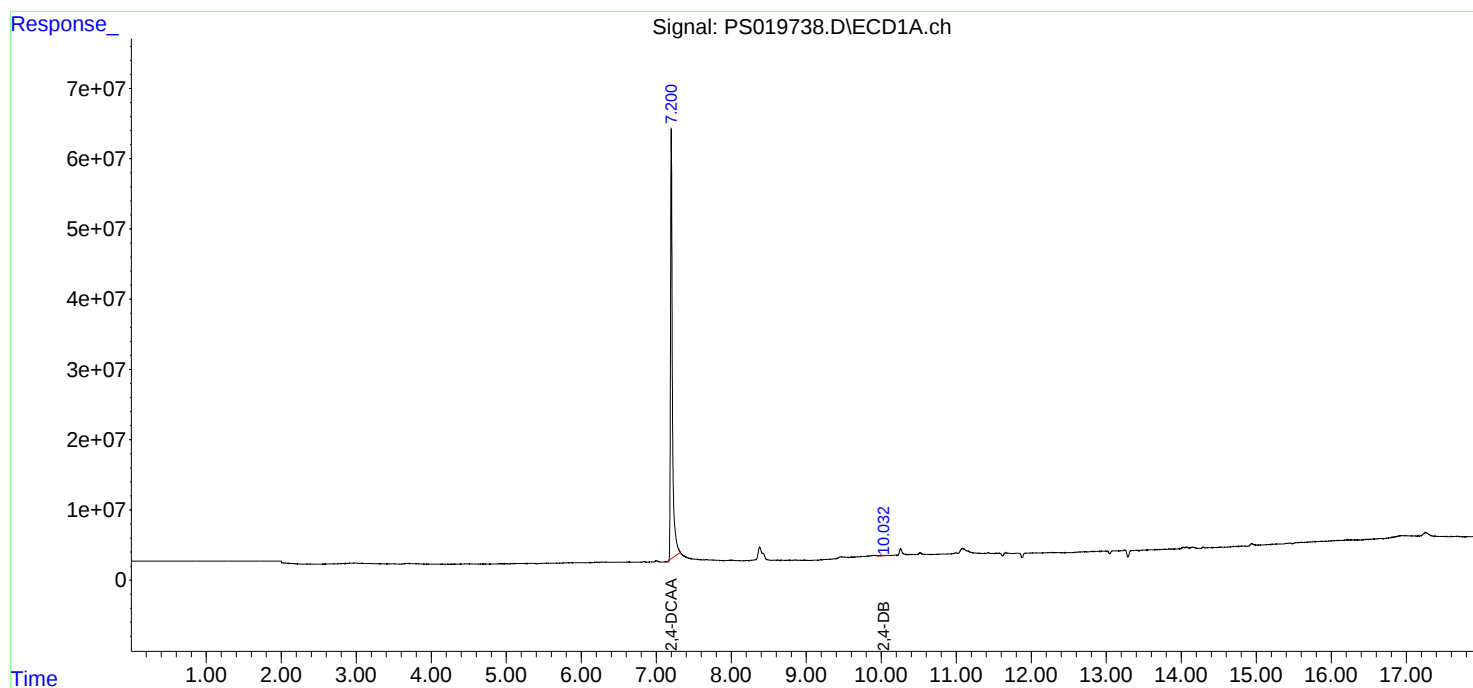


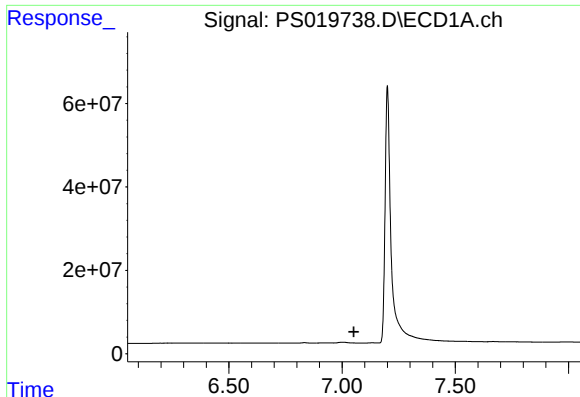

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.052 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

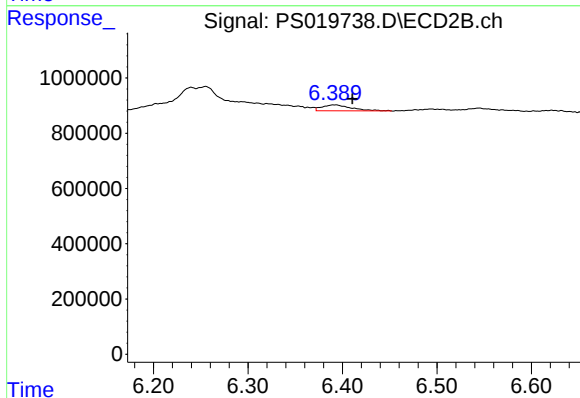


#3 4-Nitrophenol

R.T.: 6.392 min
Delta R.T.: -0.019 min
Response: 459443
Conc: 1.07 ng/ml

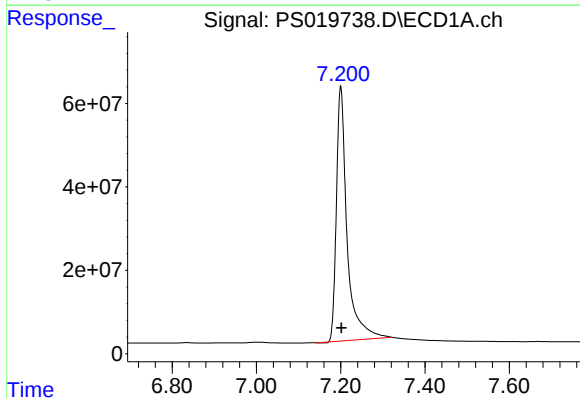


#4 2,4-DCAA

R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1072277854
Conc: 446.94 ng/ml

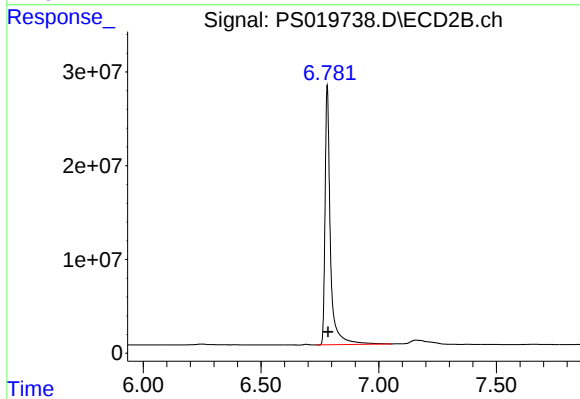

#4 2,4-DCAA


R.T.: 6.781 min
Delta R.T.: -0.003 min
Response: 436295606
Conc: 563.06 ng/ml

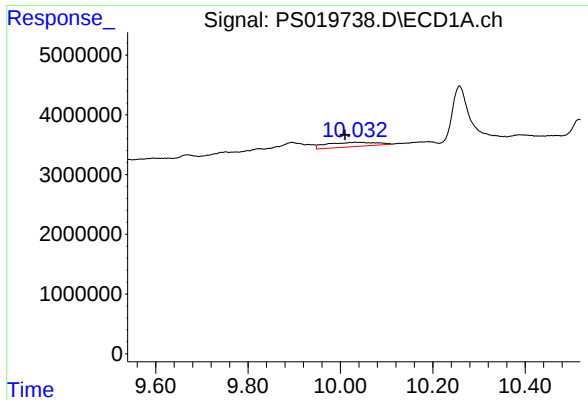

#13 2,4-DB


R.T.: 10.033 min
Delta R.T.: 0.023 min
Response: 5514129
Conc: 1.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

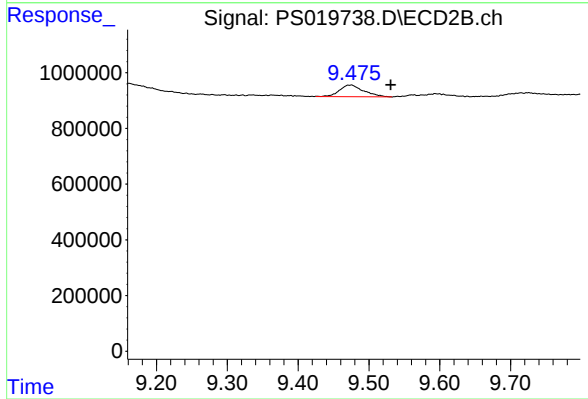


#13 2,4-DB

R.T.: 9.474 min
Delta R.T.: -0.057 min
Response: 988949
Conc: 1.60 ng/ml

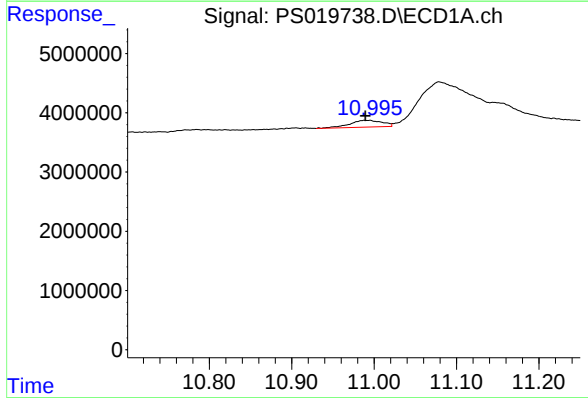

#15 Picloram

R.T.: 10.991 min
Delta R.T.: 0.002 min
Response: 3147305
Conc: N.D.

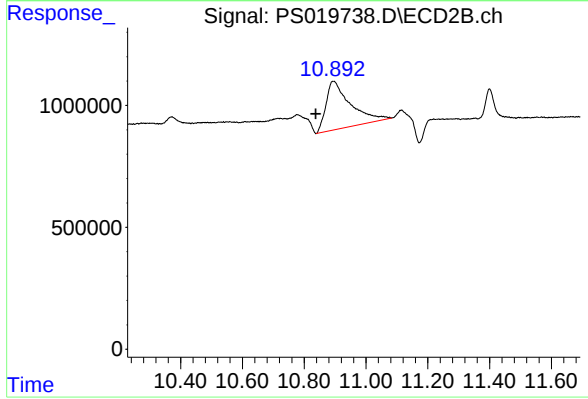

#15 Picloram

R.T.: 10.894 min
Delta R.T.: 0.057 min
Response: 10878389
Conc: 1.69 ng/ml