

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 08:27
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 13:28:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
2) T	3,5-DICHL...	4.950	0.000	898.7E6	0	476.809	N.D. #
5) T	DICAMBA	0.000	5.450	0	668.1E6	N.D.	173.961
6) T	MCP	0.000	5.450	0	668.1E6	N.D.	231.219
7) T	MCPA	5.980	0.000	2593639	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	5.988	0	24524026	N.D.	25.251
9) T	2,4-D	6.625	0.000	792.0E6	0	586.925	N.D. #
12) T	2,4,5-T	0.000	7.405	0	46193446	N.D.	9.794
15) T	Picloram	9.124	9.111	719.8E6	216.0E6	72.506	31.665 #
16) T	DCPA	0.000	9.111	0	216.0E6	N.D.	32.754



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 08:27
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 13:28:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

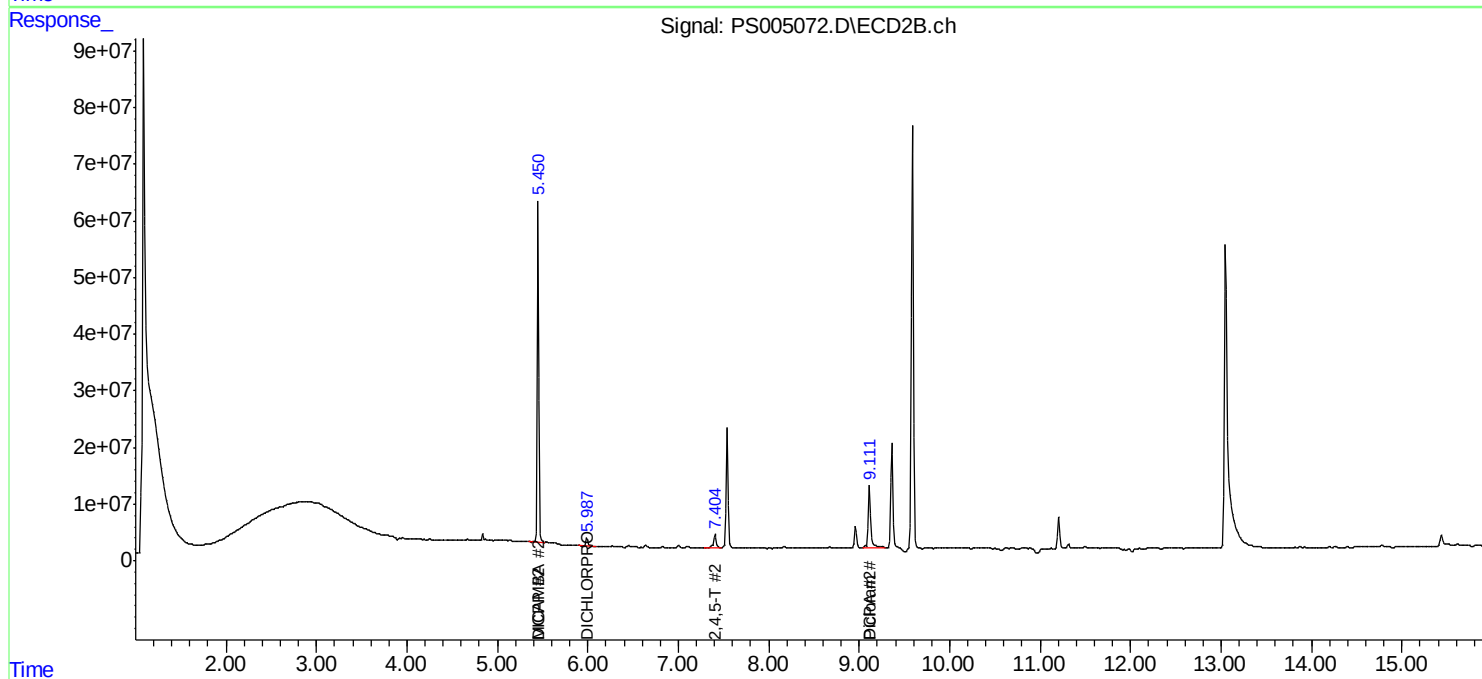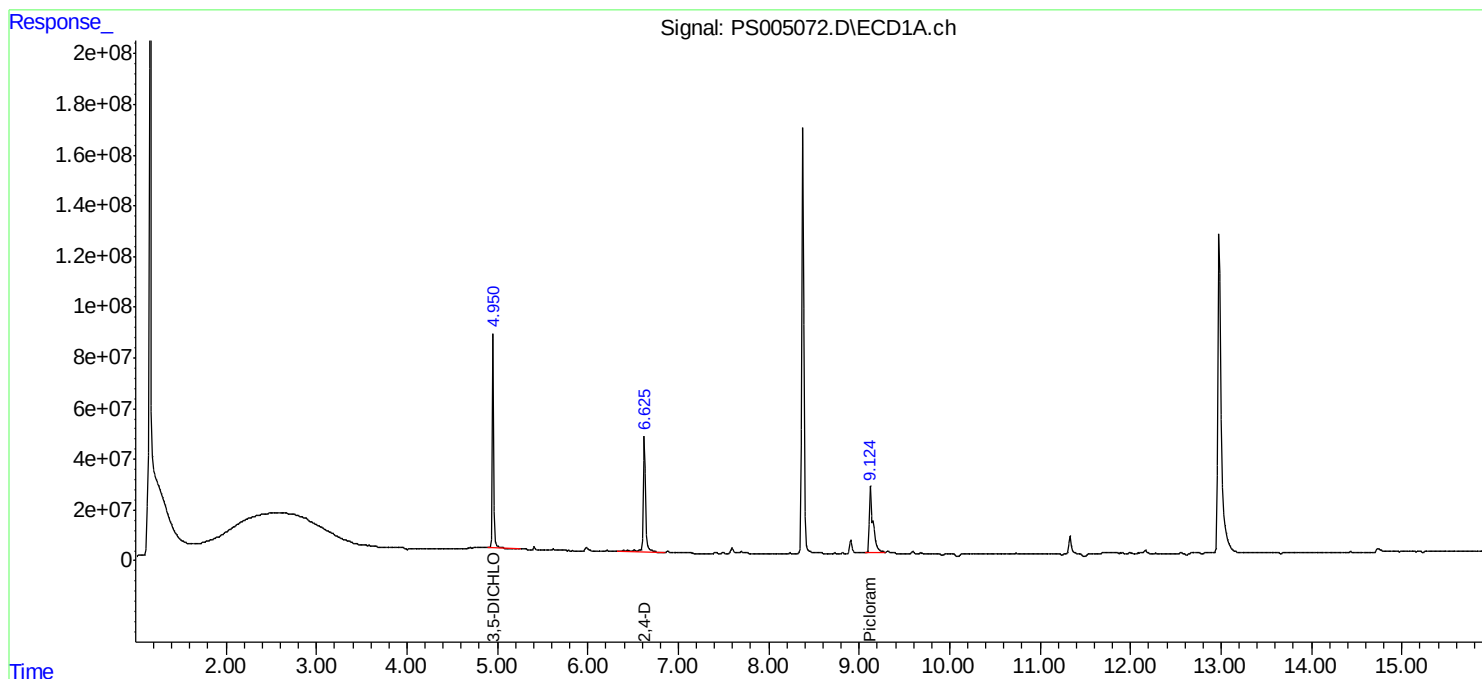


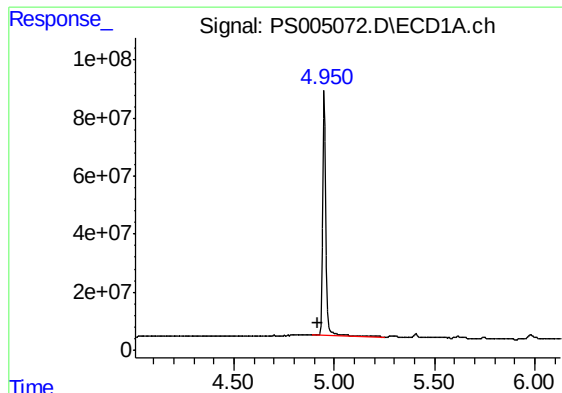

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.950 min
Delta R.T.: 0.029 min
Response: 898709437
Conc: 476.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

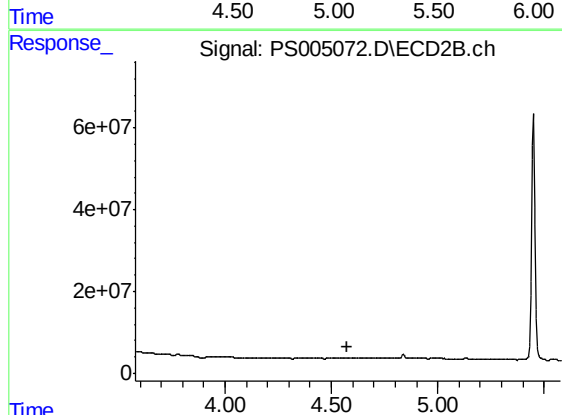


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.578 min
Response: 0
Conc: N.D.

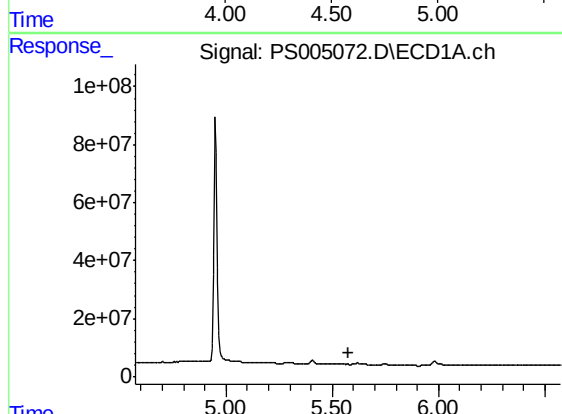


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.574 min
Response: 0
Conc: N.D.

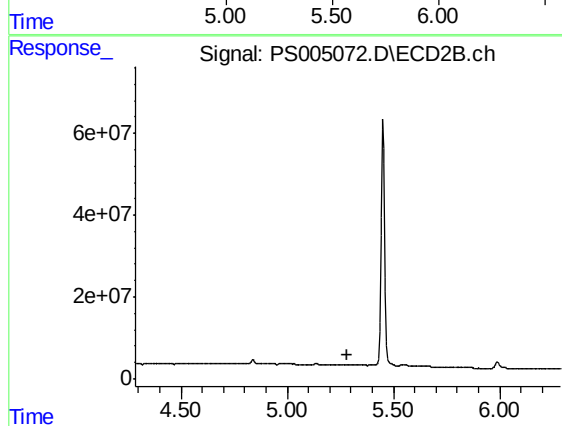

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.285 min
Response: 0
Conc: N.D.

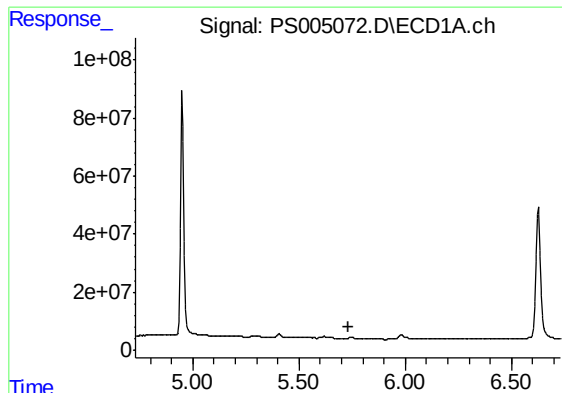

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

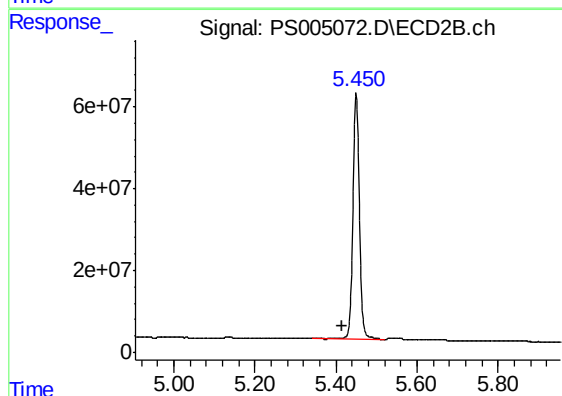


#5 DICAMBA

R.T.: 5.450 min
Delta R.T.: 0.033 min
Response: 668098107
Conc: 173.96 ng/ml

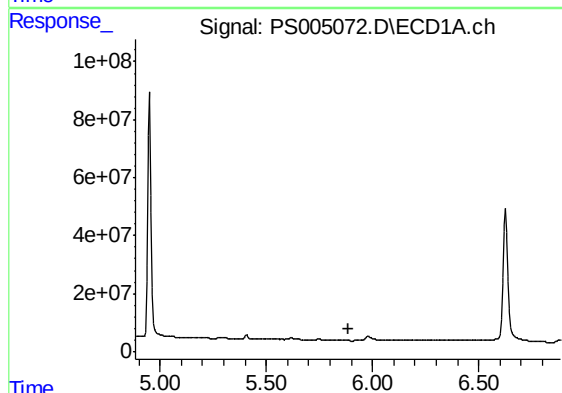


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.885 min
Response: 0
Conc: N.D.

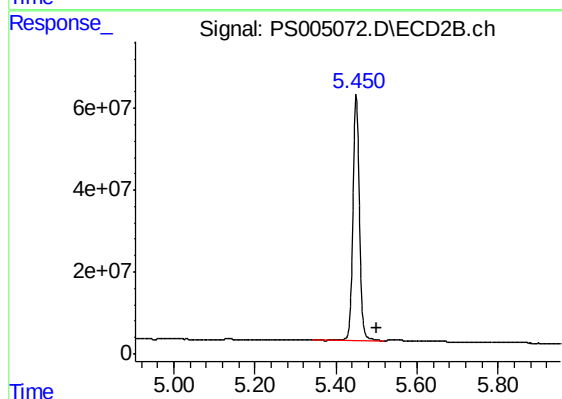

#6 MCPP


R.T.: 5.450 min
Delta R.T.: -0.050 min
Response: 668098107
Conc: 231.22 ug/ml

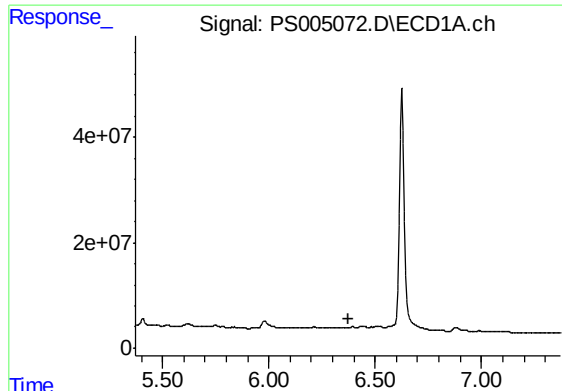

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

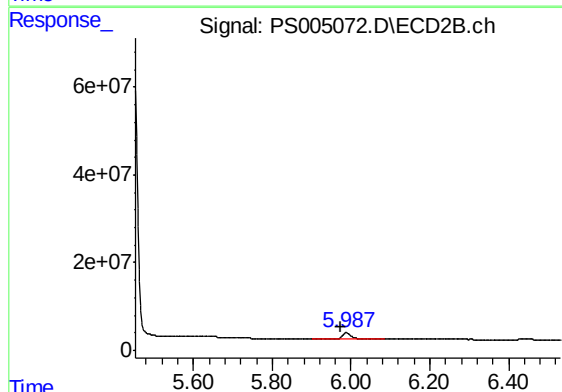


#8 DICHLORPROP

R.T.: 5.988 min
Delta R.T.: 0.015 min
Response: 24524026
Conc: 25.25 ng/ml

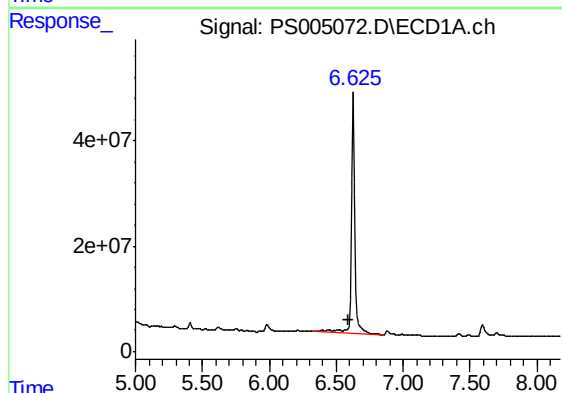


#9 2,4-D

R.T.: 6.625 min
Delta R.T.: 0.030 min
Response: 791965442
Conc: 586.93 ng/ml

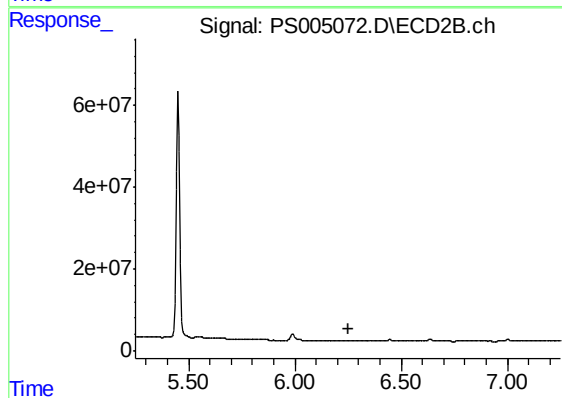

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

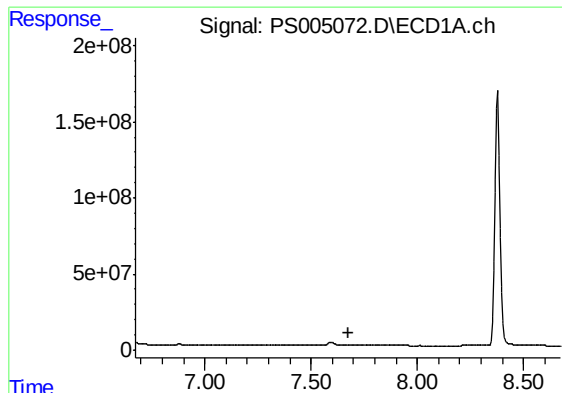

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

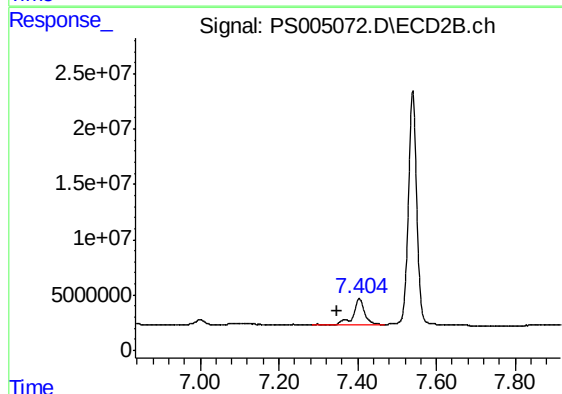


#12 2,4,5-T

R.T.: 7.405 min
Delta R.T.: 0.056 min
Response: 46193446
Conc: 9.79 ng/ml

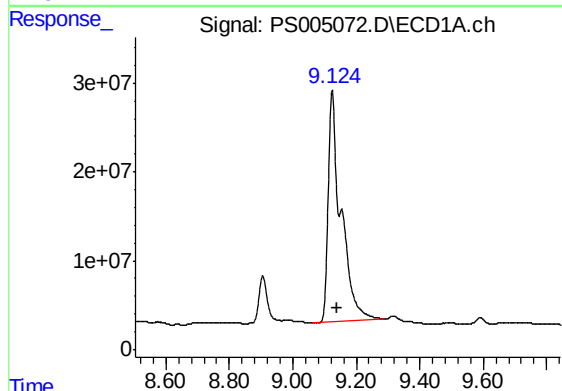


#15 Picloram

R.T.: 9.124 min
Delta R.T.: -0.015 min
Response: 719843700
Conc: 72.51 ng/ml

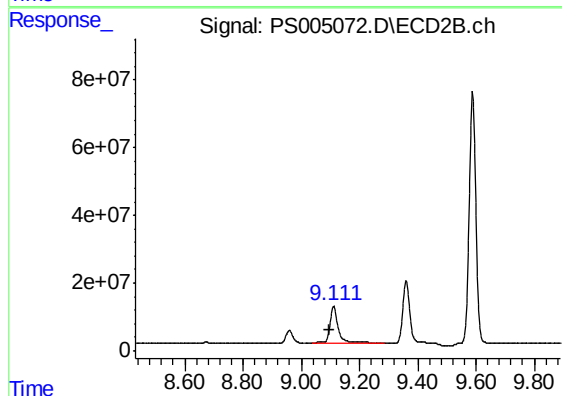

#15 Picloram


R.T.: 9.111 min
Delta R.T.: 0.016 min
Response: 215993543
Conc: 31.67 ng/ml

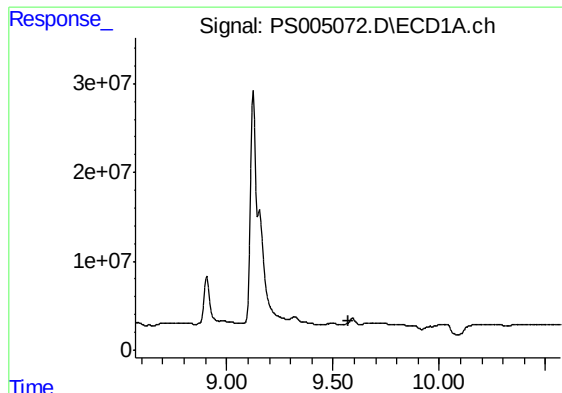

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

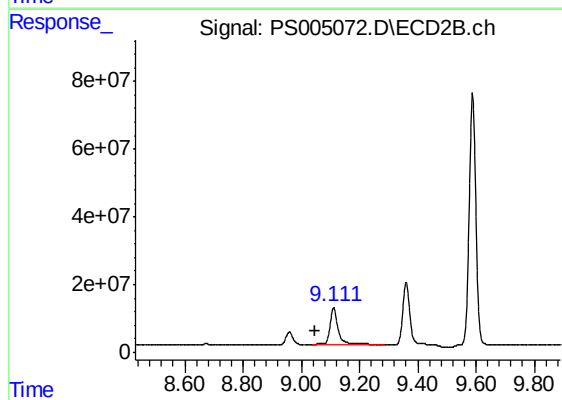

#16 DCPA

R.T.: 9.111 min
Delta R.T.: 0.061 min
Response: 215993543
Conc: 32.75 ng/ml