

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 10:49
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 13:29:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.574	5.290	532.7E6	372.5E6	404.249	373.417
Target Compounds							
9) T	2,4-D	6.661	0.000	41007328	0	30.391	N.D. #
12) T	2,4,5-T	0.000	7.397	0	44759030	N.D.	9.490
15) T	Picloram	9.146	9.103	208.4E6	149.5E6	20.994	21.918
16) T	DCPA	0.000	9.103	0	149.5E6	N.D.	22.671



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 10:49
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 13:29:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

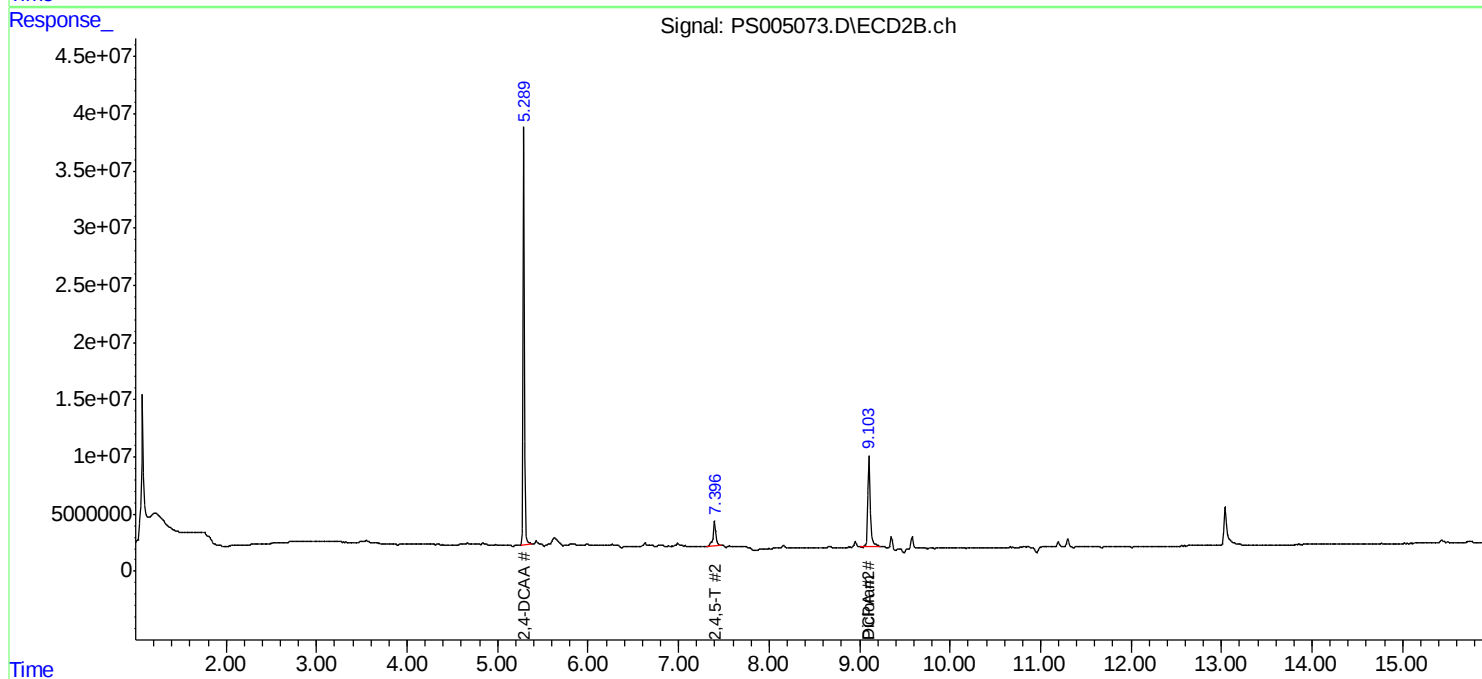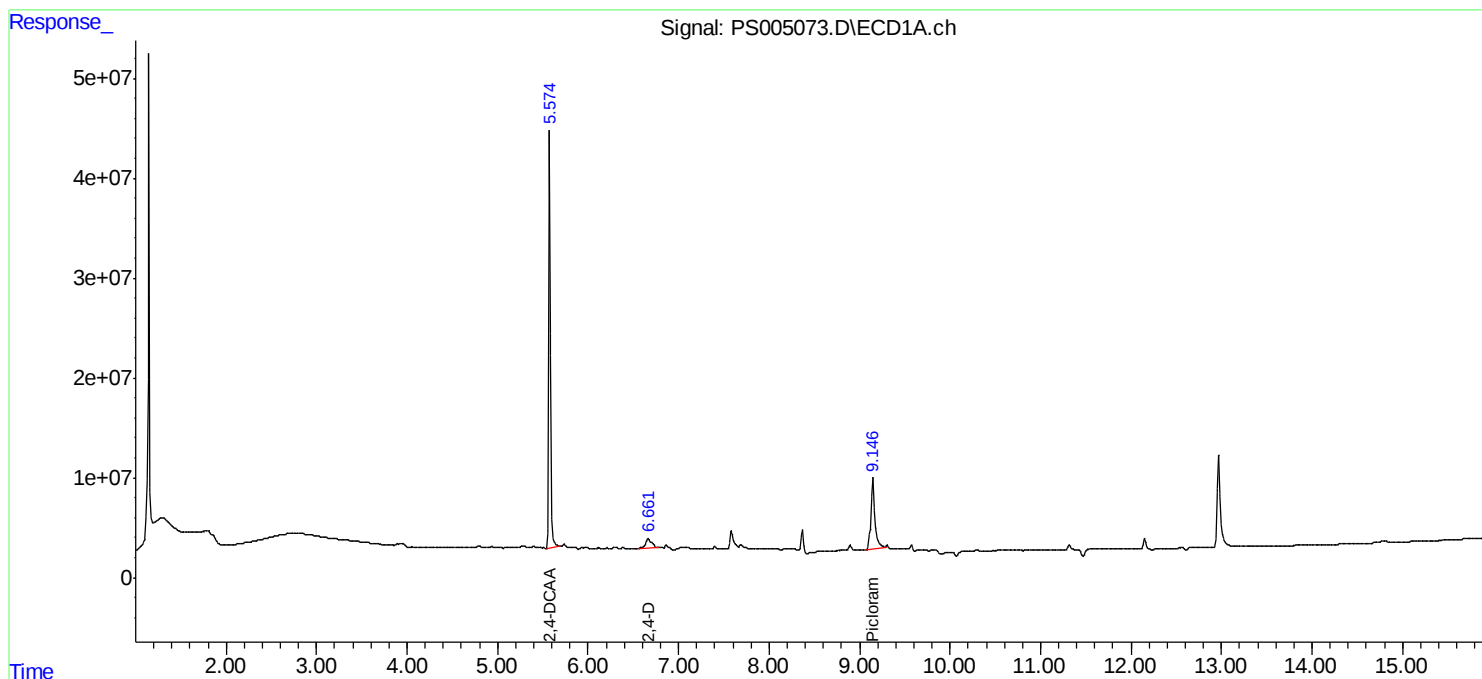


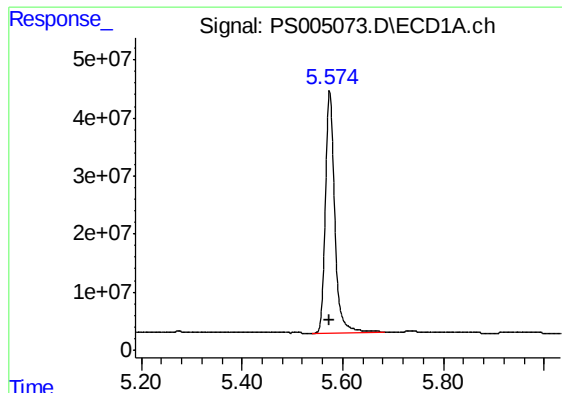

#4 2,4-DCAA


R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 532717085
Conc: 404.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

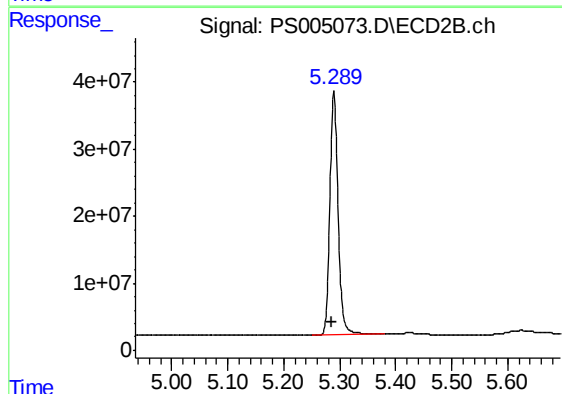


#4 2,4-DCAA

R.T.: 5.290 min
Delta R.T.: 0.005 min
Response: 372496801
Conc: 373.42 ng/ml

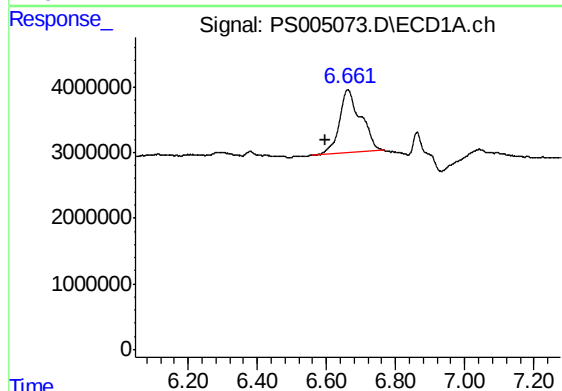


#9 2,4-D

R.T.: 6.661 min
Delta R.T.: 0.065 min
Response: 41007328
Conc: 30.39 ng/ml

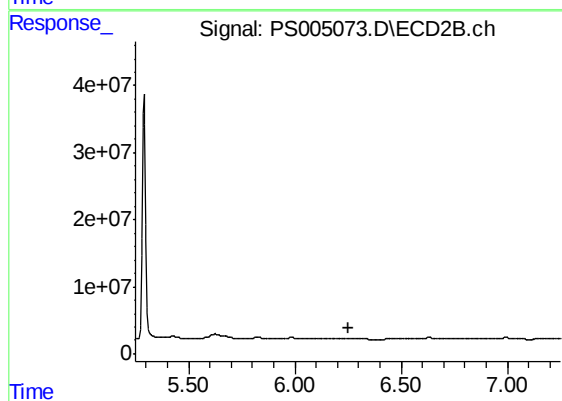

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

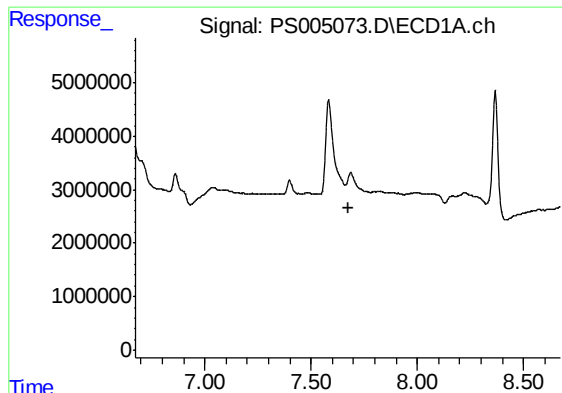

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

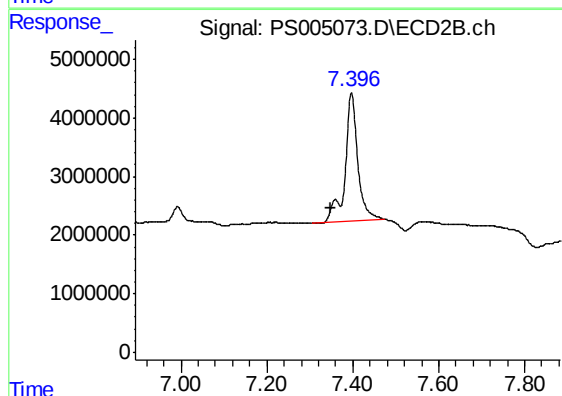


#12 2,4,5-T

R.T.: 7.397 min
Delta R.T.: 0.048 min
Response: 44759030
Conc: 9.49 ng/ml

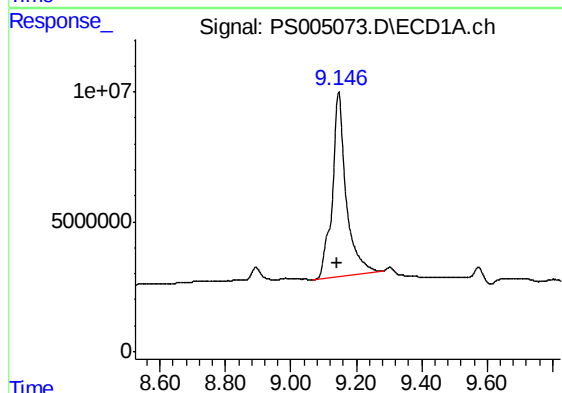


#15 Picloram

R.T.: 9.146 min
Delta R.T.: 0.007 min
Response: 208430122
Conc: 20.99 ng/ml

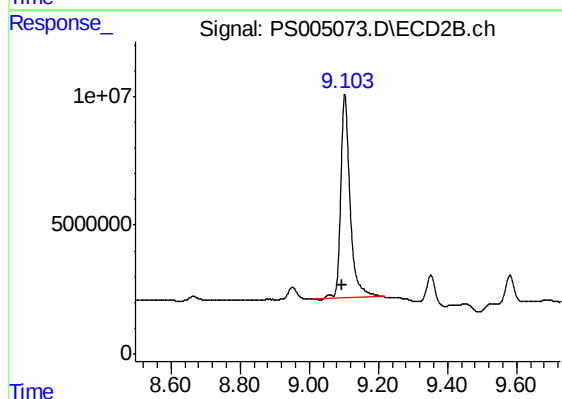

#15 Picloram


R.T.: 9.103 min
Delta R.T.: 0.008 min
Response: 149504492
Conc: 21.92 ng/ml

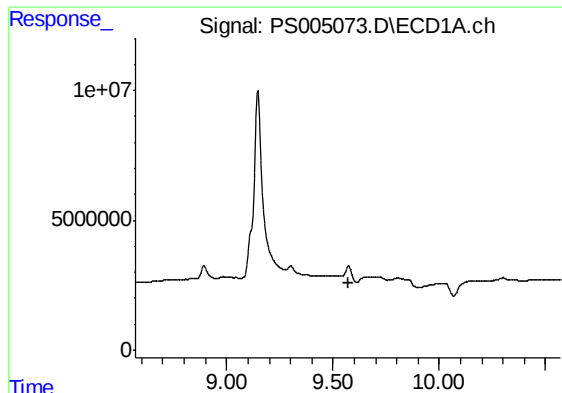

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

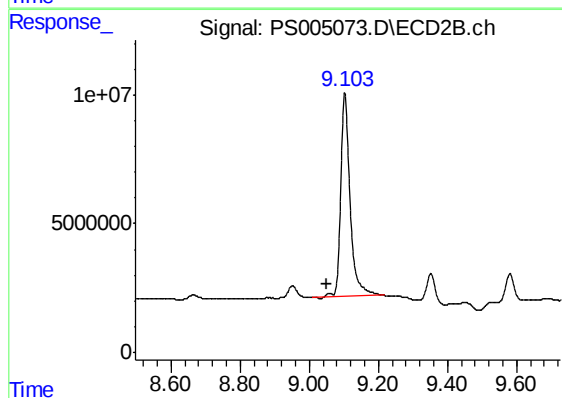

#16 DCPA

R.T.: 9.103 min
Delta R.T.: 0.053 min
Response: 149504492
Conc: 22.67 ng/ml