

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005080.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 14:33
 Operator : SM\AJ
 Sample : K3154-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 JC-02-061419-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 15:12:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.587	5.301	358.7E6	242.4E6	272.162	243.026
Target Compounds							
2) T	3,5-DICHL...	0.000	4.619	0	194.5E6	N.D.	151.964
3) T	4-Nitroph...	5.503	5.006	38955449	25367556	85.527	55.942 #
5) T	DICAMBA	5.778	5.406	16963517	19830110	2.997	5.163 #
7) T	MCPA	0.000	5.633	0	43933395	N.D.	10.422
10) T	Pentachlo...	0.000	6.567	0	28081822	N.D.	2.180
11) T	2,4,5-TP ...	0.000	6.954	0	41425445	N.D.	7.739
12) T	2,4,5-T	7.607	0.000	94829986	0	11.868	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005080.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 14:33
Operator : SM\AJ
Sample : K3154-04
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 15:12:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

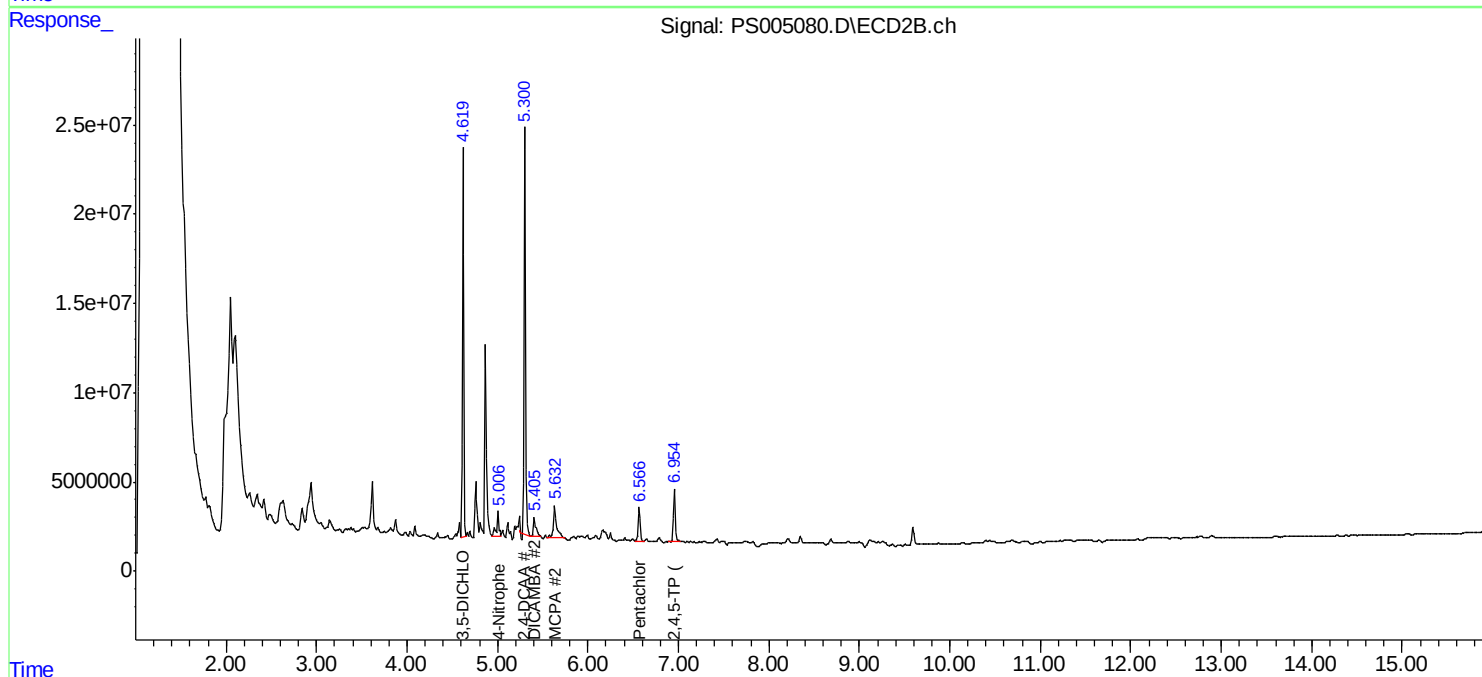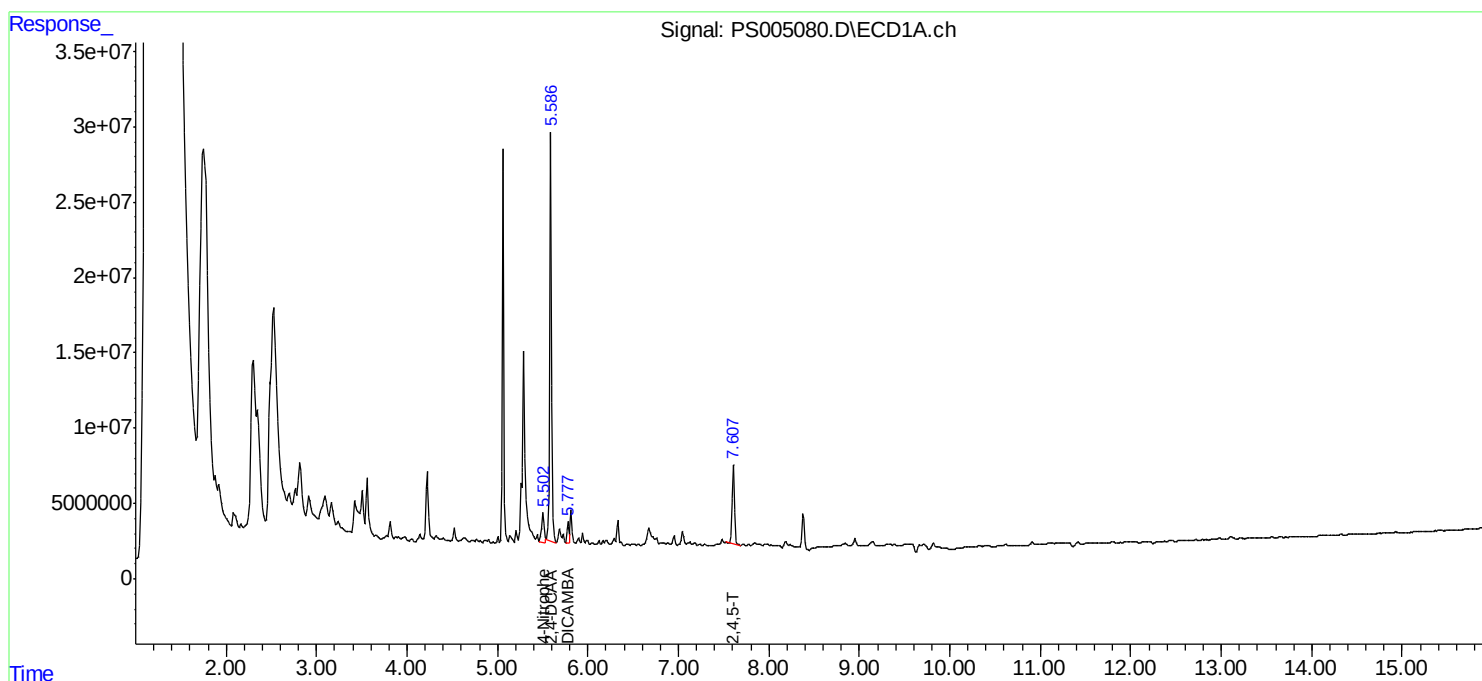


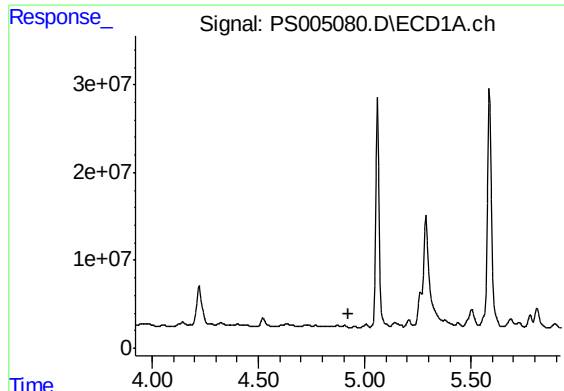

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.922 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-B

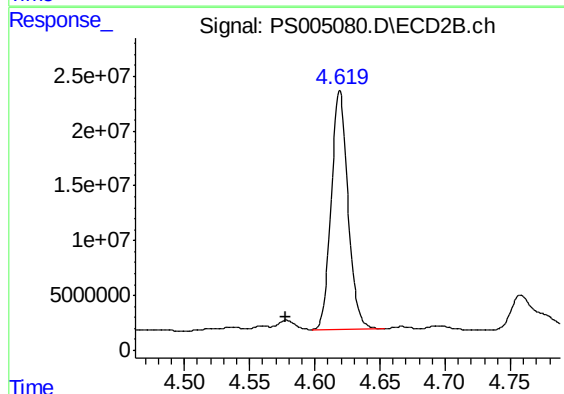


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.619 min
Delta R.T.: 0.041 min
Response: 194481561
Conc: 151.96 ng/ml

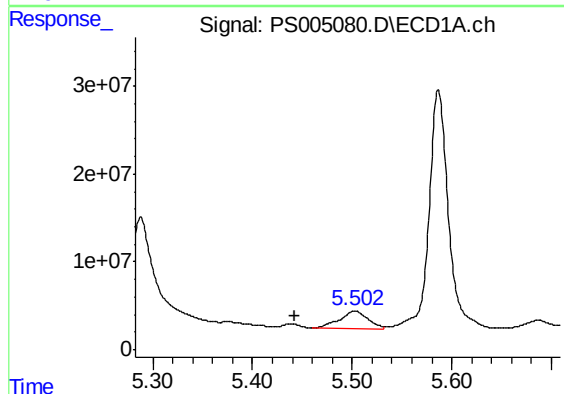


#3 4-Nitrophenol

R.T.: 5.503 min
Delta R.T.: 0.060 min
Response: 38955449
Conc: 85.53 ng/ml

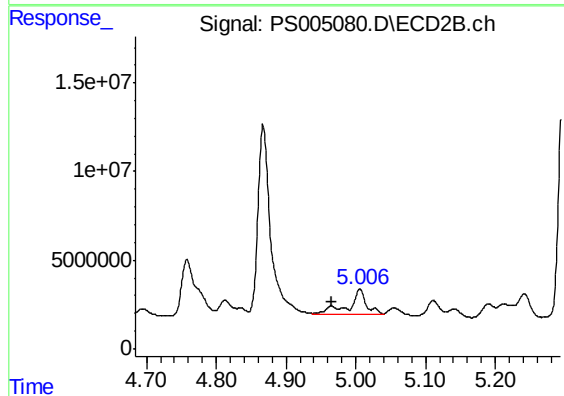

#3 4-Nitrophenol


R.T.: 5.006 min
Delta R.T.: 0.041 min
Response: 25367556
Conc: 55.94 ng/ml

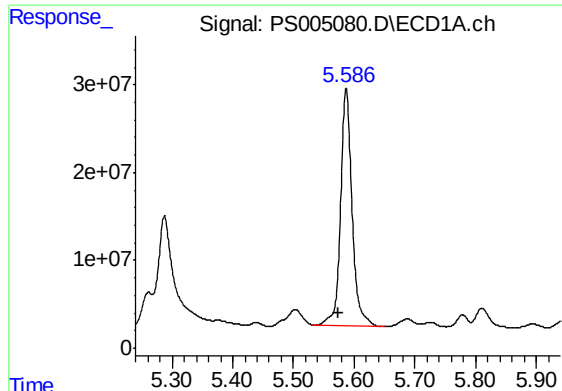

#4 2,4-DCAA


R.T.: 5.587 min
Delta R.T.: 0.013 min
Response: 358653962
Conc: 272.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-B

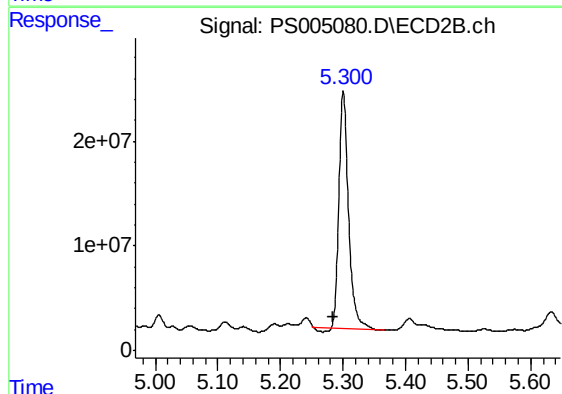


#4 2,4-DCAA

R.T.: 5.301 min
Delta R.T.: 0.016 min
Response: 242427231
Conc: 243.03 ng/ml

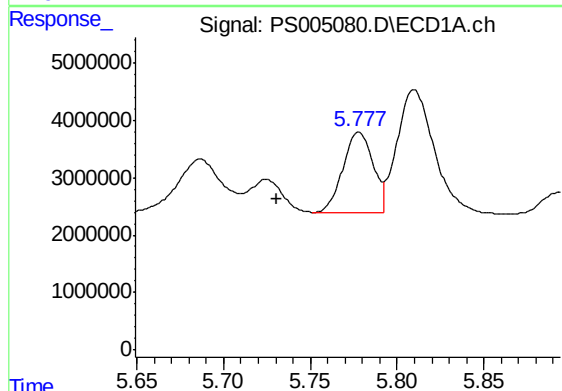


#5 DICAMBA

R.T.: 5.778 min
Delta R.T.: 0.047 min
Response: 16963517
Conc: 3.00 ng/ml

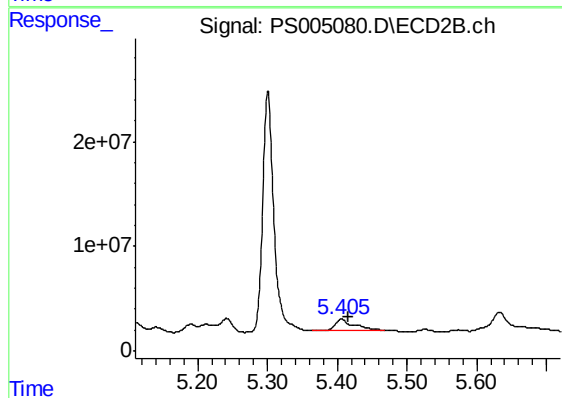

#5 DICAMBA


R.T.: 5.406 min
Delta R.T.: -0.010 min
Response: 19830110
Conc: 5.16 ng/ml

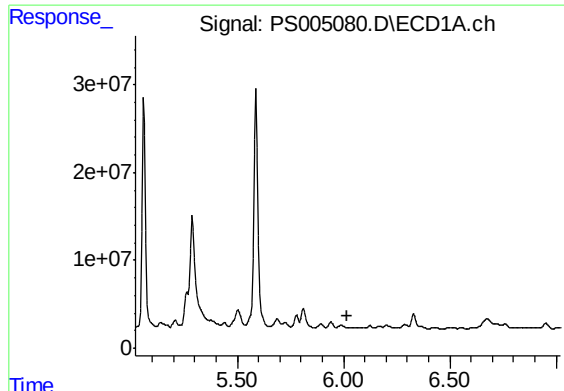

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-B

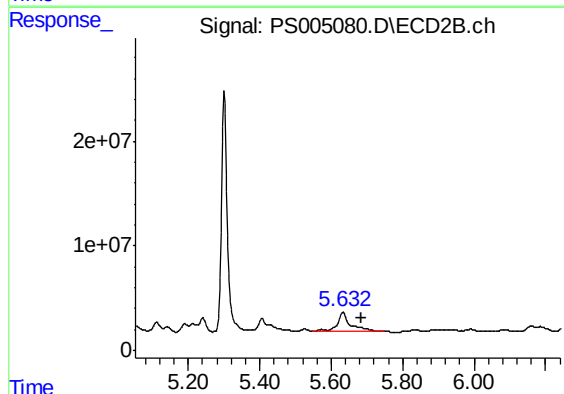


#7 MCPA

R.T.: 5.633 min
Delta R.T.: -0.051 min
Response: 43933395
Conc: 10.42 ug/ml

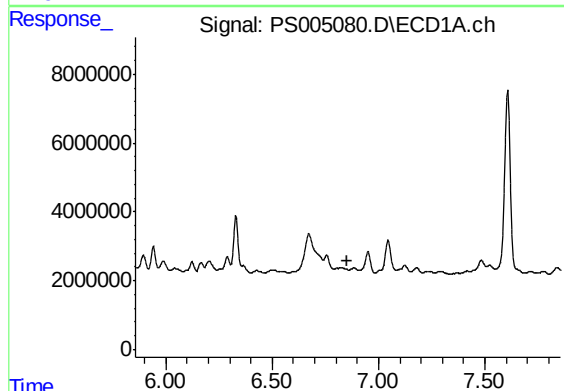


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.856 min
Response: 0
Conc: N.D.

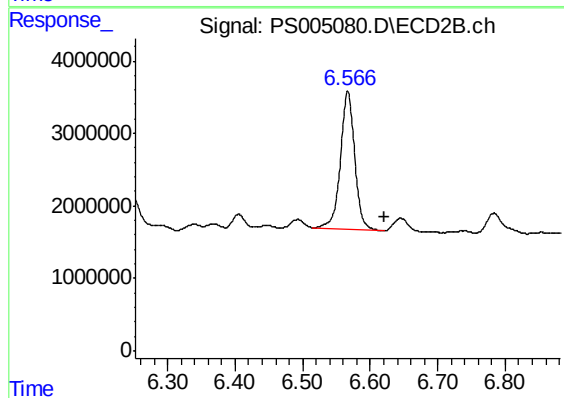

#10 Pentachlorophenol


R.T.: 6.567 min
Delta R.T.: -0.055 min
Response: 28081822
Conc: 2.18 ng/ml

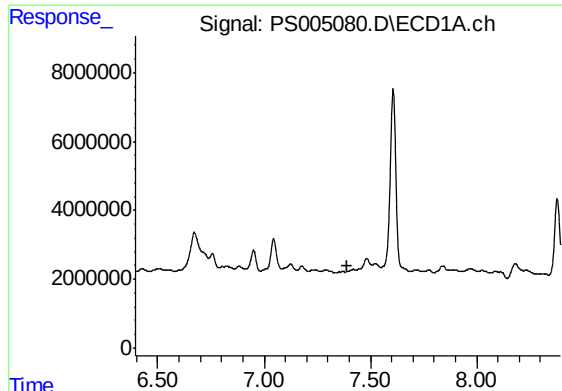

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-B

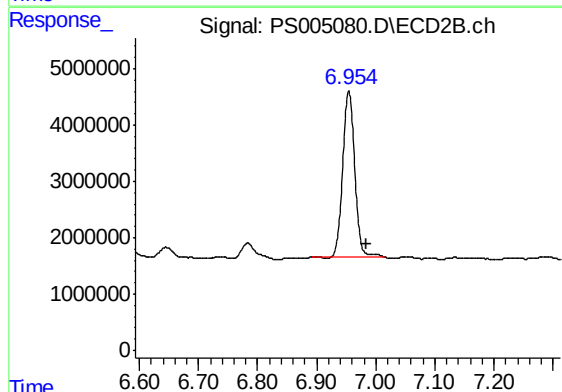


#11 2,4,5-TP (SILVEX)

R.T.: 6.954 min
Delta R.T.: -0.031 min
Response: 41425445
Conc: 7.74 ng/ml

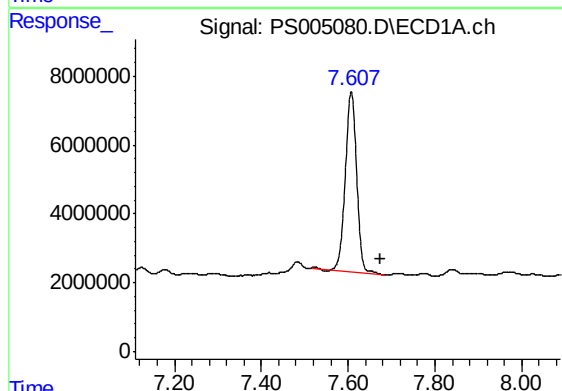

#12 2,4,5-T

R.T.: 7.607 min
Delta R.T.: -0.066 min
Response: 94829986
Conc: 11.87 ng/ml

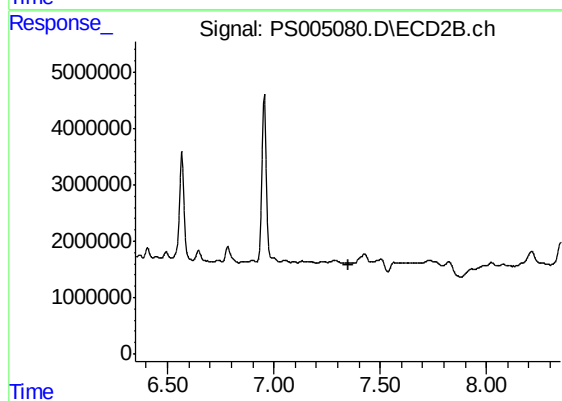

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.349 min
Response: 0
Conc: N.D.