

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005086.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 16:45
 Operator : SM\AJ
 Sample : K3154-10
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 JC-02-061419-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 17:52:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.586	5.300	385.7E6	269.6E6	292.680	270.299
Target Compounds							
1) T	Dalapon	2.083	0.000	30455302	0	17.484	N.D. #
2) T	3,5-DICHL...	0.000	4.619	0	162.9E6	N.D.	127.271
5) T	DICAMBA	0.000	5.406	0	5484530	N.D.	1.428
8) T	DICHLORPROP	0.000	5.991	0	19448004	N.D.	20.024
10) T	Pentachlo...	0.000	6.567	0	25539134	N.D.	1.982
11) T	2,4,5-TP ...	0.000	6.955	0	65194364	N.D.	12.180
12) T	2,4,5-T	7.605	7.407	97648249	21773532	12.221	4.616 #
15) T	Picloram	9.159	9.115	89464944	67913619	9.011	9.956
16) T	DCPA	0.000	9.115	0	67913619	N.D.	10.299



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005086.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 16:45
Operator : SM\AJ
Sample : K3154-10
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
JC-02-061419-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 17:52:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

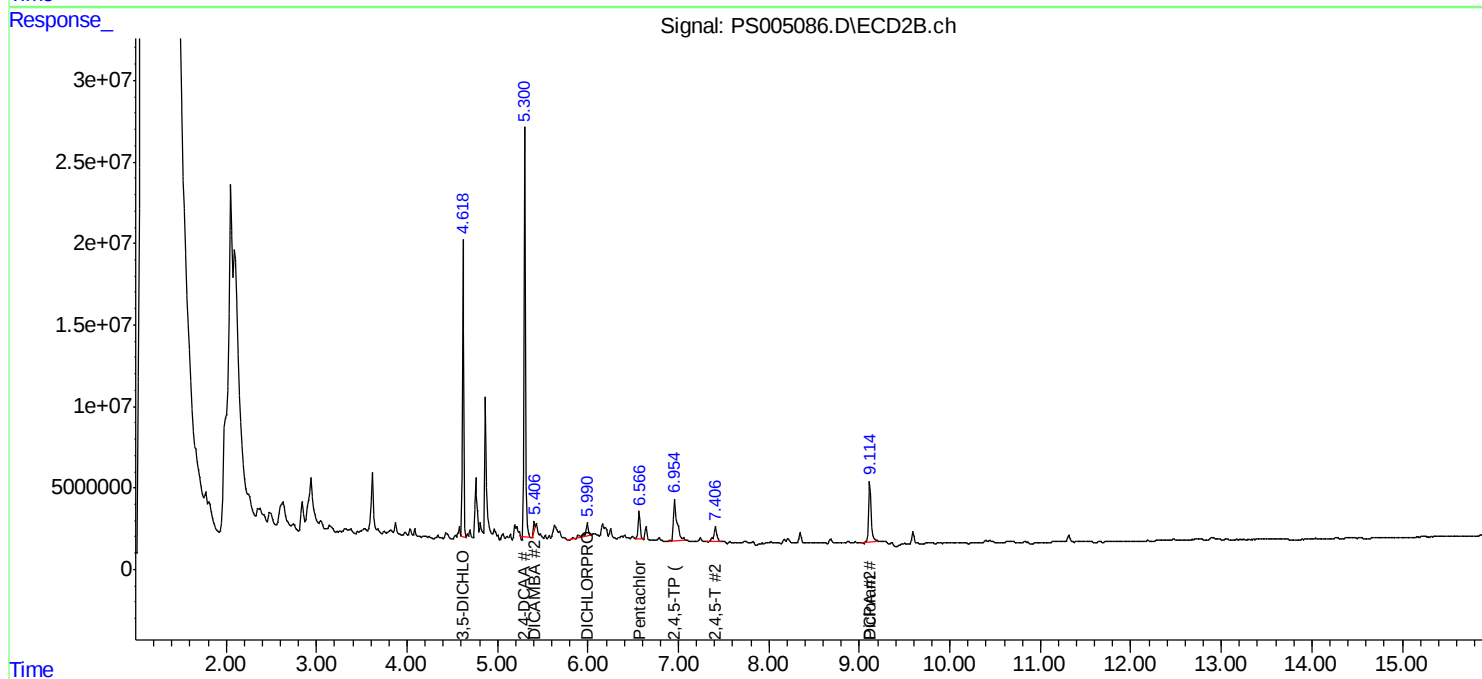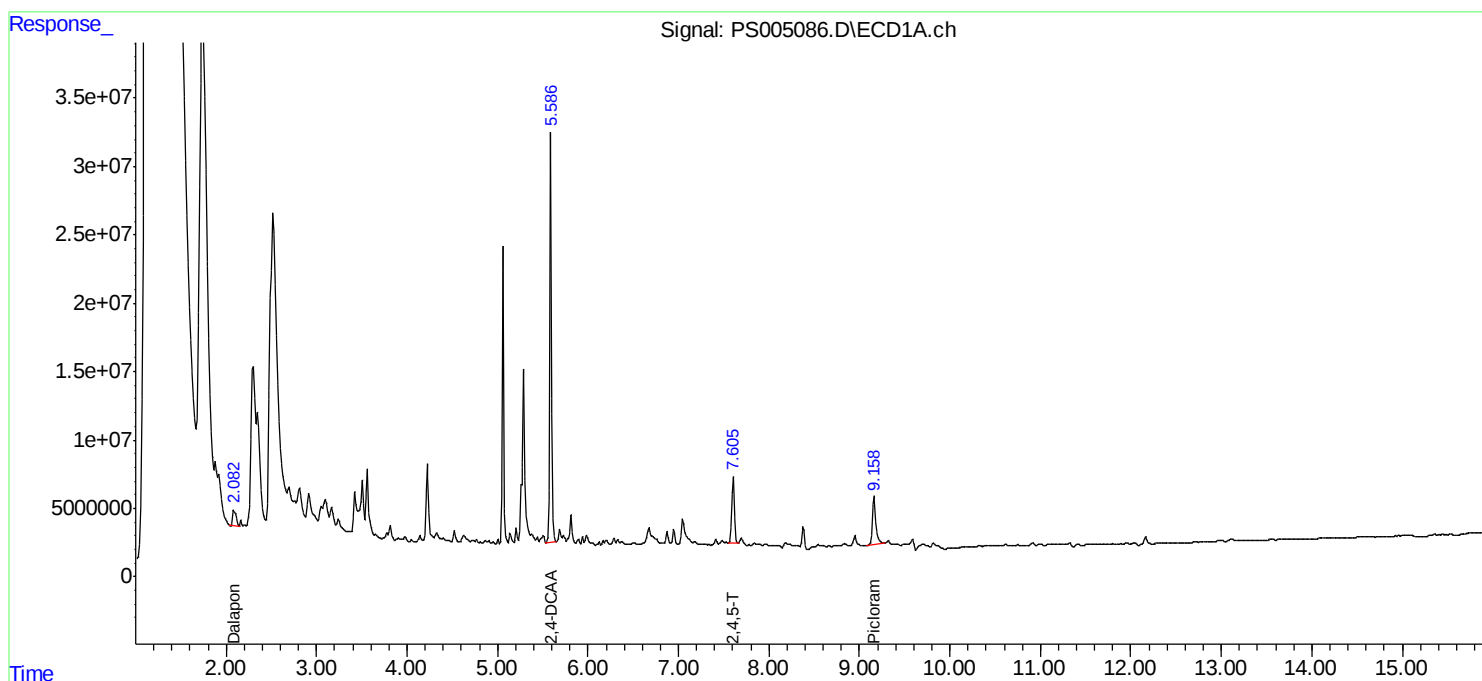


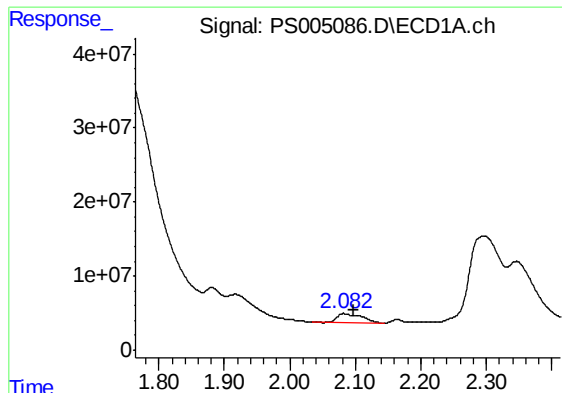

#1 Dalapon


R.T.: 2.083 min
Delta R.T.: -0.014 min
Response: 30455302
Conc: 17.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-E

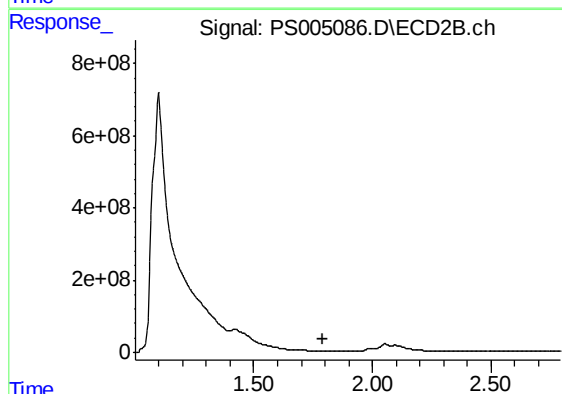


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.794 min
Response: 0
Conc: N.D.

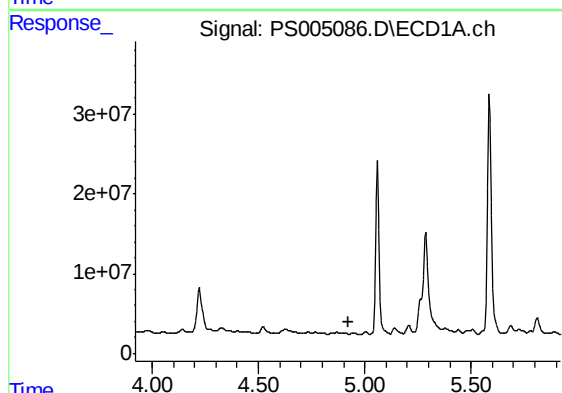


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

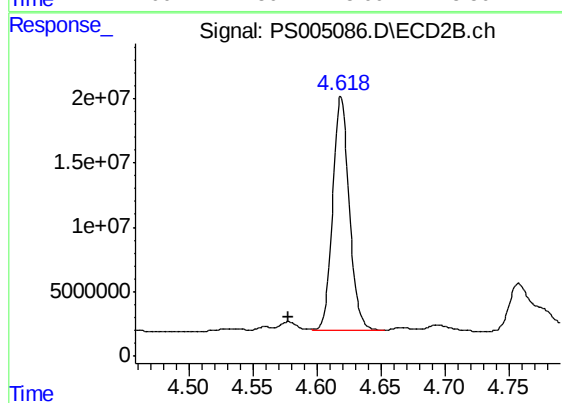

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.619 min
Delta R.T.: 0.041 min
Response: 162880145
Conc: 127.27 ng/ml

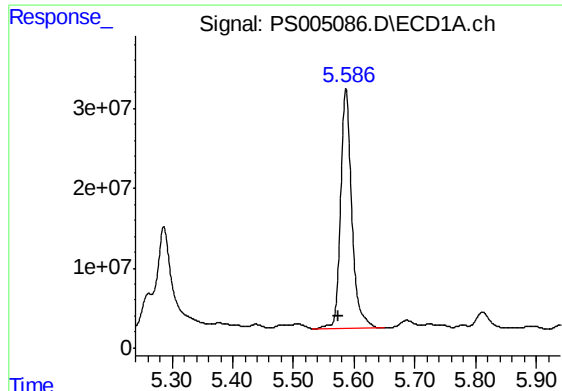

#4 2,4-DCAA


R.T.: 5.586 min
Delta R.T.: 0.013 min
Response: 385691798
Conc: 292.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-E

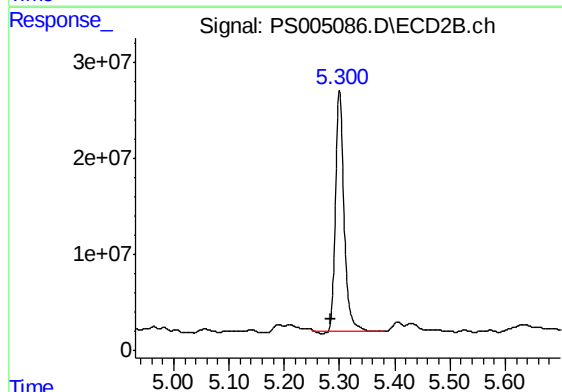


#4 2,4-DCAA

R.T.: 5.300 min
Delta R.T.: 0.015 min
Response: 269632877
Conc: 270.30 ng/ml

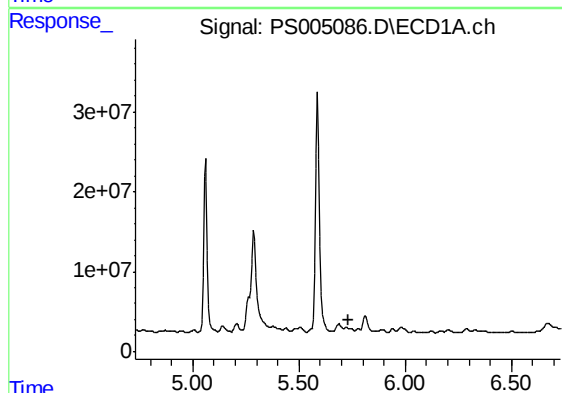


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.731 min
Response: 0
Conc: N.D.

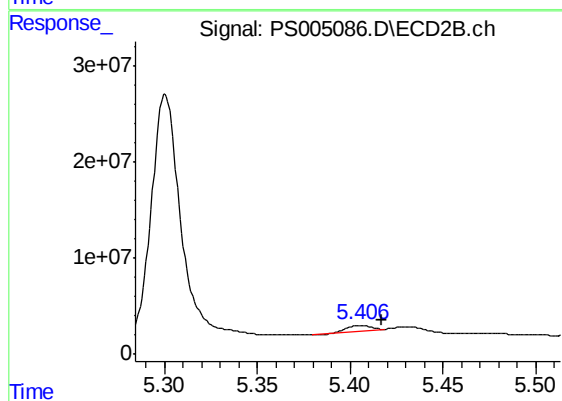

#5 DICAMBA


R.T.: 5.406 min
Delta R.T.: -0.011 min
Response: 5484530
Conc: 1.43 ng/ml

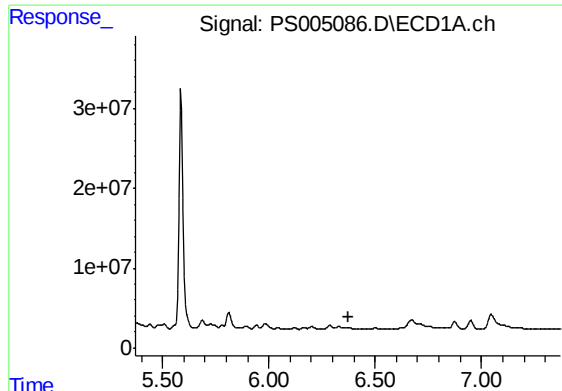

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-E

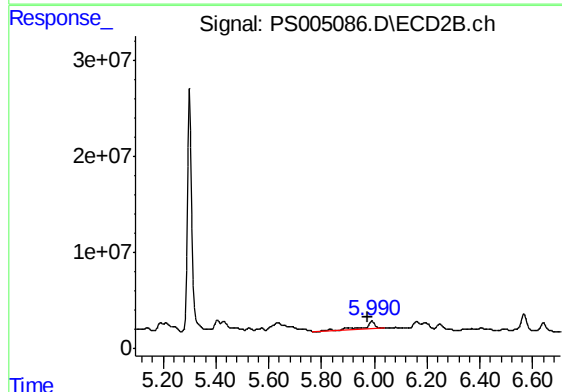


#8 DICHLORPROP

R.T.: 5.991 min
Delta R.T.: 0.017 min
Response: 19448004
Conc: 20.02 ng/ml

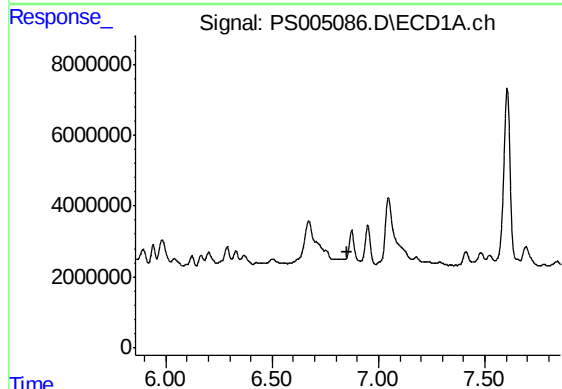


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.856 min
Response: 0
Conc: N.D.

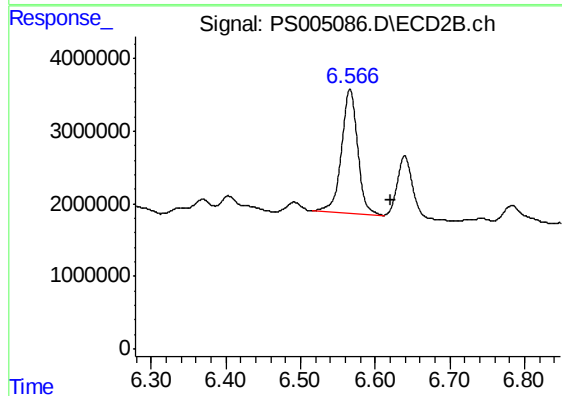

#10 Pentachlorophenol


R.T.: 6.567 min
Delta R.T.: -0.055 min
Response: 25539134
Conc: 1.98 ng/ml

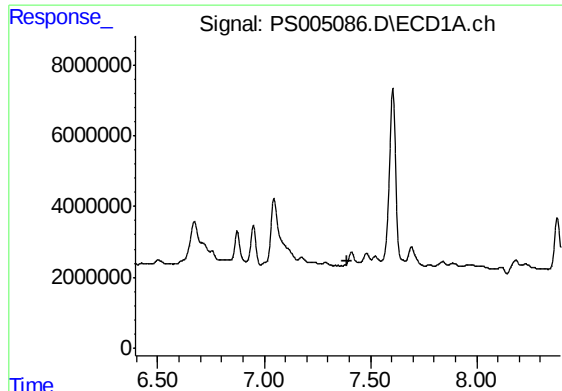

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-E

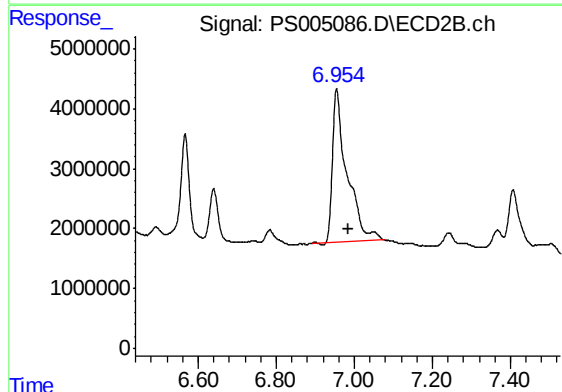


#11 2,4,5-TP (SILVEX)

R.T.: 6.955 min
Delta R.T.: -0.030 min
Response: 65194364
Conc: 12.18 ng/ml

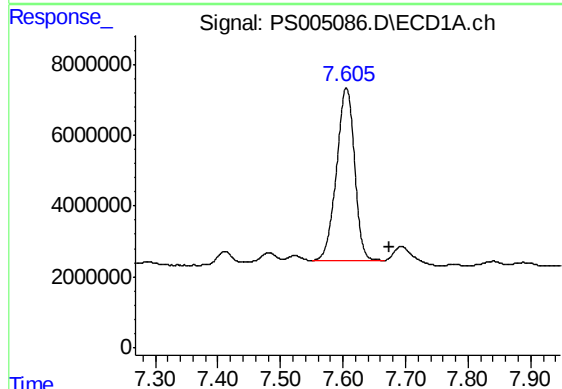


#12 2,4,5-T

R.T.: 7.605 min
Delta R.T.: -0.068 min
Response: 97648249
Conc: 12.22 ng/ml

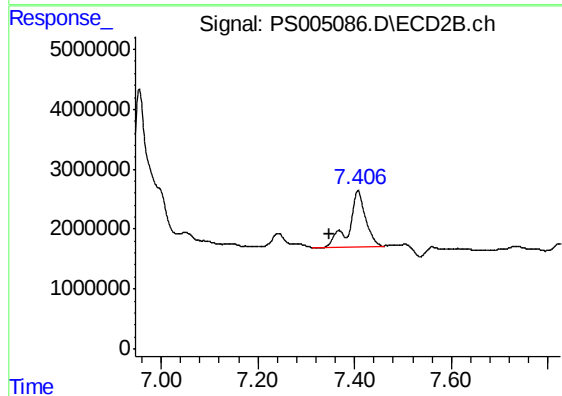

#12 2,4,5-T


R.T.: 7.407 min
Delta R.T.: 0.058 min
Response: 21773532
Conc: 4.62 ng/ml

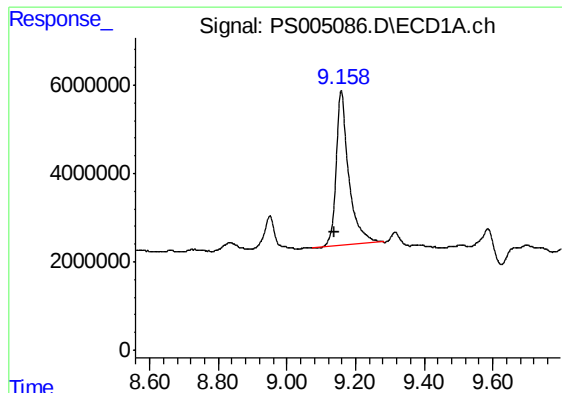

#15 Picloram


R.T.: 9.159 min
Delta R.T.: 0.019 min
Response: 89464944
Conc: 9.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-02-061419-E

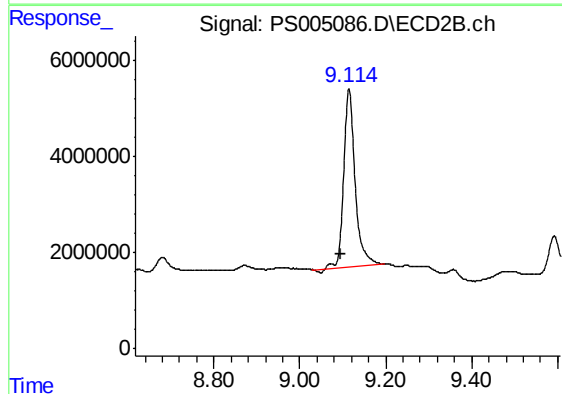


#15 Picloram

R.T.: 9.115 min
Delta R.T.: 0.019 min
Response: 67913619
Conc: 9.96 ng/ml

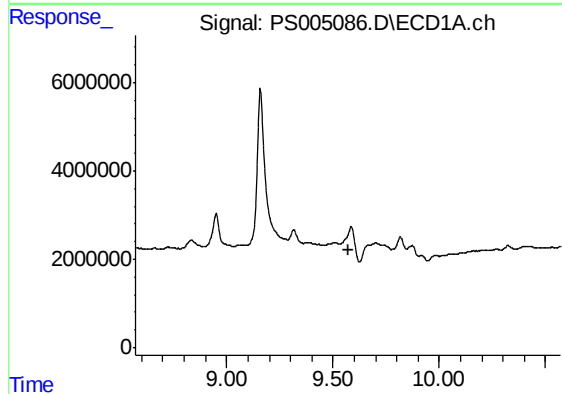

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.571 min
Response: 0
Conc: N.D.

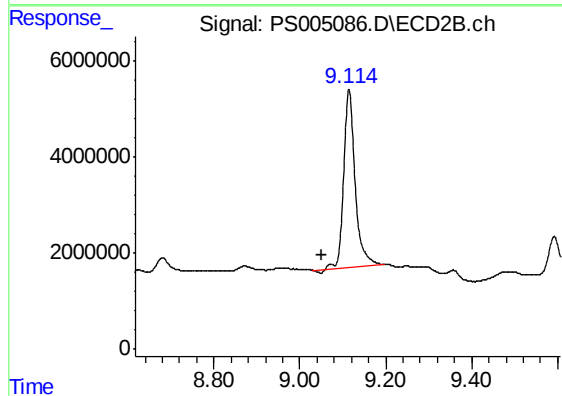

#16 DCPA

R.T.: 9.115 min
Delta R.T.: 0.065 min
Response: 67913619
Conc: 10.30 ng/ml