

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 18:35
 Operator : SM\AJ
 Sample : PB120671BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB120671BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 00:51:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.286	748.5E6	528.5E6	567.971	529.789
Target Compounds							
1) T	Dalapon	2.067	0.000	40640869	0	23.331	N.D. #
2) T	3,5-DICHL...	0.000	4.604	0	115.7E6	N.D.	90.434
3) T	4-Nitroph...	5.377	0.000	19381245	0	42.551	N.D. #
5) T	DICAMBA	5.671	0.000	8518774	0	1.505	N.D. #
6) T	MCPD	5.883	0.000	18932693	0	4.245	N.D. #
7) T	MCPA	5.977	5.677	14359977	20926262	2.291	4.964 #
9) T	2,4-D	6.656	6.233	32288382	22707521	23.929	21.219
10) T	Pentachlo...	0.000	6.553	0	26405393	N.D.	2.049



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 18:35
Operator : SM\AJ
Sample : PB120671BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB120671BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 00:51:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

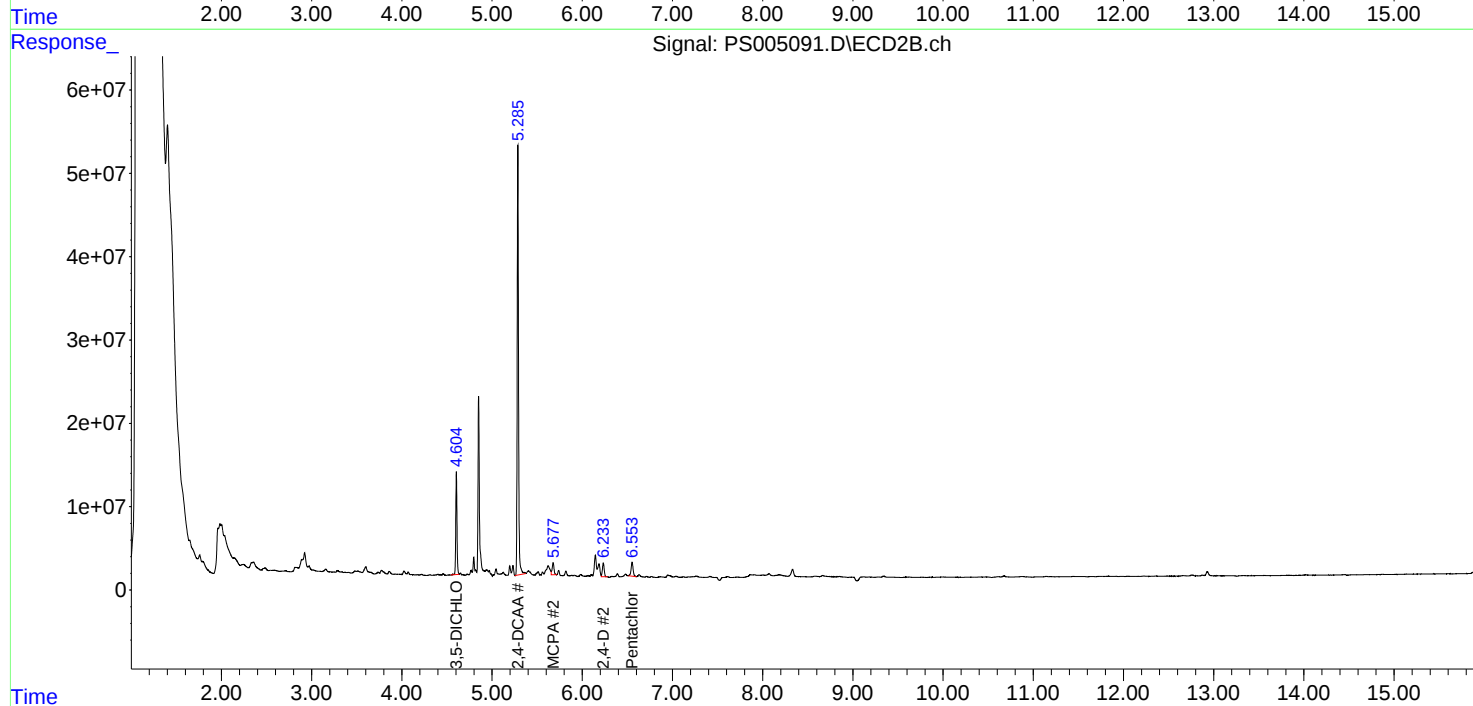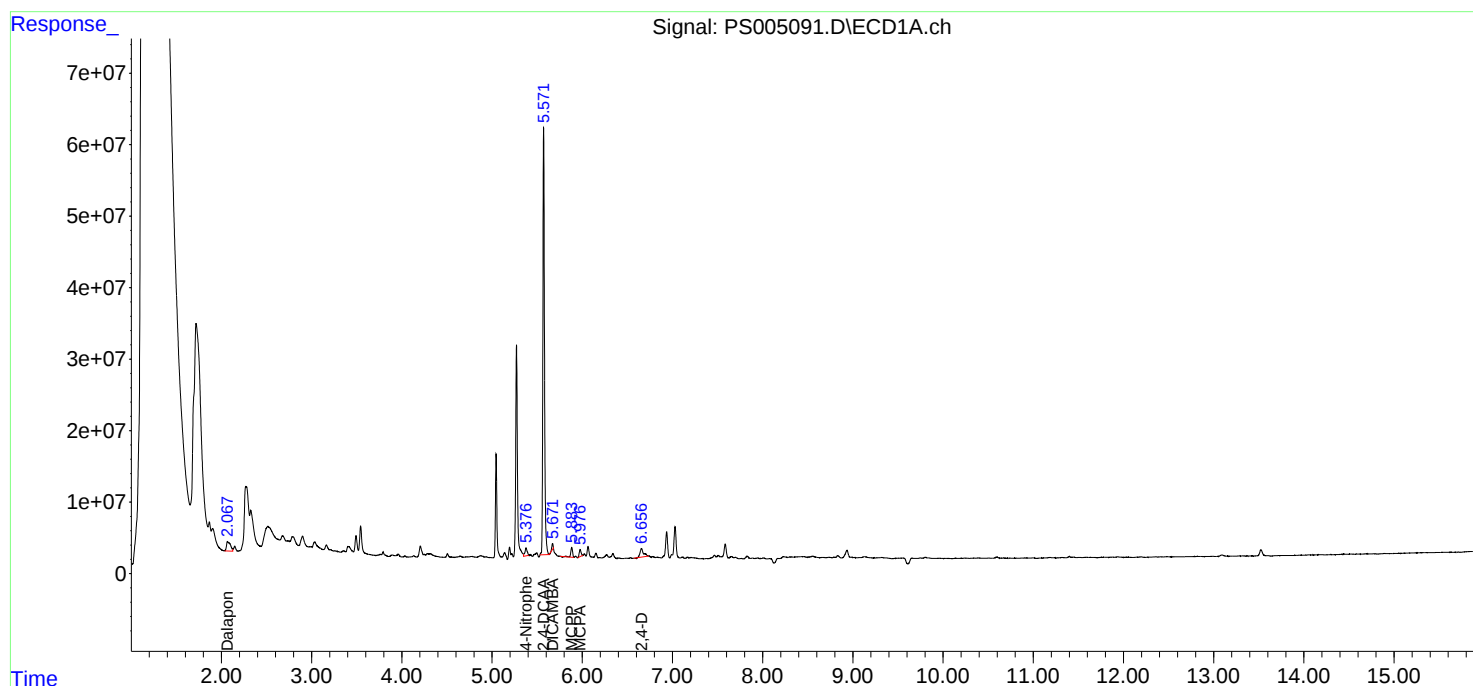


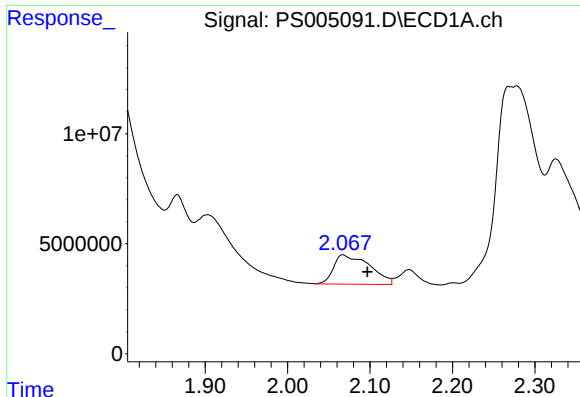

#1 Dalapon


R.T.: 2.067 min
Delta R.T.: -0.030 min
Response: 40640869
Conc: 23.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB120671BL

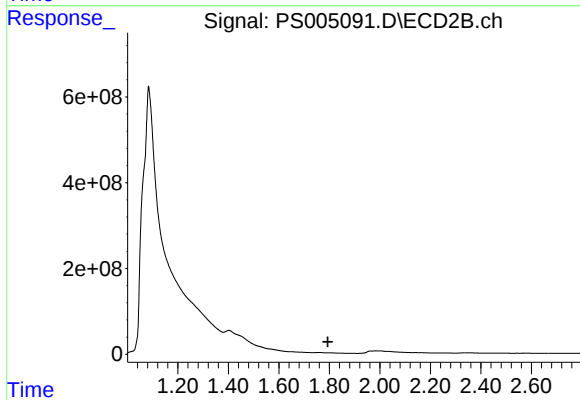


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.794 min
Response: 0
Conc: N.D.

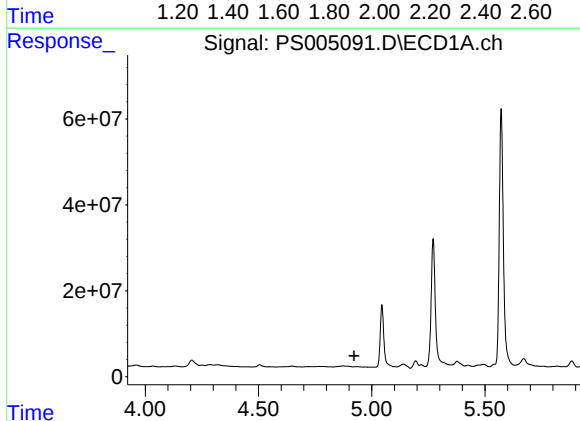


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

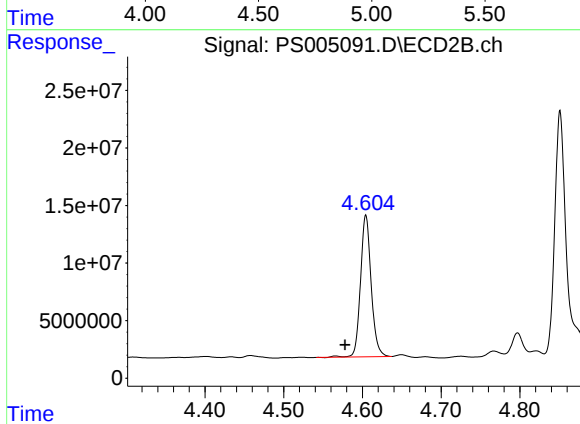

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.604 min
Delta R.T.: 0.027 min
Response: 115736925
Conc: 90.43 ng/ml

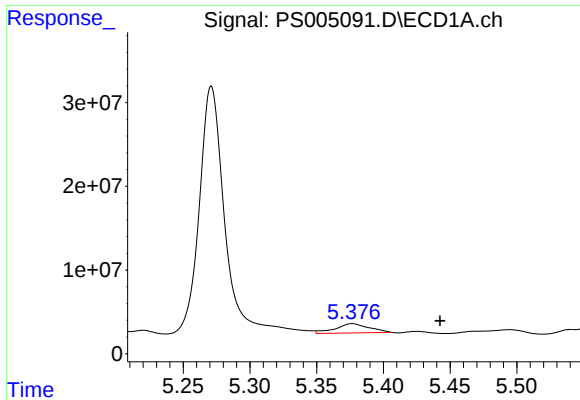

#3 4-Nitrophenol


R.T.: 5.377 min
Delta R.T.: -0.066 min
Response: 19381245
Conc: 42.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB120671BL

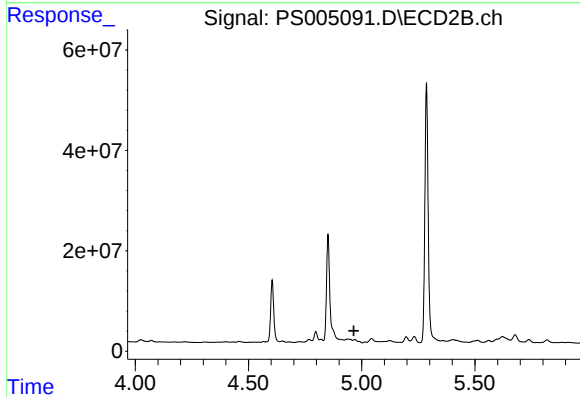


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

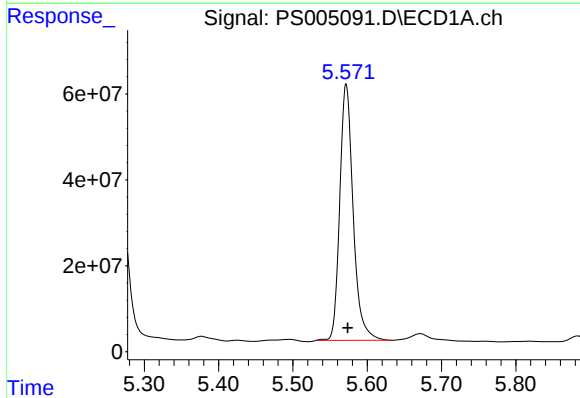


#4 2,4-DCAA

R.T.: 5.572 min
Delta R.T.: -0.002 min
Response: 748469687
Conc: 567.97 ng/ml

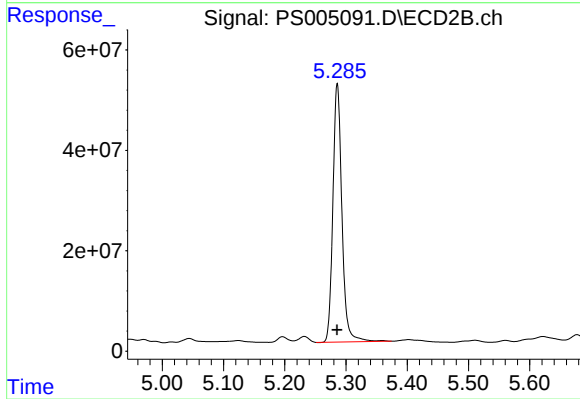

#4 2,4-DCAA


R.T.: 5.286 min
Delta R.T.: 0.000 min
Response: 528483887
Conc: 529.79 ng/ml

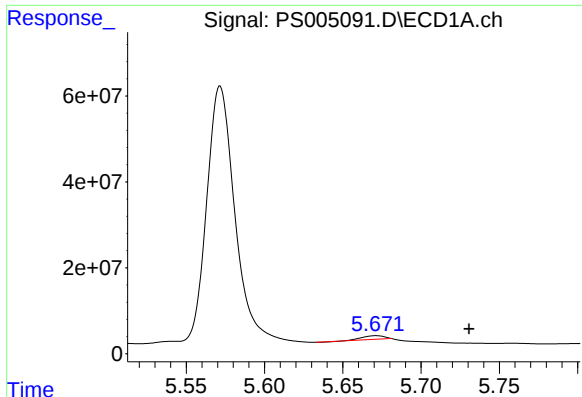

#5 DICAMBA


R.T.: 5.671 min
Delta R.T.: -0.060 min
Response: 8518774
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB120671BL

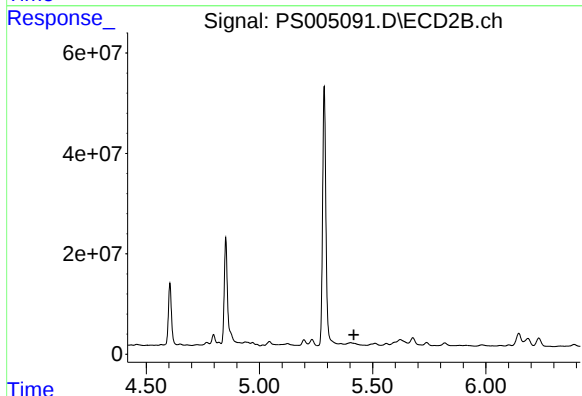


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.417 min
Response: 0
Conc: N.D.

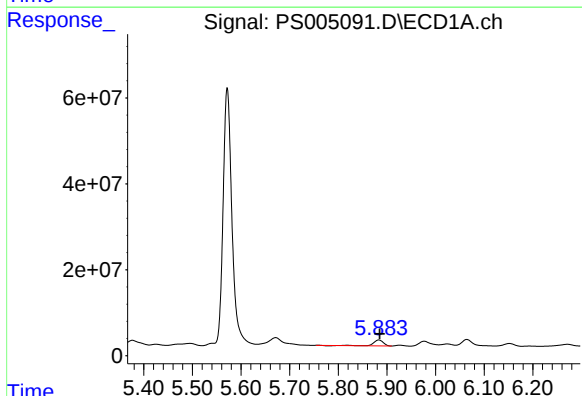


#6 MCP

R.T.: 5.883 min
Delta R.T.: -0.002 min
Response: 18932693
Conc: 4.24 ug/ml

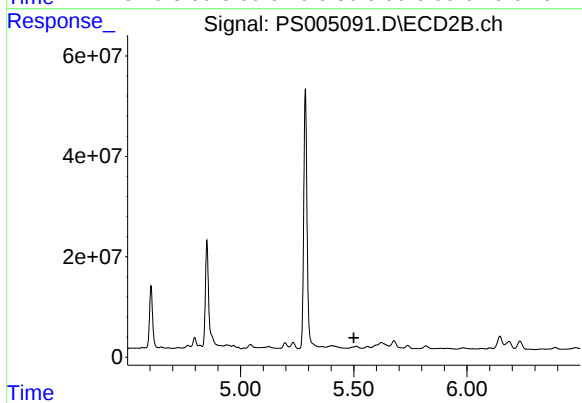

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.500 min
Response: 0
Conc: N.D.

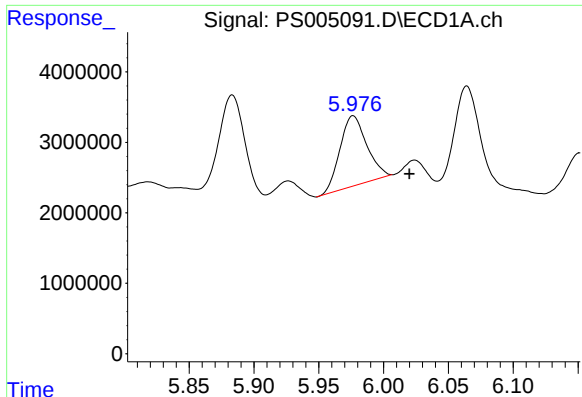

#7 MCPA


R.T.: 5.977 min
Delta R.T.: -0.043 min
Response: 14359977
Conc: 2.29 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB120671BL

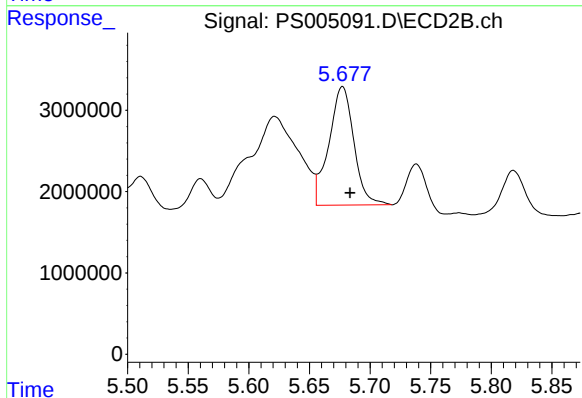


#7 MCPA

R.T.: 5.677 min
Delta R.T.: -0.006 min
Response: 20926262
Conc: 4.96 ug/ml

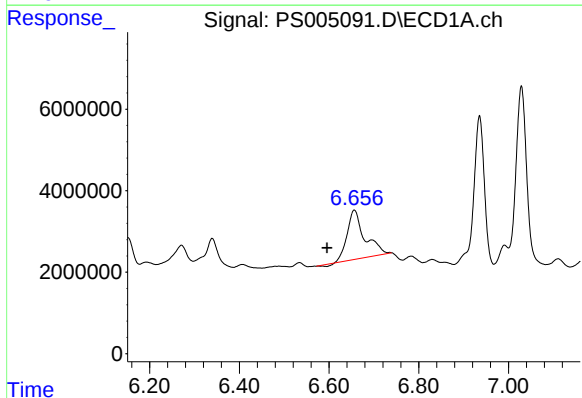


#9 2,4-D

R.T.: 6.656 min
Delta R.T.: 0.061 min
Response: 32288382
Conc: 23.93 ng/ml

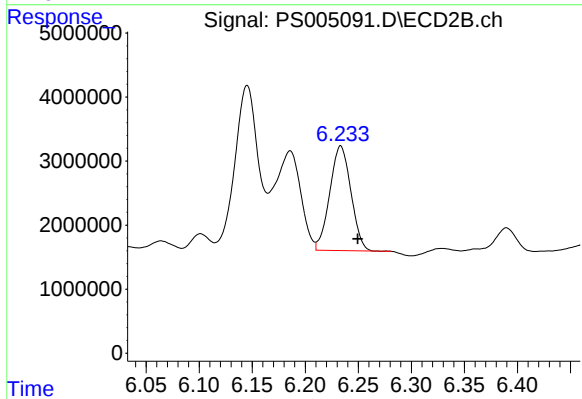

#9 2,4-D


R.T.: 6.233 min
Delta R.T.: -0.016 min
Response: 22707521
Conc: 21.22 ng/ml

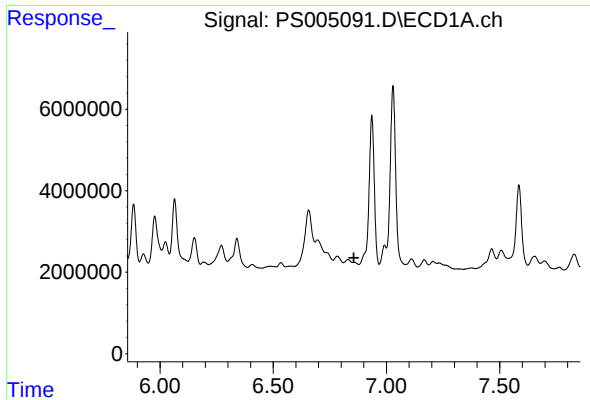

#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.856 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB120671BL

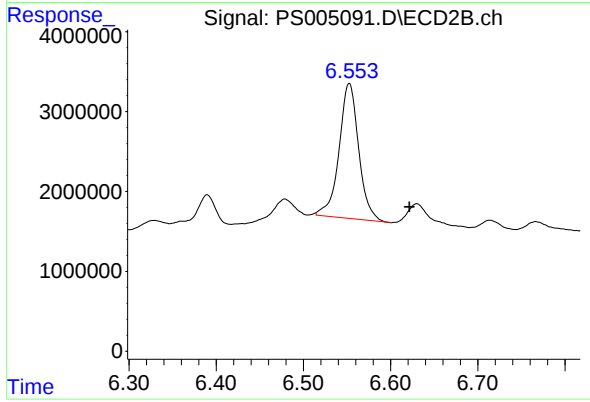

#10 Pentachlorophenol

R.T.: 6.553 min
Delta R.T.: -0.069 min
Response: 26405393
Conc: 2.05 ng/ml