

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 21:31
 Operator : SM\AJ
 Sample : K3157-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-061719-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 00:54:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.574	5.289	353.3E6	254.0E6	268.121	254.597
Target Compounds							
1) T	Dalapon	2.071	0.000	34329127	0	19.708	N.D. #
2) T	3,5-DICHL...	0.000	4.607	0	163.0E6	N.D.	127.397
5) T	DICAMBA	5.799	5.393	23928284	26318908	4.228	6.853 #
7) T	MCPA	0.000	5.622	0	33146885	N.D.	7.863
8) T	DICHLORPROP	0.000	5.979	0	35456932	N.D.	36.508
9) T	2,4-D	6.660	0.000	47340506	0	35.084	N.D. #
10) T	Pentachlo...	0.000	6.555	0	25481499	N.D.	1.978
11) T	2,4,5-TP ...	0.000	6.943	0	38199801	N.D.	7.137
12) T	2,4,5-T	0.000	7.414	0	16759090	N.D.	3.553



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 21:31
Operator : SM\AJ
Sample : K3157-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 00:54:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

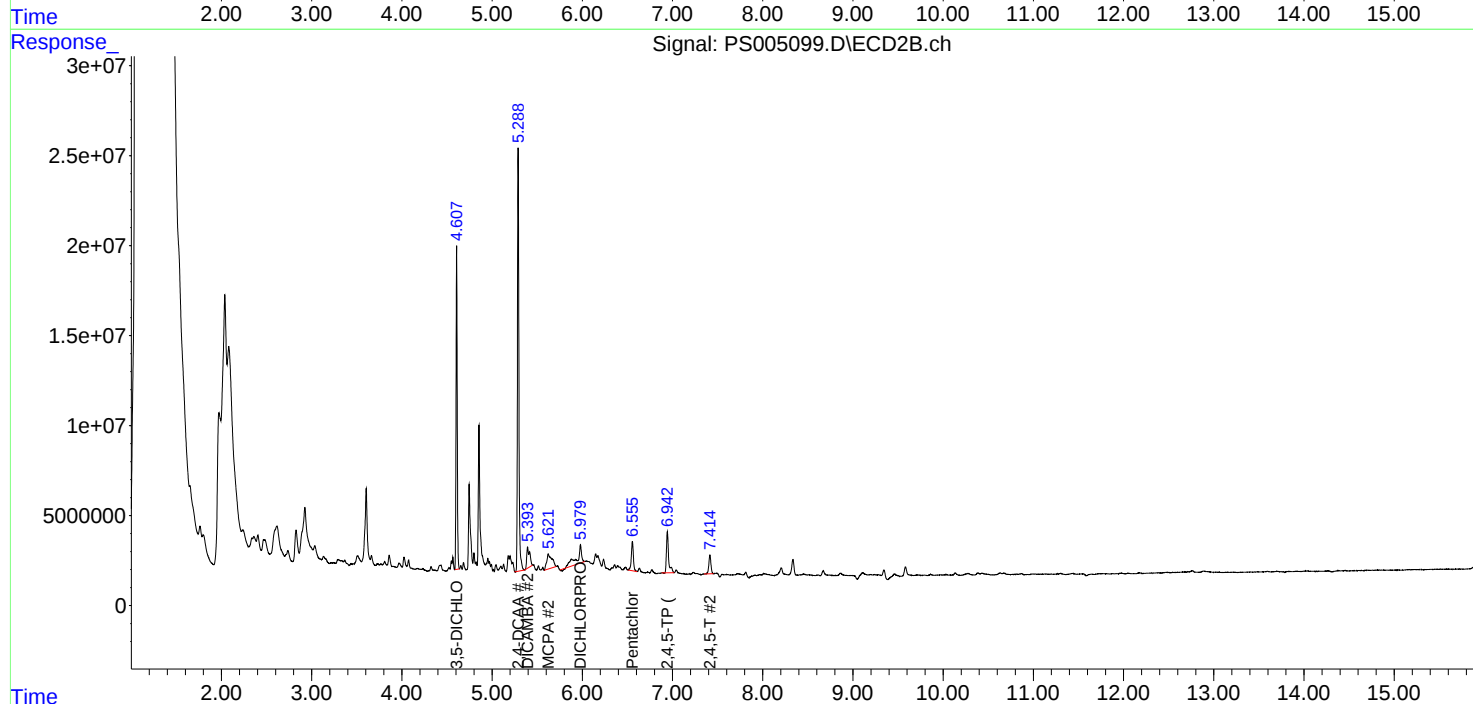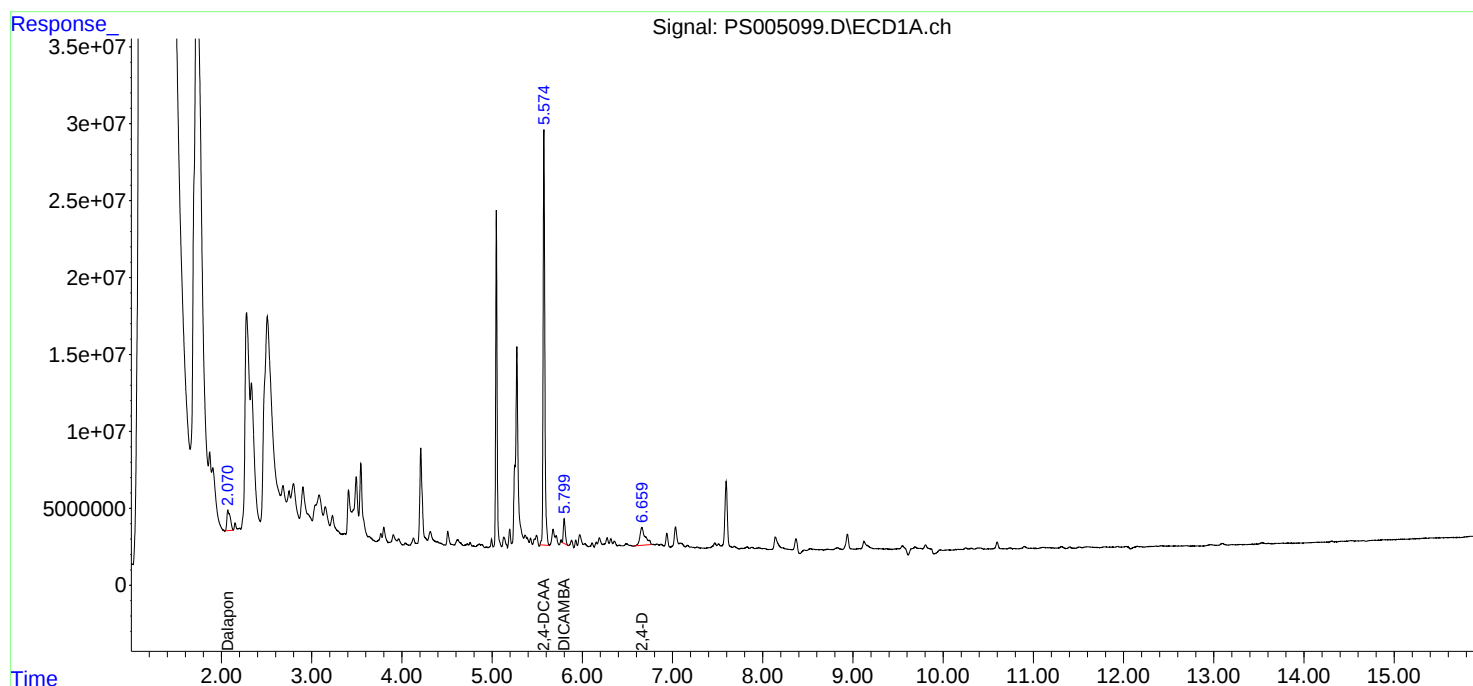


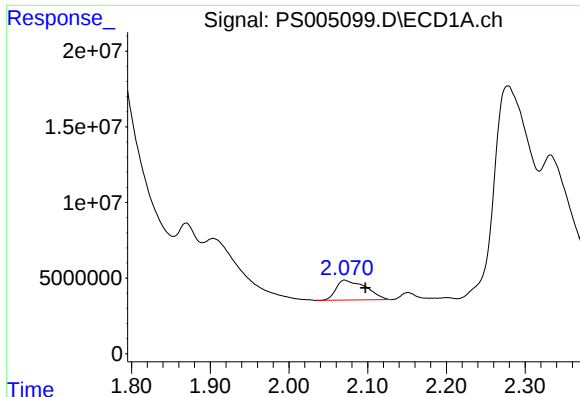

#1 Dalapon


R.T.: 2.071 min
Delta R.T.: -0.026 min
Response: 34329127
Conc: 19.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-A

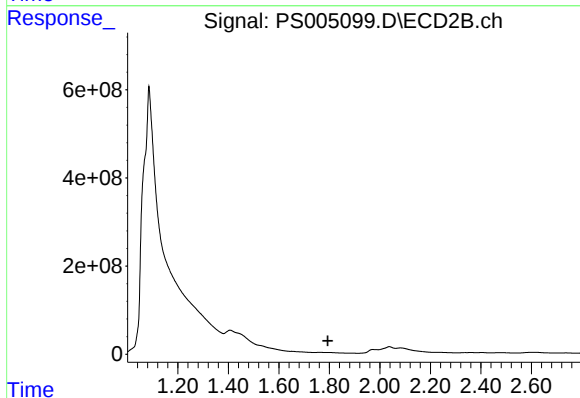


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.794 min
Response: 0
Conc: N.D.

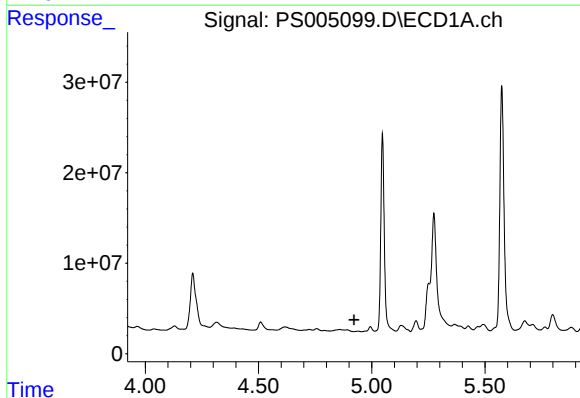


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

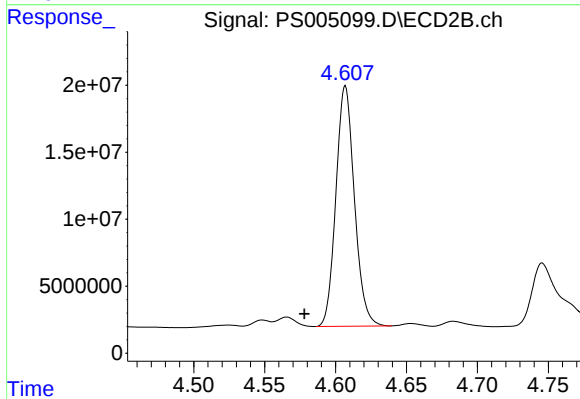

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.607 min
Delta R.T.: 0.029 min
Response: 163041298
Conc: 127.40 ng/ml

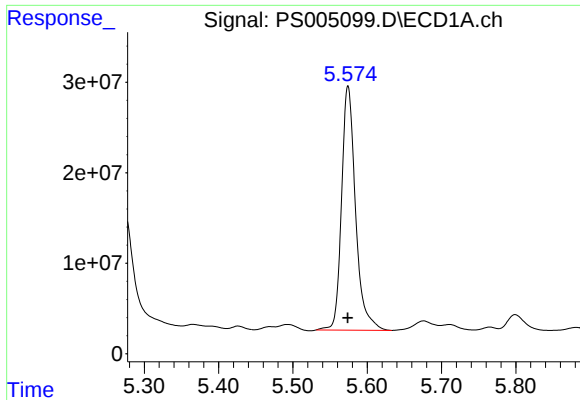

#4 2,4-DCAA


R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 353328553
Conc: 268.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-A

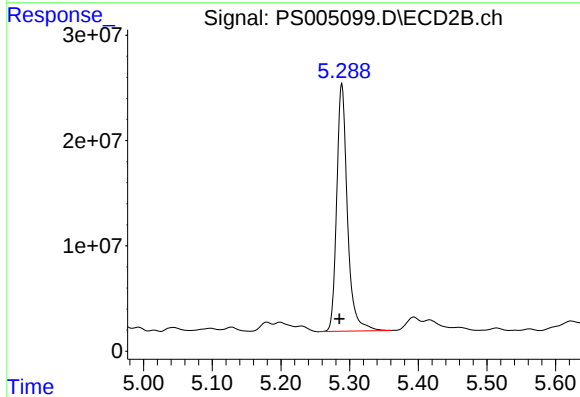


#4 2,4-DCAA

R.T.: 5.289 min
Delta R.T.: 0.004 min
Response: 253969284
Conc: 254.60 ng/ml

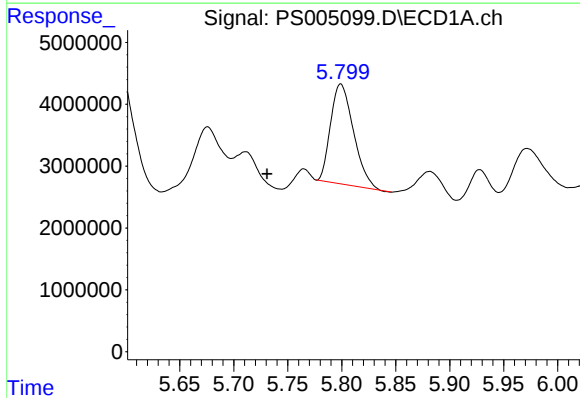


#5 DICAMBA

R.T.: 5.799 min
Delta R.T.: 0.068 min
Response: 23928284
Conc: 4.23 ng/ml

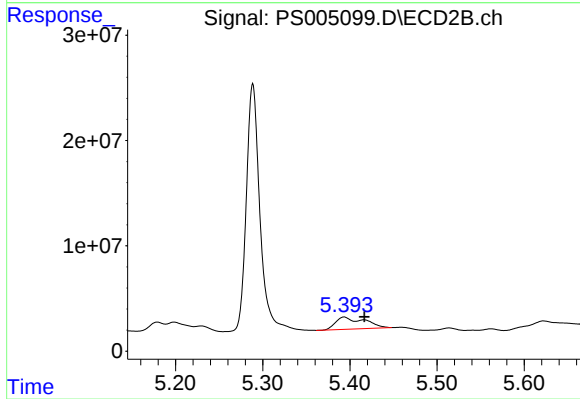

#5 DICAMBA


R.T.: 5.393 min
Delta R.T.: -0.023 min
Response: 26318908
Conc: 6.85 ng/ml

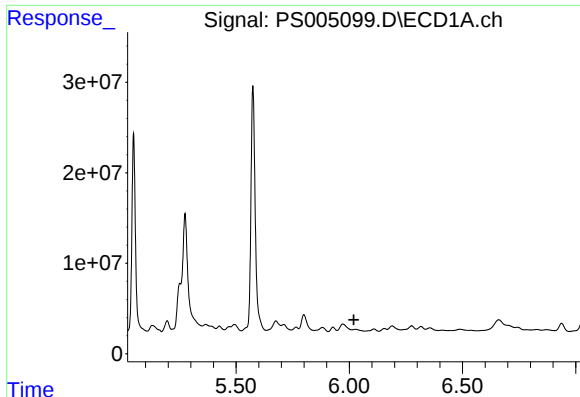

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 6.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-A

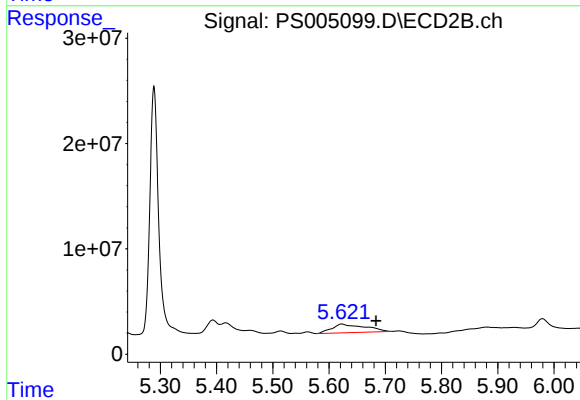


#7 MCPA

R.T.: 5.622 min
Delta R.T.: -0.061 min
Response: 33146885
Conc: 7.86 ug/ml

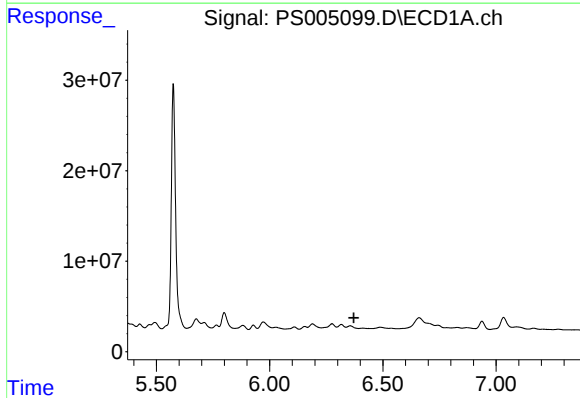


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.372 min
Response: 0
Conc: N.D.

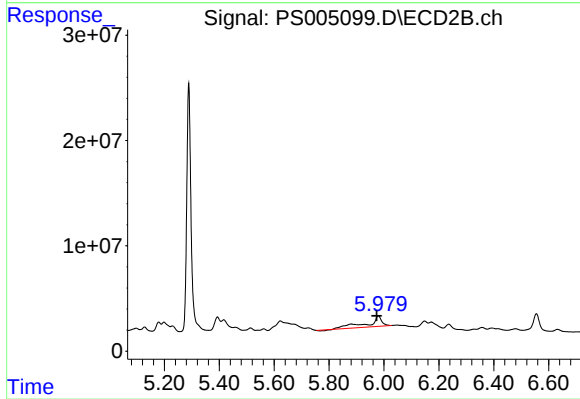

#8 DICHLORPROP


R.T.: 5.979 min
Delta R.T.: 0.006 min
Response: 35456932
Conc: 36.51 ng/ml

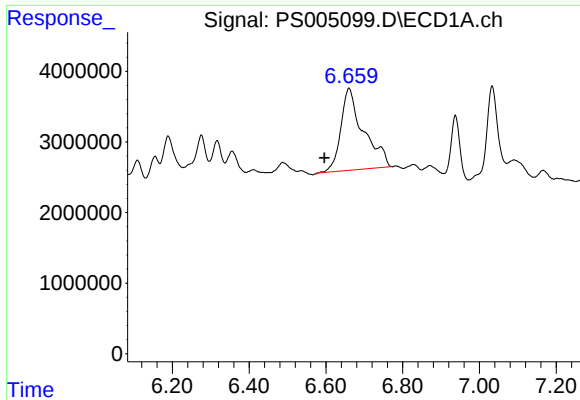

#9 2,4-D


R.T.: 6.660 min
Delta R.T.: 0.064 min
Response: 47340506
Conc: 35.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-A

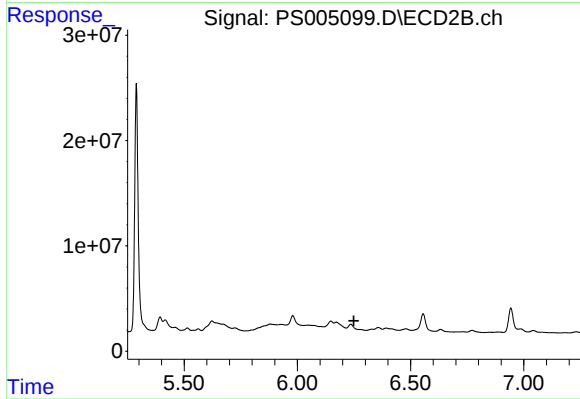


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

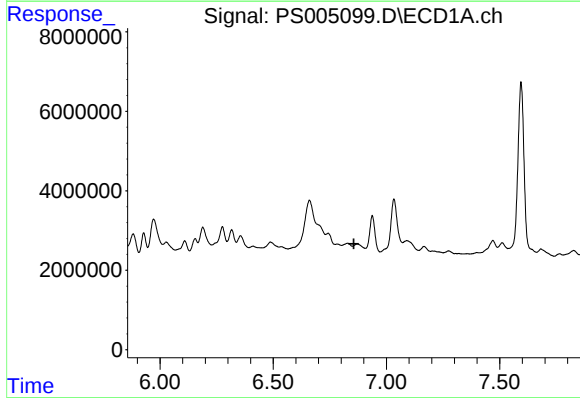


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.856 min
Response: 0
Conc: N.D.

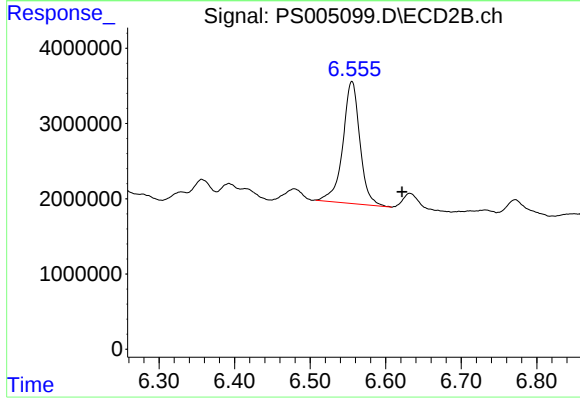

#10 Pentachlorophenol


R.T.: 6.555 min
Delta R.T.: -0.066 min
Response: 25481499
Conc: 1.98 ng/ml

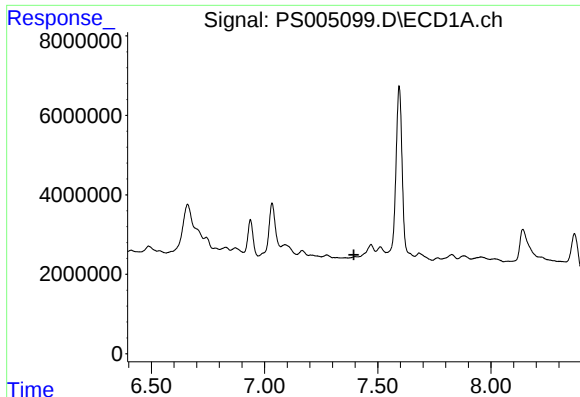

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-A

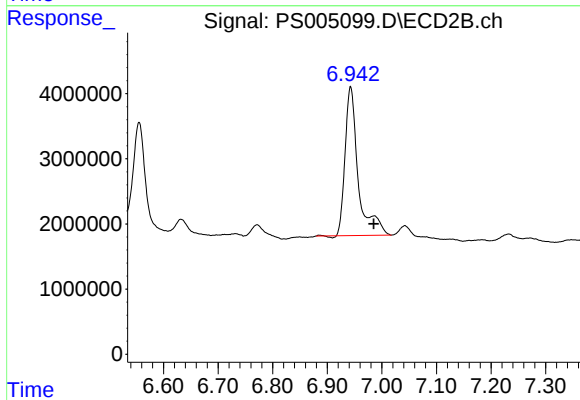


#11 2,4,5-TP (SILVEX)

R.T.: 6.943 min
Delta R.T.: -0.042 min
Response: 38199801
Conc: 7.14 ng/ml

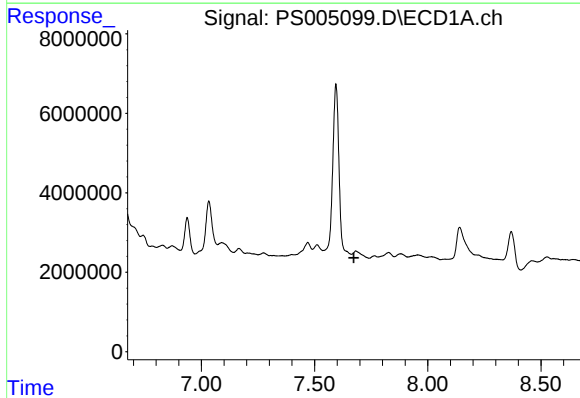

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.674 min
Response: 0
Conc: N.D.

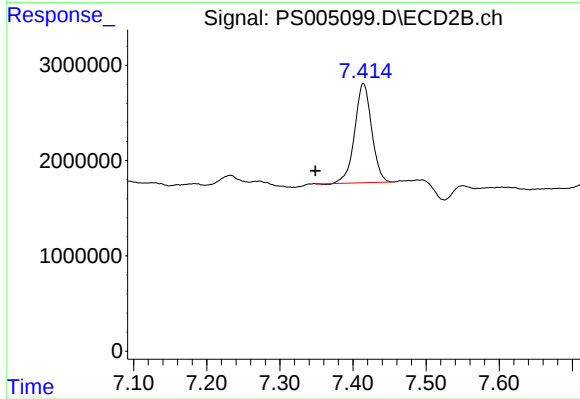

#12 2,4,5-T

R.T.: 7.414 min
Delta R.T.: 0.066 min
Response: 16759090
Conc: 3.55 ng/ml