

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 21:53
 Operator : SM\AJ
 Sample : K3157-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-061719-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 00:54:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.587	5.285	332.8E6	244.5E6	252.557	245.116
Target Compounds							
1) T	Dalapon	2.083	0.000	30983130	0	17.787	N.D. #
2) T	3,5-DICHL...	0.000	4.604	0	175.4E6	N.D.	137.068
5) T	DICAMBA	0.000	5.392	0	4047398	N.D.	1.054
7) T	MCPA	0.000	5.618	0	28956315	N.D.	6.869
8) T	DICHLORPROP	0.000	5.977	0	21734714	N.D.	22.379
11) T	2,4,5-TP ...	0.000	6.939	0	32517325	N.D.	6.075
12) T	2,4,5-T	7.608	7.411	81765205	19133784	10.233	4.057 #
13) T	2,4-DB	8.153	0.000	26431264	0	28.793	N.D. #
15) T	Picloram	9.136	0.000	21074260	0	2.123	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 21:53
Operator : SM\AJ
Sample : K3157-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 00:54:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

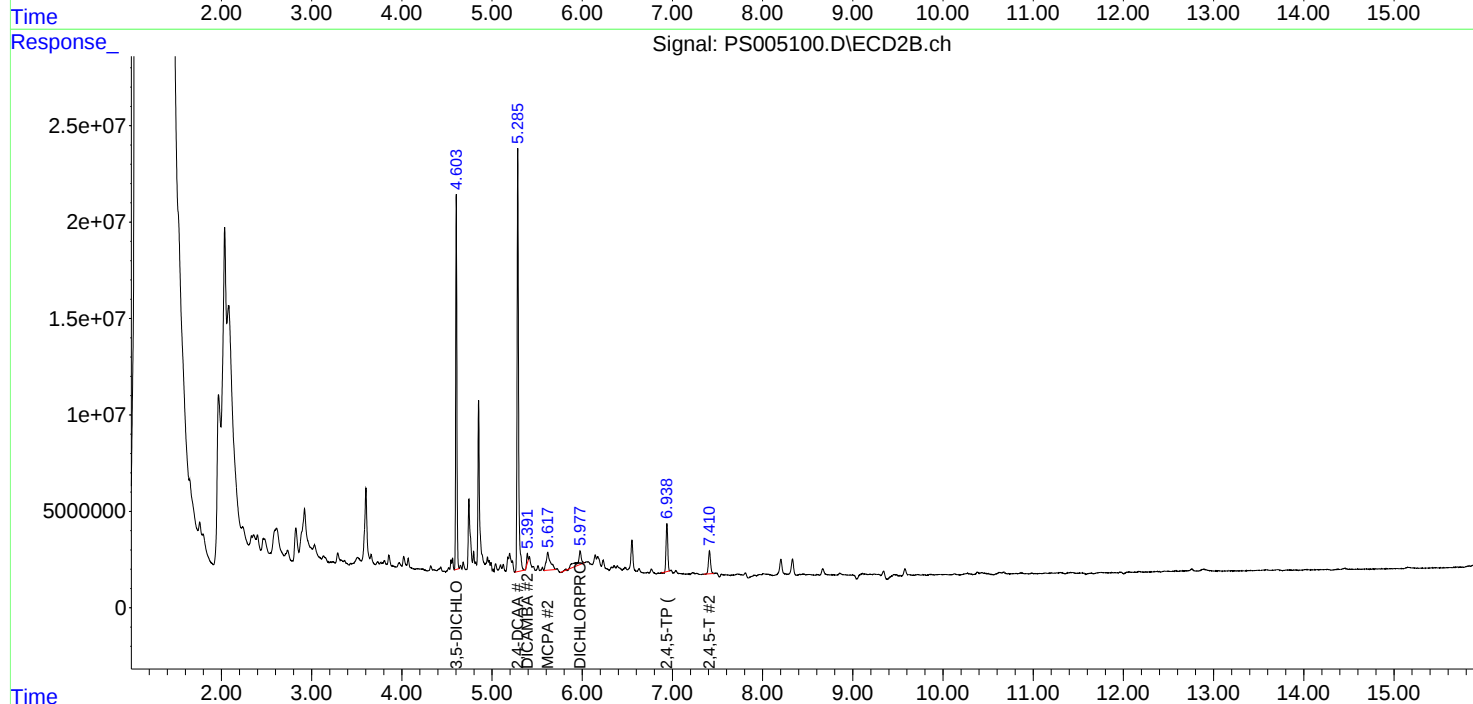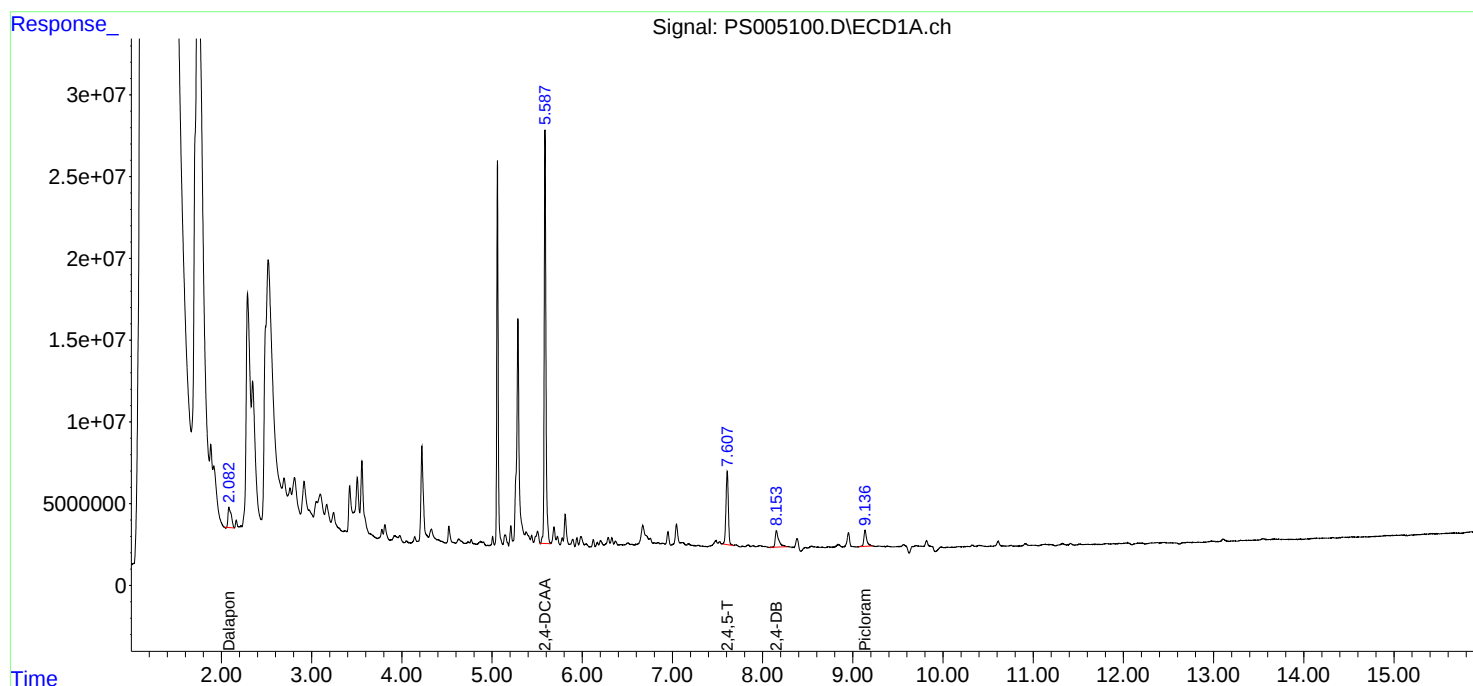


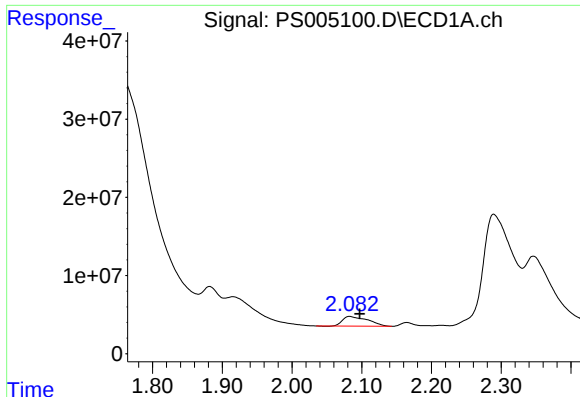

#1 Dalapon


R.T.: 2.083 min
Delta R.T.: -0.014 min
Response: 30983130
Conc: 17.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-B

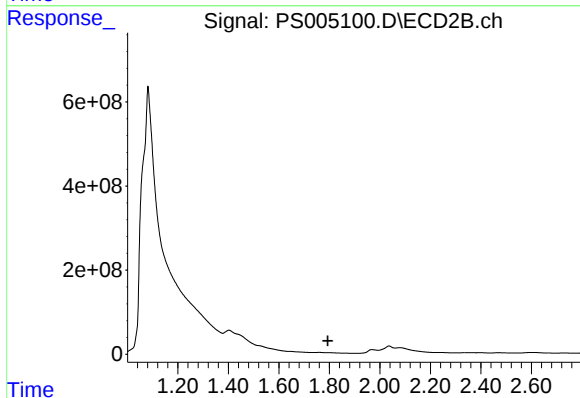


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.794 min
Response: 0
Conc: N.D.

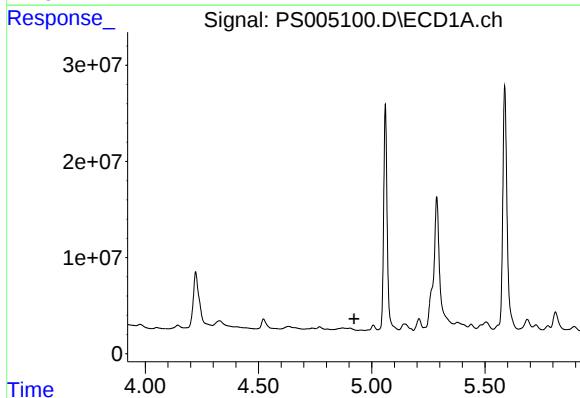


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

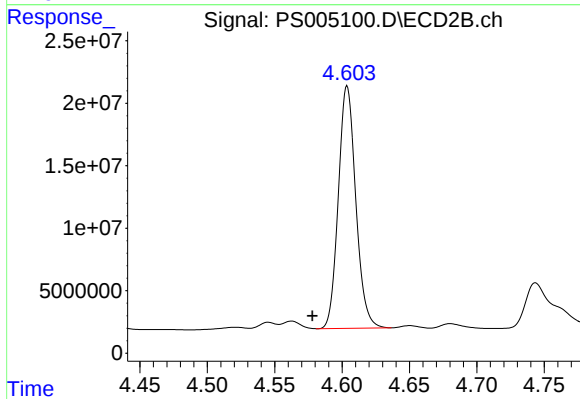

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.604 min
Delta R.T.: 0.026 min
Response: 175418278
Conc: 137.07 ng/ml

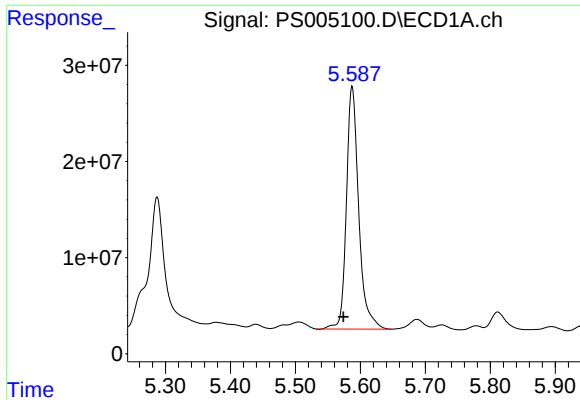

#4 2,4-DCAA


R.T.: 5.587 min
Delta R.T.: 0.014 min
Response: 332818733
Conc: 252.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-B

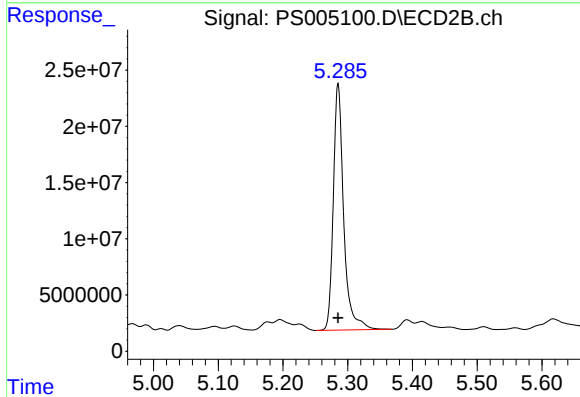


#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: 0.000 min
Response: 244511594
Conc: 245.12 ng/ml

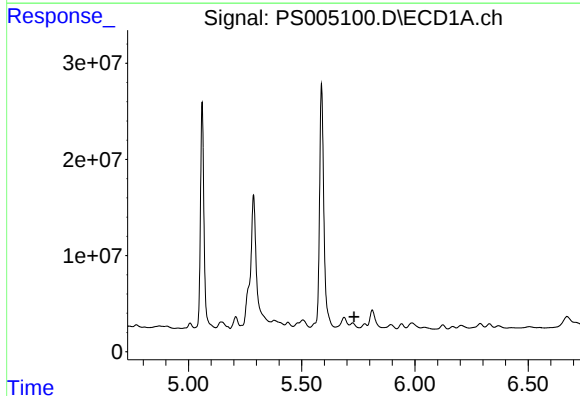


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.731 min
Response: 0
Conc: N.D.

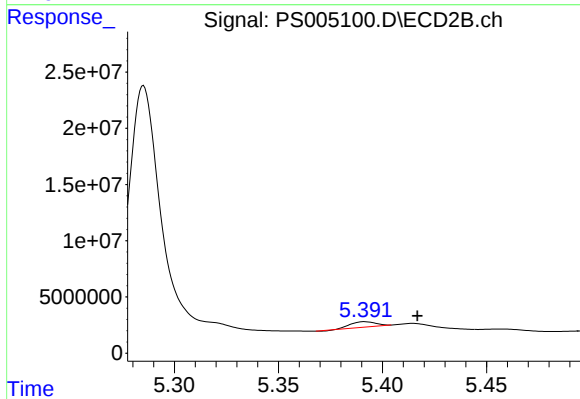

#5 DICAMBA


R.T.: 5.392 min
Delta R.T.: -0.025 min
Response: 4047398
Conc: 1.05 ng/ml

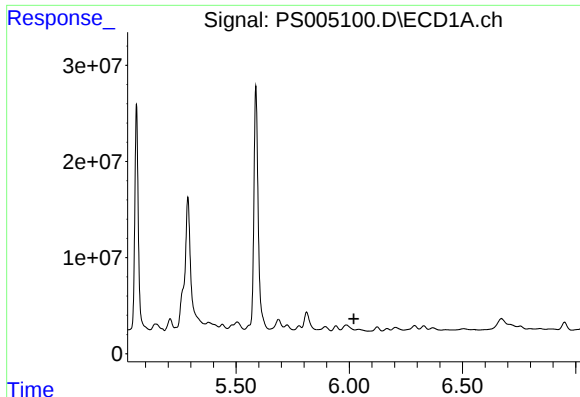

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-B

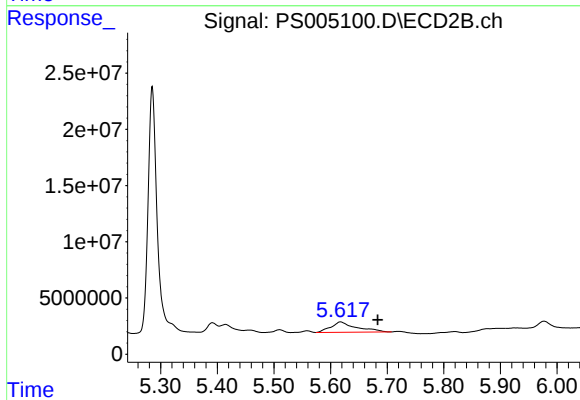


#7 MCPA

R.T.: 5.618 min
Delta R.T.: -0.066 min
Response: 28956315
Conc: 6.87 ug/ml

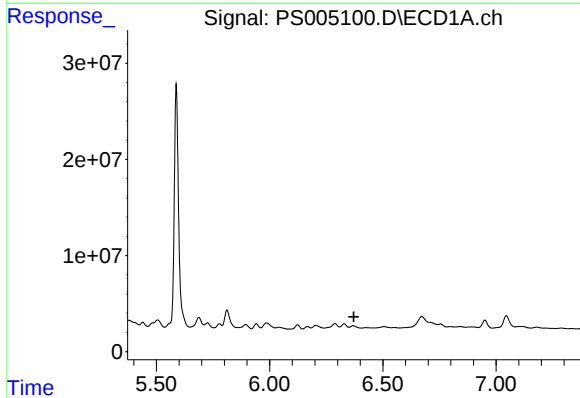


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.372 min
Response: 0
Conc: N.D.

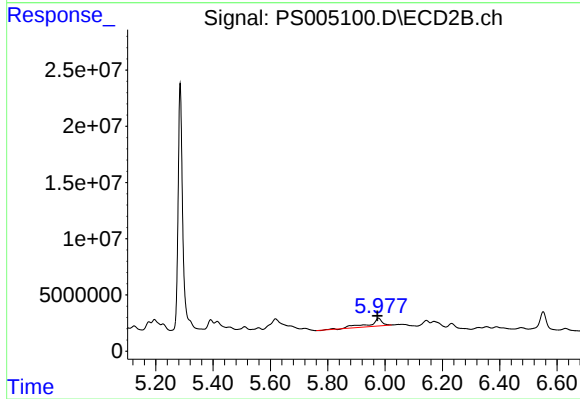

#8 DICHLORPROP


R.T.: 5.977 min
Delta R.T.: 0.003 min
Response: 21734714
Conc: 22.38 ng/ml

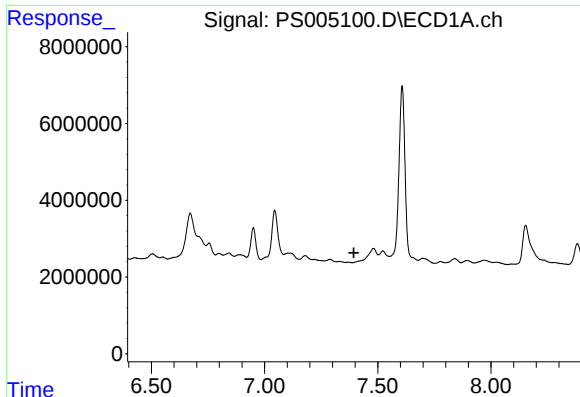

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-B

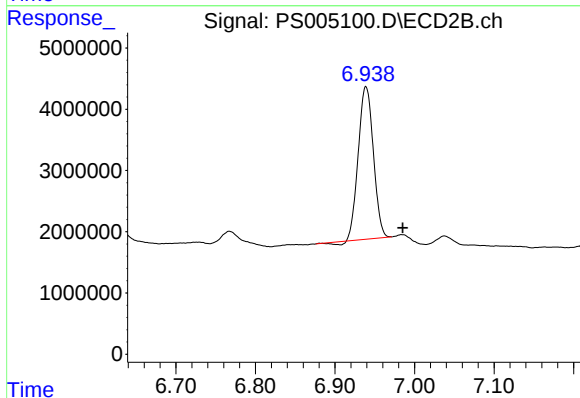


#11 2,4,5-TP (SILVEX)

R.T.: 6.939 min
Delta R.T.: -0.046 min
Response: 32517325
Conc: 6.07 ng/ml

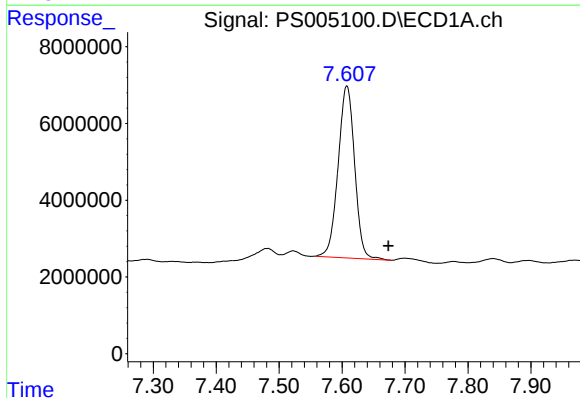


#12 2,4,5-T

R.T.: 7.608 min
Delta R.T.: -0.066 min
Response: 81765205
Conc: 10.23 ng/ml

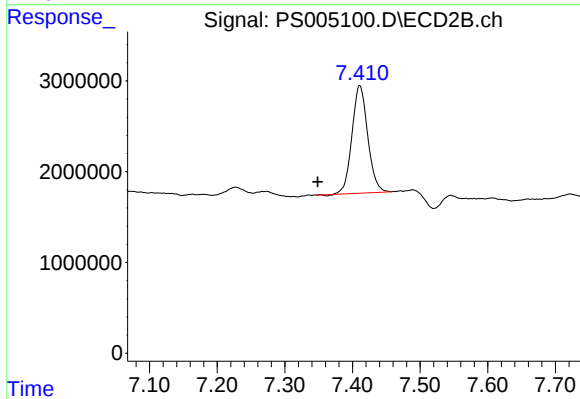

#12 2,4,5-T


R.T.: 7.411 min
Delta R.T.: 0.062 min
Response: 19133784
Conc: 4.06 ng/ml

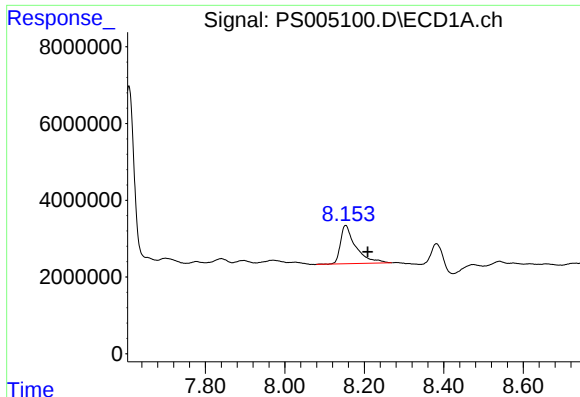

#13 2,4-DB


R.T.: 8.153 min
Delta R.T.: -0.055 min
Response: 26431264
Conc: 28.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-B

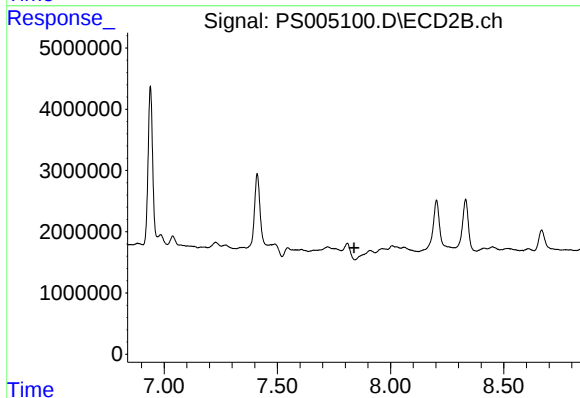


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

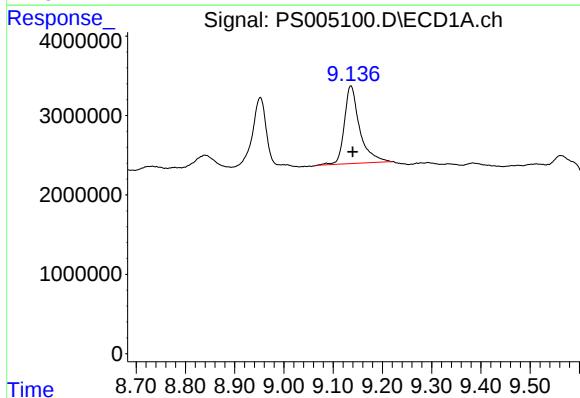

#15 Picloram

R.T.: 9.136 min
Delta R.T.: -0.003 min
Response: 21074260
Conc: 2.12 ng/ml

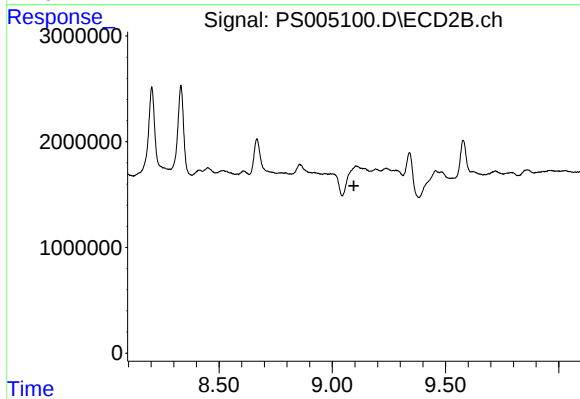

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.