

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 22:15
 Operator : SM\AJ
 Sample : K3157-06
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-061719-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 00:54:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.587	5.285	372.7E6	274.6E6	282.807	275.297
Target Compounds							
1) T	Dalapon	2.083	0.000	30533178	0	17.529	N.D. #
2) T	3,5-DICHL...	0.000	4.603	0	163.6E6	N.D.	127.811
5) T	DICAMBA	0.000	5.391	0	3380451	N.D.	<MDL
8) T	DICHLORPROP	0.000	5.977	0	23092826	N.D.	23.777
11) T	2,4,5-TP ...	0.000	6.939	0	31529668	N.D.	5.890
12) T	2,4,5-T	7.608	7.410	76539069	18766405	9.579	3.979 #
13) T	2,4-DB	8.154	0.000	21564659	0	23.491	N.D. #
14) T	DINOSEB	0.000	8.202	0	17060739	N.D.	4.392
15) T	Picloram	9.136	0.000	20622714	0	2.077	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 22:15
Operator : SM\AJ
Sample : K3157-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 00:54:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

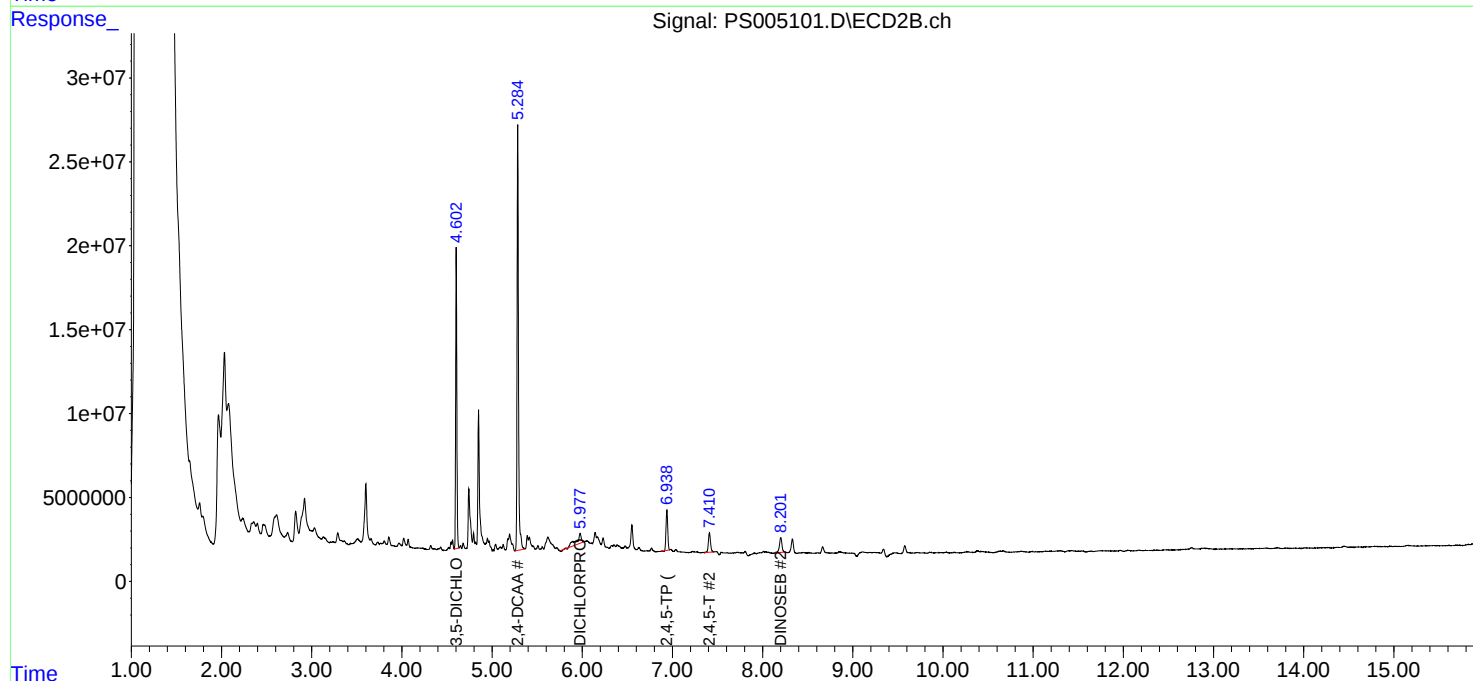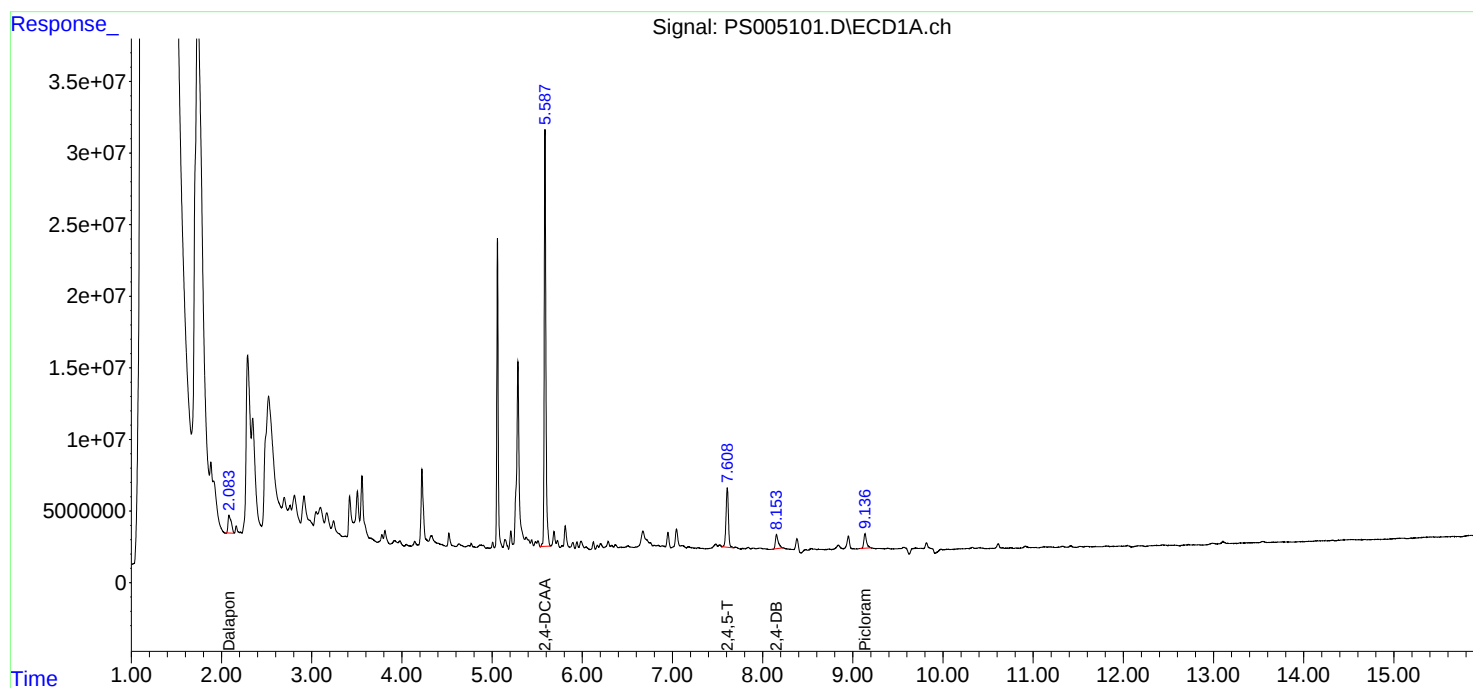


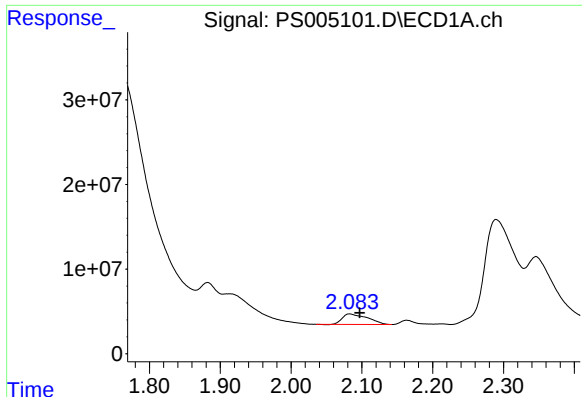

#1 Dalapon


R.T.: 2.083 min
Delta R.T.: -0.014 min
Response: 30533178
Conc: 17.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-C

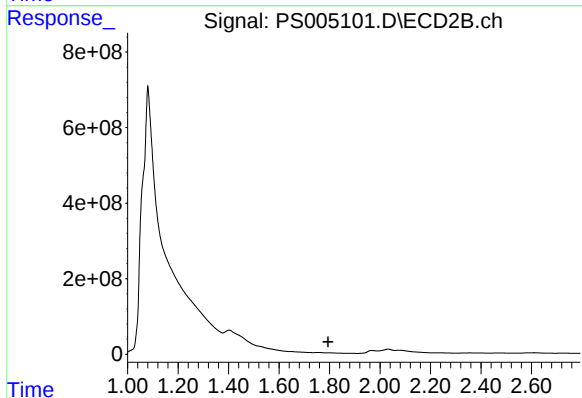


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.794 min
Response: 0
Conc: N.D.

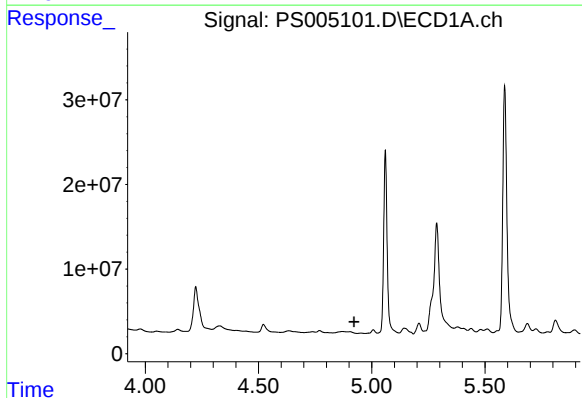


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.922 min
Response: 0
Conc: N.D.

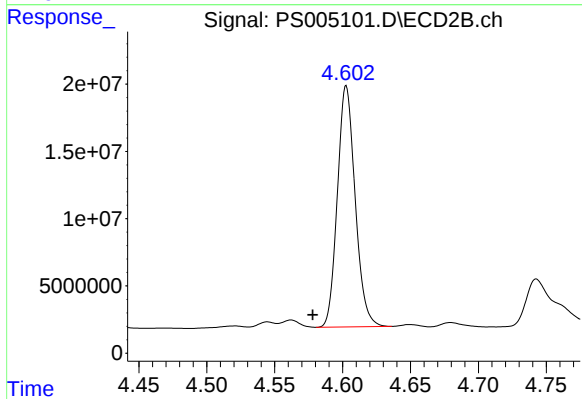

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.025 min
Response: 163570777
Conc: 127.81 ng/ml

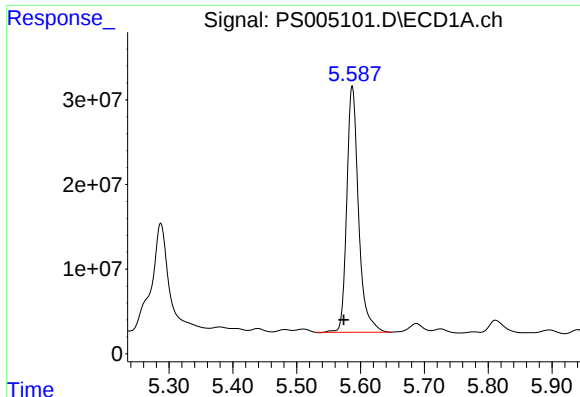

#4 2,4-DCAA


R.T.: 5.587 min
Delta R.T.: 0.013 min
Response: 372682108
Conc: 282.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-C

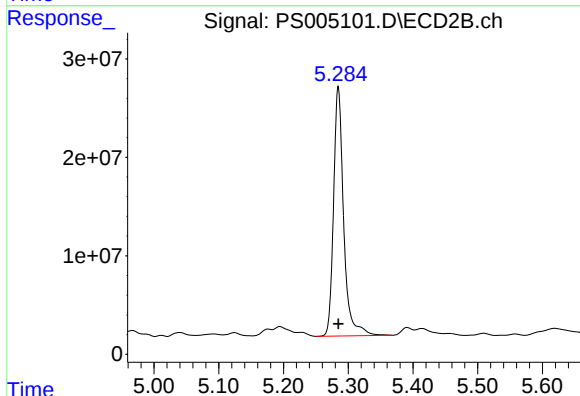


#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: 0.000 min
Response: 274618451
Conc: 275.30 ng/ml

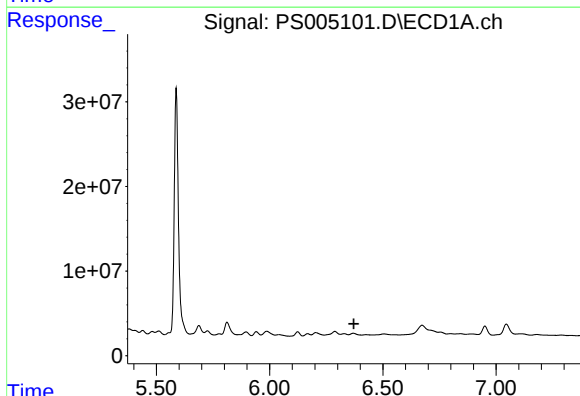


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.372 min
Response: 0
Conc: N.D.

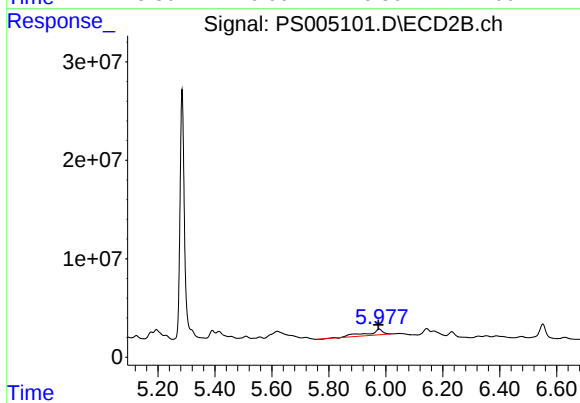

#8 DICHLORPROP


R.T.: 5.977 min
Delta R.T.: 0.003 min
Response: 23092826
Conc: 23.78 ng/ml

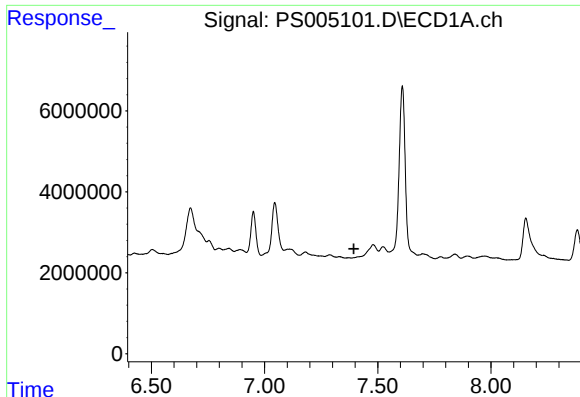

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-C

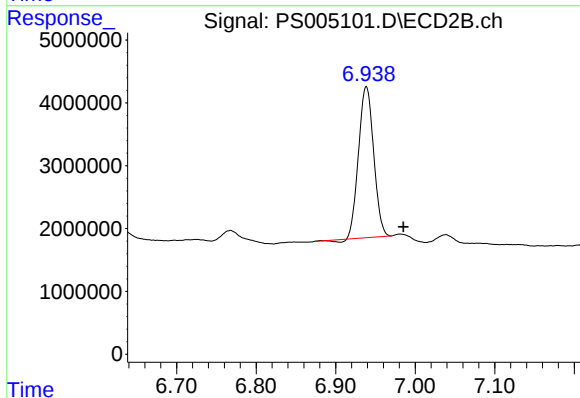


#11 2,4,5-TP (SILVEX)

R.T.: 6.939 min
Delta R.T.: -0.047 min
Response: 31529668
Conc: 5.89 ng/ml

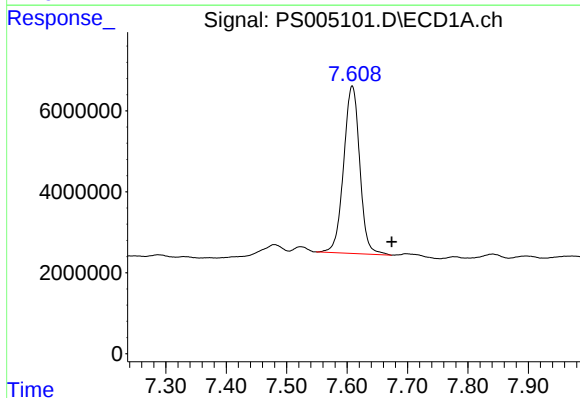


#12 2,4,5-T

R.T.: 7.608 min
Delta R.T.: -0.065 min
Response: 76539069
Conc: 9.58 ng/ml

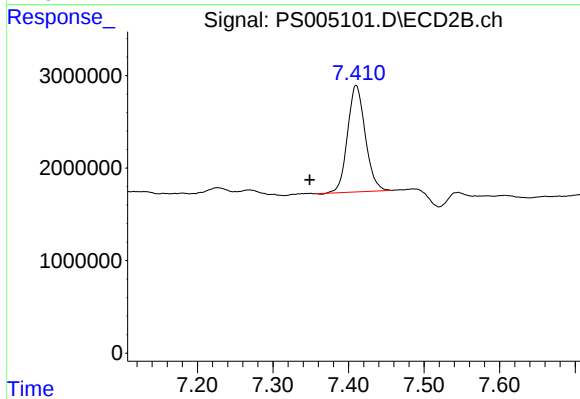

#12 2,4,5-T


R.T.: 7.410 min
Delta R.T.: 0.061 min
Response: 18766405
Conc: 3.98 ng/ml

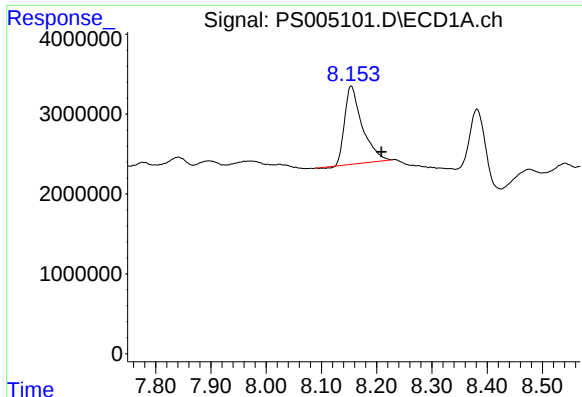

#13 2,4-DB


R.T.: 8.154 min
Delta R.T.: -0.054 min
Response: 21564659
Conc: 23.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-C

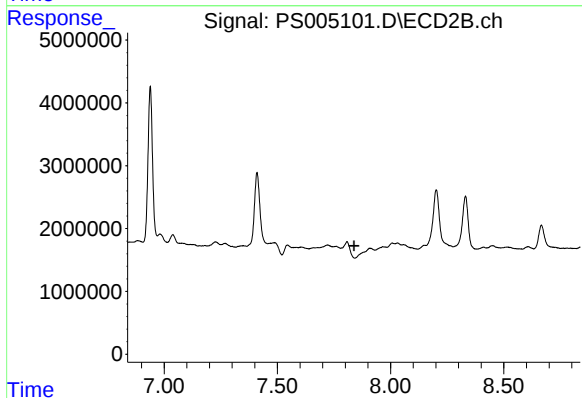


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

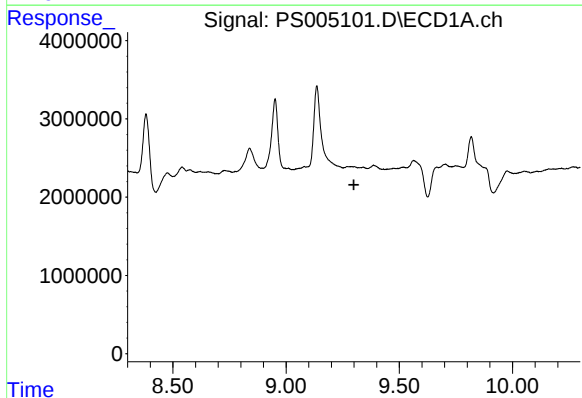


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.300 min
Response: 0
Conc: N.D.

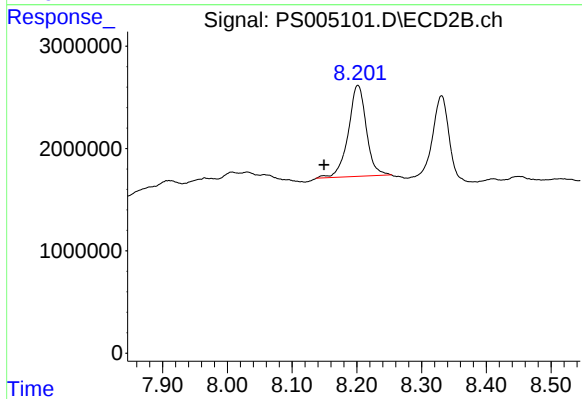

#14 DINOSEB


R.T.: 8.202 min
Delta R.T.: 0.052 min
Response: 17060739
Conc: 4.39 ng/ml

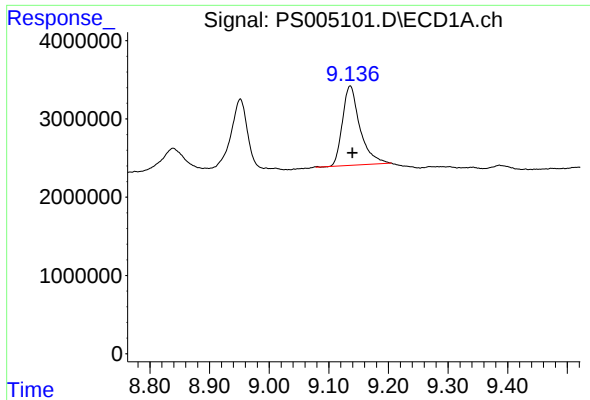

#15 Picloram

R.T.: 9.136 min
Delta R.T.: -0.004 min
Response: 20622714
Conc: 2.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-C

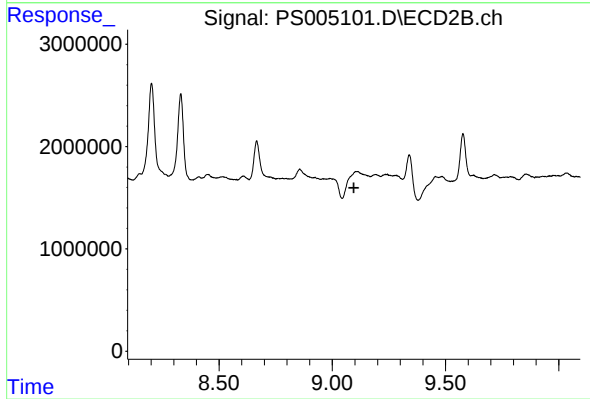

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.