

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 00:05
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 00:56:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.592	5.293	531.1E6	382.6E6	403.055	383.555
Target Compounds							
2) T	3,5-DICHL...	4.957	0.000	168.2E6	0	89.213	N.D. #
5) T	DICAMBA	0.000	5.447	0	137.8E6	N.D.	35.870
6) T	MCP	0.000	5.447	0	137.8E6	N.D.	47.677
9) T	2,4-D	6.634	0.000	163.5E6	0	121.142	N.D. #
15) T	Picloram	9.131	0.000	109.7E6	0	11.050	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 00:05
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 00:56:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

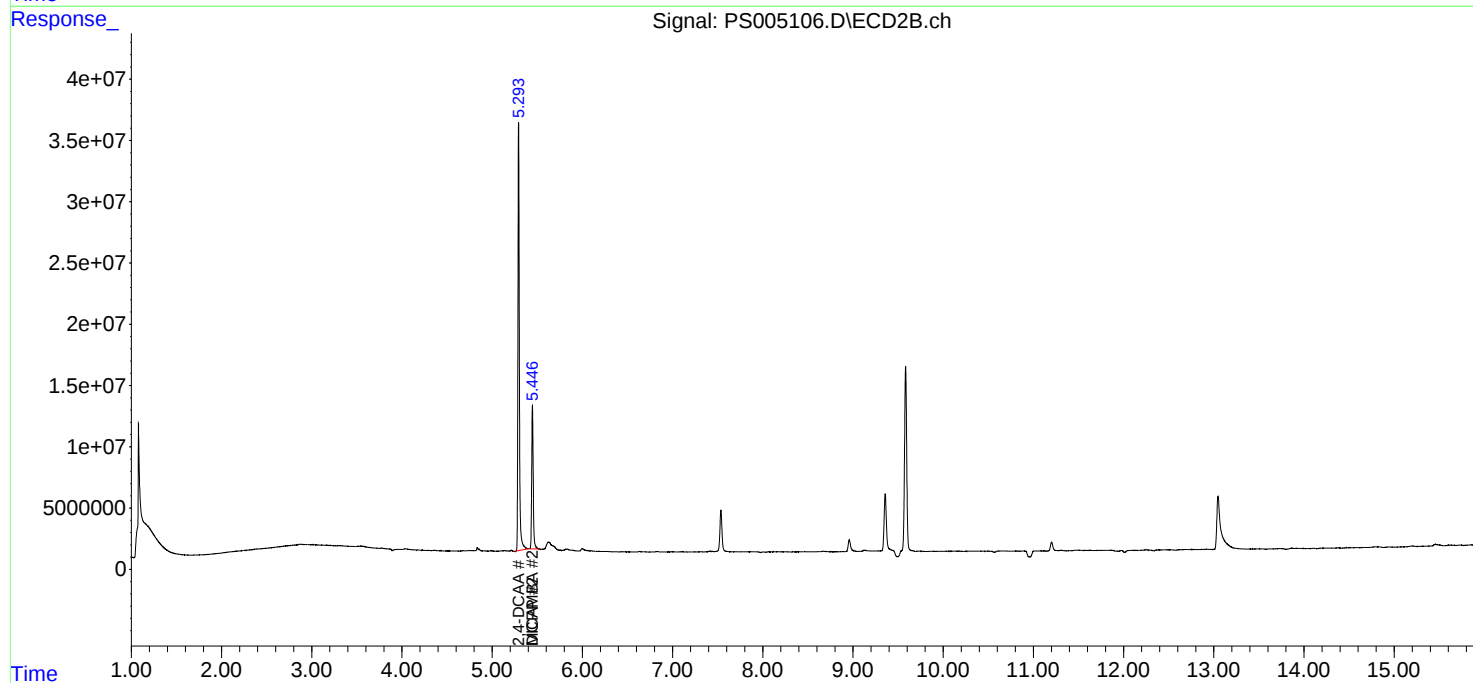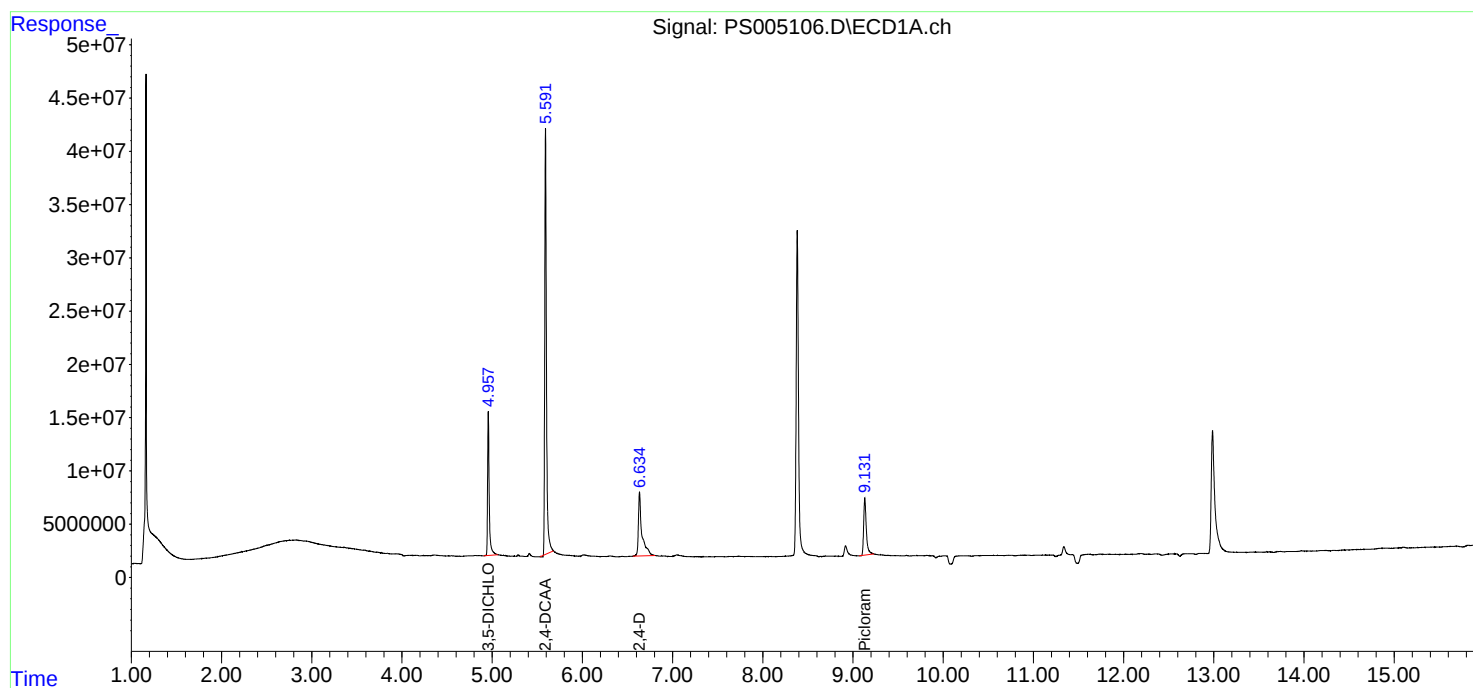


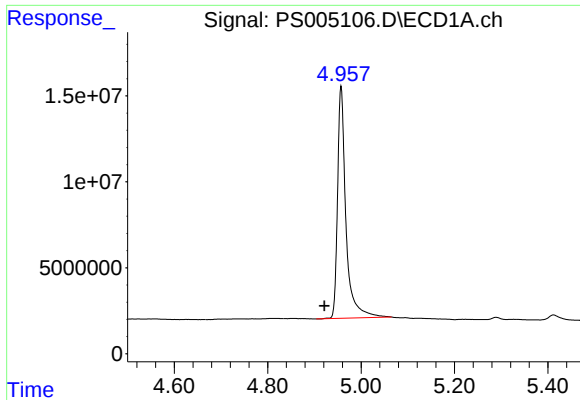

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.957 min
Delta R.T.: 0.036 min
Response: 168151782
Conc: 89.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

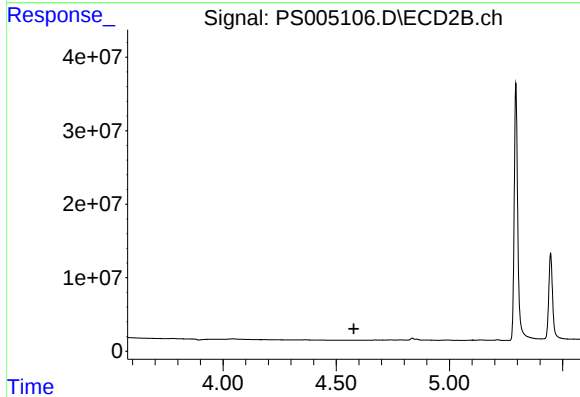


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.578 min
Response: 0
Conc: N.D.

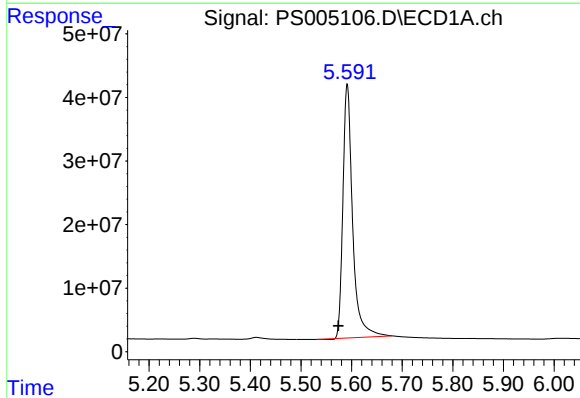


#4 2,4-DCAA

R.T.: 5.592 min
Delta R.T.: 0.018 min
Response: 531143368
Conc: 403.05 ng/ml

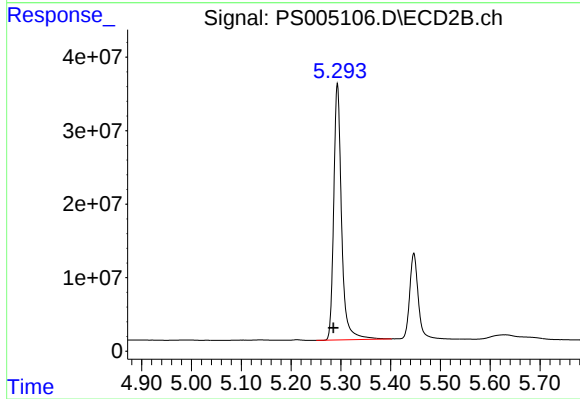

#4 2,4-DCAA


R.T.: 5.293 min
Delta R.T.: 0.008 min
Response: 382610322
Conc: 383.56 ng/ml

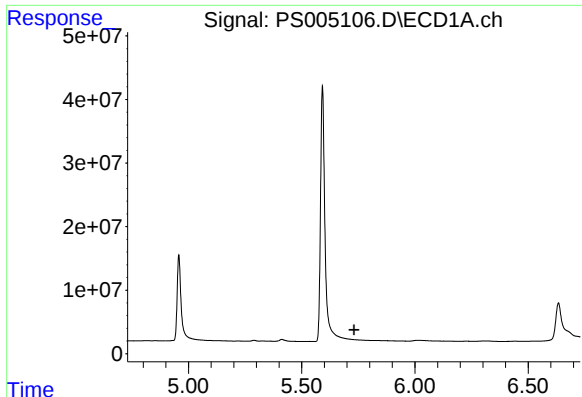

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

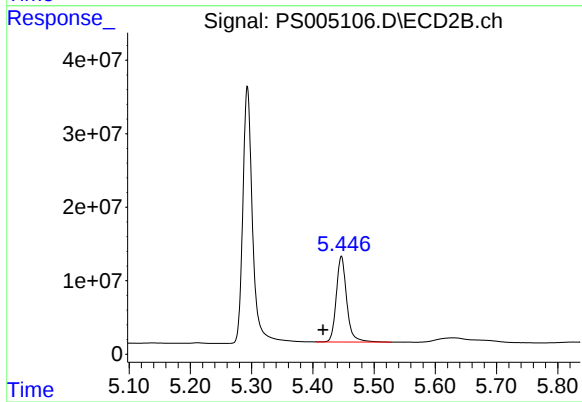


#5 DICAMBA

R.T.: 5.447 min
Delta R.T.: 0.030 min
Response: 137759865
Conc: 35.87 ng/ml

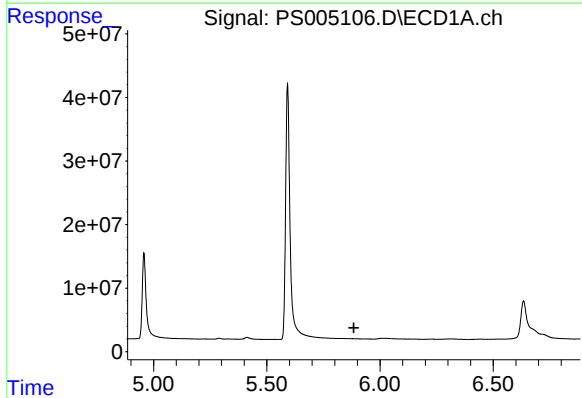


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.885 min
Response: 0
Conc: N.D.

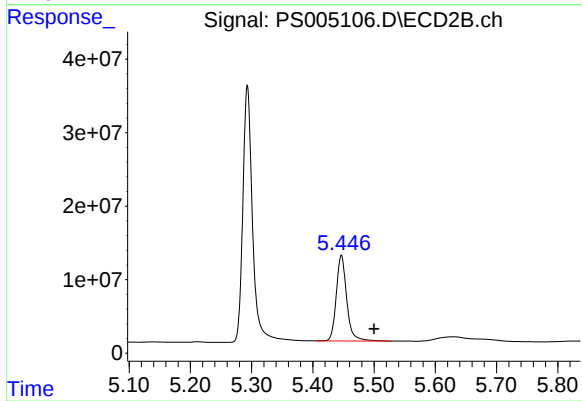

#6 MCPP


R.T.: 5.447 min
Delta R.T.: -0.053 min
Response: 137759865
Conc: 47.68 ug/ml

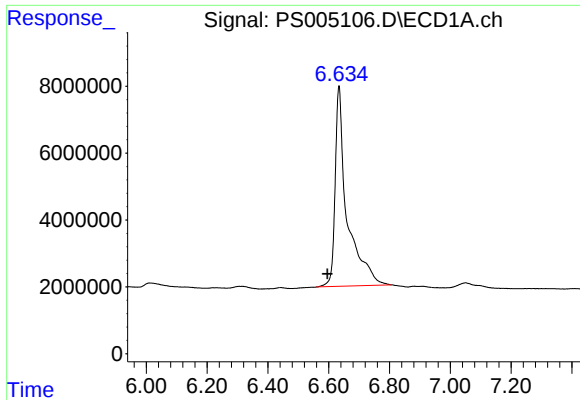

#9 2,4-D


R.T.: 6.634 min
Delta R.T.: 0.038 min
Response: 163462349
Conc: 121.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

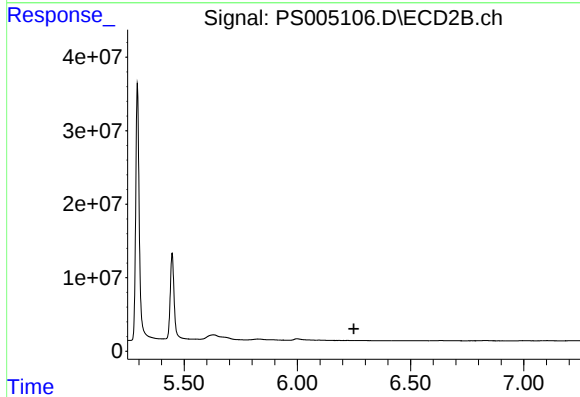


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

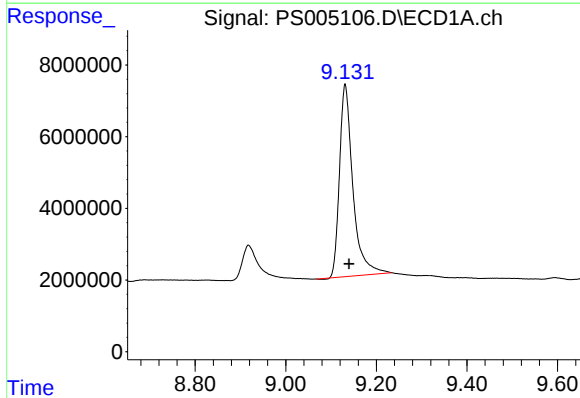

#15 Picloram

R.T.: 9.131 min
Delta R.T.: -0.008 min
Response: 109708718
Conc: 11.05 ng/ml

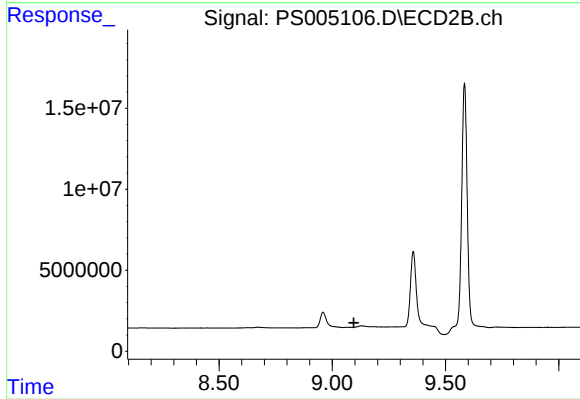

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.