

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 02:39
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:20:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.574	5.287	552.2E6	387.8E6	419.019	388.759
Target Compounds							
2) T	3,5-DICHL...	4.939	0.000	267.7E6	0	142.024	N.D. #
5) T	DICAMBA	0.000	5.440	0	209.7E6	N.D.	54.592
6) T	MCP	0.000	5.440	0	209.7E6	N.D.	72.560
9) T	2,4-D	6.616	0.000	209.2E6	0	155.060	N.D. #
15) T	Picloram	9.114	0.000	120.8E6	0	12.169	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 02:39
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:20:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

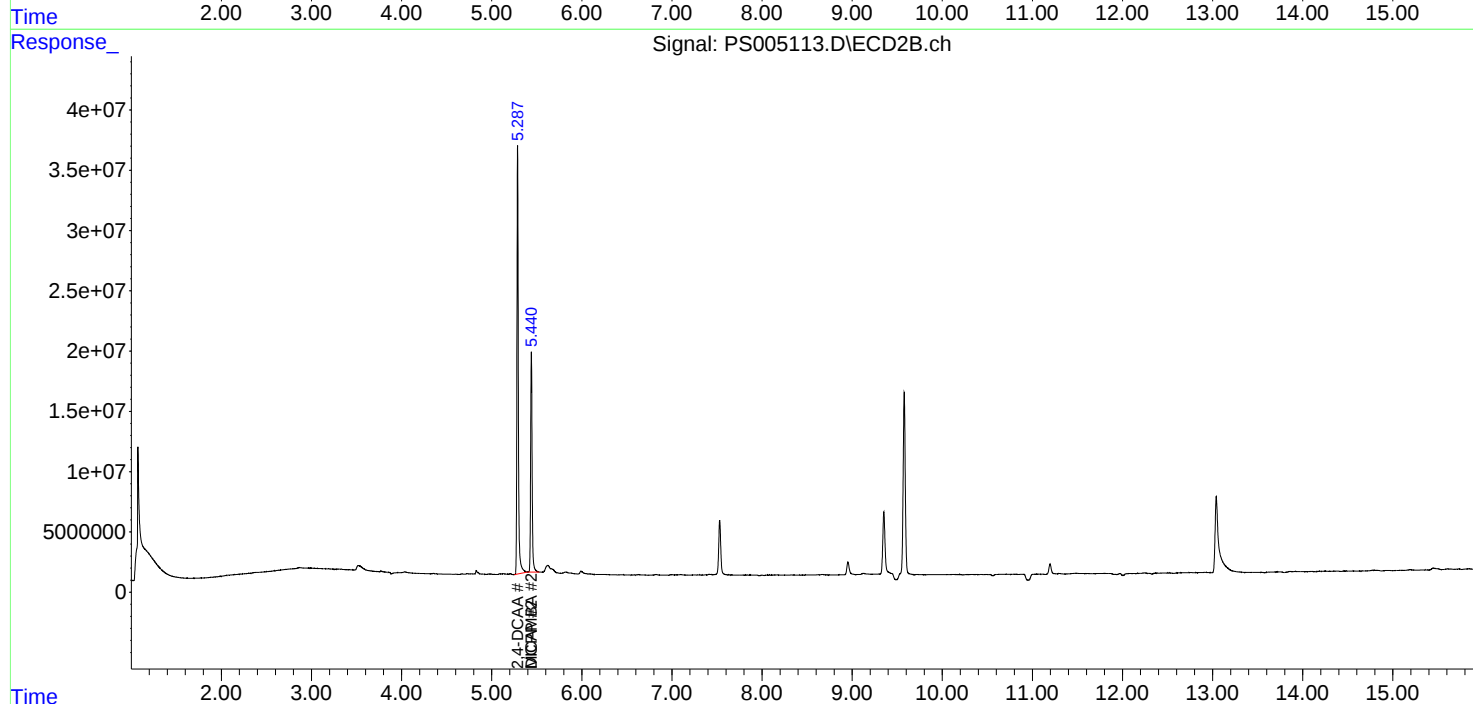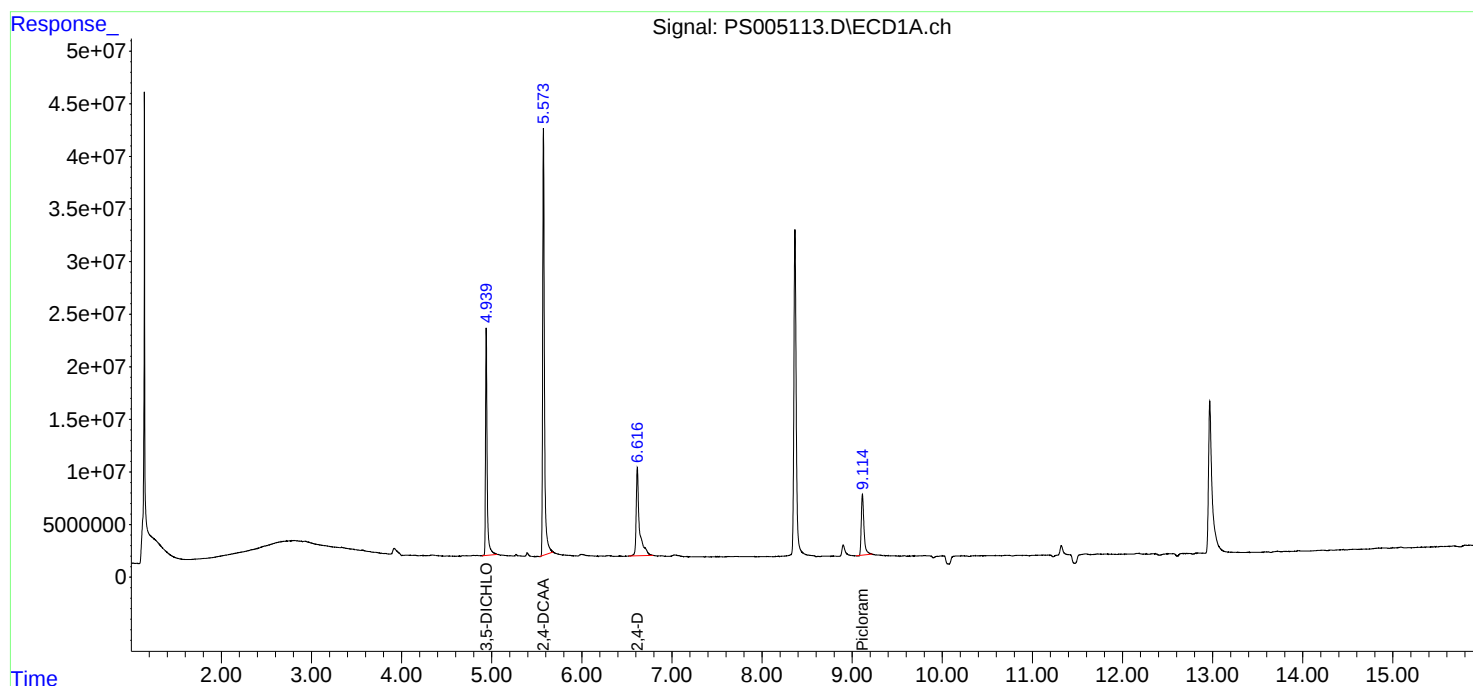


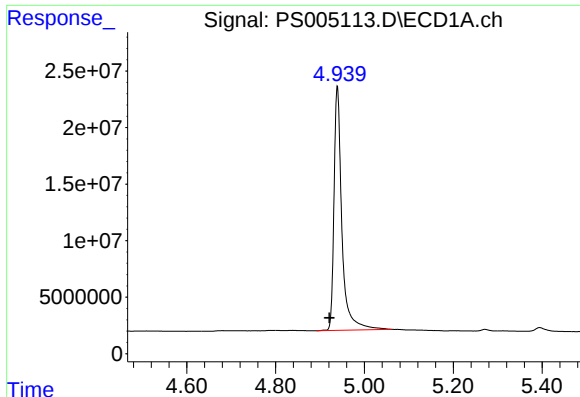

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.939 min
Delta R.T.: 0.018 min
Response: 267692471
Conc: 142.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

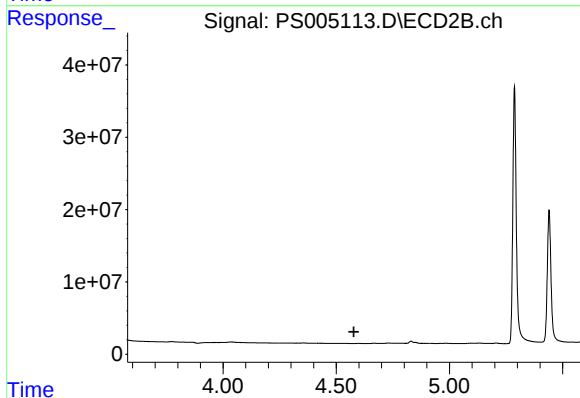


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.578 min
Response: 0
Conc: N.D.

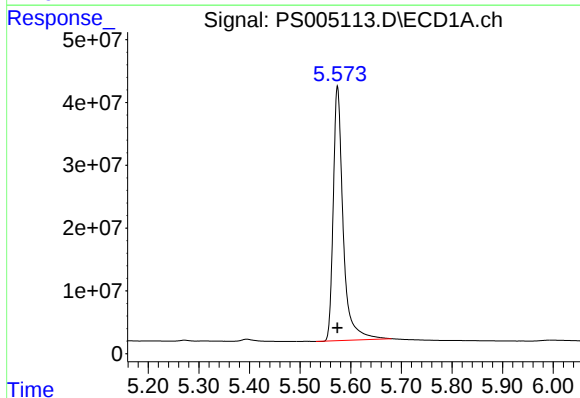


#4 2,4-DCAA

R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 552181220
Conc: 419.02 ng/ml

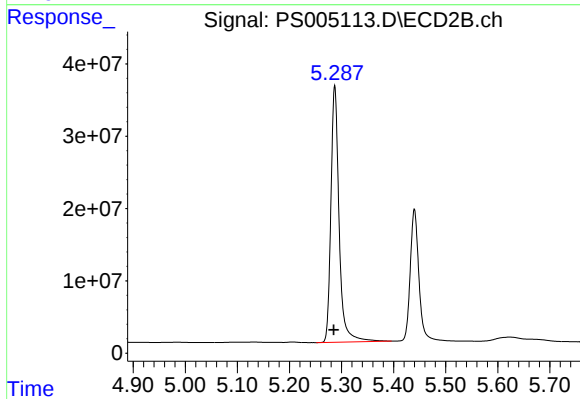

#4 2,4-DCAA


R.T.: 5.287 min
Delta R.T.: 0.002 min
Response: 387801437
Conc: 388.76 ng/ml

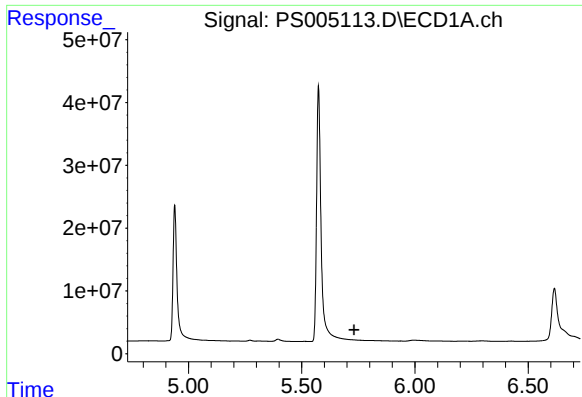

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

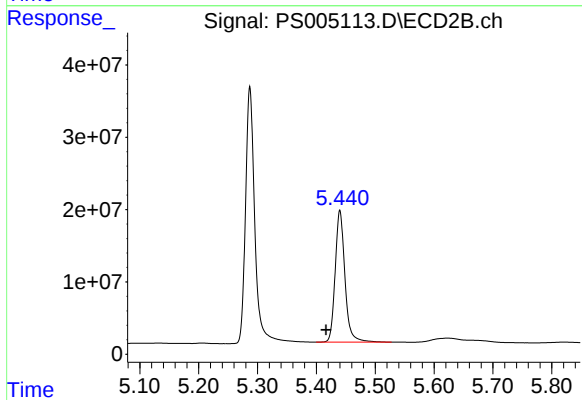


#5 DICAMBA

R.T.: 5.440 min
Delta R.T.: 0.023 min
Response: 209659917
Conc: 54.59 ng/ml

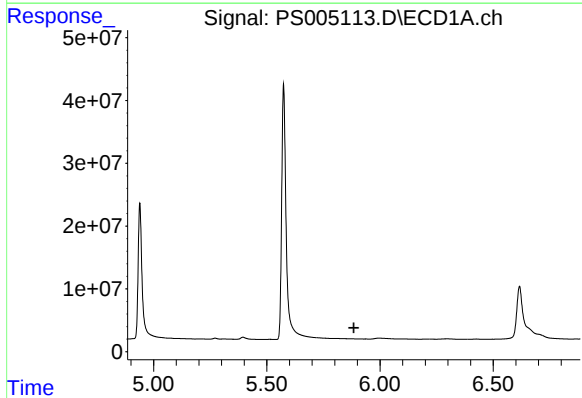


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.885 min
Response: 0
Conc: N.D.

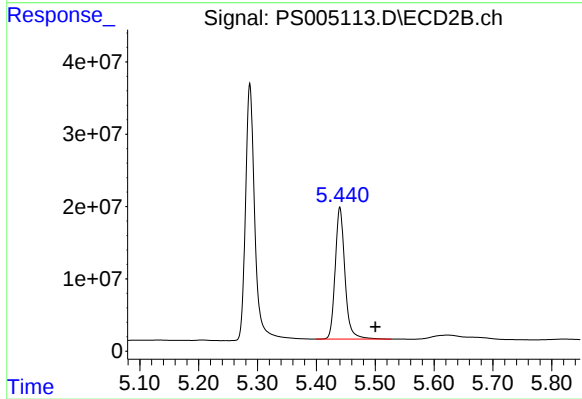

#6 MCPP


R.T.: 5.440 min
Delta R.T.: -0.060 min
Response: 209659917
Conc: 72.56 ug/ml

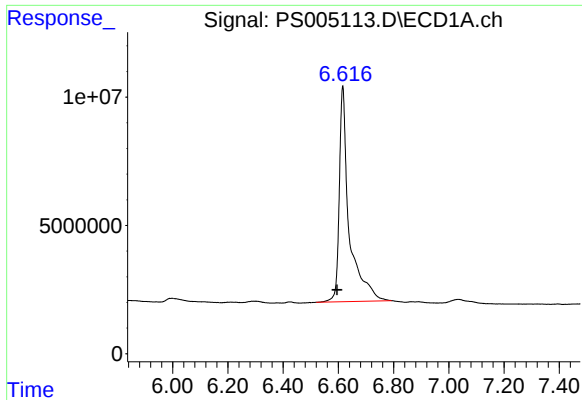

#9 2,4-D


R.T.: 6.616 min
Delta R.T.: 0.020 min
Response: 209229376
Conc: 155.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

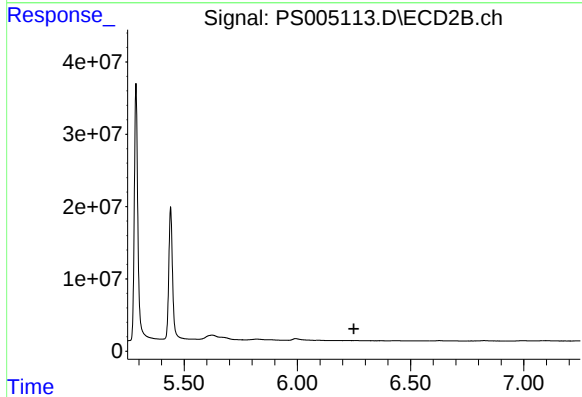


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.250 min
Response: 0
Conc: N.D.

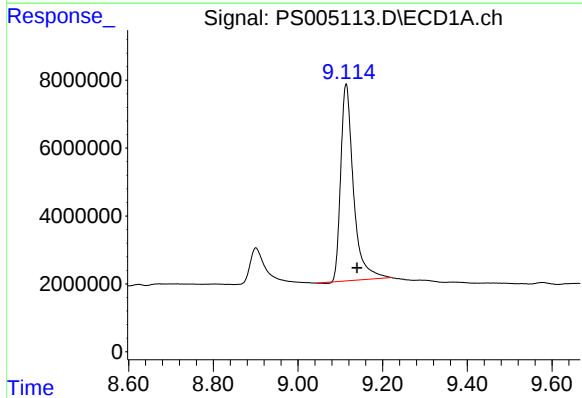

#15 Picloram

R.T.: 9.114 min
Delta R.T.: -0.026 min
Response: 120810674
Conc: 12.17 ng/ml

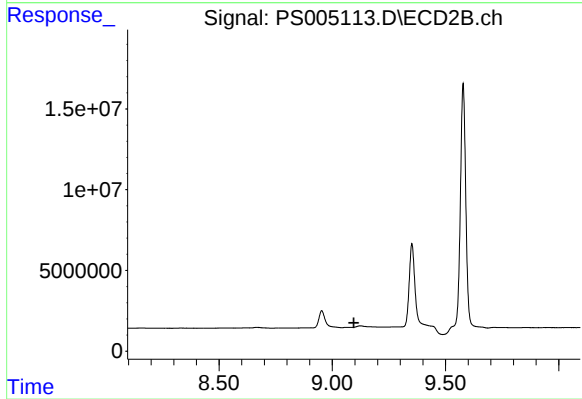

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.