

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
 Data File : PS005101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 22:15
 Operator : SM\AJ
 Sample : K3157-06
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-061719-C

Manual Integrations
 APPROVED

Ankita
 6/19/2019 1:35:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 00:54:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
 Quant Title : 8080.M
 QLast Update : Fri Jun 14 09:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	5.587	5.285	373.1E6	274.6E6	283.160m	275.297
------	----------	-------	-------	---------	---------	----------	---------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061819\
Data File : PS005101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 22:15
Operator : SM\AJ
Sample : K3157-06
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CL-01-061719-C


Manual Integrations
APPROVED

Ankita
6/19/2019 1:35:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 00:54:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061219.M
Quant Title : 8080.M
QLast Update : Fri Jun 14 09:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

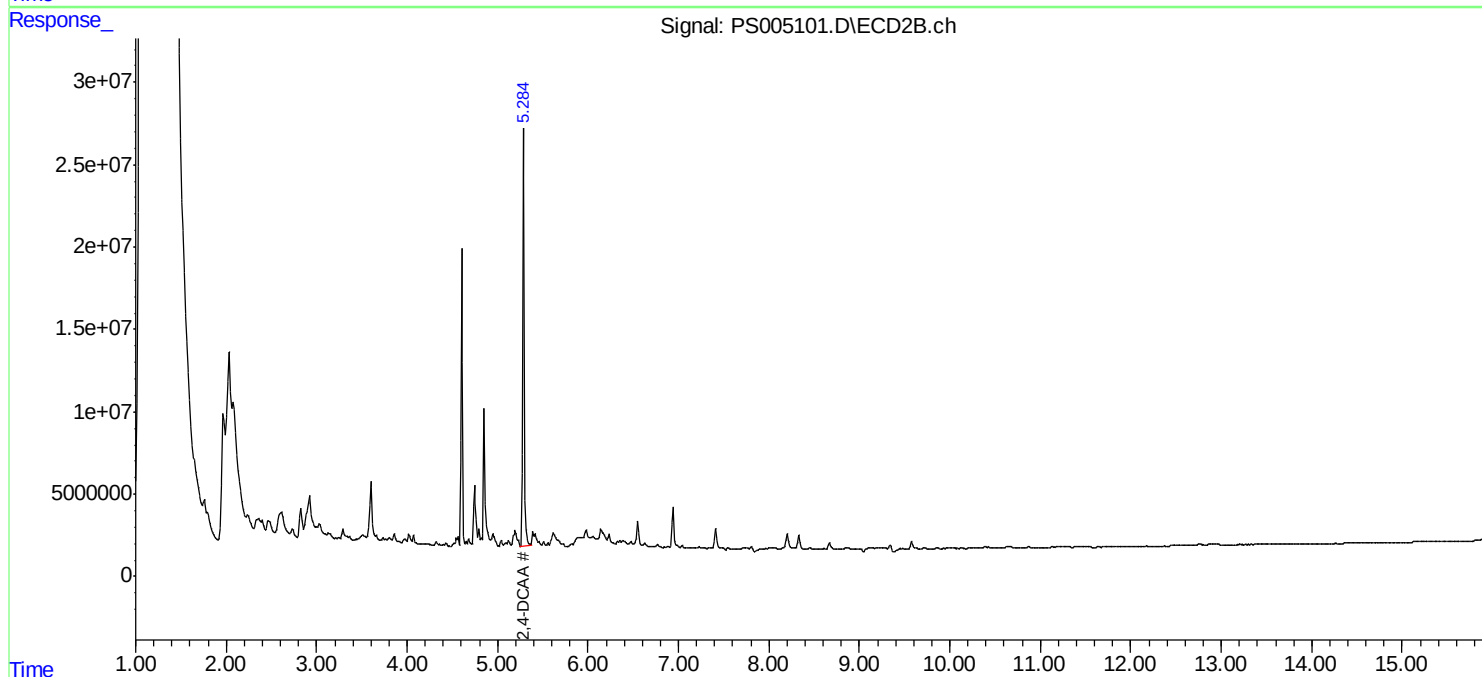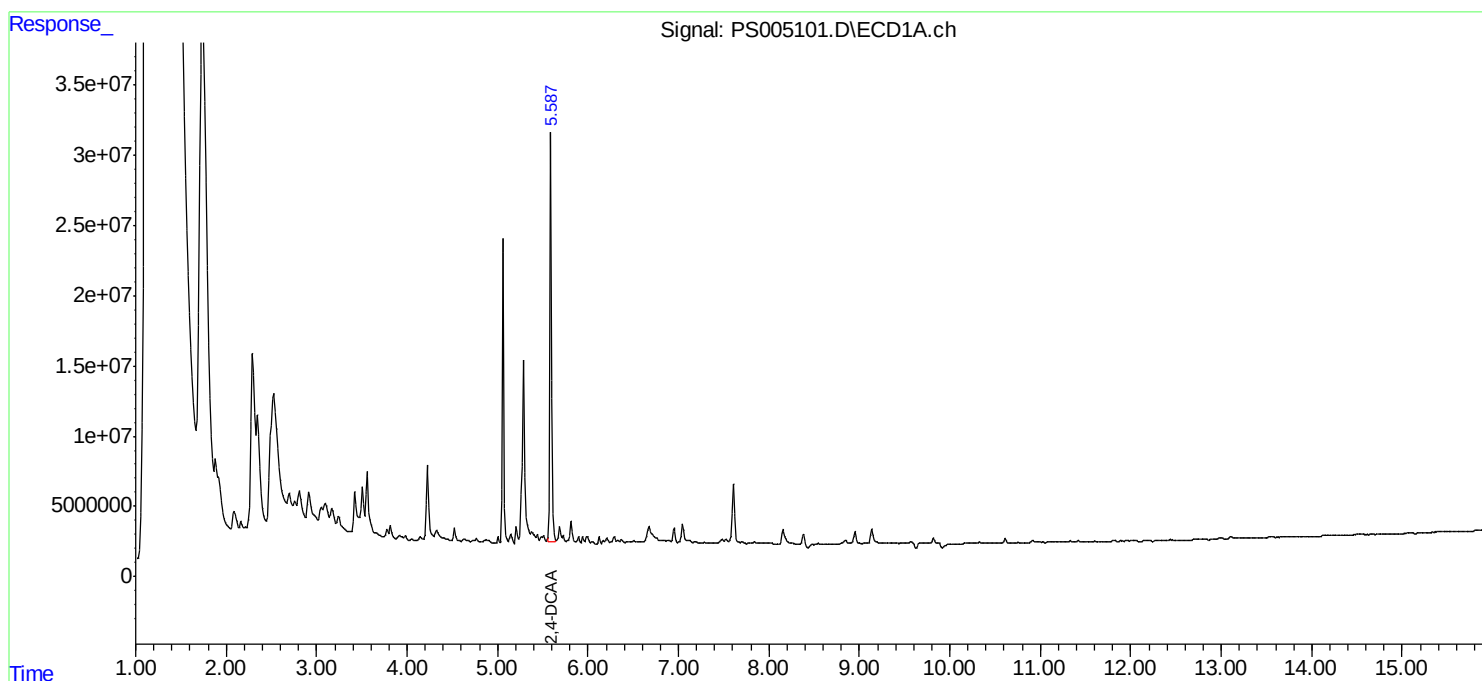

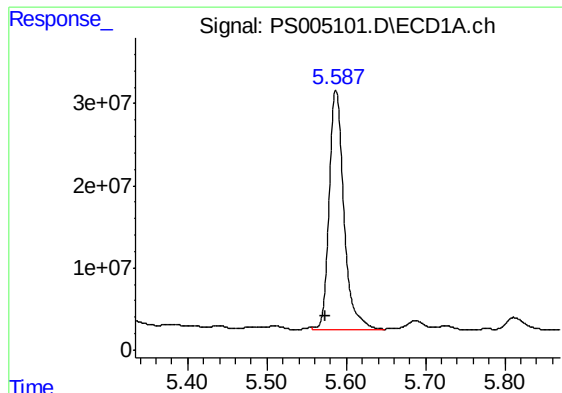


#4 2,4-DCAA

R.T.: 5.587 min
Delta R.T.: 0.013 min
Response: 373147389
Conc: 283.16 ng/ml m

Instrument :
ECD_S
ClientSampleId :
CL-01-061719-C

Manual Integrations
APPROVED

Ankita
6/19/2019 1:35:39 PM

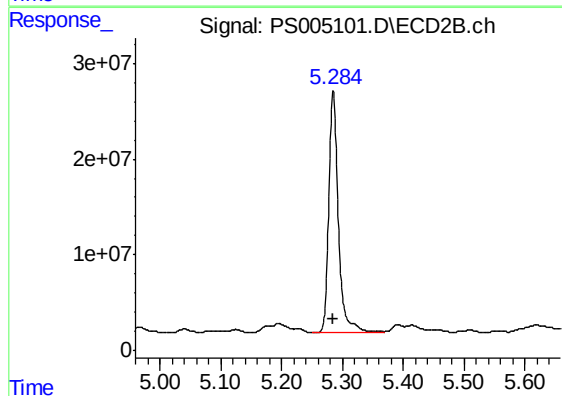

#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: 0.000 min
Response: 274618451
Conc: 275.30 ng/ml