

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
 Data File : PS010838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2020 20:33
 Operator : DD\AJ
 Sample : L2809-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-01-061720

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:47:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	267.3E6	202.7E6	337.979	371.650
Target Compounds							
1) T	Dalapon	2.995	2.584	33008766	123.6E6	33.573	168.804 #
2) T	3,5-DICHL...	0.000	6.100	0	70675205	N.D.	86.227
3) T	4-Nitroph...	6.997	0.000	3578029	0	9.651	N.D. #
5) T	DICAMBA	0.000	7.054	0	7330919	N.D.	3.257
7) T	MCPA	7.689	7.458	102.9E6	77658253	29.444	28.574
8) T	DICHLORPROP	0.000	7.739	0	15409858	N.D.	26.724
12) T	2,4,5-T	9.428	9.249	18998892	7558482	4.671	2.519 #
15) T	Picloram	10.994	0.000	15309444	0	2.999	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
Data File : PS010838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2020 20:33
Operator : DD\AJ
Sample : L2809-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HD-01-061720

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:47:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

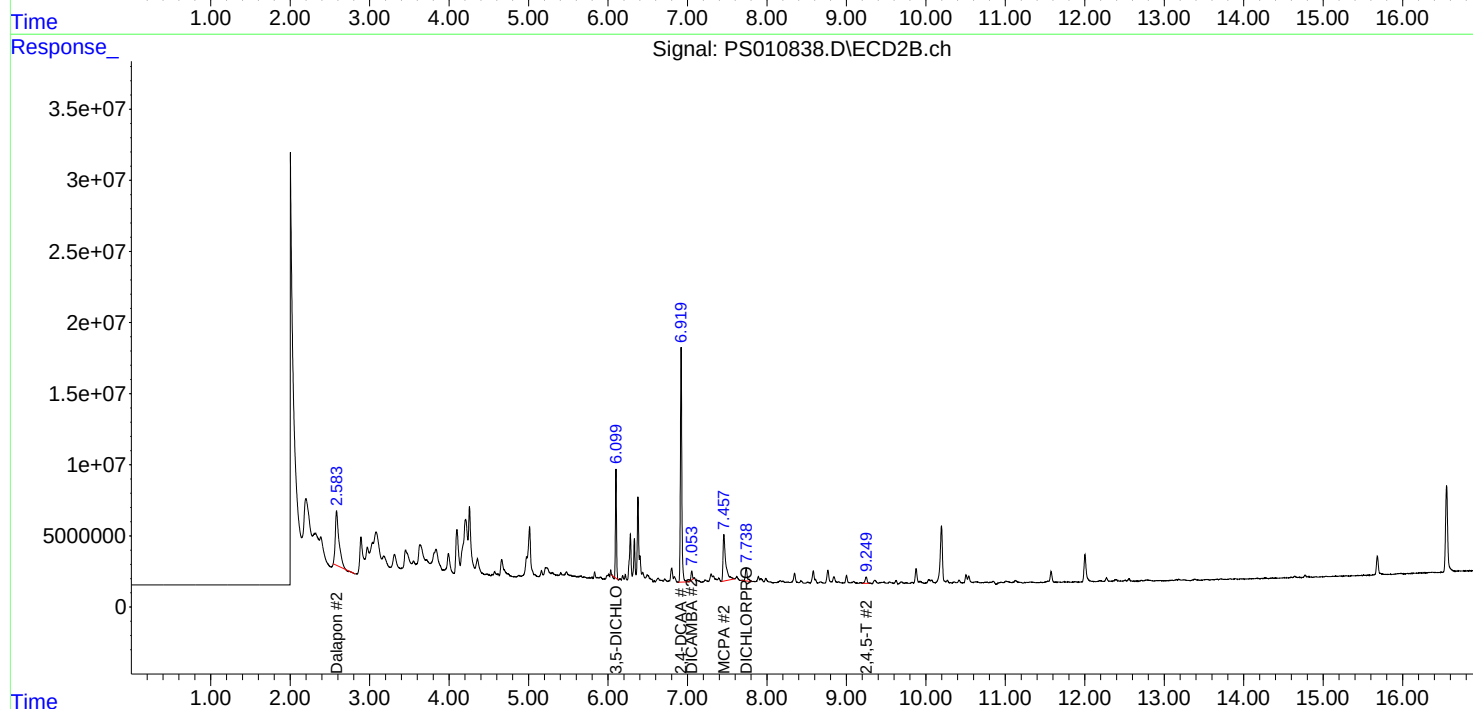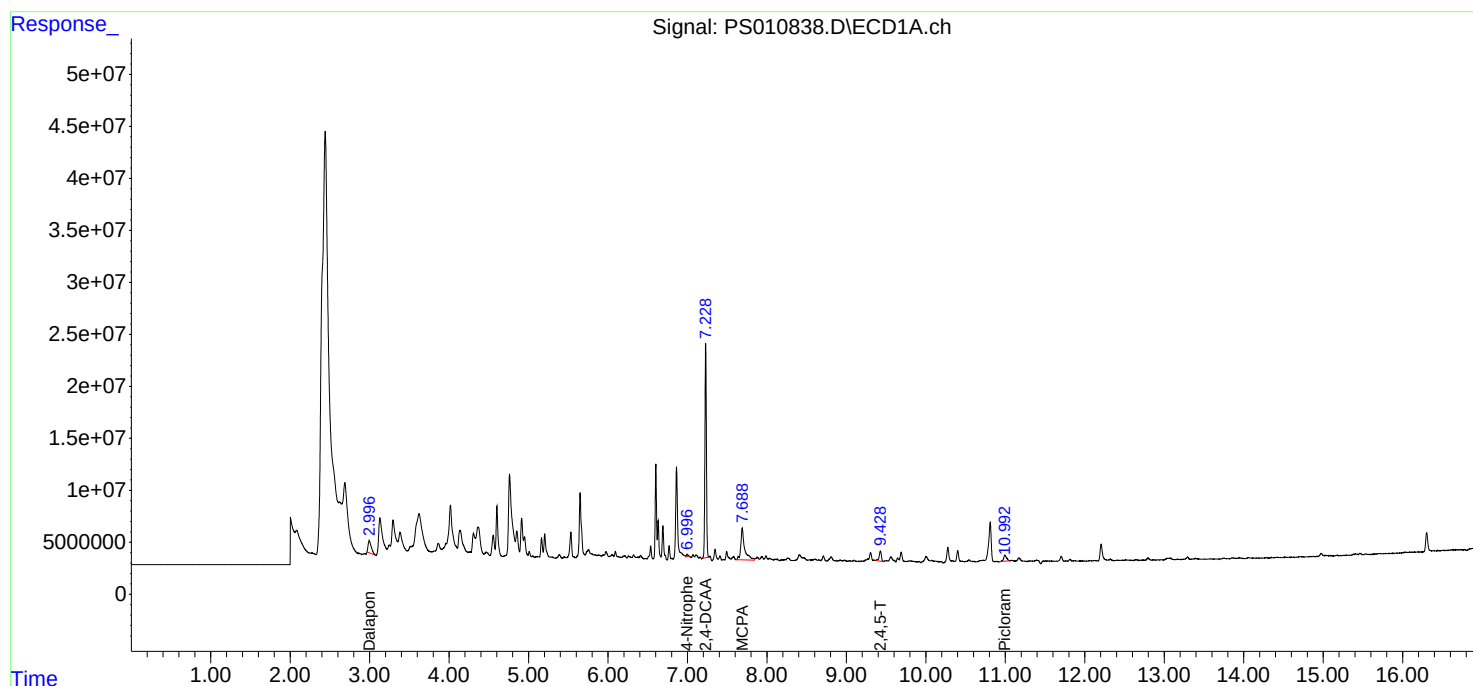


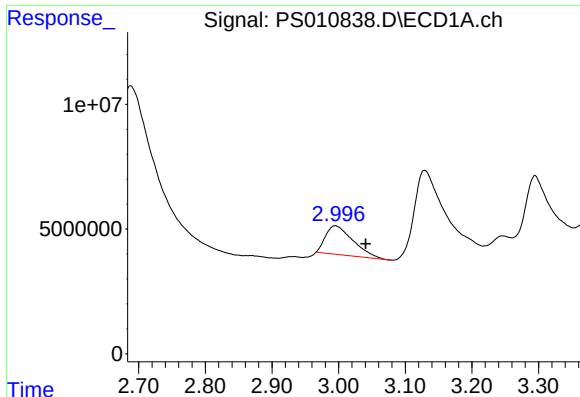

#1 Dalapon


R.T.: 2.995 min
Delta R.T.: -0.046 min
Response: 33008766
Conc: 33.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-061720

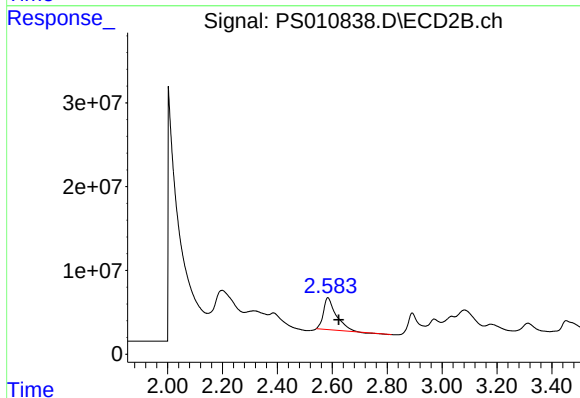


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.040 min
Response: 123589106
Conc: 168.80 ng/ml

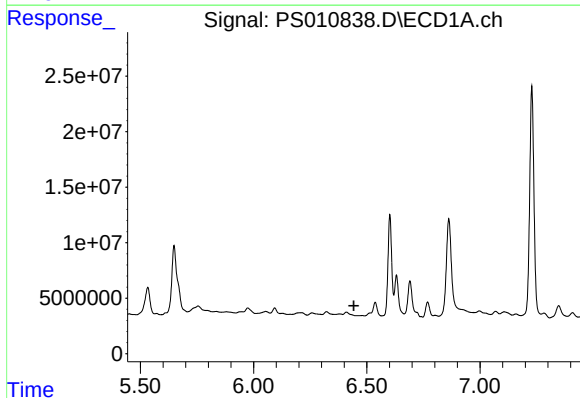


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

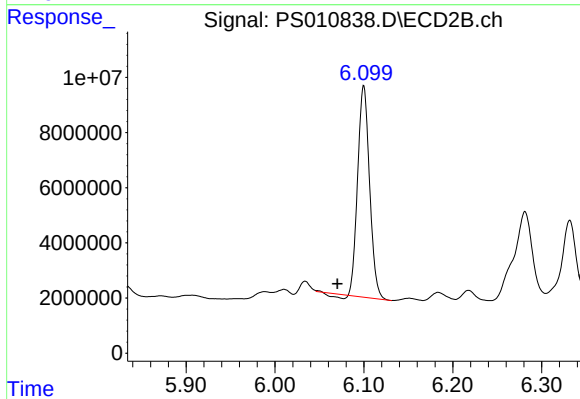

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 70675205
Conc: 86.23 ng/ml

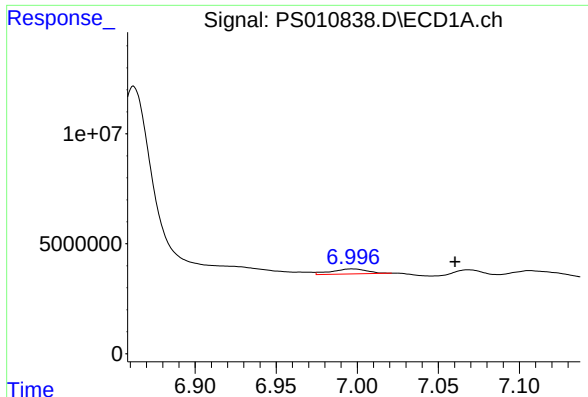

#3 4-Nitrophenol


R.T.: 6.997 min
Delta R.T.: -0.064 min
Response: 3578029
Conc: 9.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-061720

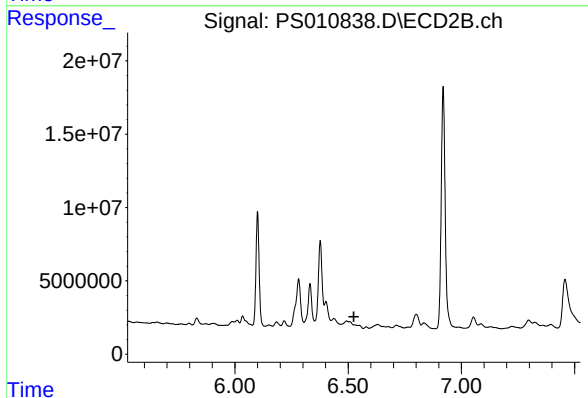


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

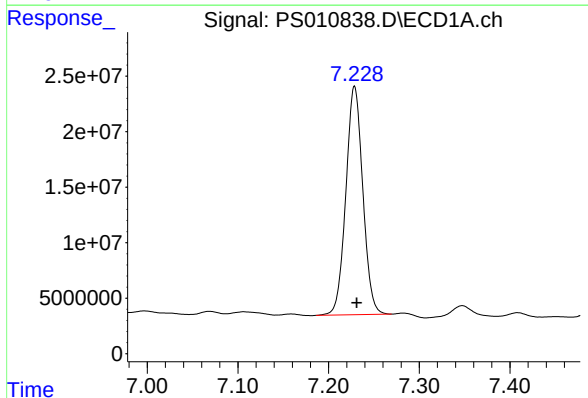


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: -0.002 min
Response: 267294655
Conc: 337.98 ng/ml

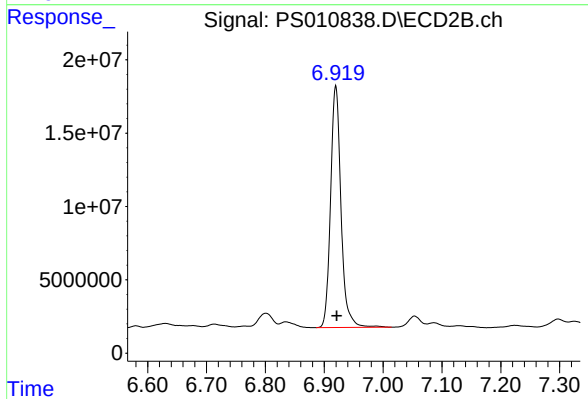

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 202703733
Conc: 371.65 ng/ml

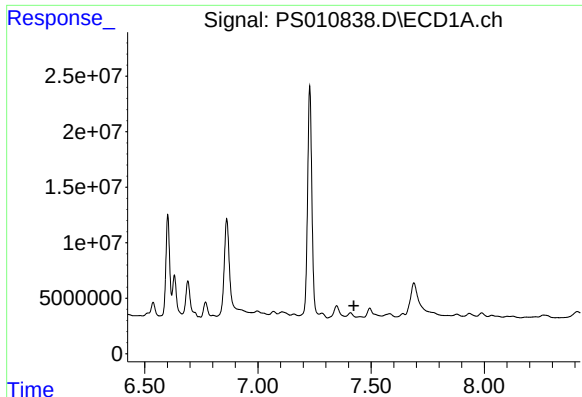

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-01-061720

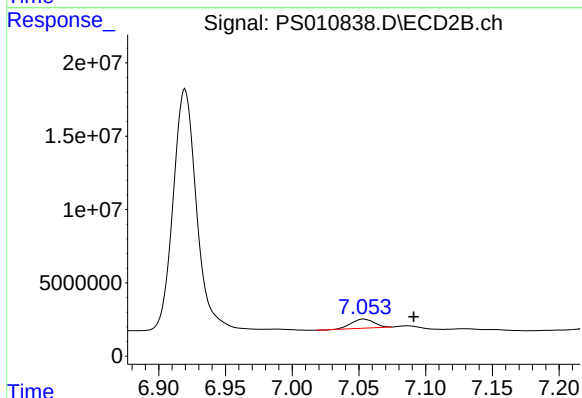


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 7330919
Conc: 3.26 ng/ml

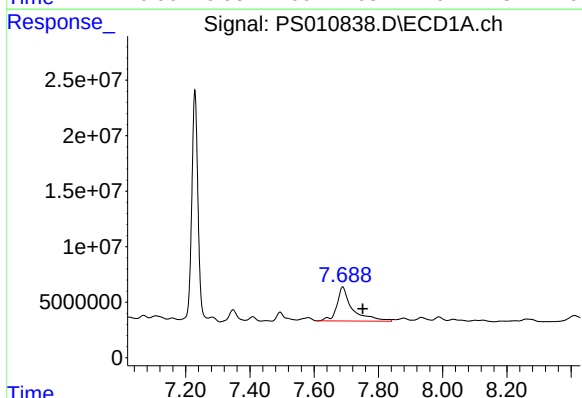


#7 MCPA

R.T.: 7.689 min
Delta R.T.: -0.062 min
Response: 102936931
Conc: 29.44 ug/ml

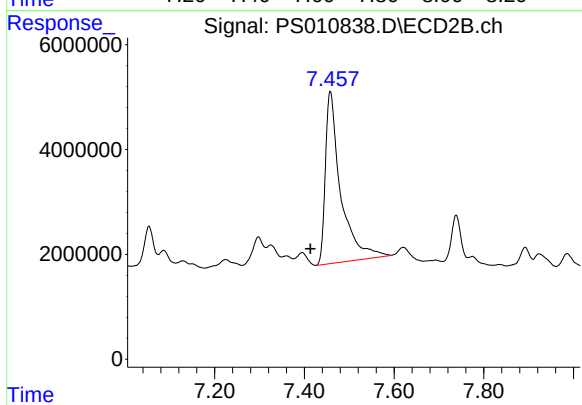

#7 MCPA


R.T.: 7.458 min
Delta R.T.: 0.044 min
Response: 77658253
Conc: 28.57 ug/ml

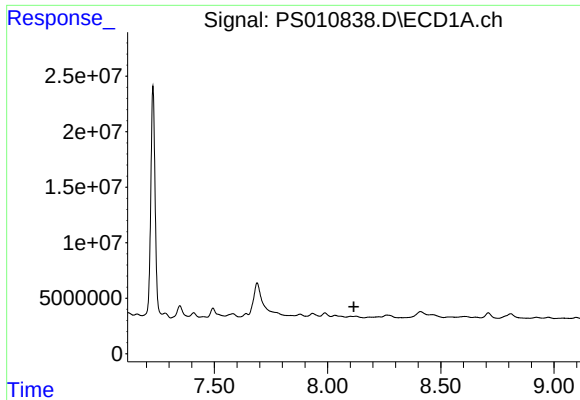

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-01-061720

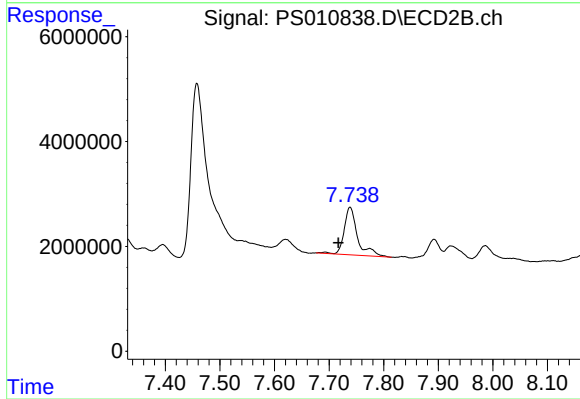


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.021 min
Response: 15409858
Conc: 26.72 ng/ml

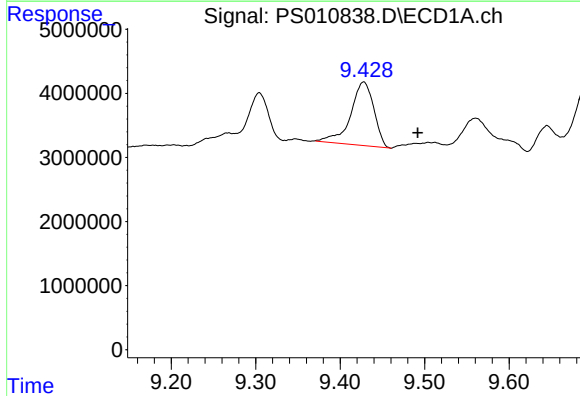


#12 2,4,5-T

R.T.: 9.428 min
Delta R.T.: -0.064 min
Response: 18998892
Conc: 4.67 ng/ml

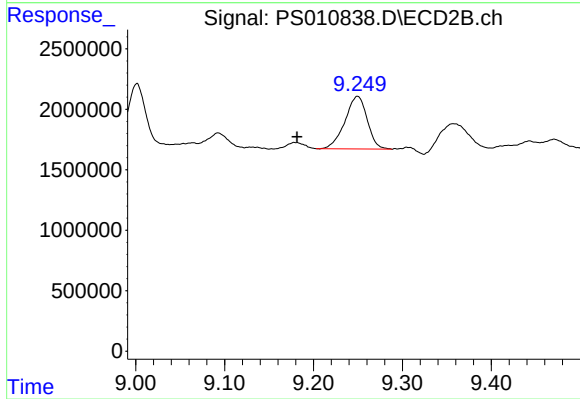

#12 2,4,5-T


R.T.: 9.249 min
Delta R.T.: 0.068 min
Response: 7558482
Conc: 2.52 ng/ml

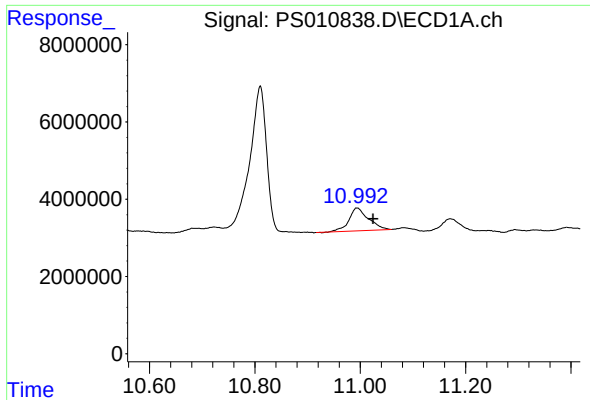

#15 Picloram

R.T.: 10.994 min
Delta R.T.: -0.030 min
Response: 15309444
Conc: 3.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-061720

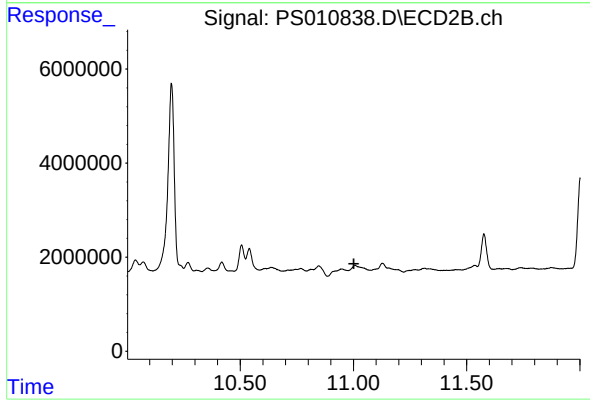

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.