

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
 Data File : PS010842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2020 22:05
 Operator : DD\AJ
 Sample : L2812-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-03-061720

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:49:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	405.2E6	292.1E6	512.356	535.536
Target Compounds							
1) T	Dalapon	2.994	2.586	36430587	138.6E6	37.053	189.319 #
2) T	3,5-DICHL...	0.000	6.100	0	72254850	N.D.	88.154
3) T	4-Nitroph...	6.996	0.000	4163235	0	11.230	N.D. #
5) T	DICAMBA	7.493	7.054	7286159	6678111	2.317	2.967 #
7) T	MCPA	7.687	7.456	114.4E6	103.6E6	32.733	38.128
8) T	DICHLORPROP	0.000	7.738	0	13998455	N.D.	24.276
10) T	Pentachlo...	8.709	0.000	7517185	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.785	0	52930858	N.D.	17.624
12) T	2,4,5-T	9.426	9.247	29177516	10985411	7.174	3.661 #
15) T	Picloram	10.997	0.000	25423484	0	4.980	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
Data File : PS010842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2020 22:05
Operator : DD\AJ
Sample : L2812-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
OK-03-061720

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:49:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

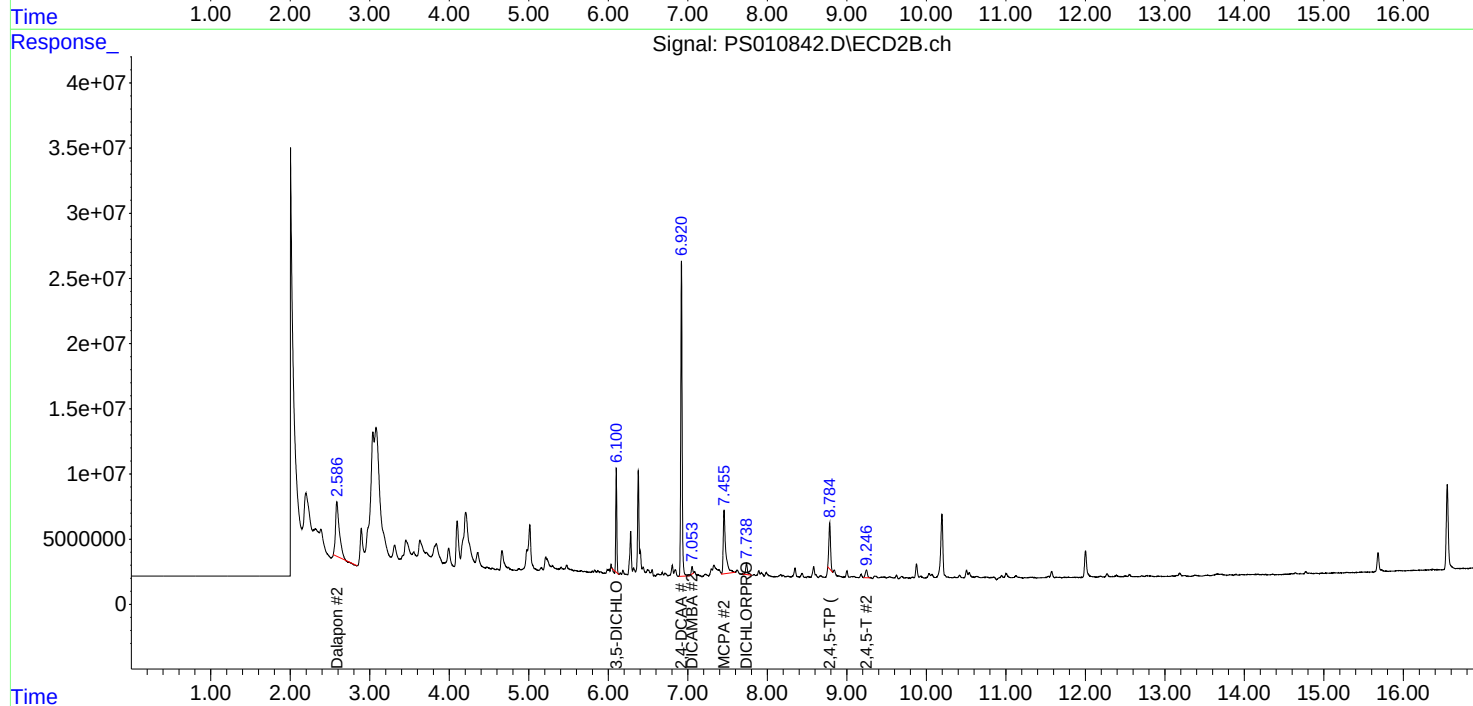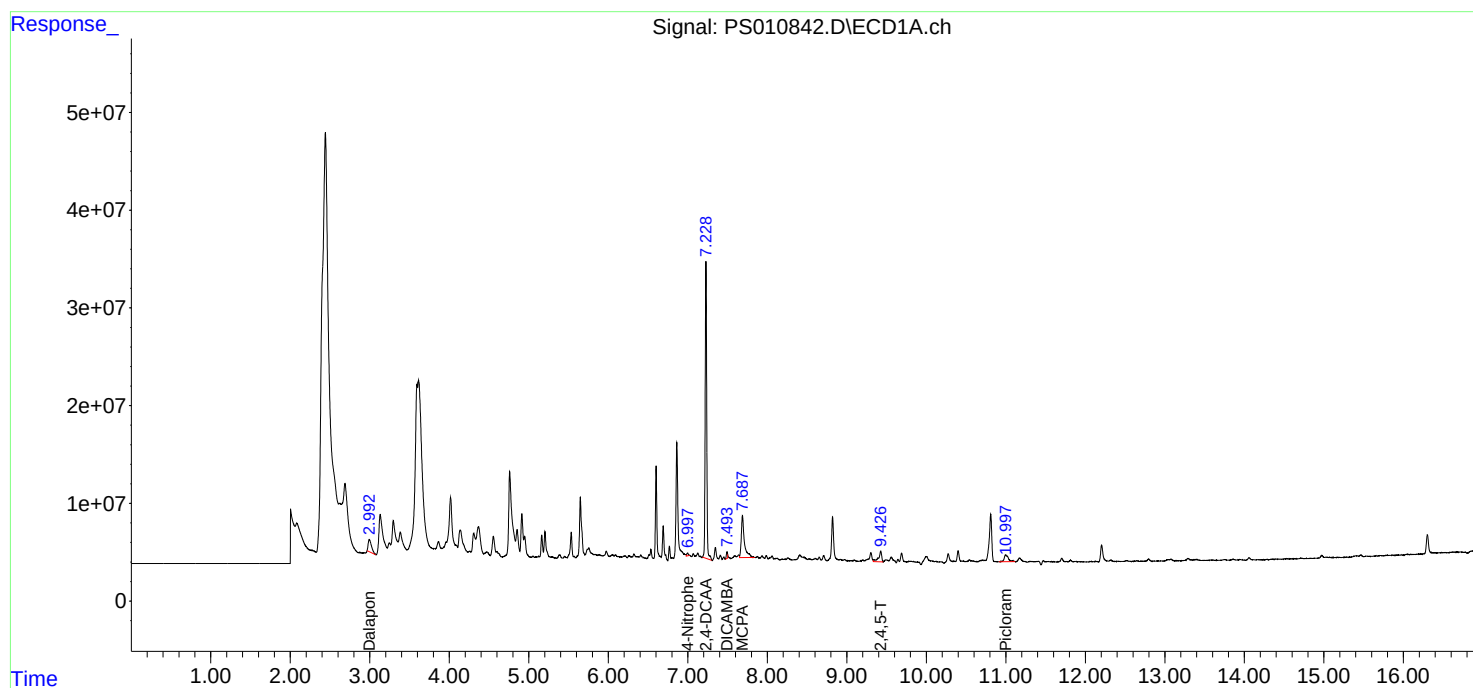


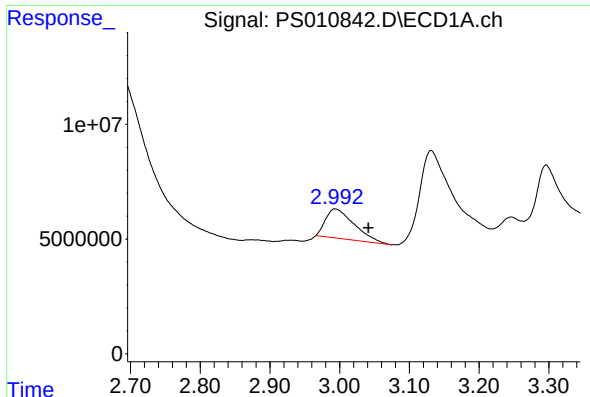

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.047 min
Response: 36430587
Conc: 37.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-061720

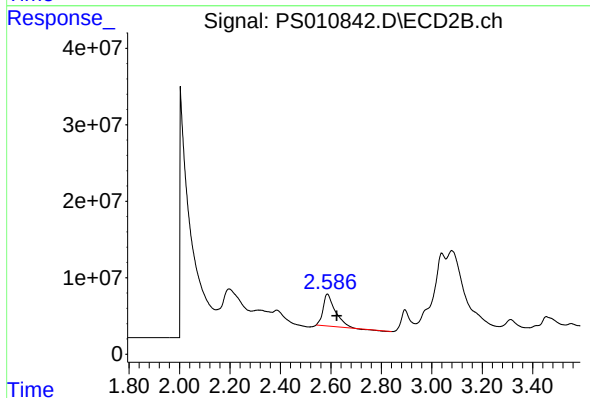


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.037 min
Response: 138608554
Conc: 189.32 ng/ml

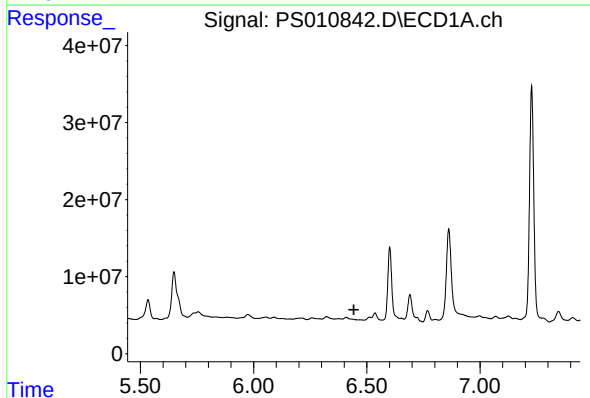


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

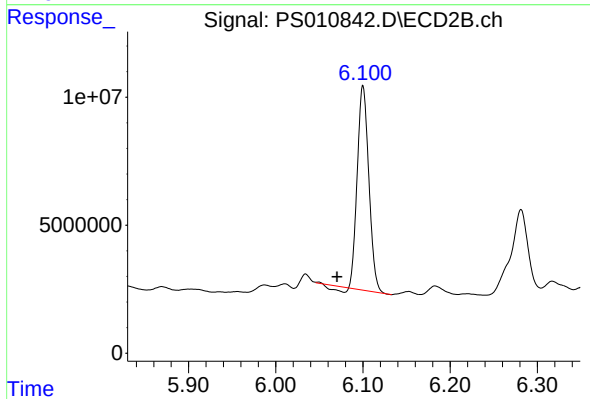

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 72254850
Conc: 88.15 ng/ml

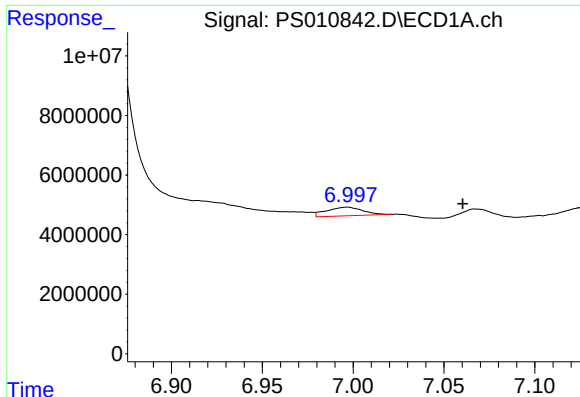

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.064 min
Response: 4163235
Conc: 11.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-061720

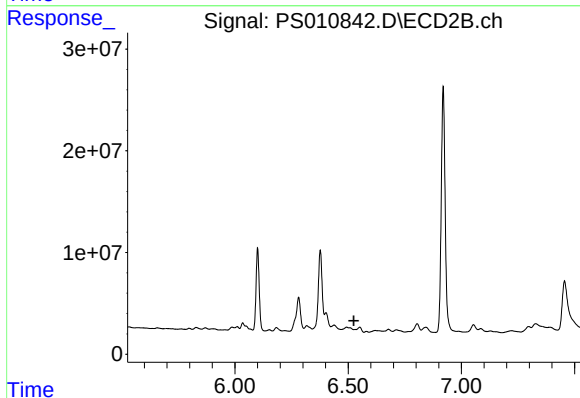


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

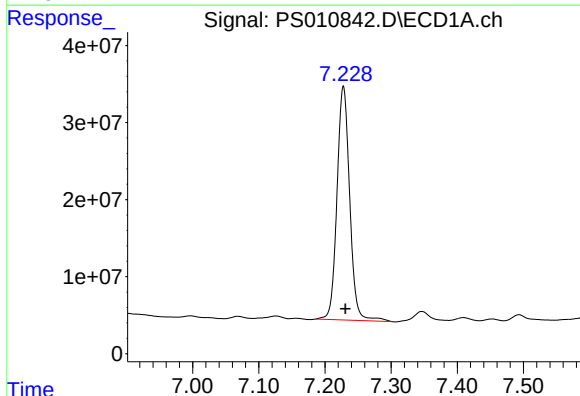


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 405203160
Conc: 512.36 ng/ml

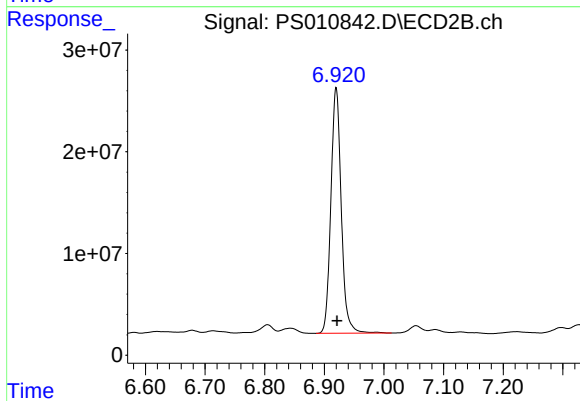

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 292089818
Conc: 535.54 ng/ml

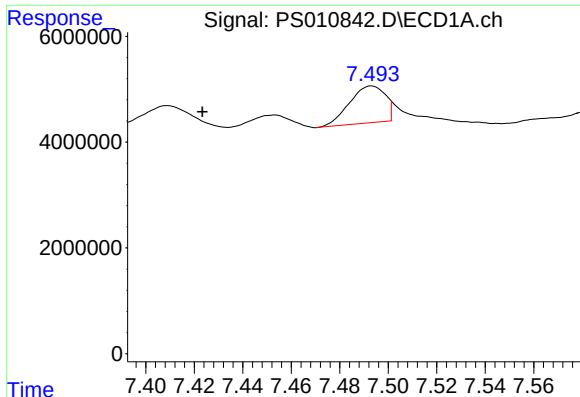

#5 DICAMBA


R.T.: 7.493 min
Delta R.T.: 0.070 min
Response: 7286159
Conc: 2.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-061720

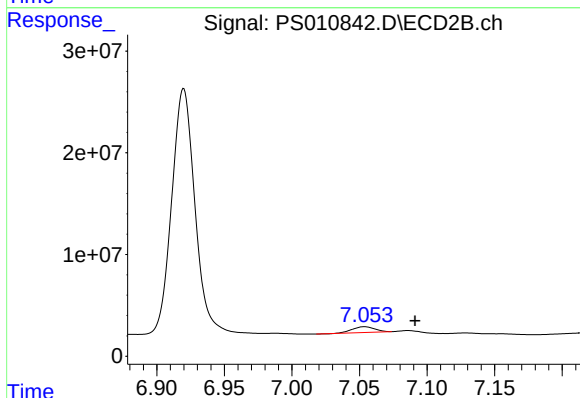


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 6678111
Conc: 2.97 ng/ml

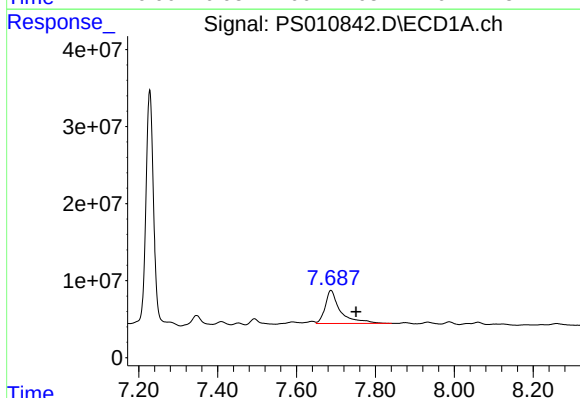


#7 MCPA

R.T.: 7.687 min
Delta R.T.: -0.064 min
Response: 114434436
Conc: 32.73 ug/ml

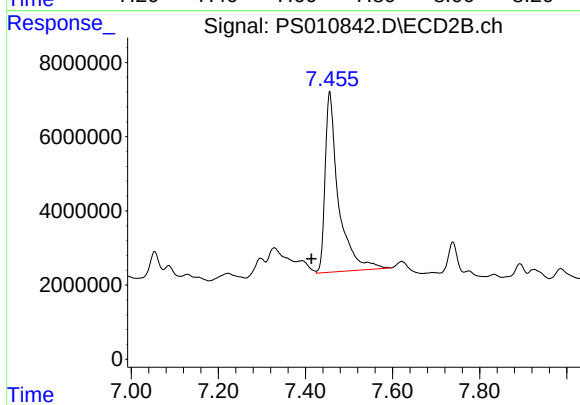

#7 MCPA


R.T.: 7.456 min
Delta R.T.: 0.042 min
Response: 103621436
Conc: 38.13 ug/ml

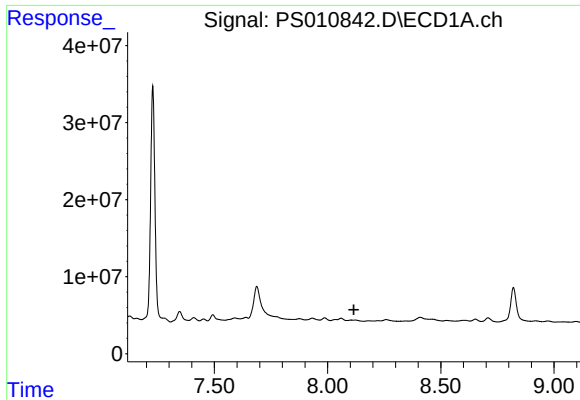

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-061720

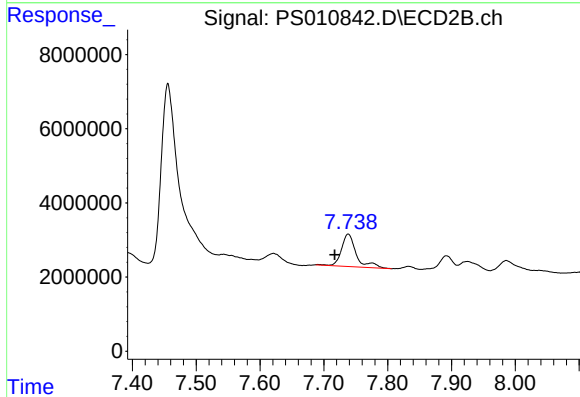


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.021 min
Response: 13998455
Conc: 24.28 ng/ml

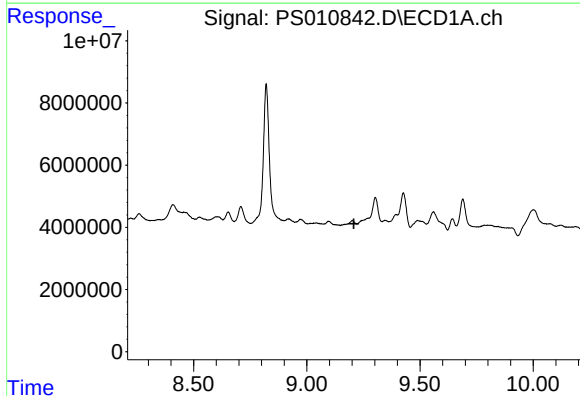


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

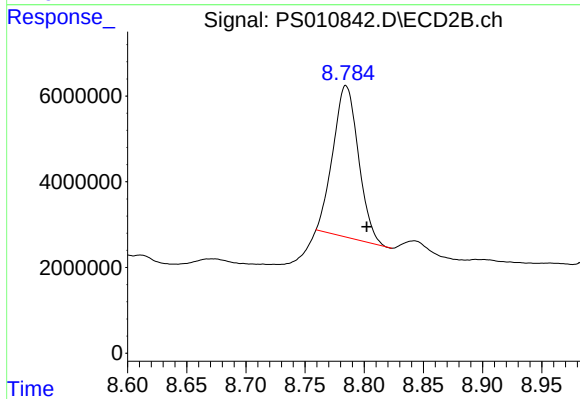

#11 2,4,5-TP (SILVEX)


R.T.: 8.785 min
Delta R.T.: -0.017 min
Response: 52930858
Conc: 17.62 ng/ml

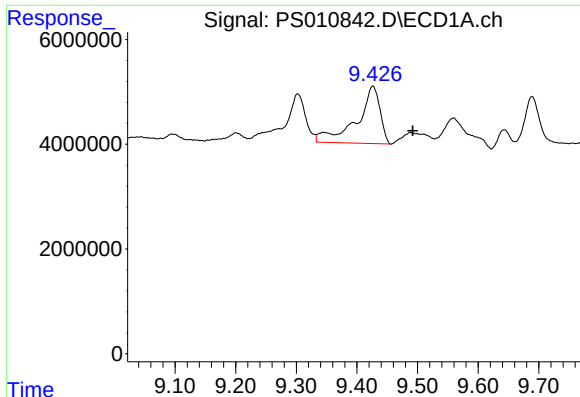

#12 2,4,5-T


R.T.: 9.426 min
Delta R.T.: -0.066 min
Response: 29177516
Conc: 7.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-061720

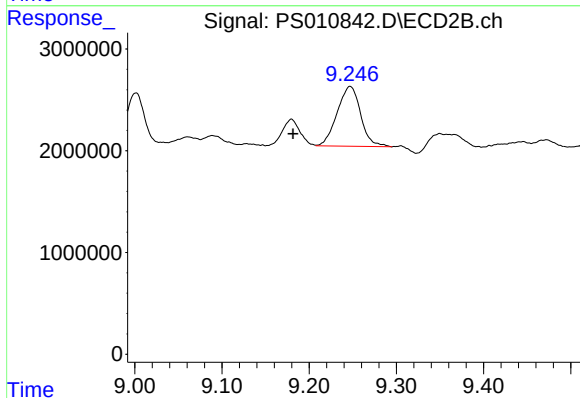


#12 2,4,5-T

R.T.: 9.247 min
Delta R.T.: 0.066 min
Response: 10985411
Conc: 3.66 ng/ml

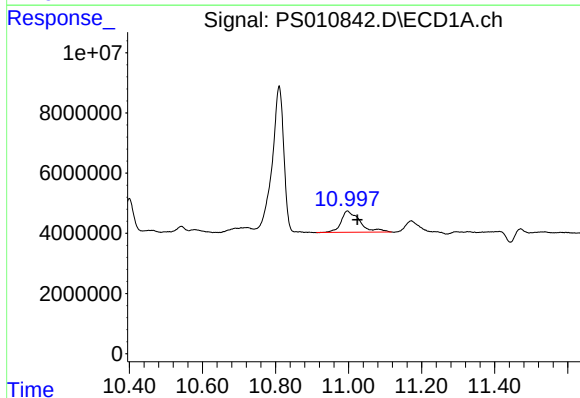

#15 Picloram

R.T.: 10.997 min
Delta R.T.: -0.027 min
Response: 25423484
Conc: 4.98 ng/ml

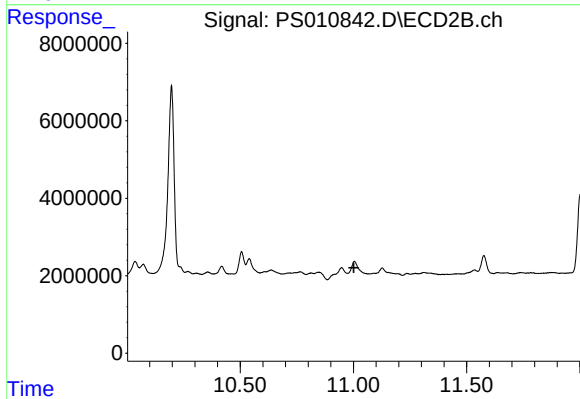

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.