

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
 Data File : PS010843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2020 22:27
 Operator : DD\AJ
 Sample : L2813-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-01-061720

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:49:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	236.8E6	165.4E6	299.366	303.177
Target Compounds							
1) T	Dalapon	2.994	2.585	30984368	88180211	31.514	120.441 #
2) T	3,5-DICHL...	0.000	6.100	0	53190097	N.D.	64.894
3) T	4-Nitroph...	6.997	6.552	4456970	6287522	12.022	18.980 #
5) T	DICAMBA	7.493	7.054	5458034	6291153	1.736	2.795 #
7) T	MCPA	7.687	7.455	153.1E6	133.4E6	43.780	49.093
8) T	DICHLORPROP	8.060	7.739	6531143	12646768	8.617	21.932 #
11) T	2,4,5-TP ...	0.000	8.783	0	14408952	N.D.	4.798
12) T	2,4,5-T	9.427	0.000	29944809	0	7.363	N.D. #
15) T	Picloram	10.996	0.000	12322718	0	2.414	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
Data File : PS010843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2020 22:27
Operator : DD\AJ
Sample : L2813-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
EO-01-061720

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:49:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

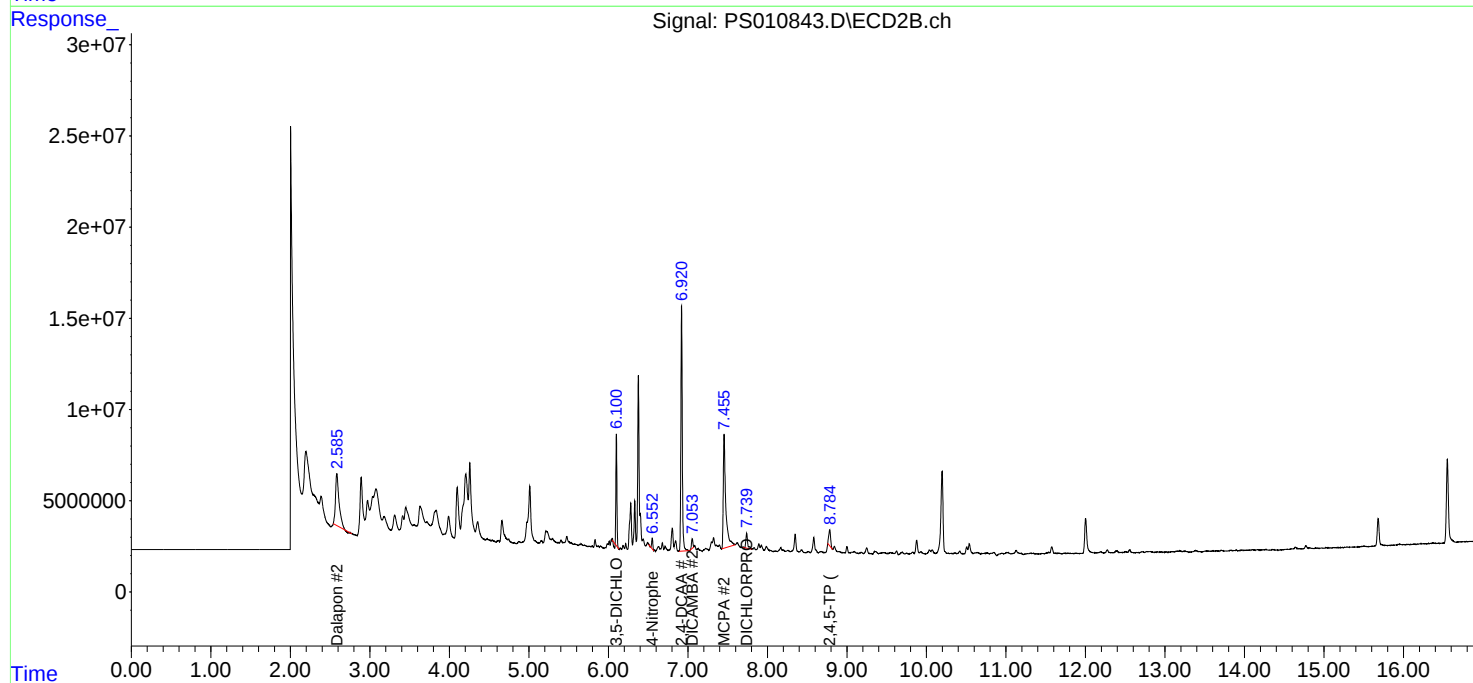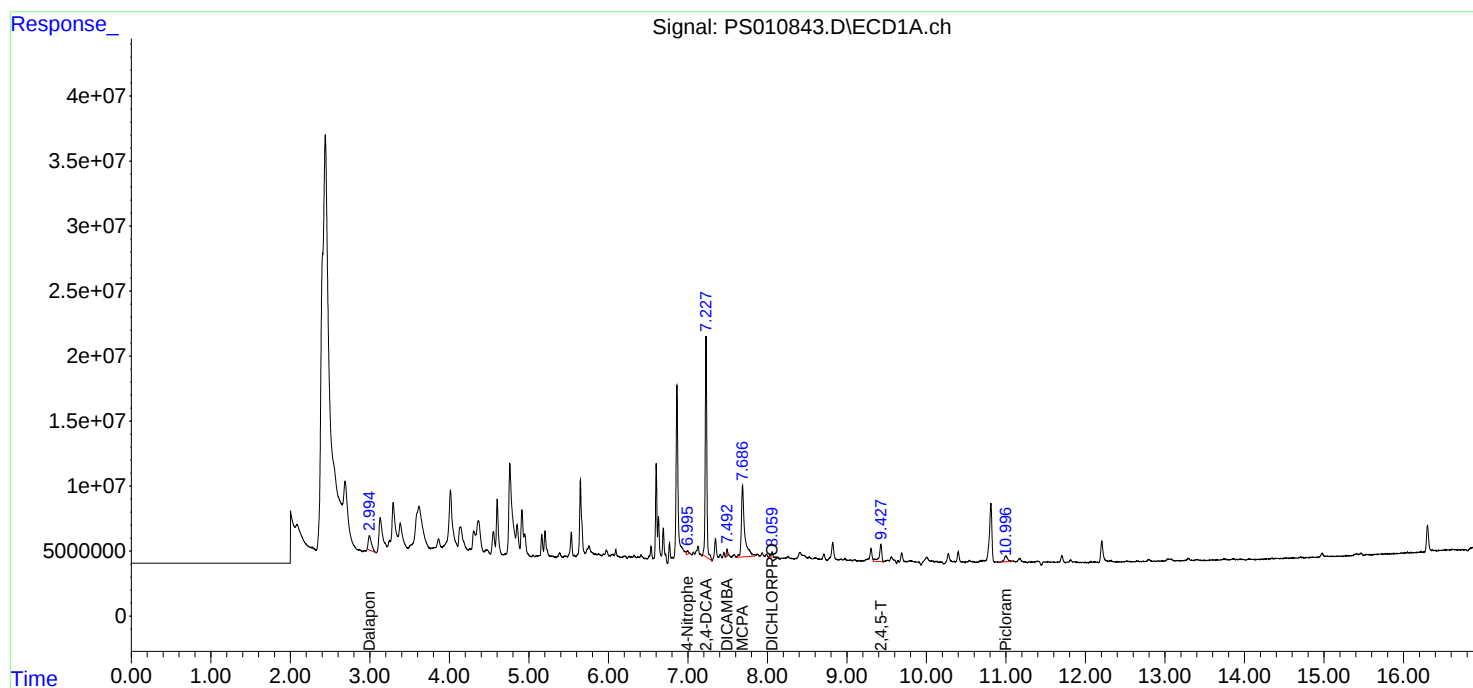


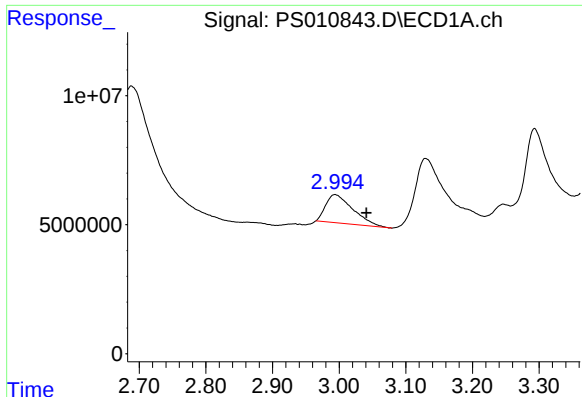

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.047 min
Response: 30984368
Conc: 31.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-061720

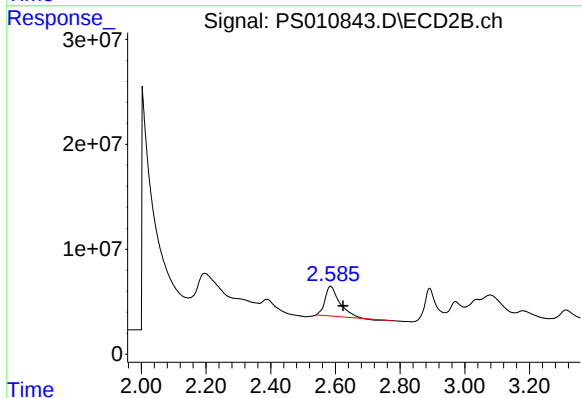


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.039 min
Response: 88180211
Conc: 120.44 ng/ml

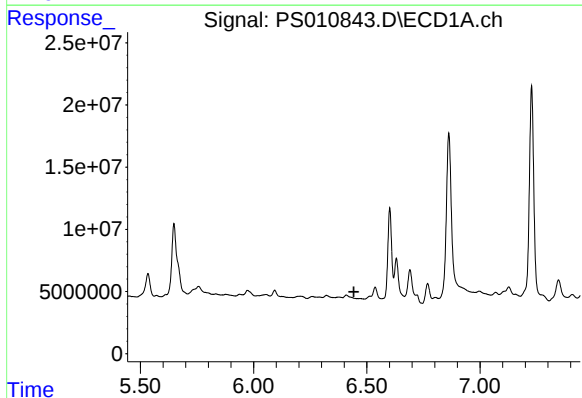


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

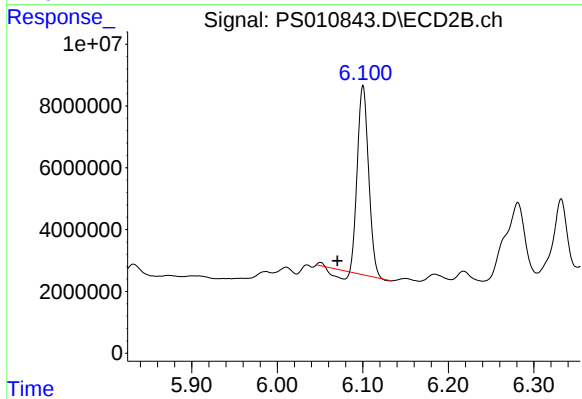

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 53190097
Conc: 64.89 ng/ml

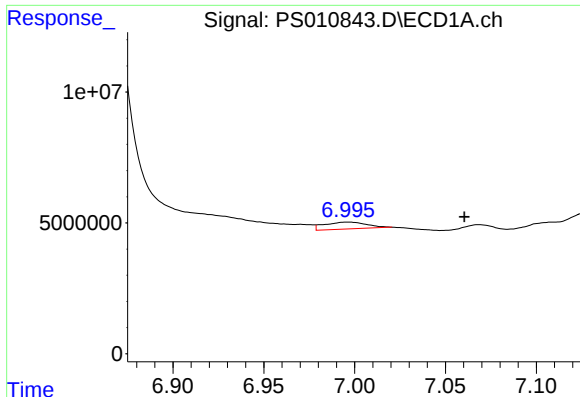

#3 4-Nitrophenol


R.T.: 6.997 min
Delta R.T.: -0.064 min
Response: 4456970
Conc: 12.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-061720

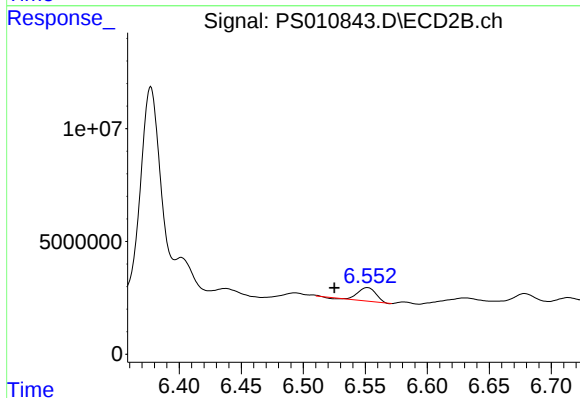


#3 4-Nitrophenol

R.T.: 6.552 min
Delta R.T.: 0.026 min
Response: 6287522
Conc: 18.98 ng/ml

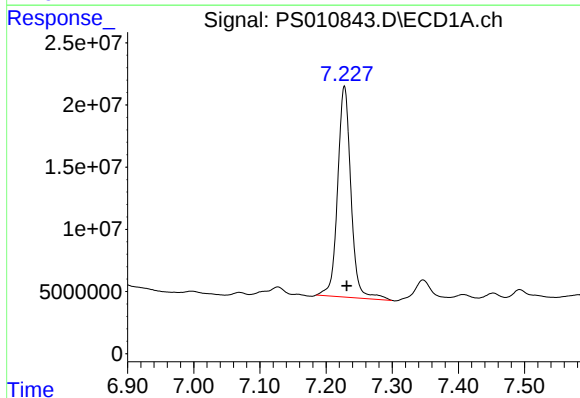


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 236756781
Conc: 299.37 ng/ml

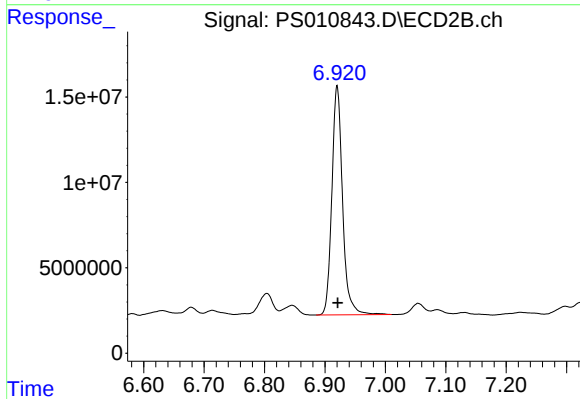

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 165357751
Conc: 303.18 ng/ml

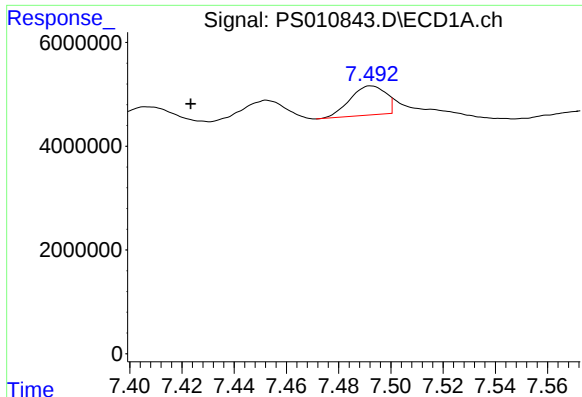

#5 DICAMBA


R.T.: 7.493 min
Delta R.T.: 0.069 min
Response: 5458034
Conc: 1.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-061720

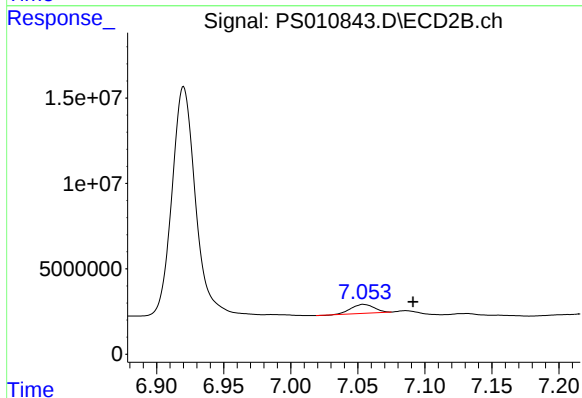


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 6291153
Conc: 2.80 ng/ml

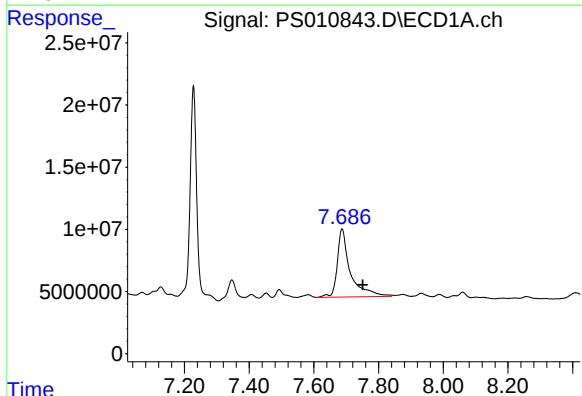


#7 MCPA

R.T.: 7.687 min
Delta R.T.: -0.064 min
Response: 153054331
Conc: 43.78 ug/ml

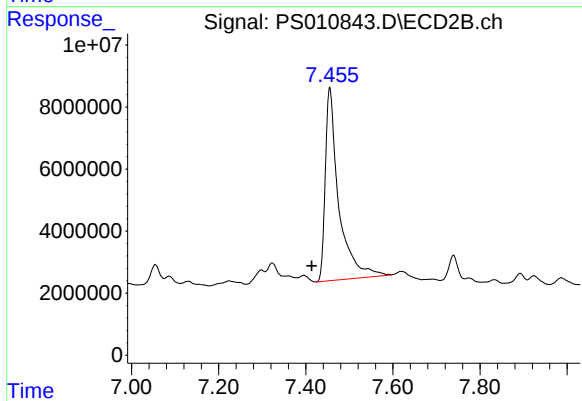

#7 MCPA


R.T.: 7.455 min
Delta R.T.: 0.041 min
Response: 133423144
Conc: 49.09 ug/ml

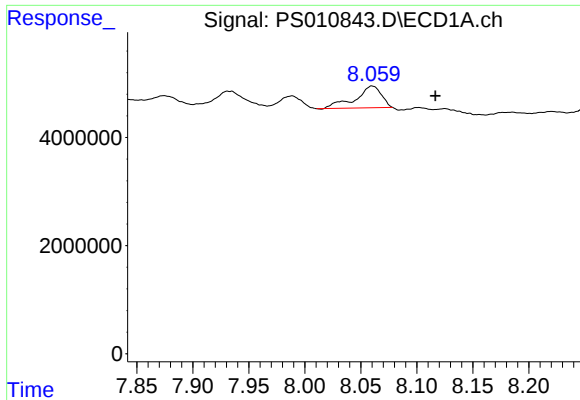

#8 DICHLORPROP


R.T.: 8.060 min
Delta R.T.: -0.056 min
Response: 6531143
Conc: 8.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-061720

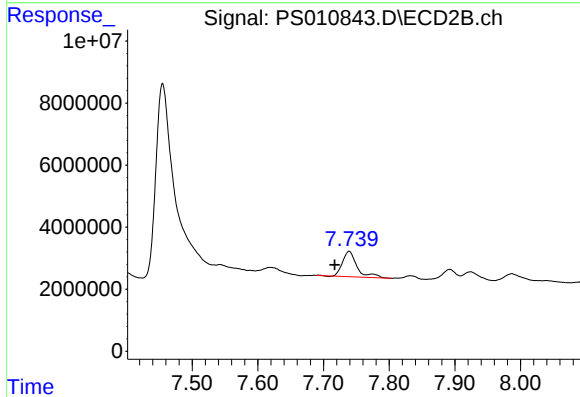


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.022 min
Response: 12646768
Conc: 21.93 ng/ml

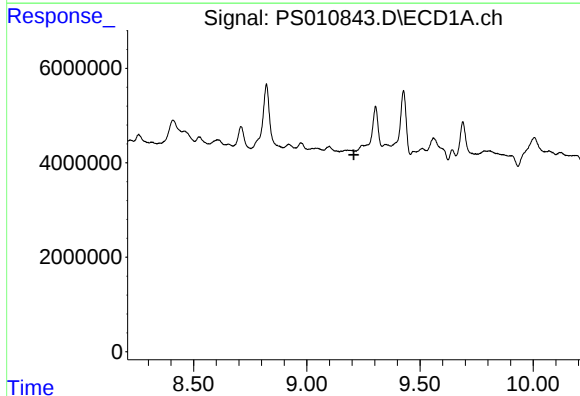


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

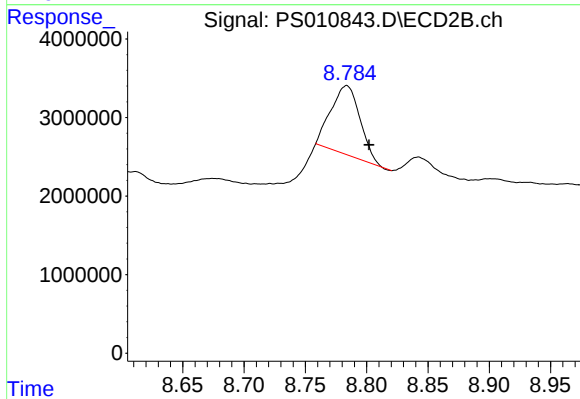

#11 2,4,5-TP (SILVEX)


R.T.: 8.783 min
Delta R.T.: -0.019 min
Response: 14408952
Conc: 4.80 ng/ml

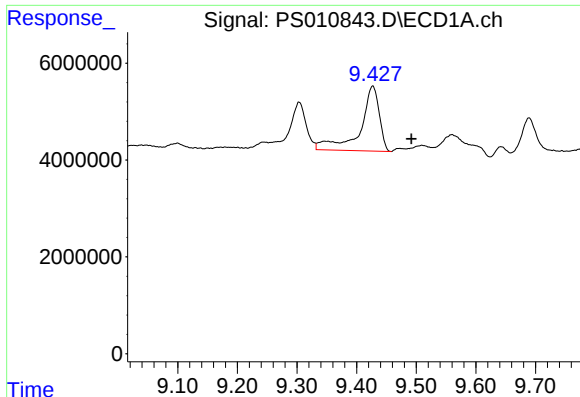

#12 2,4,5-T


R.T.: 9.427 min
Delta R.T.: -0.065 min
Response: 29944809
Conc: 7.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-061720

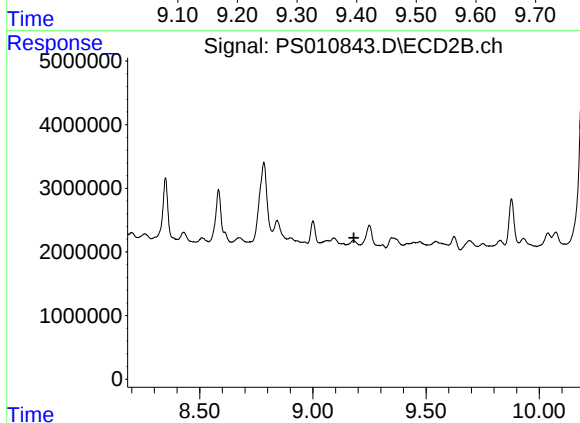


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.181 min
Response: 0
Conc: N.D.

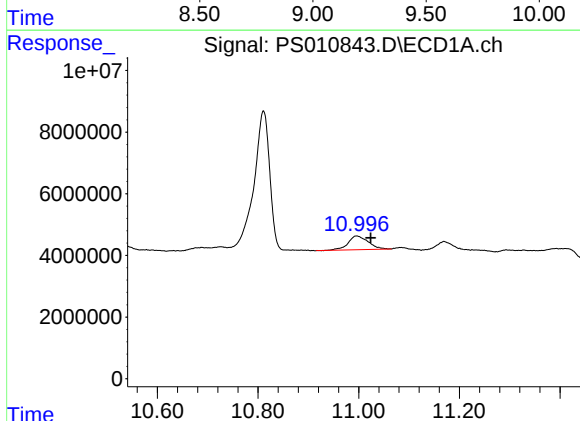

#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.028 min
Response: 12322718
Conc: 2.41 ng/ml

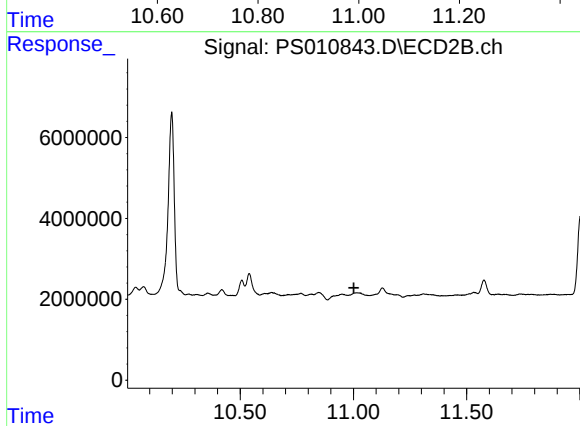

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.