

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
 Data File : PS010844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2020 22:50
 Operator : DD\AJ
 Sample : L2817-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-04-061720

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:49:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	294.7E6	208.0E6	372.624	381.322
Target Compounds							
1) T	Dalapon	2.993	2.585	36211761	144.4E6	36.831	197.195 #
2) T	3,5-DICHL...	0.000	6.100	0	68031463	N.D.	83.001
3) T	4-Nitroph...	6.997	0.000	3786301	0	10.213	N.D. #
5) T	DICAMBA	7.493	7.053	7346764	12927060	2.336	5.743 #
7) T	MCPA	7.687	7.455	150.2E6	137.6E6	42.961	50.629
8) T	DICHLORPROP	0.000	7.738	0	18873674	N.D.	32.731
10) T	Pentachlo...	8.709	0.000	7758556	0	<MDL	N.D. #
12) T	2,4,5-T	9.426	0.000	19246490	0	4.732	N.D. #
15) T	Picloram	10.995	0.000	14142635	0	2.770	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
Data File : PS010844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2020 22:50
Operator : DD\AJ
Sample : L2817-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-04-061720

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:49:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

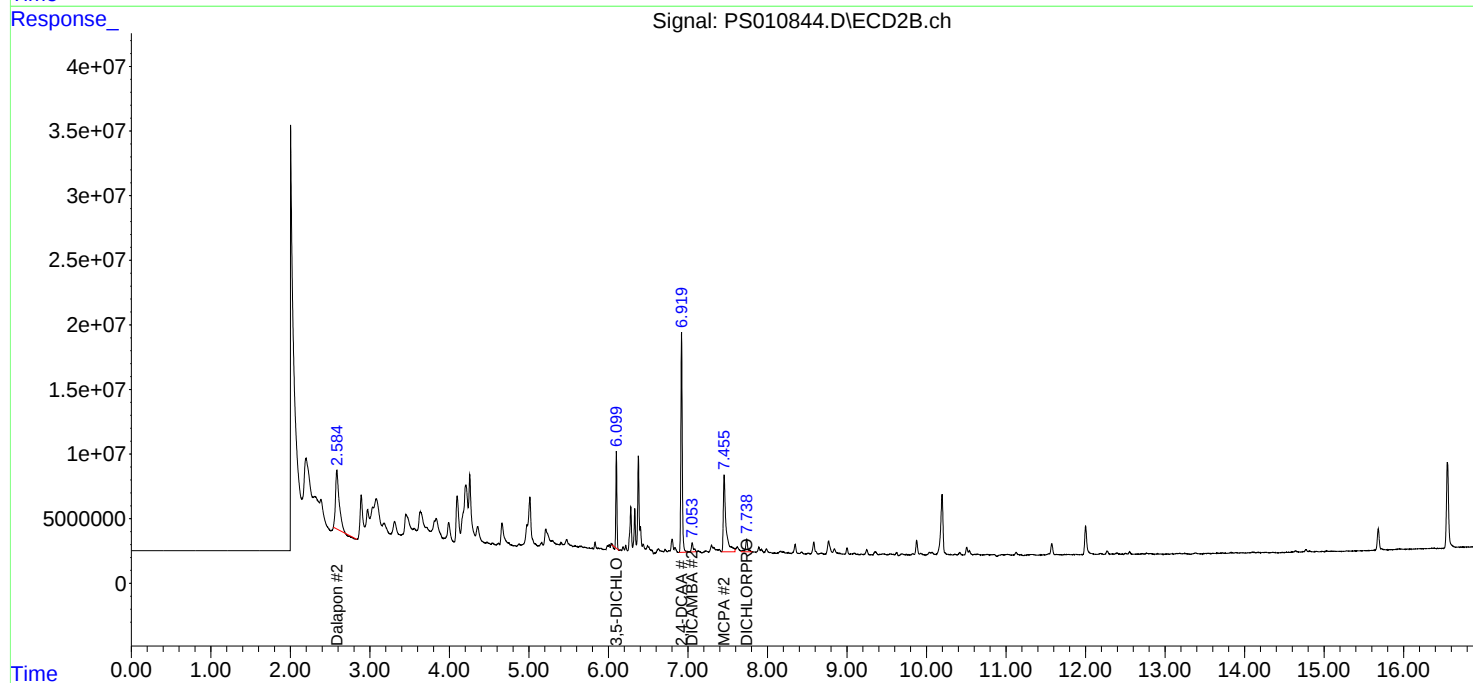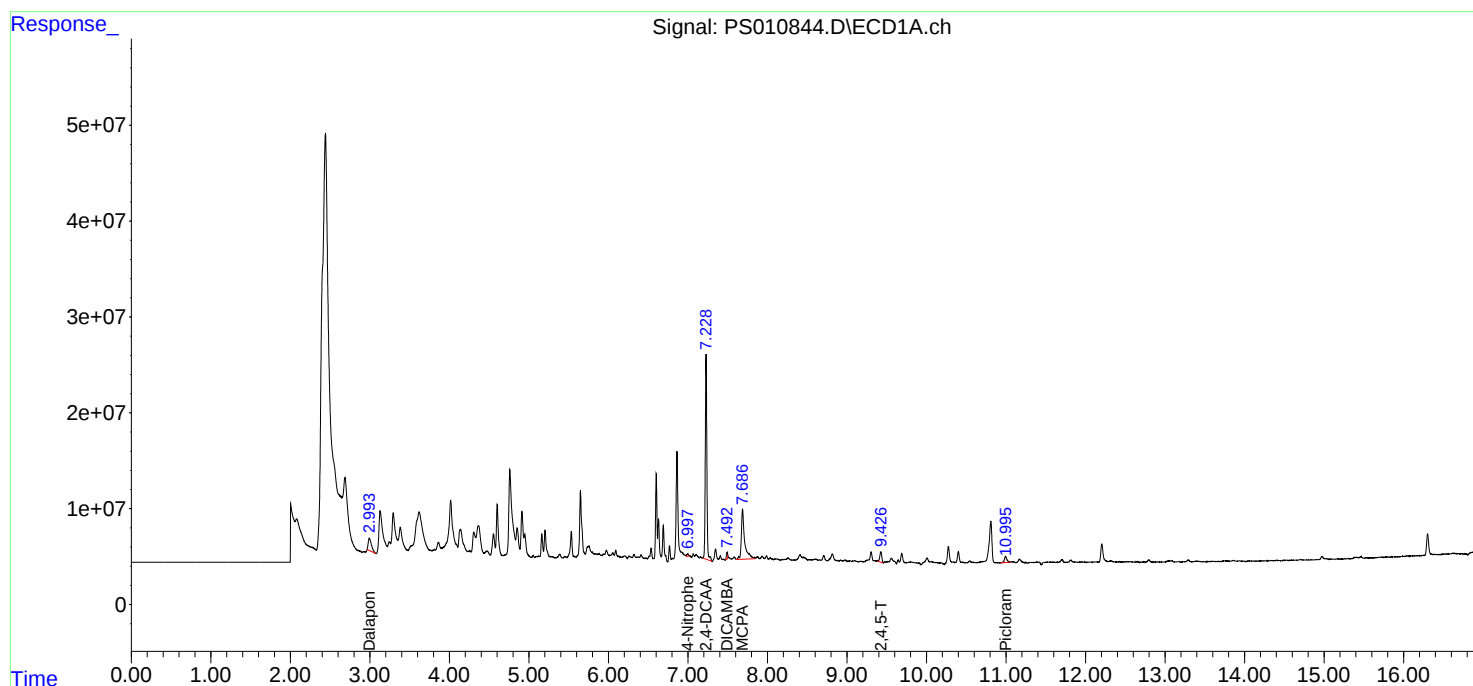


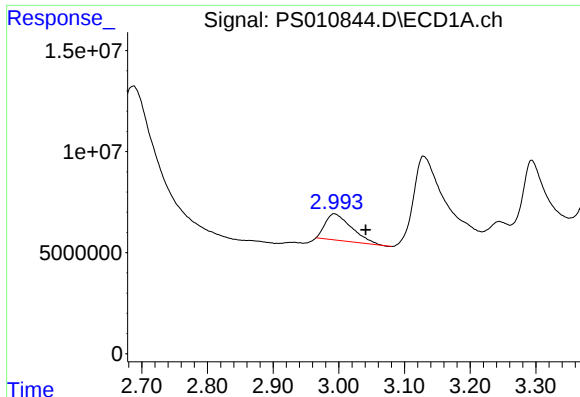

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.048 min
Response: 36211761
Conc: 36.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-061720

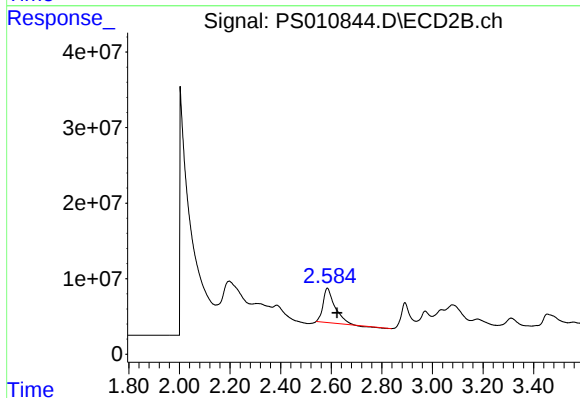


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.039 min
Response: 144374905
Conc: 197.19 ng/ml

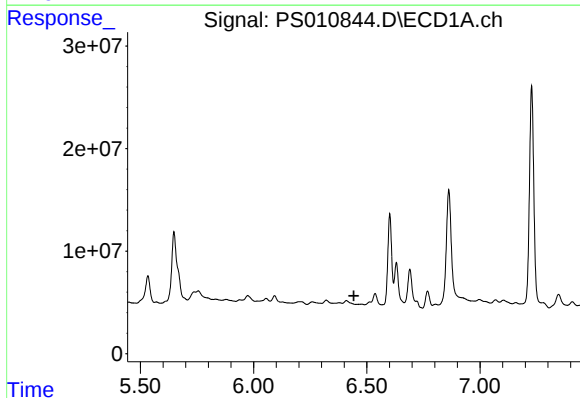


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

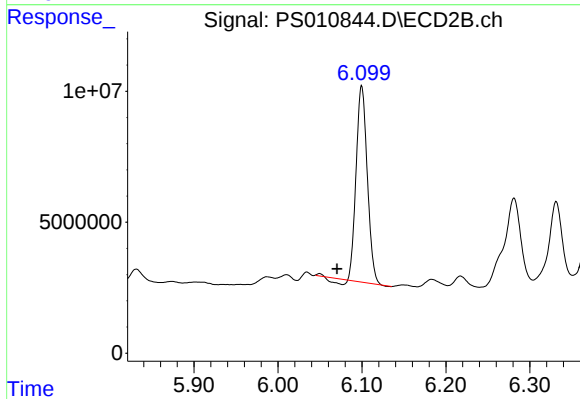

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 68031463
Conc: 83.00 ng/ml

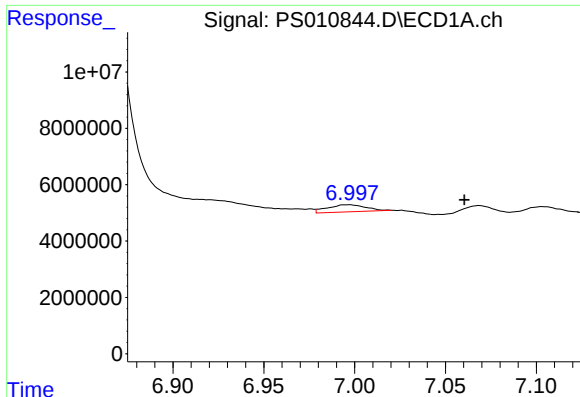

#3 4-Nitrophenol


R.T.: 6.997 min
Delta R.T.: -0.064 min
Response: 3786301
Conc: 10.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-061720

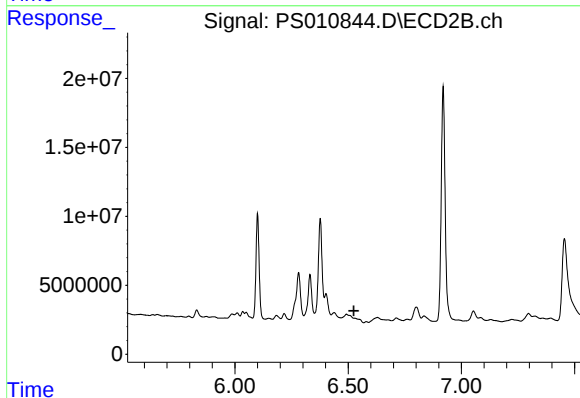


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

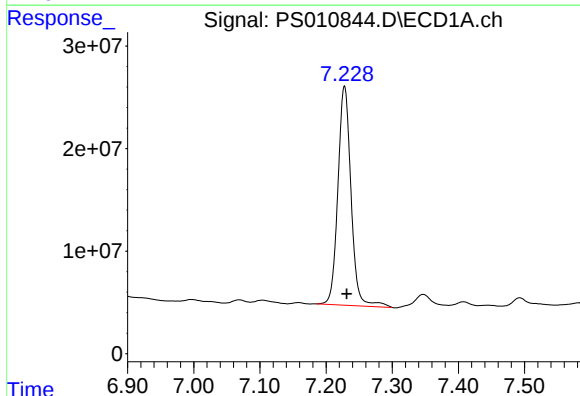


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 294694313
Conc: 372.62 ng/ml

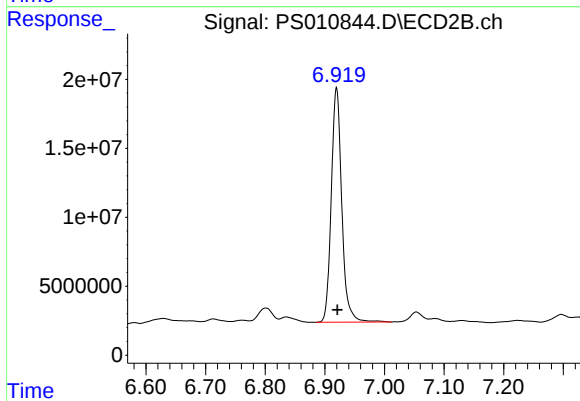

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 207979274
Conc: 381.32 ng/ml

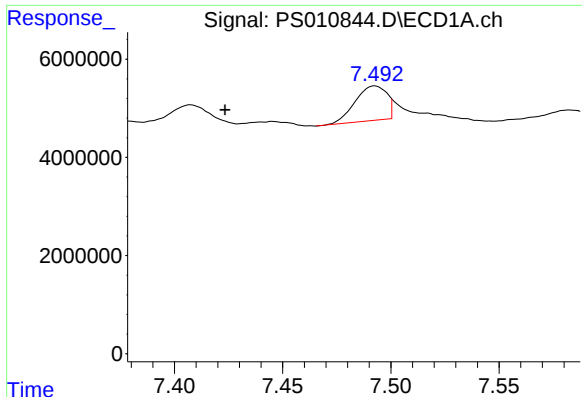

#5 DICAMBA


R.T.: 7.493 min
Delta R.T.: 0.069 min
Response: 7346764
Conc: 2.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-061720

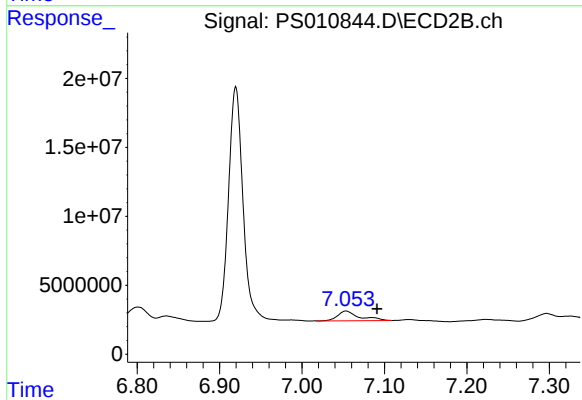


#5 DICAMBA

R.T.: 7.053 min
Delta R.T.: -0.038 min
Response: 12927060
Conc: 5.74 ng/ml

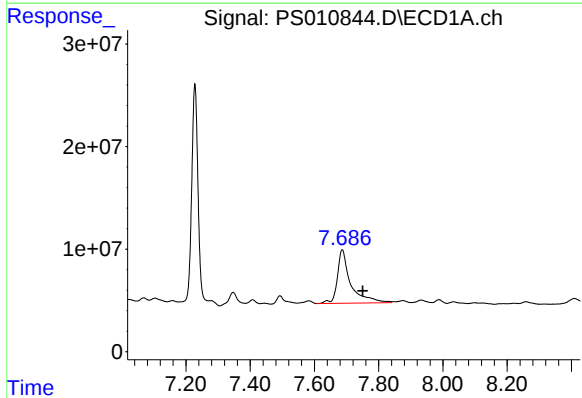


#7 MCPA

R.T.: 7.687 min
Delta R.T.: -0.064 min
Response: 150190836
Conc: 42.96 ug/ml

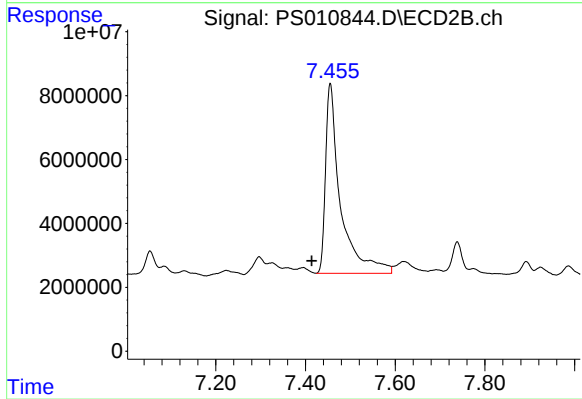

#7 MCPA


R.T.: 7.455 min
Delta R.T.: 0.042 min
Response: 137597751
Conc: 50.63 ug/ml

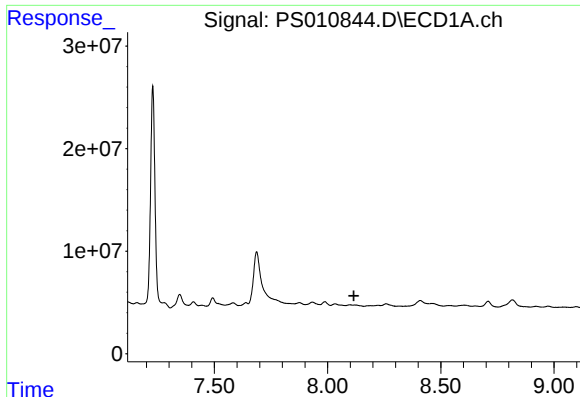

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-04-061720

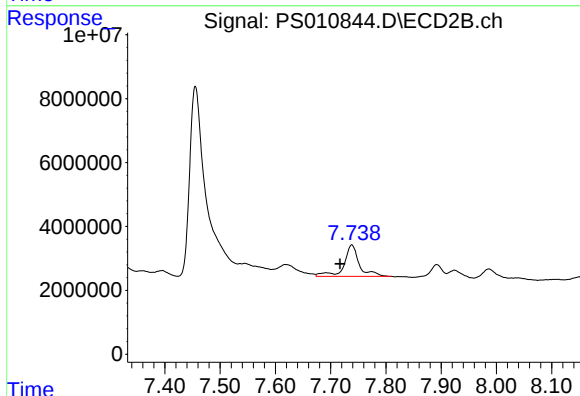


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.021 min
Response: 18873674
Conc: 32.73 ng/ml

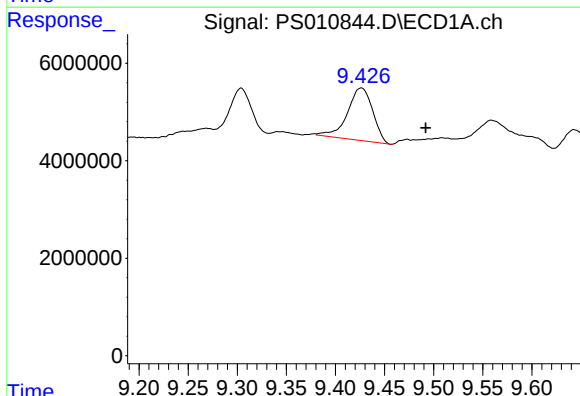


#12 2,4,5-T

R.T.: 9.426 min
Delta R.T.: -0.066 min
Response: 19246490
Conc: 4.73 ng/ml

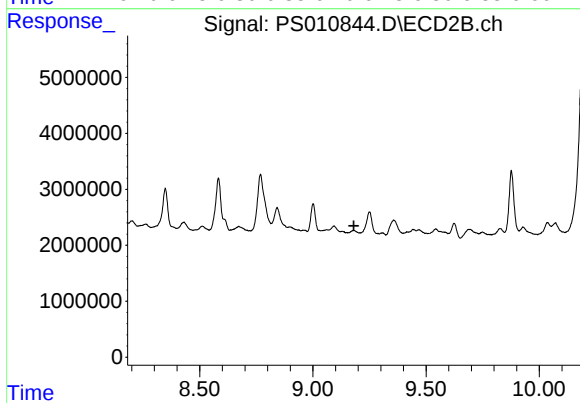

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

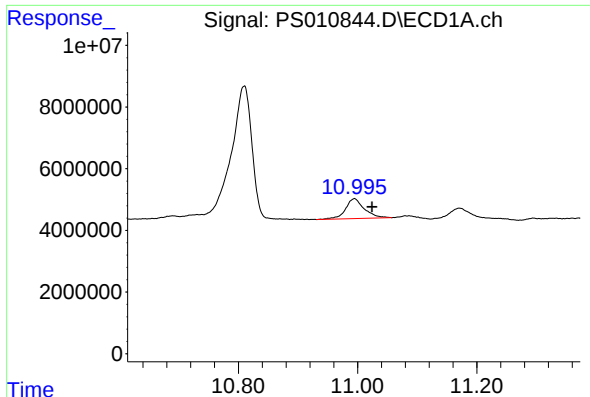

#15 Picloram

R.T.: 10.995 min
Delta R.T.: -0.029 min
Response: 14142635
Conc: 2.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-061720

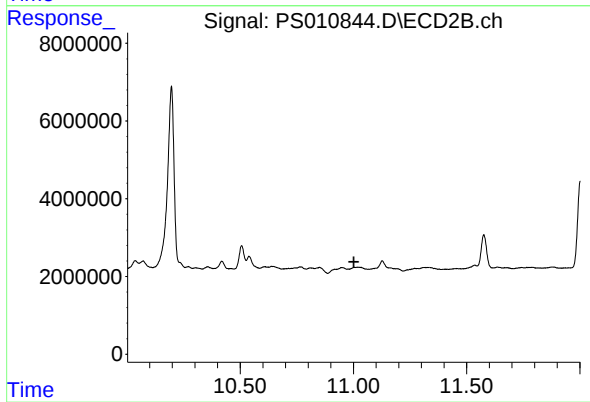

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.