

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
 Data File : PS010849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 00:45
 Operator : DD\AJ
 Sample : L3024-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:51:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	279.6E6	200.9E6	353.483	368.398
Target Compounds							
1) T	Dalapon	2.994	2.584	32036574	113.5E6	32.584	155.077 #
2) T	3,5-DICHL...	0.000	6.100	0	69644478	N.D.	84.969
3) T	4-Nitroph...	6.997	0.000	5080418	0	13.704	N.D. #
5) T	DICAMBA	7.493	7.054	4350859	6424644	1.384	2.854 #
7) T	MCPA	7.688	7.459	91798344	84280435	26.258	31.011
8) T	DICHLORPROP	0.000	7.739	0	15986326	N.D.	27.724
12) T	2,4,5-T	9.425	0.000	16507118	0	4.059	N.D. #
15) T	Picloram	10.995	0.000	11713294	0	2.294	N.D. #
16) T	DCPA	11.531	0.000	16873467	0	3.149	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
Data File : PS010849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 00:45
Operator : DD\AJ
Sample : L3024-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
RO-25

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:51:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

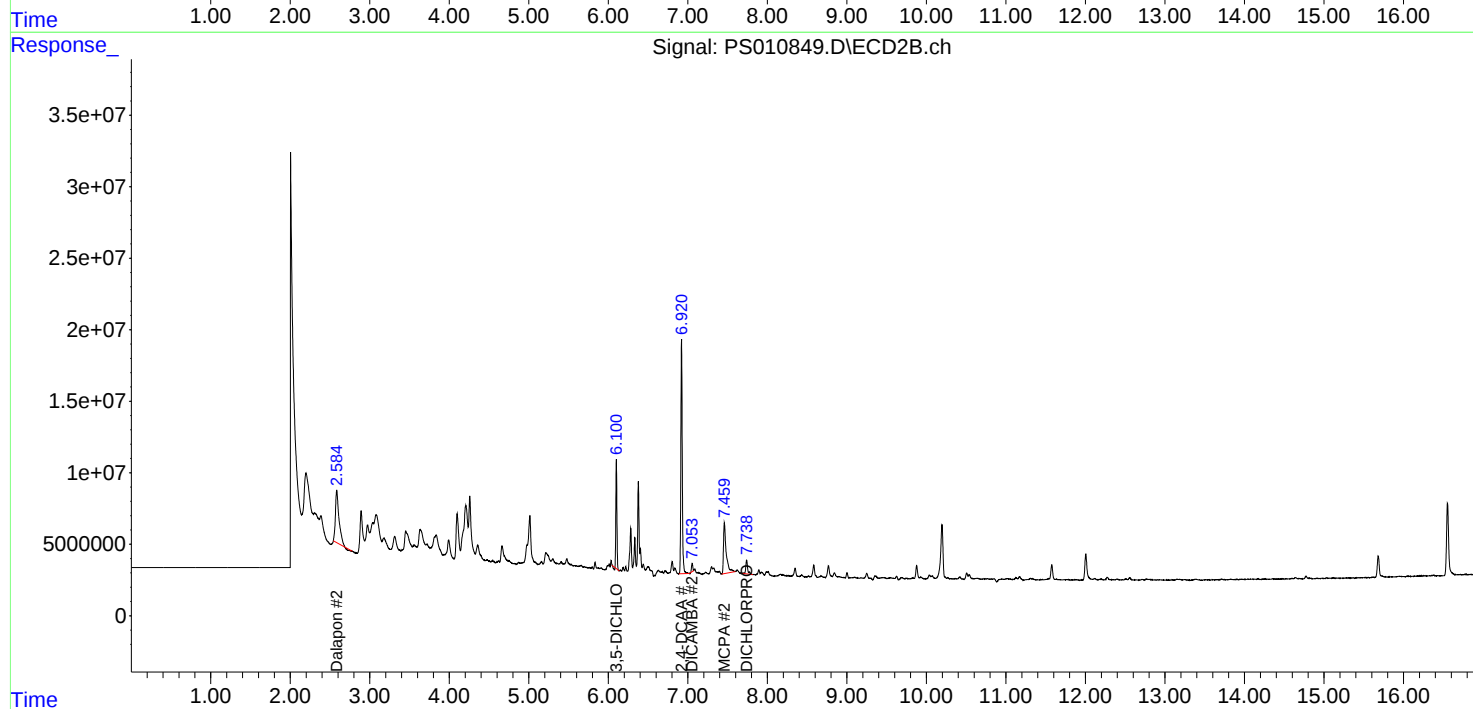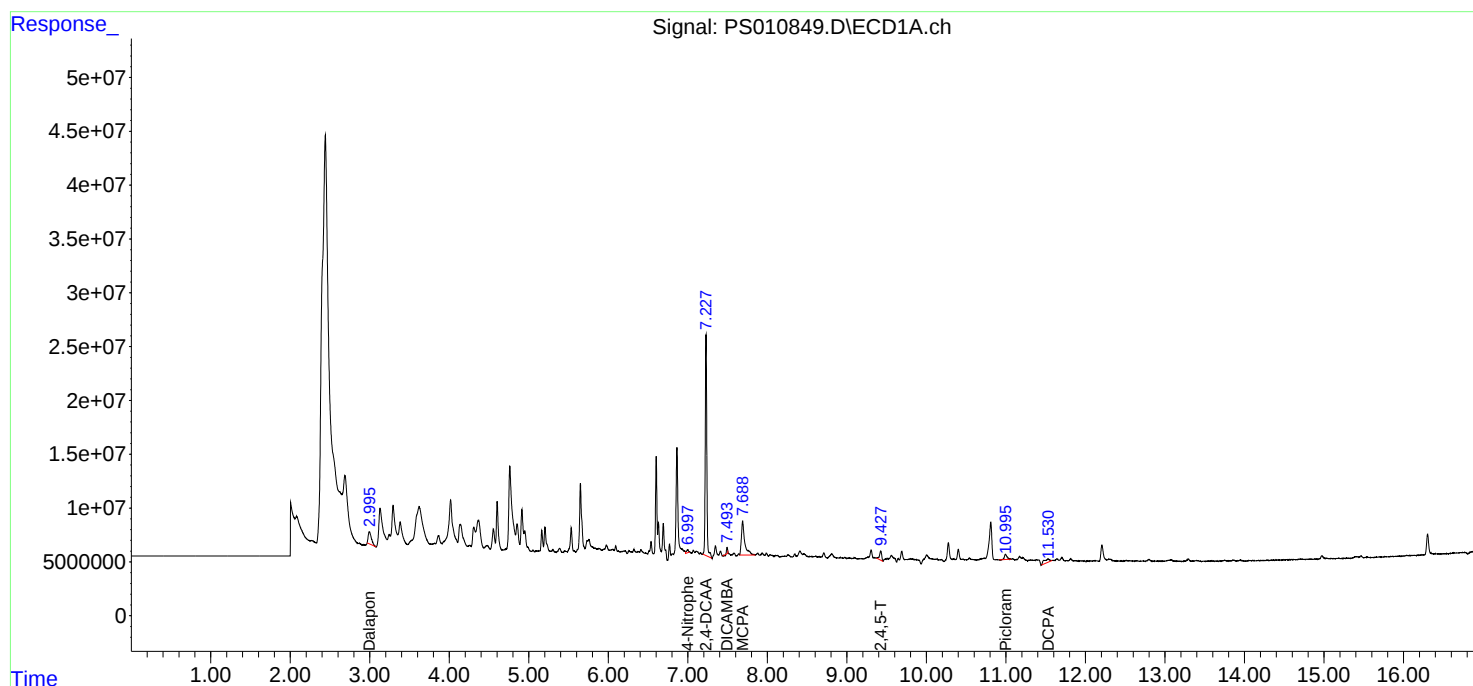


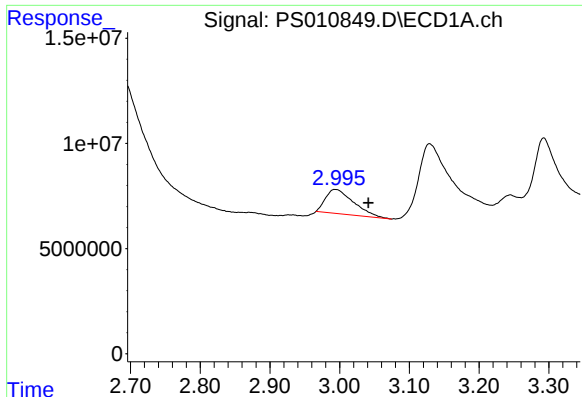

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.047 min
Response: 32036574
Conc: 32.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-25

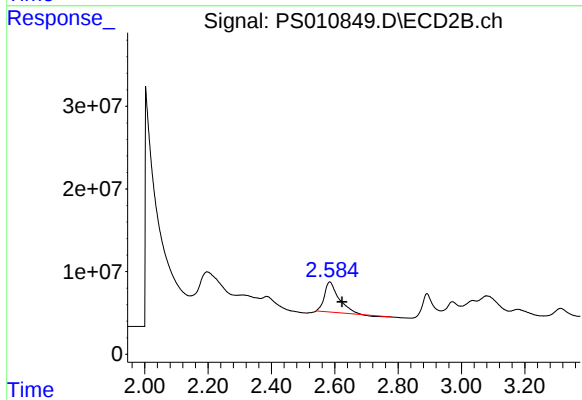


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.039 min
Response: 113538750
Conc: 155.08 ng/ml

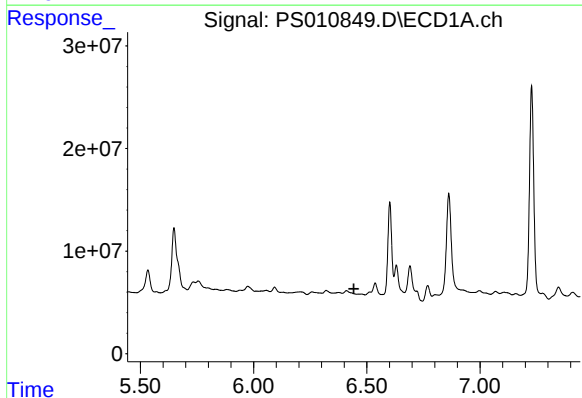


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

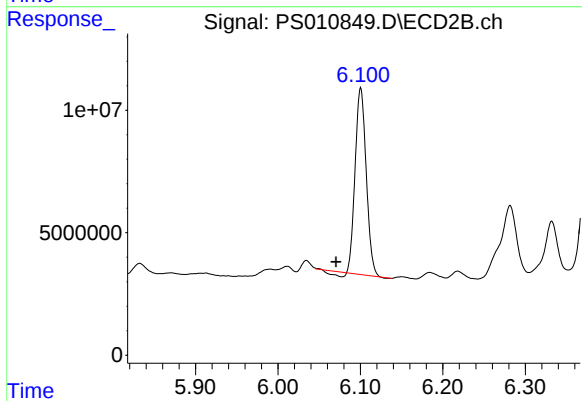

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 69644478
Conc: 84.97 ng/ml

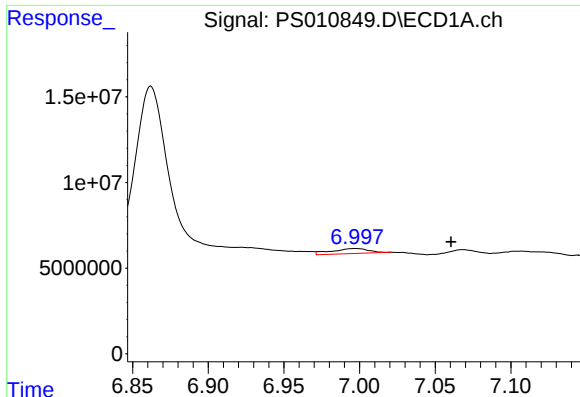

#3 4-Nitrophenol


R.T.: 6.997 min
Delta R.T.: -0.063 min
Response: 5080418
Conc: 13.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-25

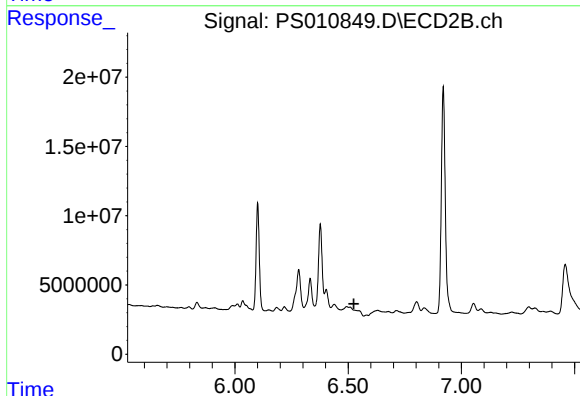


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

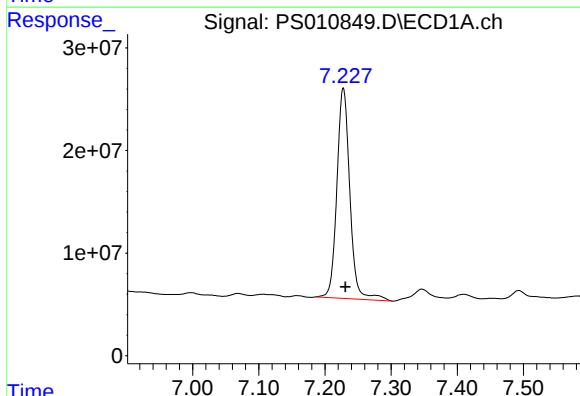


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 279556062
Conc: 353.48 ng/ml

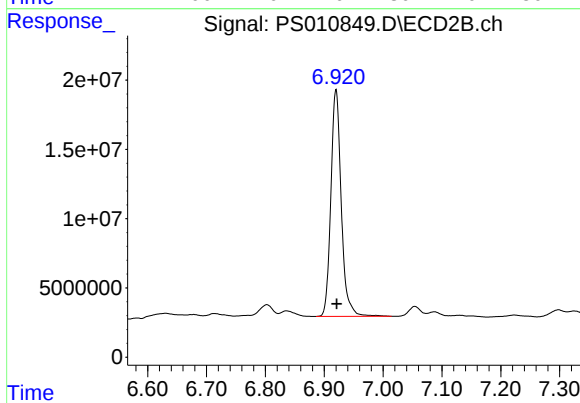

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 200929867
Conc: 368.40 ng/ml

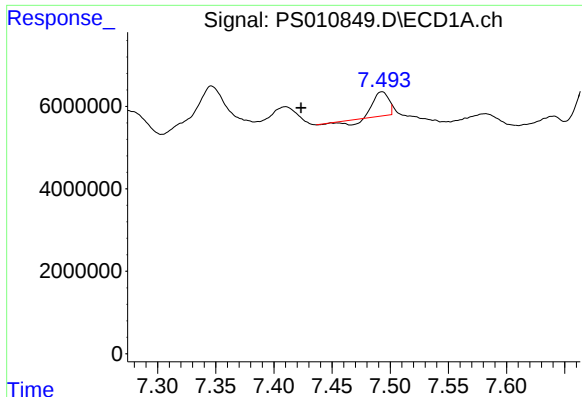

#5 DICAMBA


R.T.: 7.493 min
Delta R.T.: 0.070 min
Response: 4350859
Conc: 1.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-25

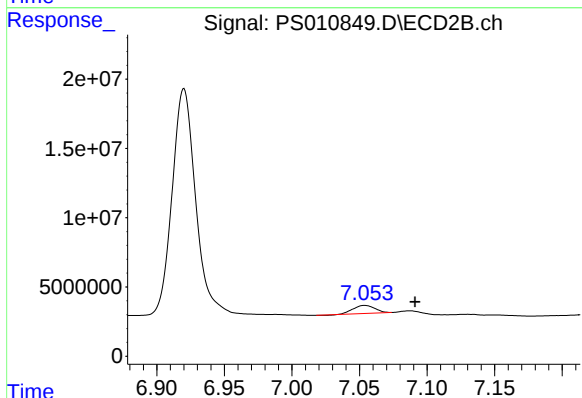


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 6424644
Conc: 2.85 ng/ml

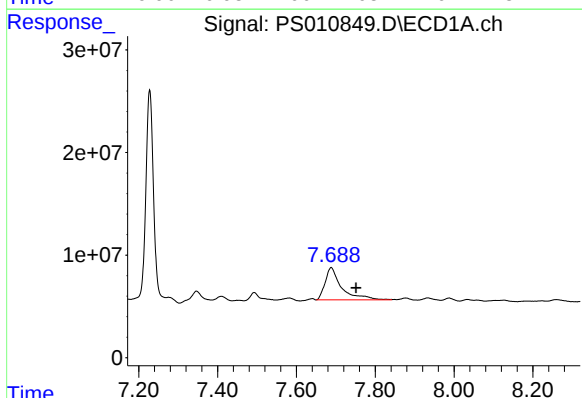


#7 MCPA

R.T.: 7.688 min
Delta R.T.: -0.063 min
Response: 91798344
Conc: 26.26 ug/ml

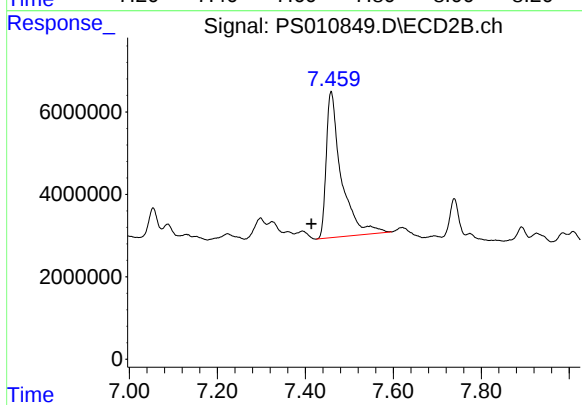

#7 MCPA


R.T.: 7.459 min
Delta R.T.: 0.045 min
Response: 84280435
Conc: 31.01 ug/ml

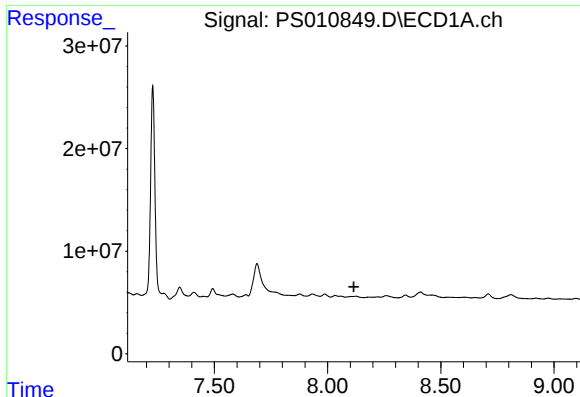

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-25

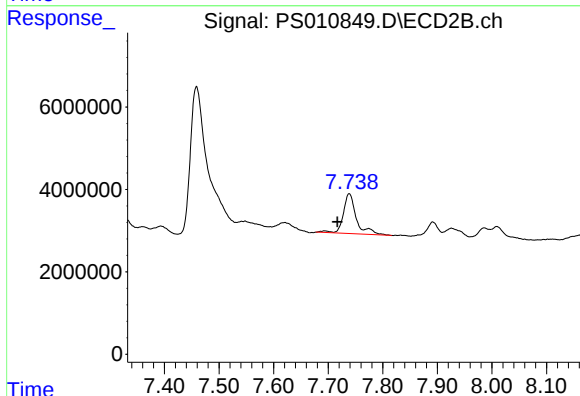


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.021 min
Response: 15986326
Conc: 27.72 ng/ml

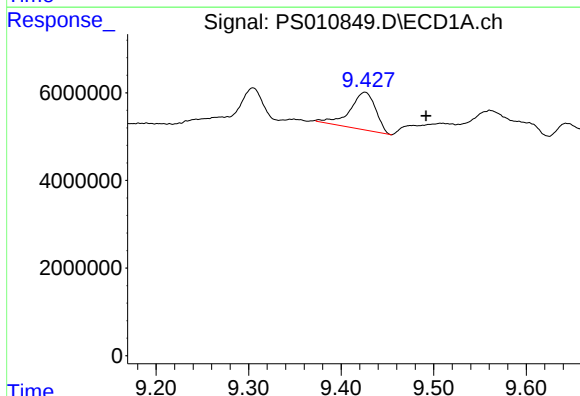


#12 2,4,5-T

R.T.: 9.425 min
Delta R.T.: -0.066 min
Response: 16507118
Conc: 4.06 ng/ml

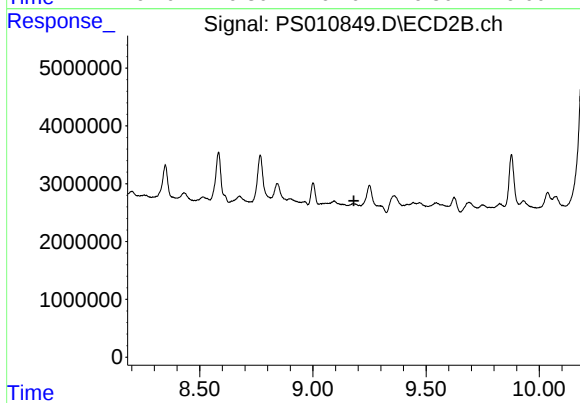

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

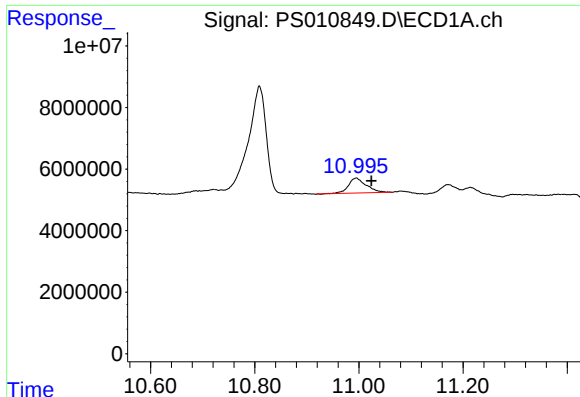

#15 Picloram


R.T.: 10.995 min
Delta R.T.: -0.029 min
Response: 11713294
Conc: 2.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-25

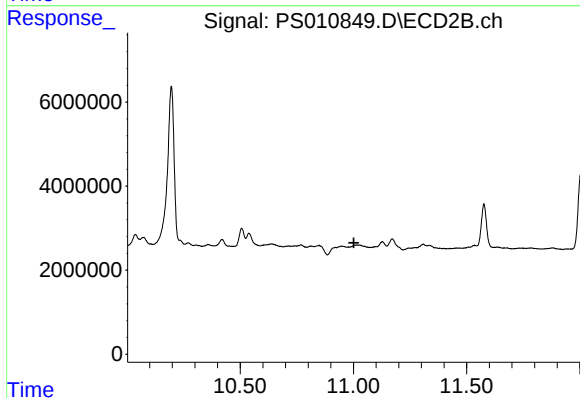


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.

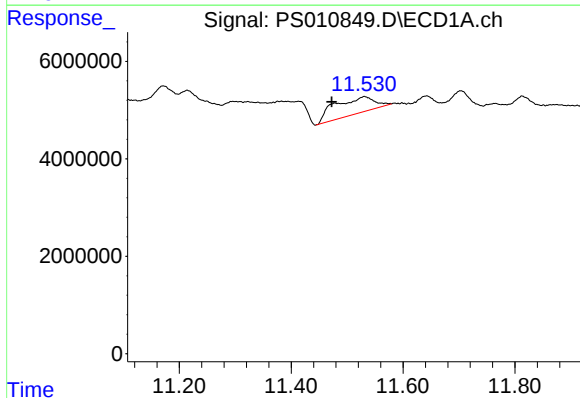

#16 DCPA

R.T.: 11.531 min
Delta R.T.: 0.059 min
Response: 16873467
Conc: 3.15 ng/ml

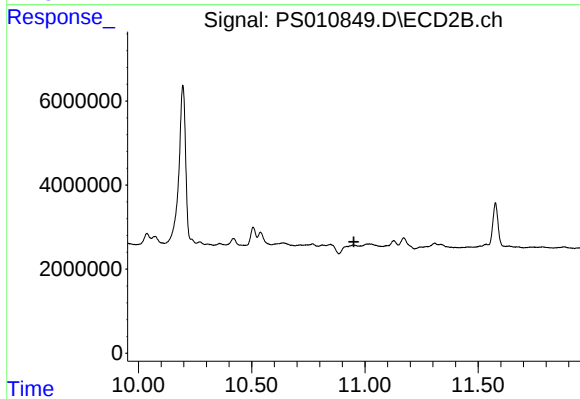

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.951 min
Response: 0
Conc: N.D.