

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
 Data File : PS010850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 01:08
 Operator : DD\AJ
 Sample : L3024-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-16

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:51:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	356.9E6	262.3E6	451.284	480.908
Target Compounds							
1) T	Dalapon	2.994	2.585	32836331	129.4E6	33.398	176.693 #
2) T	3,5-DICHL...	0.000	6.100	0	81182252	N.D.	99.046
3) T	4-Nitroph...	6.997	0.000	4219135	0	11.381	N.D. #
5) T	DICAMBA	7.493	7.054	3349616	12430765	1.065	5.523 #
7) T	MCPA	7.687	7.458	107.7E6	116.0E6	30.803	42.666 #
8) T	DICHLORPROP	0.000	7.739	0	20439004	N.D.	35.446
12) T	2,4,5-T	9.560	0.000	19589941	0	4.817	N.D. #
15) T	Picloram	10.994	0.000	11993793	0	2.349	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
Data File : PS010850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 01:08
Operator : DD\AJ
Sample : L3024-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RO-16

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:51:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

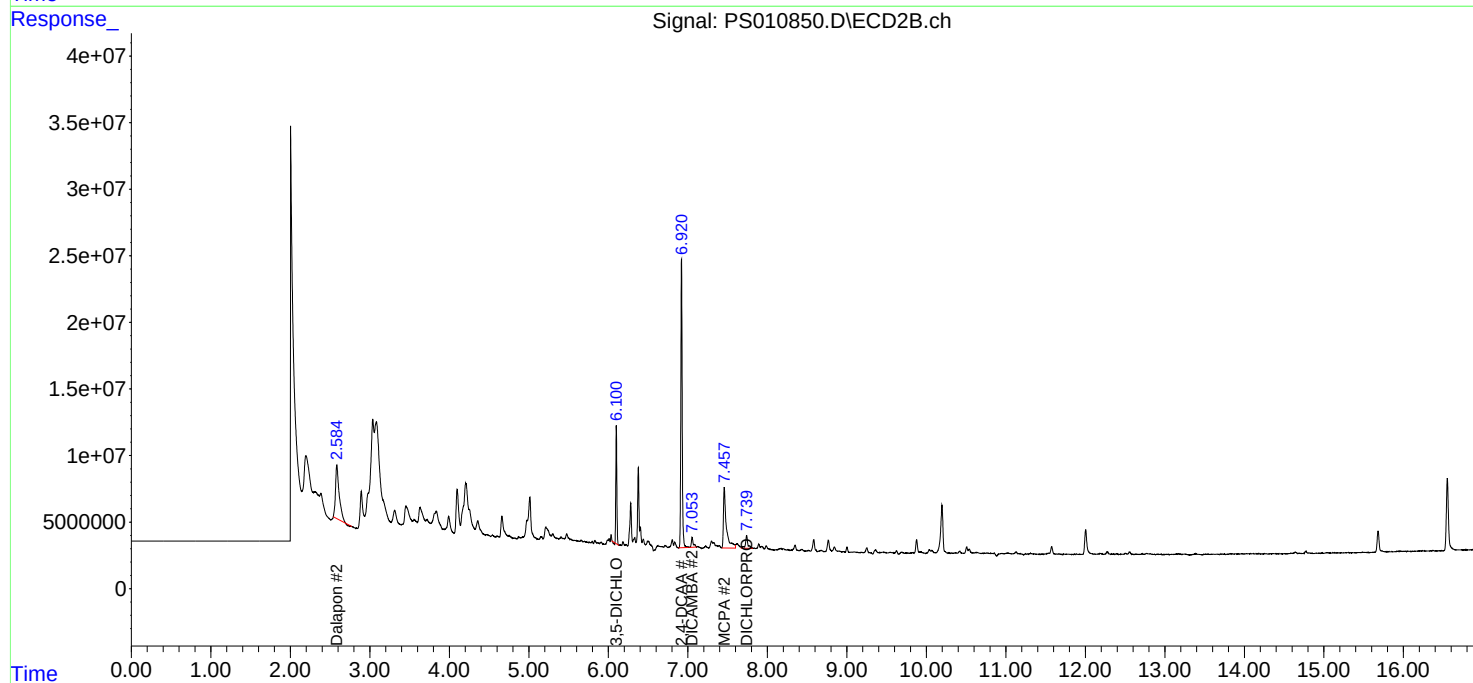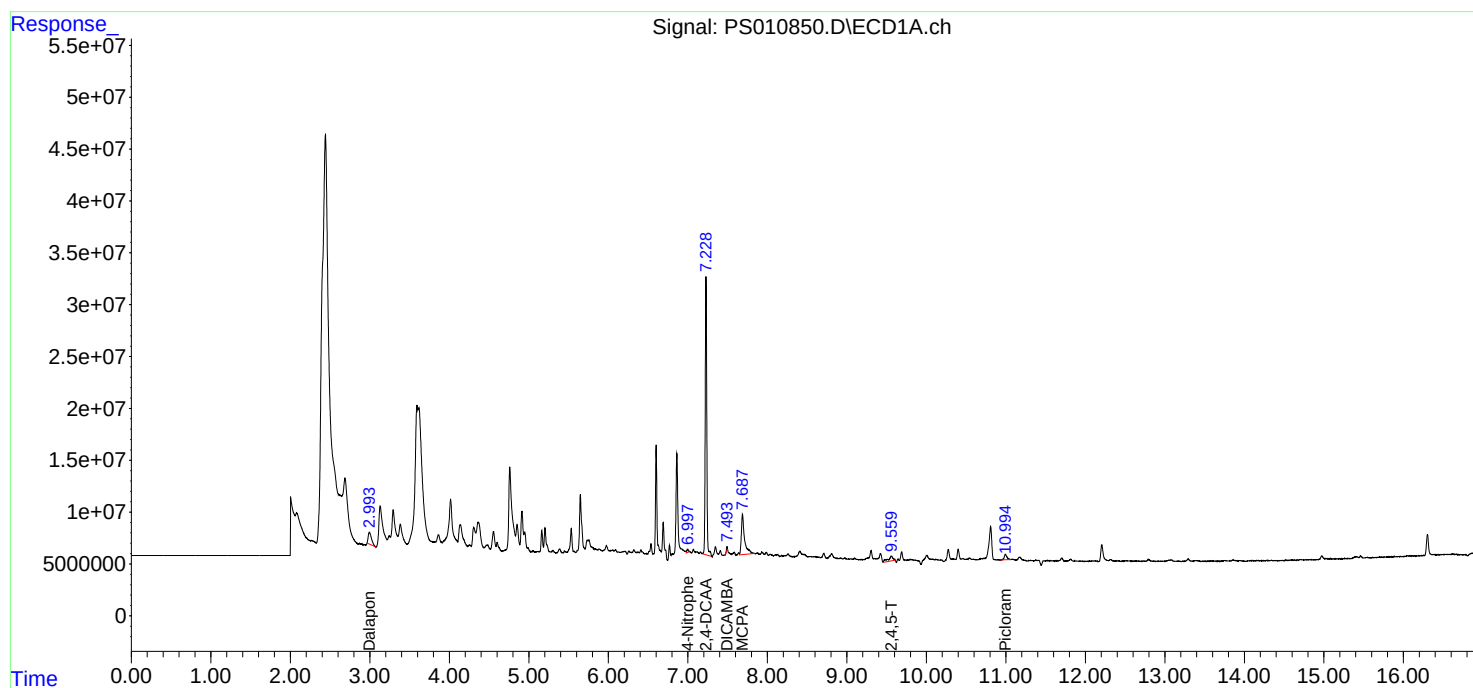


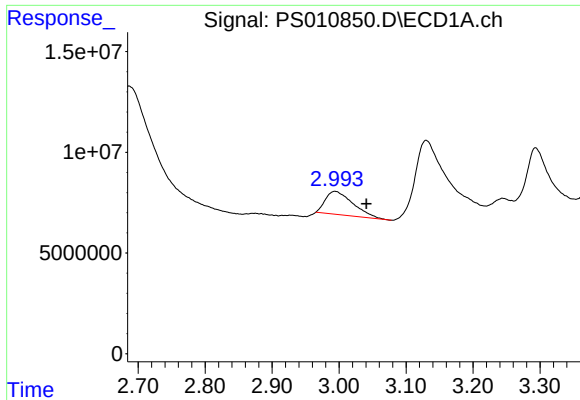

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.047 min
Response: 32836331
Conc: 33.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-16

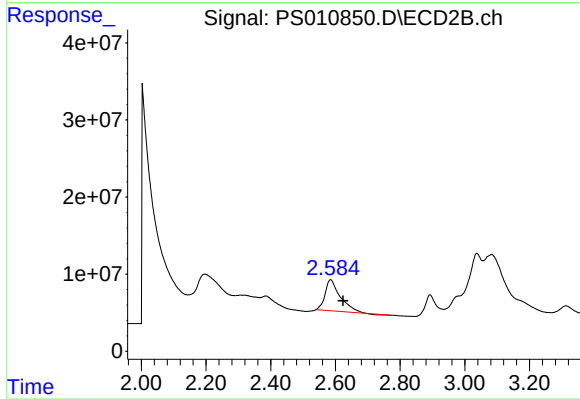


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.038 min
Response: 129365150
Conc: 176.69 ng/ml

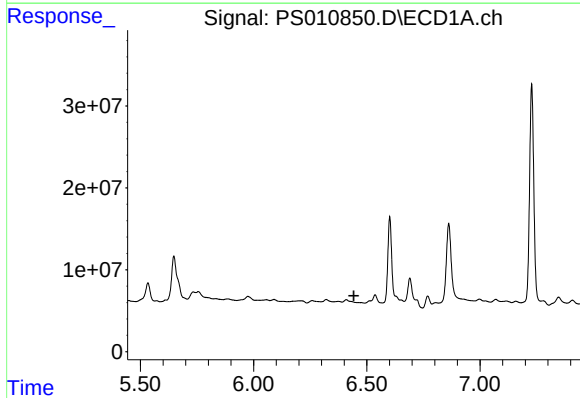


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

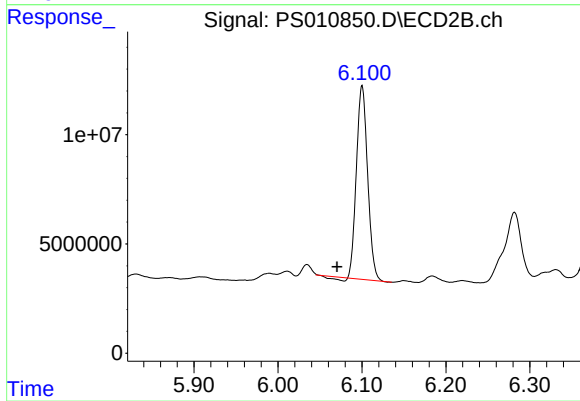

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 81182252
Conc: 99.05 ng/ml

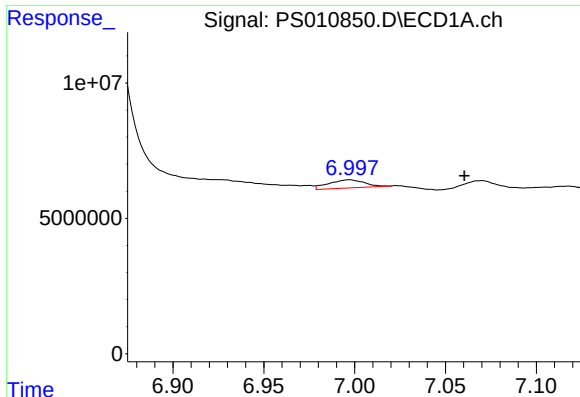

#3 4-Nitrophenol


R.T.: 6.997 min
Delta R.T.: -0.063 min
Response: 4219135
Conc: 11.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-16

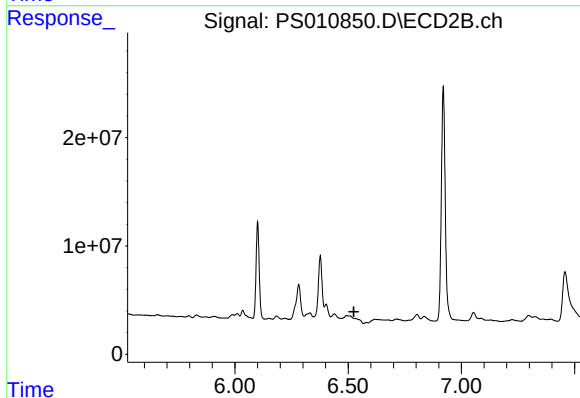


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

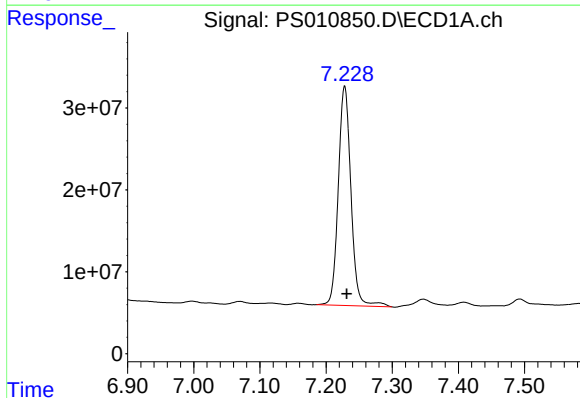


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 356903577
Conc: 451.28 ng/ml

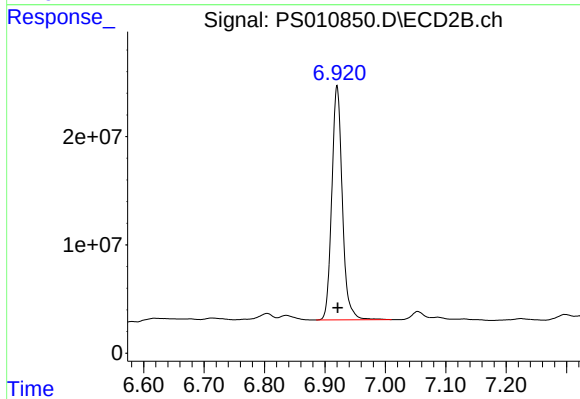

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 262294917
Conc: 480.91 ng/ml

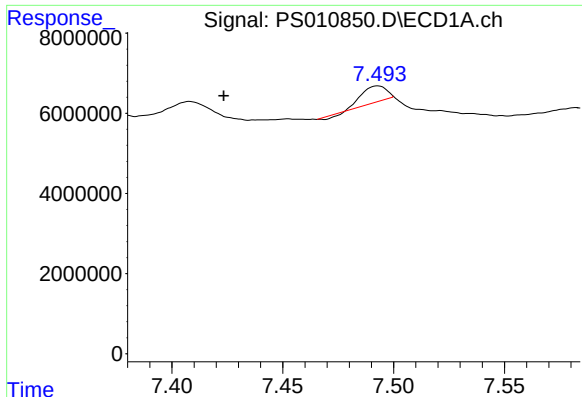

#5 DICAMBA


R.T.: 7.493 min
Delta R.T.: 0.069 min
Response: 3349616
Conc: 1.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-16

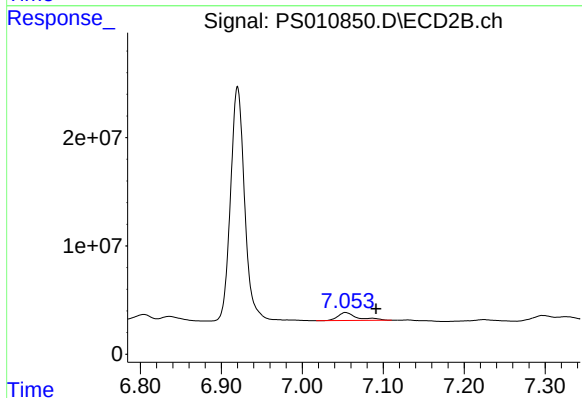


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 12430765
Conc: 5.52 ng/ml

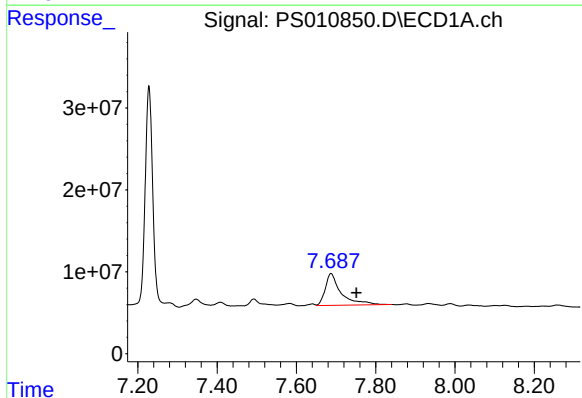


#7 MCPA

R.T.: 7.687 min
Delta R.T.: -0.064 min
Response: 107687457
Conc: 30.80 ug/ml

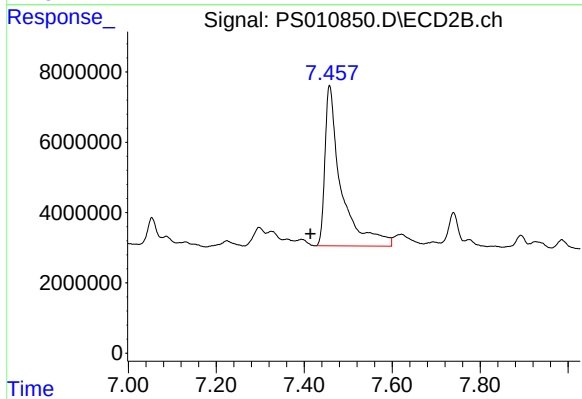

#7 MCPA


R.T.: 7.458 min
Delta R.T.: 0.044 min
Response: 115954502
Conc: 42.67 ug/ml

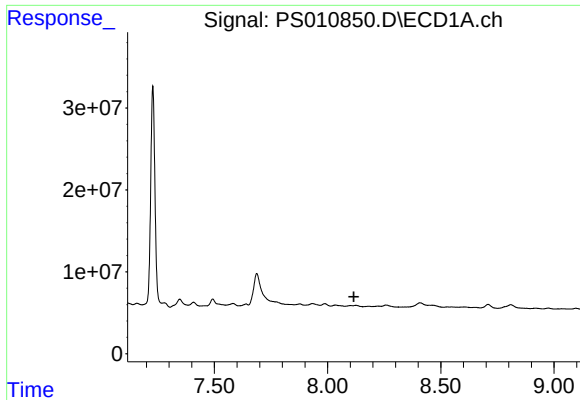

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-16

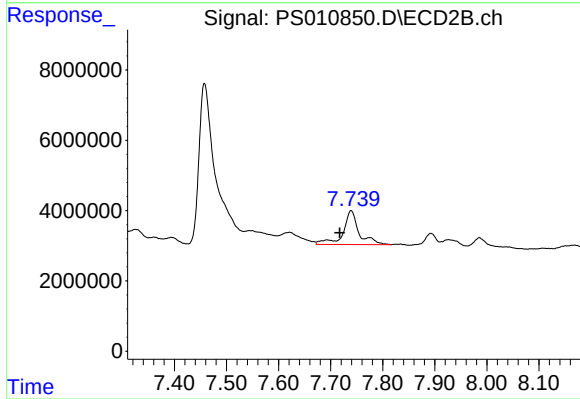


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.022 min
Response: 20439004
Conc: 35.45 ng/ml

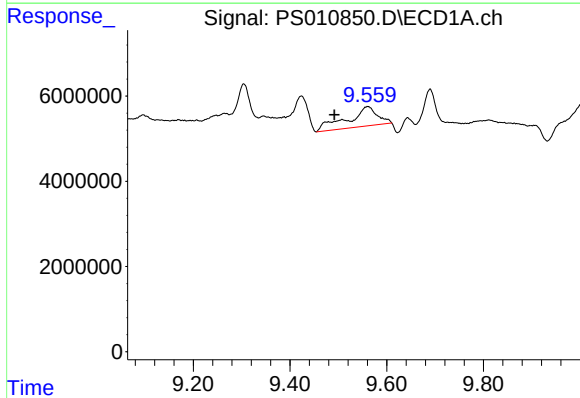


#12 2,4,5-T

R.T.: 9.560 min
Delta R.T.: 0.068 min
Response: 19589941
Conc: 4.82 ng/ml

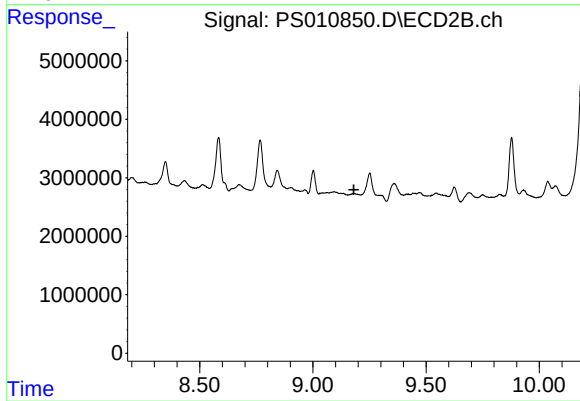

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

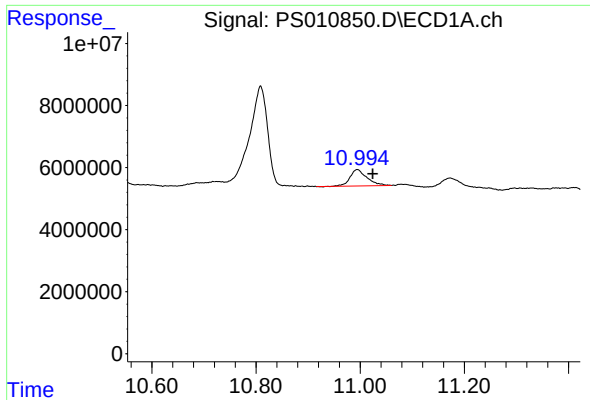

#15 Picloram

R.T.: 10.994 min
Delta R.T.: -0.030 min
Response: 11993793
Conc: 2.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-16

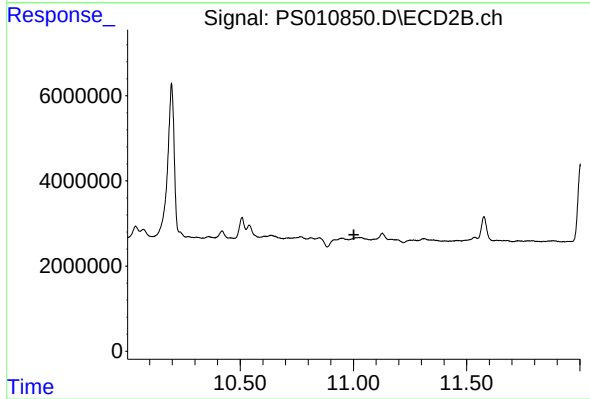

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.