

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
 Data File : PS010853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 02:17
 Operator : DD\AJ
 Sample : L3024-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:52:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	323.7E6	246.6E6	409.323	452.213
Target Compounds							
1) T	Dalapon	2.993	2.584	32417920	125.3E6	32.972	171.182 #
2) T	3,5-DICHL...	0.000	6.100	0	81930635	N.D.	99.959
3) T	4-Nitroph...	6.996	0.000	6122617	0	16.515	N.D. #
5) T	DICAMBA	7.492	7.054	5015935	12871190	1.595	5.718 #
7) T	MCPA	7.687	7.457	103.0E6	81297621	29.454	29.914
8) T	DICHLORPROP	0.000	7.739	0	17992330	N.D.	31.203
10) T	Pentachlo...	8.708	0.000	7171748	0	<MDL	N.D. #
12) T	2,4,5-T	9.559	0.000	22105494	0	5.435	N.D. #
15) T	Picloram	10.994	0.000	12153951	0	2.381	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
Data File : PS010853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 02:17
Operator : DD\AJ
Sample : L3024-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
RO-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:52:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

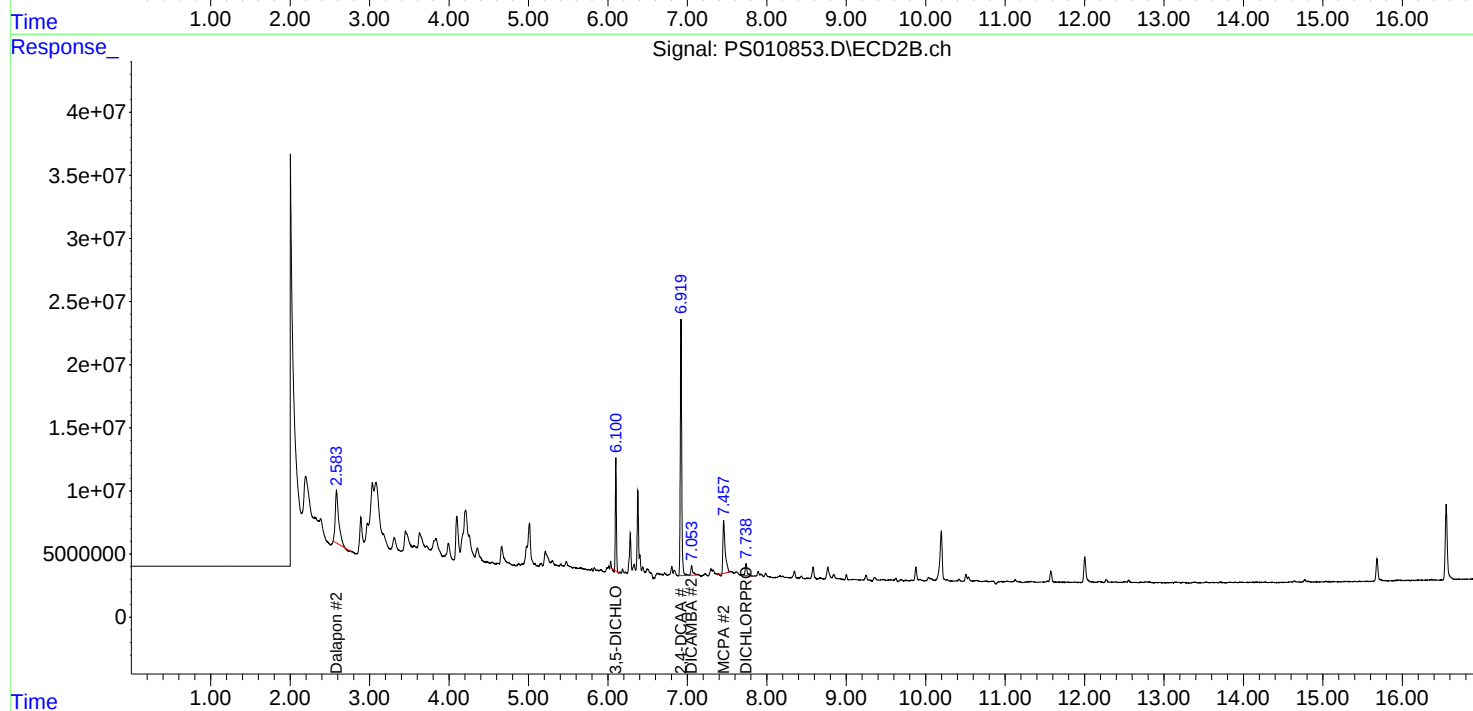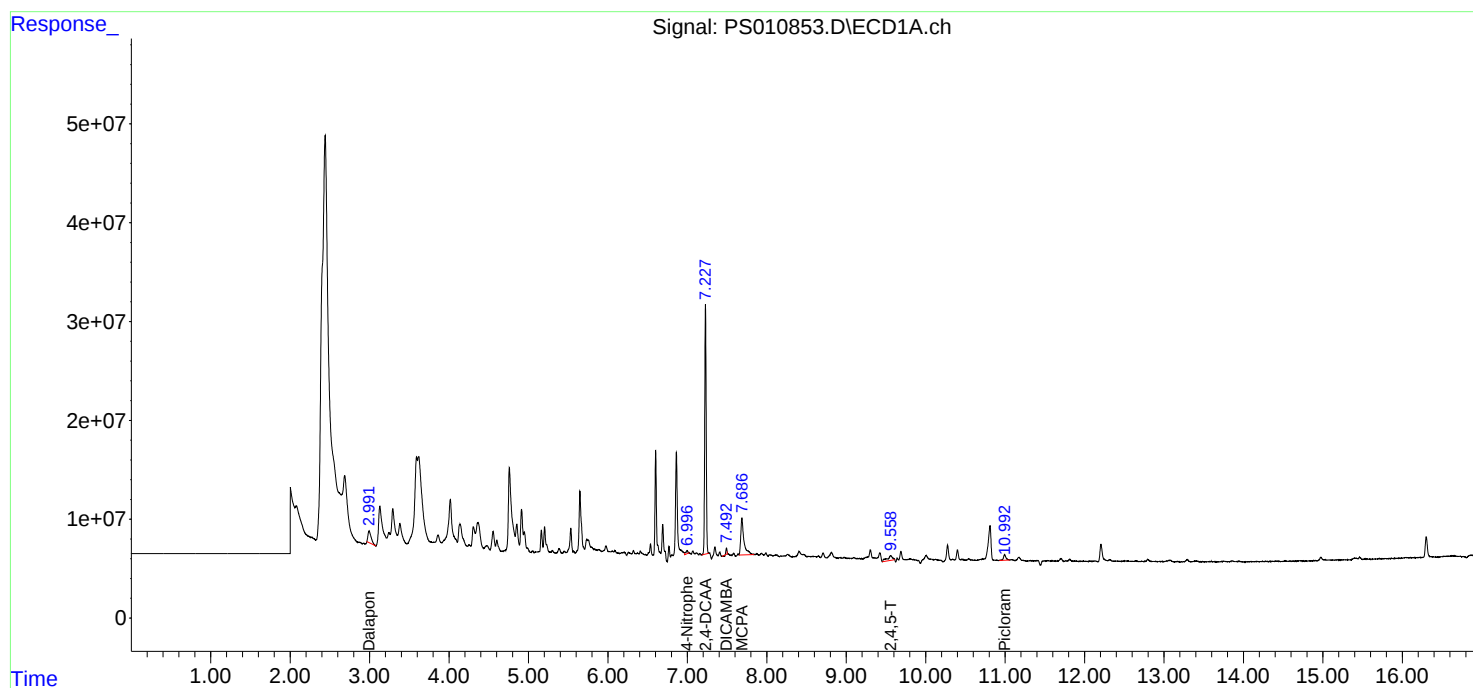


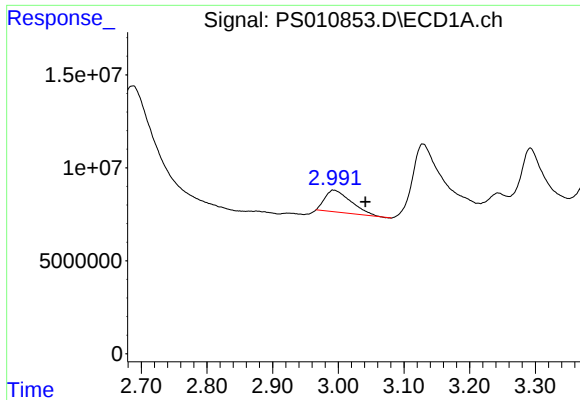

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.048 min
Response: 32417920
Conc: 32.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-6

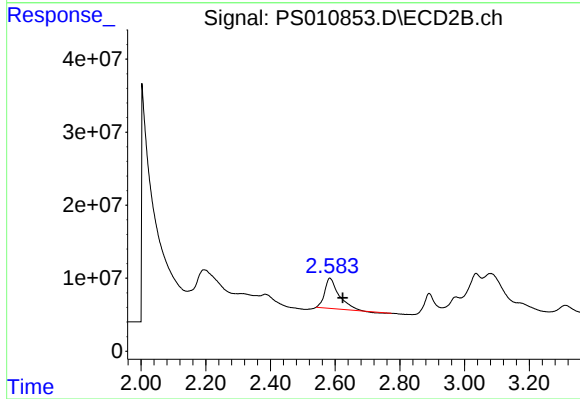


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.040 min
Response: 125329859
Conc: 171.18 ng/ml

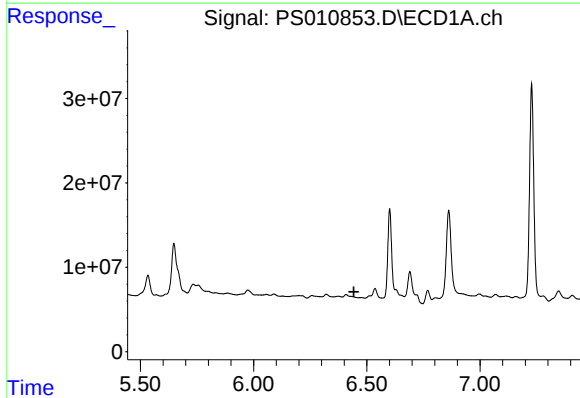


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

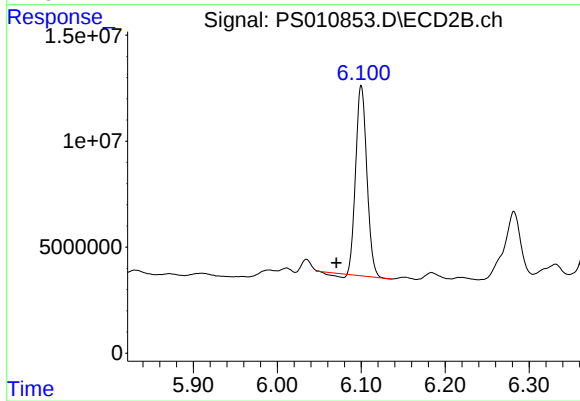

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 81930635
Conc: 99.96 ng/ml

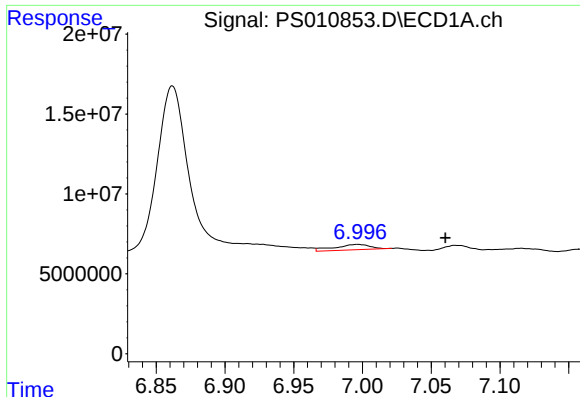

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.064 min
Response: 6122617
Conc: 16.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-6

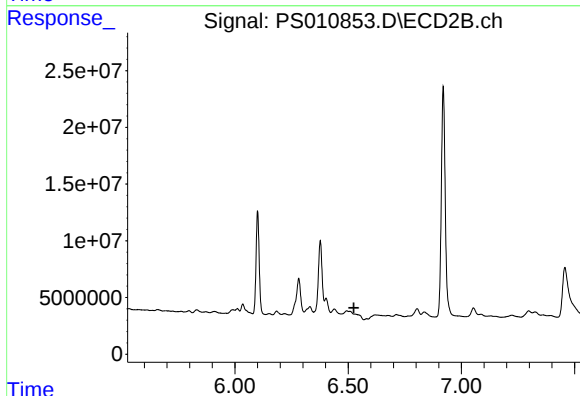


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

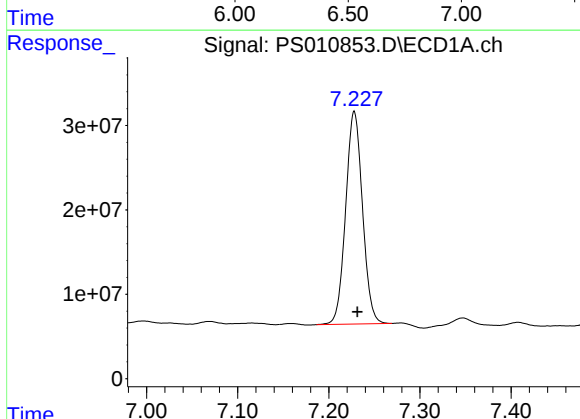


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 323717603
Conc: 409.32 ng/ml

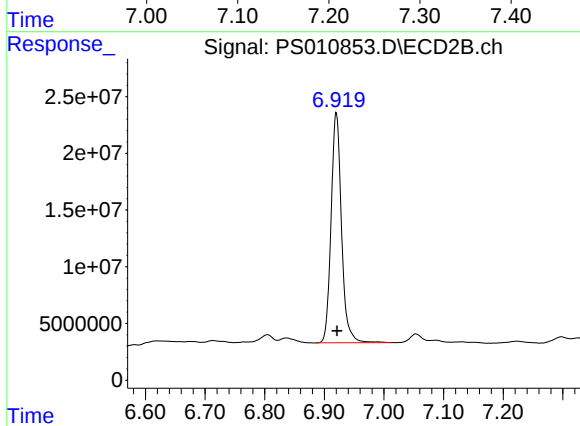

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 246644079
Conc: 452.21 ng/ml

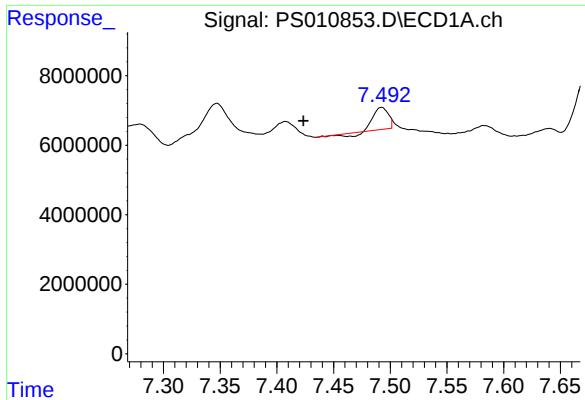

#5 DICAMBA


R.T.: 7.492 min
Delta R.T.: 0.069 min
Response: 5015935
Conc: 1.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-6

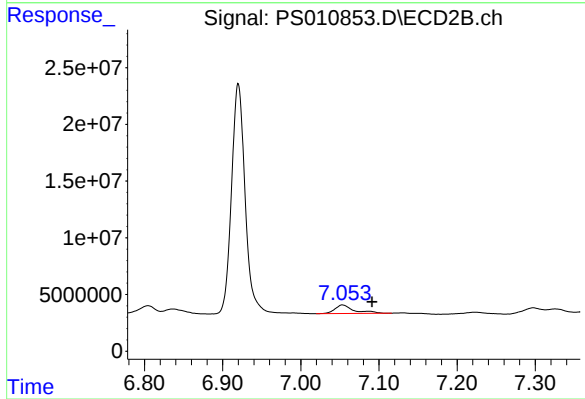


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 12871190
Conc: 5.72 ng/ml

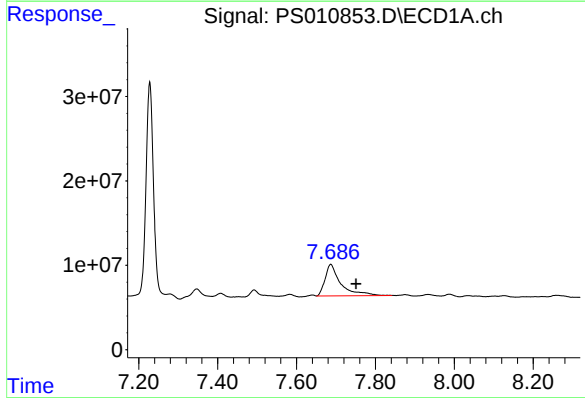


#7 MCPA

R.T.: 7.687 min
Delta R.T.: -0.064 min
Response: 102970224
Conc: 29.45 ug/ml

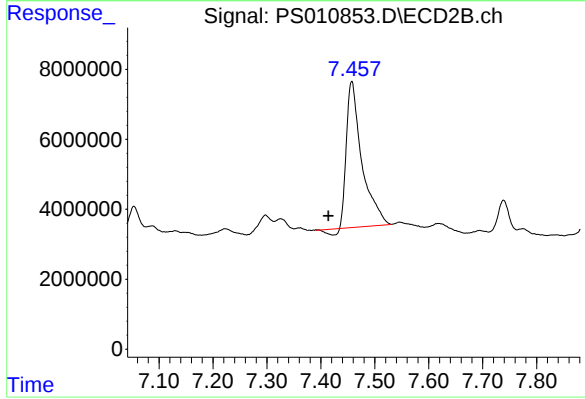

#7 MCPA


R.T.: 7.457 min
Delta R.T.: 0.044 min
Response: 81297621
Conc: 29.91 ug/ml

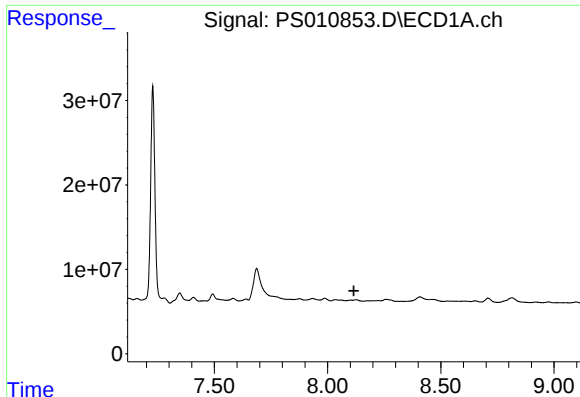

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-6

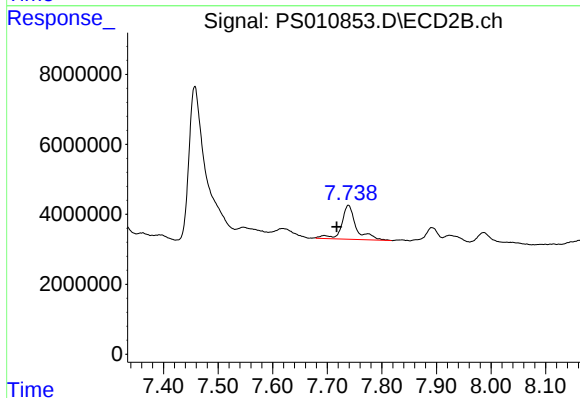


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.021 min
Response: 17992330
Conc: 31.20 ng/ml

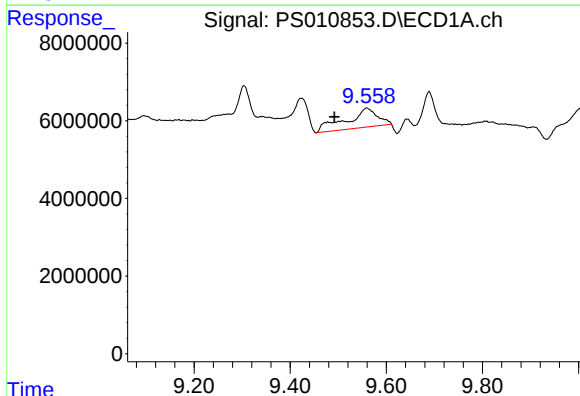


#12 2,4,5-T

R.T.: 9.559 min
Delta R.T.: 0.067 min
Response: 22105494
Conc: 5.44 ng/ml

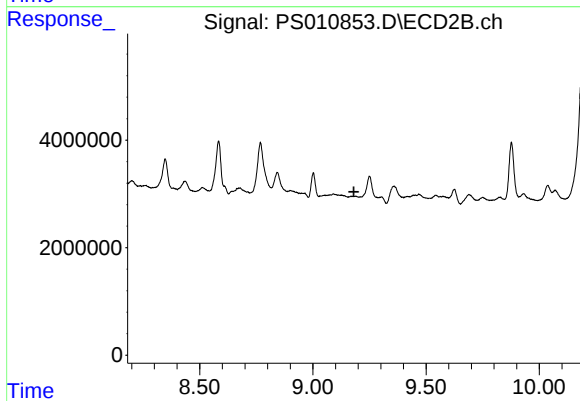

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

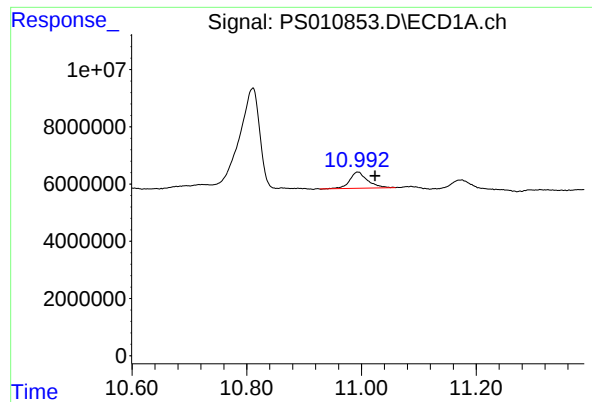

#15 Picloram

R.T.: 10.994 min
Delta R.T.: -0.030 min
Response: 12153951
Conc: 2.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-6

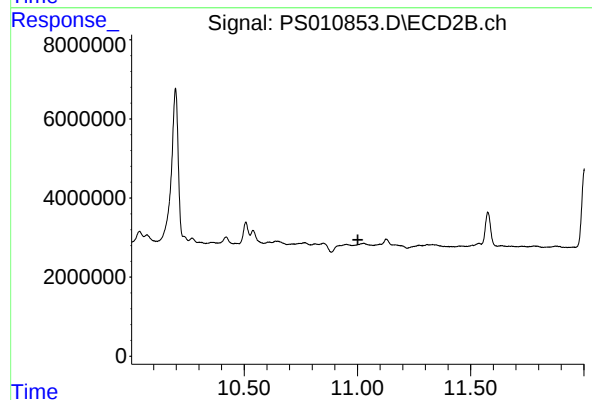

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.