

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
 Data File : PS010854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 02:40
 Operator : DD\AJ
 Sample : L3024-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:34:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	358.4E6	255.6E6	453.223	468.583
Target Compounds							
1) T	Dalapon	2.992	2.585	31934868	134.2E6	32.481	183.267 #
2) T	3,5-DICHL...	0.000	6.100	0	74446662	N.D.	90.828
3) T	4-Nitroph...	6.996	0.000	5366948	0	14.477	N.D. #
5) T	DICAMBA	7.493	7.054	3322166	6580160	1.057	2.923 #
7) T	MCPA	7.687	7.458	92530239	69952421	26.468	25.739
8) T	DICHLORPROP	0.000	7.738	0	10564768	N.D.	18.322
9) T	2,4-D	8.277	0.000	8014273	0	10.167	N.D. #
10) T	Pentachlo...	8.709	0.000	7810801	0	<MDL	N.D. #
12) T	2,4,5-T	9.558	0.000	39348689	0	9.675	N.D. #
15) T	Picloram	10.993	0.000	12299798	0	2.409	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
Data File : PS010854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 02:40
Operator : DD\AJ
Sample : L3024-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RO-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:34:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

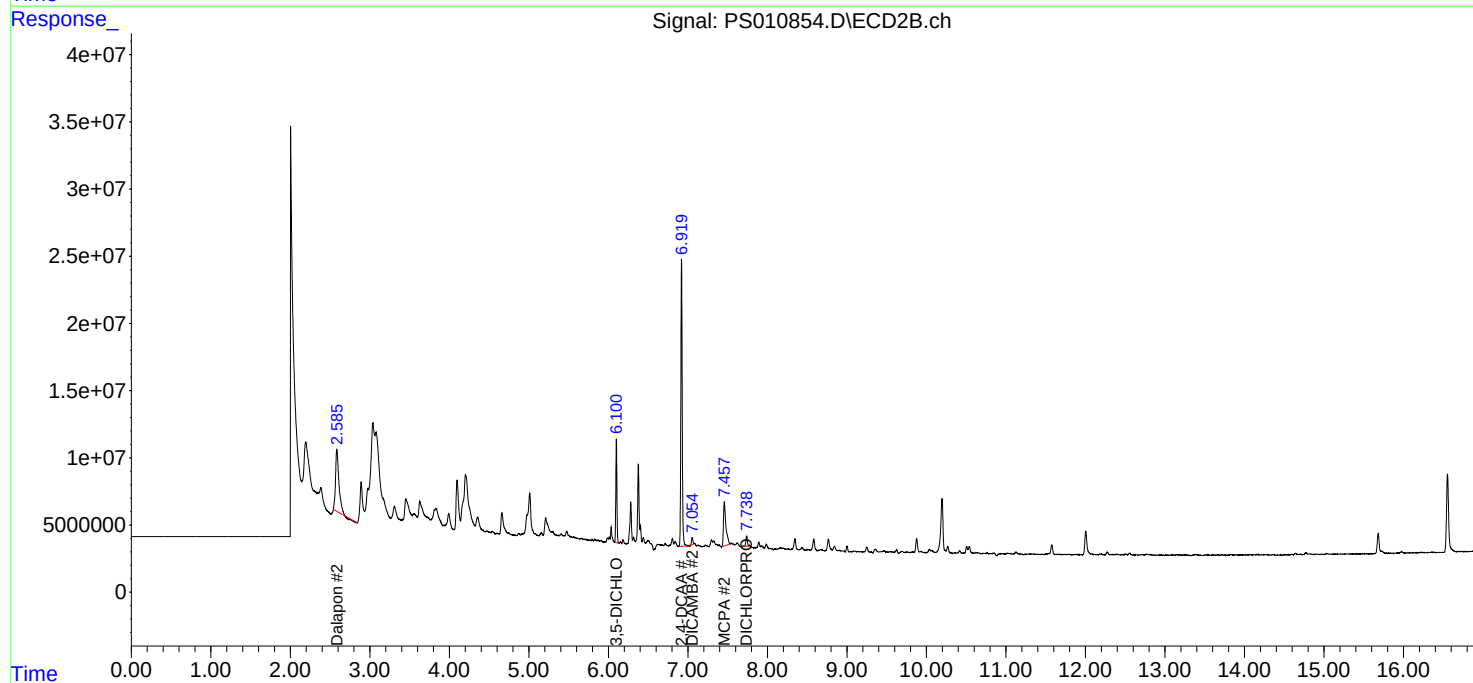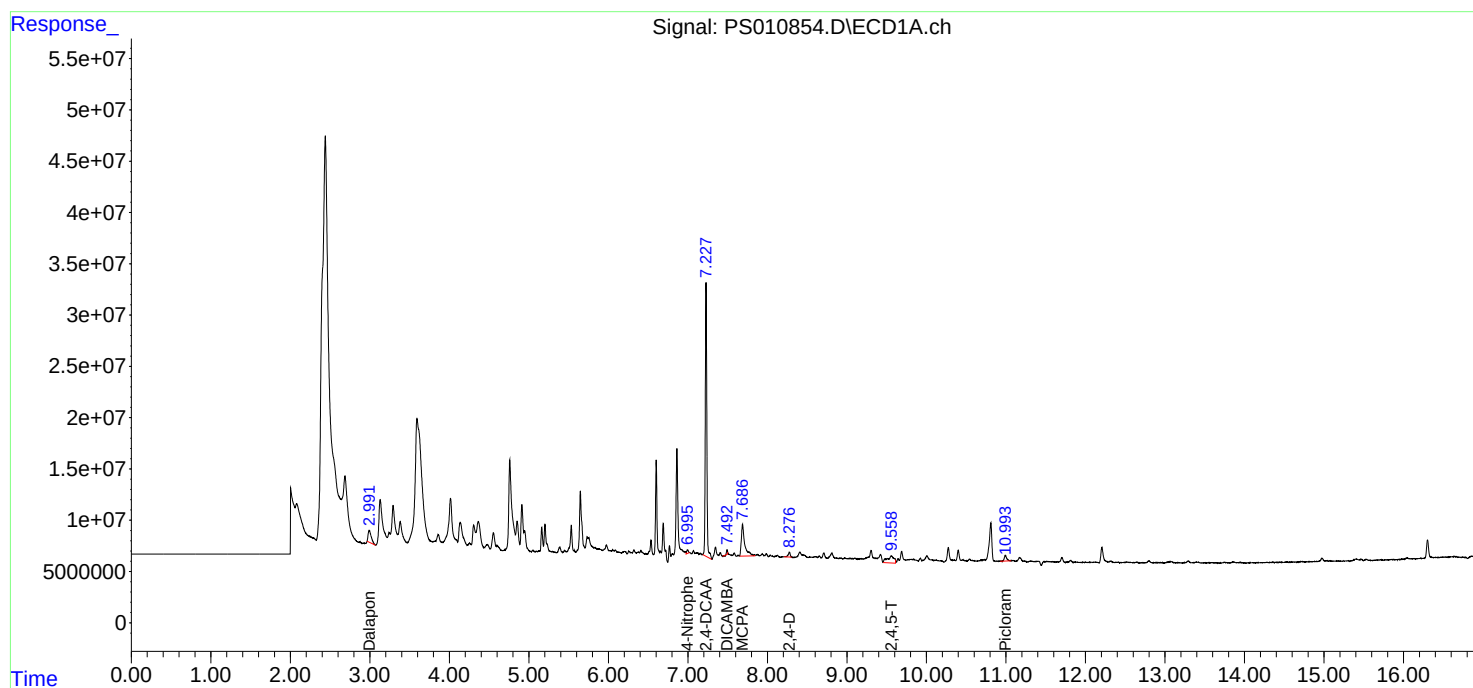


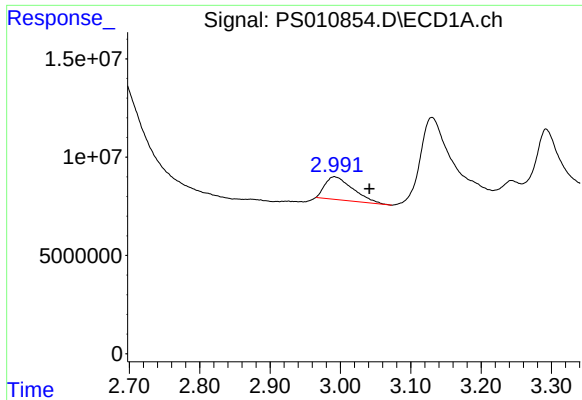

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.049 min
Response: 31934868
Conc: 32.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-17

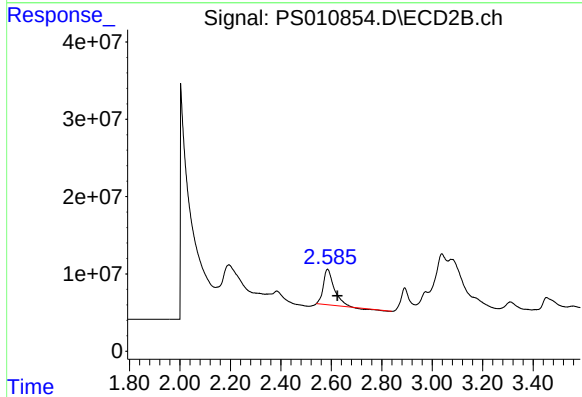


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.038 min
Response: 134178162
Conc: 183.27 ng/ml

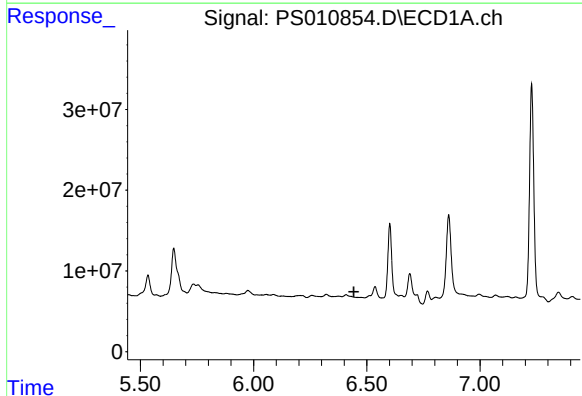


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

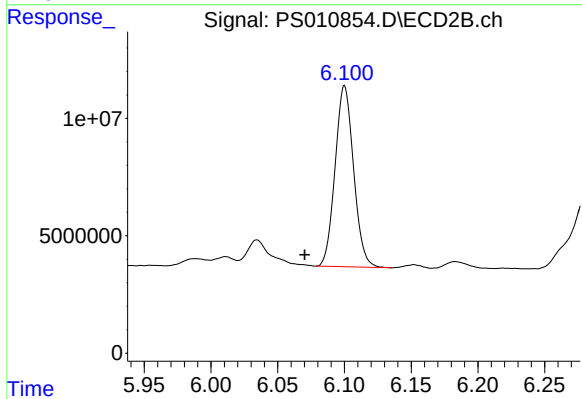

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 74446662
Conc: 90.83 ng/ml

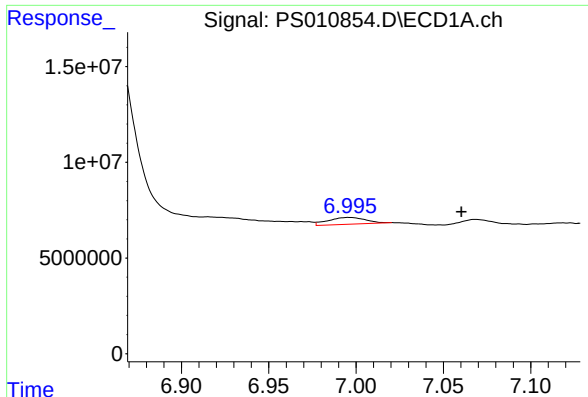

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.065 min
Response: 5366948
Conc: 14.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-17

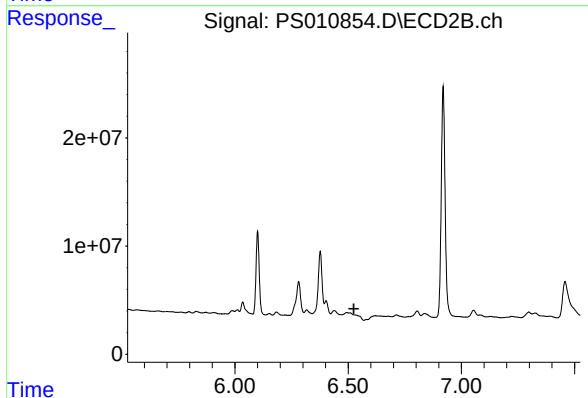


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

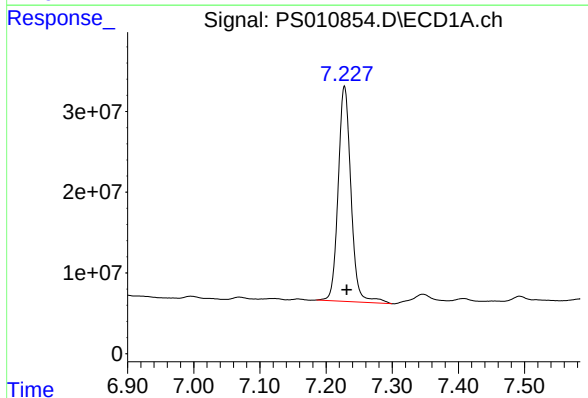


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 358436757
Conc: 453.22 ng/ml

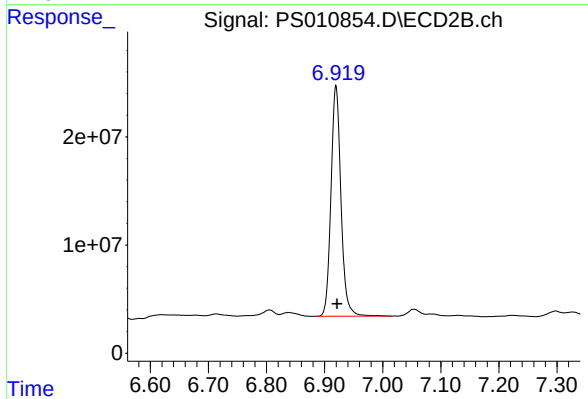

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 255572611
Conc: 468.58 ng/ml

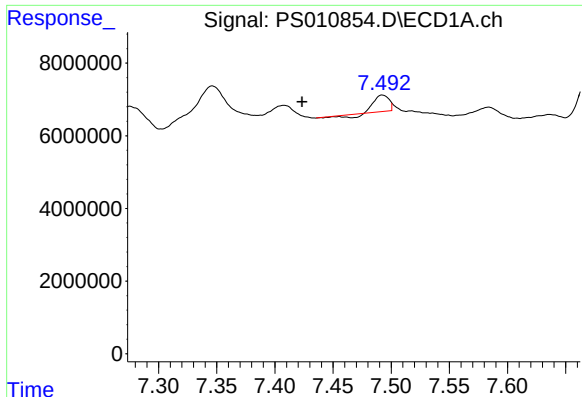

#5 DICAMBA


R.T.: 7.493 min
Delta R.T.: 0.069 min
Response: 3322166
Conc: 1.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-17

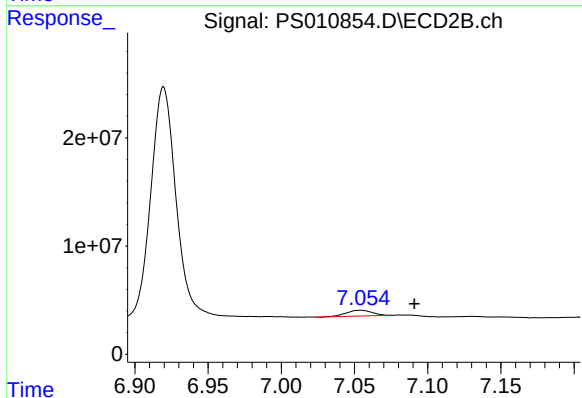


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 6580160
Conc: 2.92 ng/ml

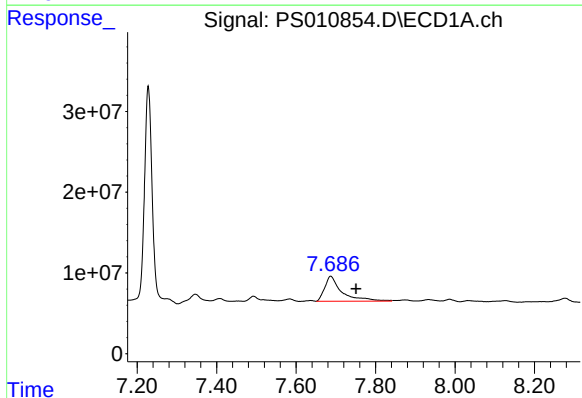


#7 MCPA

R.T.: 7.687 min
Delta R.T.: -0.064 min
Response: 92530239
Conc: 26.47 ug/ml

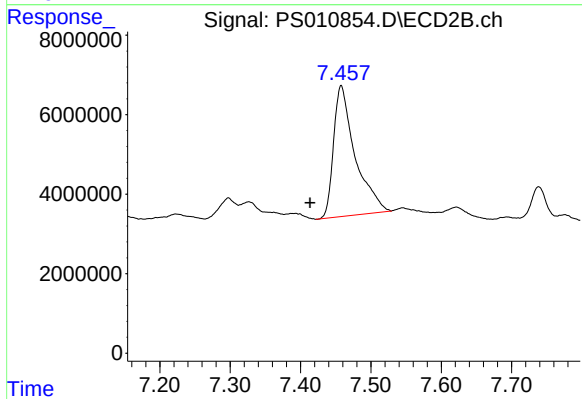

#7 MCPA


R.T.: 7.458 min
Delta R.T.: 0.044 min
Response: 69952421
Conc: 25.74 ug/ml

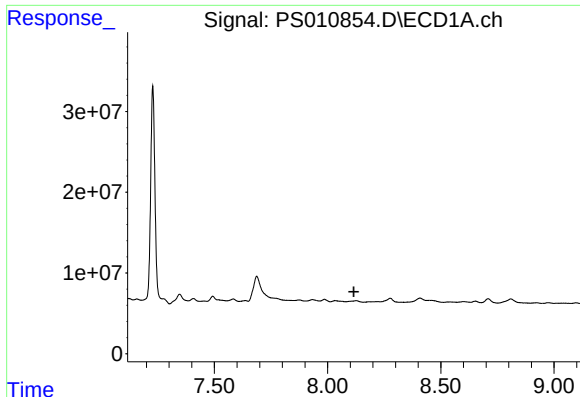

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-17

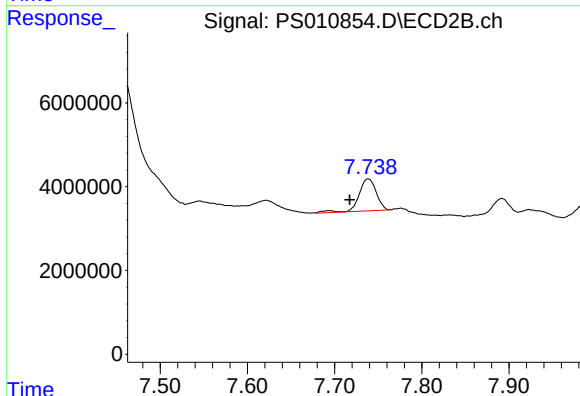


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.021 min
Response: 10564768
Conc: 18.32 ng/ml

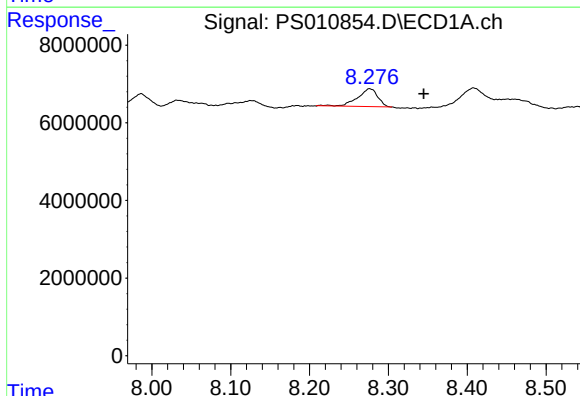


#9 2,4-D

R.T.: 8.277 min
Delta R.T.: -0.068 min
Response: 8014273
Conc: 10.17 ng/ml

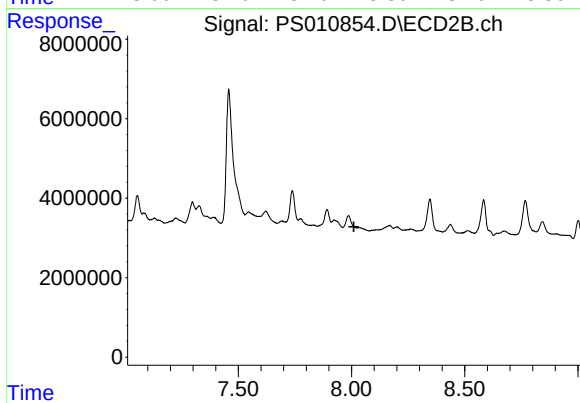

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.010 min
Response: 0
Conc: N.D.

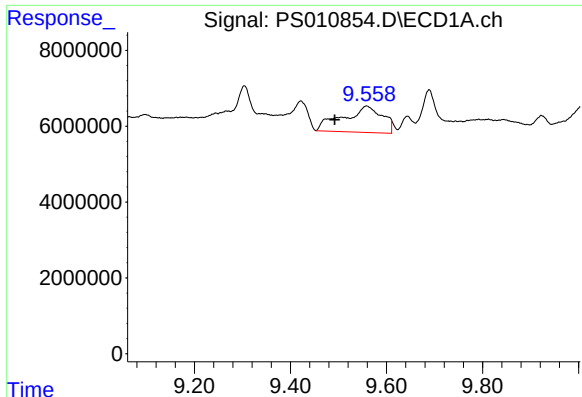

#12 2,4,5-T


R.T.: 9.558 min
Delta R.T.: 0.066 min
Response: 39348689
Conc: 9.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-17

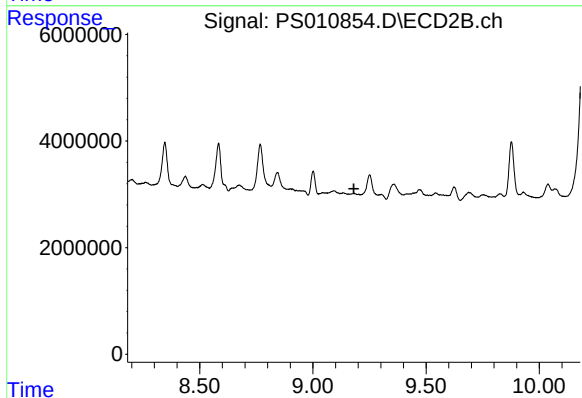


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.181 min
Response: 0
Conc: N.D.

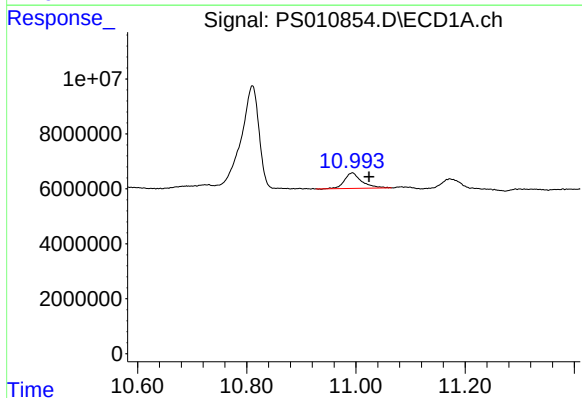

#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.031 min
Response: 12299798
Conc: 2.41 ng/ml

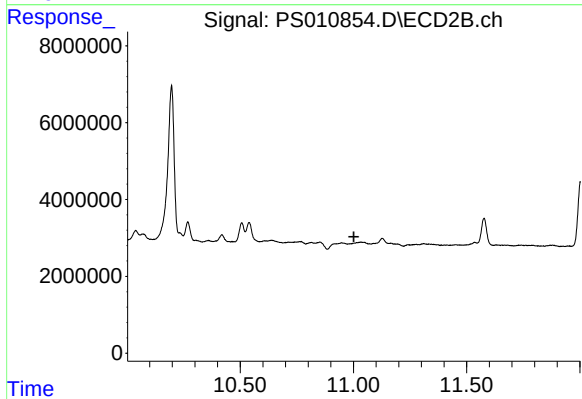

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.