

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
 Data File : PS010855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 03:03
 Operator : DD\AJ
 Sample : L3024-23
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:35:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	315.1E6	223.6E6	398.446	409.914
Target Compounds							
1) T	Dalapon	2.994	2.583	34335916	121.7E6	34.923	166.215 #
2) T	3,5-DICHL...	0.000	6.100	0	81003832	N.D.	98.828
3) T	4-Nitroph...	6.996	0.000	5727343	0	15.449	N.D. #
5) T	DICAMBA	7.493	7.053	6812925	10019763	2.167	4.452 #
7) T	MCPA	7.690	7.461	63667968	45731384	18.212	16.827
8) T	DICHLORPROP	0.000	7.739	0	8721090	N.D.	15.124
12) T	2,4,5-T	9.560	0.000	41190576	0	10.128	N.D. #
14) T	DINOSEB	0.000	10.034	0	2862279	N.D.	1.330
15) T	Picloram	10.995	0.000	12667886	0	2.481	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061820\
Data File : PS010855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 03:03
Operator : DD\AJ
Sample : L3024-23
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RO-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:35:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

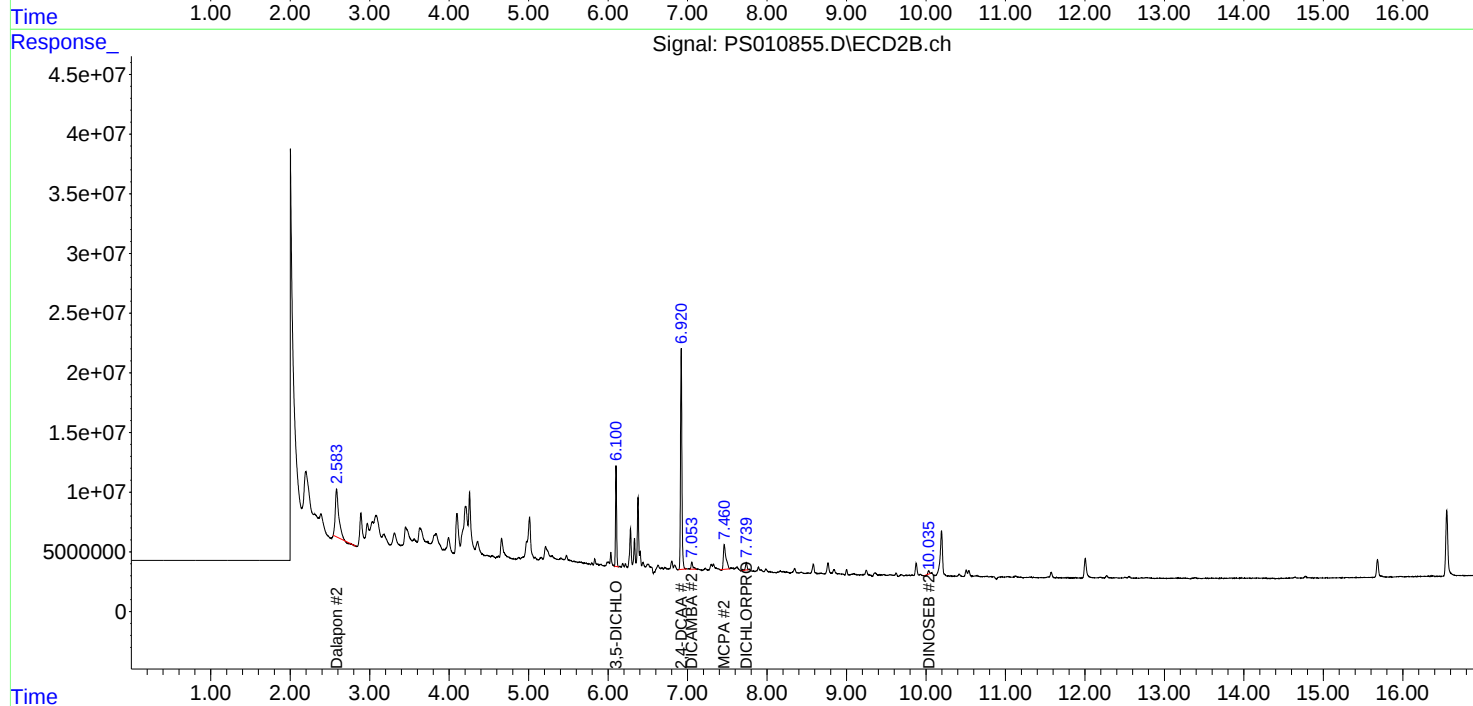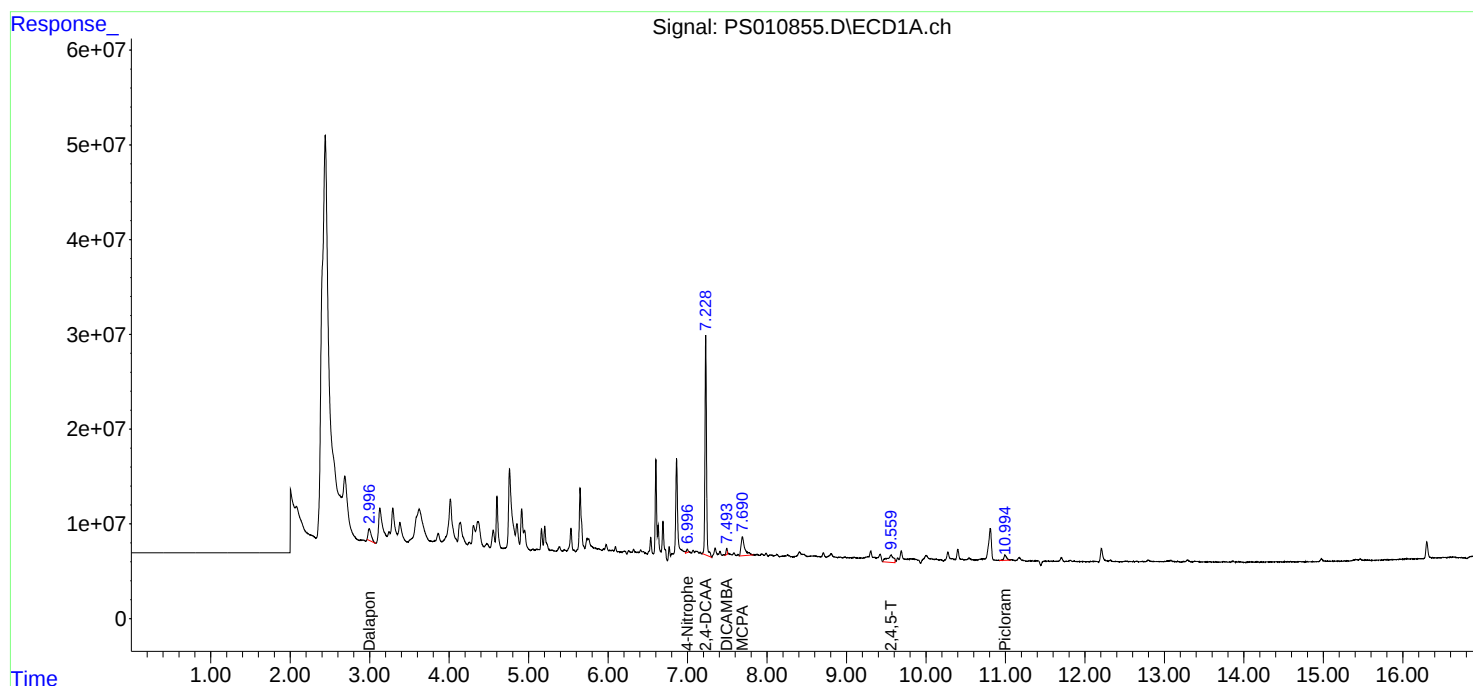


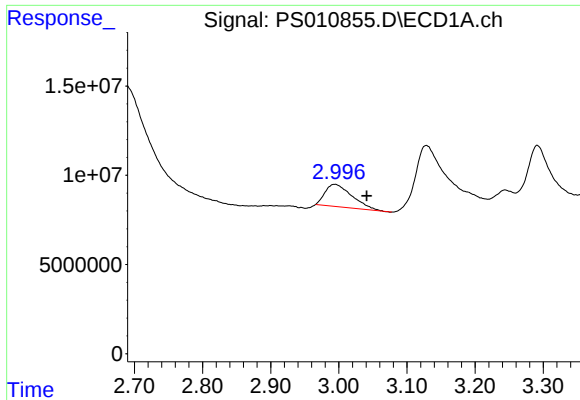

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.047 min
Response: 34335916
Conc: 34.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-11

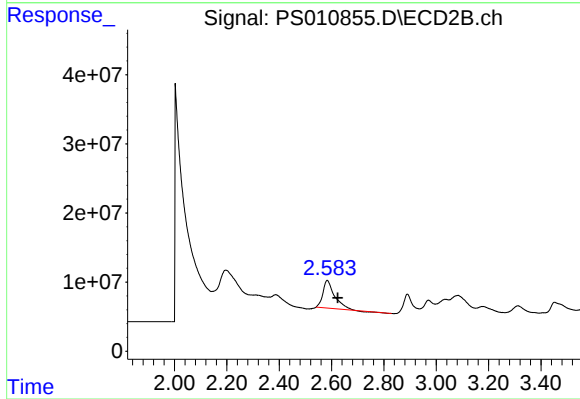


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.040 min
Response: 121693718
Conc: 166.22 ng/ml

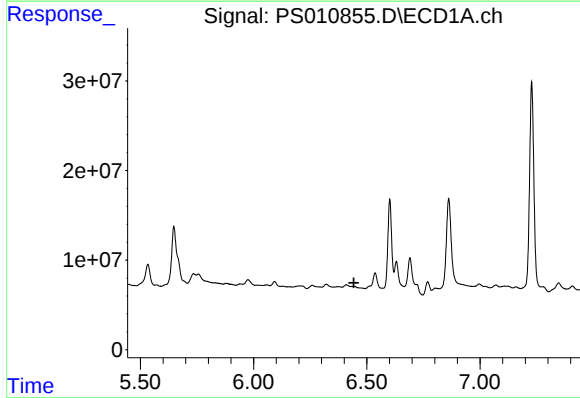


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

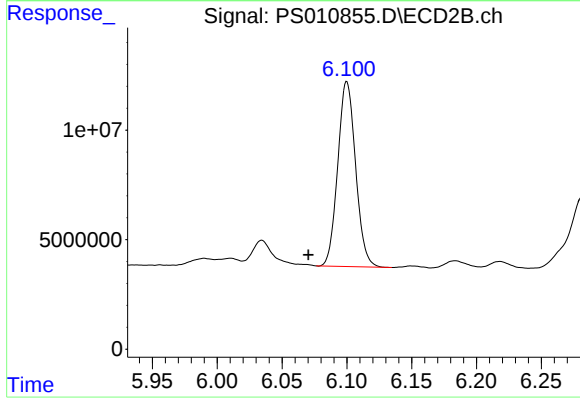

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 81003832
Conc: 98.83 ng/ml

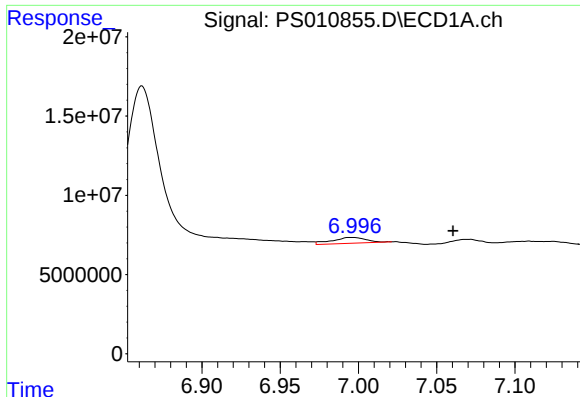

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.064 min
Response: 5727343
Conc: 15.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-11

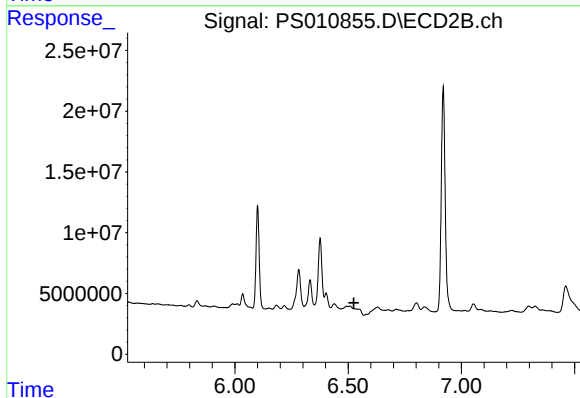


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

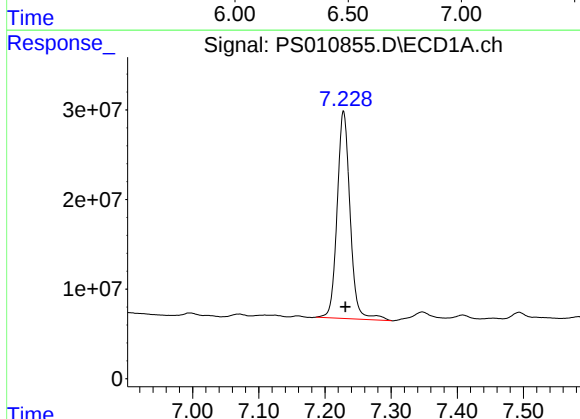


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.003 min
Response: 315115781
Conc: 398.45 ng/ml

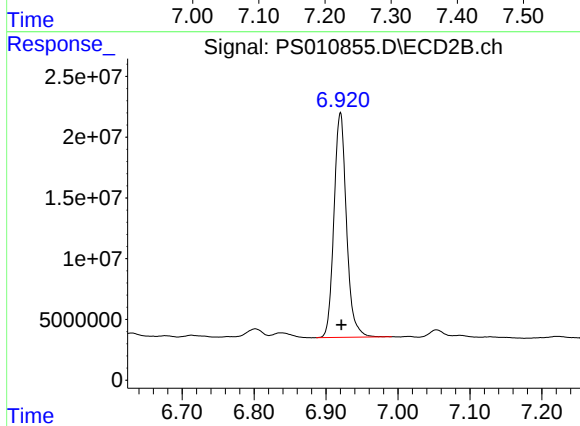

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 223573488
Conc: 409.91 ng/ml

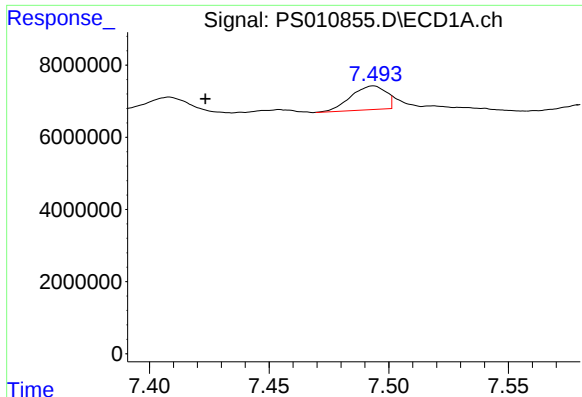

#5 DICAMBA


R.T.: 7.493 min
Delta R.T.: 0.070 min
Response: 6812925
Conc: 2.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-11

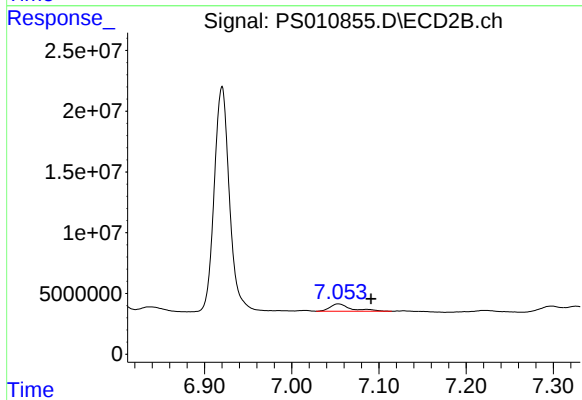


#5 DICAMBA

R.T.: 7.053 min
Delta R.T.: -0.038 min
Response: 10019763
Conc: 4.45 ng/ml

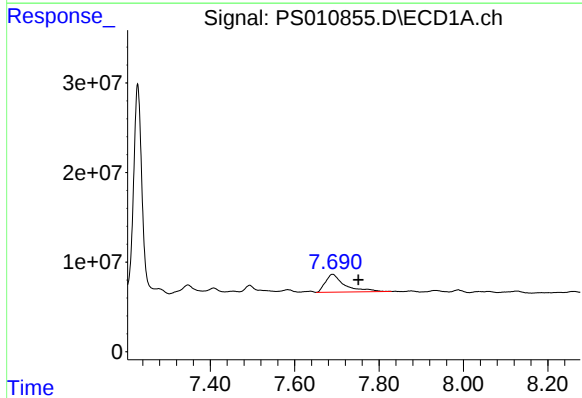


#7 MCPA

R.T.: 7.690 min
Delta R.T.: -0.061 min
Response: 63667968
Conc: 18.21 ug/ml

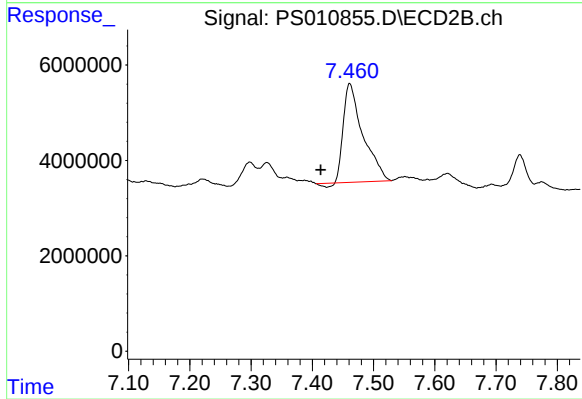

#7 MCPA


R.T.: 7.461 min
Delta R.T.: 0.048 min
Response: 45731384
Conc: 16.83 ug/ml

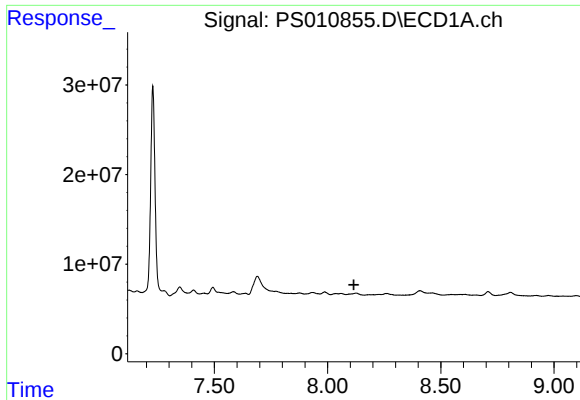

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-11

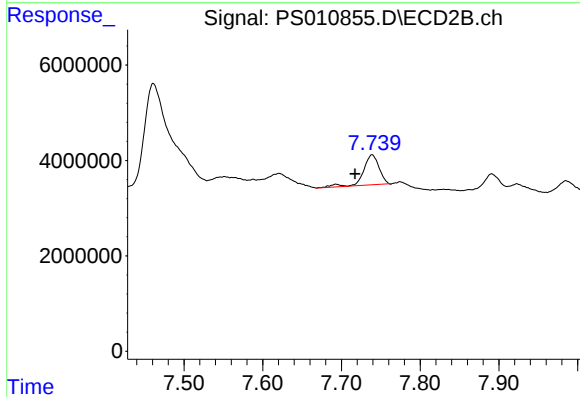


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.022 min
Response: 8721090
Conc: 15.12 ng/ml

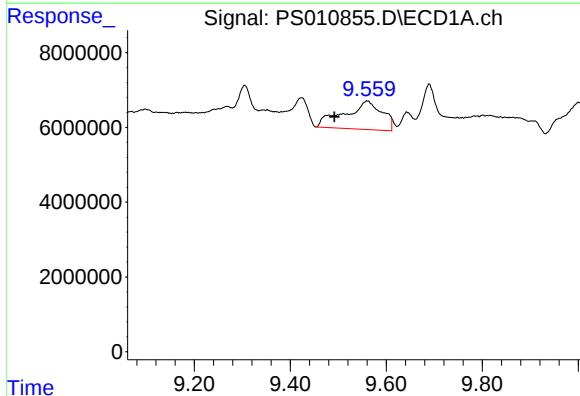


#12 2,4,5-T

R.T.: 9.560 min
Delta R.T.: 0.068 min
Response: 41190576
Conc: 10.13 ng/ml

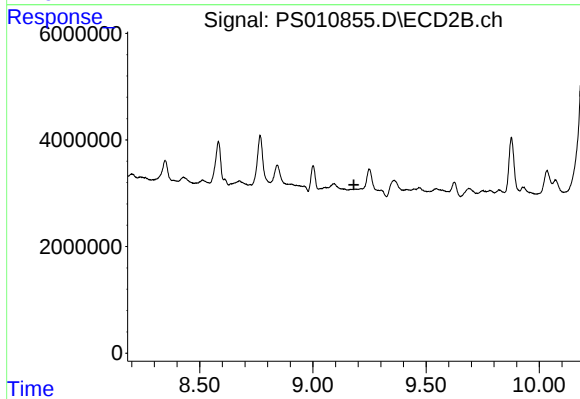

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

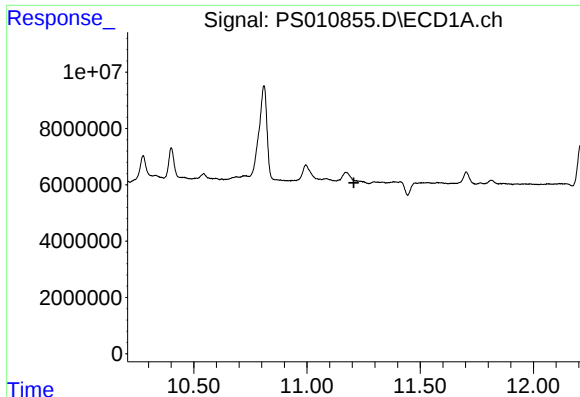

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-11

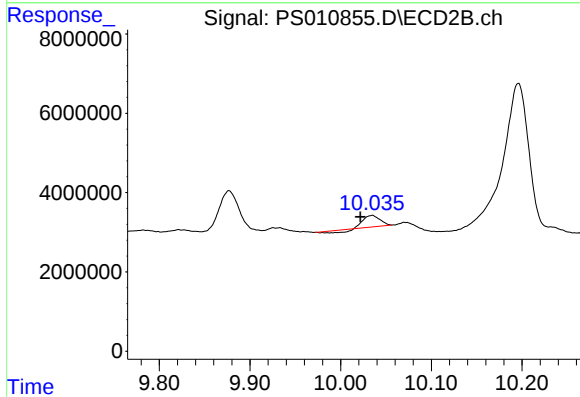


#14 DINOSEB

R.T.: 10.034 min
Delta R.T.: 0.012 min
Response: 2862279
Conc: 1.33 ng/ml

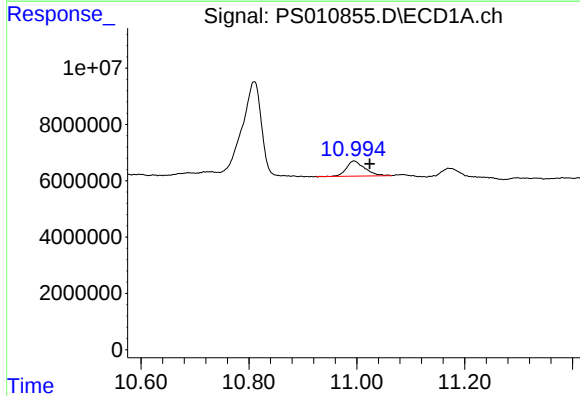

#15 Picloram

R.T.: 10.995 min
Delta R.T.: -0.029 min
Response: 12667886
Conc: 2.48 ng/ml

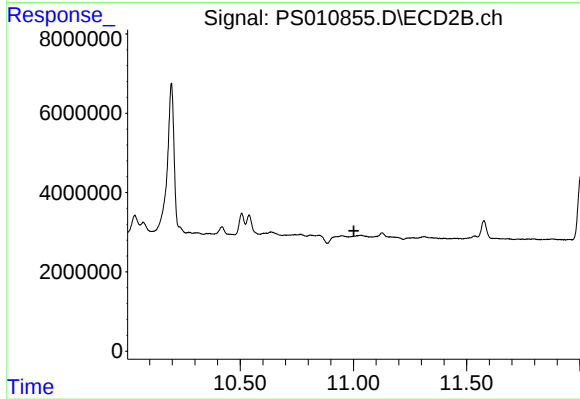

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.002 min
Response: 0
Conc: N.D.