

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS061821\  
 Data File : PS015788.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Jun 2021 21:34  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 18 23:20:09 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS061521.M  
 Quant Title : 8080.M  
 QLast Update : Tue Jun 15 18:15:49 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm



|                             | Compound | RT#1   | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|--------|-------|----------|---------|---------|---------|
| -----                       |          |        |       |          |         |         |         |
| System Monitoring Compounds |          |        |       |          |         |         |         |
| 4) S                        | 2,4-DCAA | 7.190  | 6.767 | 813.6E6  | 282.1E6 | 489.678 | 559.961 |
| Target Compounds            |          |        |       |          |         |         |         |
| 15) T                       | Picloram | 10.980 | 0.000 | 18147537 | 0       | 1.327   | N.D. #  |
| -----                       |          |        |       |          |         |         |         |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS061821\  
Data File : PS015788.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Jun 2021 21:34  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 18 23:20:09 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS061521.M  
Quant Title : 8080.M  
QLast Update : Tue Jun 15 18:15:49 2021  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

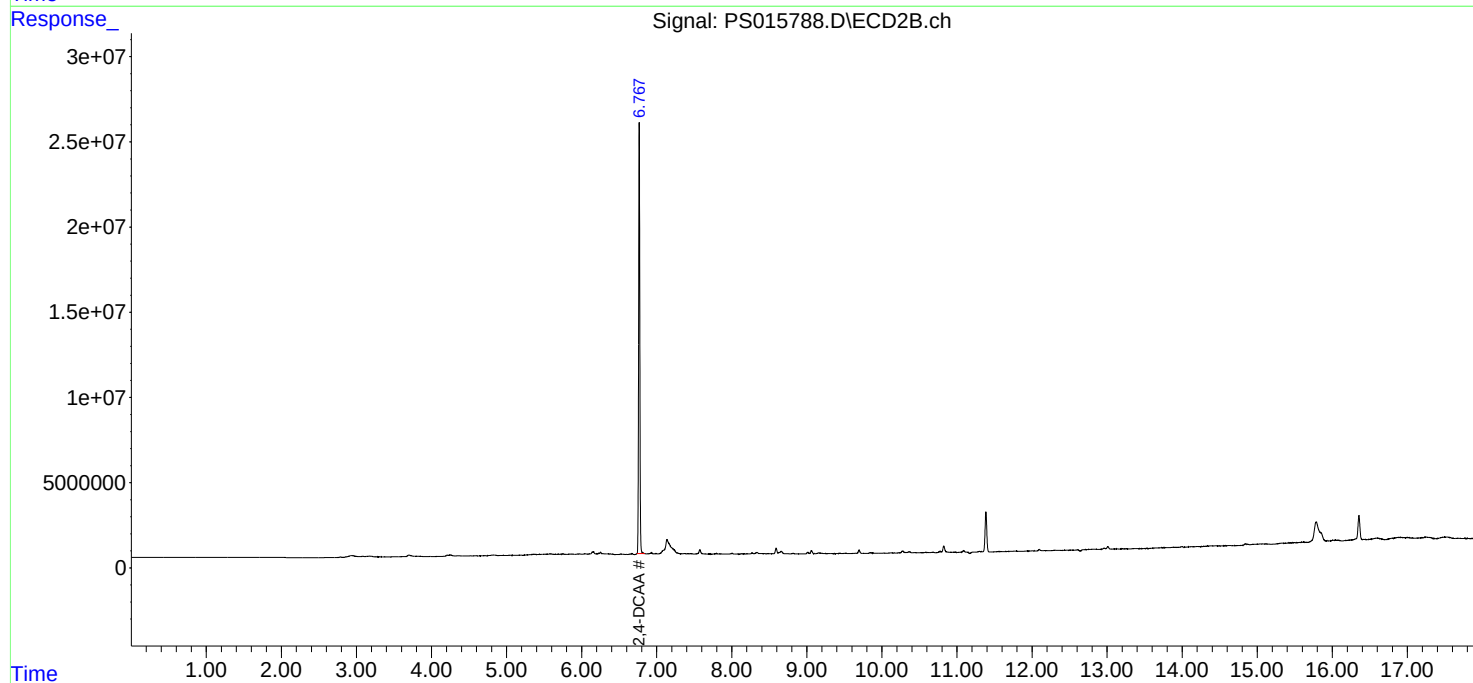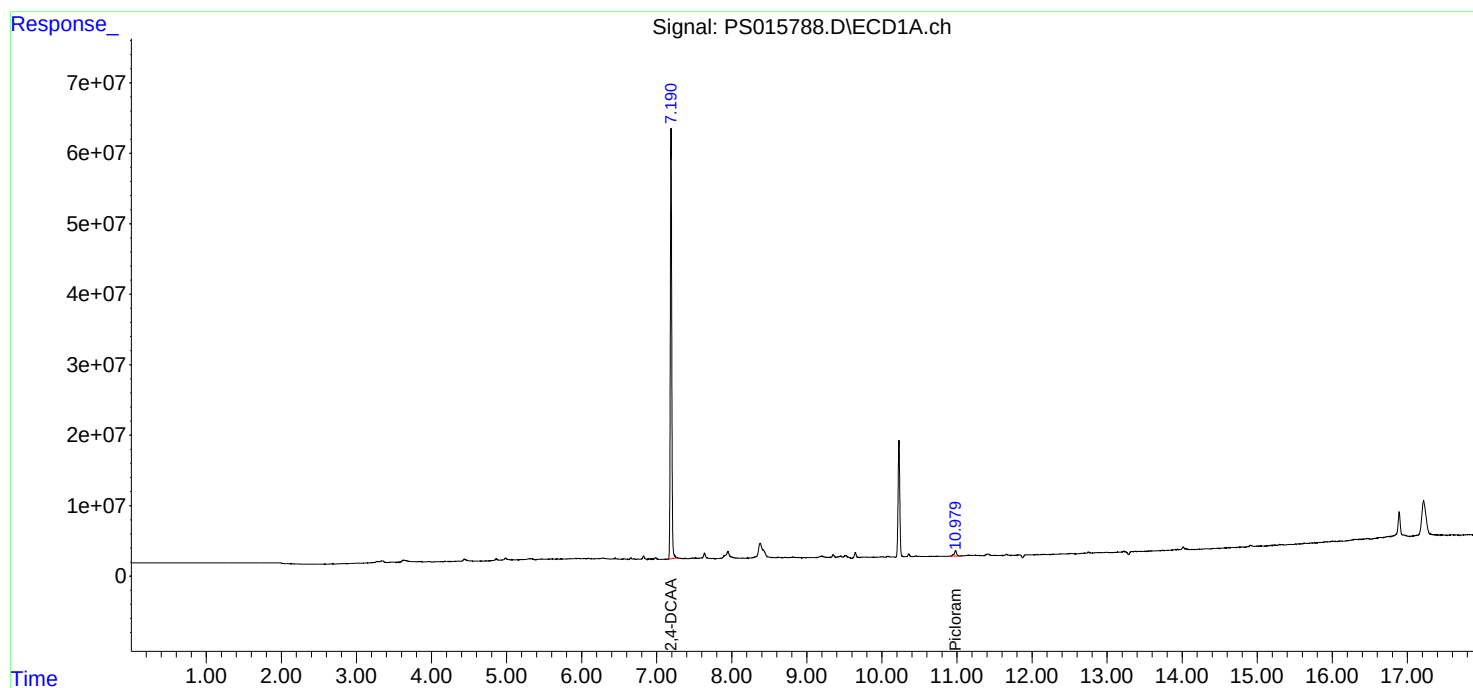

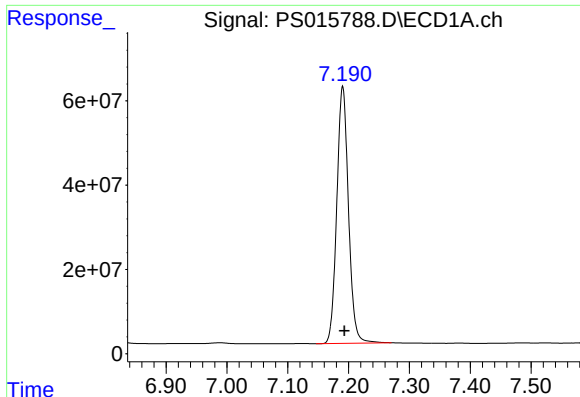


#4 2,4-DCAA

R.T.: 7.190 min  
Delta R.T.: -0.003 min  
Response: 813574626  
Conc: 489.68 ng/ml

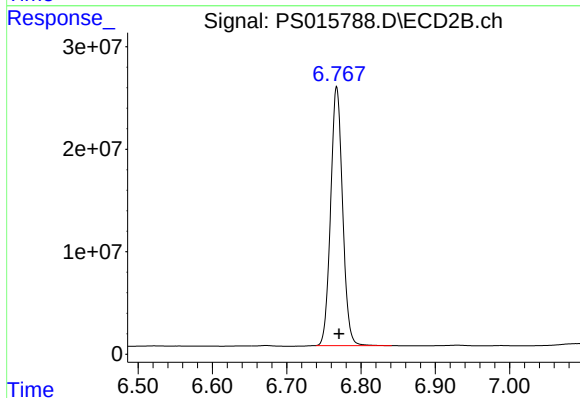


#4 2,4-DCAA

R.T.: 6.767 min  
Delta R.T.: -0.003 min  
Response: 282137417  
Conc: 559.96 ng/ml

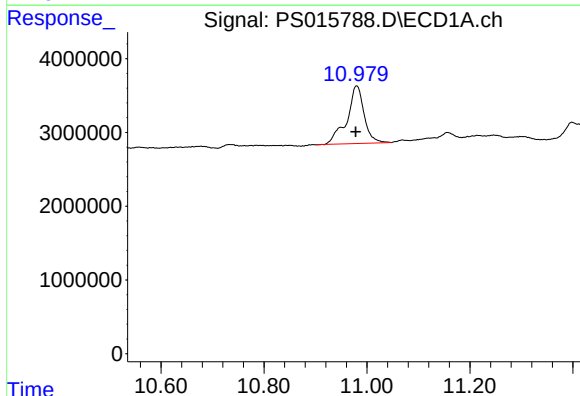

#15 Picloram

R.T.: 10.980 min  
Delta R.T.: 0.002 min  
Response: 18147537  
Conc: 1.33 ng/ml

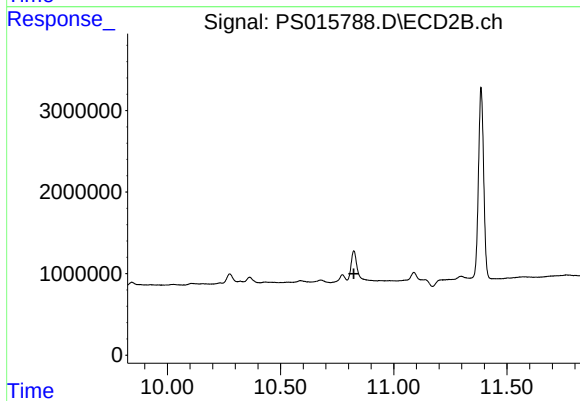

#15 Picloram

R.T.: 0.000 min  
Exp R.T.: 10.824 min  
Response: 0  
Conc: N.D.