

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
 Data File : PS015806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2021 04:49
 Operator : DD\AJ
 Sample : PB137081BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 05:33:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.191	6.767	767.1E6	261.5E6	461.722	518.990
Target Compounds							
3) T	4-Nitroph...	6.992	0.000	3380507	0	3.718	N.D. #
5) T	DICAMBA	7.382	0.000	6979519	0	1.086	N.D. #
8) T	DICHLORPROP	8.076	0.000	3044128	0	1.923	N.D. #
9) T	2,4-D	8.310	0.000	11503842	0	6.564	N.D. #
10) T	Pentachlo...	8.612	0.000	7385726	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.163	0.000	9229493	0	1.056	N.D. #
12) T	2,4,5-T	9.449	9.010	38254488	10694788	4.333	3.792
13) T	2,4-DB	9.996	0.000	35013505	0	17.117	N.D. #
14) T	DINOSEB	11.156	0.000	21631834	0	3.340	N.D. #
15) T	Picloram	10.976	10.819	630.4E6	232.5E6	46.113	55.290
16) T	DCPA	11.423	10.772	28738066	11035207	2.173	2.625


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
Data File : PS015806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2021 04:49
Operator : DD\AJ
Sample : PB137081BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 05:33:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

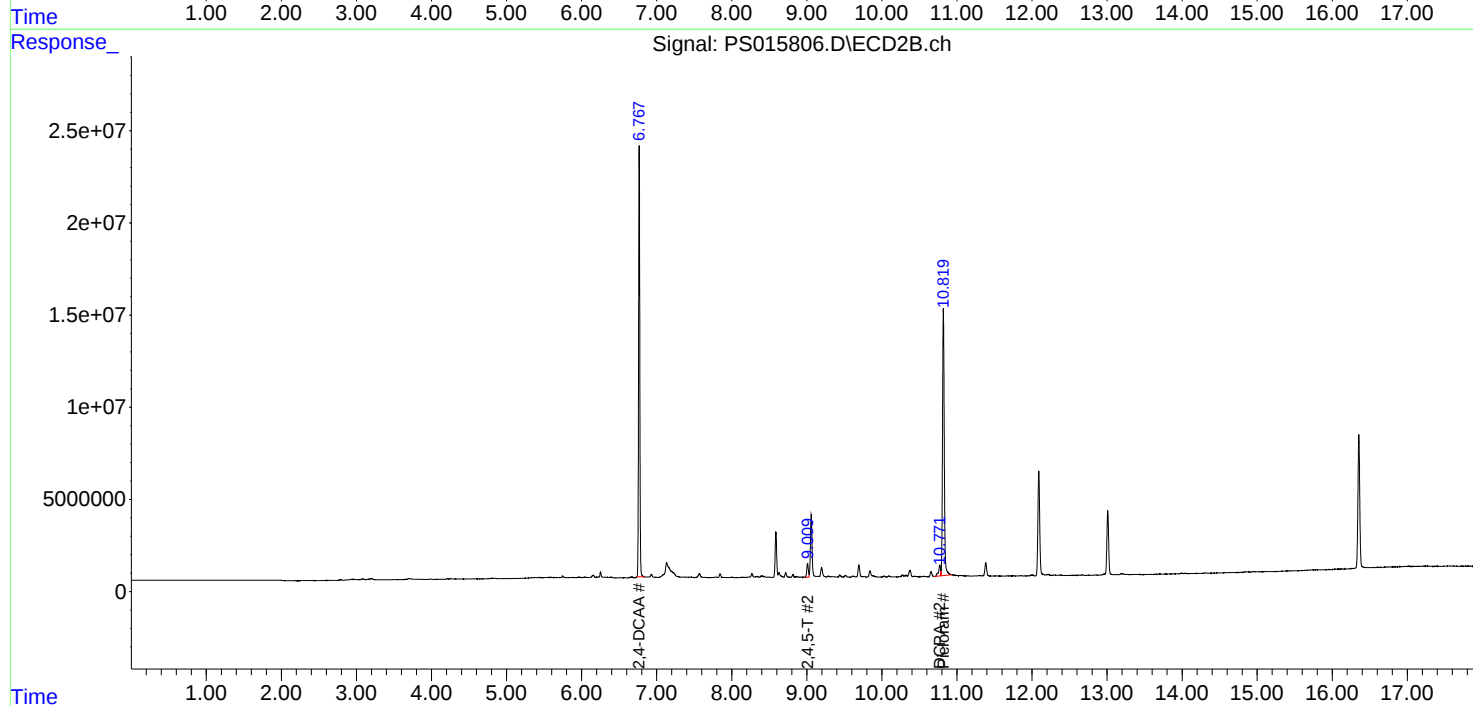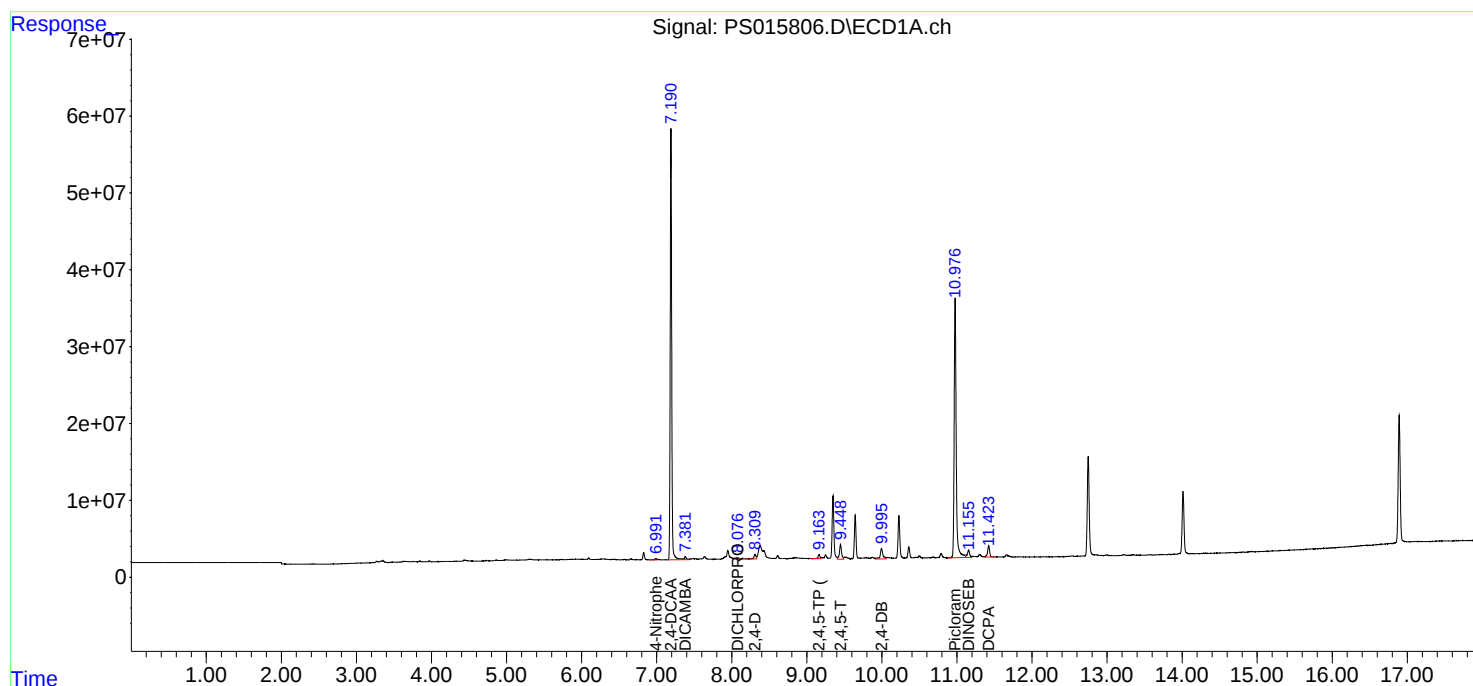

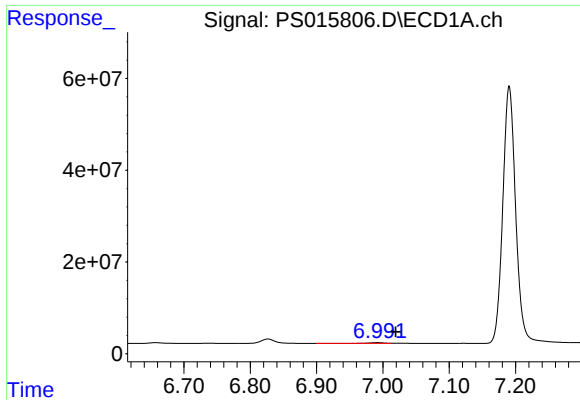


#3 4-Nitrophenol

R.T.: 6.992 min
Delta R.T.: -0.027 min
Response: 3380507
Conc: 3.72 ng/ml

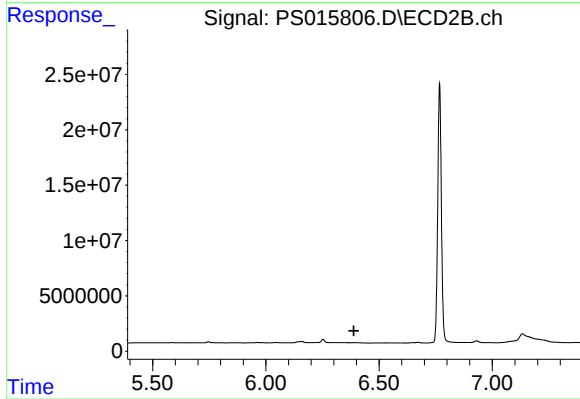


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

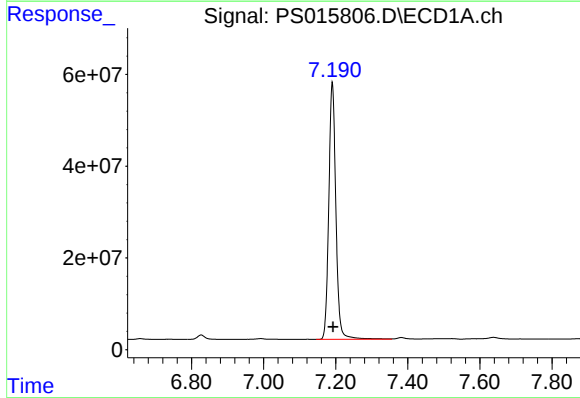


#4 2,4-DCAA

R.T.: 7.191 min
Delta R.T.: -0.002 min
Response: 767126260
Conc: 461.72 ng/ml

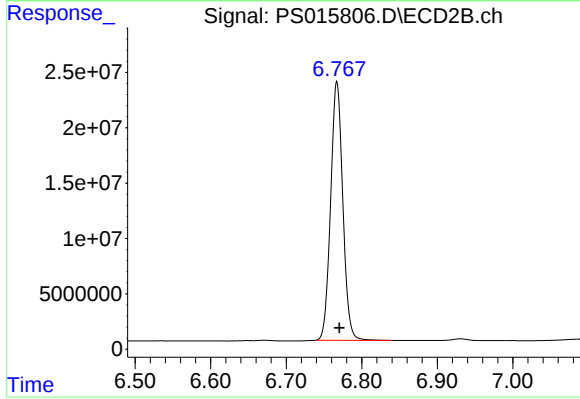


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: -0.003 min
Response: 261494237
Conc: 518.99 ng/ml

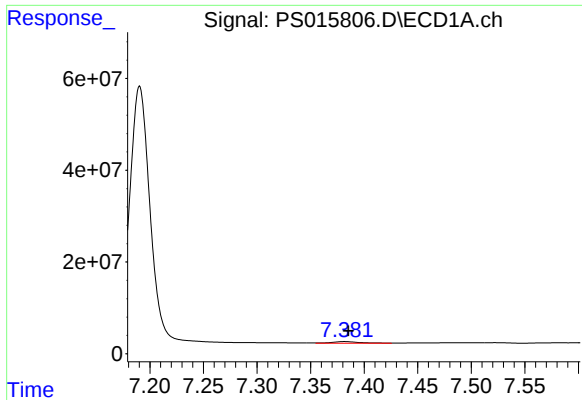


#5 DICAMBA

R.T.: 7.382 min
Delta R.T.: -0.003 min
Response: 6979519
Conc: 1.09 ng/ml

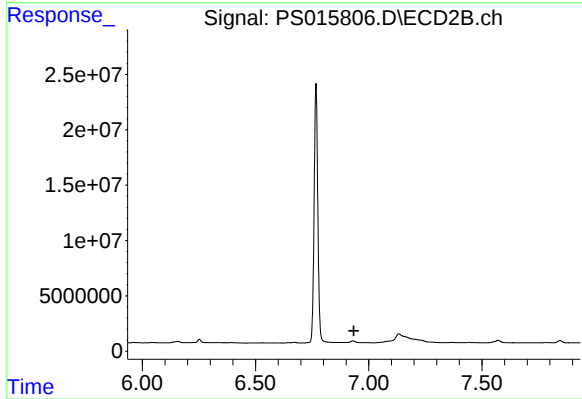


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.935 min
Response: 0
Conc: N.D.

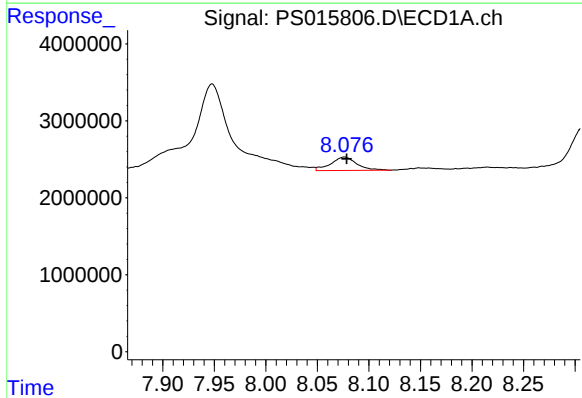


#8 DICHLORPROP

R.T.: 8.076 min
Delta R.T.: -0.002 min
Response: 3044128
Conc: 1.92 ng/ml

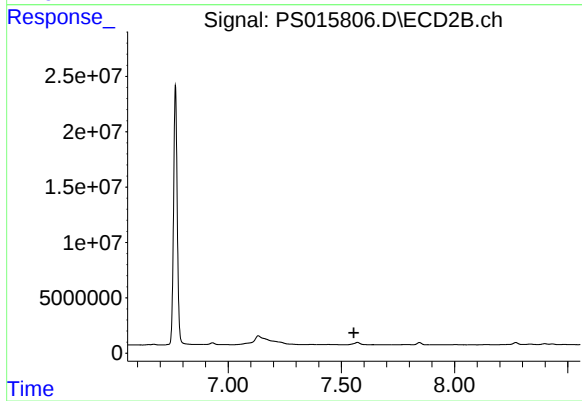


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.555 min
Response: 0
Conc: N.D.

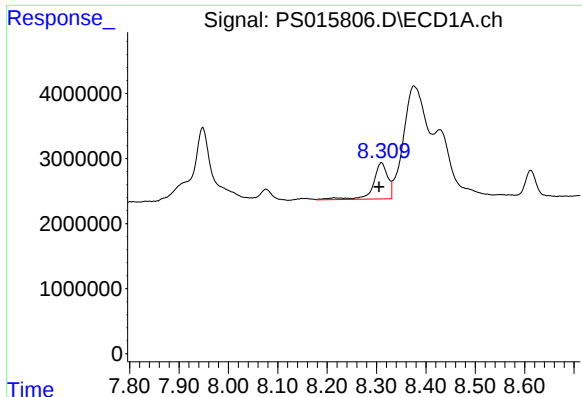


#9 2,4-D

R.T.: 8.310 min
Delta R.T.: 0.004 min
Response: 11503842
Conc: 6.56 ng/ml

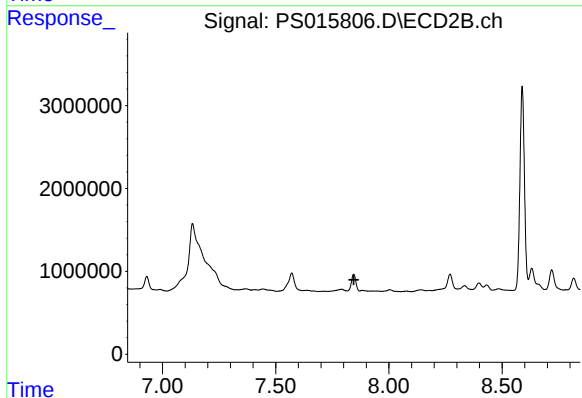


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.845 min
Response: 0
Conc: N.D.

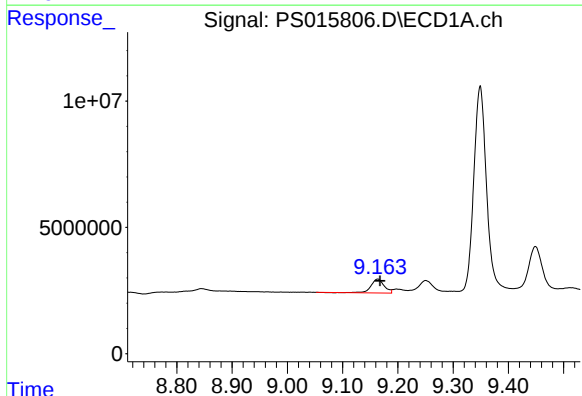


#11 2,4,5-TP (SILVEX)

R.T.: 9.163 min
Delta R.T.: -0.005 min
Response: 9229493
Conc: 1.06 ng/ml

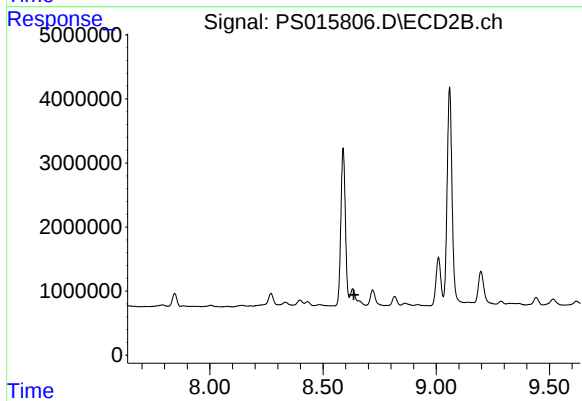


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.636 min
Response: 0
Conc: N.D.

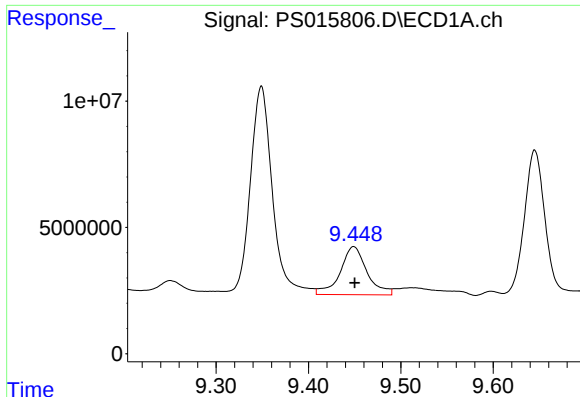


#12 2,4,5-T

R.T.: 9.449 min
Delta R.T.: -0.001 min
Response: 38254488
Conc: 4.33 ng/ml

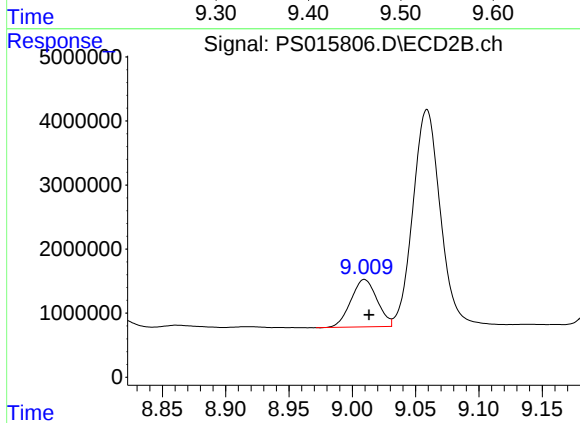


#12 2,4,5-T

R.T.: 9.010 min
Delta R.T.: -0.003 min
Response: 10694788
Conc: 3.79 ng/ml

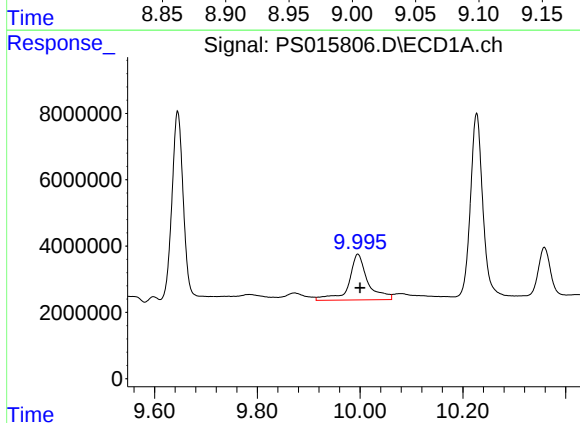


#13 2,4-DB

R.T.: 9.996 min
Delta R.T.: -0.004 min
Response: 35013505
Conc: 17.12 ng/ml

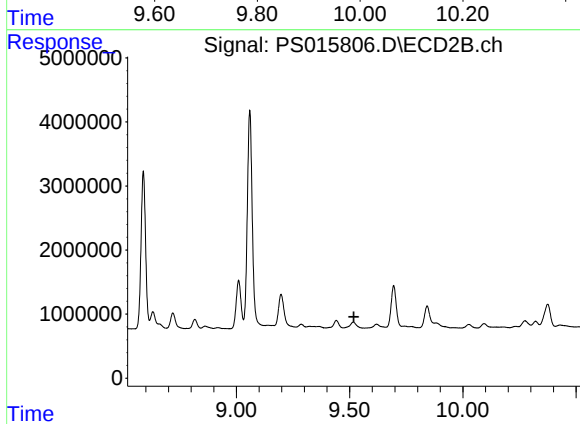


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.519 min
Response: 0
Conc: N.D.

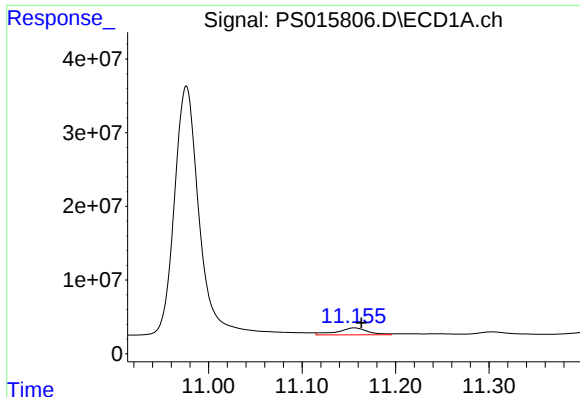


#14 DINOSEB

R.T.: 11.156 min
Delta R.T.: -0.007 min
Response: 21631834
Conc: 3.34 ng/ml

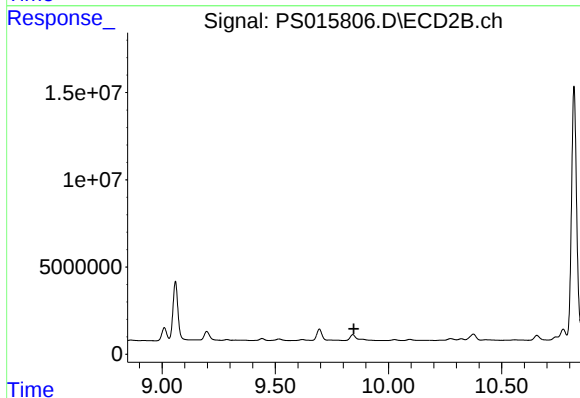


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.847 min
Response: 0
Conc: N.D.

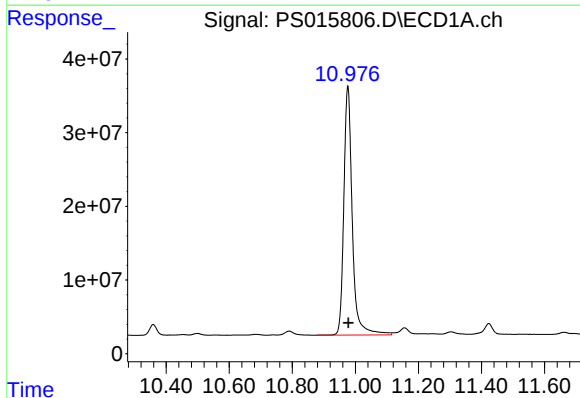


#15 Picloram

R.T.: 10.976 min
Delta R.T.: -0.002 min
Response: 630405118
Conc: 46.11 ng/ml

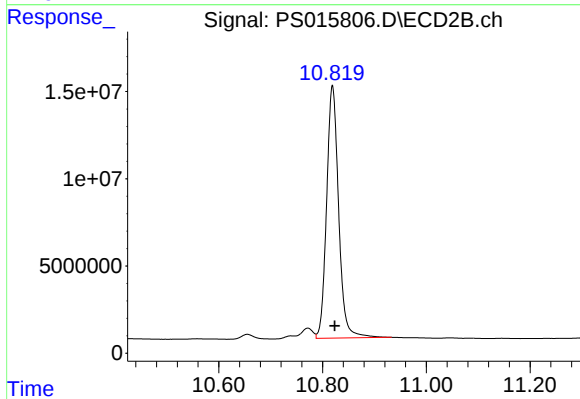


#15 Picloram

R.T.: 10.819 min
Delta R.T.: -0.005 min
Response: 232527067
Conc: 55.29 ng/ml

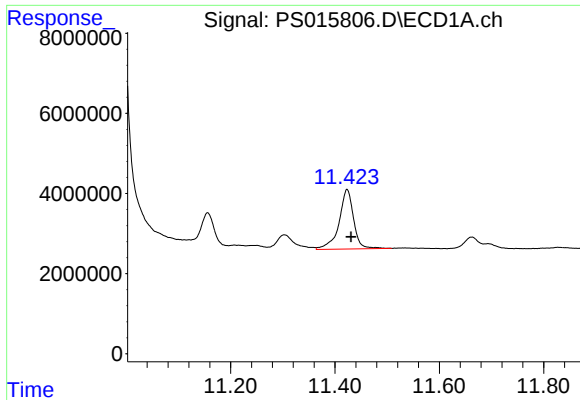

#16 DCPA

R.T.: 11.423 min
Delta R.T.: -0.008 min
Response: 28738066
Conc: 2.17 ng/ml

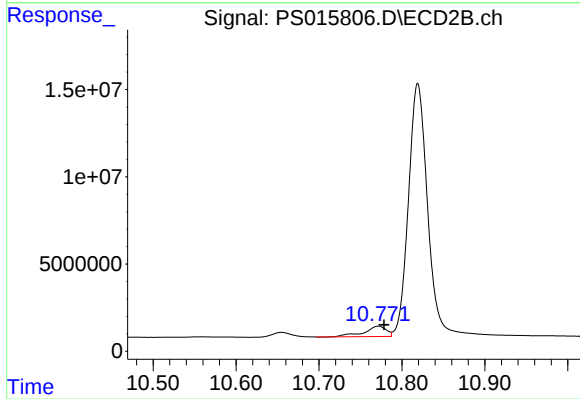

#16 DCPA

R.T.: 10.772 min
Delta R.T.: -0.007 min
Response: 11035207
Conc: 2.62 ng/ml