

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
 Data File : PS015811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2021 06:50
 Operator : DD\AJ
 Sample : PB137147BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 09:06:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.190	6.767	782.2E6	266.1E6	470.822	528.209
Target Compounds							
3) T	4-Nitroph...	6.992	0.000	2882968	0	3.171	N.D. #
5) T	DICAMBA	7.382	0.000	9045590	0	1.407	N.D. #
8) T	DICHLORPROP	8.076	0.000	3548673	0	2.241	N.D. #
9) T	2,4-D	8.309	0.000	11786971	0	6.726	N.D. #
10) T	Pentachlo...	8.613	0.000	7040310	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.164	0.000	13063893	0	1.495	N.D. #
12) T	2,4,5-T	9.449	9.009	45318678	12889796	5.133	4.570
13) T	2,4-DB	9.997	0.000	45463672	0	22.226	N.D. #
14) T	DINOSEB	11.156	0.000	23573230	0	3.640	N.D. #
15) T	Picloram	10.976	10.819	736.3E6	273.6E6	53.856	65.046
16) T	DCPA	11.424	10.771	31316538	13042277	2.368	3.102 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
Data File : PS015811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2021 06:50
Operator : DD\AJ
Sample : PB137147BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 09:06:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

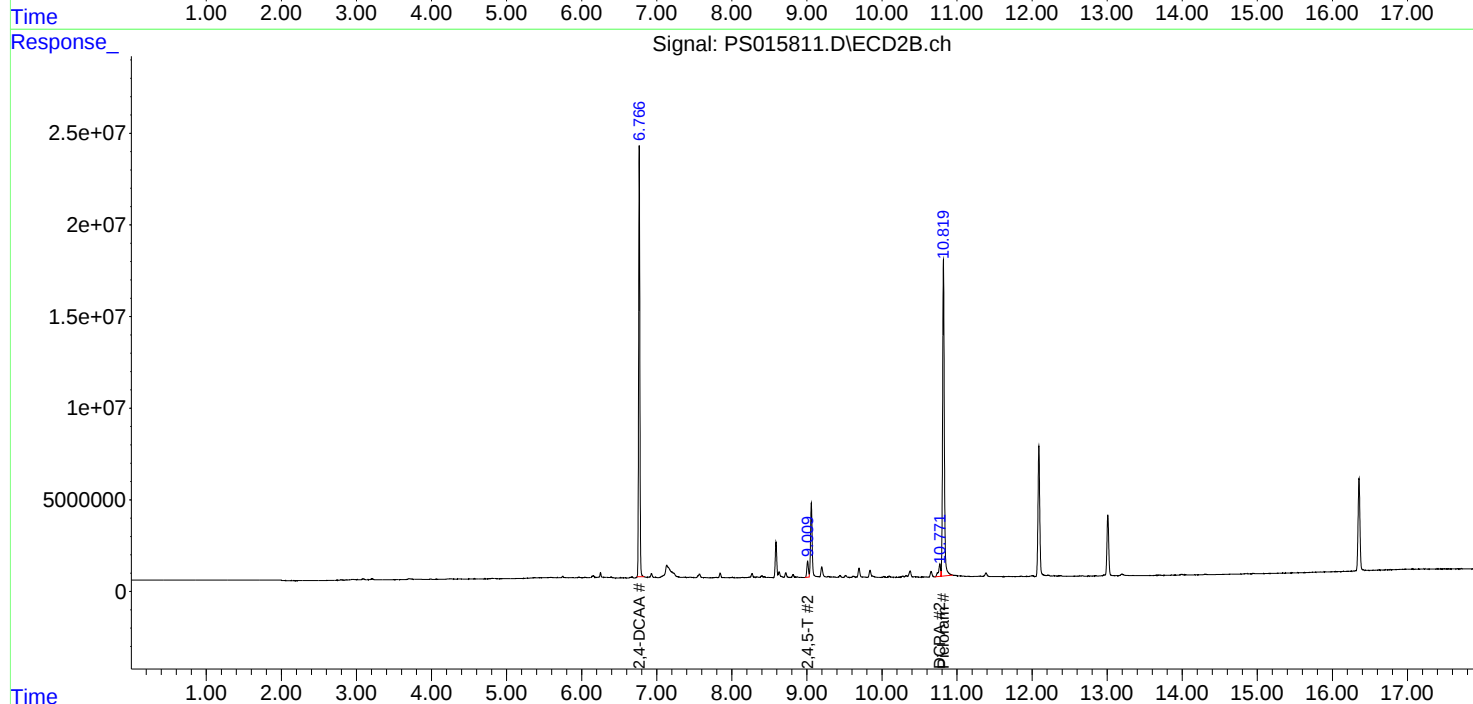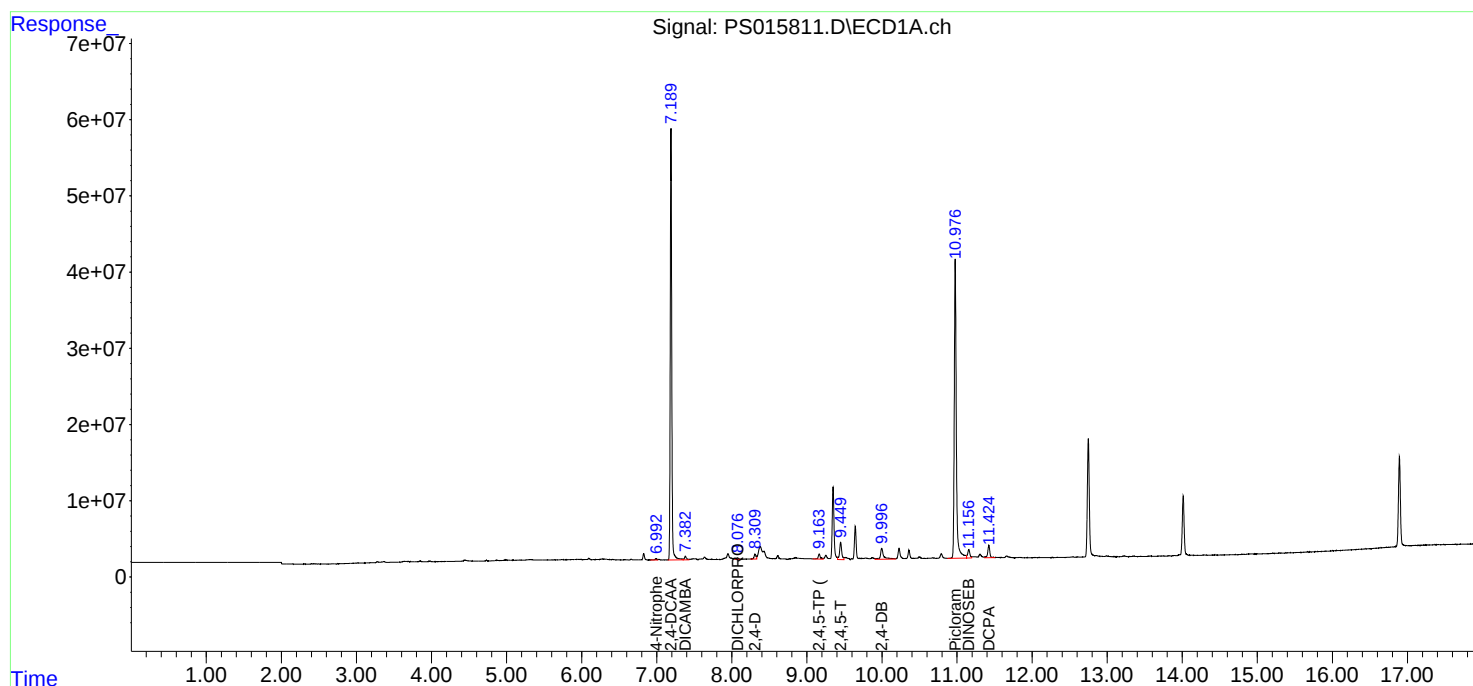

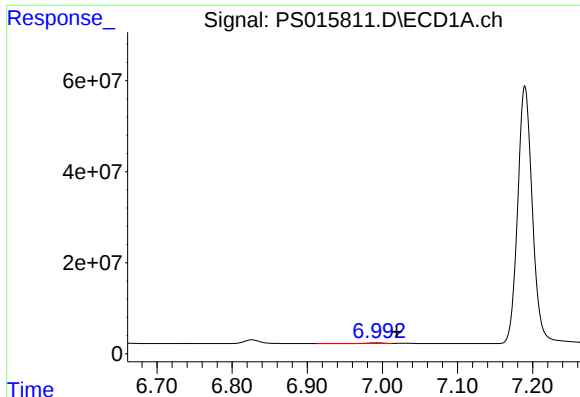


#3 4-Nitrophenol

R.T.: 6.992 min
Delta R.T.: -0.027 min
Response: 2882968
Conc: 3.17 ng/ml

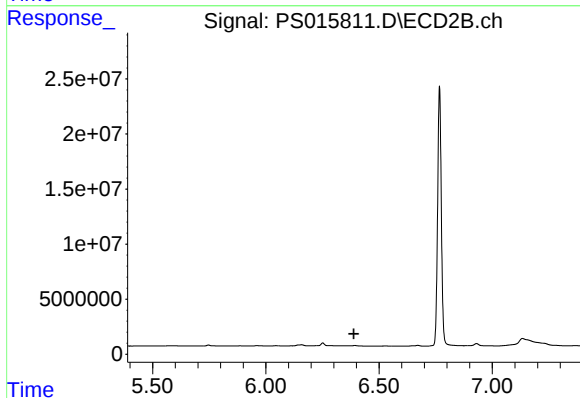


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

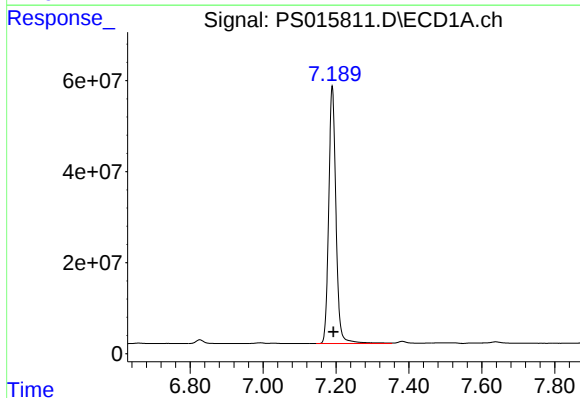


#4 2,4-DCAA

R.T.: 7.190 min
Delta R.T.: -0.003 min
Response: 782246481
Conc: 470.82 ng/ml

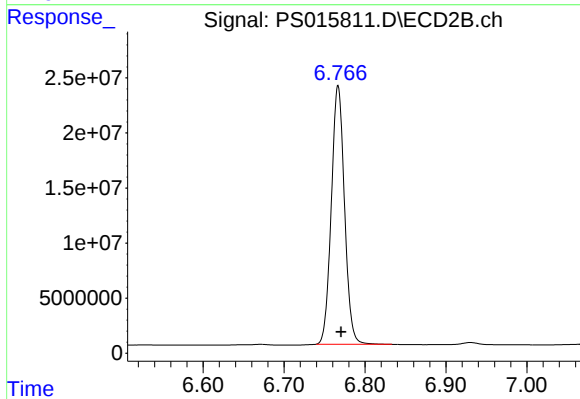


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: -0.004 min
Response: 266139055
Conc: 528.21 ng/ml

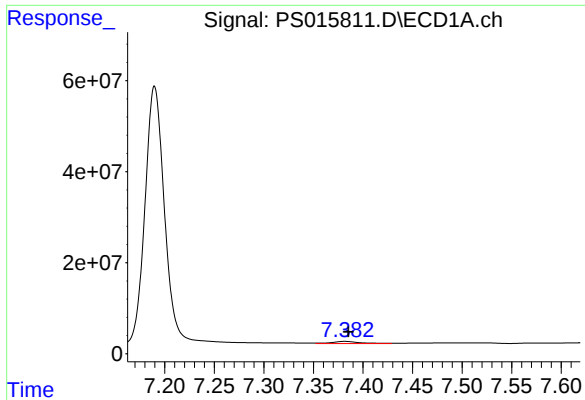


#5 DICAMBA

R.T.: 7.382 min
Delta R.T.: -0.003 min
Response: 9045590
Conc: 1.41 ng/ml

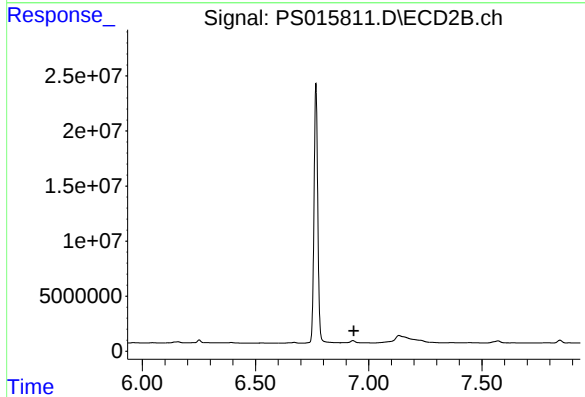


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.935 min
Response: 0
Conc: N.D.

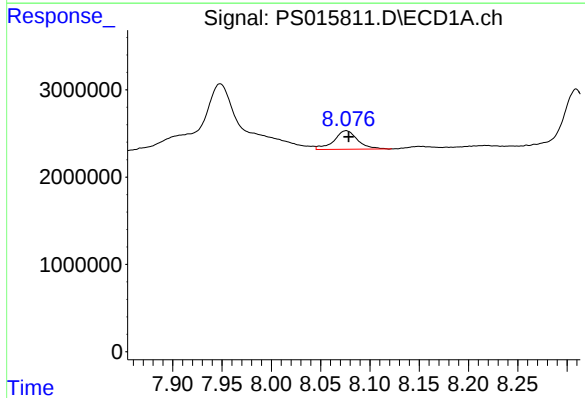


#8 DICHLORPROP

R.T.: 8.076 min
Delta R.T.: -0.003 min
Response: 3548673
Conc: 2.24 ng/ml

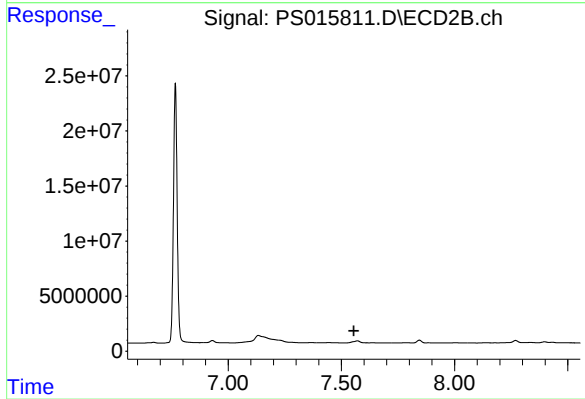


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.555 min
Response: 0
Conc: N.D.

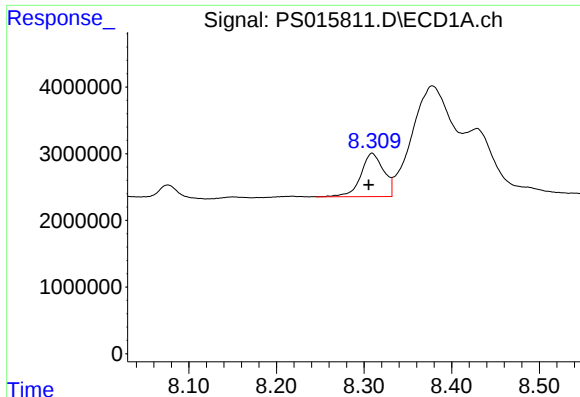


#9 2,4-D

R.T.: 8.309 min
Delta R.T.: 0.004 min
Response: 11786971
Conc: 6.73 ng/ml

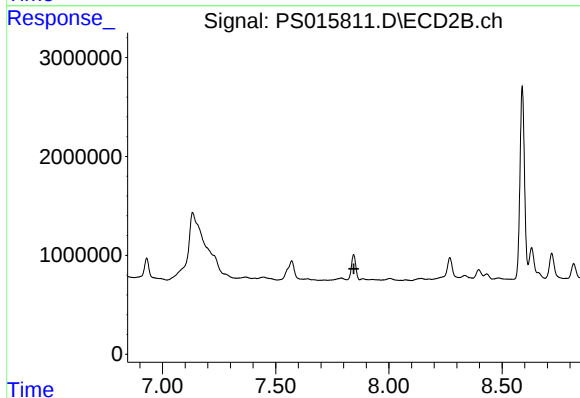


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.845 min
Response: 0
Conc: N.D.

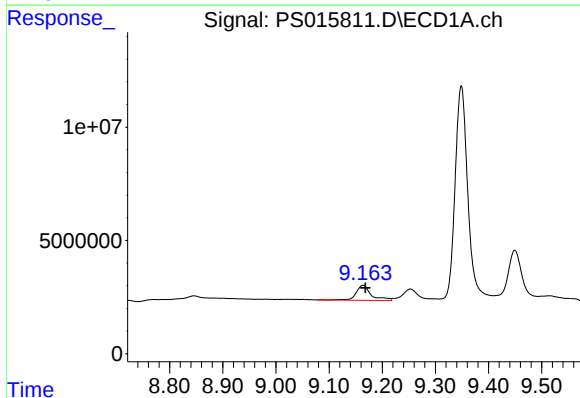


#11 2,4,5-TP (SILVEX)

R.T.: 9.164 min
Delta R.T.: -0.004 min
Response: 13063893
Conc: 1.49 ng/ml

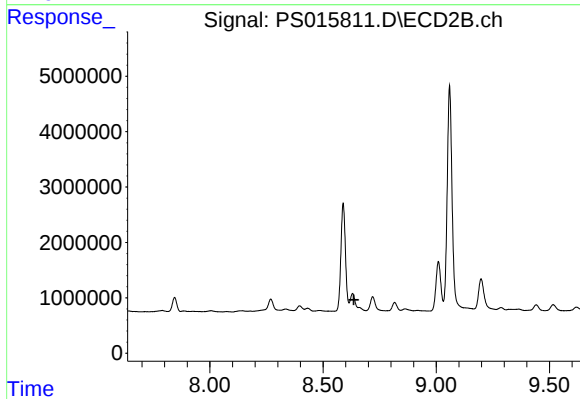


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.636 min
Response: 0
Conc: N.D.

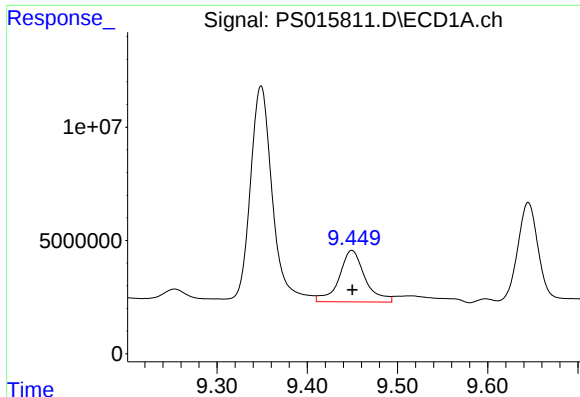


#12 2,4,5-T

R.T.: 9.449 min
Delta R.T.: 0.000 min
Response: 45318678
Conc: 5.13 ng/ml

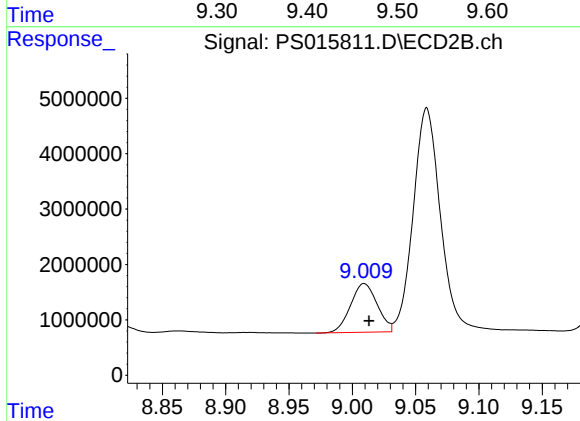


#12 2,4,5-T

R.T.: 9.009 min
Delta R.T.: -0.004 min
Response: 12889796
Conc: 4.57 ng/ml

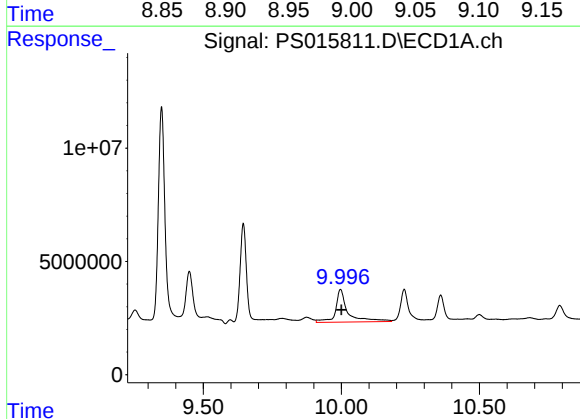


#13 2,4-DB

R.T.: 9.997 min
Delta R.T.: -0.003 min
Response: 45463672
Conc: 22.23 ng/ml

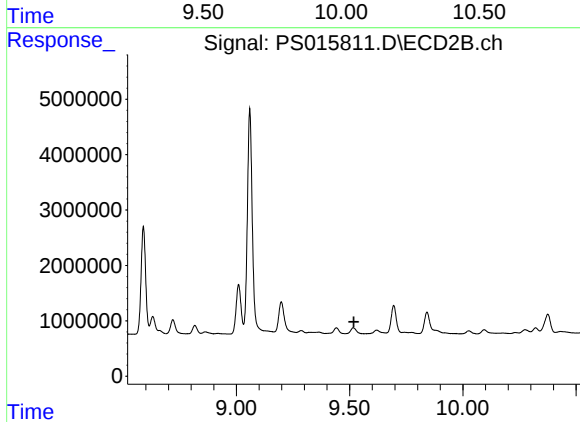


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.519 min
Response: 0
Conc: N.D.

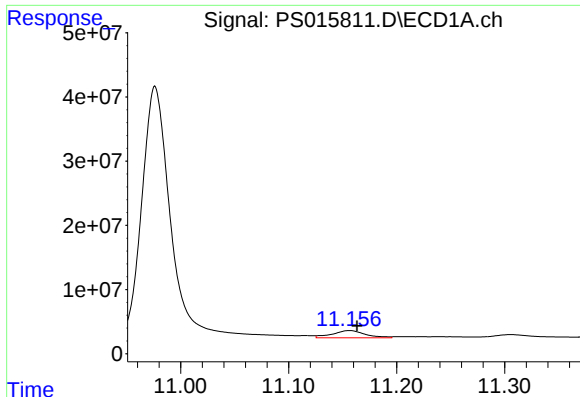


#14 DINOSEB

R.T.: 11.156 min
Delta R.T.: -0.007 min
Response: 23573230
Conc: 3.64 ng/ml

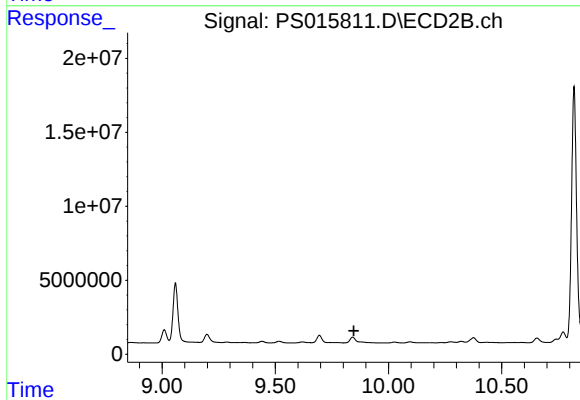


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.847 min
Response: 0
Conc: N.D.

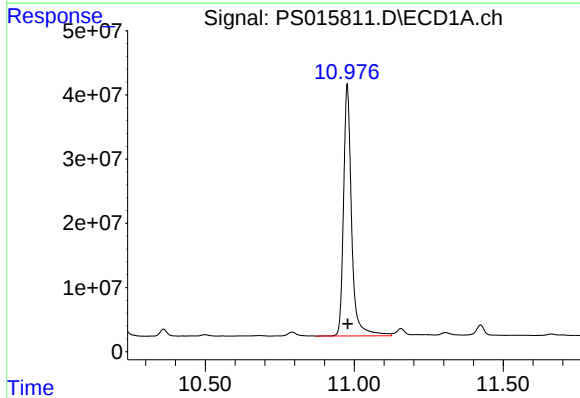


#15 Picloram

R.T.: 10.976 min
Delta R.T.: -0.002 min
Response: 736251539
Conc: 53.86 ng/ml

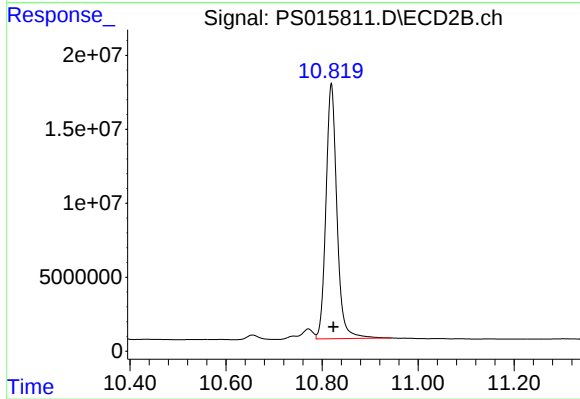


#15 Picloram

R.T.: 10.819 min
Delta R.T.: -0.005 min
Response: 273553552
Conc: 65.05 ng/ml

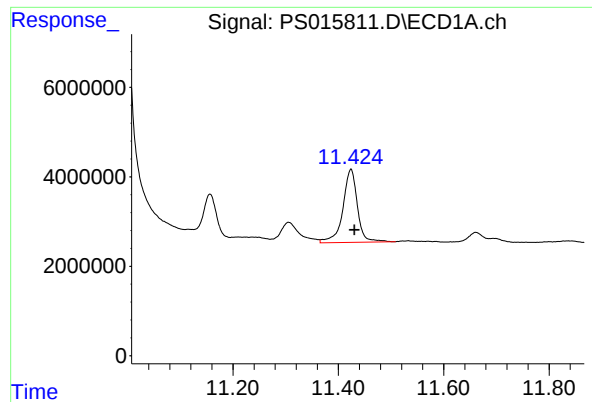

#16 DCPA

R.T.: 11.424 min
Delta R.T.: -0.007 min
Response: 31316538
Conc: 2.37 ng/ml

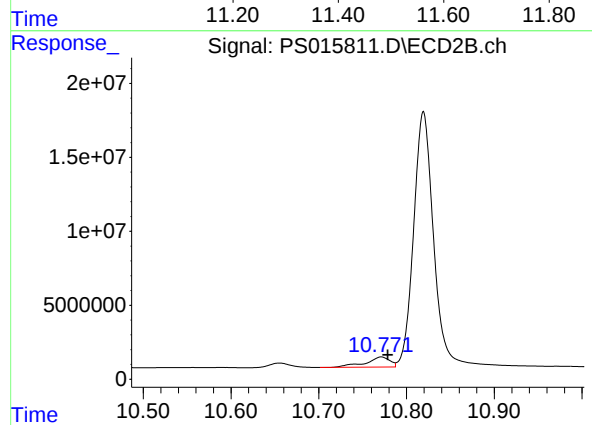

#16 DCPA

R.T.: 10.771 min
Delta R.T.: -0.007 min
Response: 13042277
Conc: 3.10 ng/ml