

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
 Data File : PS015812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2021 07:14
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 09:04:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.190	6.767	861.0E6	294.4E6	518.206	584.213
Target Compounds							
2) T	3,5-DICHL...	6.444	0.000	4212836	0	1.877	N.D. #
3) T	4-Nitroph...	6.986	0.000	5163269	0	5.679	N.D. #
5) T	DICAMBA	7.381	0.000	10059007	0	1.565	N.D. #
6) T	MCP	7.521f	0.000	2811834	0	<MDL	N.D. #
8) T	DICHLORPROP	8.076	0.000	4597822	0	2.904	N.D. #
9) T	2,4-D	8.310	0.000	13839956	0	7.897	N.D. #
10) T	Pentachlo...	8.613	0.000	6875006	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.163	0.000	17355398	0	1.985	N.D. #
12) T	2,4,5-T	9.449	9.010	52322616	15211115	5.927	5.393
13) T	2,4-DB	9.997	0.000	44979405	0	21.989	N.D. #
14) T	DINOSEB	11.156	9.841	30978730	6944578	4.783	3.448 #
15) T	Picloram	10.976	10.819	632.8E6	233.7E6	46.291	55.558
16) T	DCPA	11.423	10.771	39461796	17174355	2.984	4.085 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
Data File : PS015812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2021 07:14
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 09:04:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

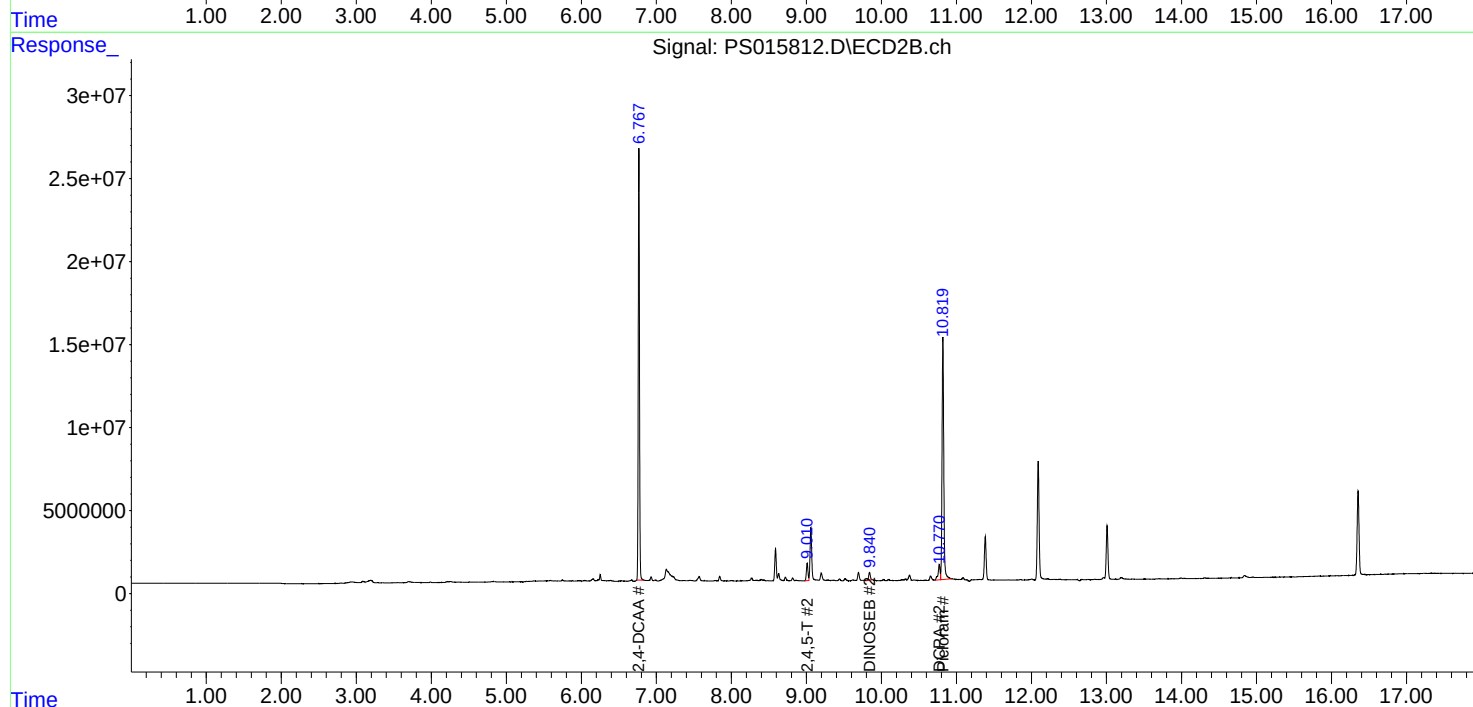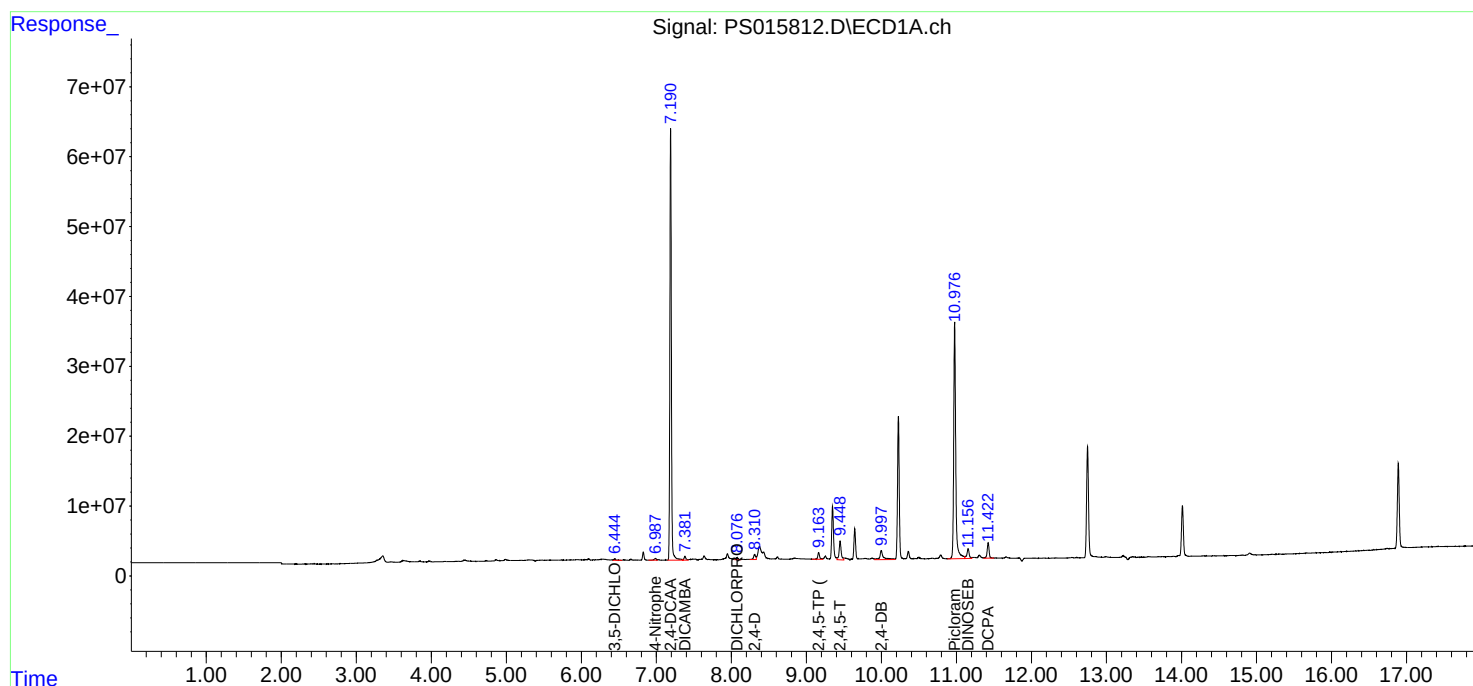

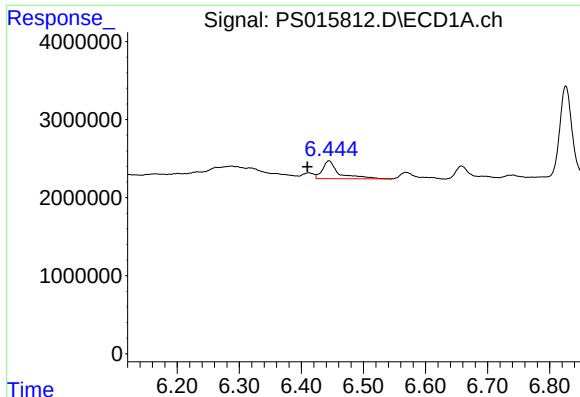


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.444 min
Delta R.T.: 0.035 min
Response: 4212836
Conc: 1.88 ng/ml

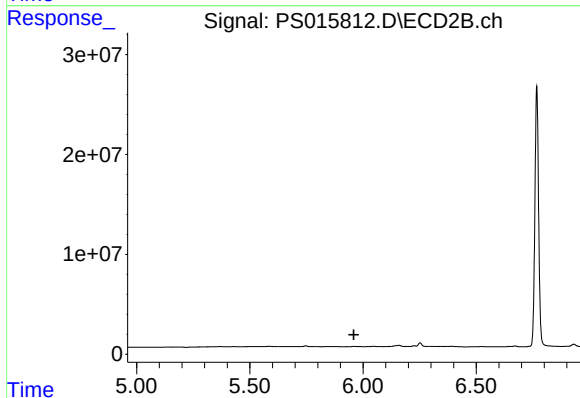


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.960 min
Response: 0
Conc: N.D.

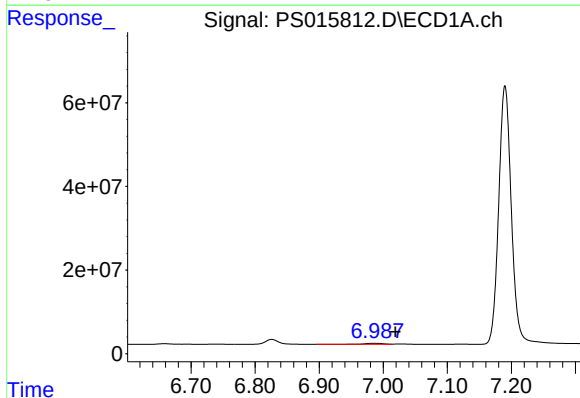


#3 4-Nitrophenol

R.T.: 6.986 min
Delta R.T.: -0.033 min
Response: 5163269
Conc: 5.68 ng/ml

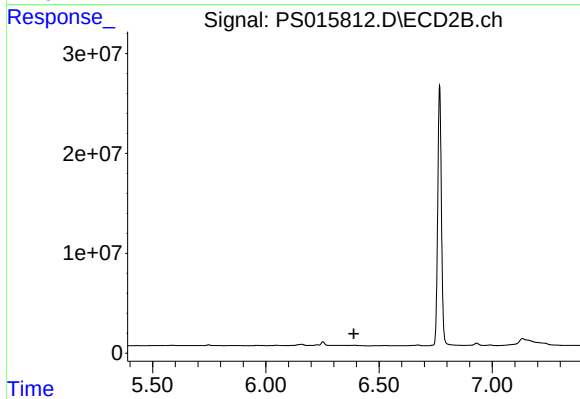


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

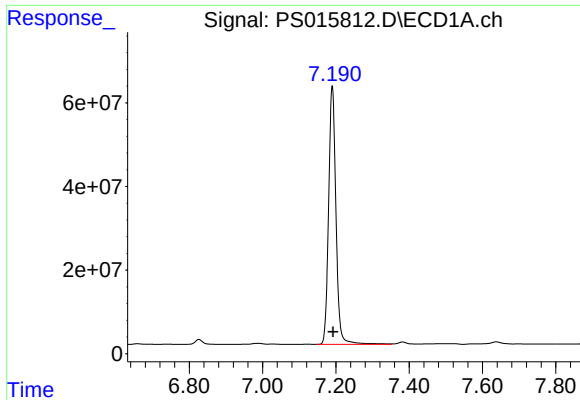


#4 2,4-DCAA

R.T.: 7.190 min
Delta R.T.: -0.003 min
Response: 860971165
Conc: 518.21 ng/ml

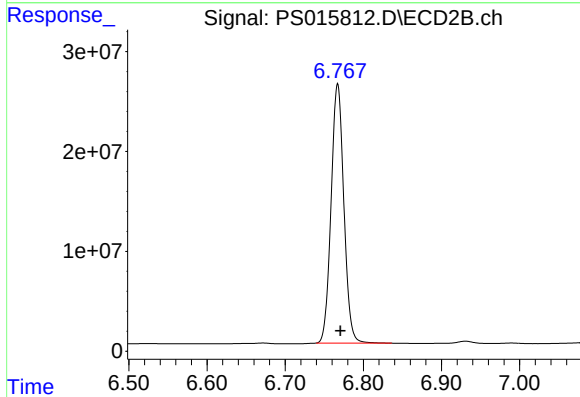


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: -0.003 min
Response: 294356835
Conc: 584.21 ng/ml

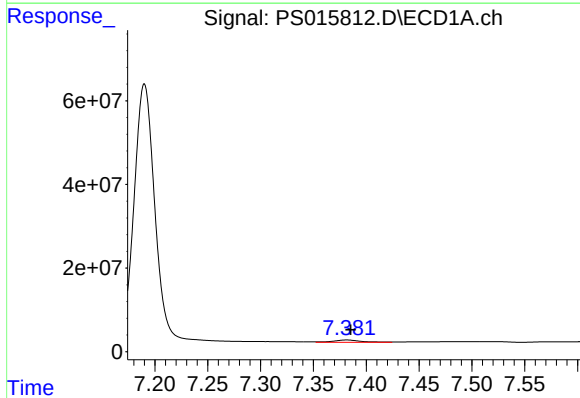


#5 DICAMBA

R.T.: 7.381 min
Delta R.T.: -0.004 min
Response: 10059007
Conc: 1.56 ng/ml

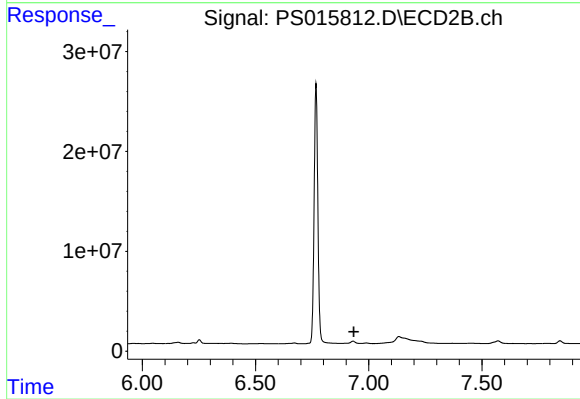


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.935 min
Response: 0
Conc: N.D.

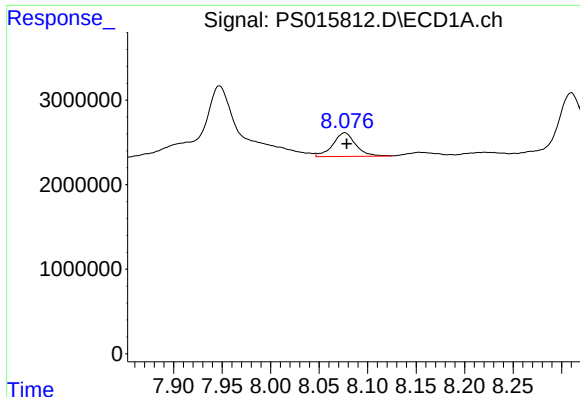


#8 DICHLORPROP

R.T.: 8.076 min
Delta R.T.: -0.002 min
Response: 4597822
Conc: 2.90 ng/ml

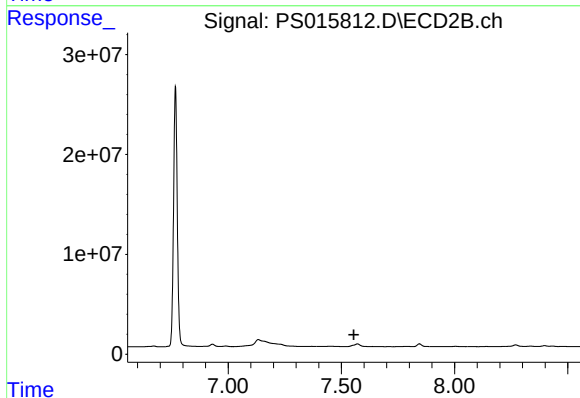


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.555 min
Response: 0
Conc: N.D.

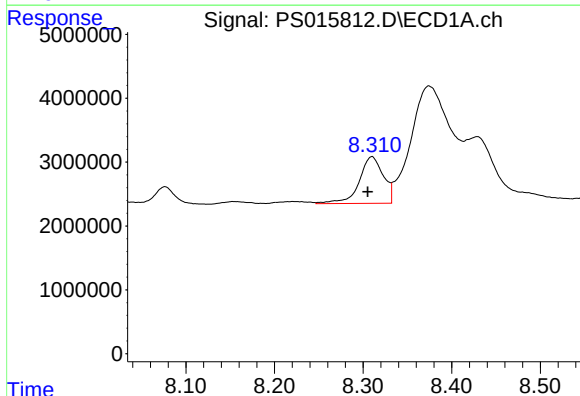


#9 2,4-D

R.T.: 8.310 min
Delta R.T.: 0.005 min
Response: 13839956
Conc: 7.90 ng/ml

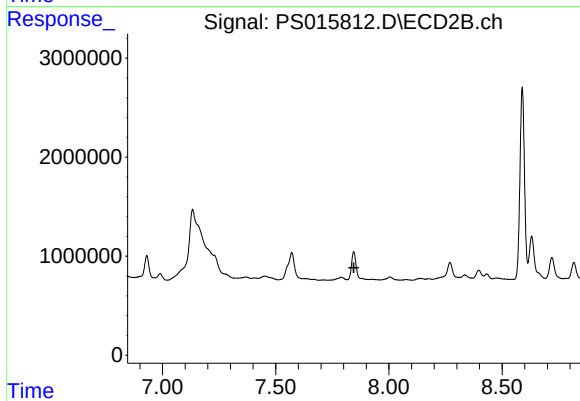


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.845 min
Response: 0
Conc: N.D.

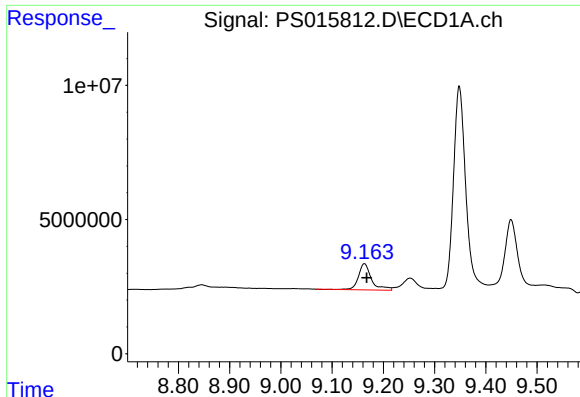


#11 2,4,5-TP (SILVEX)

R.T.: 9.163 min
Delta R.T.: -0.005 min
Response: 17355398
Conc: 1.99 ng/ml

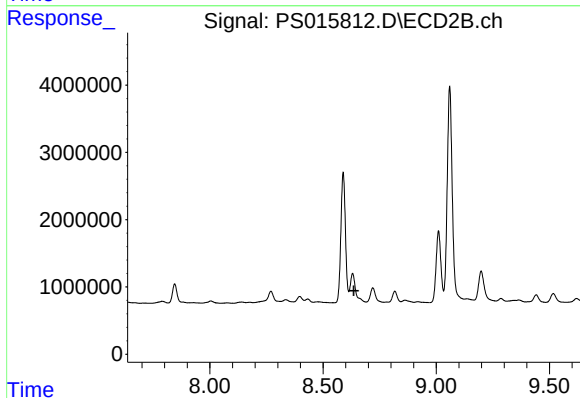


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 8.636 min
Response: 0
Conc: N.D.

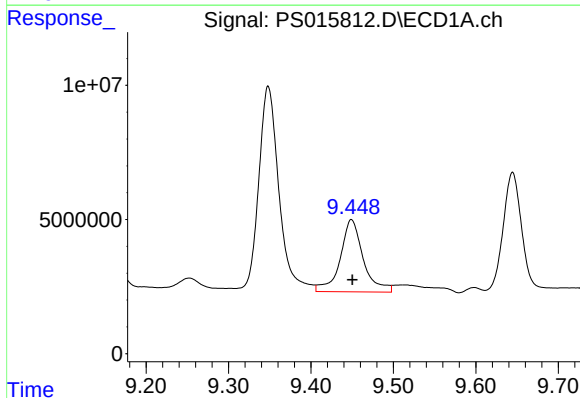


#12 2,4,5-T

R.T.: 9.449 min
Delta R.T.: 0.000 min
Response: 52322616
Conc: 5.93 ng/ml

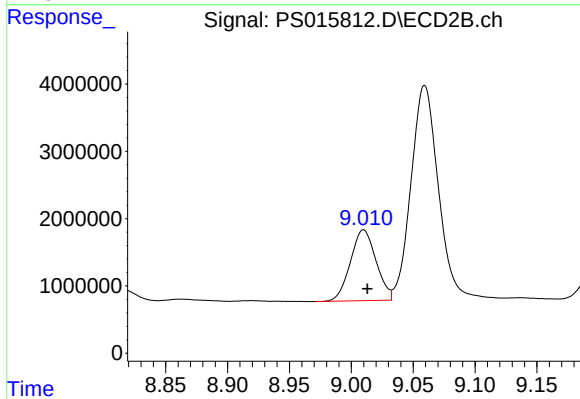


#12 2,4,5-T

R.T.: 9.010 min
Delta R.T.: -0.003 min
Response: 15211115
Conc: 5.39 ng/ml

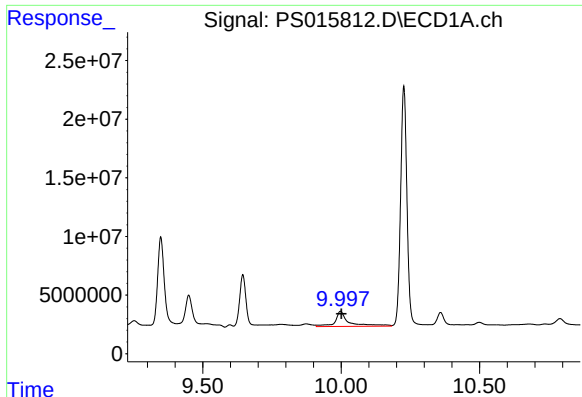


#13 2,4-DB

R.T.: 9.997 min
Delta R.T.: -0.003 min
Response: 44979405
Conc: 21.99 ng/ml

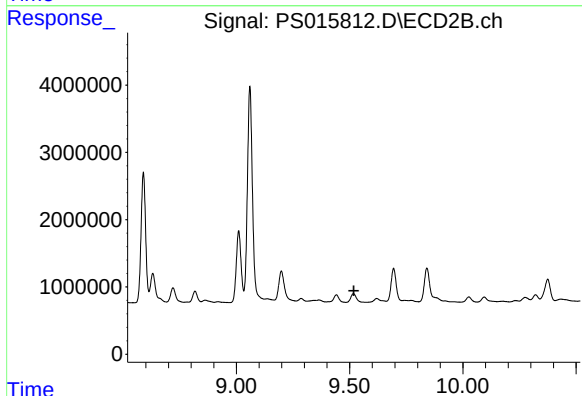


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.519 min
Response: 0
Conc: N.D.

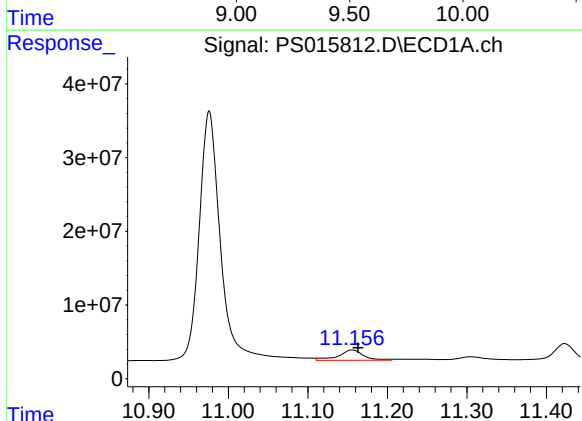


#14 DINOSEB

R.T.: 11.156 min
Delta R.T.: -0.008 min
Response: 30978730
Conc: 4.78 ng/ml

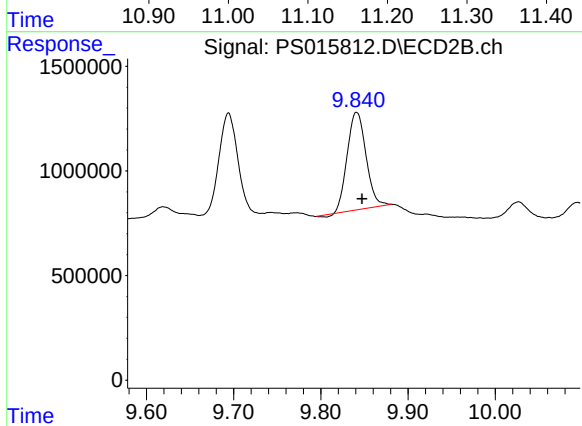


#14 DINOSEB

R.T.: 9.841 min
Delta R.T.: -0.006 min
Response: 6944578
Conc: 3.45 ng/ml

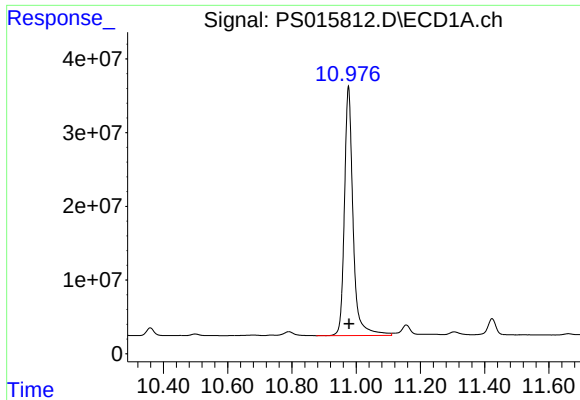


#15 Picloram

R.T.: 10.976 min
Delta R.T.: -0.002 min
Response: 632835503
Conc: 46.29 ng/ml

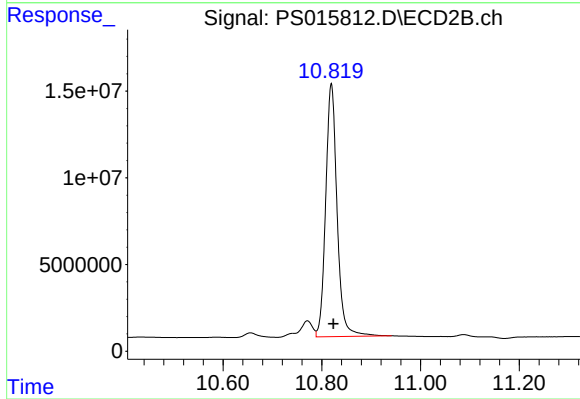


#15 Picloram

R.T.: 10.819 min
Delta R.T.: -0.005 min
Response: 233651320
Conc: 55.56 ng/ml

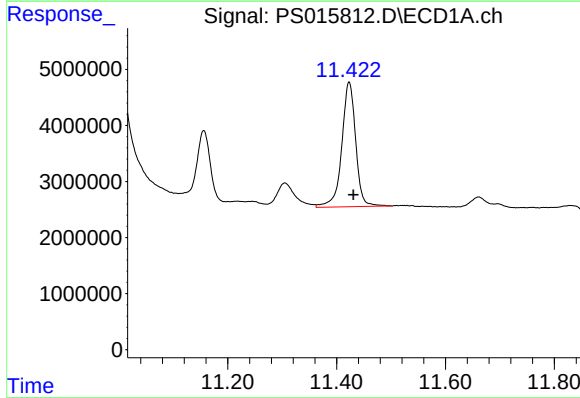

#16 DCPA

R.T.: 11.423 min
Delta R.T.: -0.008 min
Response: 39461796
Conc: 2.98 ng/ml

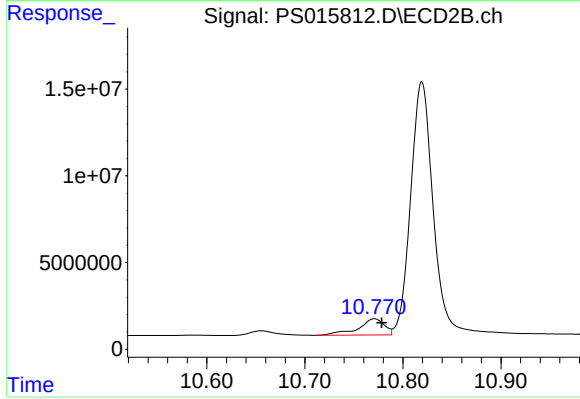

#16 DCPA

R.T.: 10.771 min
Delta R.T.: -0.008 min
Response: 17174355
Conc: 4.09 ng/ml