

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
 Data File : PS015822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2021 11:15
 Operator : DD\AJ
 Sample : PB137193BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:32:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.190	6.767	771.4E6	269.7E6	464.315	535.288
Target Compounds							
15) T	Picloram	10.984	10.823	33997918	13952332	2.487	3.318 #
16) T	DCPA	0.000	10.823f	0	13952332	N.D.	3.319


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
Data File : PS015822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2021 11:15
Operator : DD\AJ
Sample : PB137193BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:32:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

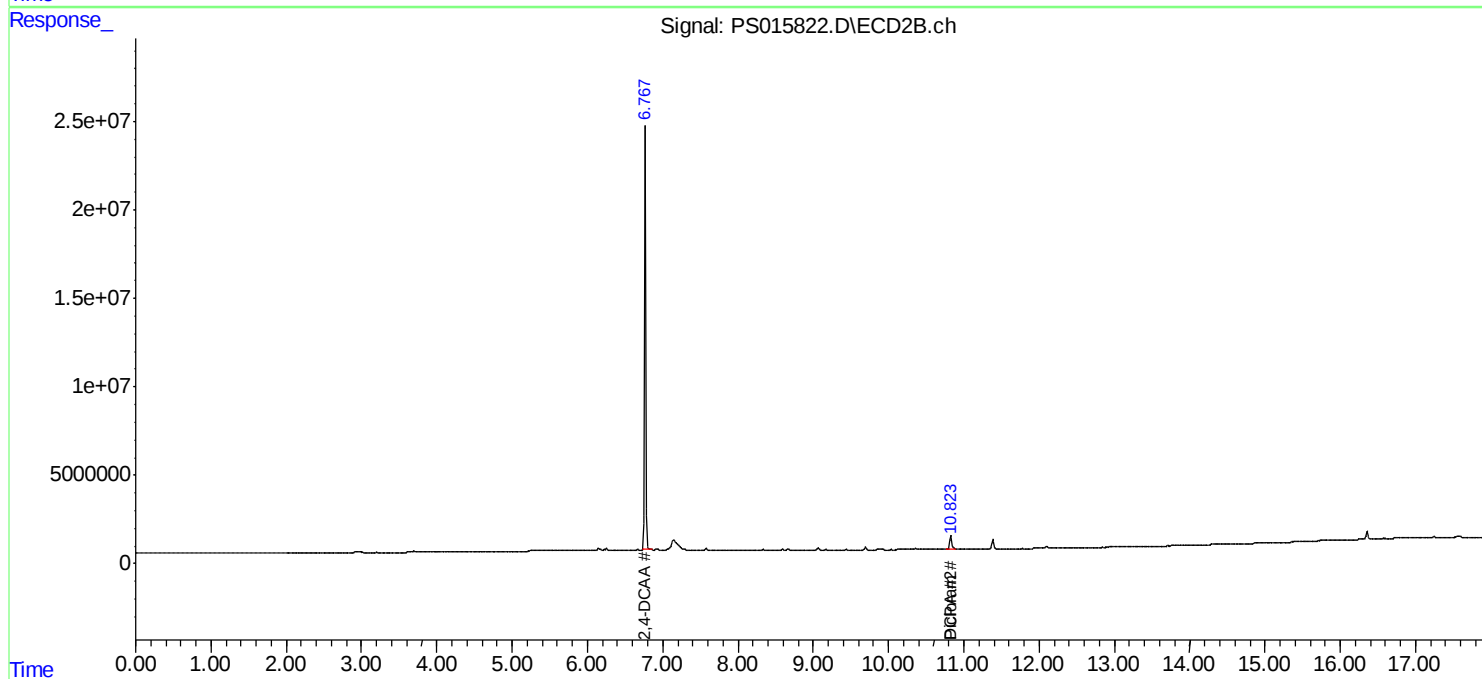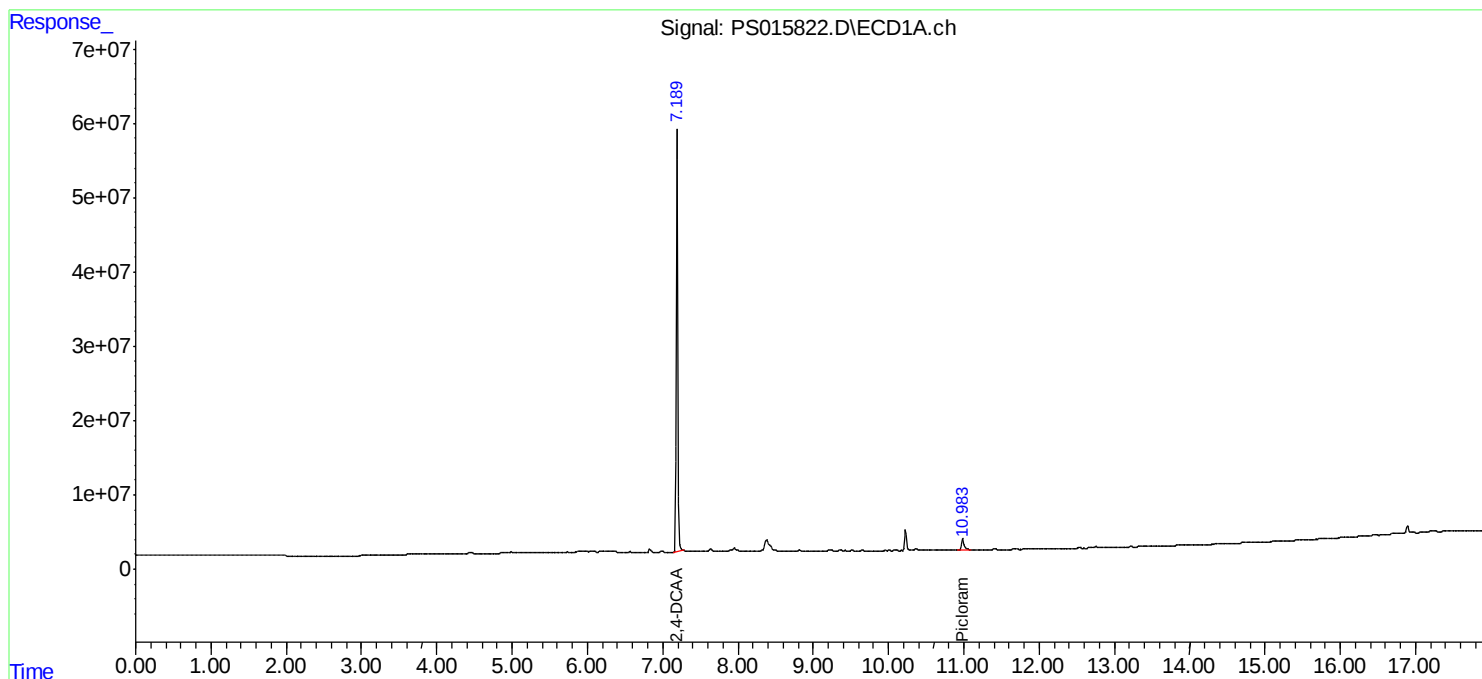

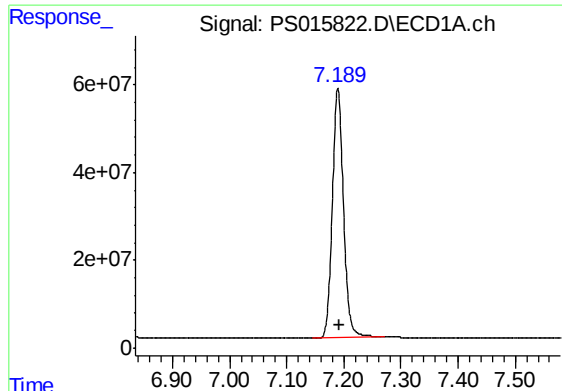


#4 2,4-DCAA

R.T.: 7.190 min
Delta R.T.: -0.003 min
Response: 771434343
Conc: 464.31 ng/ml

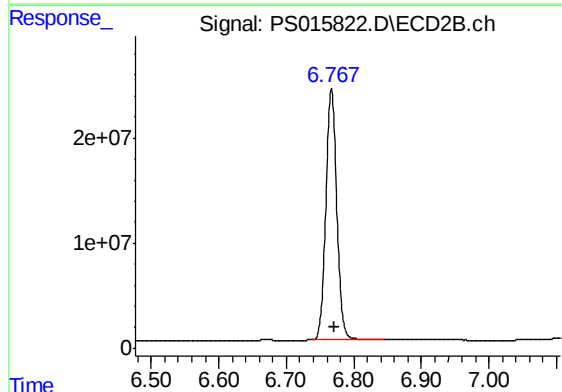


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: -0.004 min
Response: 269706064
Conc: 535.29 ng/ml

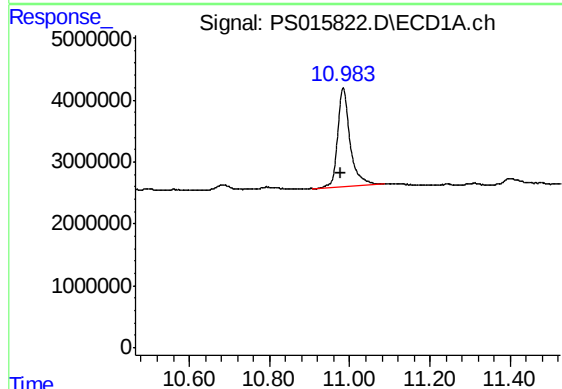


#15 Picloram

R.T.: 10.984 min
Delta R.T.: 0.006 min
Response: 33997918
Conc: 2.49 ng/ml

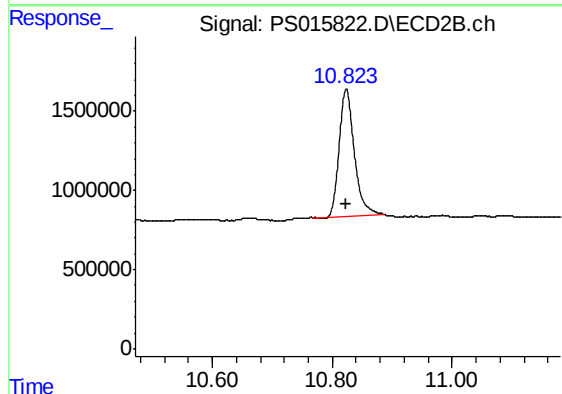


#15 Picloram

R.T.: 10.823 min
Delta R.T.: 0.000 min
Response: 13952332
Conc: 3.32 ng/ml

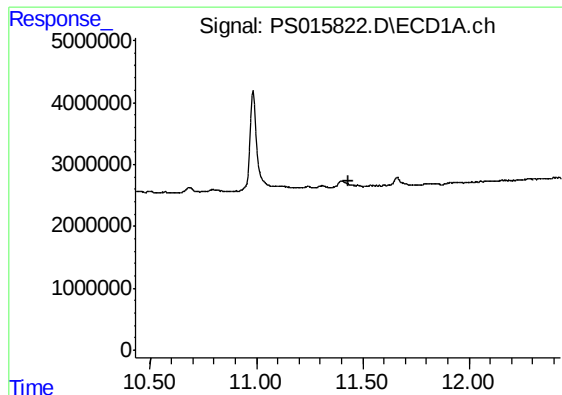

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.431 min
Response: 0
Conc: N.D.

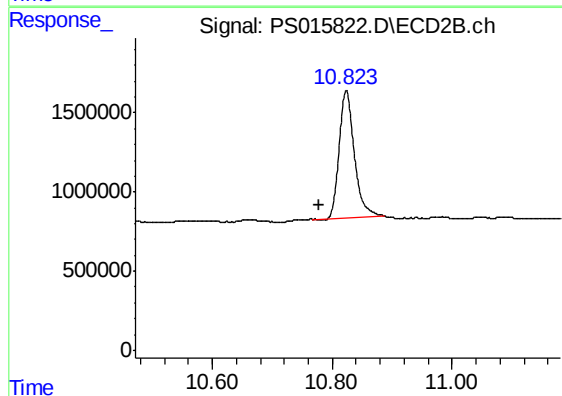

#16 DCPA

R.T.: 10.823 min
Delta R.T.: 0.045 min
Response: 13952332
Conc: 3.32 ng/ml