

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
 Data File : PS015824.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2021 12:03
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:33:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.190	6.767	860.5E6	300.6E6	517.927	596.667
Target Compounds							
2) T	3,5-DICHL...	6.410	0.000	3751014	0	1.671	N.D. #
5) T	DICAMBA	7.381	6.930	25047298	9500545	3.896	4.579
8) T	DICHLORPROP	8.076	0.000	9465392	0	5.978	N.D. #
9) T	2,4-D	8.308	7.844	15030218	6895456	8.576	11.117 #
10) T	Pentachlo...	8.612	8.269	37365577	14654721	1.731	2.086
11) T	2,4,5-TP ...	9.163	8.630	35450258	-6593889	4.056	N.D. #
12) T	2,4,5-T	9.449	9.009	76910236	26972001	8.712	9.563
13) T	2,4-DB	9.996	0.000	41615627	0	20.345	N.D. #
14) T	DINOSEB	11.156	9.841	40991961	12134098	6.329	6.024
15) T	Picloram	10.975	10.819	758.0E6	283.8E6	55.446	67.491
16) T	DCPA	11.423	10.771	62311605	25955624	4.711	6.174 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
Data File : PS015824.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2021 12:03
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:33:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

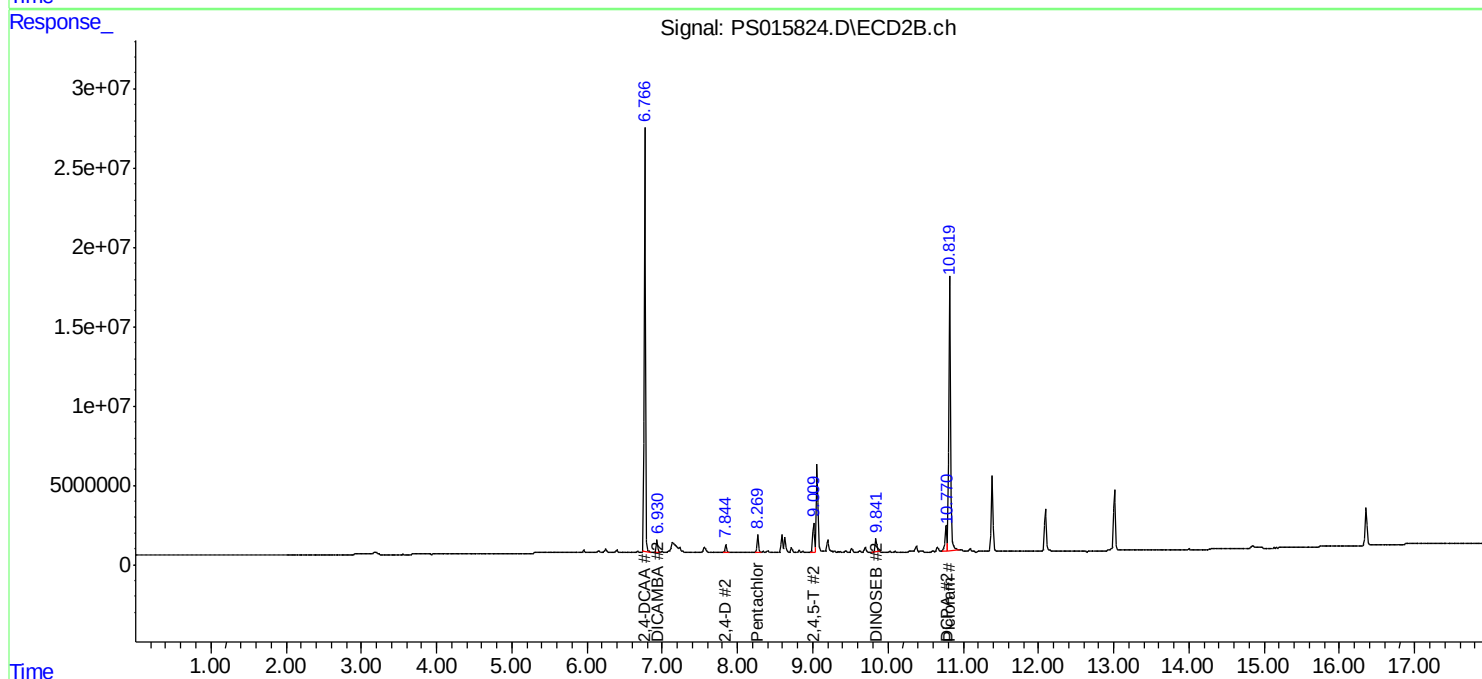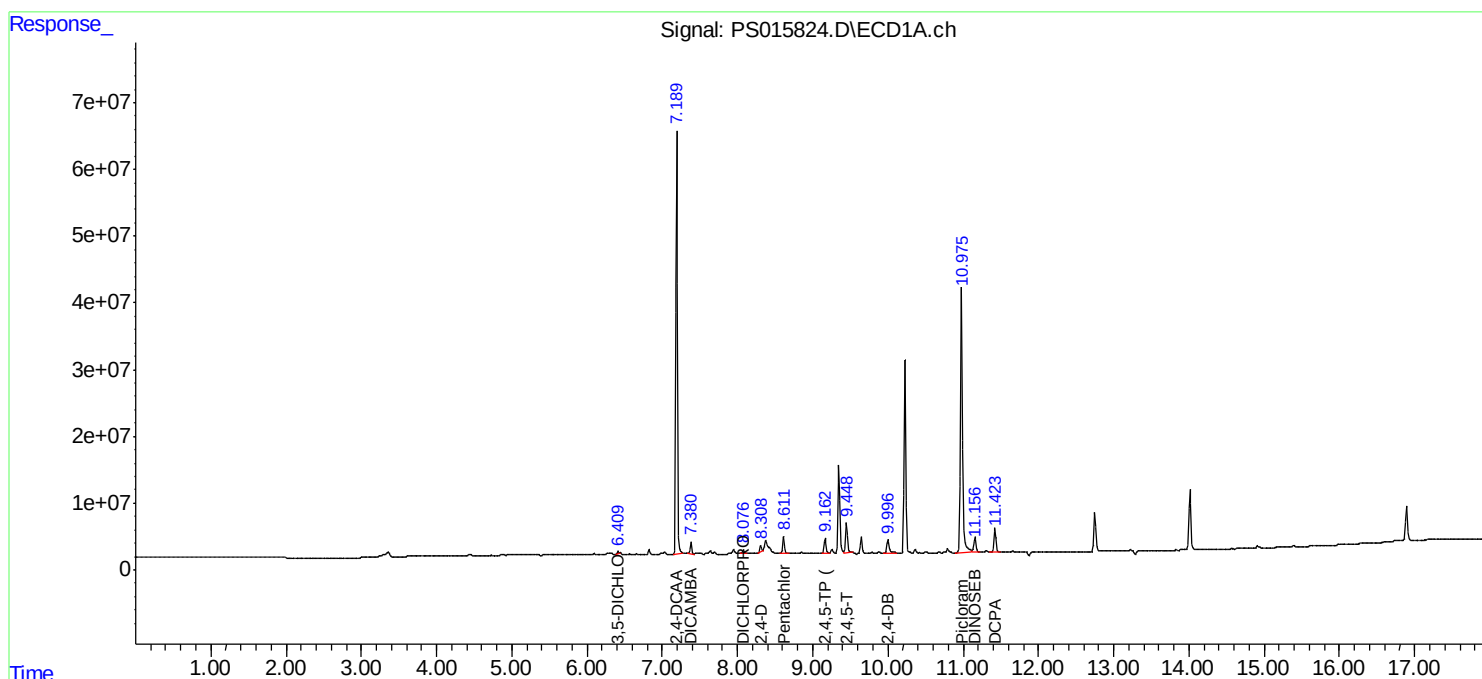

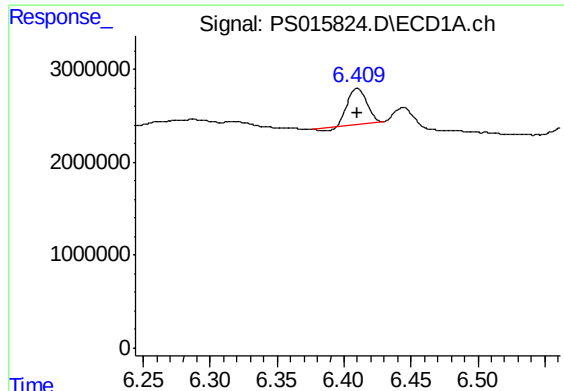


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.410 min
Delta R.T.: 0.000 min
Response: 3751014
Conc: 1.67 ng/ml

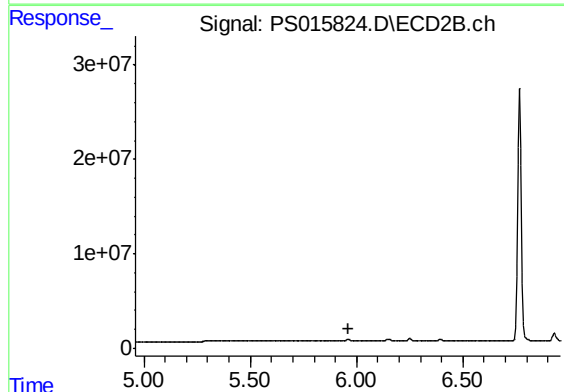


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

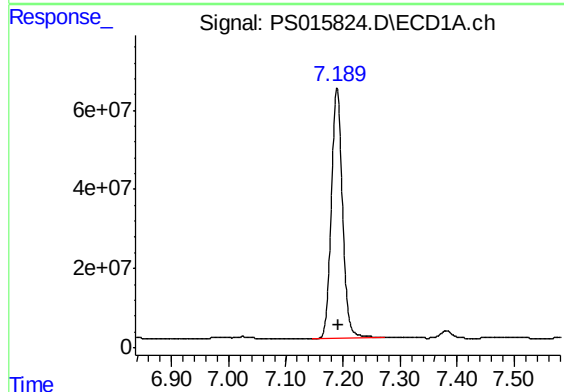


#4 2,4-DCAA

R.T.: 7.190 min
Delta R.T.: -0.003 min
Response: 860507737
Conc: 517.93 ng/ml

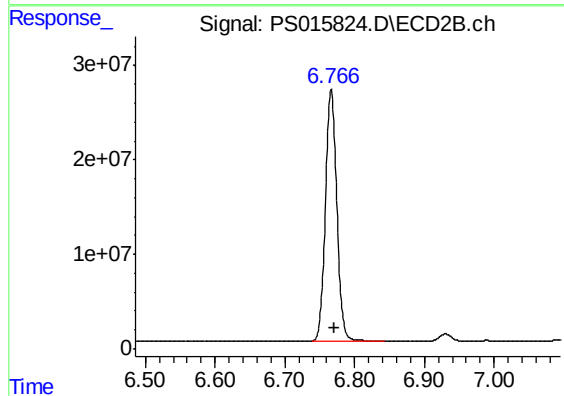


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: -0.004 min
Response: 300632022
Conc: 596.67 ng/ml

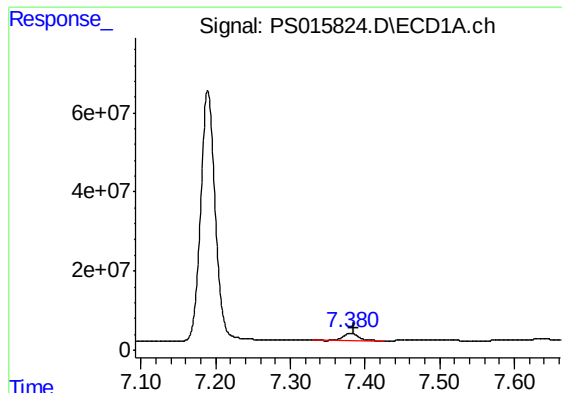


#5 DICAMBA

R.T.: 7.381 min
Delta R.T.: -0.004 min
Response: 25047298
Conc: 3.90 ng/ml

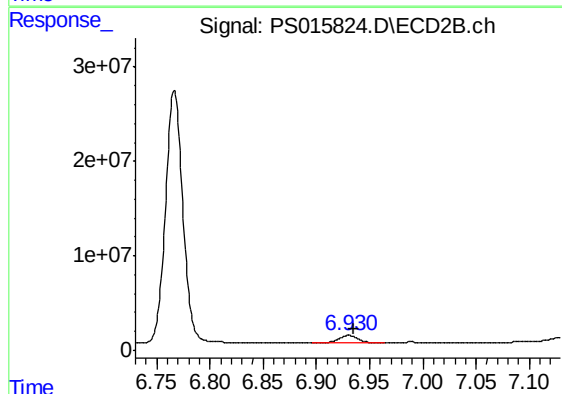


#5 DICAMBA

R.T.: 6.930 min
Delta R.T.: -0.004 min
Response: 9500545
Conc: 4.58 ng/ml

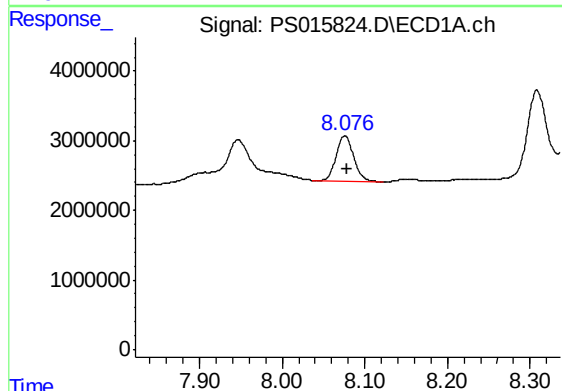


#8 DICHLORPROP

R.T.: 8.076 min
Delta R.T.: -0.003 min
Response: 9465392
Conc: 5.98 ng/ml

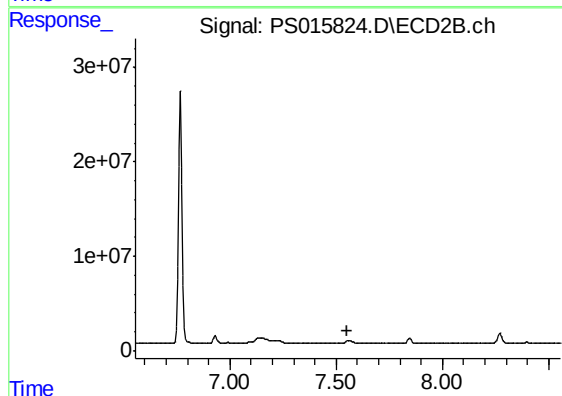


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.555 min
Response: 0
Conc: N.D.

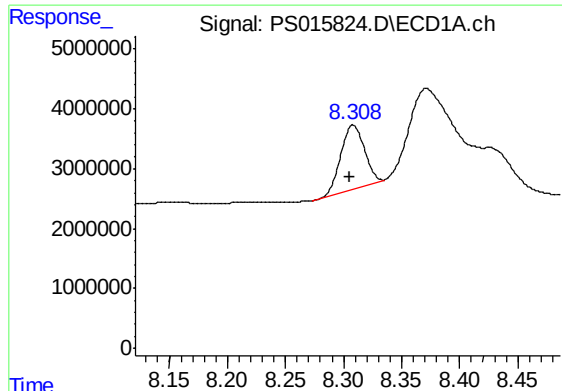


#9 2,4-D

R.T.: 8.308 min
Delta R.T.: 0.003 min
Response: 15030218
Conc: 8.58 ng/ml

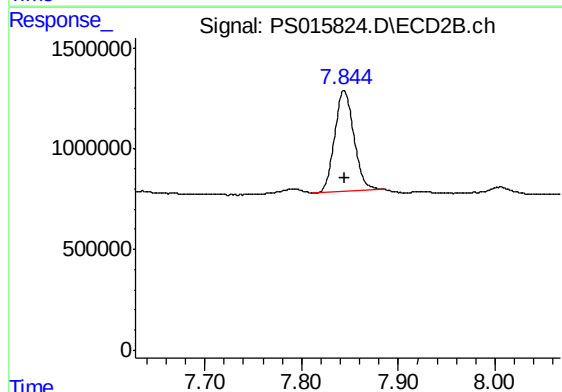


#9 2,4-D

R.T.: 7.844 min
Delta R.T.: -0.001 min
Response: 6895456
Conc: 11.12 ng/ml

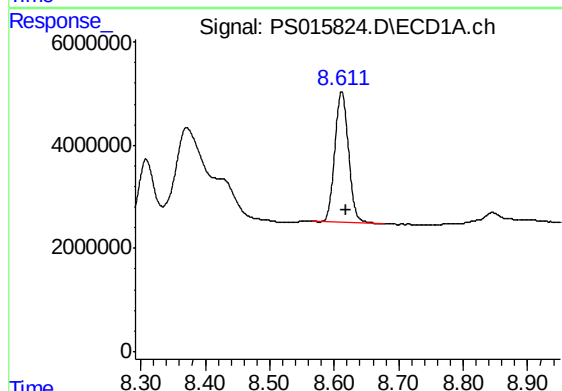


#10 Pentachlorophenol

R.T.: 8.612 min
Delta R.T.: -0.006 min
Response: 37365577
Conc: 1.73 ng/ml

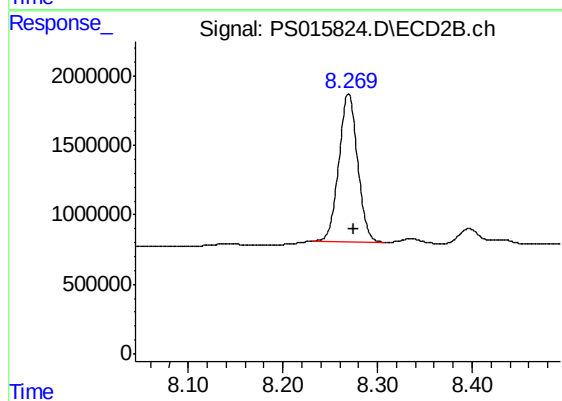


#10 Pentachlorophenol

R.T.: 8.269 min
Delta R.T.: -0.006 min
Response: 14654721
Conc: 2.09 ng/ml

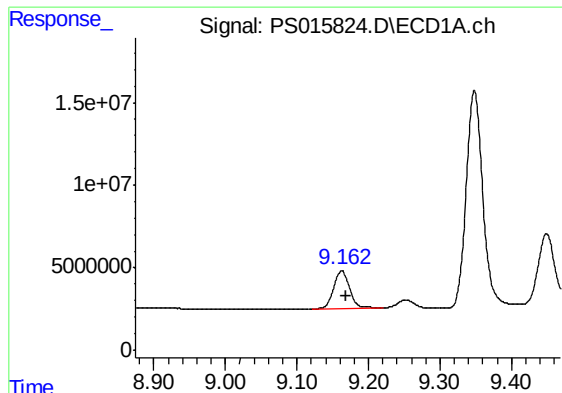


#11 2,4,5-TP (SILVEX)

R.T.: 9.163 min
Delta R.T.: -0.005 min
Response: 35450258
Conc: 4.06 ng/ml

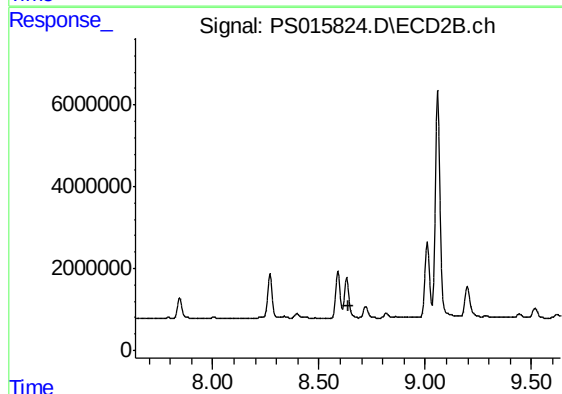


#11 2,4,5-TP (SILVEX)

R.T.: 8.630 min
Delta R.T.: -0.006 min
Response: -6593889
Conc: N.D.

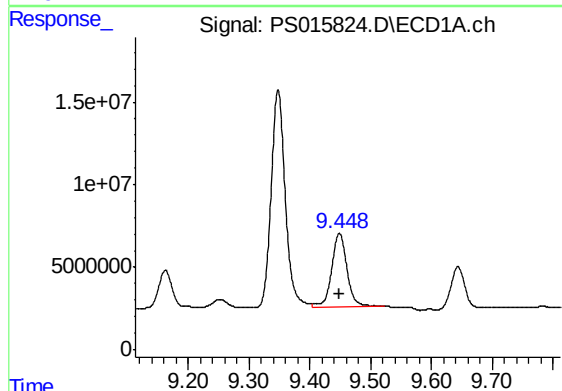


#12 2,4,5-T

R.T.: 9.449 min
Delta R.T.: -0.001 min
Response: 76910236
Conc: 8.71 ng/ml

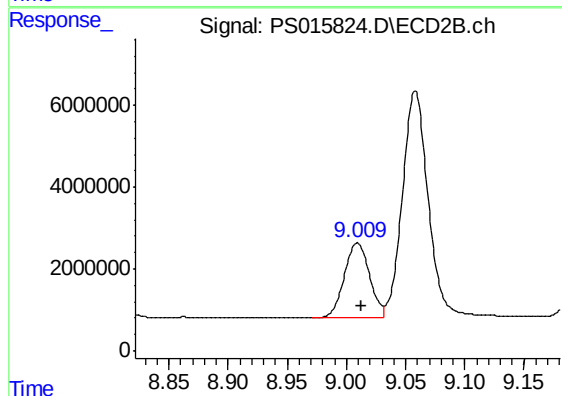


#12 2,4,5-T

R.T.: 9.009 min
Delta R.T.: -0.004 min
Response: 26972001
Conc: 9.56 ng/ml

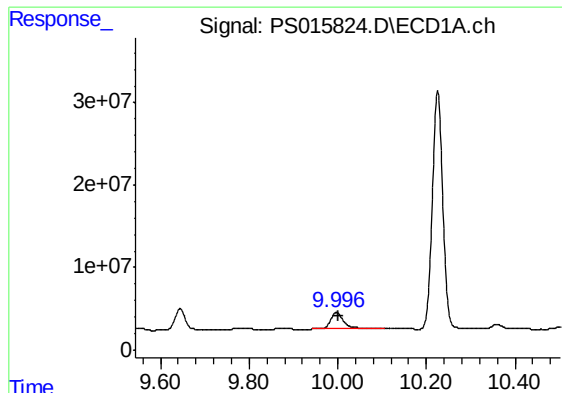


#13 2,4-DB

R.T.: 9.996 min
Delta R.T.: -0.004 min
Response: 41615627
Conc: 20.34 ng/ml

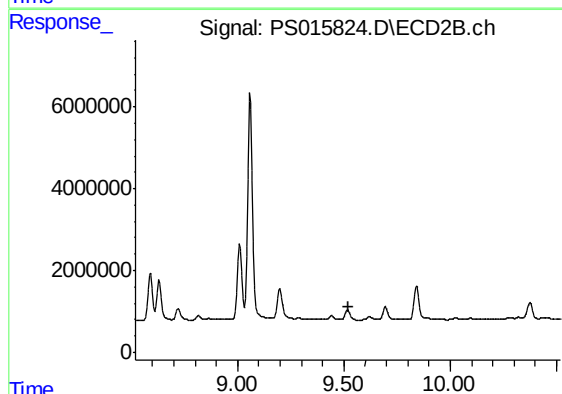


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.519 min
Response: 0
Conc: N.D.

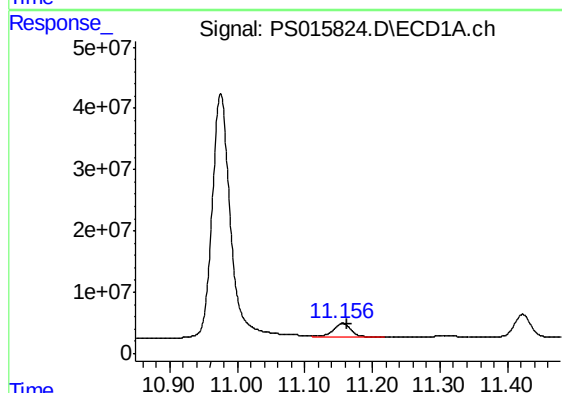


#14 DINOSEB

R.T.: 11.156 min
Delta R.T.: -0.007 min
Response: 40991961
Conc: 6.33 ng/ml

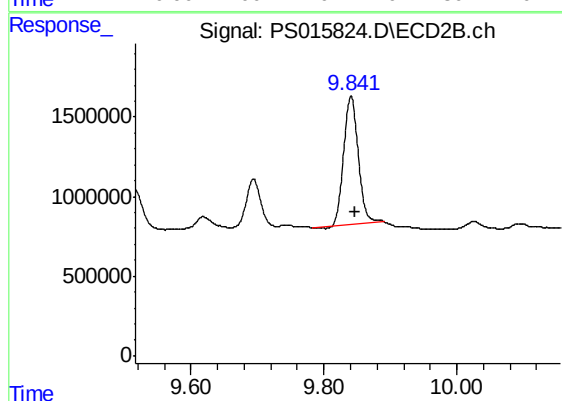


#14 DINOSEB

R.T.: 9.841 min
Delta R.T.: -0.006 min
Response: 12134098
Conc: 6.02 ng/ml

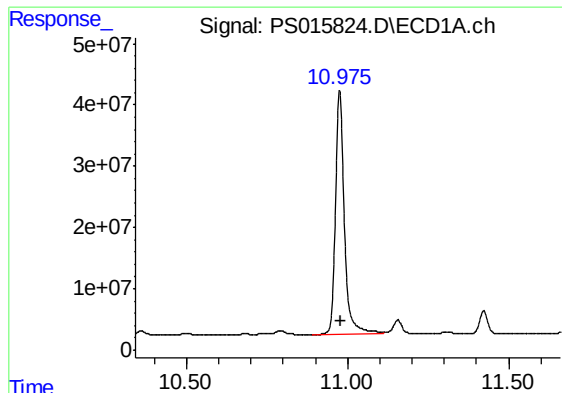


#15 Picloram

R.T.: 10.975 min
Delta R.T.: -0.002 min
Response: 757991944
Conc: 55.45 ng/ml

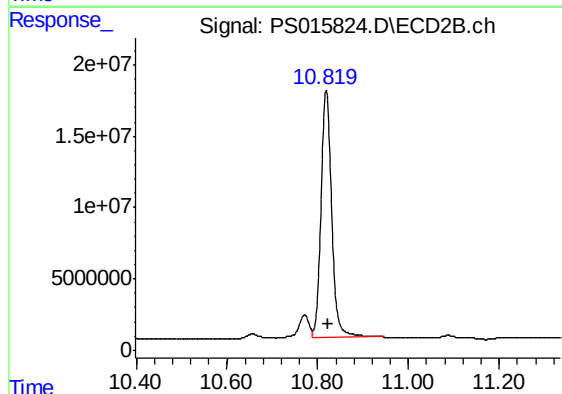


#15 Picloram

R.T.: 10.819 min
Delta R.T.: -0.005 min
Response: 283835923
Conc: 67.49 ng/ml

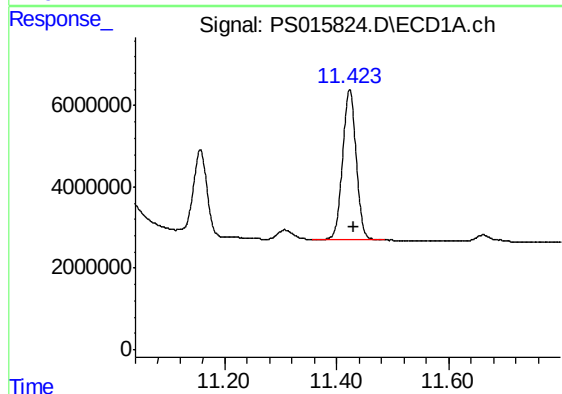

#16 DCPA

R.T.: 11.423 min
Delta R.T.: -0.008 min
Response: 62311605
Conc: 4.71 ng/ml

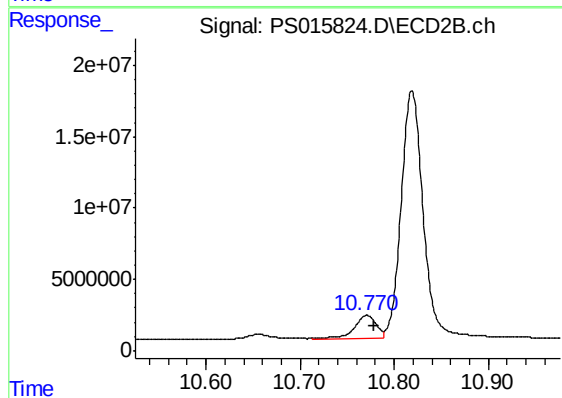

#16 DCPA

R.T.: 10.771 min
Delta R.T.: -0.008 min
Response: 25955624
Conc: 6.17 ng/ml