

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
 Data File : PS015826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2021 12:51
 Operator : DD\AJ
 Sample : PB137193TB
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:33:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.190	6.767	774.8E6	271.5E6	466.357	538.913
Target Compounds							
5) T	DICAMBA	7.382	6.930	14958844	6131008	2.327	2.955 #
9) T	2,4-D	8.311	0.000	6977852	0	3.982	N.D. #
10) T	Pentachlo...	8.613	8.270	27604319	10921509	1.279	1.555
11) T	2,4,5-TP ...	9.163	0.000	19109524	0	2.186	N.D. #
12) T	2,4,5-T	9.450	9.011	42731554	15164483	4.840	5.377
13) T	2,4-DB	9.999	0.000	27686419	0	13.535	N.D. #
14) T	DINOSEB	11.156	9.842	23368639	6865234	3.608	3.409
15) T	Picloram	10.977	10.820	607.0E6	229.1E6	44.401	54.483
16) T	DCPA	11.423	10.771	35431194	14829402	2.679	3.527 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
Data File : PS015826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2021 12:51
Operator : DD\AJ
Sample : PB137193TB
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:33:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

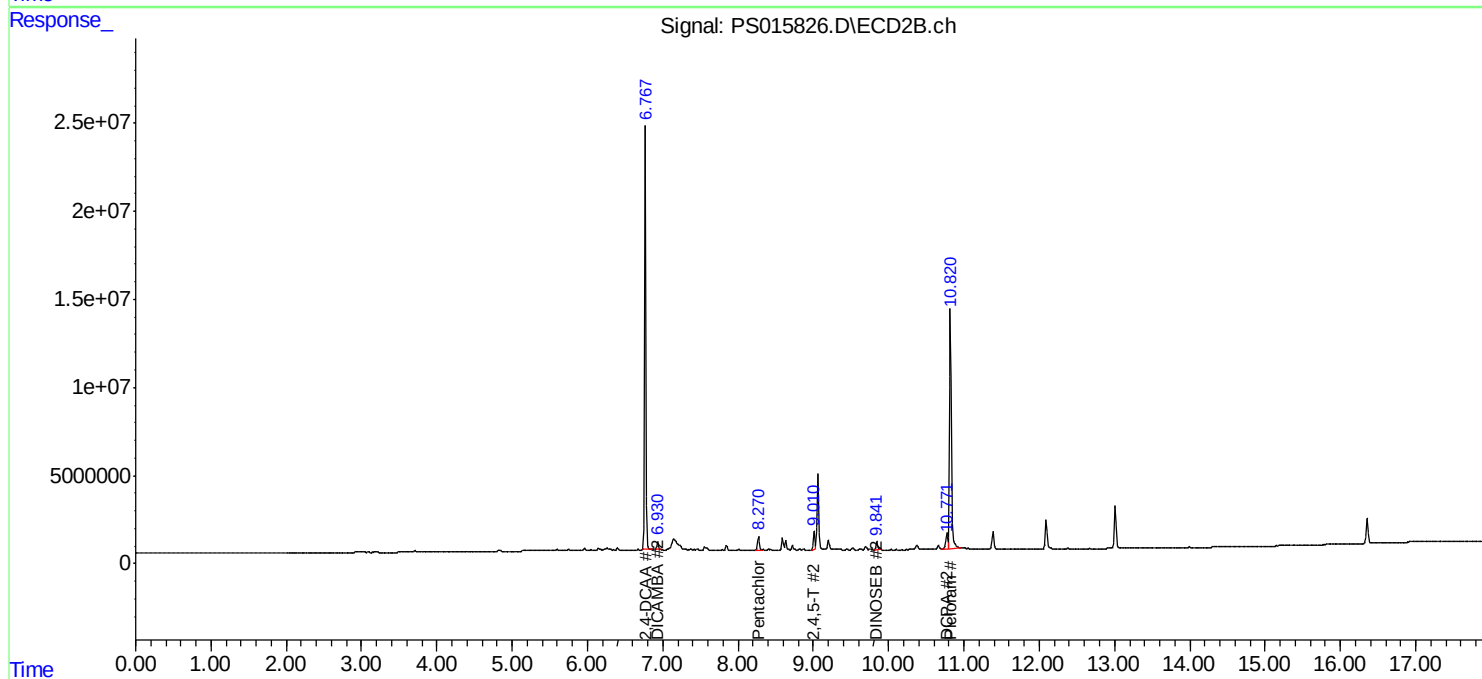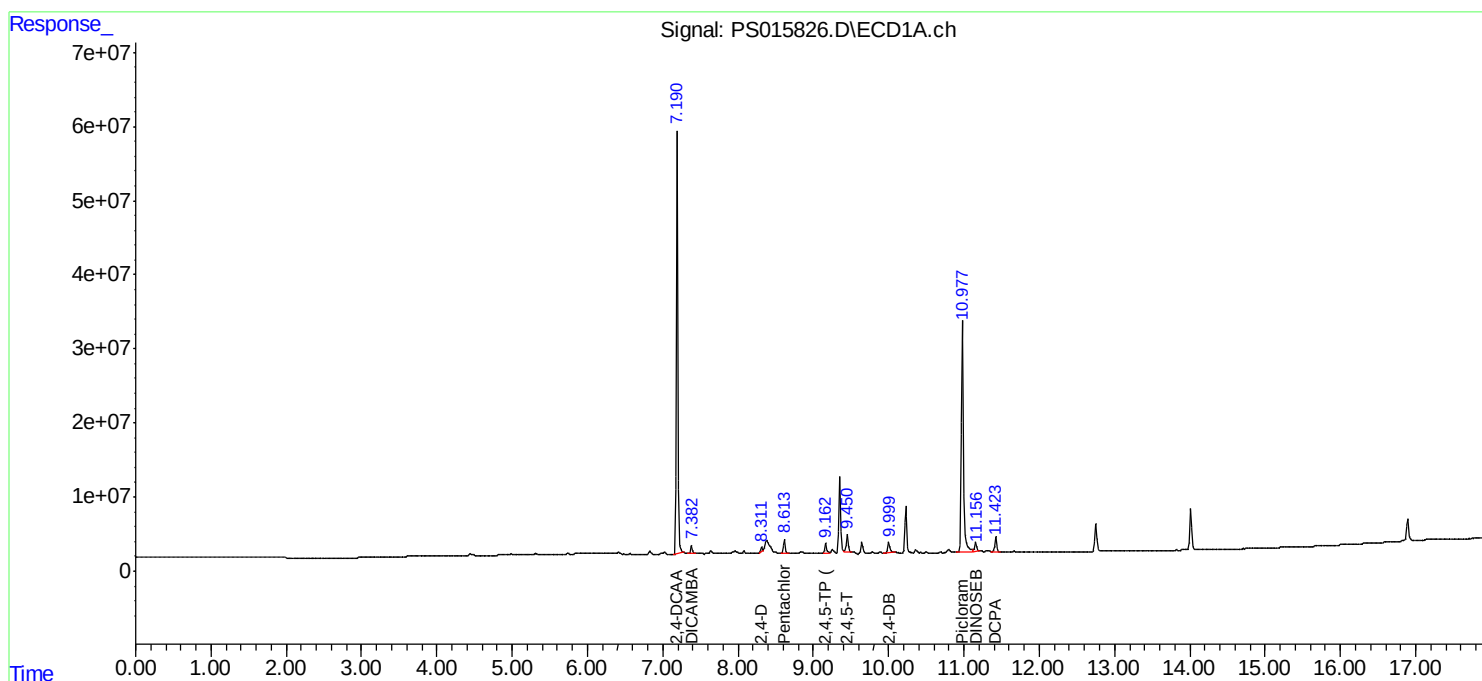

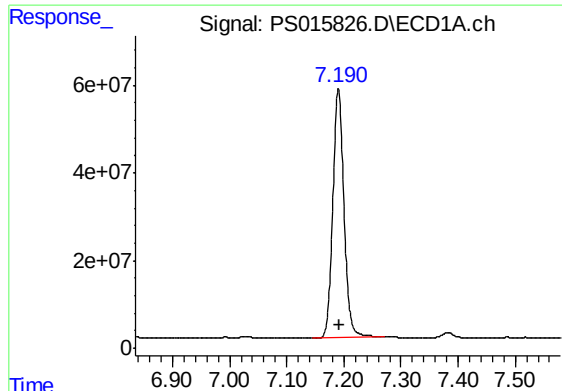


#4 2,4-DCAA

R.T.: 7.190 min
Delta R.T.: -0.002 min
Response: 774828073
Conc: 466.36 ng/ml

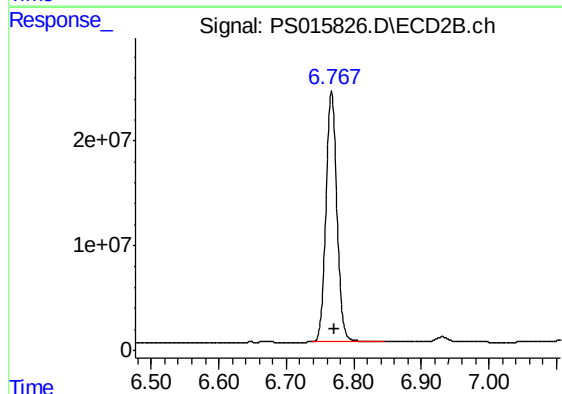


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: -0.003 min
Response: 271532528
Conc: 538.91 ng/ml

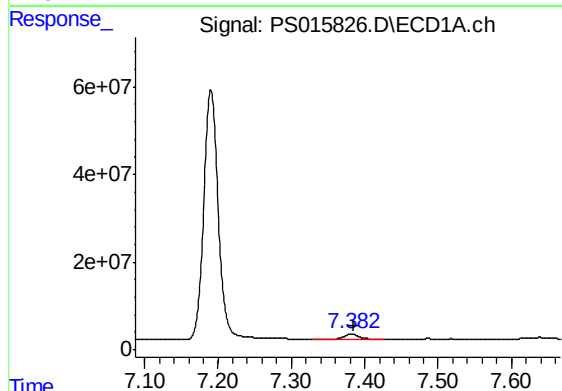


#5 DICAMBA

R.T.: 7.382 min
Delta R.T.: -0.003 min
Response: 14958844
Conc: 2.33 ng/ml

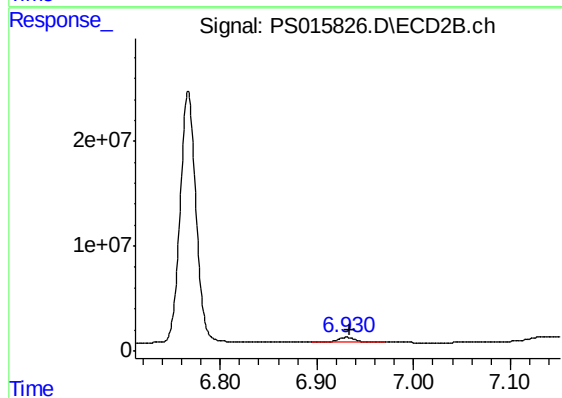


#5 DICAMBA

R.T.: 6.930 min
Delta R.T.: -0.004 min
Response: 6131008
Conc: 2.95 ng/ml

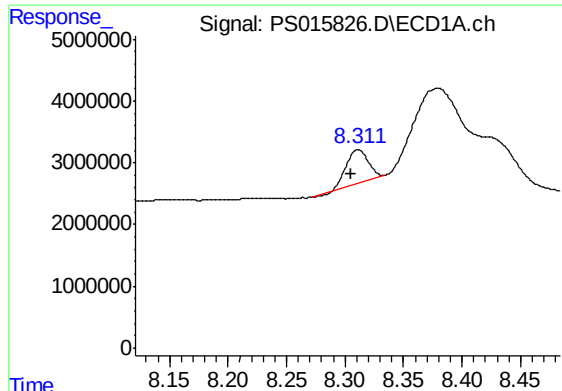


#9 2,4-D

R.T.: 8.311 min
Delta R.T.: 0.006 min
Response: 6977852
Conc: 3.98 ng/ml

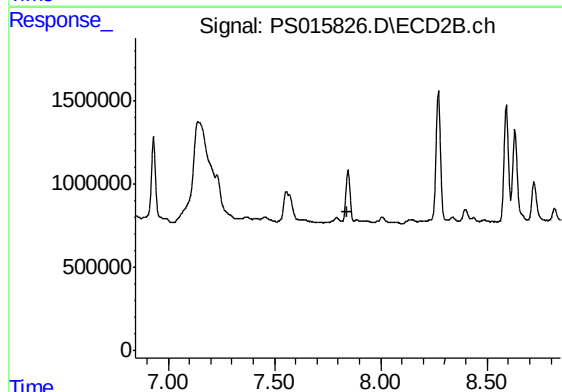


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

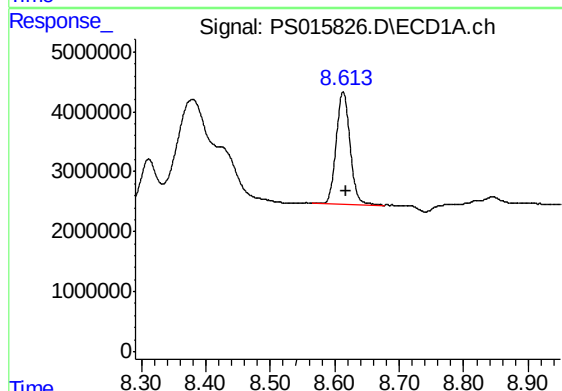


#10 Pentachlorophenol

R.T.: 8.613 min
Delta R.T.: -0.005 min
Response: 27604319
Conc: 1.28 ng/ml

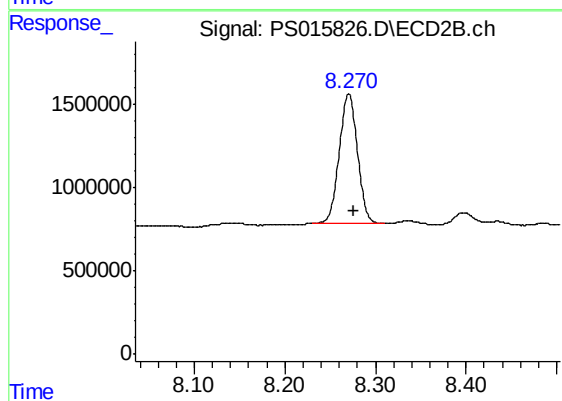


#10 Pentachlorophenol

R.T.: 8.270 min
Delta R.T.: -0.005 min
Response: 10921509
Conc: 1.55 ng/ml

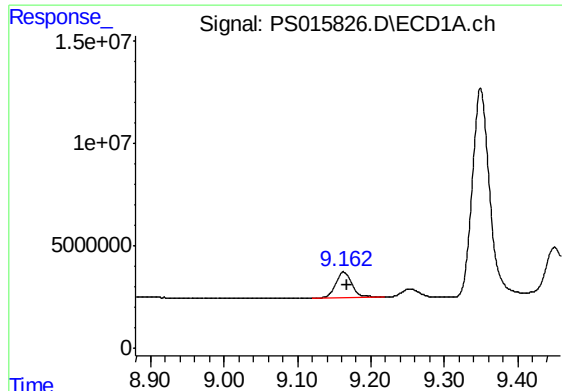


#11 2,4,5-TP (SILVEX)

R.T.: 9.163 min
Delta R.T.: -0.005 min
Response: 19109524
Conc: 2.19 ng/ml

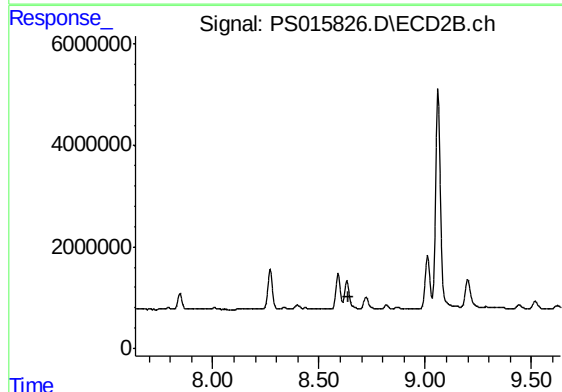


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.636 min
Response: 0
Conc: N.D.

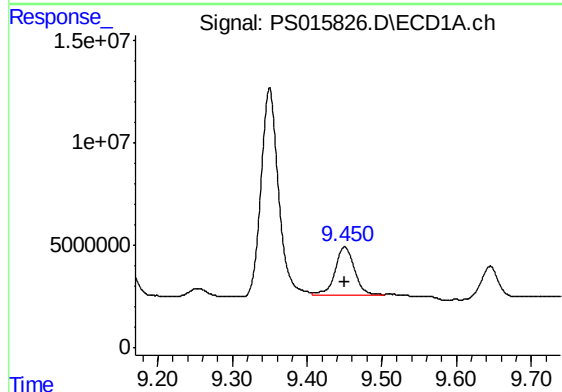


#12 2,4,5-T

R.T.: 9.450 min
Delta R.T.: 0.000 min
Response: 42731554
Conc: 4.84 ng/ml

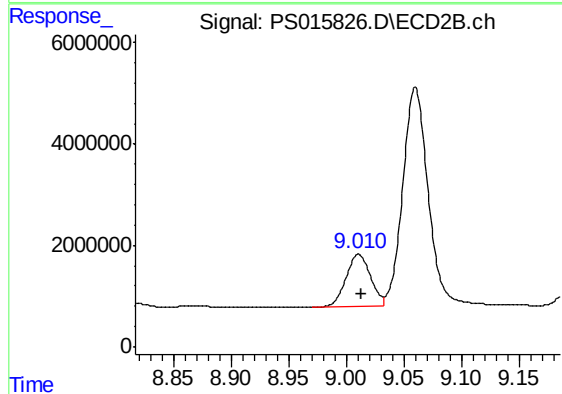


#12 2,4,5-T

R.T.: 9.011 min
Delta R.T.: -0.002 min
Response: 15164483
Conc: 5.38 ng/ml

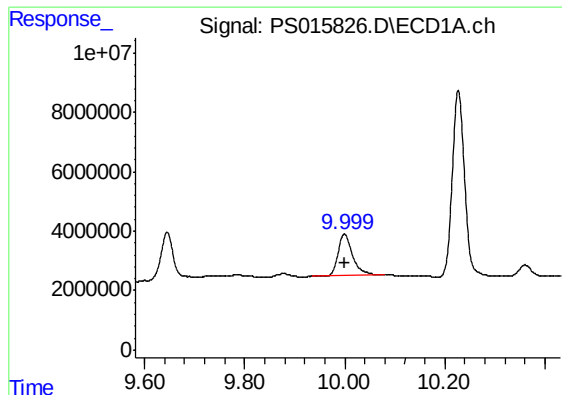


#13 2,4-DB

R.T.: 9.999 min
Delta R.T.: 0.000 min
Response: 27686419
Conc: 13.53 ng/ml

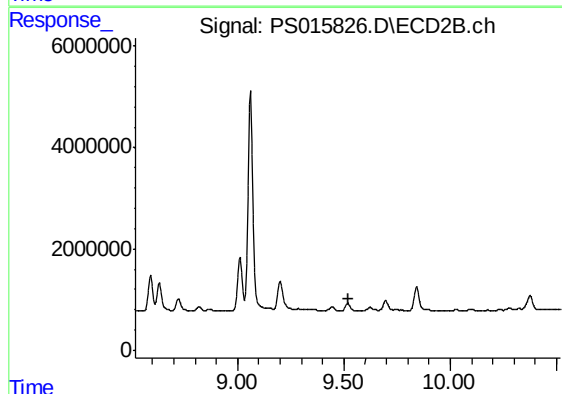


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.519 min
Response: 0
Conc: N.D.

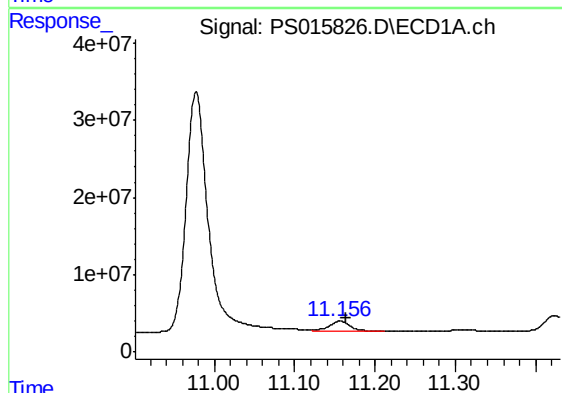


#14 DINOSEB

R.T.: 11.156 min
Delta R.T.: -0.007 min
Response: 23368639
Conc: 3.61 ng/ml

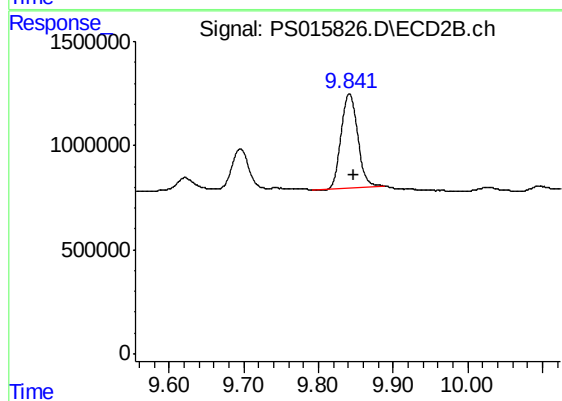


#14 DINOSEB

R.T.: 9.842 min
Delta R.T.: -0.006 min
Response: 6865234
Conc: 3.41 ng/ml

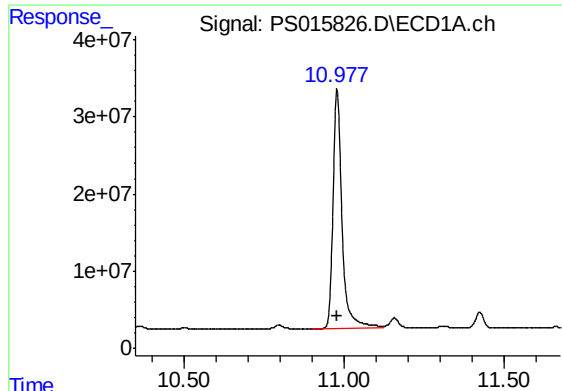


#15 Picloram

R.T.: 10.977 min
Delta R.T.: 0.000 min
Response: 606994233
Conc: 44.40 ng/ml

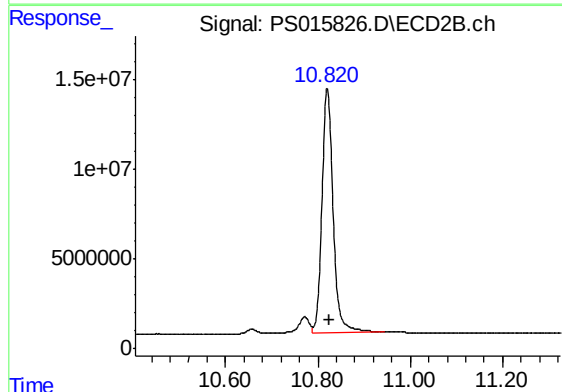


#15 Picloram

R.T.: 10.820 min
Delta R.T.: -0.003 min
Response: 229131906
Conc: 54.48 ng/ml

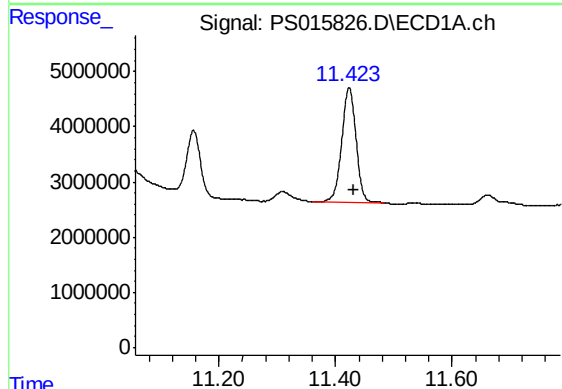

#16 DCPA

R.T.: 11.423 min
Delta R.T.: -0.007 min
Response: 35431194
Conc: 2.68 ng/ml

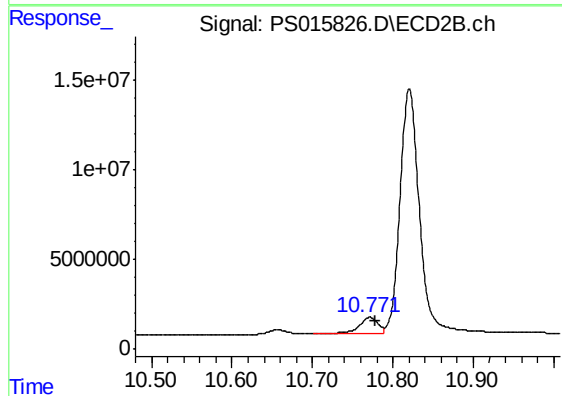

#16 DCPA

R.T.: 10.771 min
Delta R.T.: -0.007 min
Response: 14829402
Conc: 3.53 ng/ml