

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
 Data File : PS015829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2021 14:04
 Operator : DD\AJ
 Sample : PB137126BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:34:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.190	6.767	781.4E6	274.9E6	470.294	545.550
Target Compounds							
10) T	Pentachlo...	8.613	0.000	13193380	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.164	0.000	5614170	0	<MDL	N.D. #
12) T	2,4,5-T	9.452	0.000	9398380	0	1.065	N.D. #
15) T	Picloram	10.986	10.824	38217496	15558122	2.796	3.699 #
16) T	DCPA	11.423	10.824f	10564132	15558122	<MDL	3.701 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061821\
Data File : PS015829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2021 14:04
Operator : DD\AJ
Sample : PB137126BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:34:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

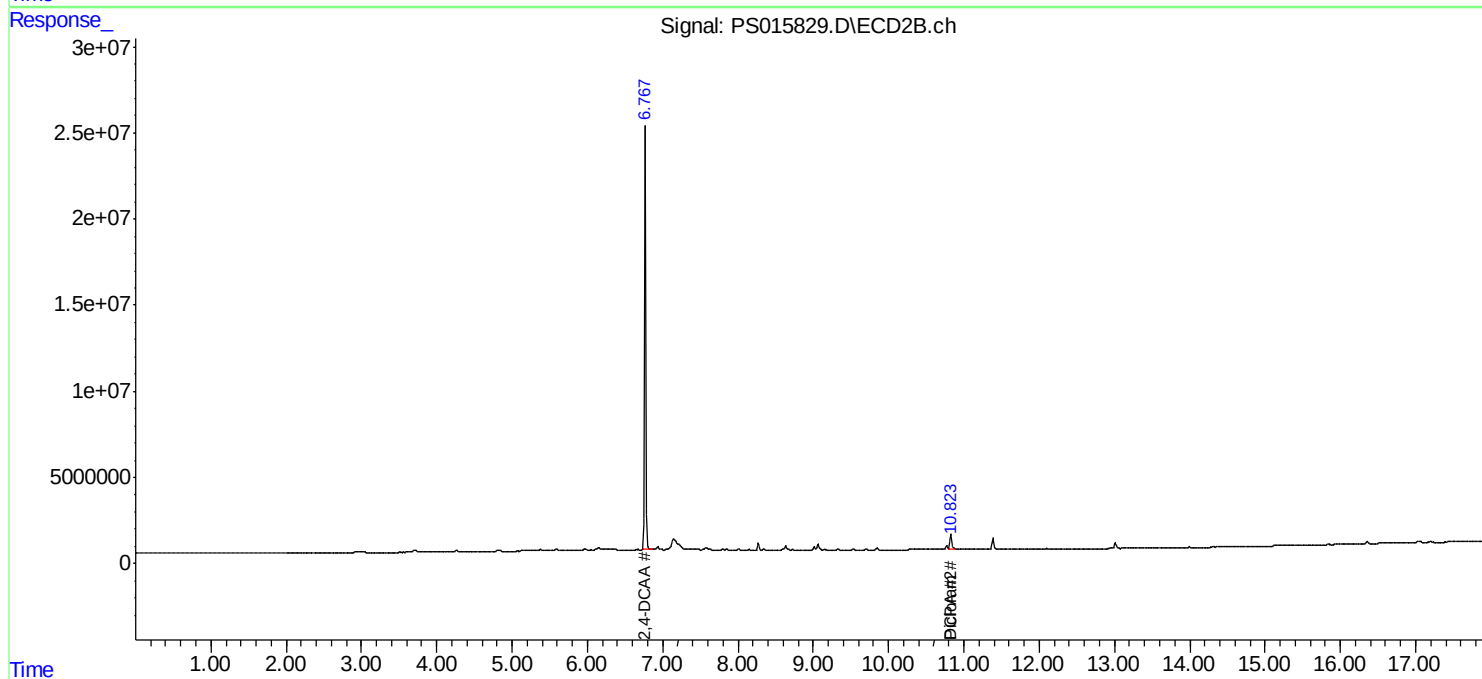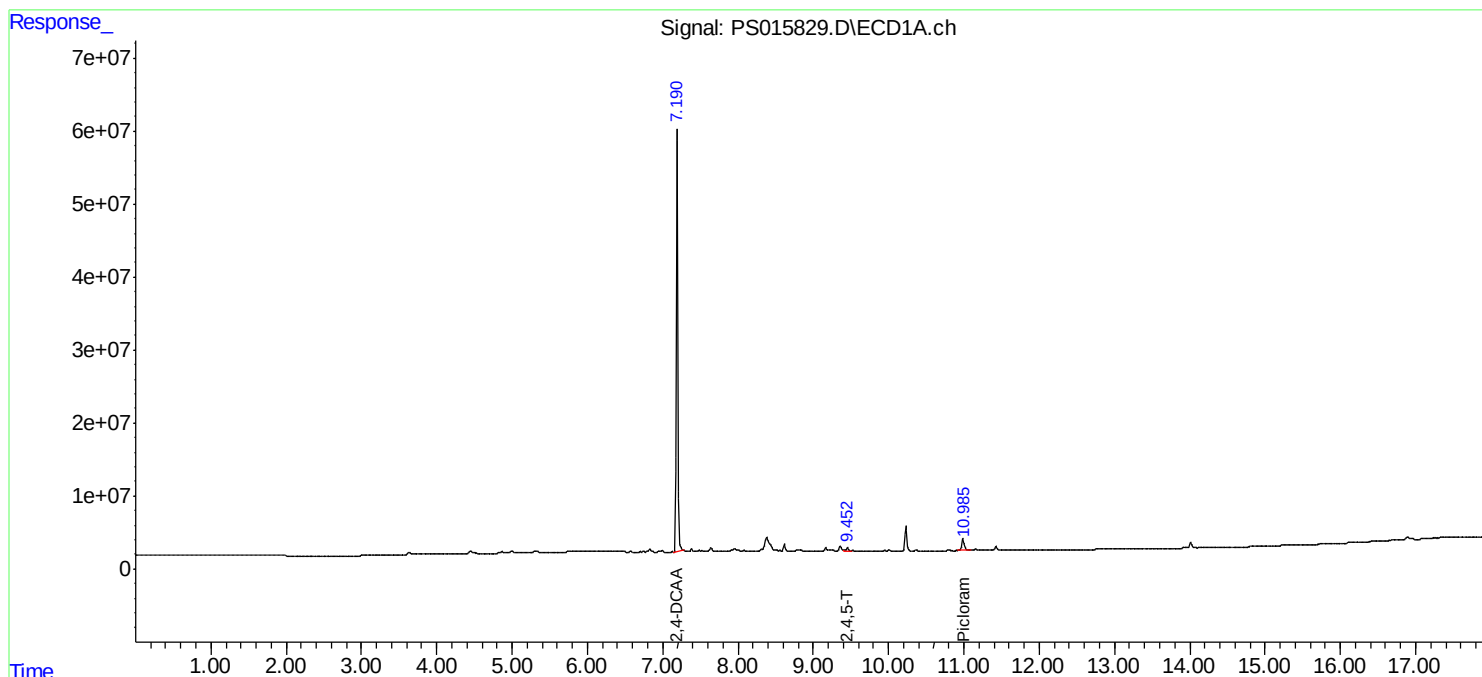

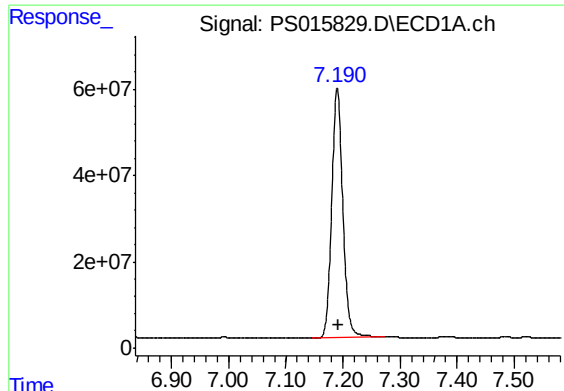


#4 2,4-DCAA

R.T.: 7.190 min
Delta R.T.: -0.003 min
Response: 781368627
Conc: 470.29 ng/ml

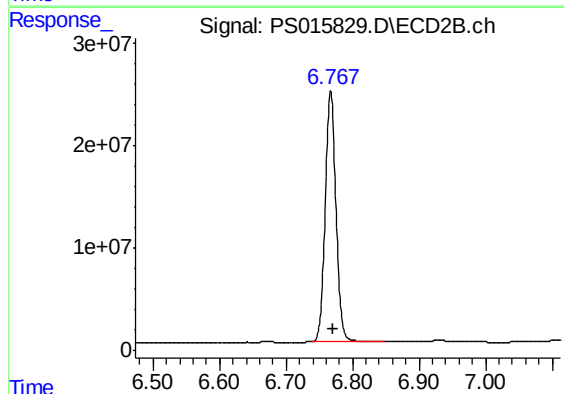


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: -0.003 min
Response: 274876213
Conc: 545.55 ng/ml

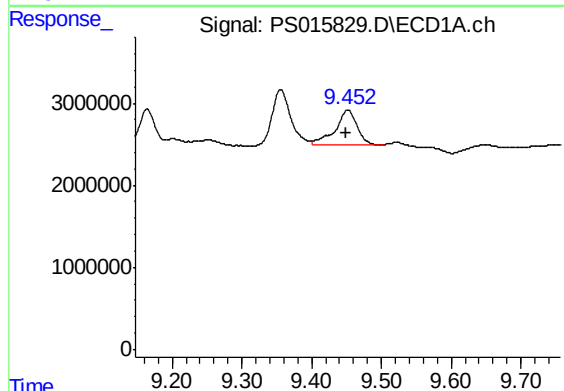


#12 2,4,5-T

R.T.: 9.452 min
Delta R.T.: 0.002 min
Response: 9398380
Conc: 1.06 ng/ml

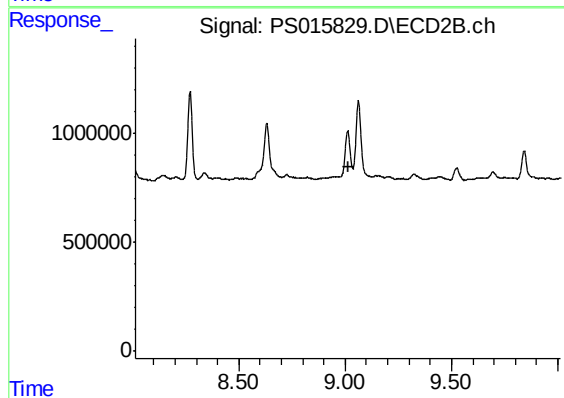


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.013 min
Response: 0
Conc: N.D.

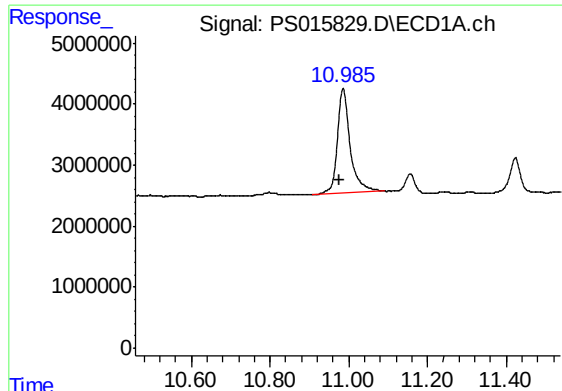


#15 Picloram

R.T.: 10.986 min
Delta R.T.: 0.008 min
Response: 38217496
Conc: 2.80 ng/ml

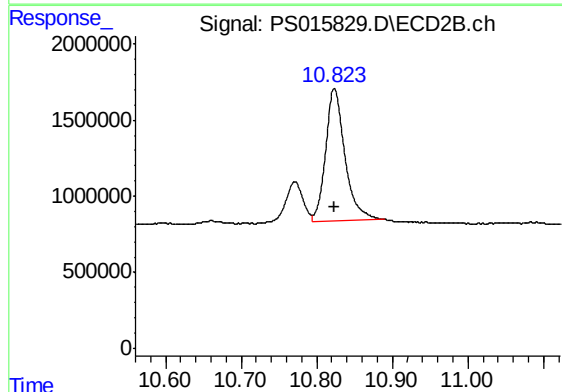


#15 Picloram

R.T.: 10.824 min
Delta R.T.: 0.000 min
Response: 15558122
Conc: 3.70 ng/ml

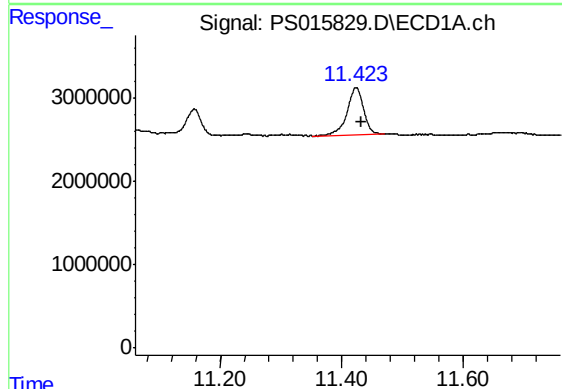

#16 DCPA

R.T.: 11.423 min
Delta R.T.: -0.008 min
Response: 10564132
Conc: N.D.

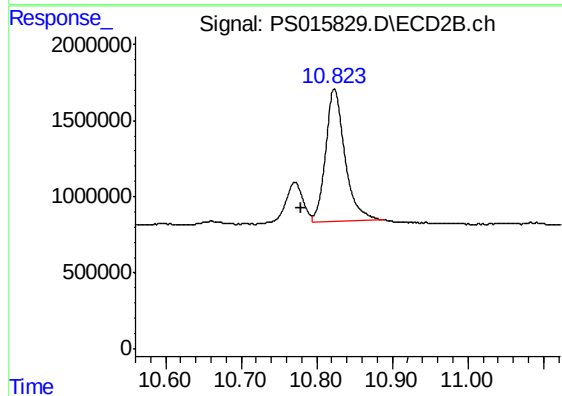

#16 DCPA

R.T.: 10.824 min
Delta R.T.: 0.045 min
Response: 15558122
Conc: 3.70 ng/ml