

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061824\
 Data File : PS027042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2024 02:58
 Operator : AR\AJ
 Sample : P2922-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 C0AB4

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/19/2024
 Supervised By :Ankita Jodhani 06/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 04:45:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061724.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 18 02:58:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	7.766	624.9E6	531.6E6	245.555	229.633m
Target Compounds							
10) T	Pentachlo...	8.622	9.531	41257.6E6	41601.8E6	1071.147m	1101.477

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061824\
Data File : PS027042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 02:58
Operator : AR\AJ
Sample : P2922-13
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
C0AB4


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/19/2024
Supervised By : Ankita Jodhani 06/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 04:45:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061724.M
Quant Title : 8080.M
QLast Update : Tue Jun 18 02:58:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

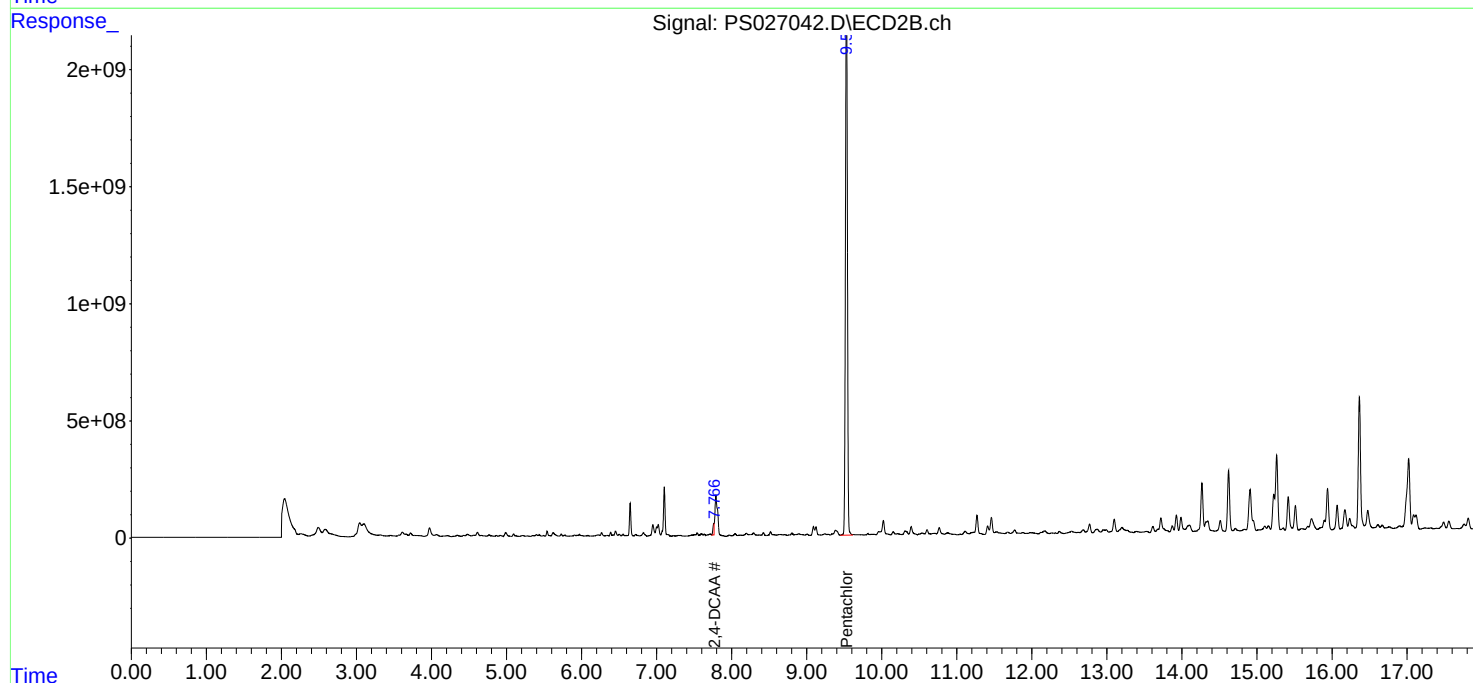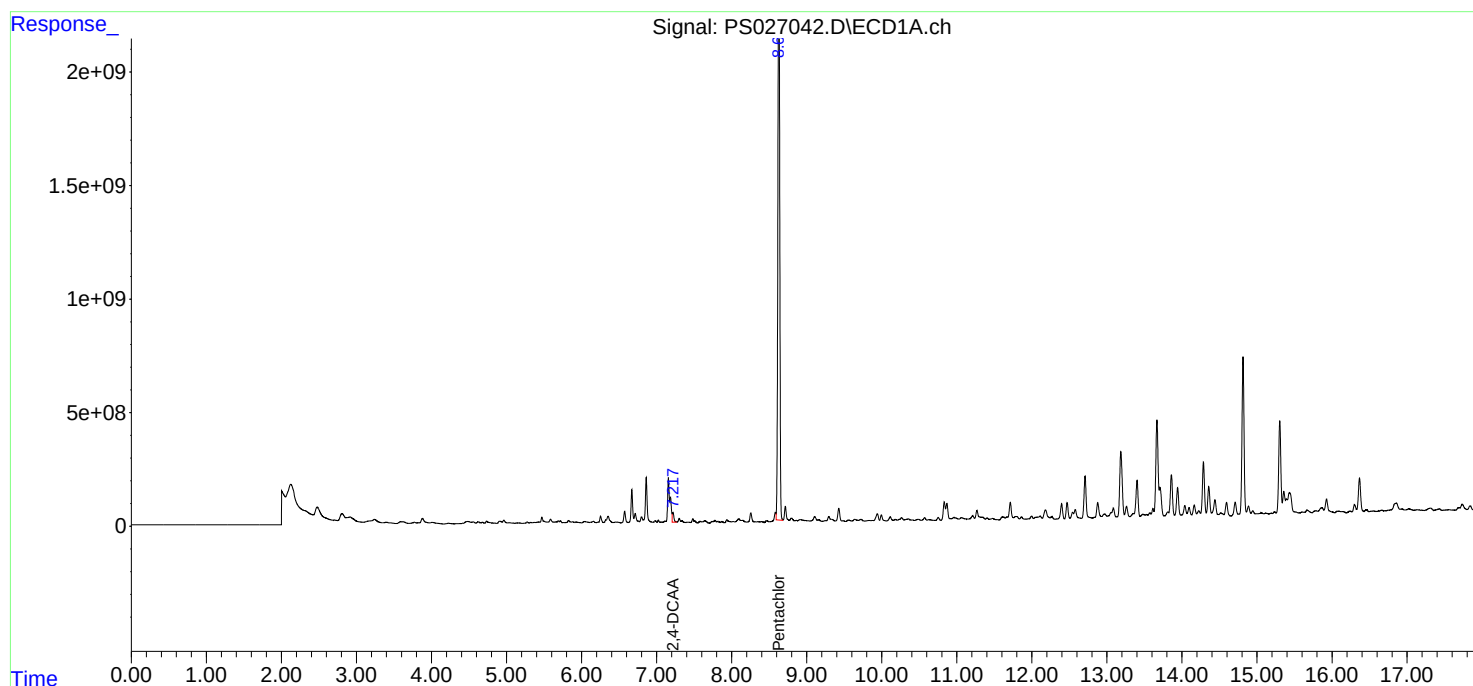

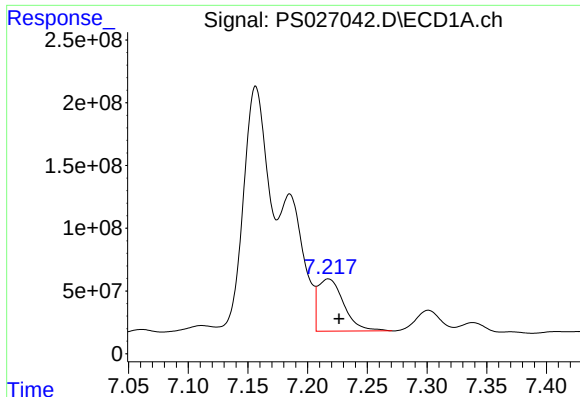


#4 2,4-DCAA

R.T.: 7.217 min
Delta R.T.: -0.009 min
Response: 624902817
Conc: 245.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
C0AB4


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/19/2024
Supervised By :Ankita Jodhani 06/19/2024

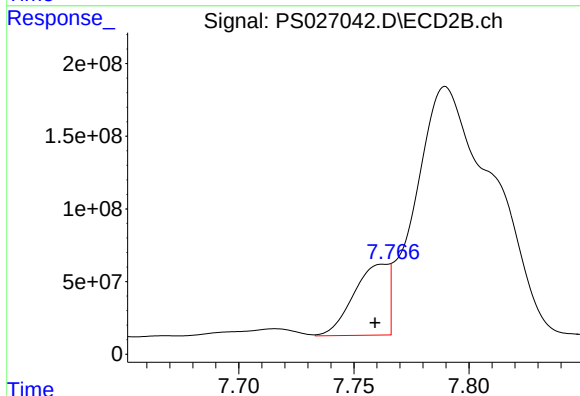


#4 2,4-DCAA

R.T.: 7.766 min
Delta R.T.: 0.007 min
Response: 531633526
Conc: 229.63 ng/ml m

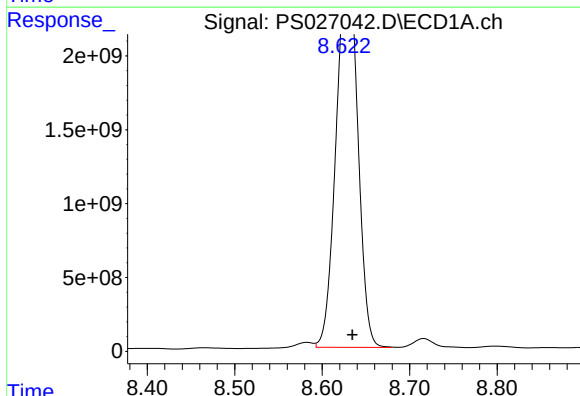

#10 Pentachlorophenol

R.T.: 8.622 min
Delta R.T.: -0.013 min
Response: 41257589979
Conc: 1071.15 ng/ml m

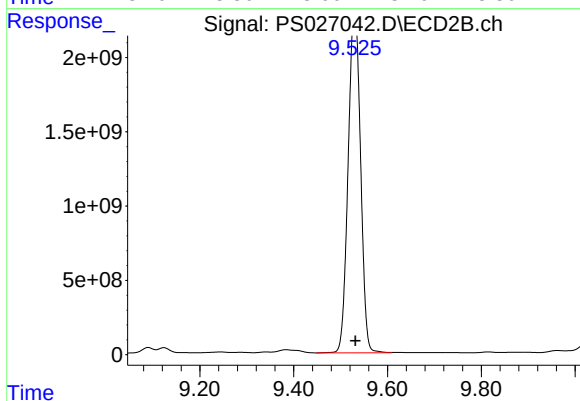

#10 Pentachlorophenol

R.T.: 9.531 min
Delta R.T.: 0.000 min
Response: 41601849016
Conc: 1101.48 ng/ml