

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061918\
 Data File : PS000441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2018 09:29
 Operator : UA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 14:22:17 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	2.560	0	140102	N.D.	0.321 #
10) T	Pentachlo...	14.075	0.000	482820	0	0.092	N.D. #
12) T	2,4,5-T	15.342	14.808	833959	497887	0.387	0.294
15) T	Picloram	17.363	17.131	1136238	901246	0.389	0.361
16) T	DCPA	17.946	17.069	860720	435424	0.336	0.189 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061918\
Data File : PS000441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2018 09:29
Operator : UA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 14:22:17 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

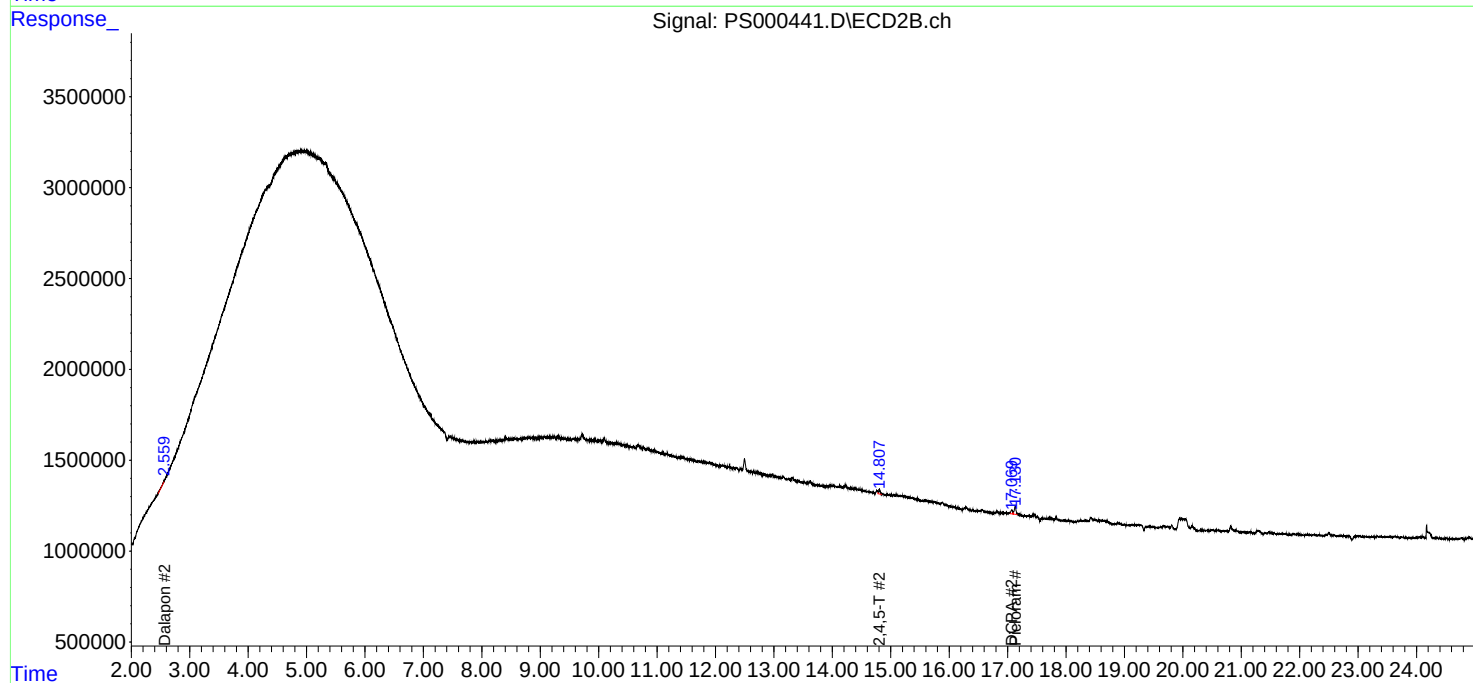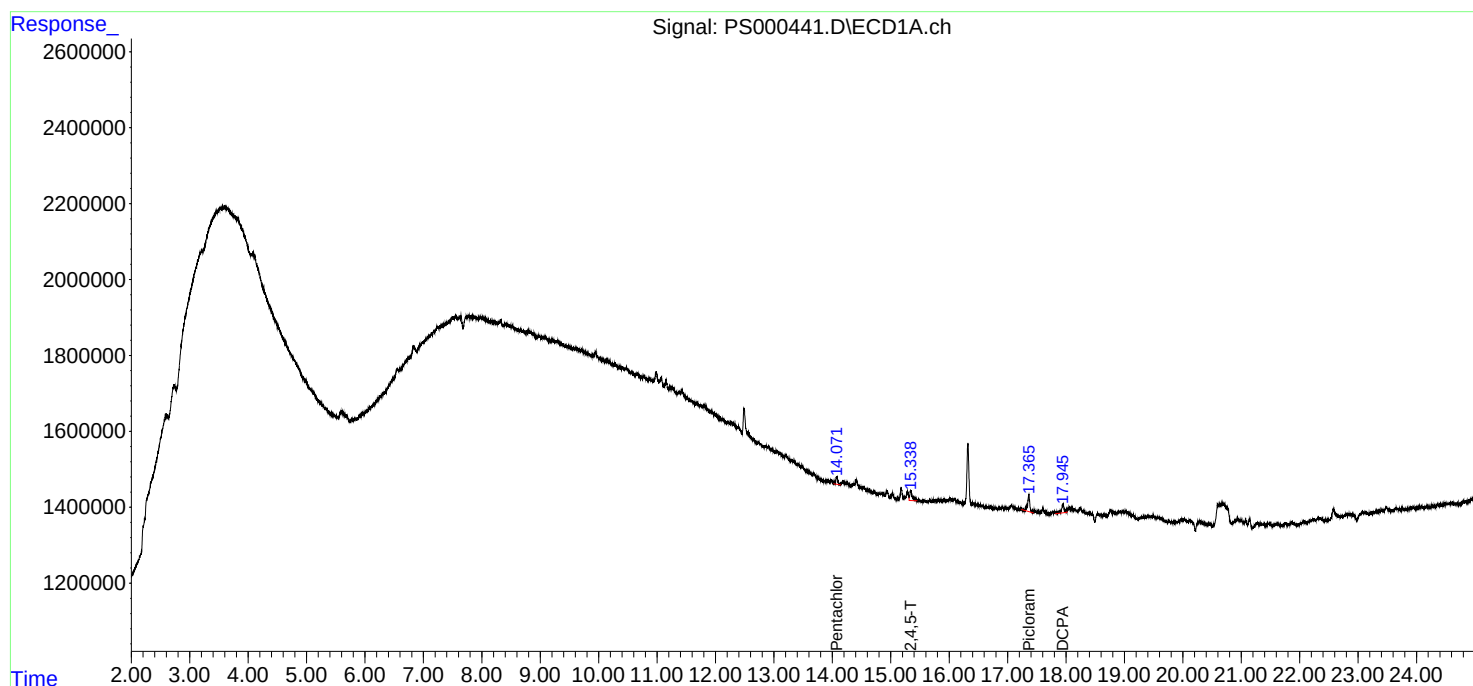


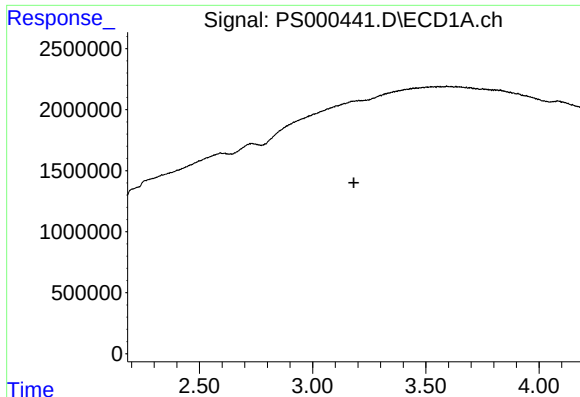

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

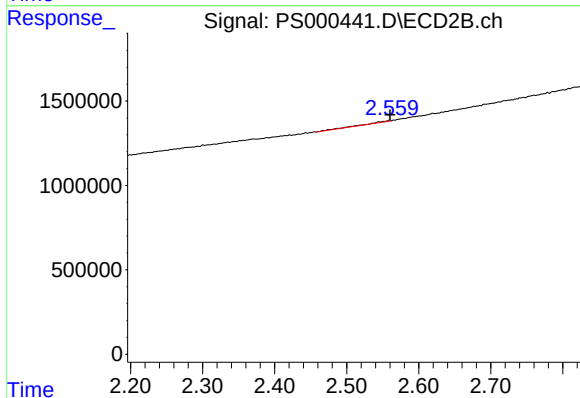


#1 Dalapon

R.T.: 2.560 min
Delta R.T.: 0.000 min
Response: 140102
Conc: 0.32 ng/ml

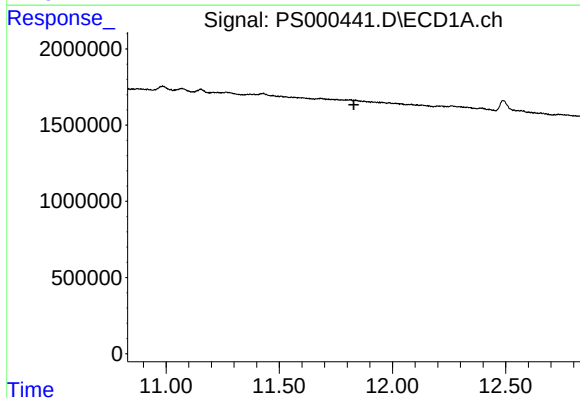


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.829 min
Response: 0
Conc: N.D.

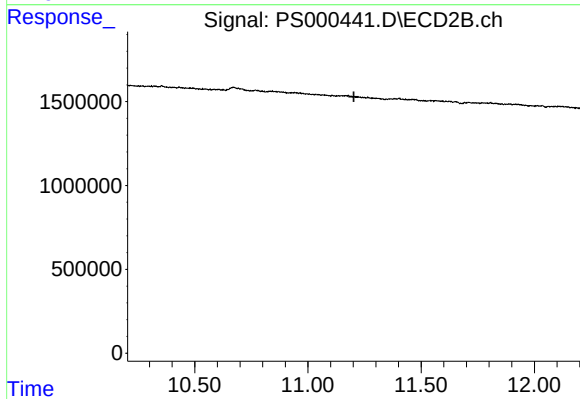

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.203 min
Response: 0
Conc: N.D.

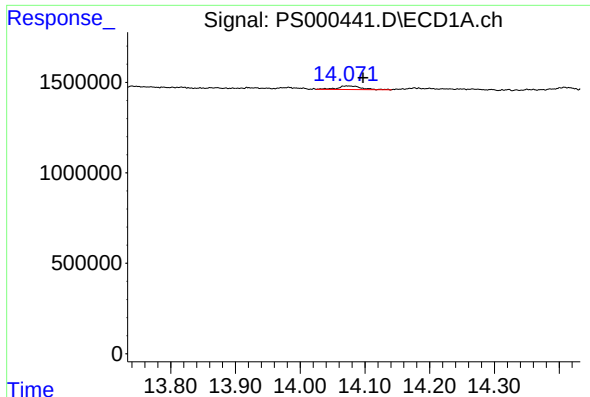

#10 Pentachlorophenol


R.T.: 14.075 min
Delta R.T.: -0.022 min
Response: 482820
Conc: 0.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

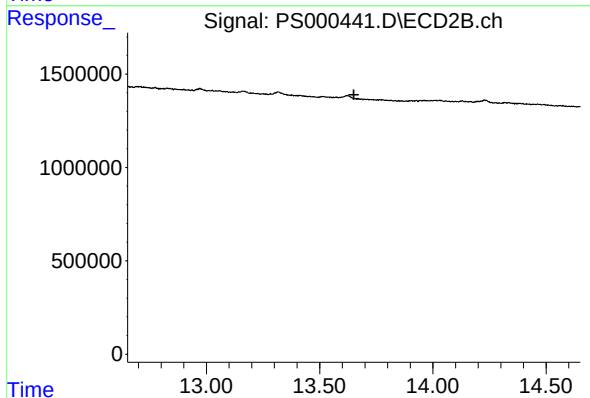


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.651 min
Response: 0
Conc: N.D.

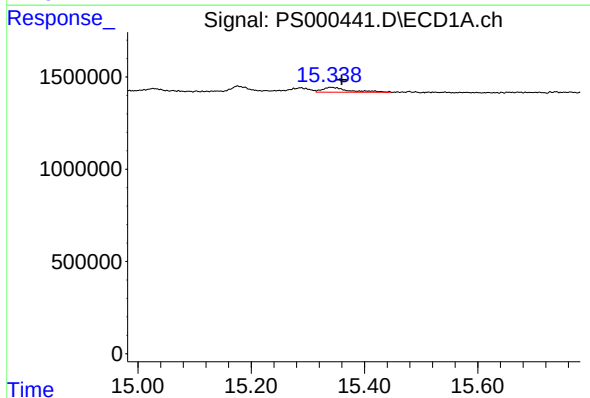


#12 2,4,5-T

R.T.: 15.342 min
Delta R.T.: -0.018 min
Response: 833959
Conc: 0.39 ng/ml

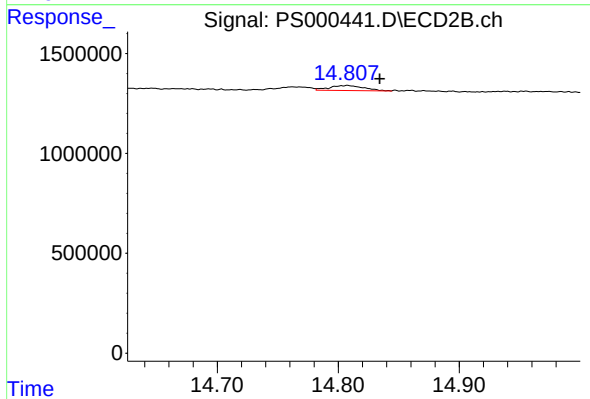

#12 2,4,5-T


R.T.: 14.808 min
Delta R.T.: -0.027 min
Response: 497887
Conc: 0.29 ng/ml

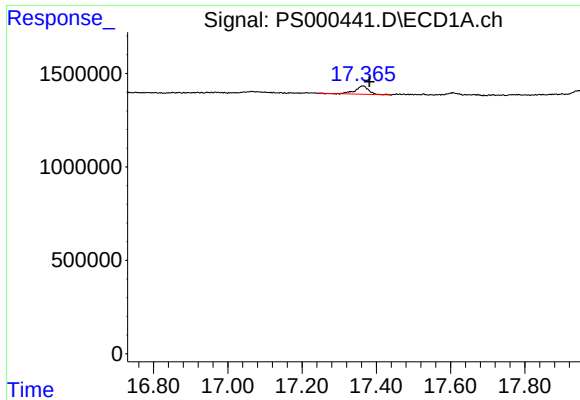

#15 Picloram


R.T.: 17.363 min
Delta R.T.: -0.019 min
Response: 1136238
Conc: 0.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

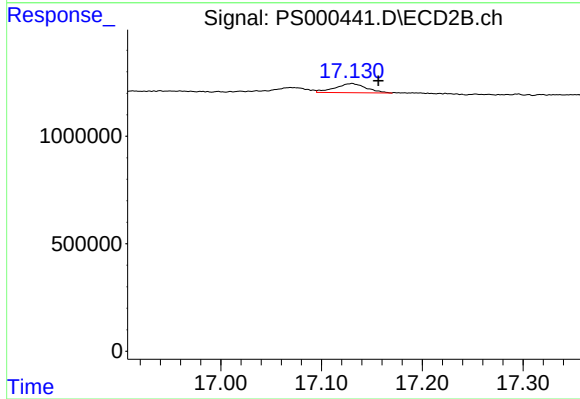


#15 Picloram

R.T.: 17.131 min
Delta R.T.: -0.026 min
Response: 901246
Conc: 0.36 ng/ml

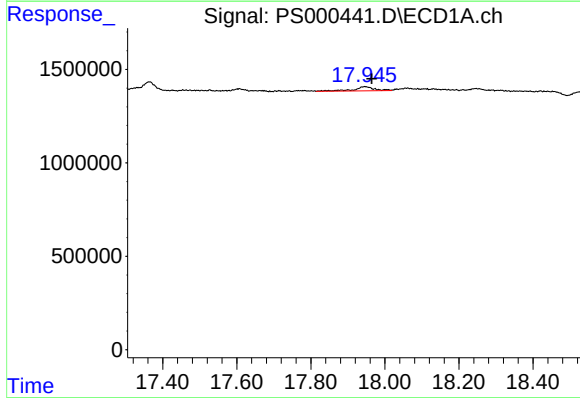

#16 DCPA

R.T.: 17.946 min
Delta R.T.: -0.019 min
Response: 860720
Conc: 0.34 ng/ml

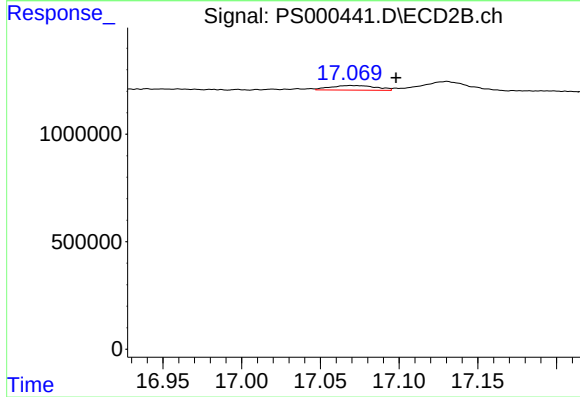

#16 DCPA

R.T.: 17.069 min
Delta R.T.: -0.029 min
Response: 435424
Conc: 0.19 ng/ml