

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061918\
 Data File : PS000455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2018 17:53
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 00:48:34 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.840	11.214	194.4E6	131.9E6	516.165	387.704
Target Compounds							
1) T	Dalapon	0.000	2.604	0	18910	N.D.	0.043 #
3) T	4-Nitroph...	11.464	0.000	550360	0	2.341	N.D. #
6) T	MCP	12.523	0.000	435060	0	0.384	N.D. #
11) T	2,4,5-TP ...	14.963	0.000	359451	0	0.166	N.D. #
12) T	2,4,5-T	15.298	0.000	144761	0	0.067	N.D. #
15) T	Picloram	0.000	17.175	0	148951	N.D.	0.060 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061918\
Data File : PS000455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2018 17:53
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 00:48:34 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

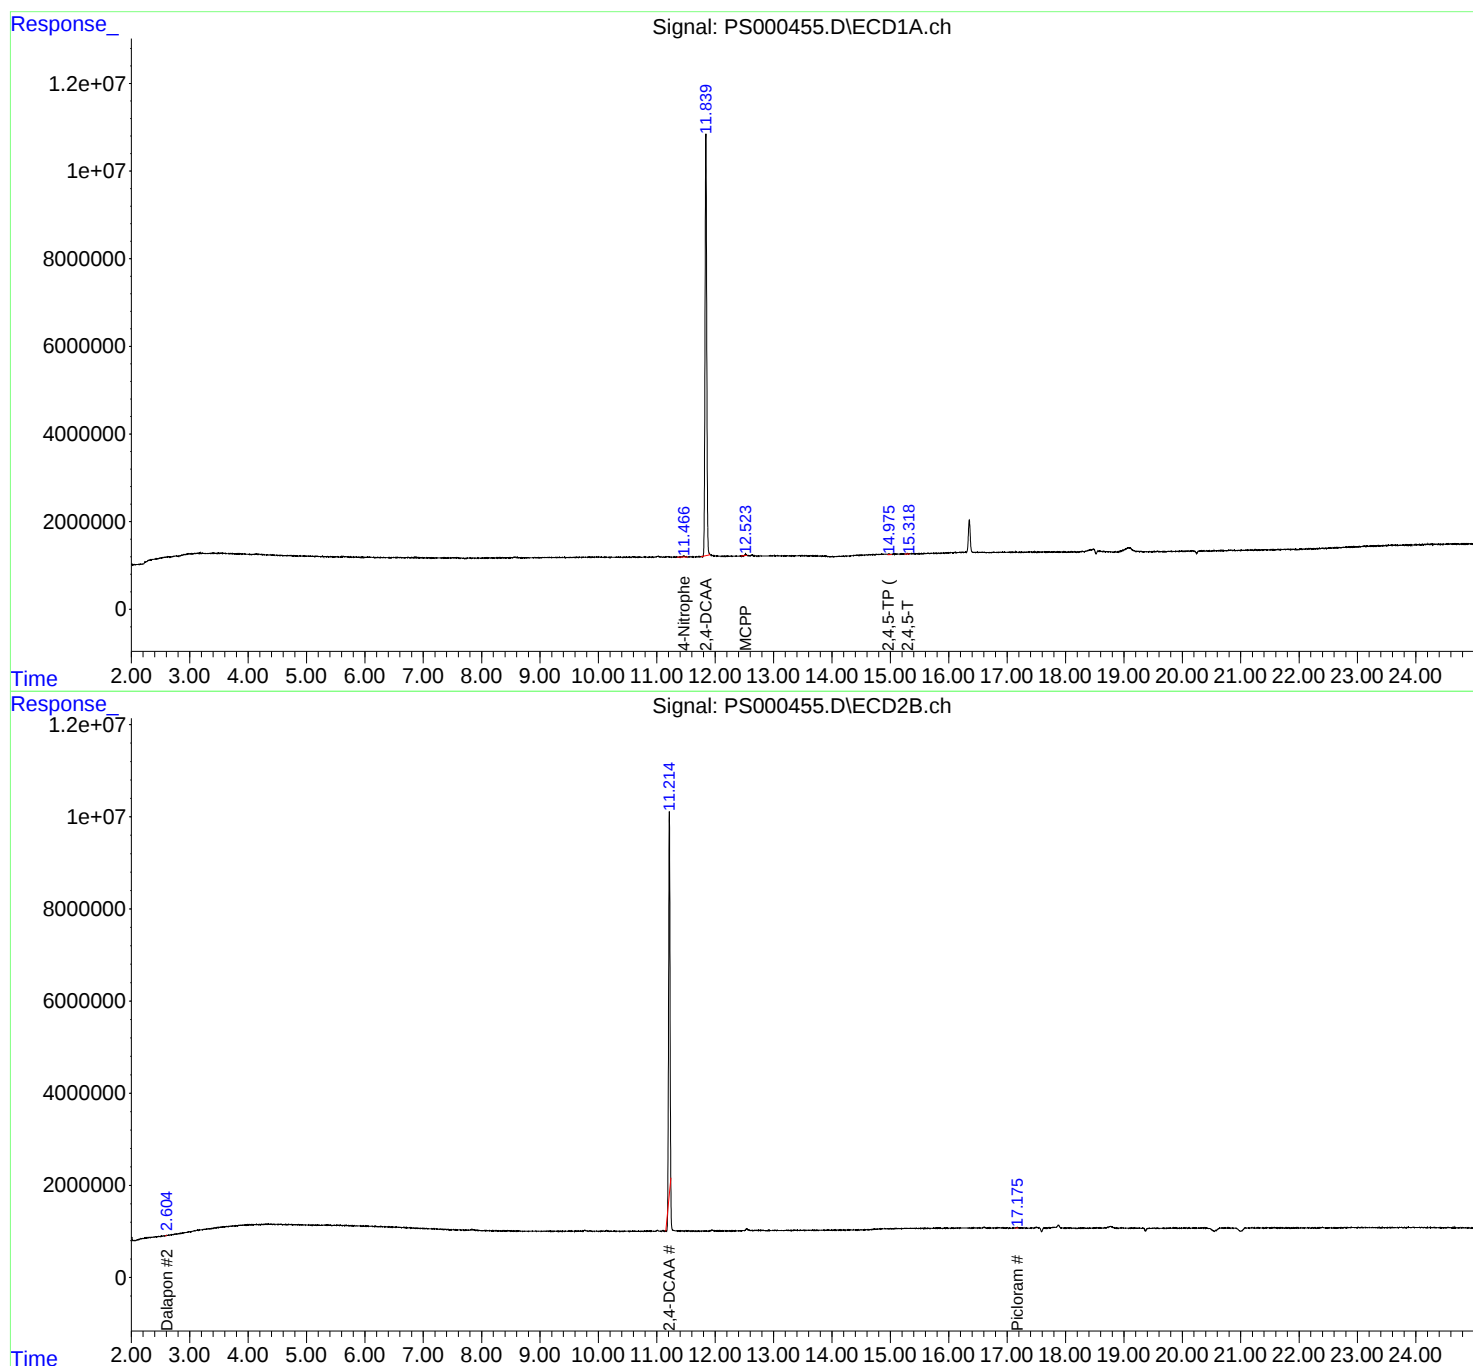


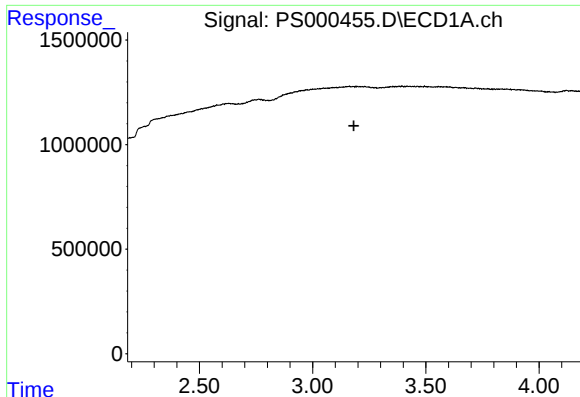

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

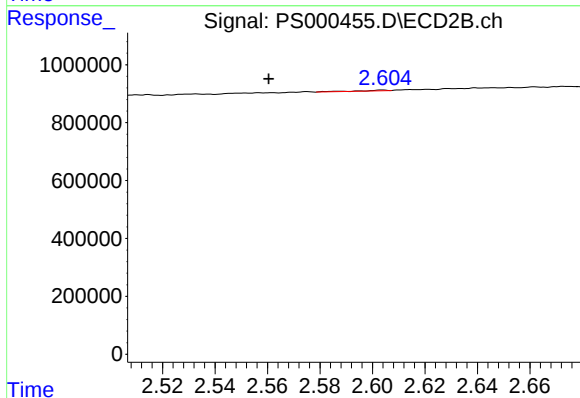


#1 Dalapon

R.T.: 2.604 min
Delta R.T.: 0.044 min
Response: 18910
Conc: 0.04 ng/ml

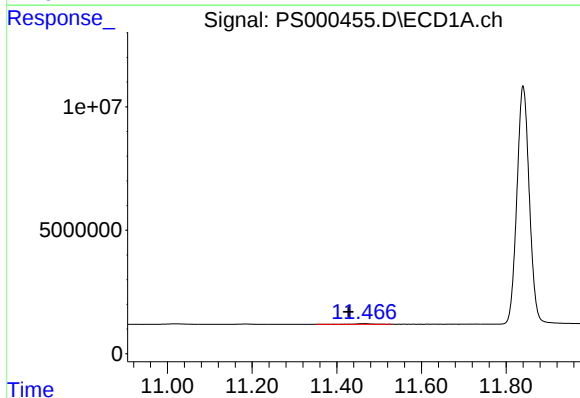


#3 4-Nitrophenol

R.T.: 11.464 min
Delta R.T.: 0.037 min
Response: 550360
Conc: 2.34 ng/ml

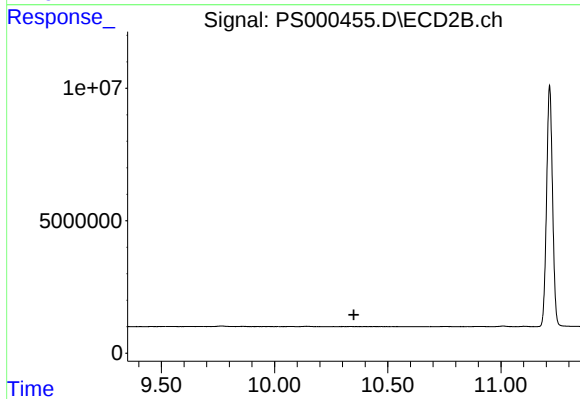

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.350 min
Response: 0
Conc: N.D.

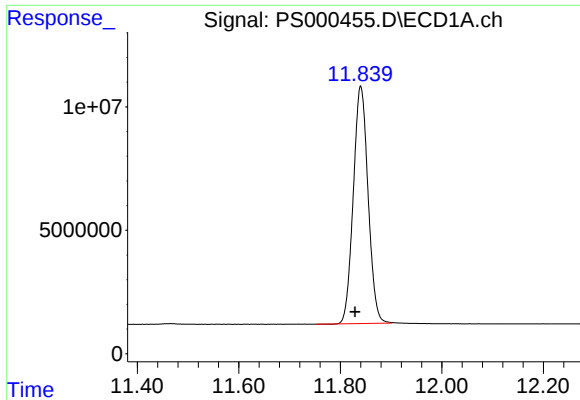

#4 2,4-DCAA


R.T.: 11.840 min
Delta R.T.: 0.011 min
Response: 194415860
Conc: 516.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

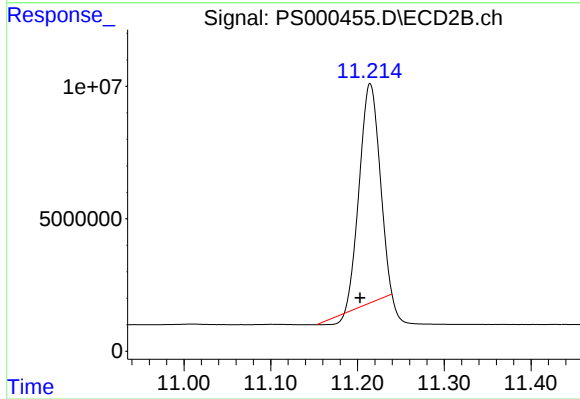


#4 2,4-DCAA

R.T.: 11.214 min
Delta R.T.: 0.012 min
Response: 131939121
Conc: 387.70 ng/ml

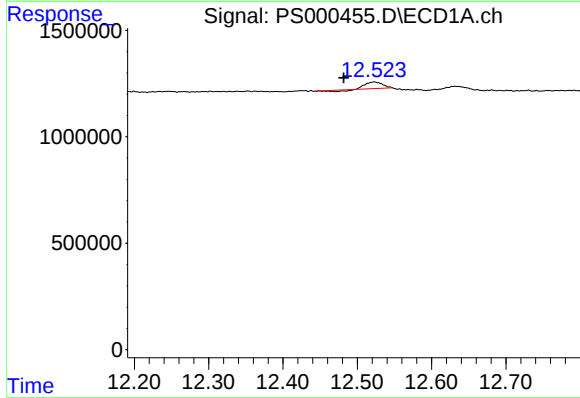


#6 MCP

R.T.: 12.523 min
Delta R.T.: 0.041 min
Response: 435060
Conc: 0.38 ug/ml

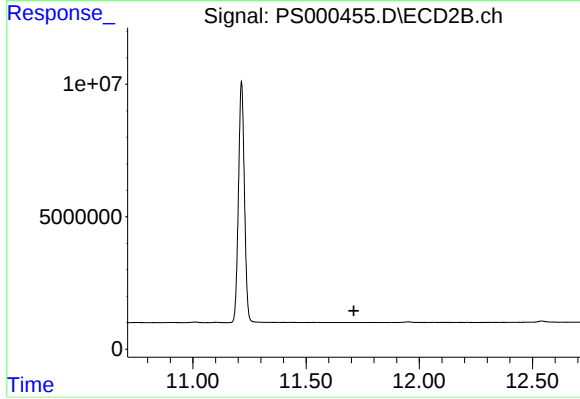

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

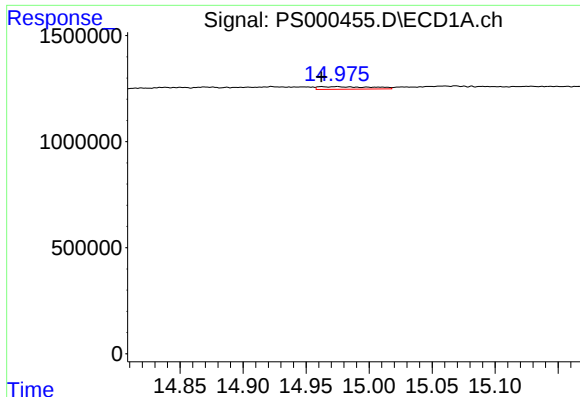

#11 2,4,5-TP (SILVEX)


R.T.: 14.963 min
Delta R.T.: 0.000 min
Response: 359451
Conc: 0.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

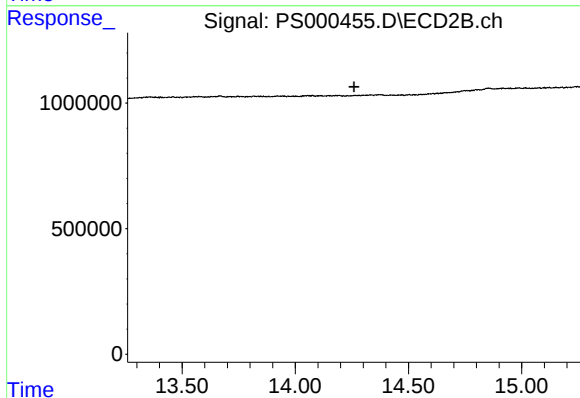


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.259 min
Response: 0
Conc: N.D.

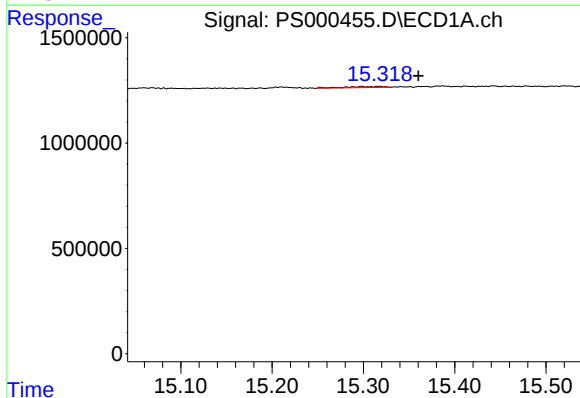


#12 2,4,5-T

R.T.: 15.298 min
Delta R.T.: -0.062 min
Response: 144761
Conc: 0.07 ng/ml

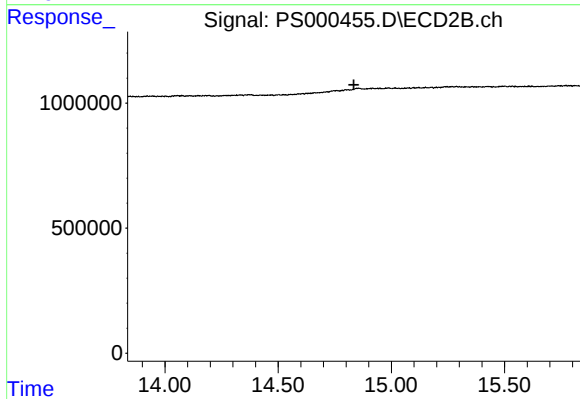

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.834 min
Response: 0
Conc: N.D.

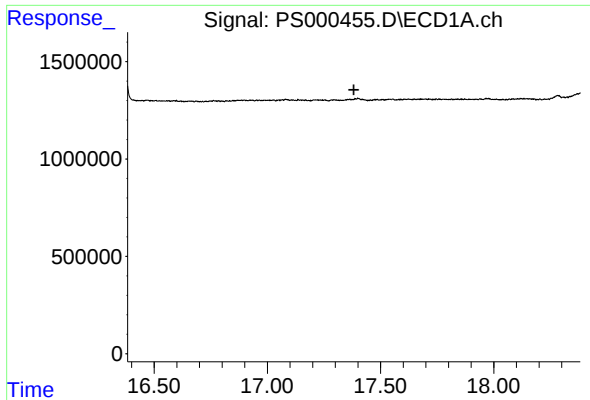

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

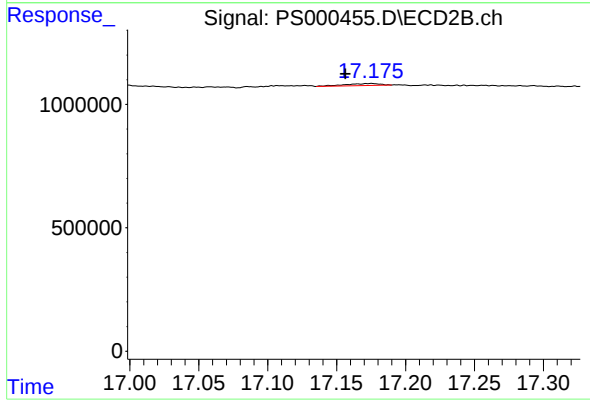

#15 Picloram

R.T.: 17.175 min
Delta R.T.: 0.019 min
Response: 148951
Conc: 0.06 ng/ml