

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061918\
 Data File : PS000467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2018 00:04
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 00:54:35 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	11.848	11.223	196.4E6	121.5E6	521.477	357.136	#
Target Compounds								
3) T	4-Nitroph...	11.471	0.000	552752	0	2.351	N.D.	#
6) T	MCP	12.528	0.000	543889	0	0.480	N.D.	#
8) T	DICHLORPROP	0.000	12.546	0	1021816	N.D.	3.174	#
10) T	Pentachlo...	14.113	0.000	341655	0	0.065	N.D.	#
15) T	Picloram	17.372	17.179	164491	406020	0.056	0.163	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061918\
Data File : PS000467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2018 00:04
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 00:54:35 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

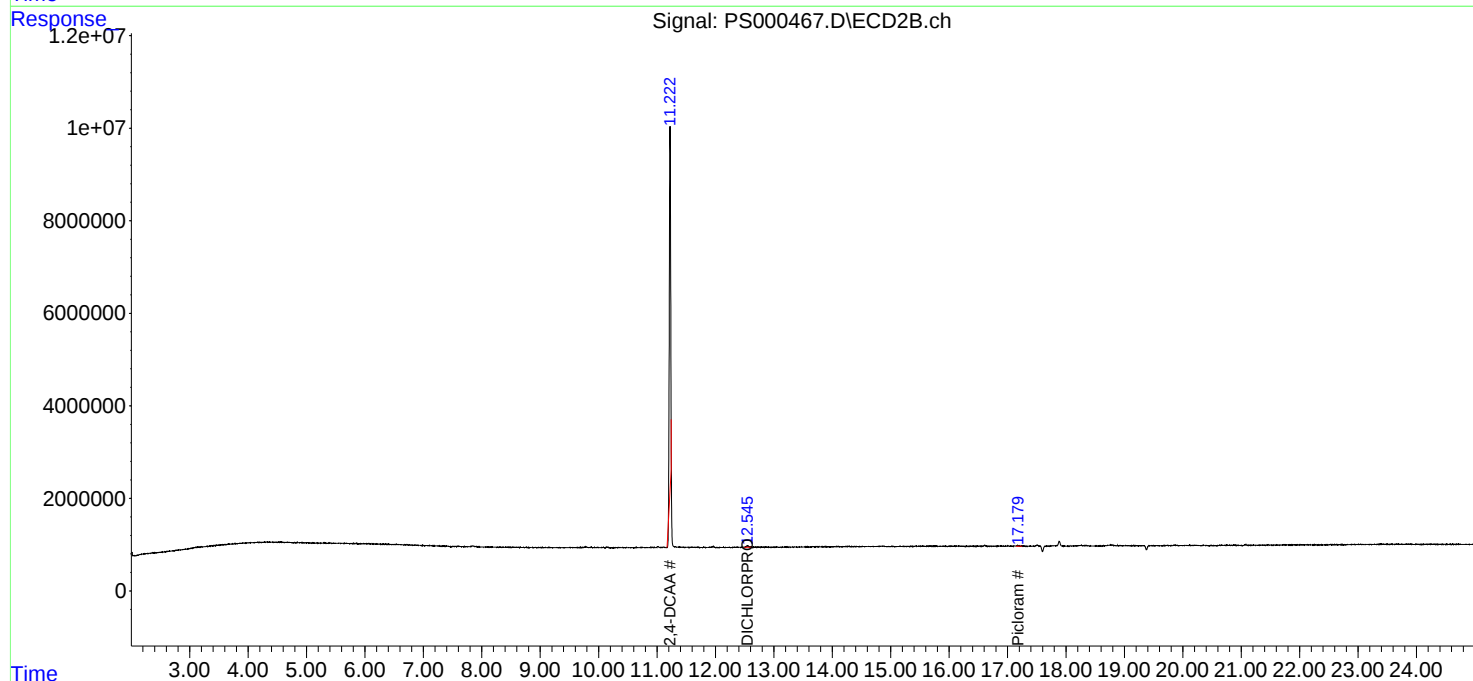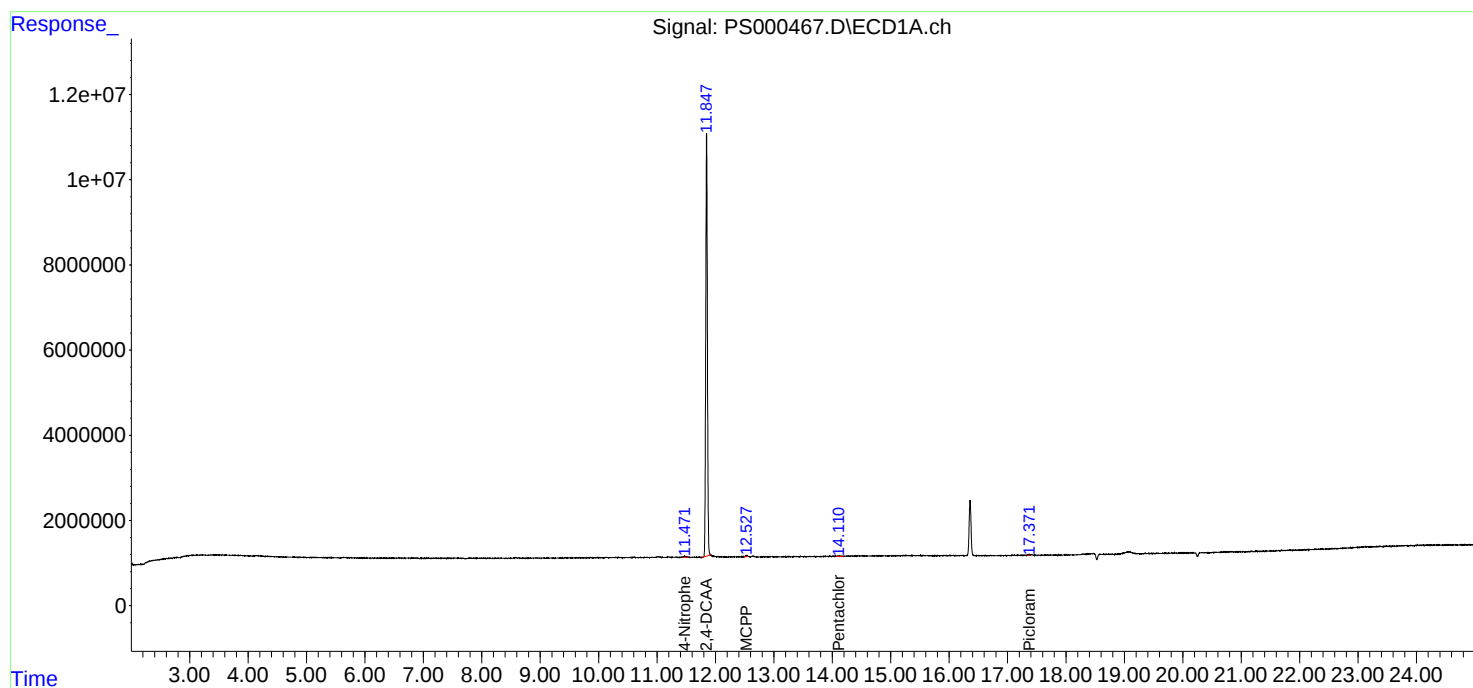


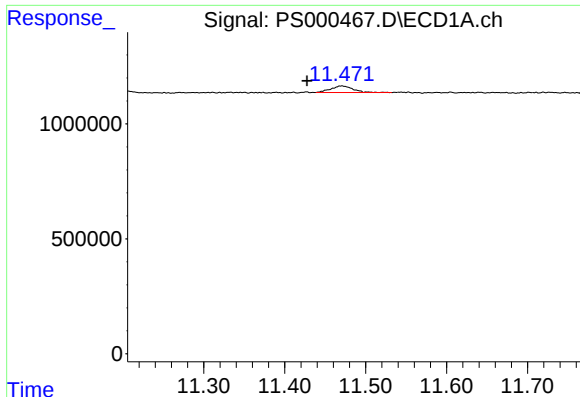

#3 4-Nitrophenol


R.T.: 11.471 min
Delta R.T.: 0.043 min
Response: 552752
Conc: 2.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

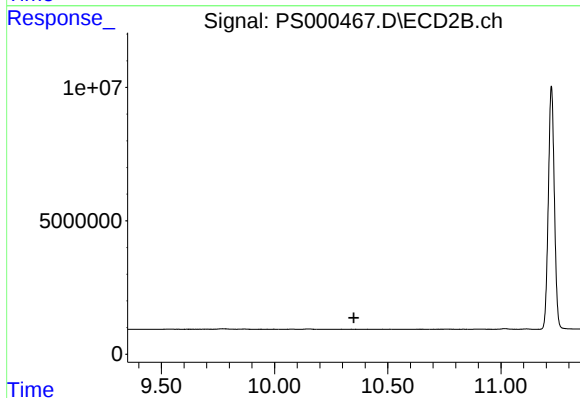


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.350 min
Response: 0
Conc: N.D.

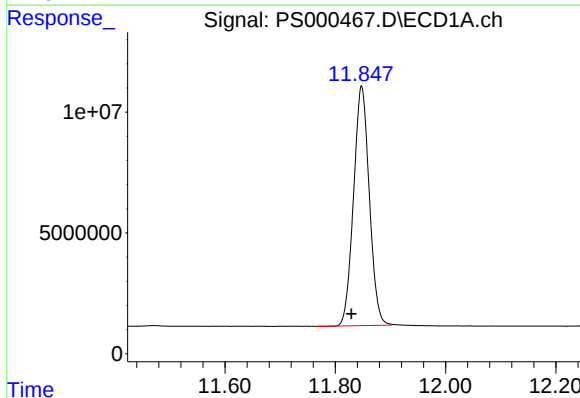


#4 2,4-DCAA

R.T.: 11.848 min
Delta R.T.: 0.018 min
Response: 196416832
Conc: 521.48 ng/ml

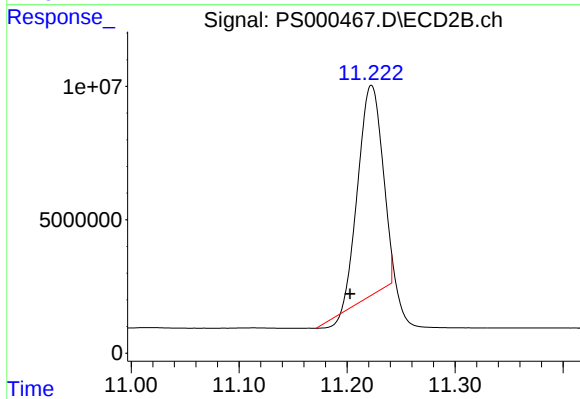

#4 2,4-DCAA


R.T.: 11.223 min
Delta R.T.: 0.020 min
Response: 121536477
Conc: 357.14 ng/ml

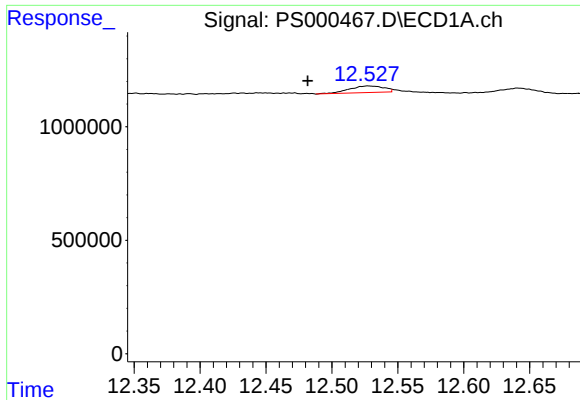

#6 MCP


R.T.: 12.528 min
Delta R.T.: 0.047 min
Response: 543889
Conc: 0.48 ug/ml

Instrument :
ECD_S
ClientSampleId :

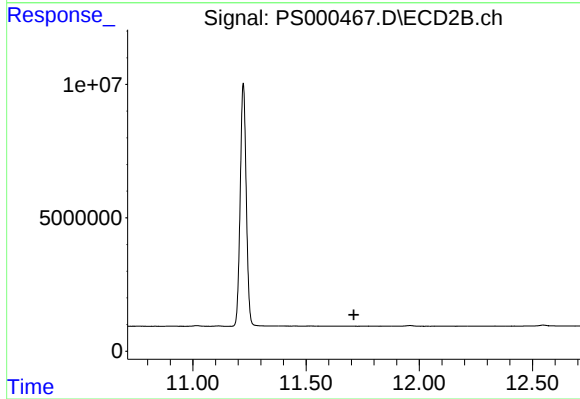


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.711 min
Response: 0
Conc: N.D.

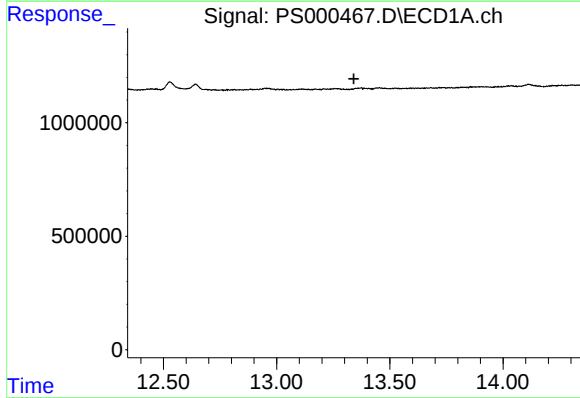


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.341 min
Response: 0
Conc: N.D.

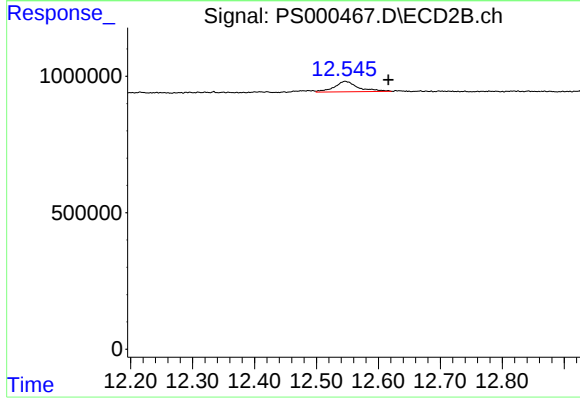

#8 DICHLORPROP


R.T.: 12.546 min
Delta R.T.: -0.070 min
Response: 1021816
Conc: 3.17 ng/ml

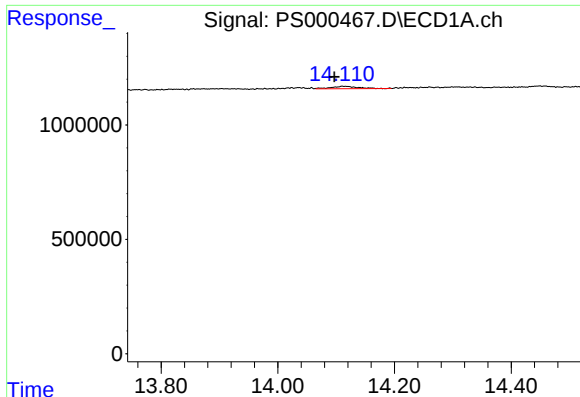

#10 Pentachlorophenol


R.T.: 14.113 min
Delta R.T.: 0.016 min
Response: 341655
Conc: 0.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

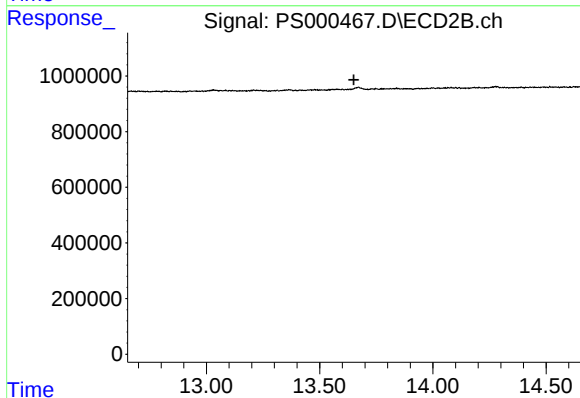


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.651 min
Response: 0
Conc: N.D.

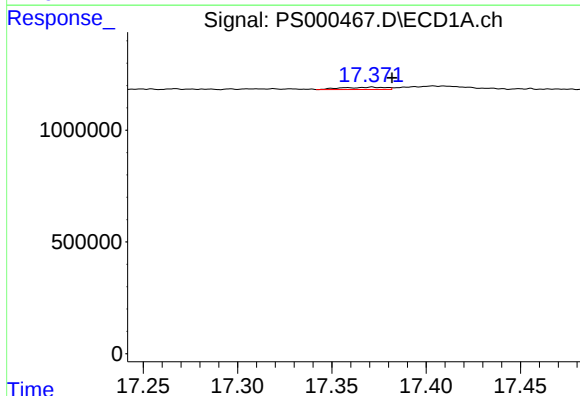

#15 Picloram

R.T.: 17.372 min
Delta R.T.: -0.010 min
Response: 164491
Conc: 0.06 ng/ml

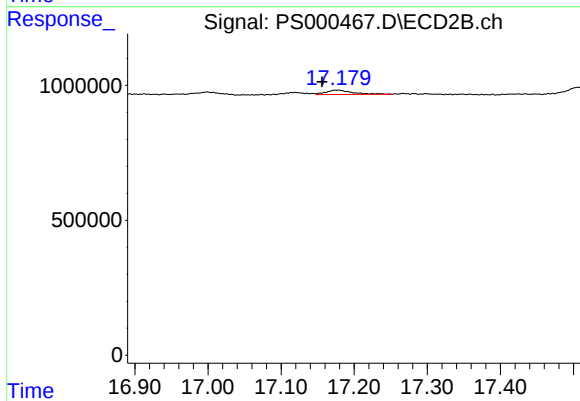

#15 Picloram

R.T.: 17.179 min
Delta R.T.: 0.023 min
Response: 406020
Conc: 0.16 ng/ml