

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061919\
 Data File : PS005115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 09:49
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 11:07:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	4.917	0.000	2937.0E6	0	1461.378	N.D. #
3) T	4-Nitroph...	5.372	0.000	27104104	0	37.421	N.D. #
5) T	DICAMBA	0.000	5.418	0	2065.7E6	N.D.	551.847
6) T	MCP	5.937	0.000	41815662	0	9.552	N.D. #
8) T	DICHLORPROP	0.000	5.953	0	23163927	N.D.	23.991
9) T	2,4-D	6.587	0.000	2416.8E6	0	1554.619	N.D. #
10) T	Pentachlo...	6.849	0.000	24301730	0	1.235	N.D. #
12) T	2,4,5-T	0.000	7.367	0	49804518	N.D.	9.764
15) T	Picloram	9.086	9.074	1229.0E6	151.3E6	106.955	20.045 #
16) T	DCPA	0.000	9.074	0	151.3E6	N.D.	22.221



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061919\
Data File : PS005115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 09:49
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 11:07:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

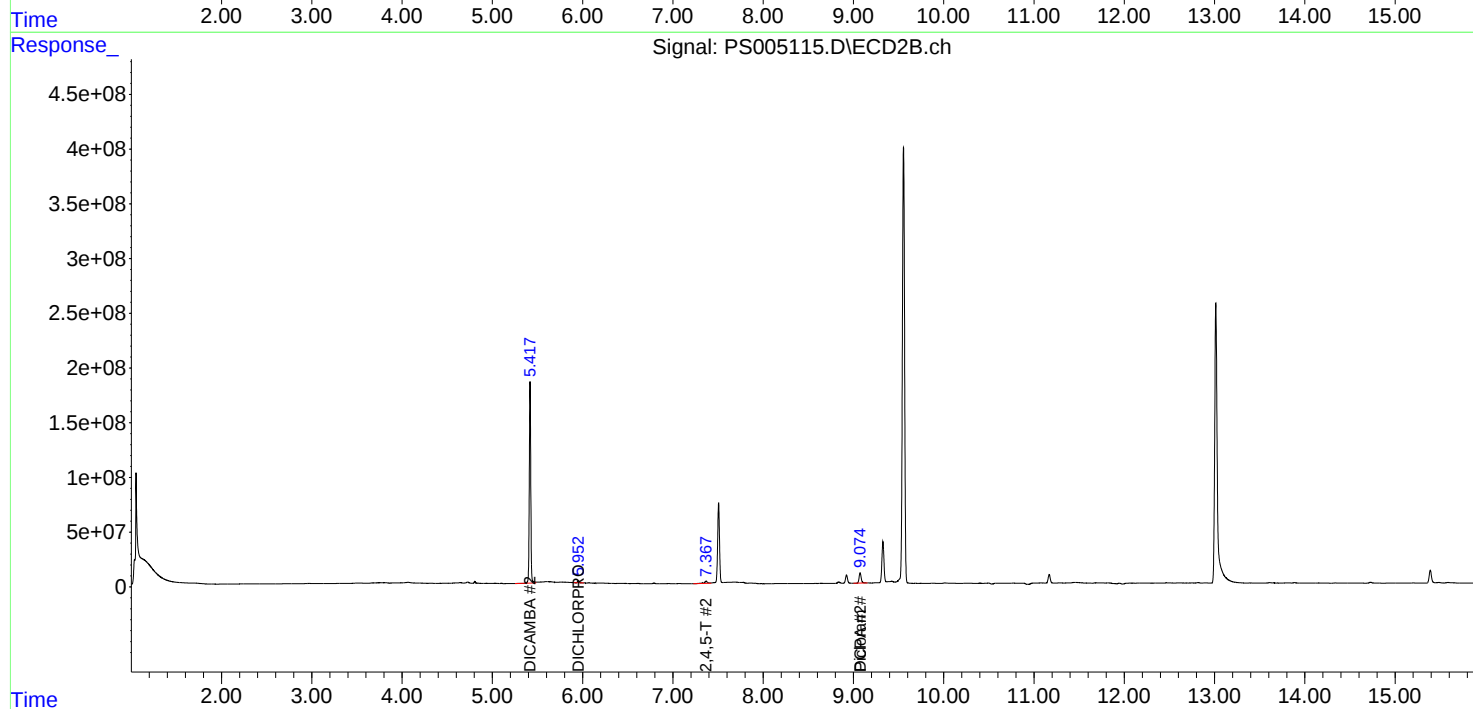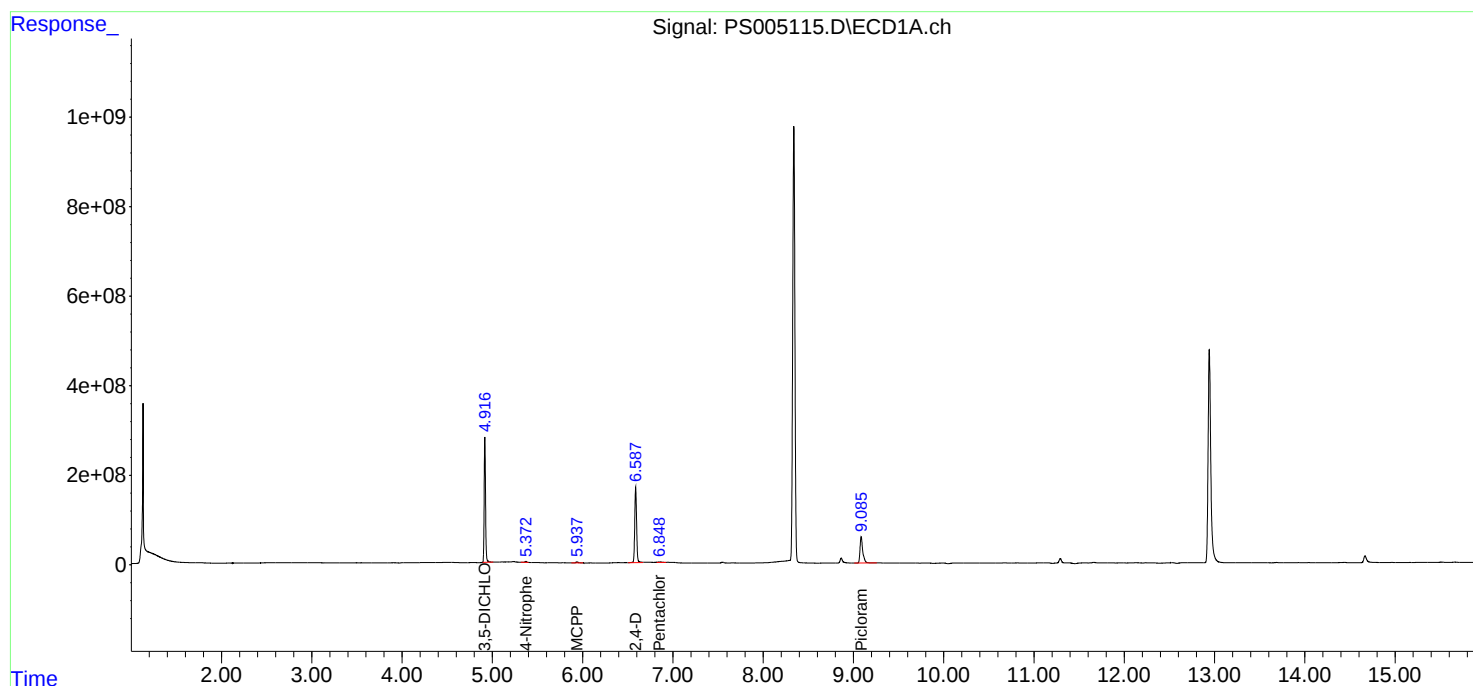


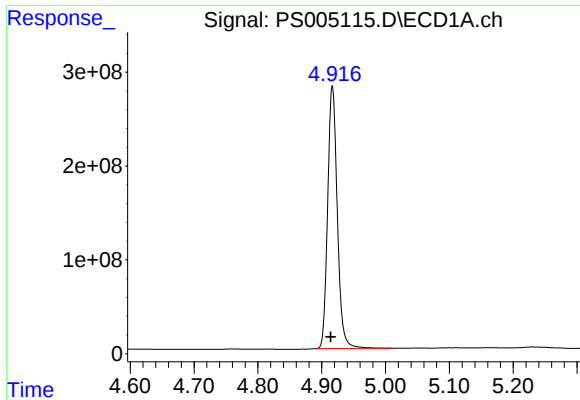

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.917 min
Delta R.T.: 0.003 min
Response: 2936957459
Conc: 1461.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

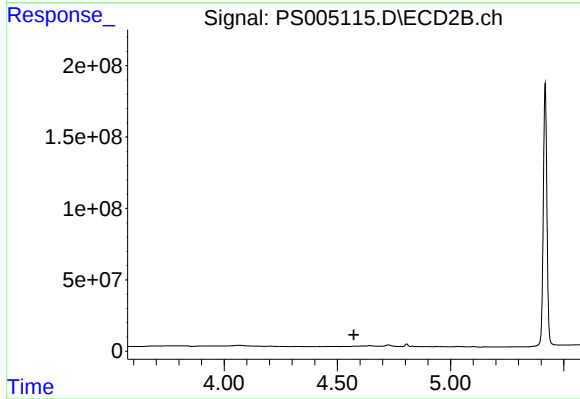


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

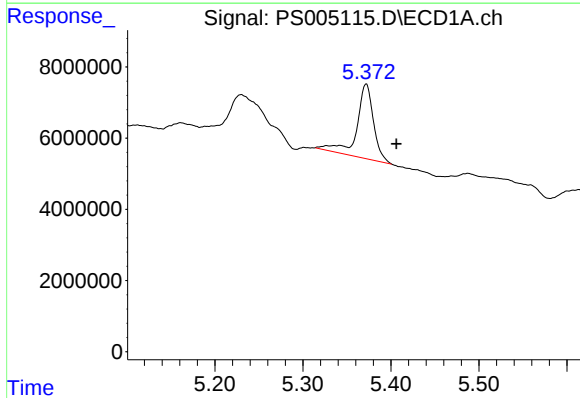


#3 4-Nitrophenol

R.T.: 5.372 min
Delta R.T.: -0.034 min
Response: 27104104
Conc: 37.42 ng/ml

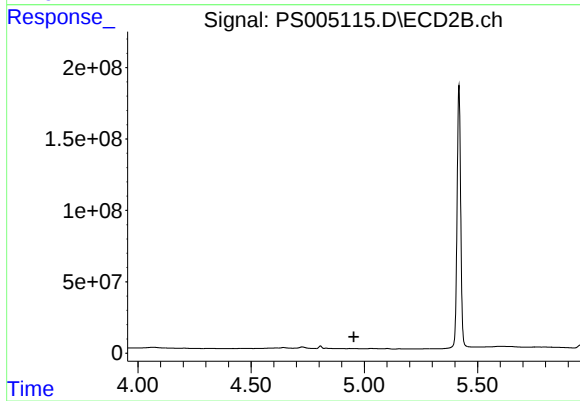

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

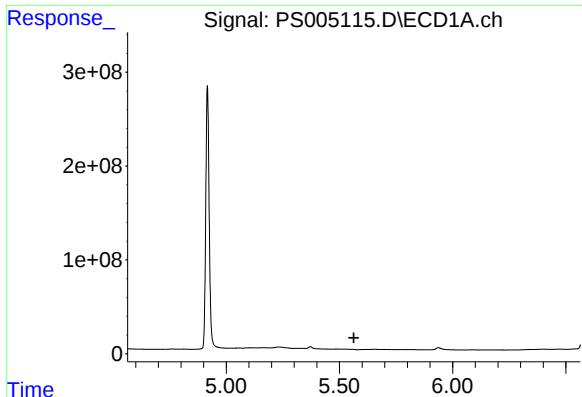

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

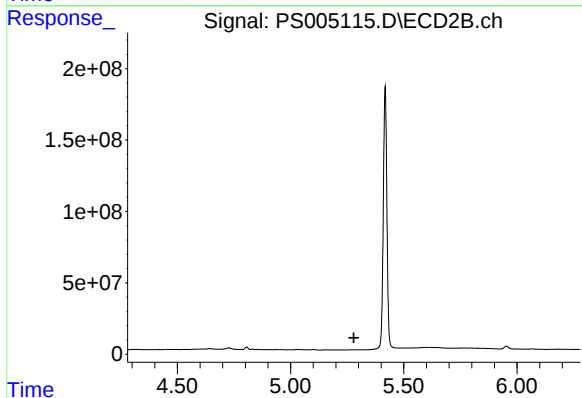


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

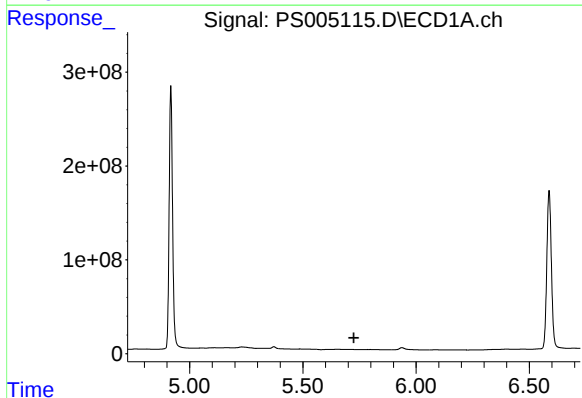


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

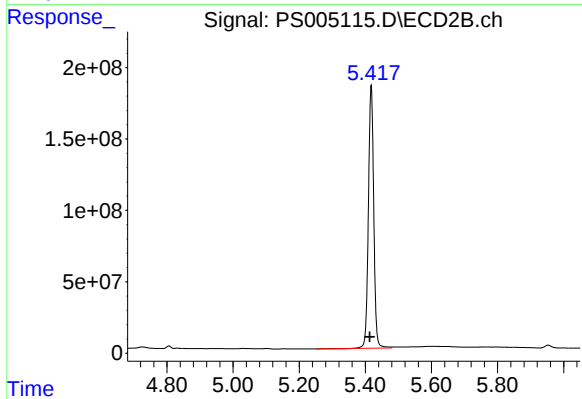

#5 DICAMBA


R.T.: 5.418 min
Delta R.T.: 0.004 min
Response: 2065742600
Conc: 551.85 ng/ml

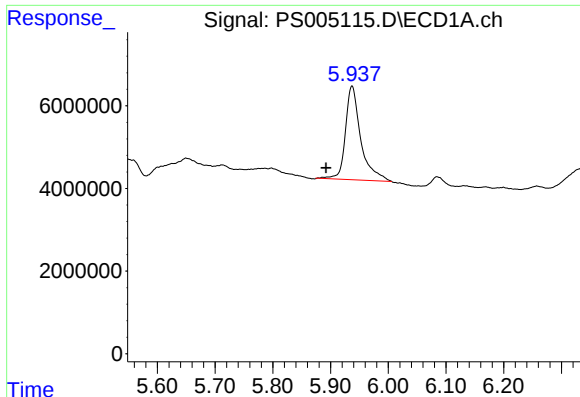

#6 MCP


R.T.: 5.937 min
Delta R.T.: 0.045 min
Response: 41815662
Conc: 9.55 ug/ml

Instrument :
ECD_S
ClientSampleId :

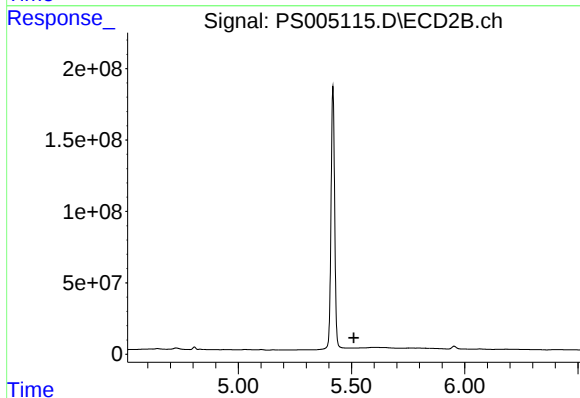


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

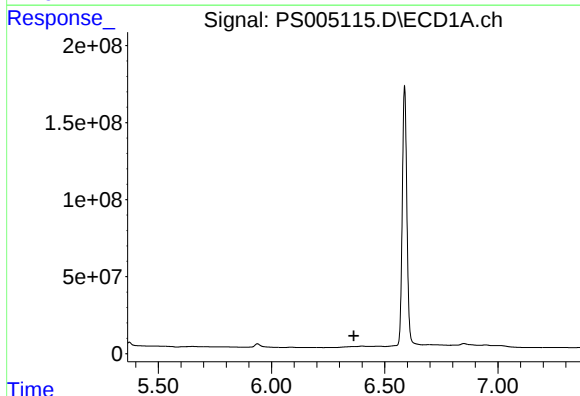


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

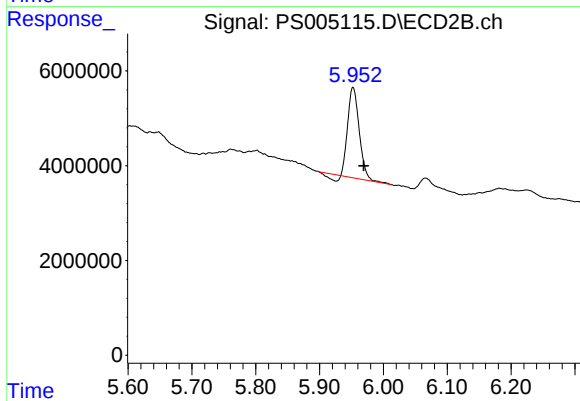

#8 DICHLORPROP


R.T.: 5.953 min
Delta R.T.: -0.016 min
Response: 23163927
Conc: 23.99 ng/ml

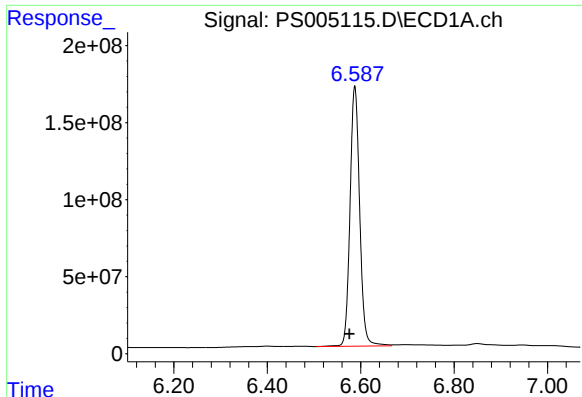

#9 2,4-D


R.T.: 6.587 min
Delta R.T.: 0.011 min
Response: 2416810429
Conc: 1554.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

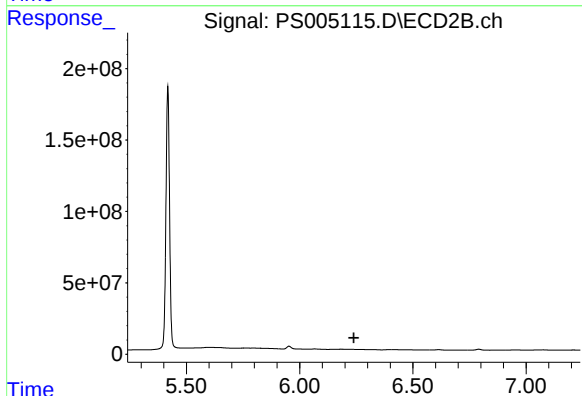


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.240 min
Response: 0
Conc: N.D.

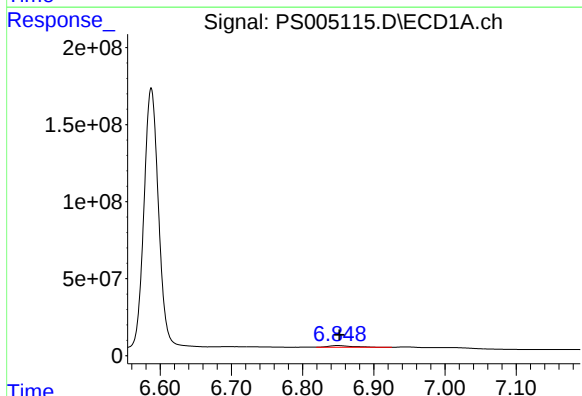


#10 Pentachlorophenol

R.T.: 6.849 min
Delta R.T.: -0.002 min
Response: 24301730
Conc: 1.24 ng/ml

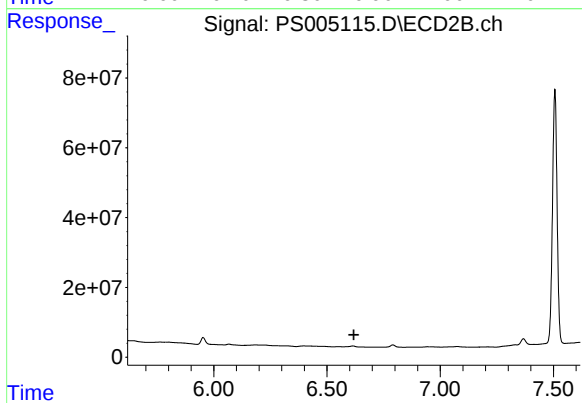

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.619 min
Response: 0
Conc: N.D.

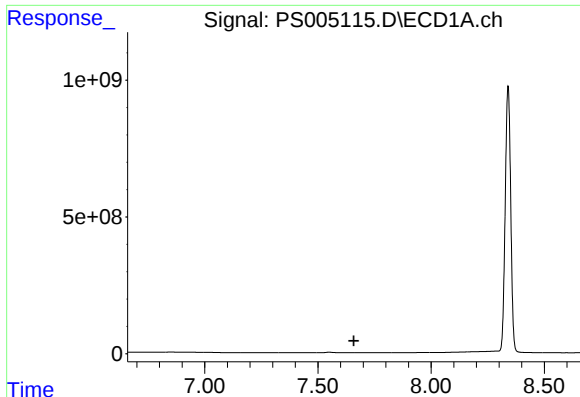

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.659 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

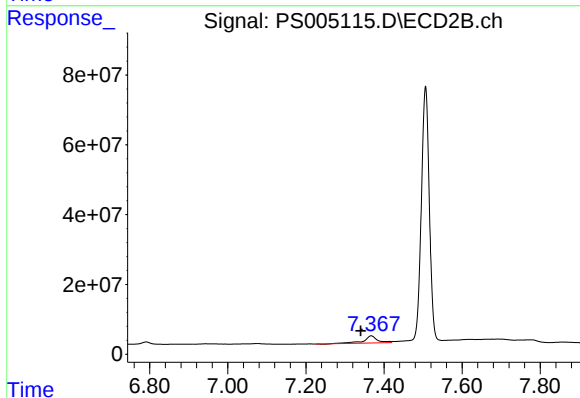


#12 2,4,5-T

R.T.: 7.367 min
Delta R.T.: 0.027 min
Response: 49804518
Conc: 9.76 ng/ml

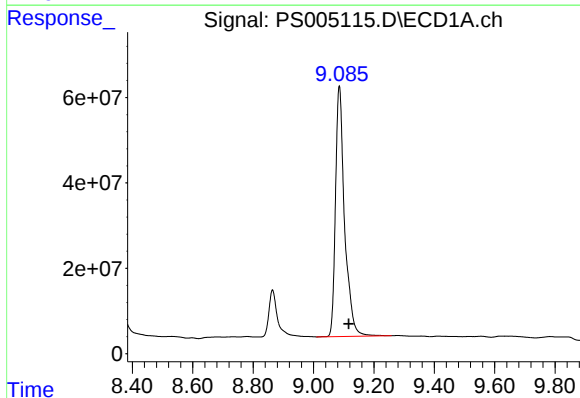


#15 Picloram

R.T.: 9.086 min
Delta R.T.: -0.031 min
Response: 1229034965
Conc: 106.96 ng/ml

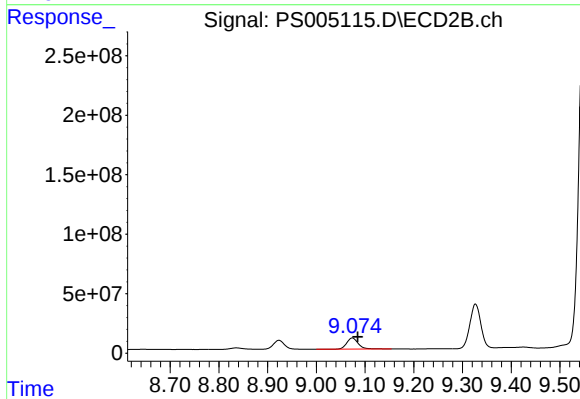

#15 Picloram


R.T.: 9.074 min
Delta R.T.: -0.011 min
Response: 151266006
Conc: 20.04 ng/ml

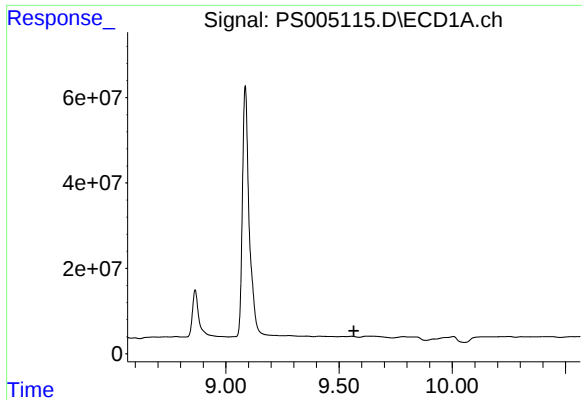

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

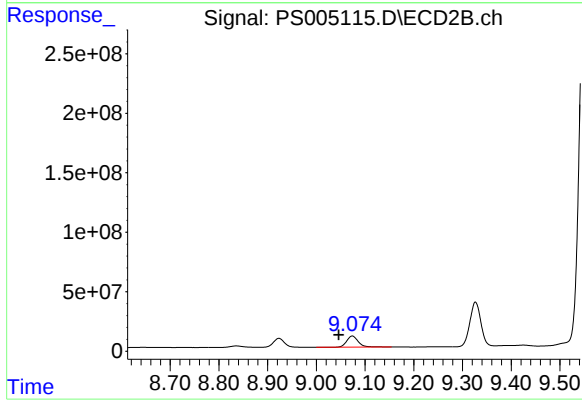

#16 DCPA

R.T.: 9.074 min
Delta R.T.: 0.028 min
Response: 151266006
Conc: 22.22 ng/ml