

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061919\
 Data File : PS005119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 11:17
 Operator : SM\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 12:46:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 19 12:45:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.585	5.300	1081.0E6	733.2E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.111	1.808	1244.7E6	898.0E6	682.500	682.500
2) T	3,5-DICHL...	4.935	4.593	1374.3E6	903.9E6	697.500	697.500
3) T	4-Nitroph...	5.428	4.974	486.1E6	334.8E6	682.500	682.500
5) T	DICAMBA	5.746	5.434	3966.7E6	2586.3E6	705.000	705.000
6) T	MCPD	5.906	5.524	308.7E6	195.4E6	70.500	70.500
7) T	MCPA	6.044	5.709	431.8E6	276.9E6	69.750	69.750
8) T	DICHLORPROP	6.385	5.989	992.1E6	664.1E6	705.000	705.000
9) T	2,4-D	6.599	6.261	1075.0E6	767.2E6	705.000	705.000
10) T	Pentachlo...	6.872	6.639	13746.4E6	8937.7E6	712.500	712.500
11) T	2,4,5-TP ...	7.408	7.001	5698.2E6	3702.9E6	712.500	712.500
12) T	2,4,5-T	7.680	7.362	5631.9E6	3582.9E6	712.500	712.500
13) T	2,4-DB	8.211	7.851	813.8E6	460.2E6	712.500	712.500
14) T	DINOSEB	9.314	8.166	4460.5E6	2791.9E6	705.000	705.000
15) T	Picloram	9.139	9.106	8147.0E6	5331.5E6	712.500	712.500
16) T	DCPA	9.586	9.067	7080.2E6	4812.8E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061919\
Data File : PS005119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 11:17
Operator : SM\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 12:46:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Wed Jun 19 12:45:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

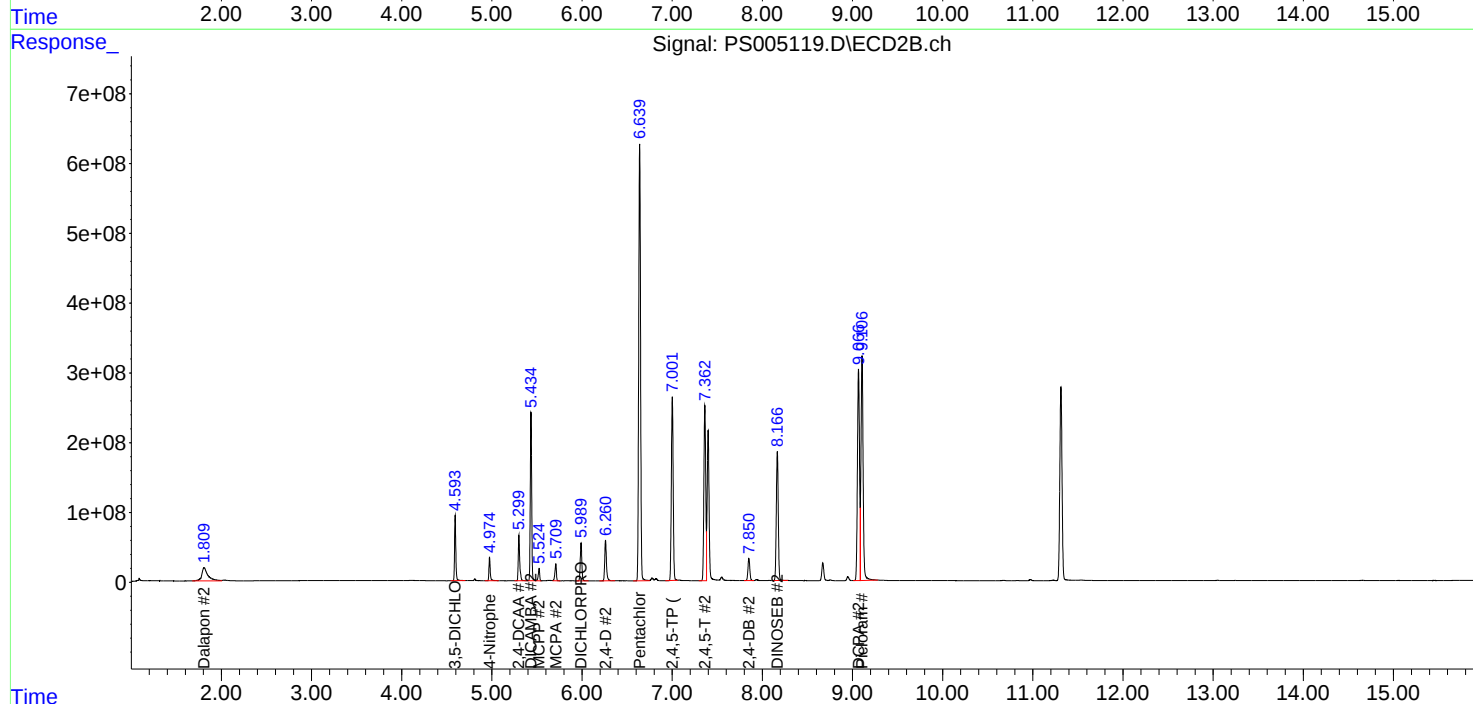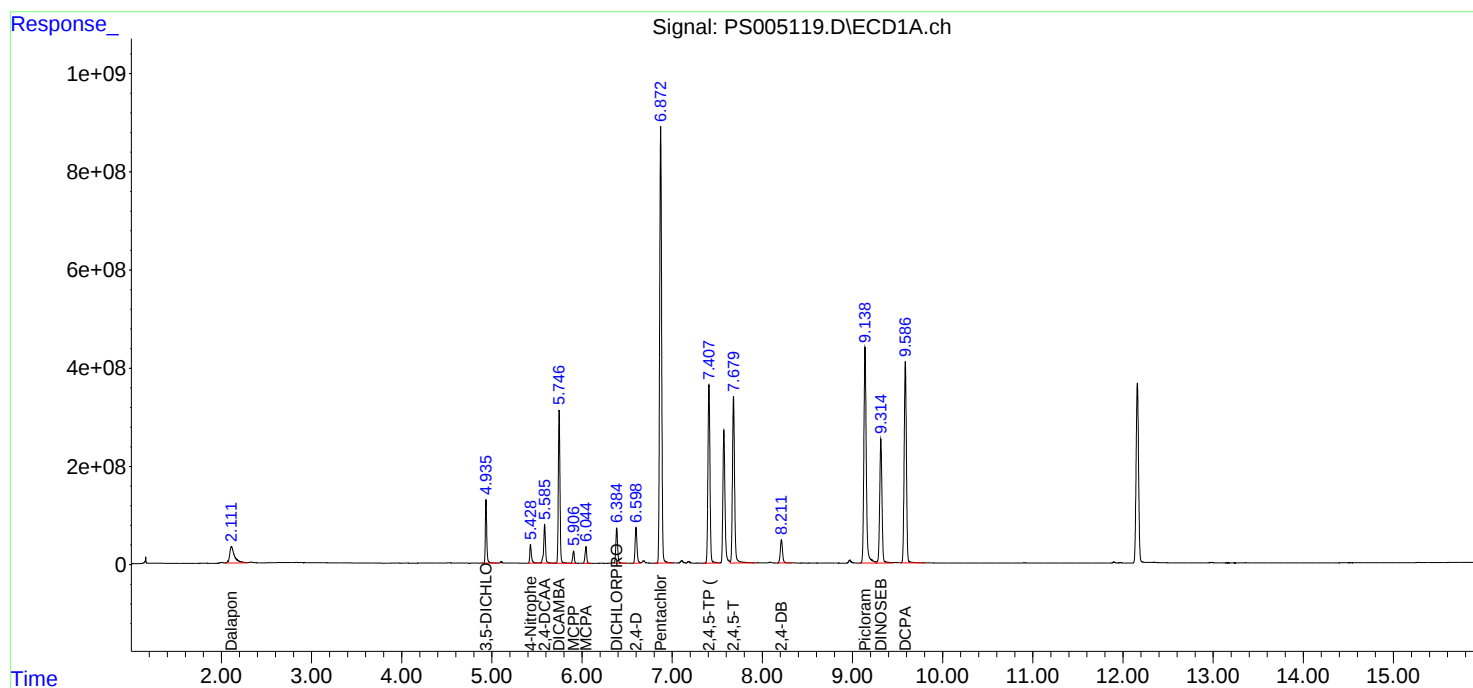


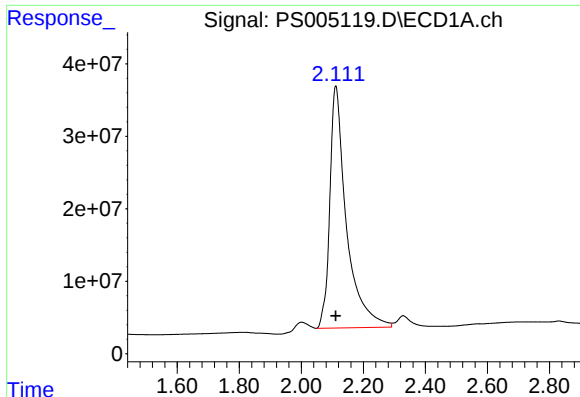

#1 Dalapon


R.T.: 2.111 min
Delta R.T.: 0.000 min
Response: 1244688086
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

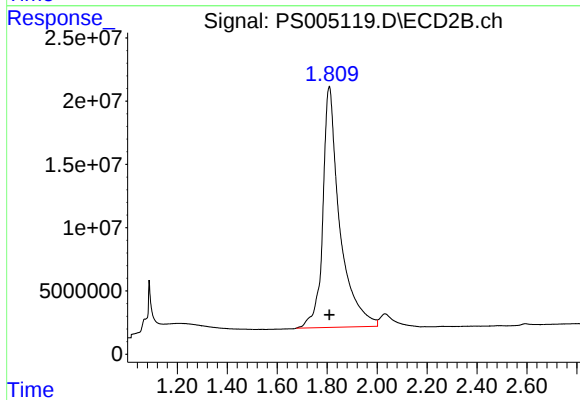


#1 Dalapon

R.T.: 1.808 min
Delta R.T.: 0.000 min
Response: 898017436
Conc: 682.50 ng/ml

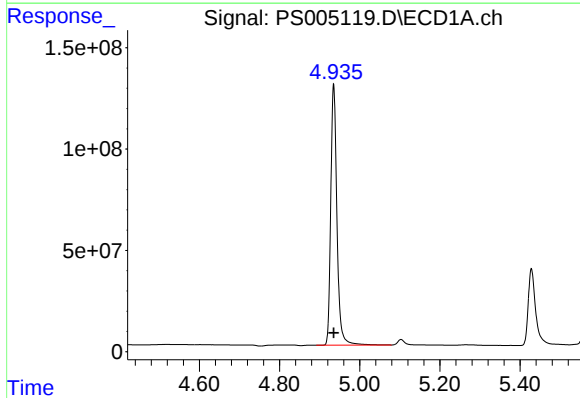


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 1374326248
Conc: 697.50 ng/ml

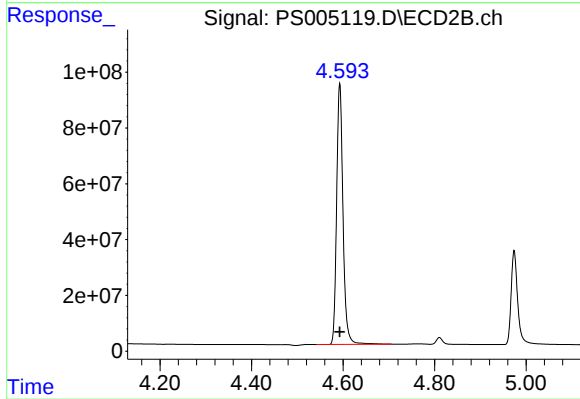

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.593 min
Delta R.T.: 0.000 min
Response: 903902373
Conc: 697.50 ng/ml

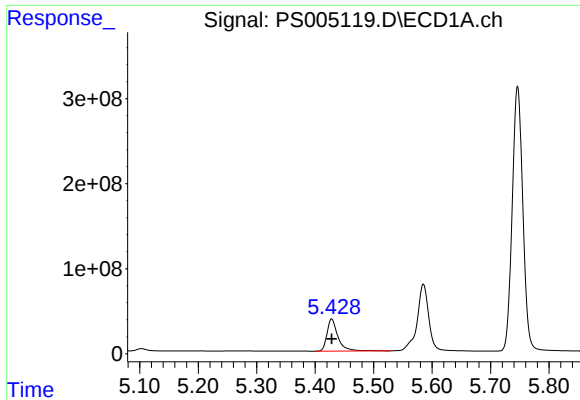

#3 4-Nitrophenol


R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 486133013
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

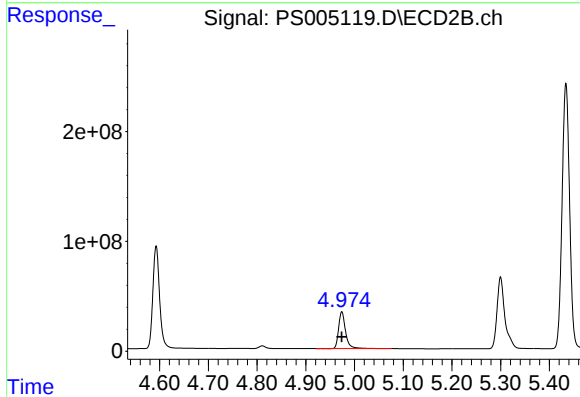


#3 4-Nitrophenol

R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 334841195
Conc: 682.50 ng/ml

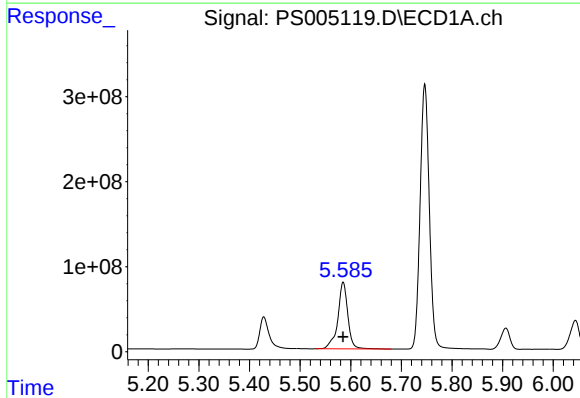


#4 2,4-DCAA

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 1080988595
Conc: 750.00 ng/ml

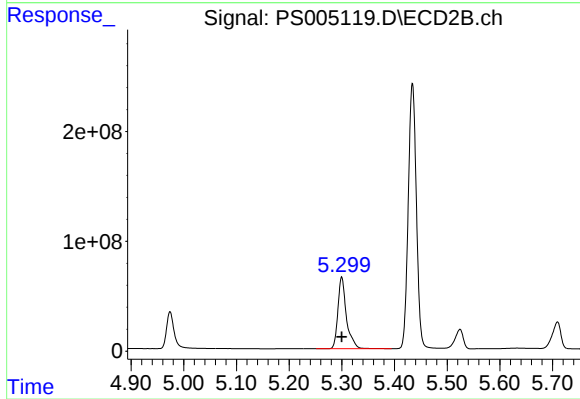

#4 2,4-DCAA


R.T.: 5.300 min
Delta R.T.: 0.000 min
Response: 733157649
Conc: 750.00 ng/ml

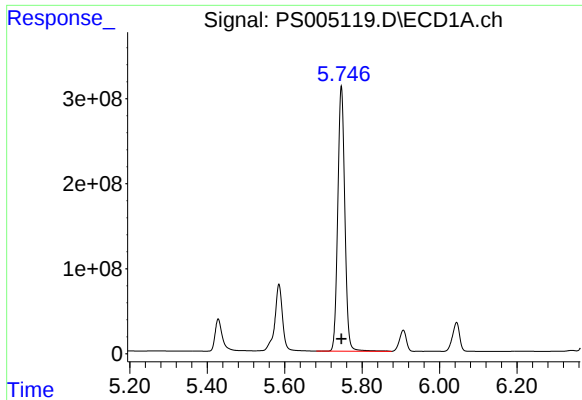

#5 DICAMBA


R.T.: 5.746 min
Delta R.T.: 0.000 min
Response: 3966694675
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

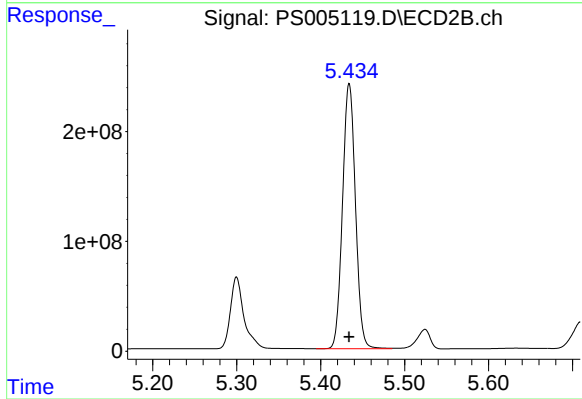


#5 DICAMBA

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 2586326381
Conc: 705.00 ng/ml

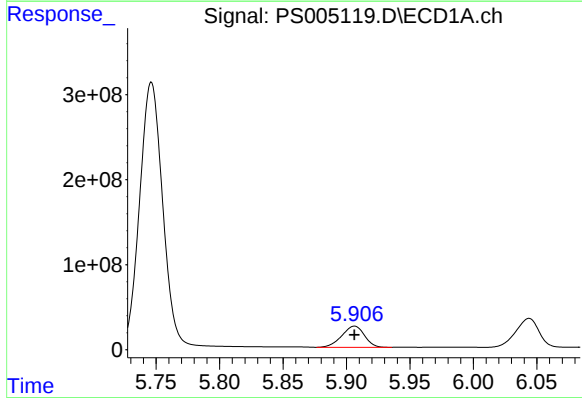


#6 MCP

R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 308683874
Conc: 70.50 ug/ml

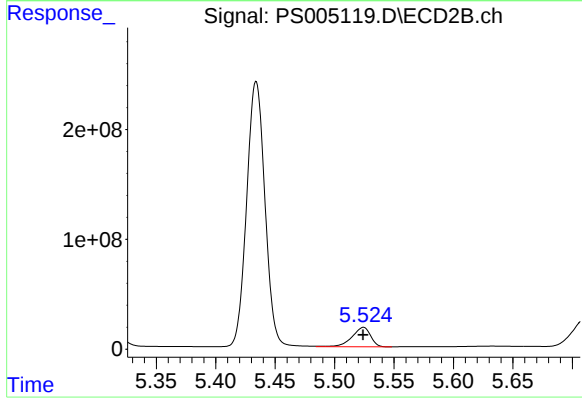

#6 MCP


R.T.: 5.524 min
Delta R.T.: 0.000 min
Response: 195393016
Conc: 70.50 ug/ml

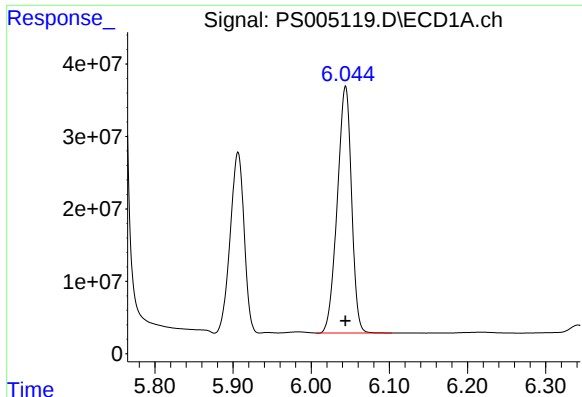

#7 MCPA


R.T.: 6.044 min
Delta R.T.: 0.000 min
Response: 431814176
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :

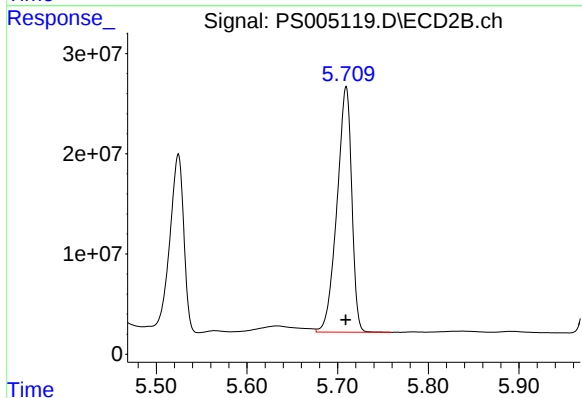


#7 MCPA

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 276893677
Conc: 69.75 ug/ml

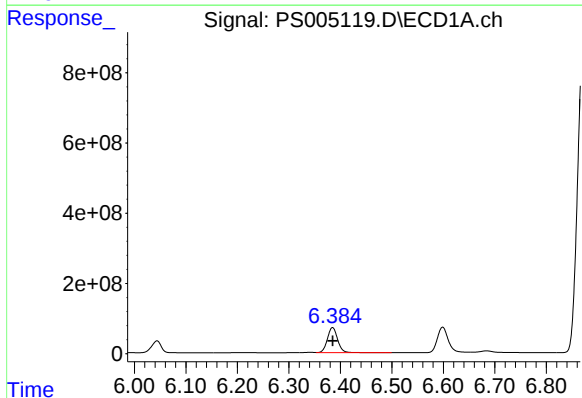


#8 DICHLORPROP

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 992130937
Conc: 705.00 ng/ml

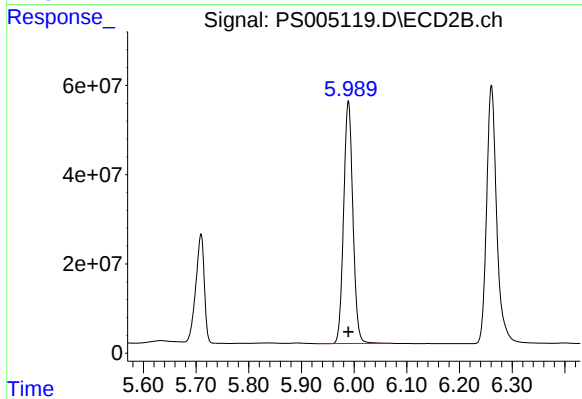

#8 DICHLORPROP


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 664082179
Conc: 705.00 ng/ml

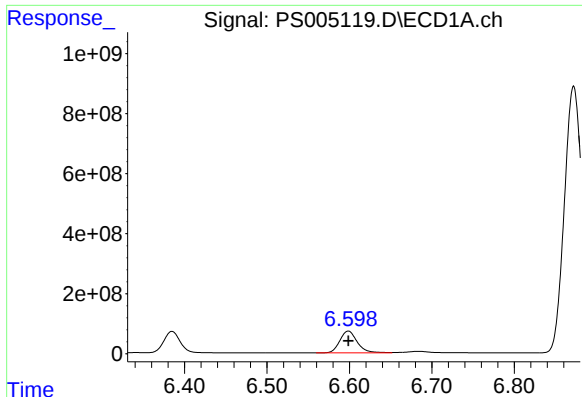

#9 2,4-D


R.T.: 6.599 min
Delta R.T.: 0.000 min
Response: 1074966151
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

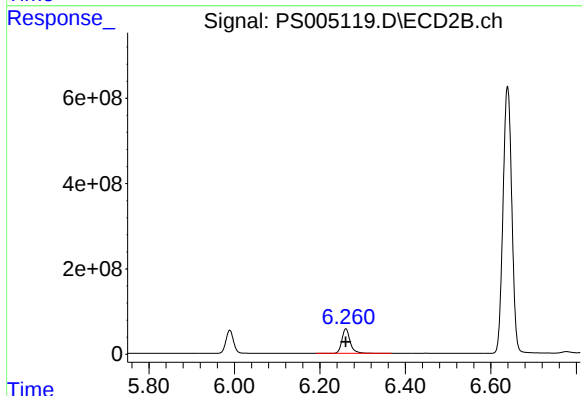


#9 2,4-D

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 767233411
Conc: 705.00 ng/ml

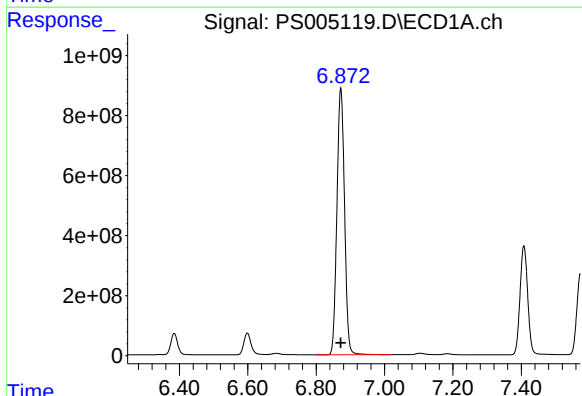


#10 Pentachlorophenol

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 13746432884
Conc: 712.50 ng/ml

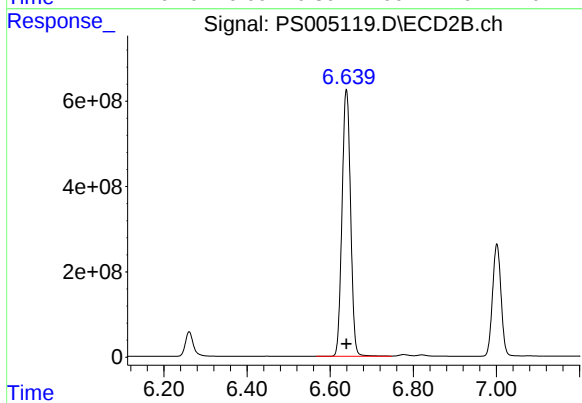

#10 Pentachlorophenol


R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 8937708864
Conc: 712.50 ng/ml

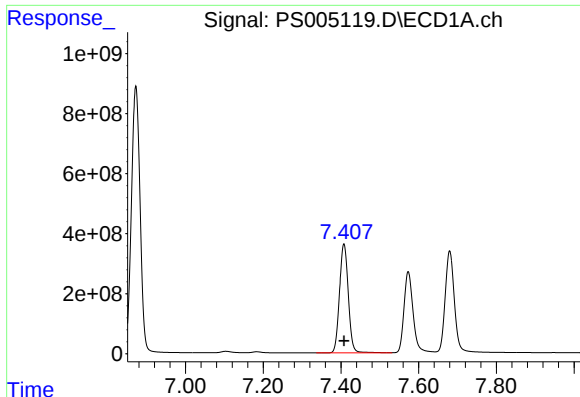

#11 2,4,5-TP (SILVEX)


R.T.: 7.408 min
Delta R.T.: 0.000 min
Response: 5698168655
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

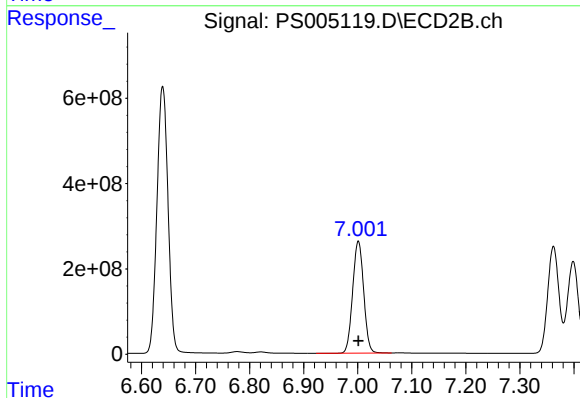


#11 2,4,5-TP (SILVEX)

R.T.: 7.001 min
Delta R.T.: 0.000 min
Response: 3702932878
Conc: 712.50 ng/ml

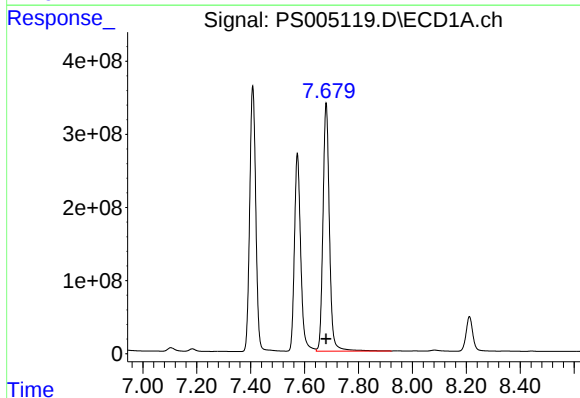


#12 2,4,5-T

R.T.: 7.680 min
Delta R.T.: 0.000 min
Response: 5631876566
Conc: 712.50 ng/ml

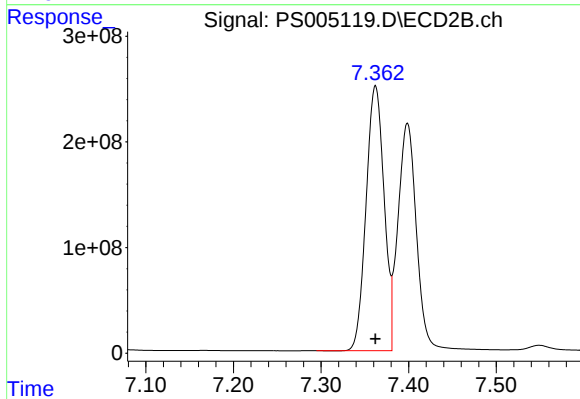

#12 2,4,5-T


R.T.: 7.362 min
Delta R.T.: 0.000 min
Response: 3582920504
Conc: 712.50 ng/ml

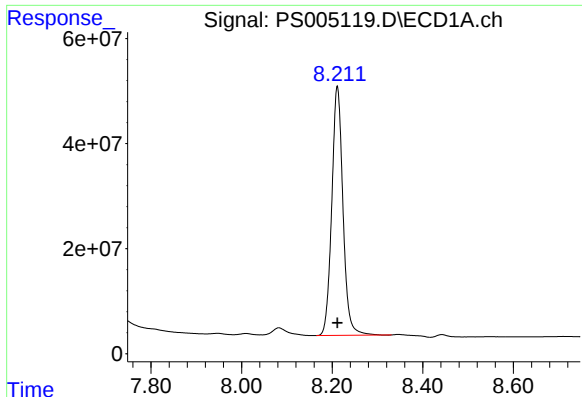

#13 2,4-DB


R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 813834043
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

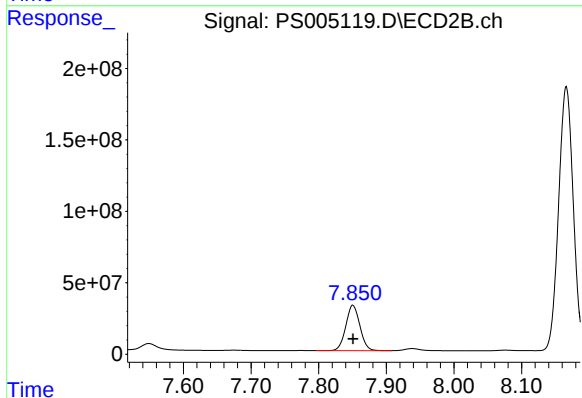


#13 2,4-DB

R.T.: 7.851 min
Delta R.T.: 0.000 min
Response: 460189753
Conc: 712.50 ng/ml

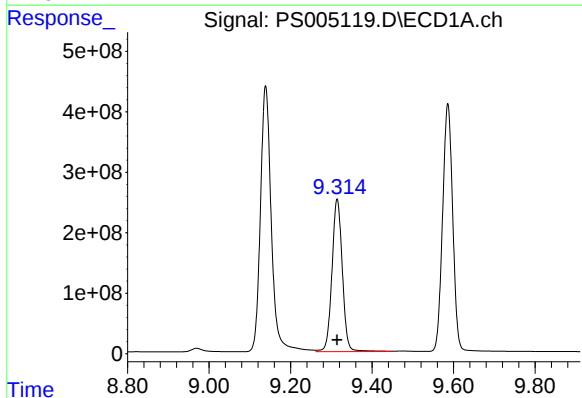


#14 DINOSEB

R.T.: 9.314 min
Delta R.T.: 0.000 min
Response: 4460509423
Conc: 705.00 ng/ml

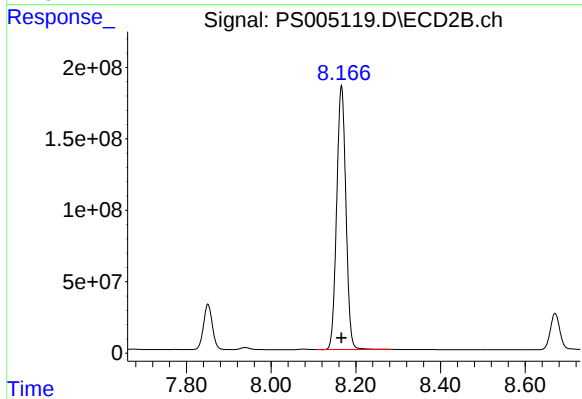

#14 DINOSEB


R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 2791899426
Conc: 705.00 ng/ml

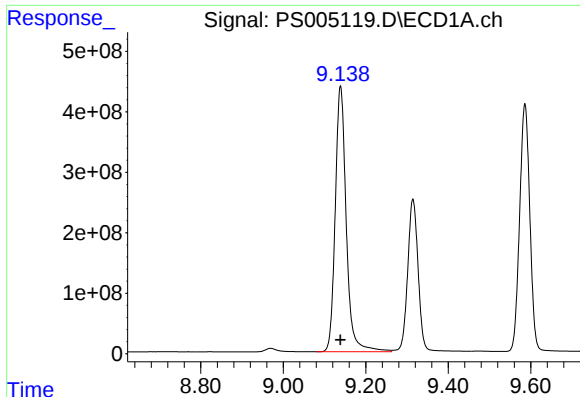

#15 Picloram


R.T.: 9.139 min
Delta R.T.: 0.000 min
Response: 8147014817
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

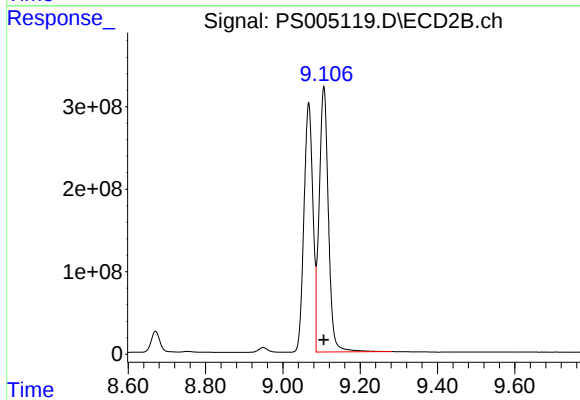


#15 Picloram

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 5331472886
Conc: 712.50 ng/ml

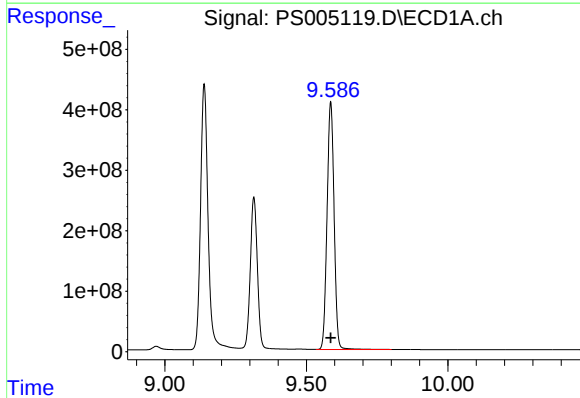

#16 DCPA

R.T.: 9.586 min
Delta R.T.: 0.000 min
Response: 7080245668
Conc: 720.00 ng/ml

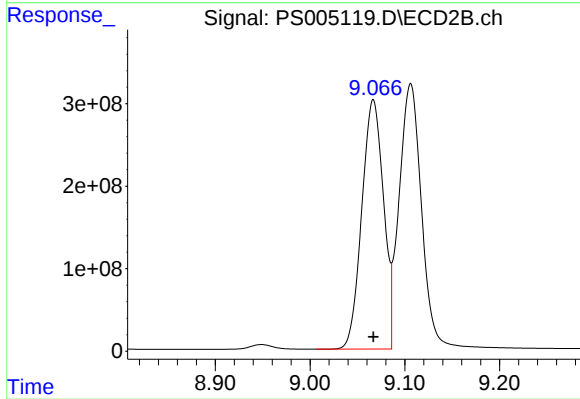

#16 DCPA

R.T.: 9.067 min
Delta R.T.: 0.000 min
Response: 4812755353
Conc: 720.00 ng/ml