

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061919\
 Data File : PS005123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 12:59
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 11:16:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.587	5.280	538.3E6	360.7E6	366.747	359.877
Target Compounds							
10) T	Pentachlo...	6.875	6.620	22400883	16647677	1.138	1.295
12) T	2,4,5-T	7.690	7.347	25500241	12422720	3.169	2.435
15) T	Picloram	9.151	9.091	485.5E6	360.5E6	42.252	47.770
16) T	DCPA	9.590	9.091	17974061	360.5E6	1.802	52.956 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061919\
Data File : PS005123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 12:59
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 11:16:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

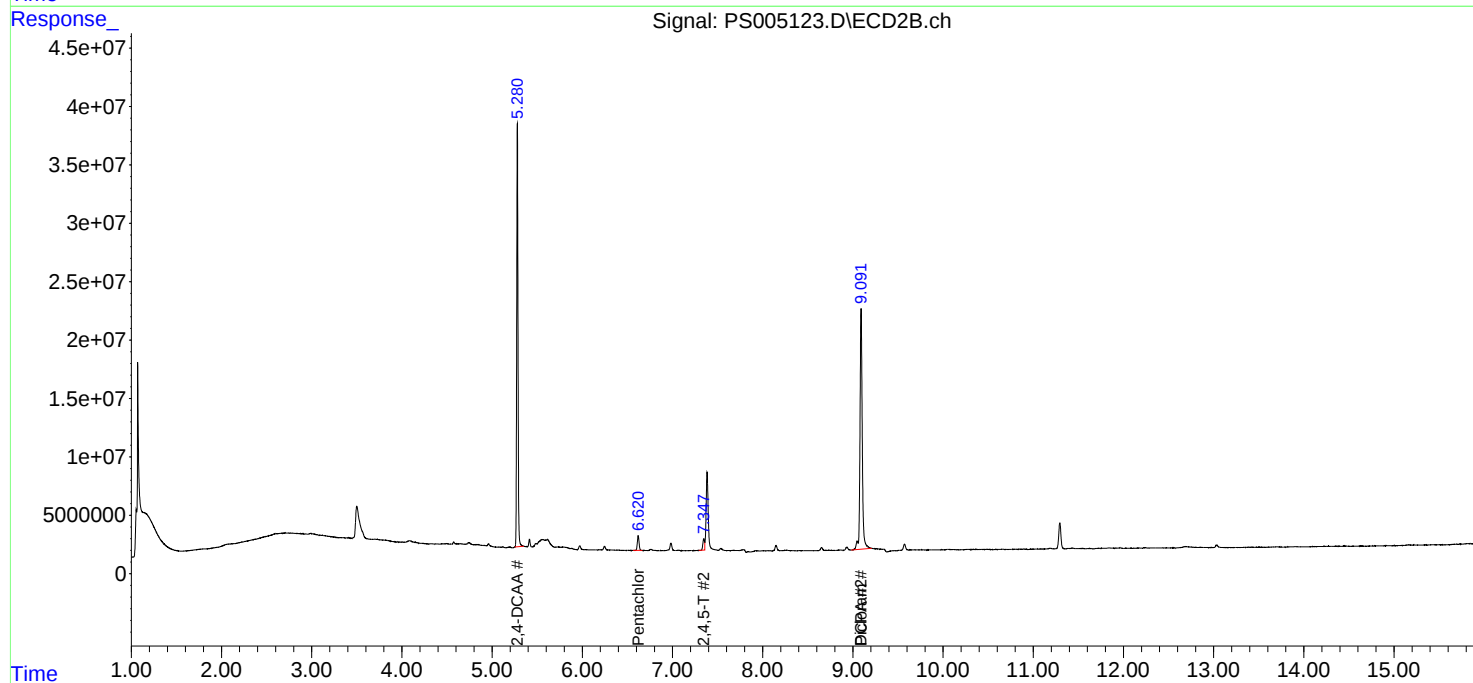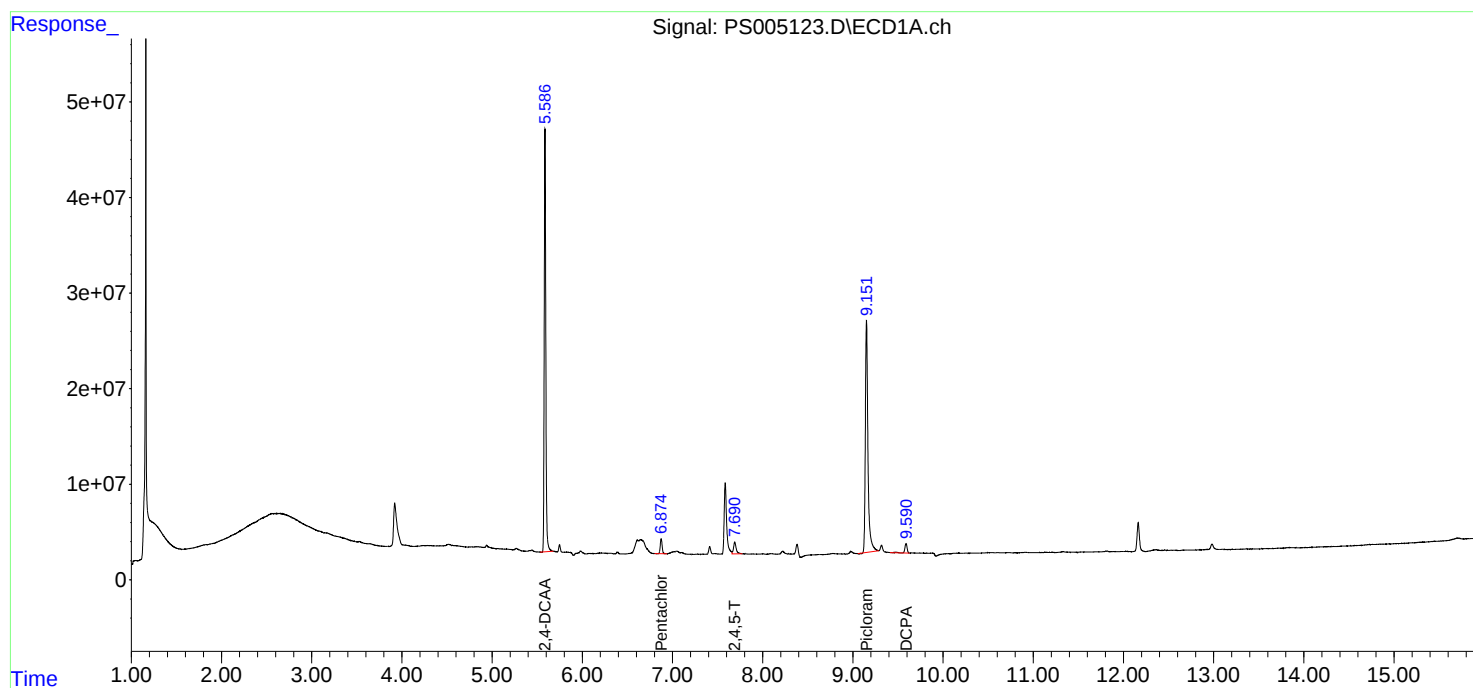


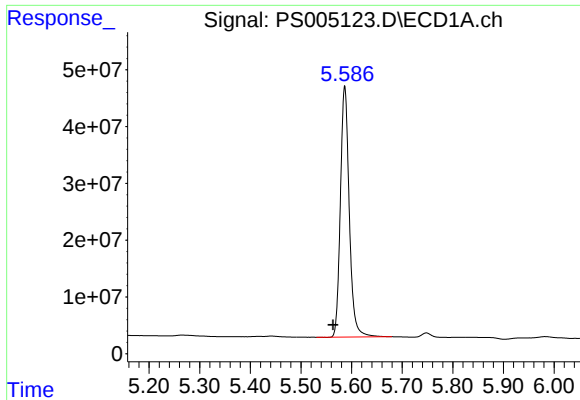

#4 2,4-DCAA


R.T.: 5.587 min
Delta R.T.: 0.023 min
Response: 538345027
Conc: 366.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

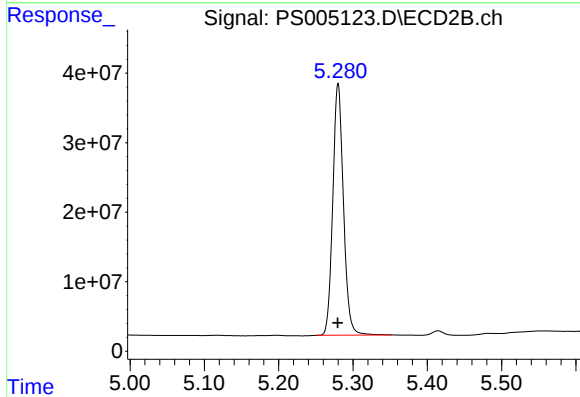


#4 2,4-DCAA

R.T.: 5.280 min
Delta R.T.: 0.000 min
Response: 360729038
Conc: 359.88 ng/ml

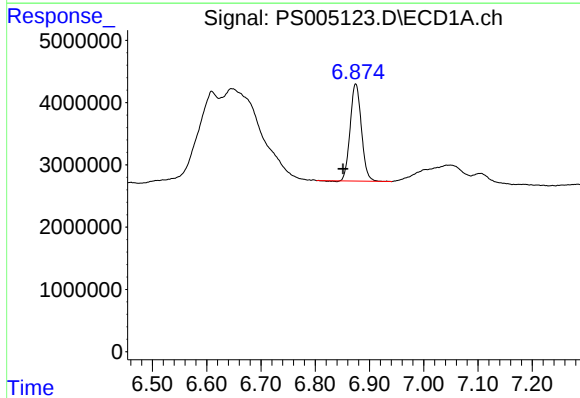


#10 Pentachlorophenol

R.T.: 6.875 min
Delta R.T.: 0.023 min
Response: 22400883
Conc: 1.14 ng/ml

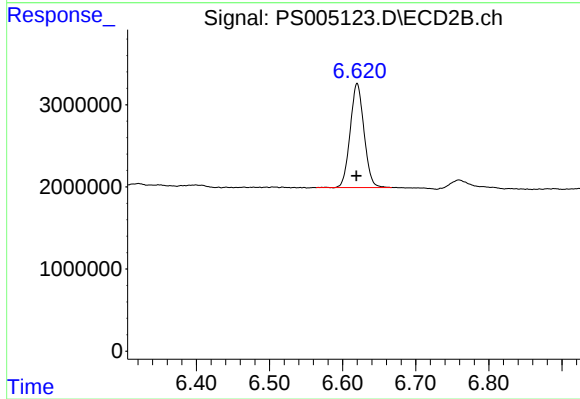

#10 Pentachlorophenol


R.T.: 6.620 min
Delta R.T.: 0.000 min
Response: 16647677
Conc: 1.29 ng/ml

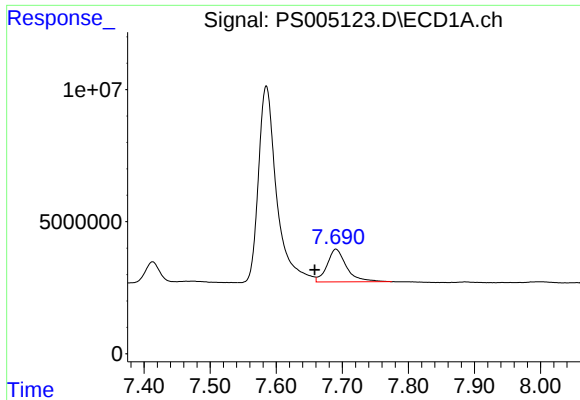

#12 2,4,5-T


R.T.: 7.690 min
Delta R.T.: 0.032 min
Response: 25500241
Conc: 3.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

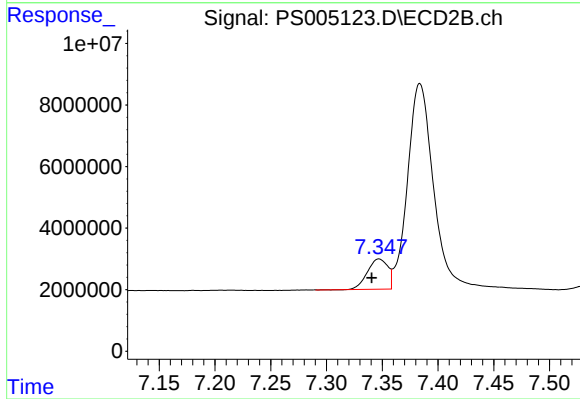


#12 2,4,5-T

R.T.: 7.347 min
Delta R.T.: 0.007 min
Response: 12422720
Conc: 2.44 ng/ml

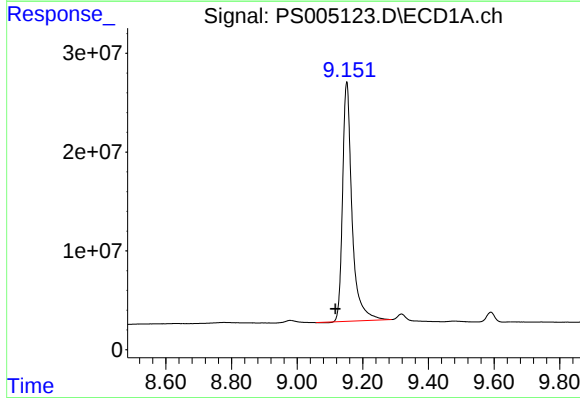


#15 Picloram

R.T.: 9.151 min
Delta R.T.: 0.034 min
Response: 485528831
Conc: 42.25 ng/ml

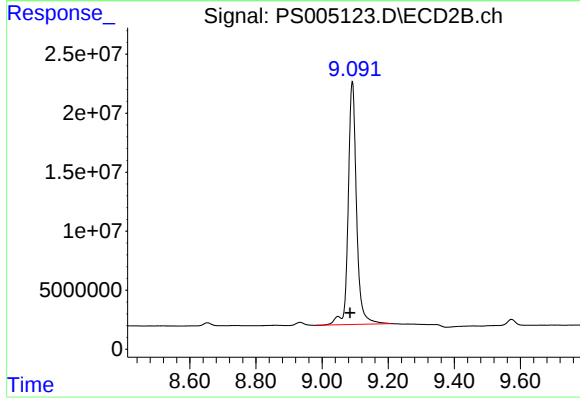

#15 Picloram


R.T.: 9.091 min
Delta R.T.: 0.006 min
Response: 360496417
Conc: 47.77 ng/ml

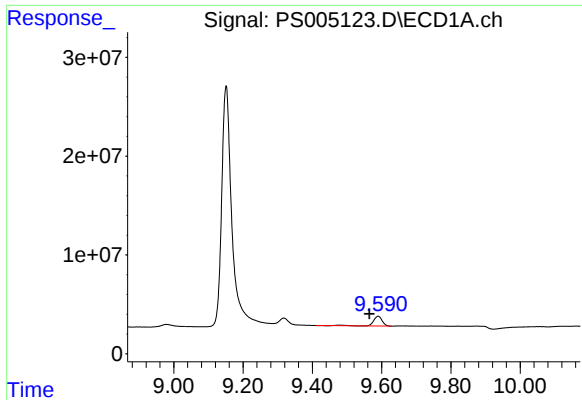

#16 DCPA

R.T.: 9.590 min
Delta R.T.: 0.025 min
Response: 17974061
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

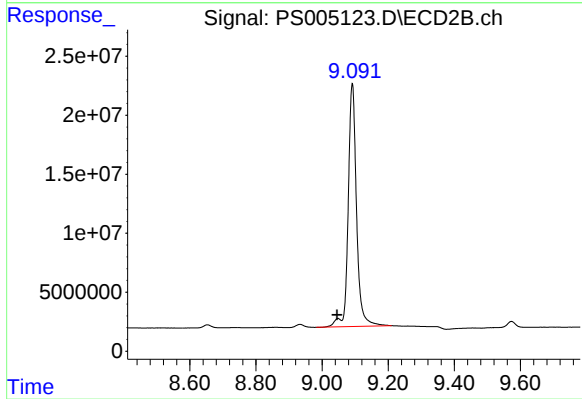

#16 DCPA

R.T.: 9.091 min
Delta R.T.: 0.046 min
Response: 360496417
Conc: 52.96 ng/ml