

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061920\
 Data File : PS010859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 10:03
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 19:00:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds								
2) T	3,5-DICHL...	6.483	0.000	10986991	0	10.050	N.D.	#
5) T	DICAMBA	0.000	7.154	0	13787770	N.D.	6.126	
6) T	MCP	0.000	7.154	0	13787770	N.D.	7.399	
15) T	Picloram	11.041	11.015	20561890	19726249	4.028	4.781	
16) T	DCPA	0.000	11.015	0	19726249	N.D.	5.320	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061920\
Data File : PS010859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 10:03
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 19:00:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

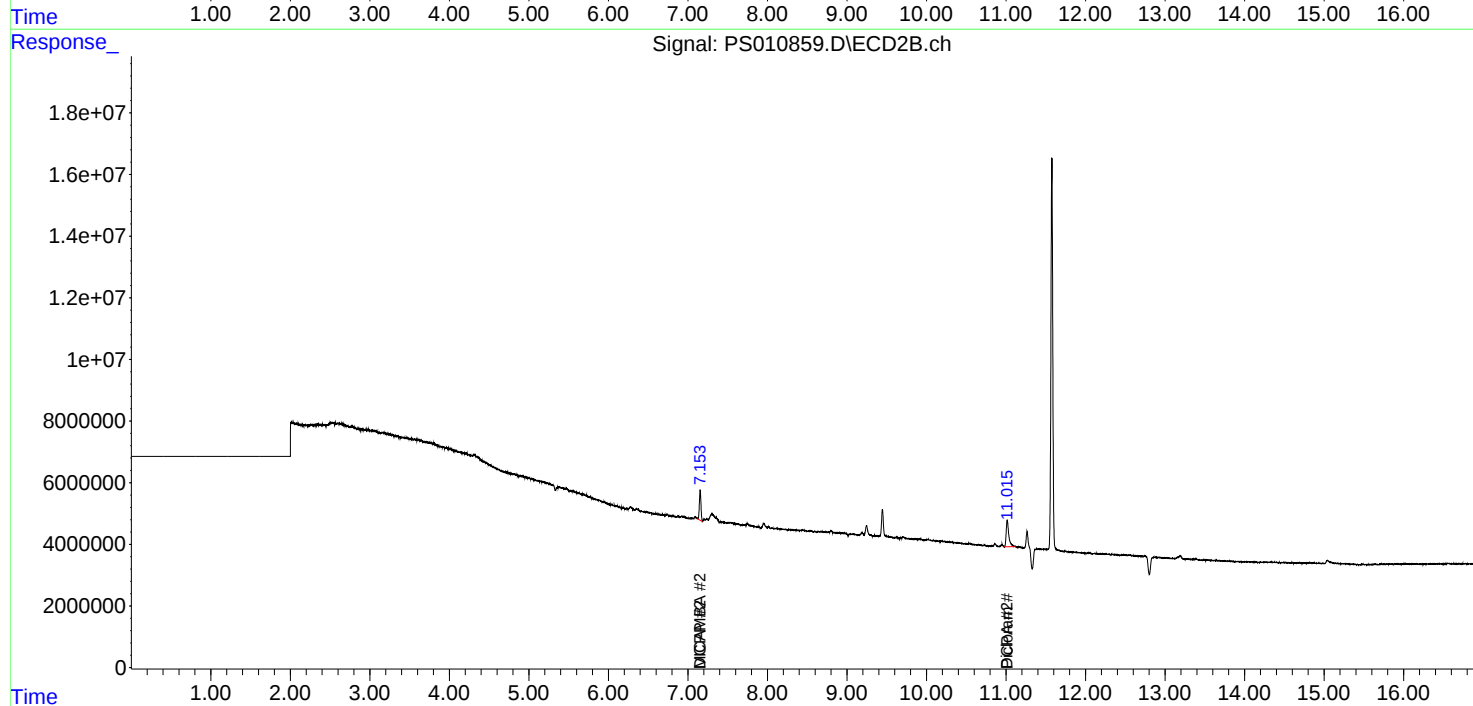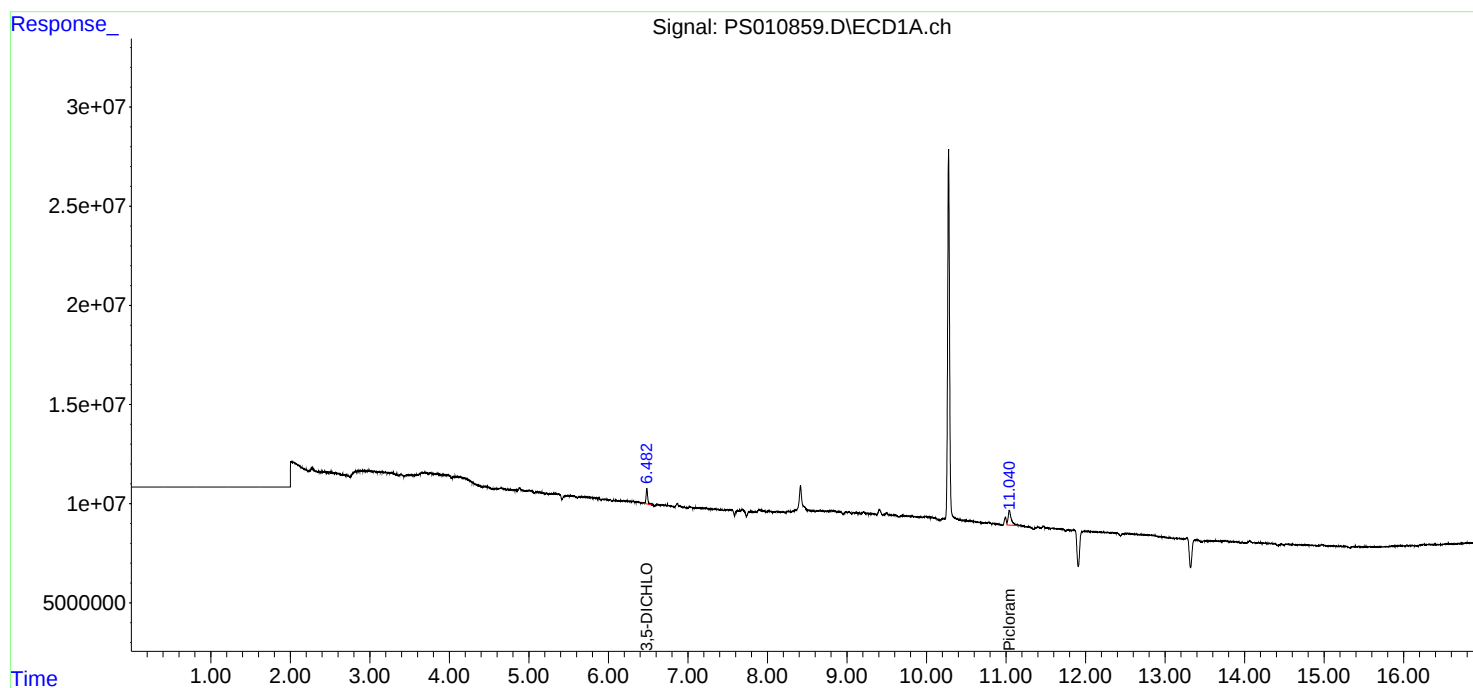


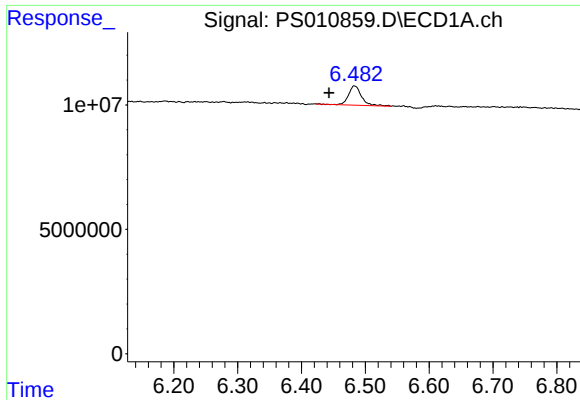

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.483 min
Delta R.T.: 0.040 min
Response: 10986991
Conc: 10.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

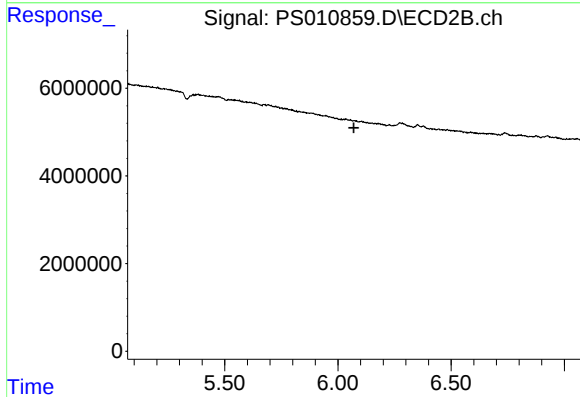


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.070 min
Response: 0
Conc: N.D.

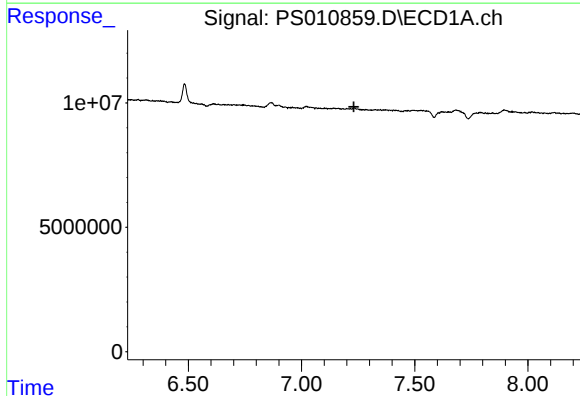


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.231 min
Response: 0
Conc: N.D.

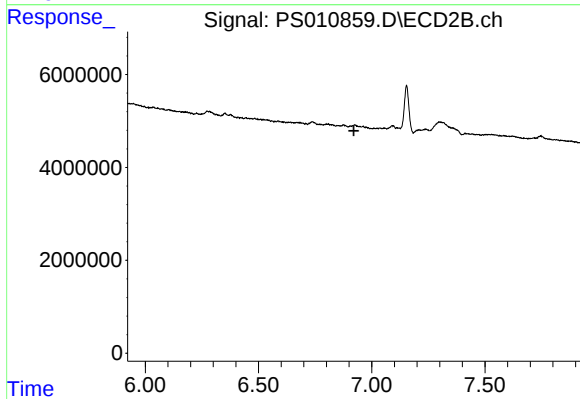

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

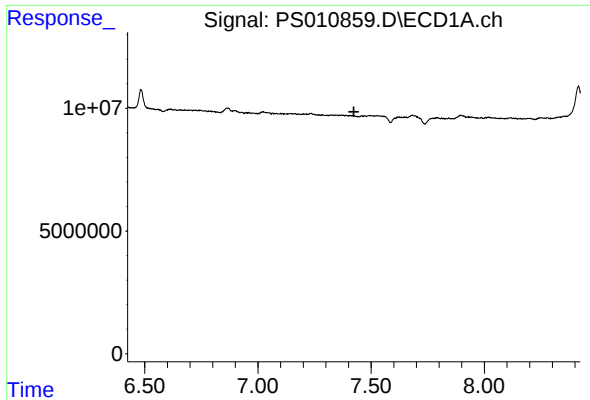

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

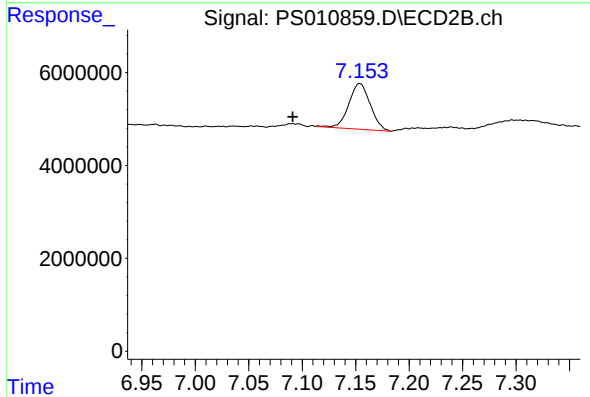


#5 DICAMBA

R.T.: 7.154 min
Delta R.T.: 0.063 min
Response: 13787770
Conc: 6.13 ng/ml

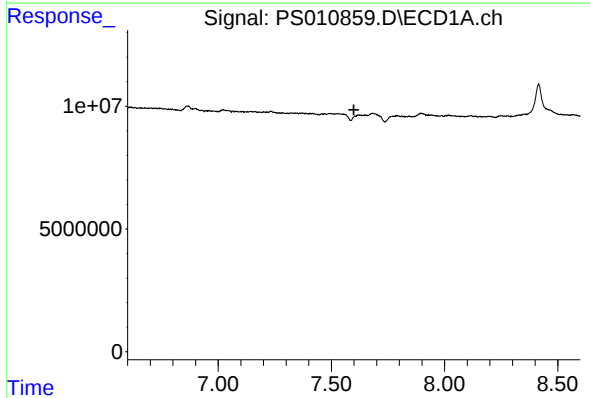


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.600 min
Response: 0
Conc: N.D.

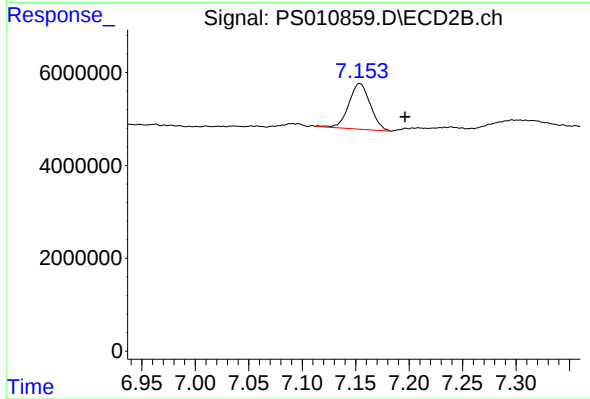

#6 MCP


R.T.: 7.154 min
Delta R.T.: -0.042 min
Response: 13787770
Conc: 7.40 ug/ml

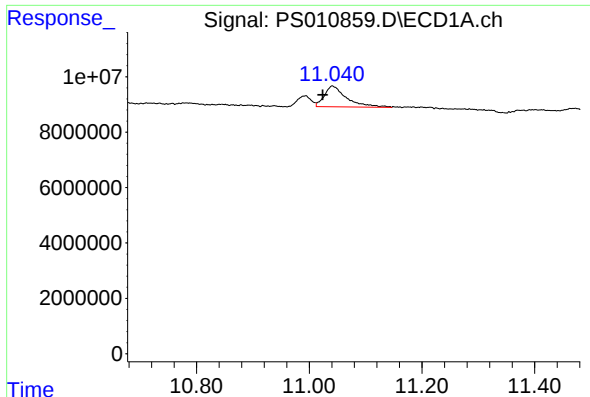

#15 Picloram


R.T.: 11.041 min
Delta R.T.: 0.017 min
Response: 20561890
Conc: 4.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

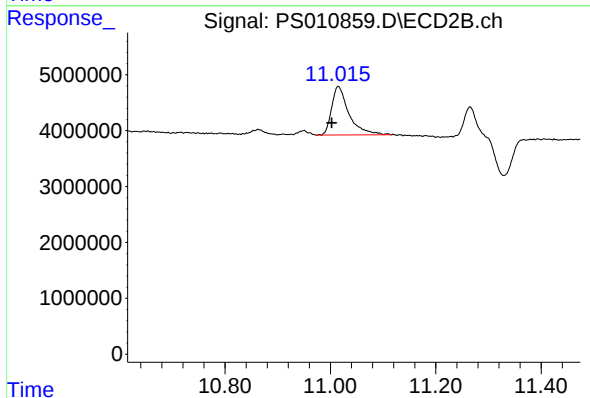


#15 Picloram

R.T.: 11.015 min
Delta R.T.: 0.013 min
Response: 19726249
Conc: 4.78 ng/ml

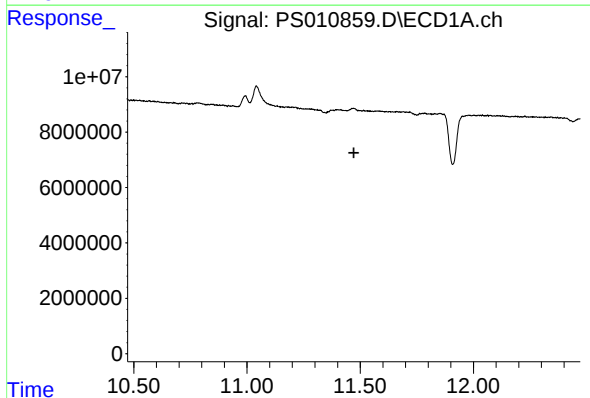

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.472 min
Response: 0
Conc: N.D.

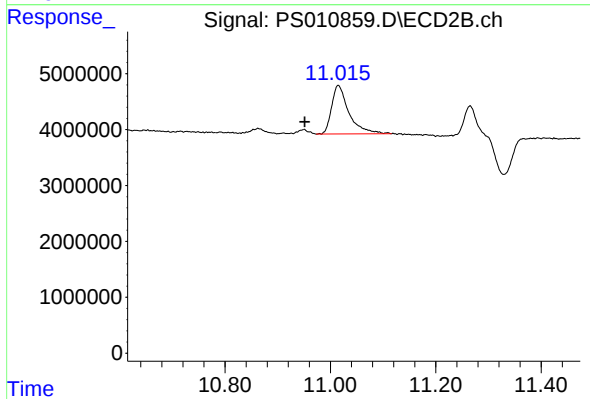

#16 DCPA

R.T.: 11.015 min
Delta R.T.: 0.064 min
Response: 19726249
Conc: 5.32 ng/ml