

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
 Data File : PS015847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2021 21:20
 Operator : DD\AJ
 Sample : M2687-08
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DUP-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 00:54:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.766	663.1E6	214.3E6	399.126	425.267
Target Compounds							
1) T	Dalapon	2.974f	2.481	17445080	26941968	8.643	41.482 #
2) T	3,5-DICHL...	0.000	5.982	0	61865767	N.D.	82.032
5) T	DICAMBA	7.368	0.000	16739998	0	2.604	N.D. #
6) T	MCP	7.545	0.000	16294974	0	3.000	N.D. #
7) T	MCPA	7.679	7.225	17375652	17359865	2.220	6.767 #
8) T	DICHLORPROP	8.043	7.569	46551045	14106917	29.400	27.247
9) T	2,4-D	8.363f	7.872	9023086	21239036	5.149	34.241 #
10) T	Pentachlo...	8.676f	8.333f	21631586	6852845	1.002	<MDL #
11) T	2,4,5-TP ...	9.195	0.000	9448821	0	1.081	N.D. #
13) T	2,4-DB	10.038	0.000	46754546	0	22.857	N.D. #
14) T	DINOSEB	11.120f	9.861	149.6E6	28993042	23.092	14.395 #
15) T	Picloram	10.969	10.820	161.9E6	16143793	11.840	3.839 #
16) T	DCPA	11.459	10.820f	43231204	16143793	3.269	3.840



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
Data File : PS015847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2021 21:20
Operator : DD\AJ
Sample : M2687-08
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
DUP-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 00:54:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

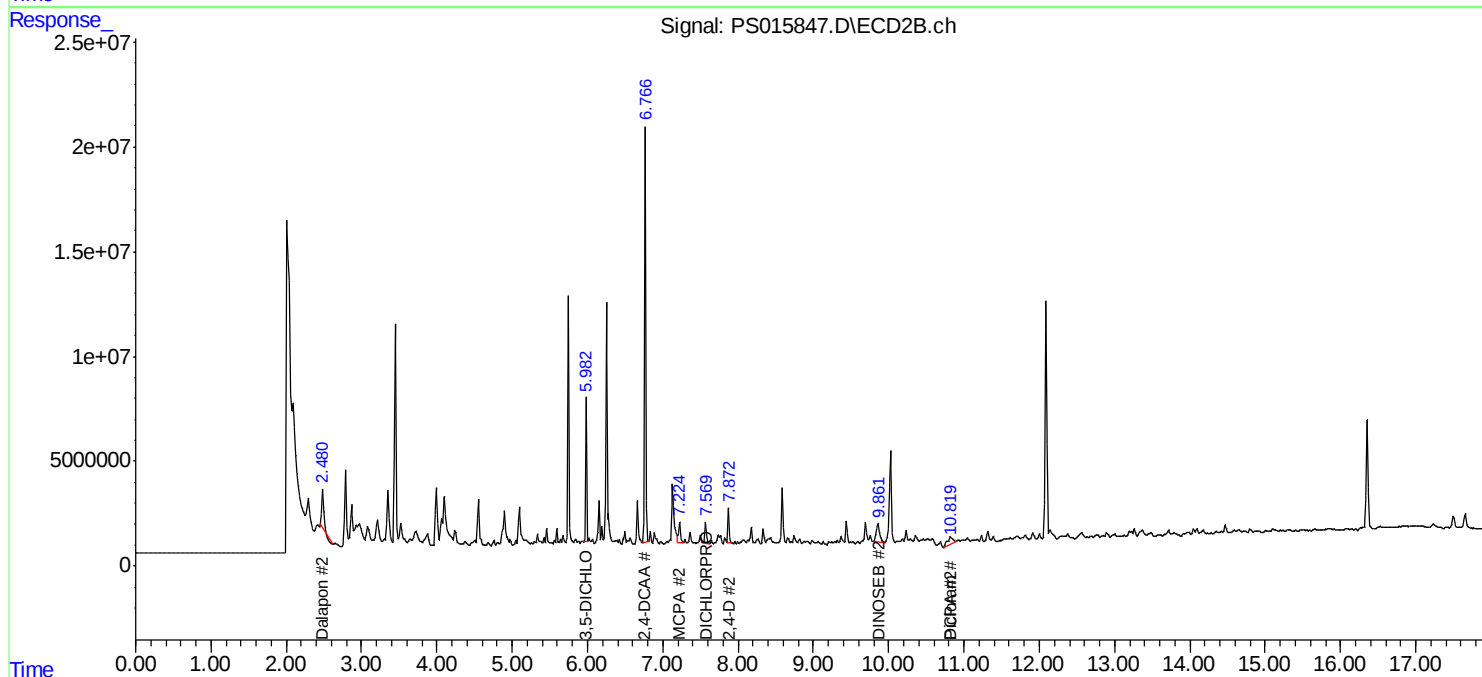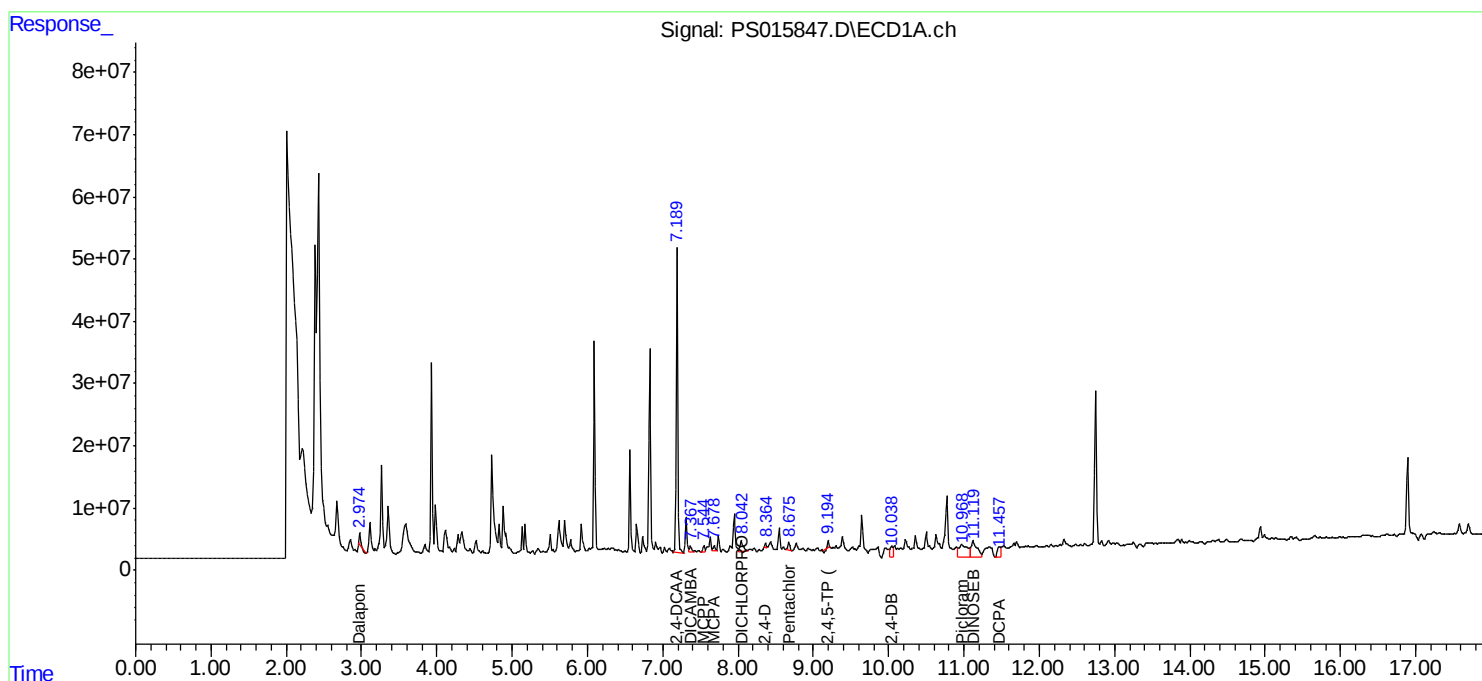


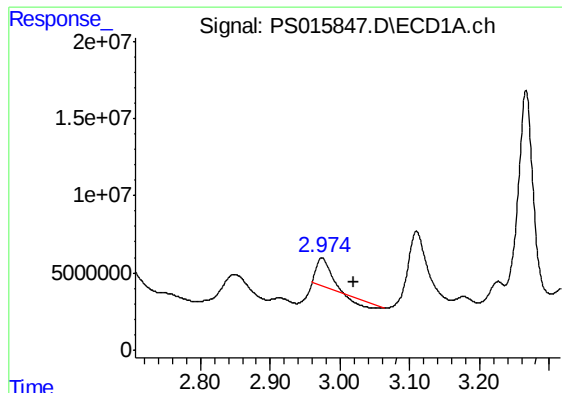

#1 Dalapon


R.T.: 2.974 min
Delta R.T.: -0.046 min
Response: 17445080
Conc: 8.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUP-01

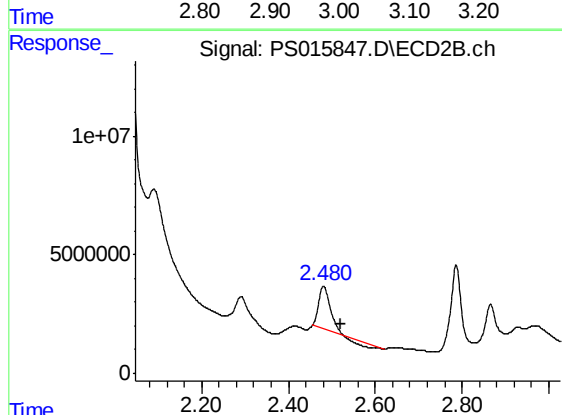


#1 Dalapon

R.T.: 2.481 min
Delta R.T.: -0.040 min
Response: 26941968
Conc: 41.48 ng/ml

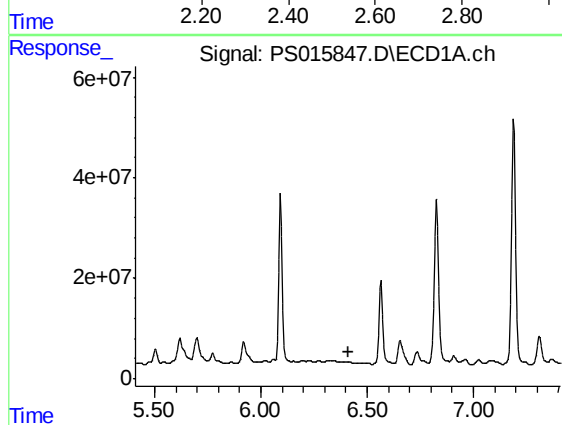


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

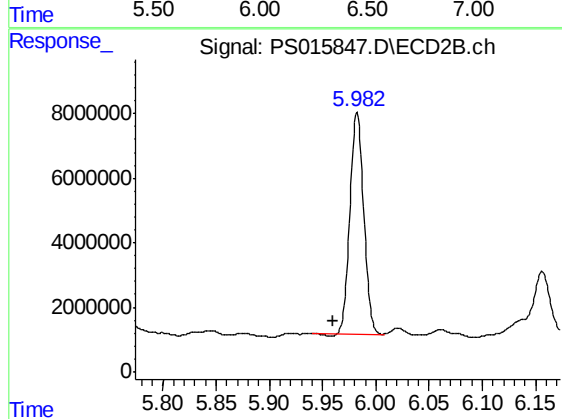

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.982 min
Delta R.T.: 0.023 min
Response: 61865767
Conc: 82.03 ng/ml

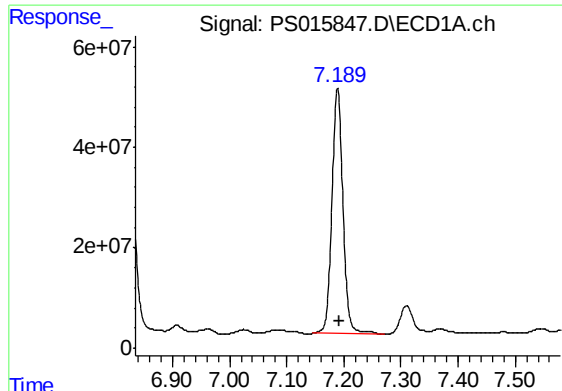

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: -0.004 min
Response: 663126341
Conc: 399.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUP-01

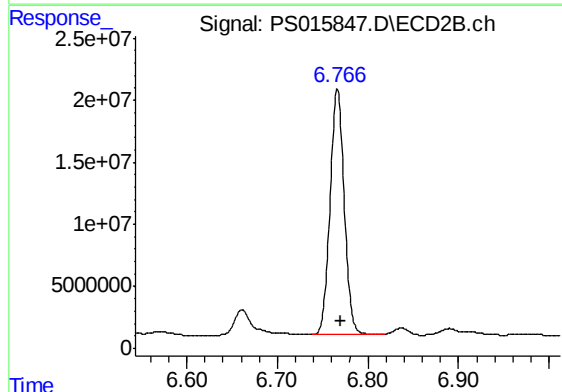


#4 2,4-DCAA

R.T.: 6.766 min
Delta R.T.: -0.004 min
Response: 214271533
Conc: 425.27 ng/ml

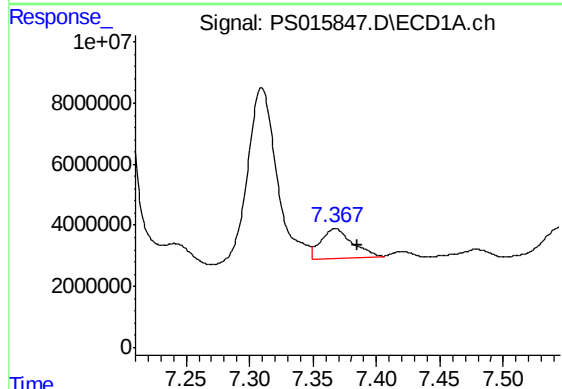


#5 DICAMBA

R.T.: 7.368 min
Delta R.T.: -0.018 min
Response: 16739998
Conc: 2.60 ng/ml

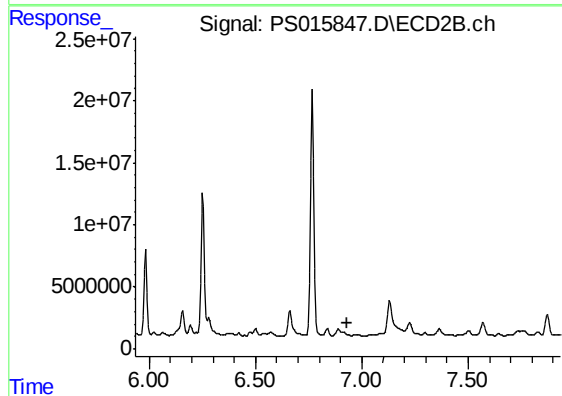

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

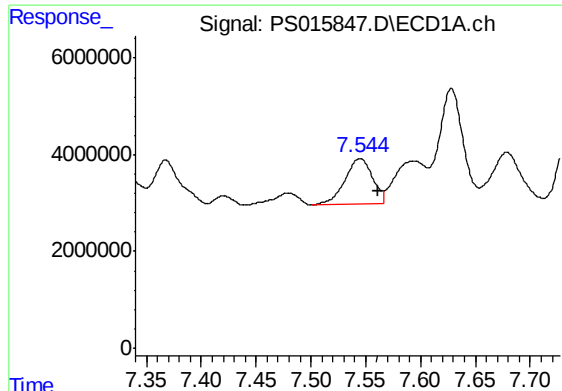

#6 MCPP


R.T.: 7.545 min
Delta R.T.: -0.016 min
Response: 16294974
Conc: 3.00 ug/ml

Instrument :
ECD_S
ClientSampleId :
DUP-01

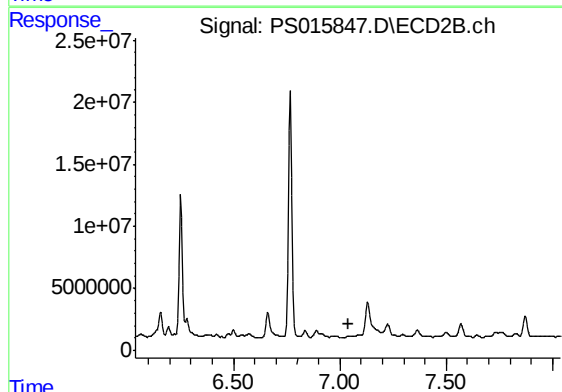


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.038 min
Response: 0
Conc: N.D.

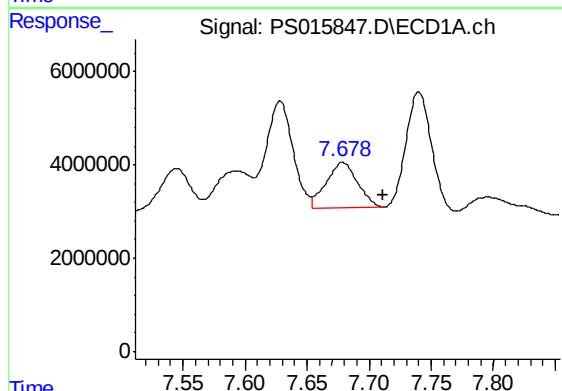


#7 MCPA

R.T.: 7.679 min
Delta R.T.: -0.033 min
Response: 17375652
Conc: 2.22 ug/ml

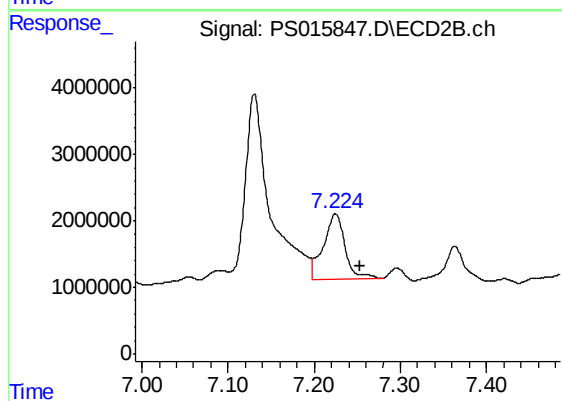

#7 MCPA


R.T.: 7.225 min
Delta R.T.: -0.028 min
Response: 17359865
Conc: 6.77 ug/ml

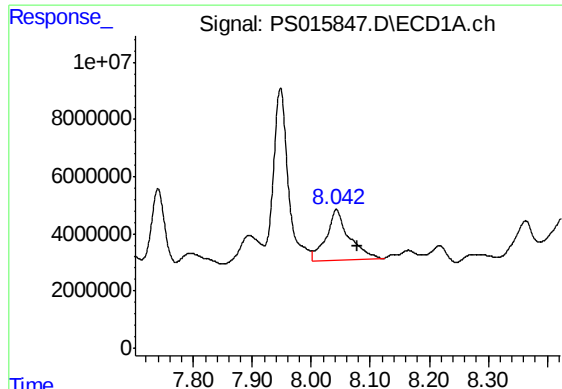

#8 DICHLORPROP


R.T.: 8.043 min
Delta R.T.: -0.036 min
Response: 46551045
Conc: 29.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUP-01

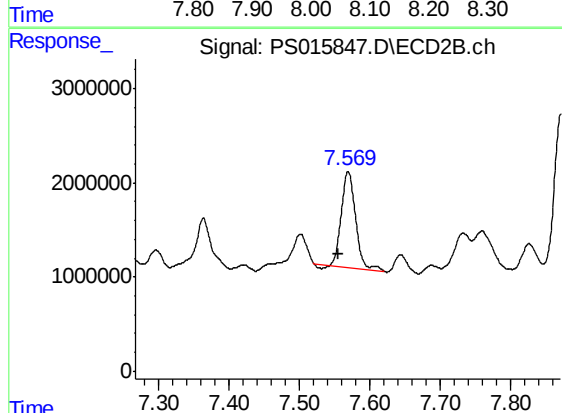


#8 DICHLORPROP

R.T.: 7.569 min
Delta R.T.: 0.014 min
Response: 14106917
Conc: 27.25 ng/ml

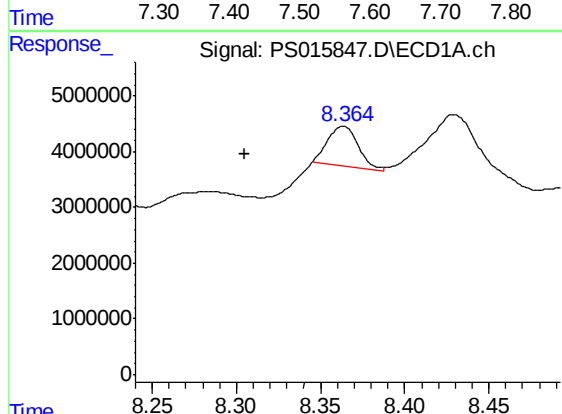


#9 2,4-D

R.T.: 8.363 min
Delta R.T.: 0.058 min
Response: 9023086
Conc: 5.15 ng/ml

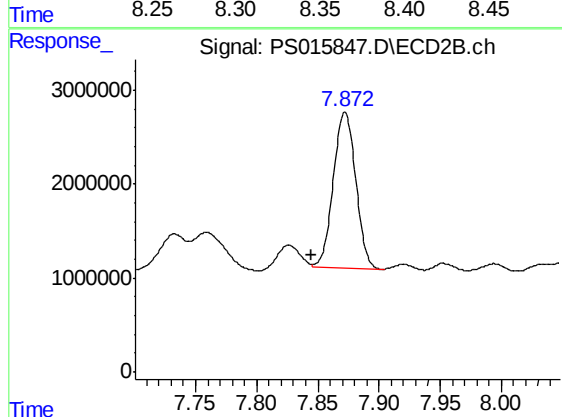

#9 2,4-D


R.T.: 7.872 min
Delta R.T.: 0.027 min
Response: 21239036
Conc: 34.24 ng/ml

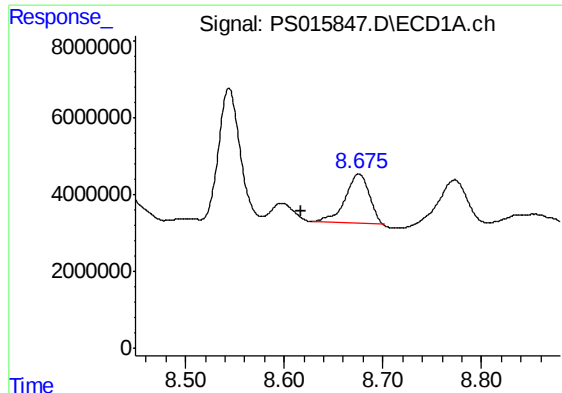

#10 Pentachlorophenol


R.T.: 8.676 min
Delta R.T.: 0.058 min
Response: 21631586
Conc: 1.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUP-01

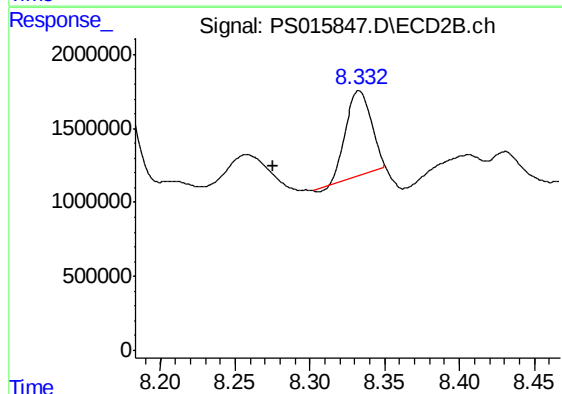


#10 Pentachlorophenol

R.T.: 8.333 min
Delta R.T.: 0.058 min
Response: 6852845
Conc: N.D.

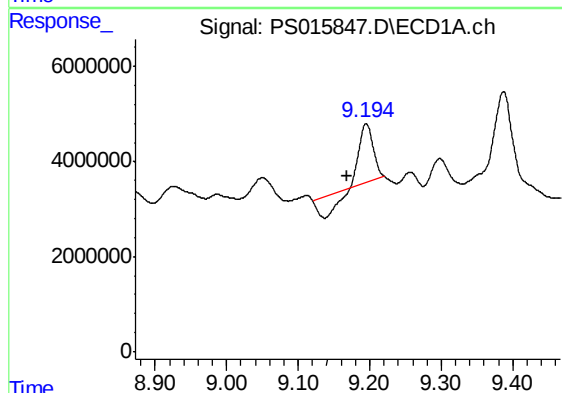


#11 2,4,5-TP (SILVEX)

R.T.: 9.195 min
Delta R.T.: 0.027 min
Response: 9448821
Conc: 1.08 ng/ml

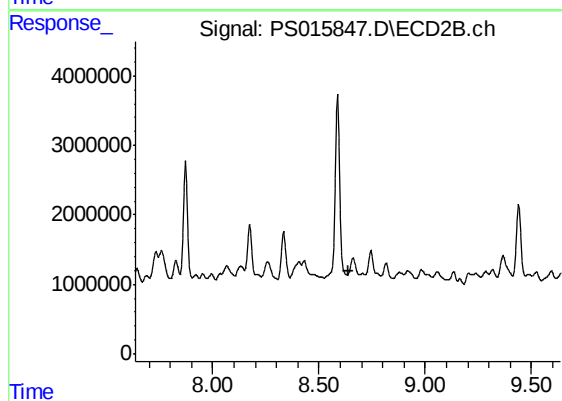

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.636 min
Response: 0
Conc: N.D.

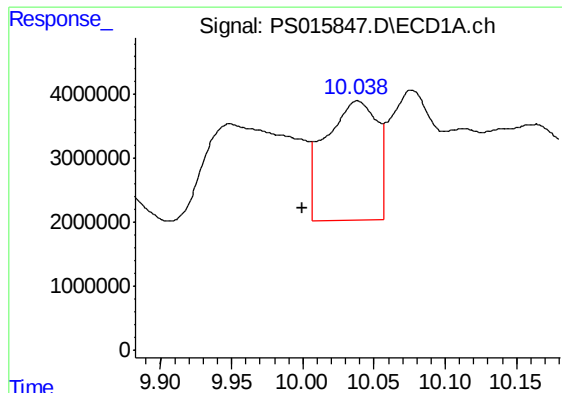

#13 2,4-DB


R.T.: 10.038 min
Delta R.T.: 0.038 min
Response: 46754546
Conc: 22.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUP-01

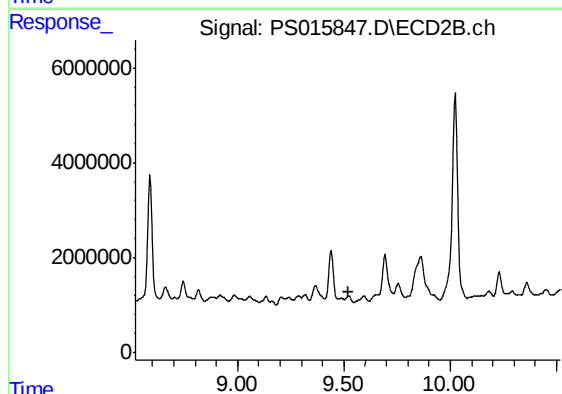


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.519 min
Response: 0
Conc: N.D.

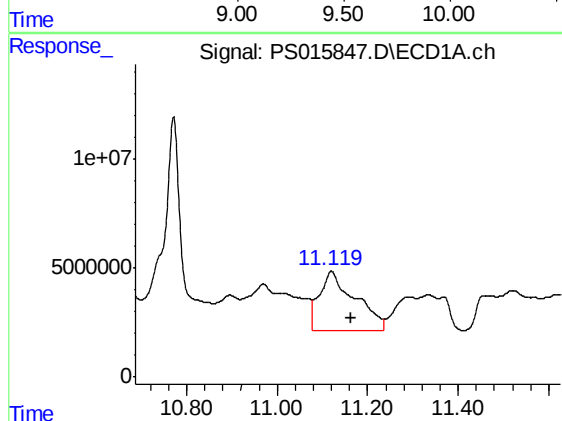


#14 DINOSEB

R.T.: 11.120 min
Delta R.T.: -0.044 min
Response: 149556307
Conc: 23.09 ng/ml

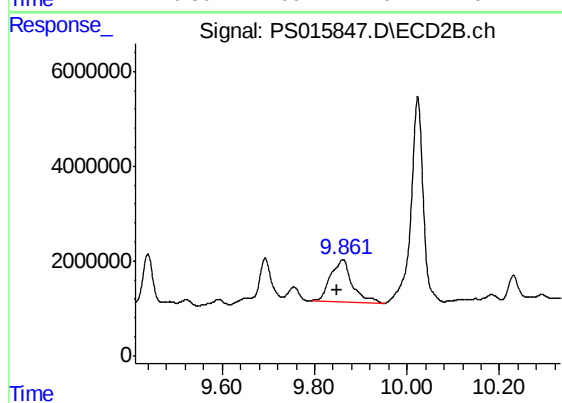

#14 DINOSEB


R.T.: 9.861 min
Delta R.T.: 0.014 min
Response: 28993042
Conc: 14.39 ng/ml

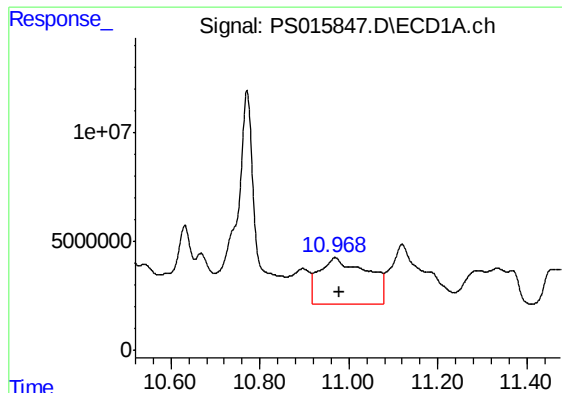

#15 Picloram


R.T.: 10.969 min
Delta R.T.: -0.009 min
Response: 161858738
Conc: 11.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUP-01

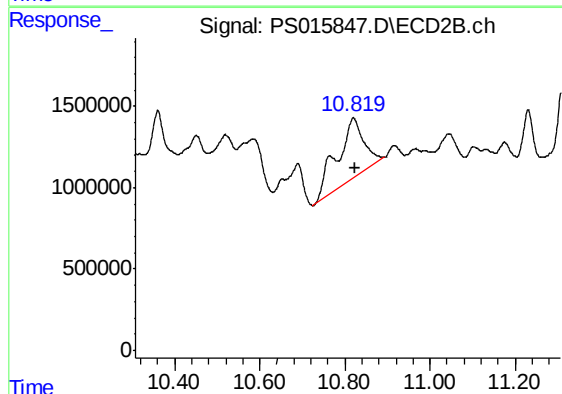


#15 Picloram

R.T.: 10.820 min
Delta R.T.: -0.004 min
Response: 16143793
Conc: 3.84 ng/ml

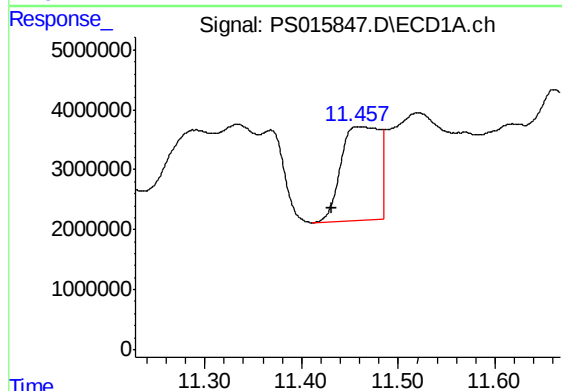

#16 DCPA

R.T.: 11.459 min
Delta R.T.: 0.028 min
Response: 43231204
Conc: 3.27 ng/ml

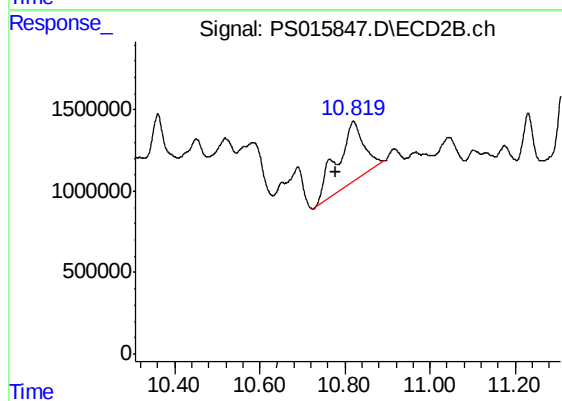

#16 DCPA

R.T.: 10.820 min
Delta R.T.: 0.041 min
Response: 16143793
Conc: 3.84 ng/ml