

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
 Data File : PS015861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2021 03:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 05:17:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 15 18:15:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.189	6.767	789.6E6	279.4E6	475.238	554.460
Target Compounds							
9) T	2,4-D	8.375f	0.000	48533714	0	27.693	N.D. #
10) T	Pentachlo...	8.612	8.270	16184149	6263628	<MDL	<MDL #
11) T	2,4,5-TP ...	9.163	0.000	8192469	0	<MDL	N.D. #
12) T	2,4,5-T	9.448	0.000	12237090	0	1.386	N.D. #
15) T	Picloram	10.979	10.821	23279800	8530316	1.703	2.028
16) T	DCPA	11.422	10.821f	12093122	8530316	<MDL	2.029 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061921\
Data File : PS015861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2021 03:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 05:17:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061521.M
Quant Title : 8080.M
QLast Update : Tue Jun 15 18:15:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

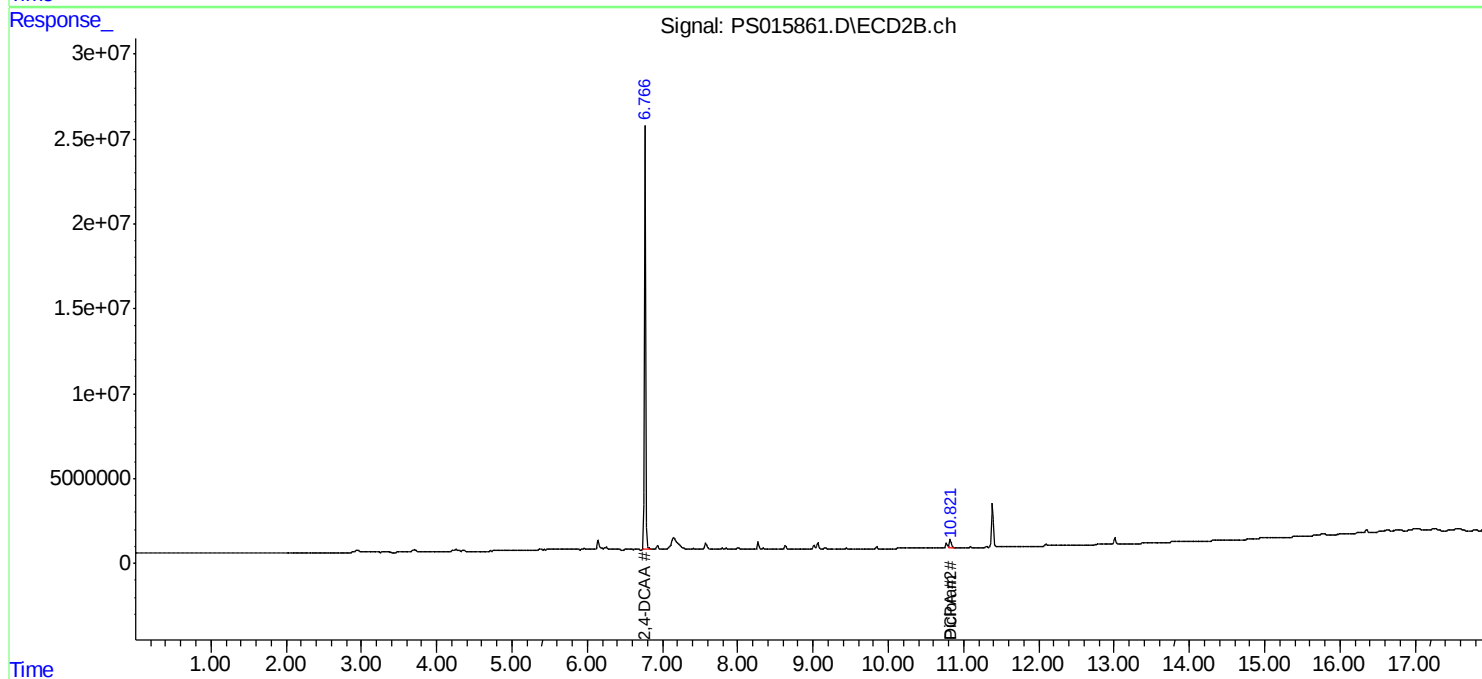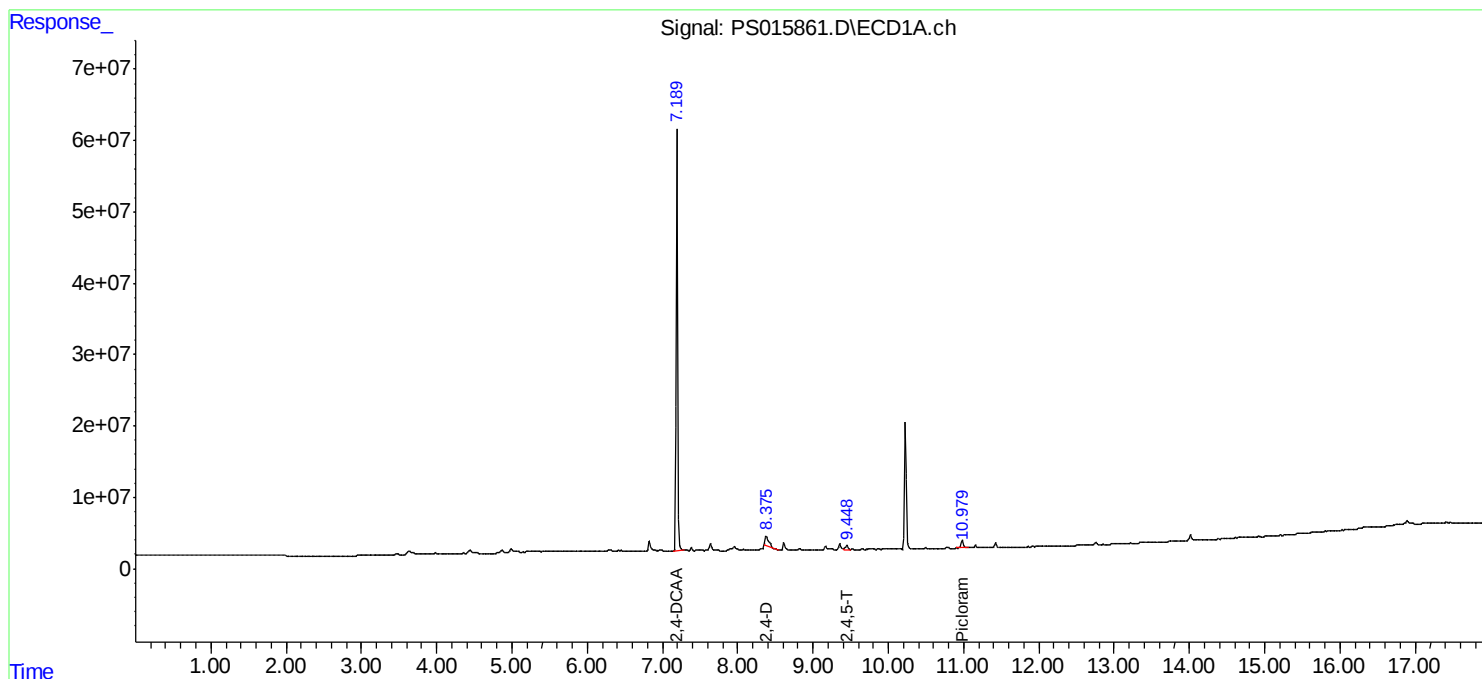


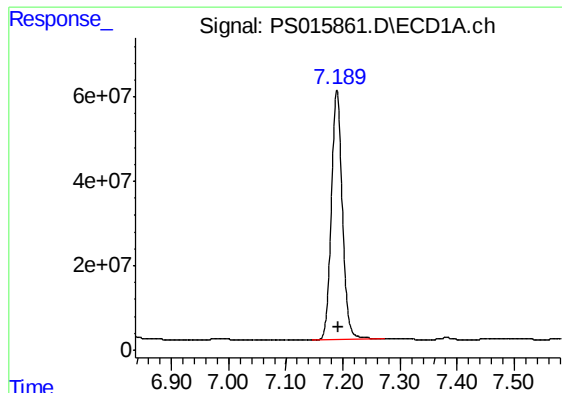

#4 2,4-DCAA


R.T.: 7.189 min
Delta R.T.: -0.003 min
Response: 789583072
Conc: 475.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

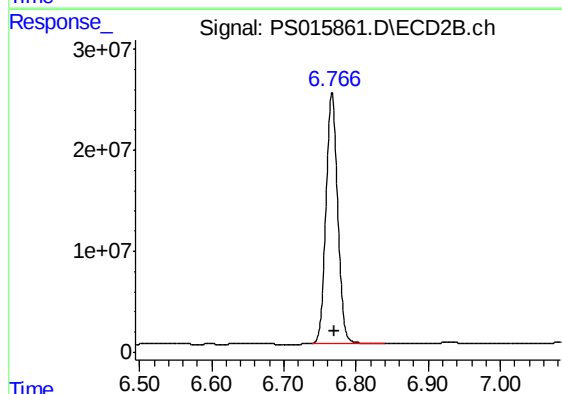


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: -0.004 min
Response: 279365712
Conc: 554.46 ng/ml

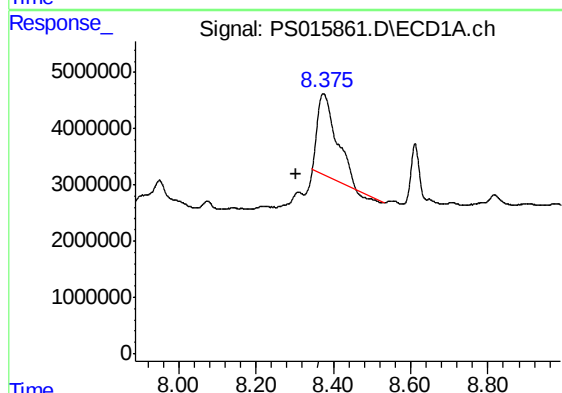


#9 2,4-D

R.T.: 8.375 min
Delta R.T.: 0.069 min
Response: 48533714
Conc: 27.69 ng/ml

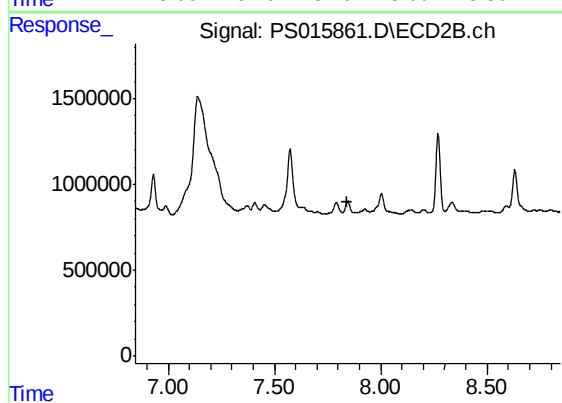

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.845 min
Response: 0
Conc: N.D.

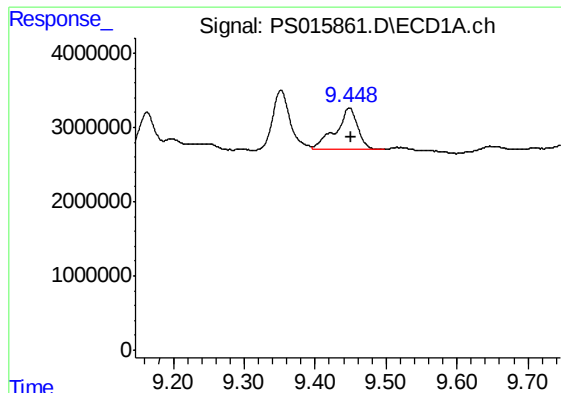

#12 2,4,5-T


R.T.: 9.448 min
Delta R.T.: -0.002 min
Response: 12237090
Conc: 1.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

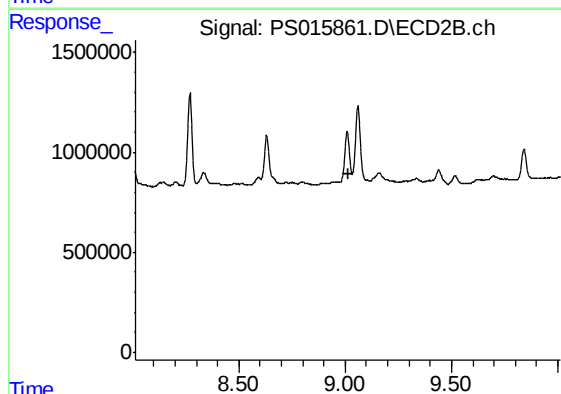


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.013 min
Response: 0
Conc: N.D.

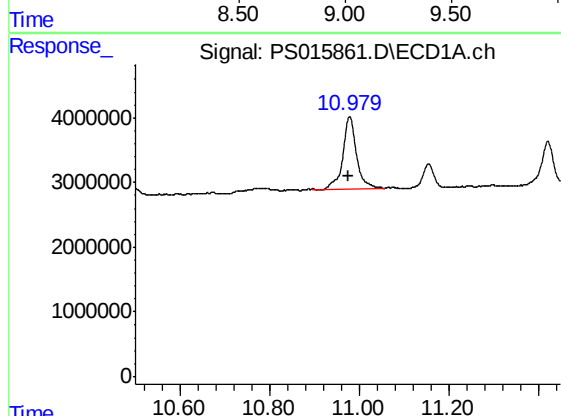


#15 Picloram

R.T.: 10.979 min
Delta R.T.: 0.002 min
Response: 23279800
Conc: 1.70 ng/ml

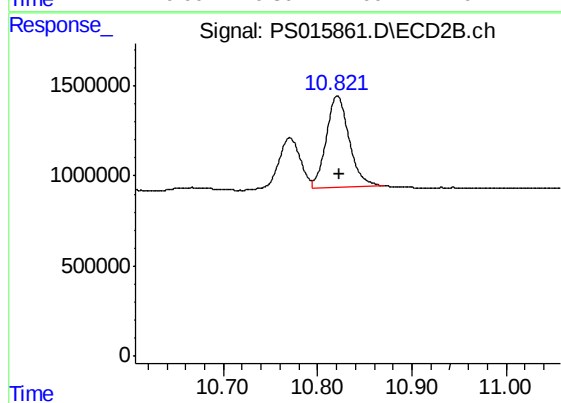

#15 Picloram


R.T.: 10.821 min
Delta R.T.: -0.003 min
Response: 8530316
Conc: 2.03 ng/ml

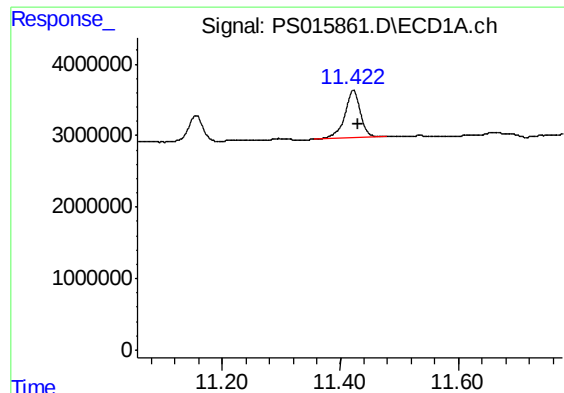

#16 DCPA

R.T.: 11.422 min
Delta R.T.: -0.009 min
Response: 12093122
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

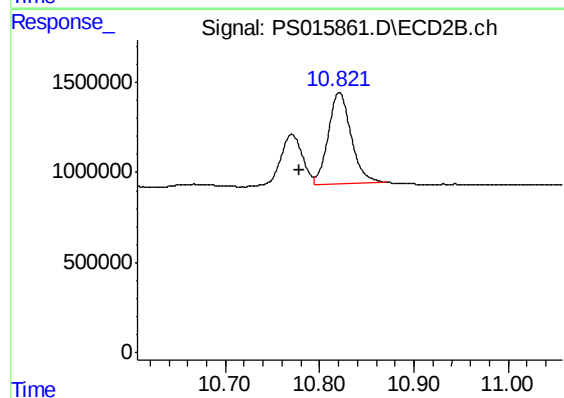

#16 DCPA

R.T.: 10.821 min
Delta R.T.: 0.042 min
Response: 8530316
Conc: 2.03 ng/ml